Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
Operator: PN & BR
Date: 11/13/2009

L0 (without object)
CH_1
Mean: -29.43
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH_2
Mean: 9.21
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_1
Mean: 63.88
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_2
Mean: 67.15
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_1
Mean: -29.22
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_2
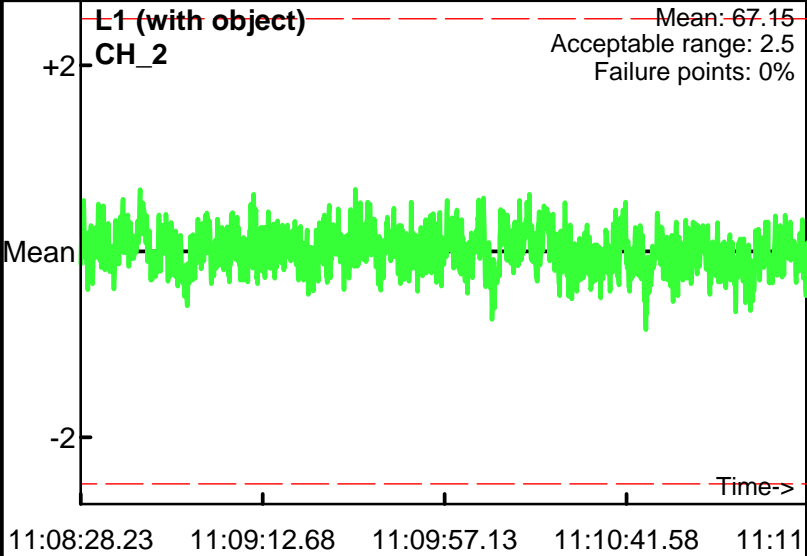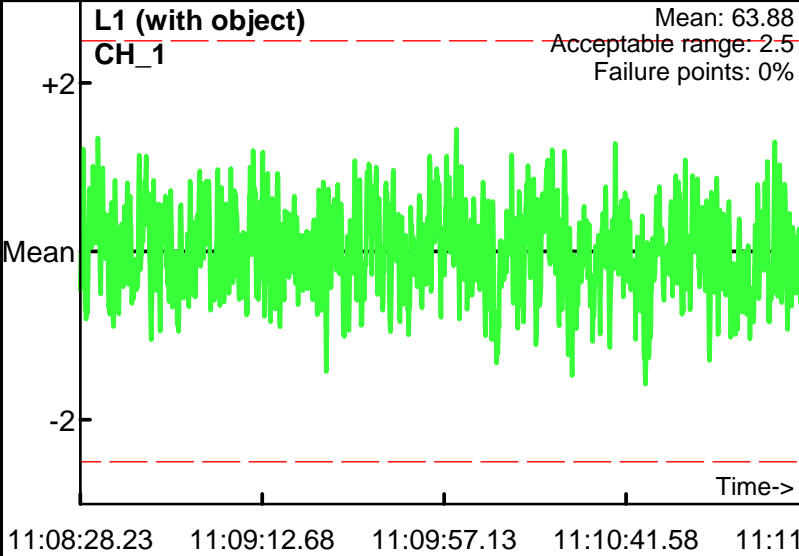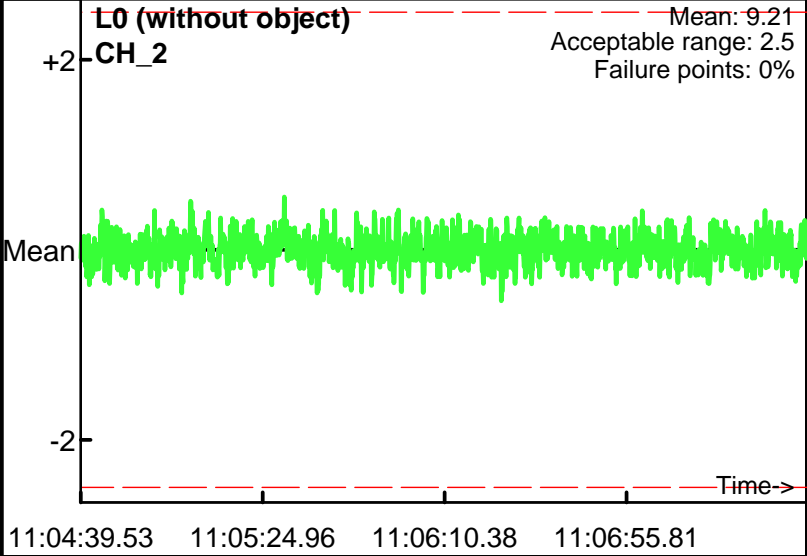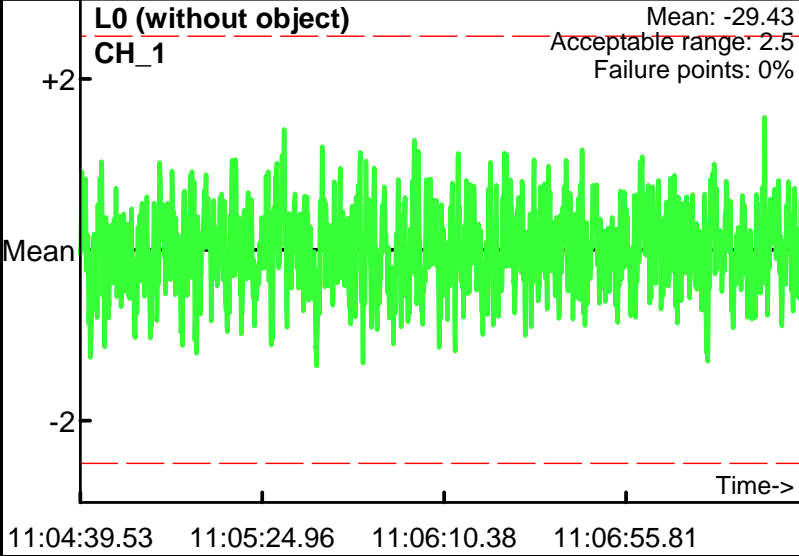Mean: 9.25
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

AM test
Operator: PN & BR
Date: 11/13/2009

L0 (without object)
CH_3
Mean: 6.99
Acceptable range: 2.5
Failure points: 0%

11:04:39.53   11:05:24.96   11:06:10.38   11:06:55.81

L0 (without object)
CH_4
Mean: -1.19
Acceptable range: 2.5
Failure points: 0%

11:04:39.53   11:05:24.96   11:06:10.38   11:06:55.81

L1 (with object)
CH_3
Mean: 37.14
Acceptable range: 2.5
Failure points: 0%

11:08:28.23   11:09:12.68   11:09:57.13   11:10:41.58   11:11

L1 (with object)
CH_4
Mean: 12.05
Acceptable range: 2.5
Failure points: 0%

11:08:28.23   11:09:12.68   11:09:57.13   11:10:41.58   11:11

L2 (without object)
CH_3
Mean: 6.94
Acceptable range: 2.5
Failure points: 0%

11:12:12.03   11:12:26.50   11:12:40.98   11:12:55.45   11:13

L2 (without object)
CH_4
Mean: -1.27
Acceptable range: 2.5
Failure points: 0%

11:12:12.03   11:12:26.50   11:12:40.98   11:12:55.45   11:13

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
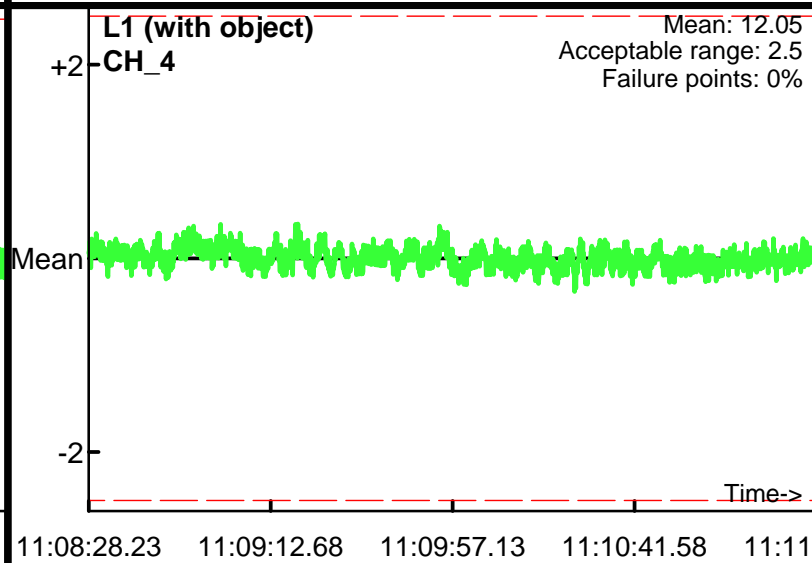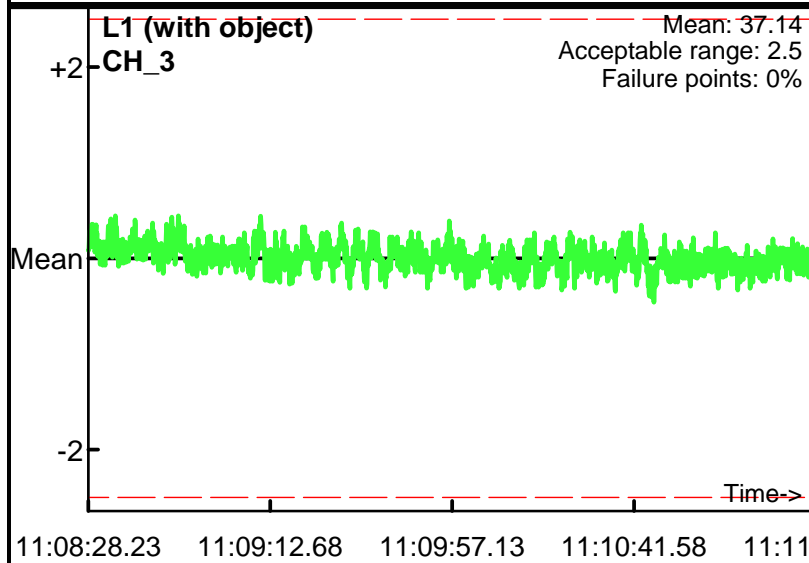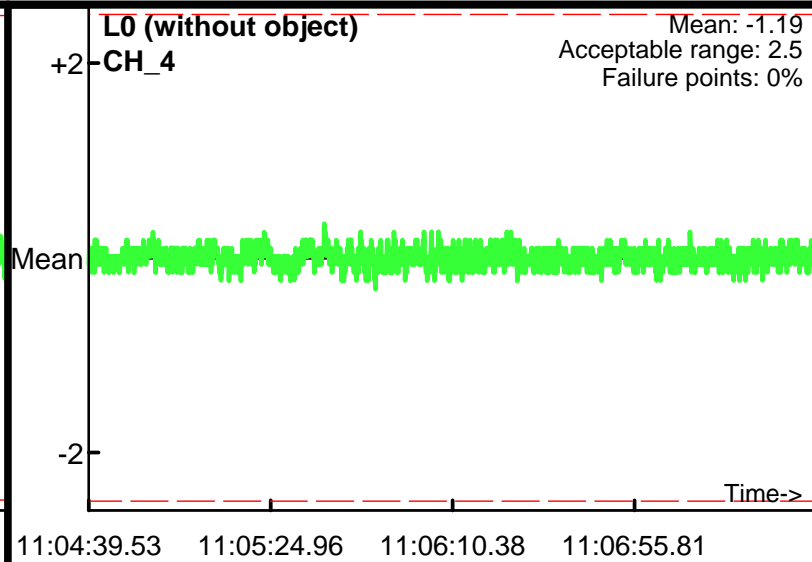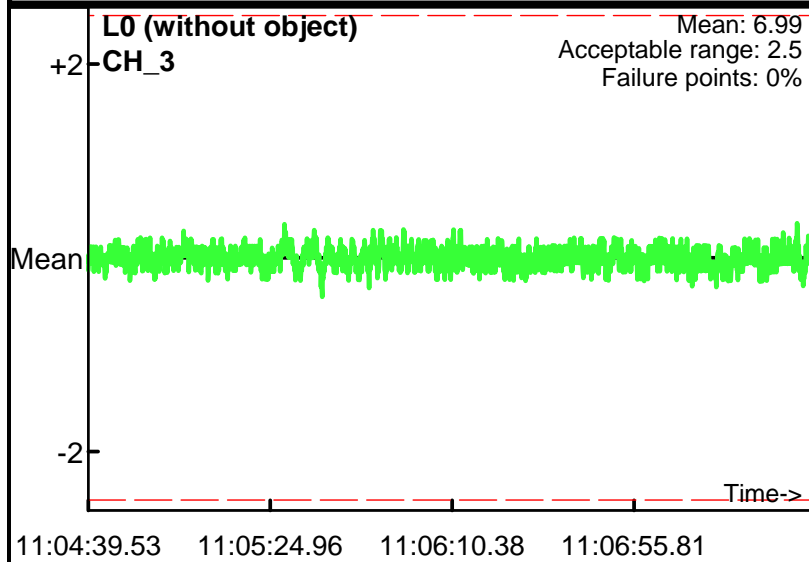Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
Date: 11/13/2009

L0.1 (without object) CH_1 — Mean: -62.7, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:04:39.48 · 11:05:24.91 · 11:06:10.34 · 11:06:55.76

L0.1 (without object) CH_2 — Mean: 13.32, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:04:39.48 · 11:05:24.91 · 11:06:10.34 · 11:06:55.76

L1.1 (with object) CH_1 — Mean: 60.9, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:08:28.30 · 11:09:12.72 · 11:09:57.15 · 11:10:41.57

L1.1 (with object) CH_2 — Mean: 106.28, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:08:28.30 · 11:09:12.72 · 11:09:57.15 · 11:10:41.57

L2.1 (without object) CH_1 — Mean: -62.9, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:12:12.09 · 11:12:26.55 · 11:12:41.00 · 11:12:55.45 · 11:13

L2.1 (without object) CH_2 — Mean: 13.28, Acceptable range: 2.5, Failure points: 0%
Time axis: 11:12:12.09 · 11:12:26.55 · 11:12:41.00 · 11:12:55.45 · 11:13

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
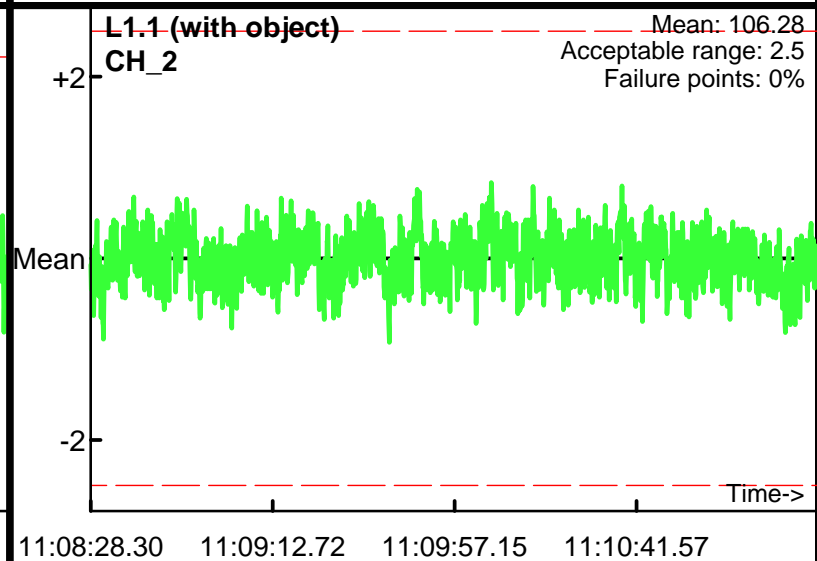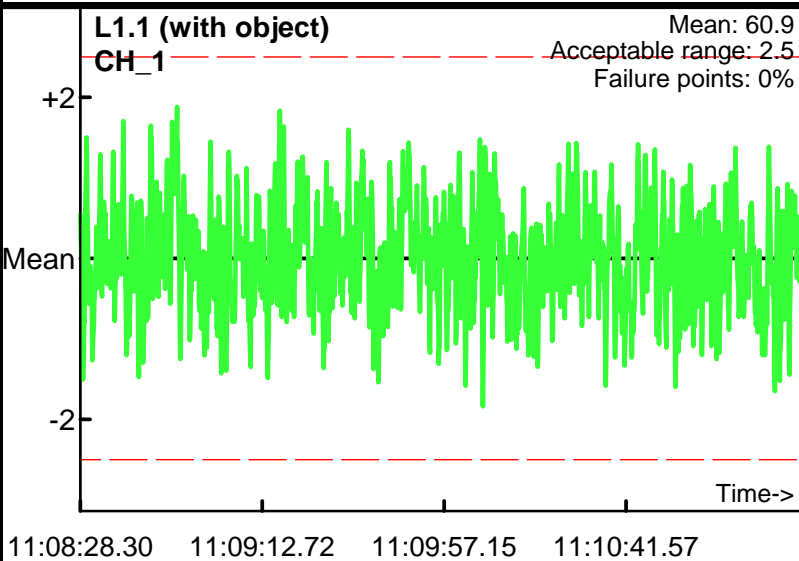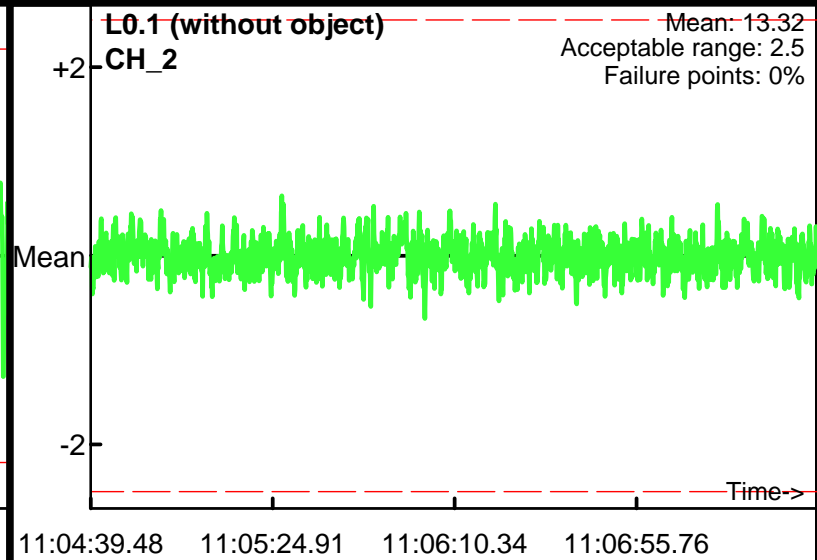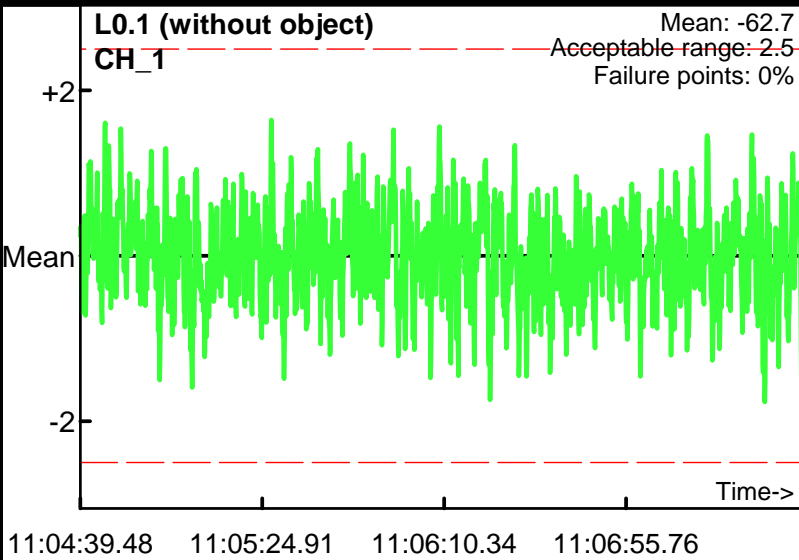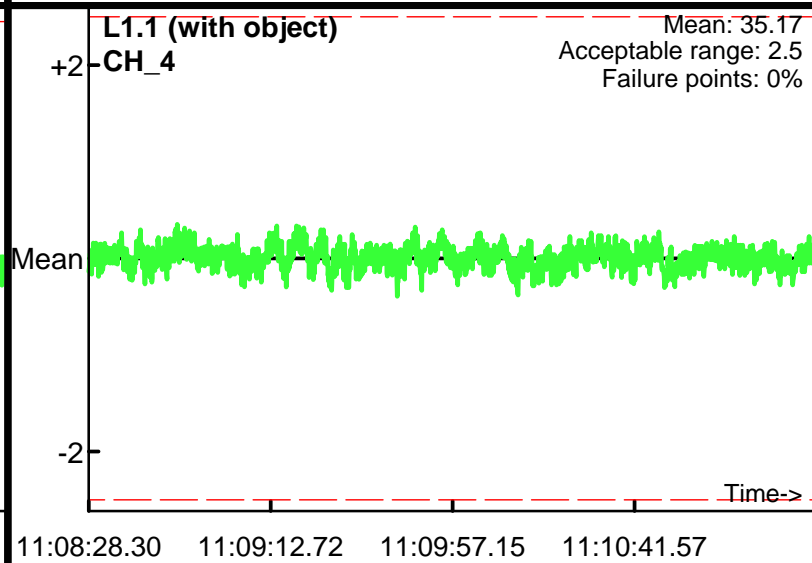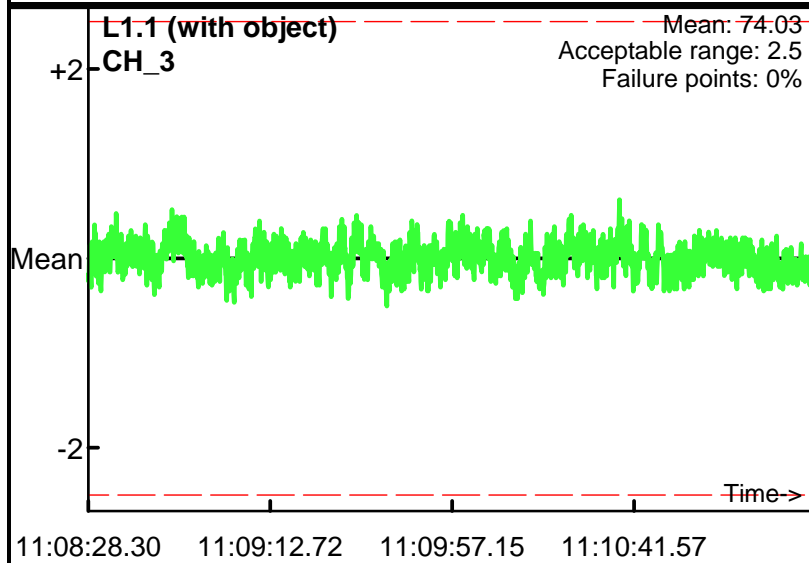Date: 11/13/2009

L0.1 (without object)
CH_3

Mean: 14.66
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:04:39.48   11:05:24.91   11:06:10.34   11:06:55.76

L0.1 (without object)
CH_4

Mean: 3.41
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:04:39.48   11:05:24.91   11:06:10.34   11:06:55.76

L1.1 (with object)
CH_3

Mean: 74.03
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:08:28.30   11:09:12.72   11:09:57.15   11:10:41.57

L1.1 (with object)
CH_4

Mean: 35.17
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:08:28.30   11:09:12.72   11:09:57.15   11:10:41.57

L2.1 (without object)
CH_3

Mean: 14.66
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:12:12.09   11:12:26.55   11:12:41.00   11:12:55.45   11:13

L2.1 (without object)
CH_4

Mean: 3.39
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:12:12.09   11:12:26.55   11:12:41.00   11:12:55.45   11:13

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

● Outside range
- - - Acceptable limits

L0.2 (without object)
CH_1
Mean: -57.24
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:04:39.47   11:05:24.92   11:06:10.37   11:06:55.82

L0.2 (without object)
CH_2
Mean: 5.48
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:04:39.47   11:05:24.92   11:06:10.37   11:06:55.82

L1.2 (with object)
CH_1
Mean: 29.18
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:08:28.27   11:09:12.71   11:09:57.16   11:10:41.61   11:11

L1.2 (with object)
CH_2
Mean: 58.47
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:08:28.27   11:09:12.71   11:09:57.16   11:10:41.61   11:11

L2.2 (without object)
CH_1
Mean: -57.54
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:12:12.06   11:12:26.52   11:12:40.97   11:12:55.42   11:13

L2.2 (without object)
CH_2
Mean: 5.4
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:12:12.06   11:12:26.52   11:12:40.97   11:12:55.42   11:13
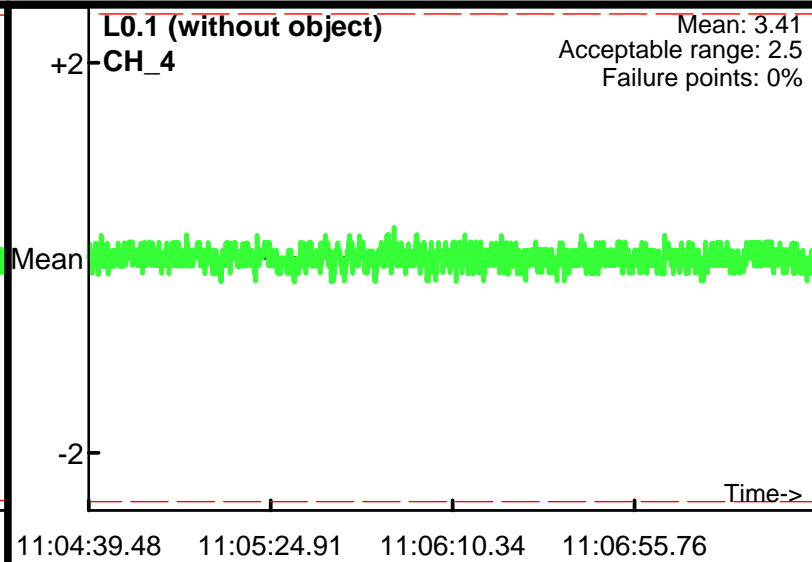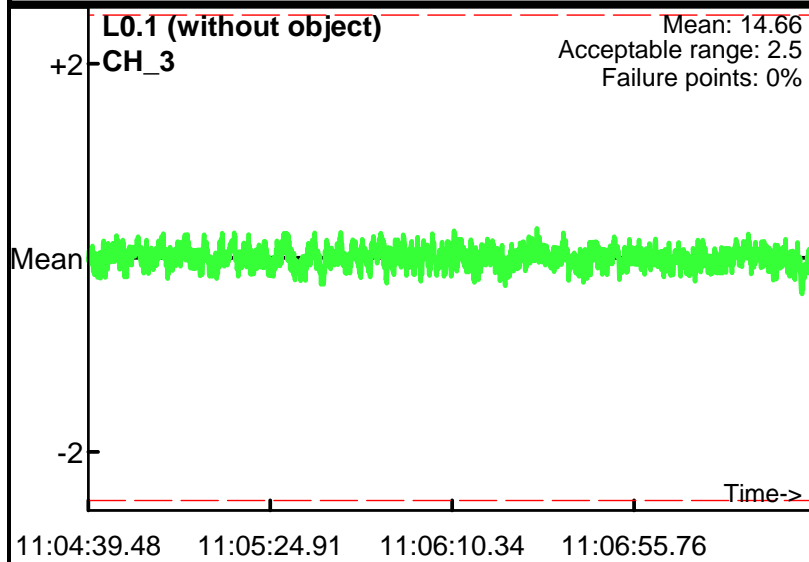
Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
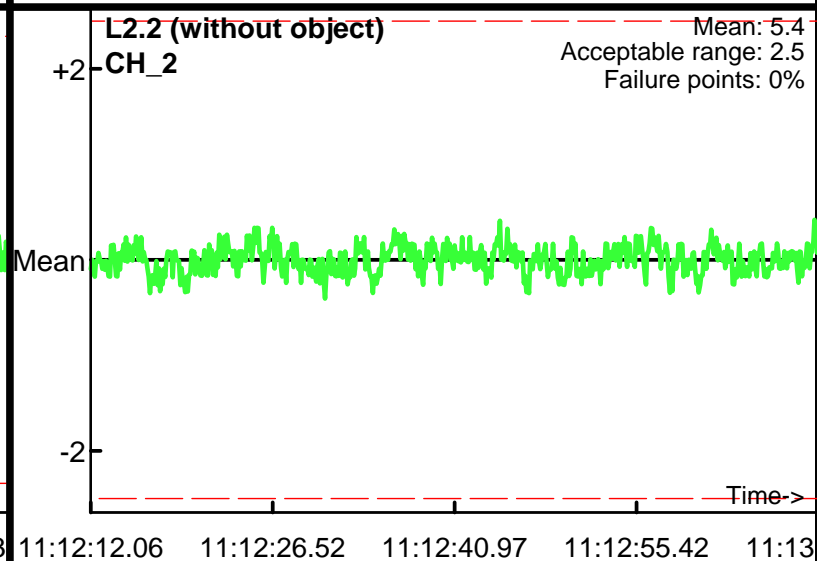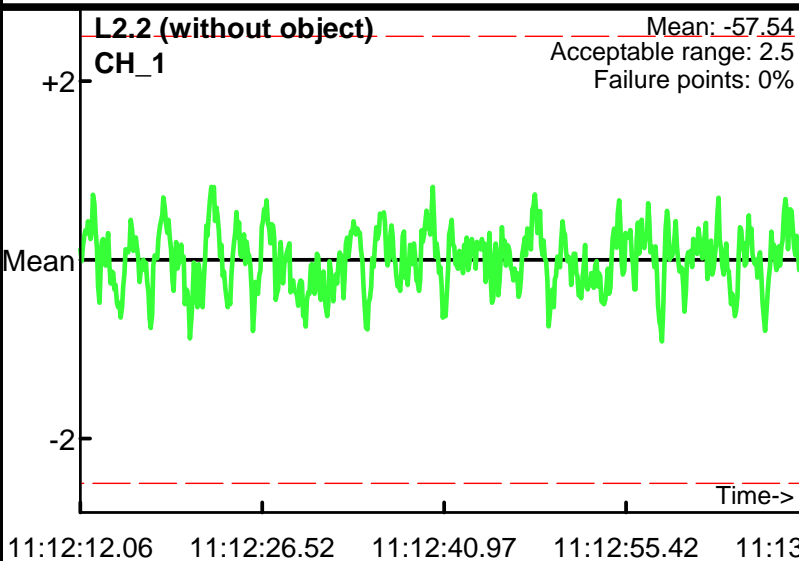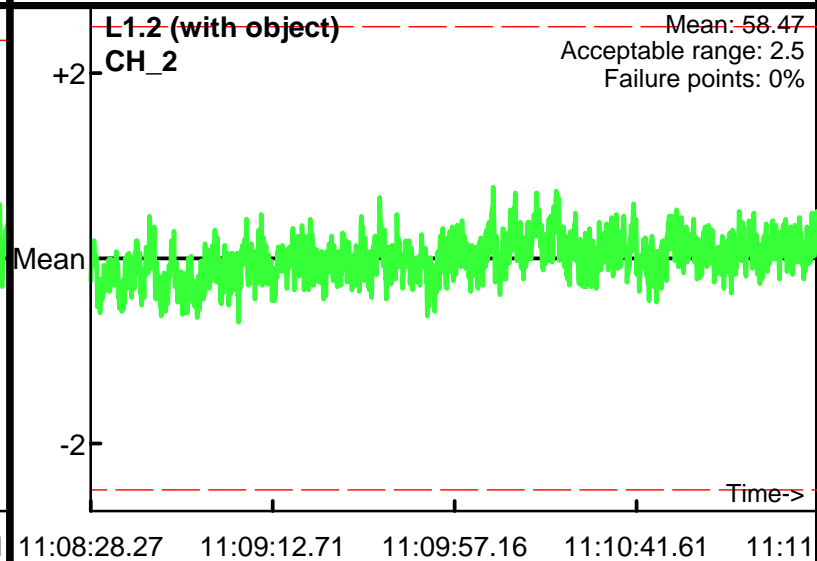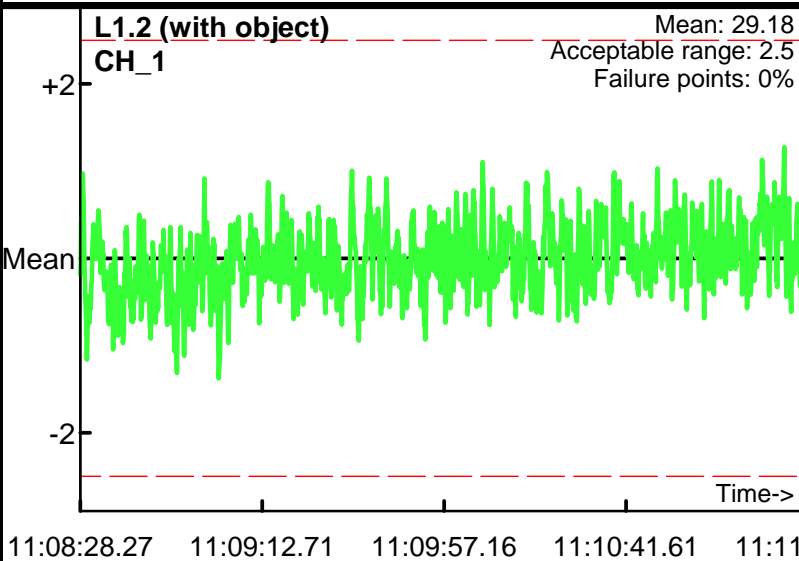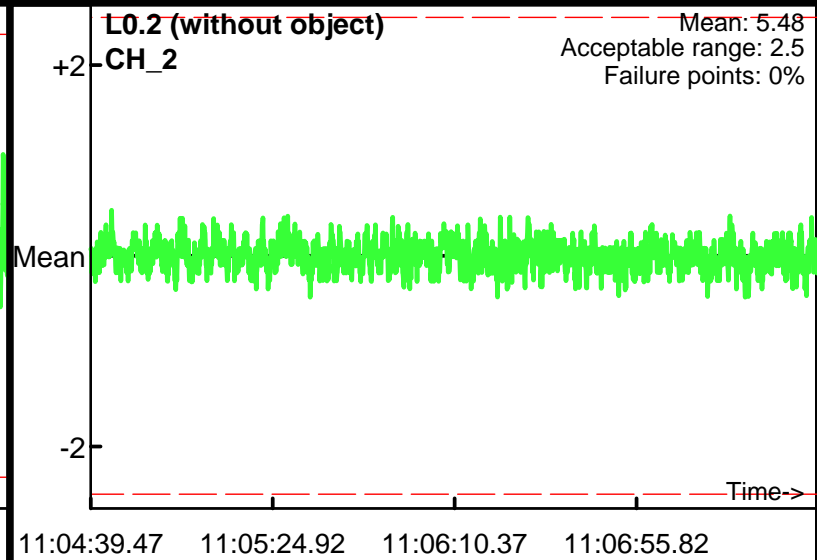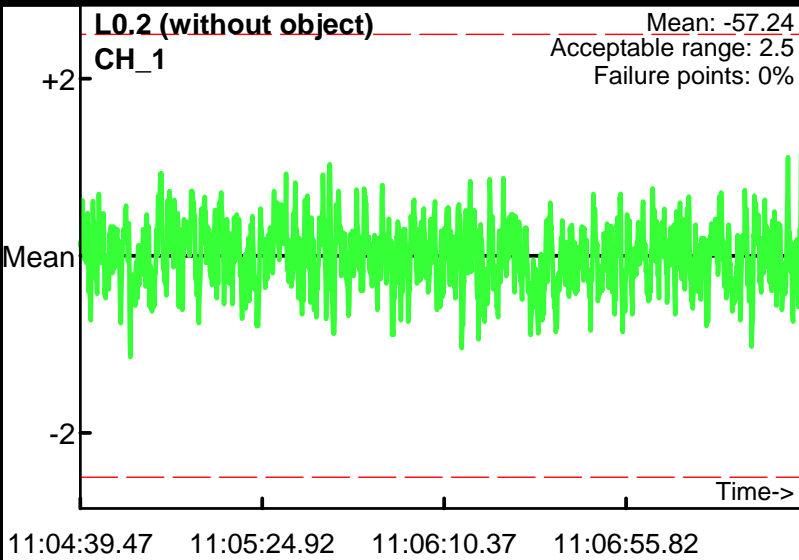– – – Acceptable limits

AM test
Operator: PN & BR
Date: 11/13/2009

L0.2 (without object)
CH_3
Mean: 6.69
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:04:39.47   11:05:24.92   11:06:10.37   11:06:55.82

L0.2 (without object)
CH_4
Mean: -0.56
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:04:39.47   11:05:24.92   11:06:10.37   11:06:55.82

L1.2 (with object)
CH_3
Mean: 33.74
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:08:28.27   11:09:12.71   11:09:57.16   11:10:41.61   11:11

L1.2 (with object)
CH_4
Mean: 11.07
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:08:28.27   11:09:12.71   11:09:57.16   11:10:41.61   11:11

L2.2 (without object)
CH_3
Mean: 6.7
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:12:12.06   11:12:26.52   11:12:40.97   11:12:55.42   11:13

L2.2 (without object)
CH_4
Mean: -0.55
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:12:12.06   11:12:26.52   11:12:40.97   11:12:55.42   11:13

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009
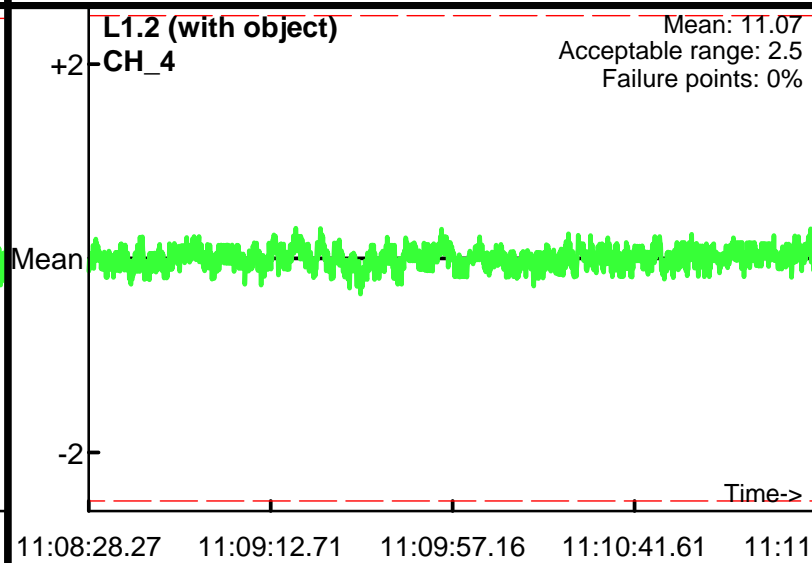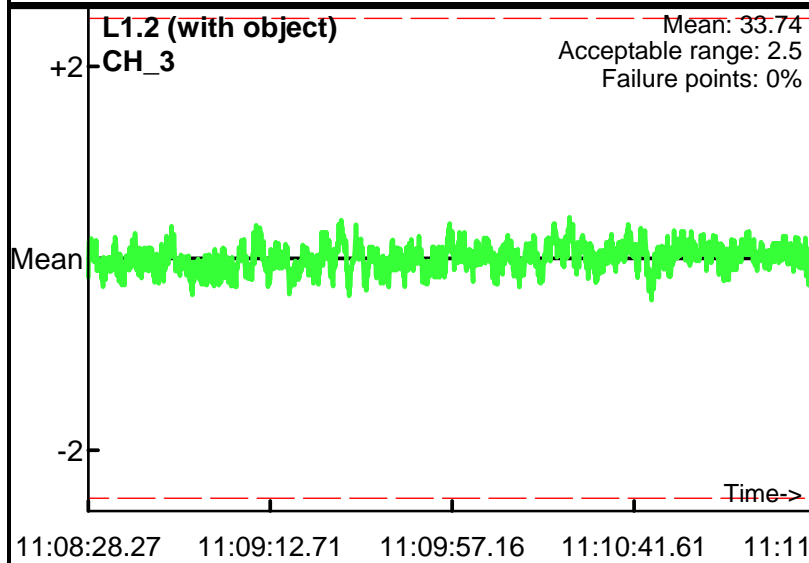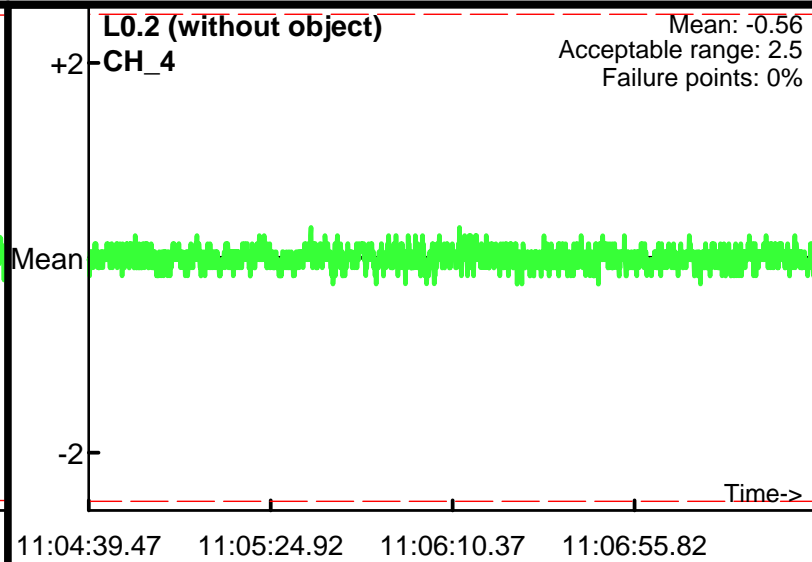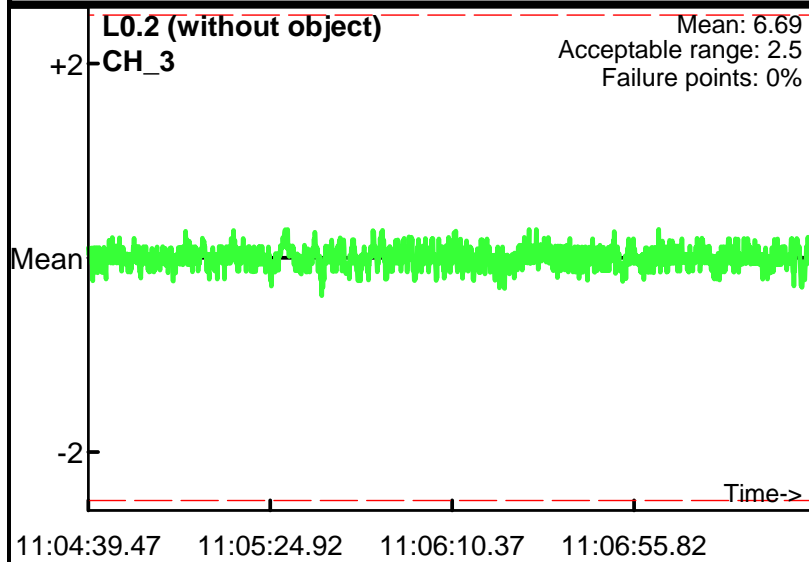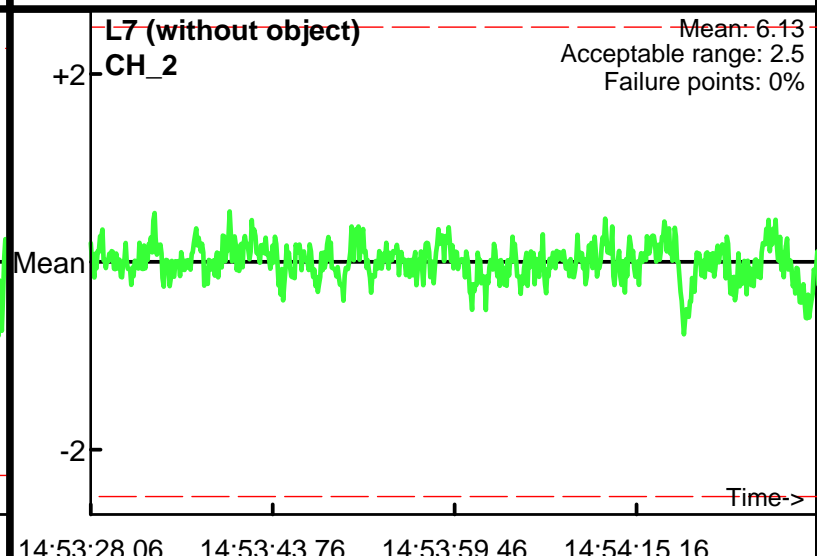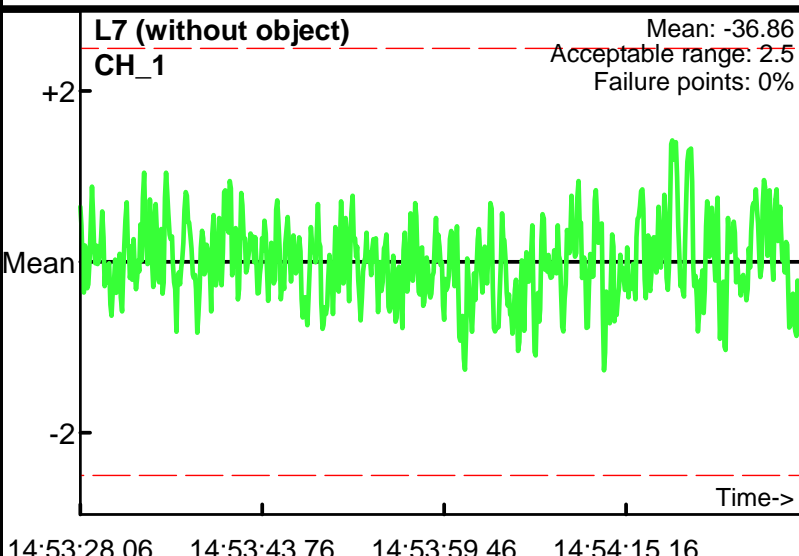
L5 (without object)
CH_1

Mean: -37.03
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:45:46.45   14:46:32.15   14:47:17.85   14:48:03.55

L5 (without object)
CH_2

Mean: 5.91
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:45:46.45   14:46:32.15   14:47:17.85   14:48:03.55

L6 (with object)
CH_1

Mean: 57
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:49:53.25   14:50:38.43   14:51:23.60   14:52:08.78   14:52

L6 (with object)
CH_2

Mean: 64.49
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:49:53.25   14:50:38.43   14:51:23.60   14:52:08.78   14:52

L7 (without object)
CH_1

Mean: -36.86
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:53:28.06   14:53:43.76   14:53:59.46   14:54:15.16

L7 (without object)
CH_2

Mean: 6.13
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:53:28.06   14:53:43.76   14:53:59.46   14:54:15.16

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
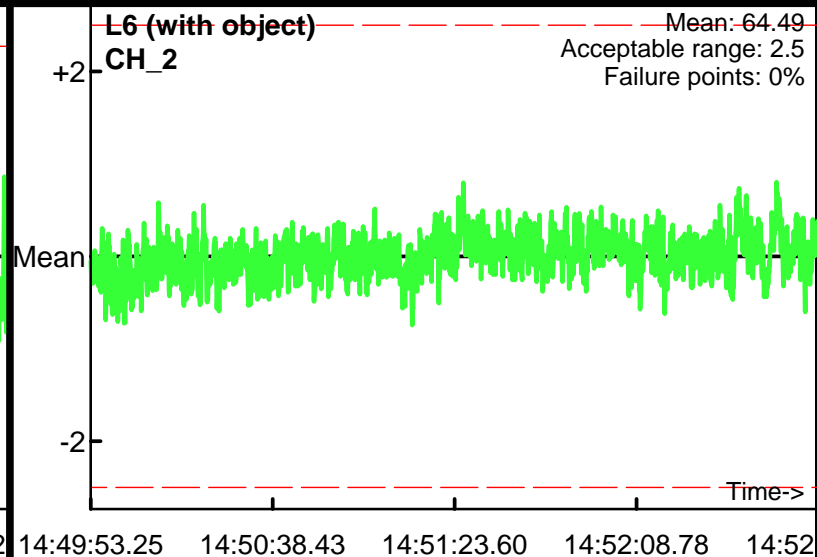Line Name: L5 L6 L7

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
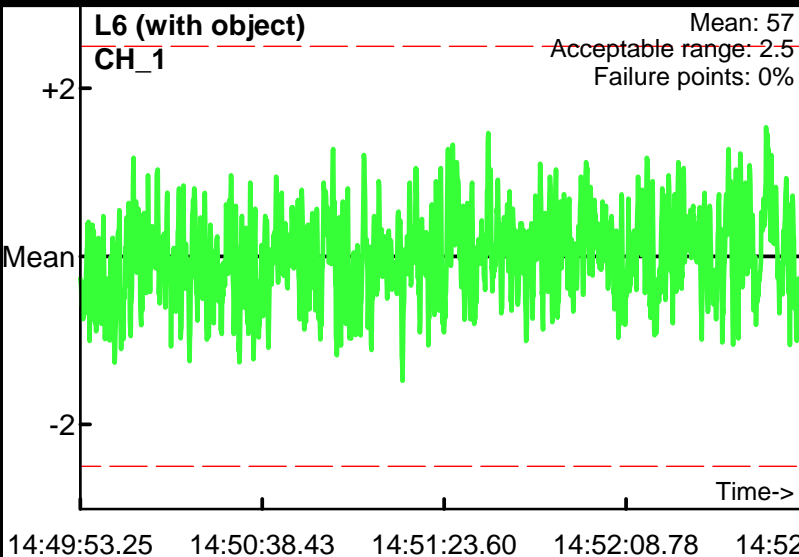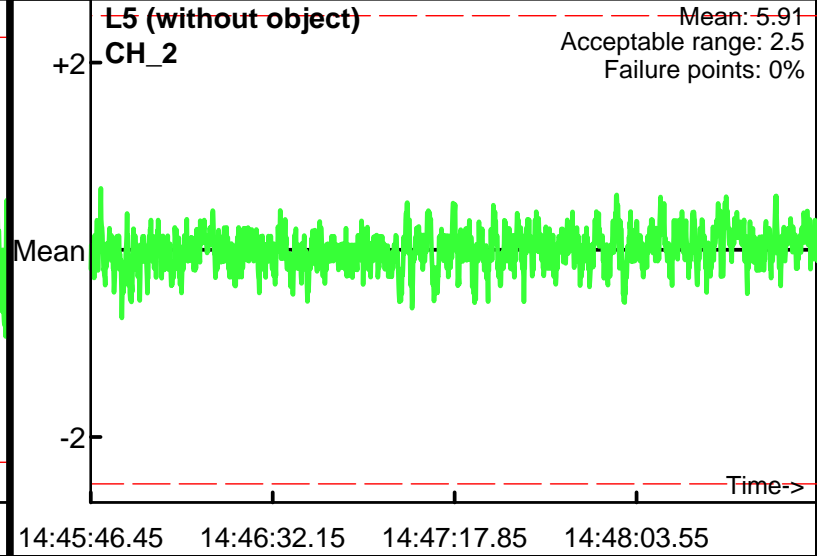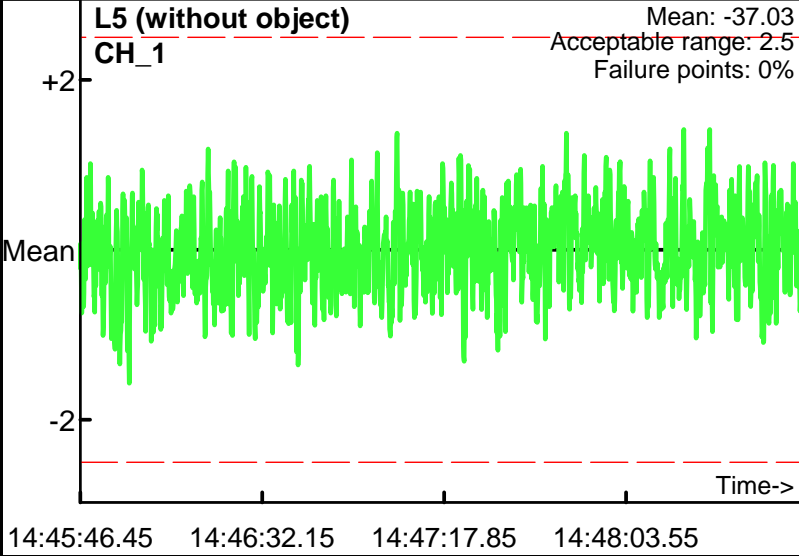– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009

L5 (without object)
CH_3
Mean: 5.15
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:45:46.45   14:46:32.15   14:47:17.85   14:48:03.55

L5 (without object)
CH_4
Mean: -2.45
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:45:46.45   14:46:32.15   14:47:17.85   14:48:03.55

L6 (with object)
CH_3
Mean: 35.75
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:49:53.25   14:50:38.43   14:51:23.60   14:52:08.78   14:52

L6 (with object)
CH_4
Mean: 11.04
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:49:53.25   14:50:38.43   14:51:23.60   14:52:08.78   14:52

L7 (without object)
CH_3
Mean: 5.36
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:53:28.06   14:53:43.76   14:53:59.46   14:54:15.16

L7 (without object)
CH_4
Mean: -2.3
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
14:53:28.06   14:53:43.76   14:53:59.46   14:54:15.16

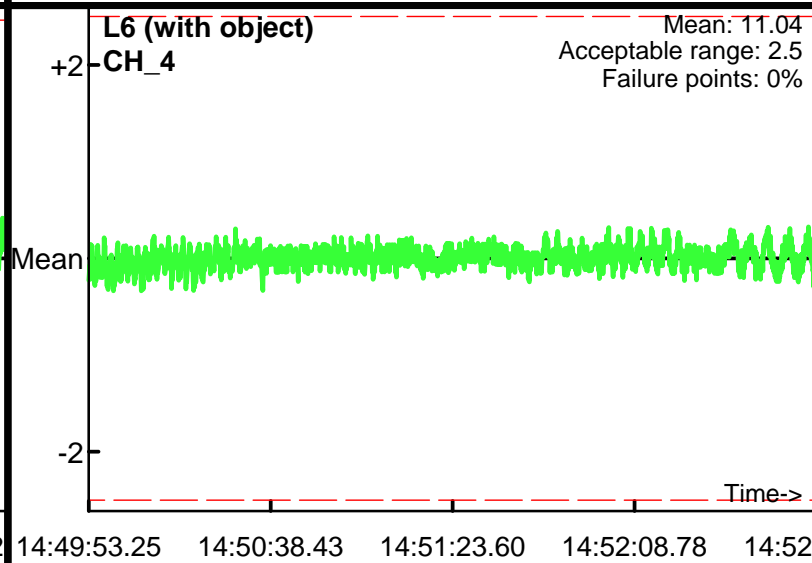Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L5 L6 L7

Page: 2

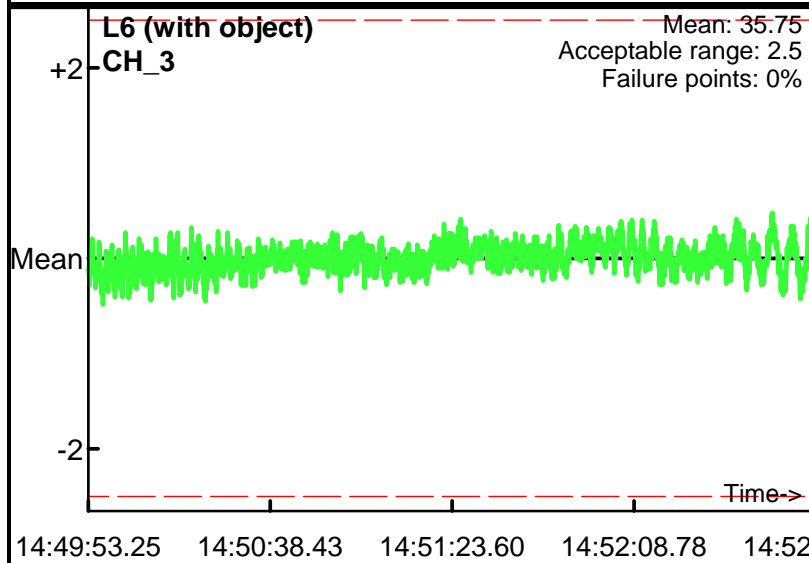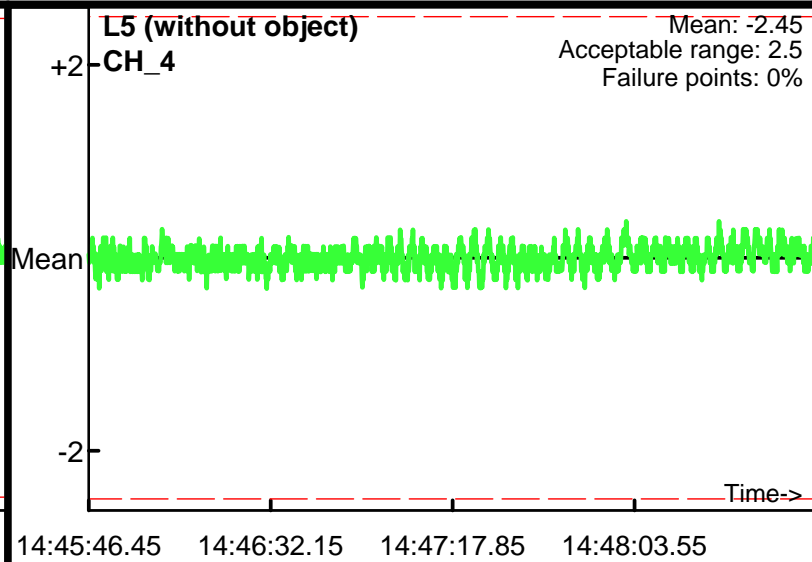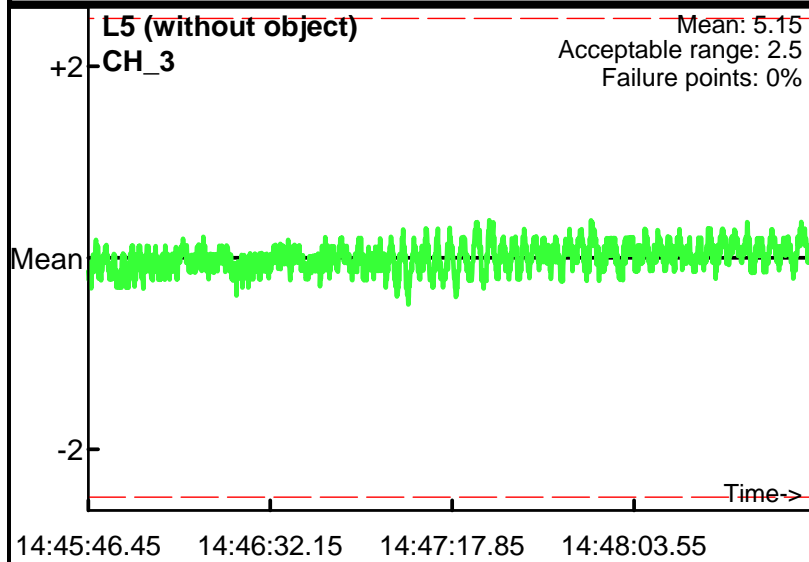# Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009

L5.1 (without object) CH_1 — Mean: -59.48, Acceptable range: 2.5, Failure points: 0%

L5.1 (without object) CH_2 — Mean: 13.64, Acceptable range: 2.5, Failure points: 0%

L6.1 (with object) CH_1 — Mean: 57.59, Acceptable range: 2.5, Failure points: 0%

L6.1 (with object) CH_2 — Mean: 102.27, Acceptable range: 2.5, Failure points: 0%

L7.1 (without object) CH_1 — Mean: -60.47, Acceptable range: 2.5, Failure points: 0%

L7.1 (without object) CH_2 — Mean: 13.45, Acceptable range: 2.5, Failure points: 0%
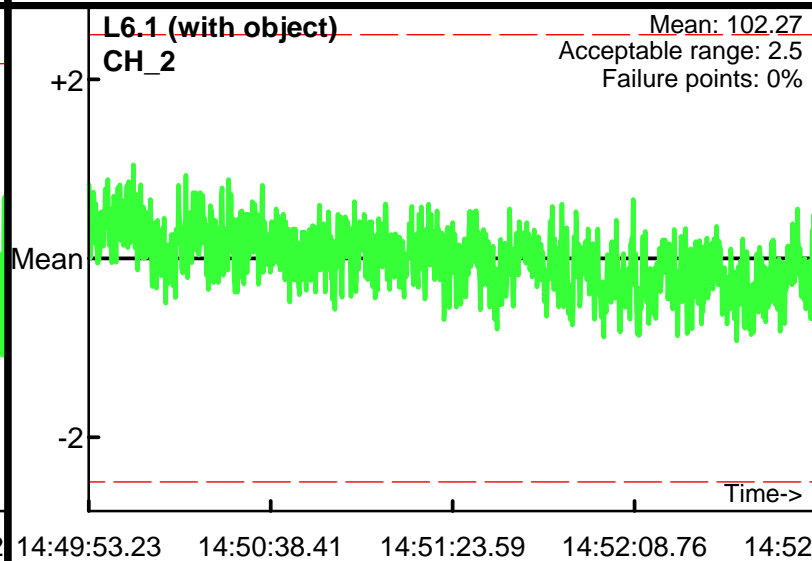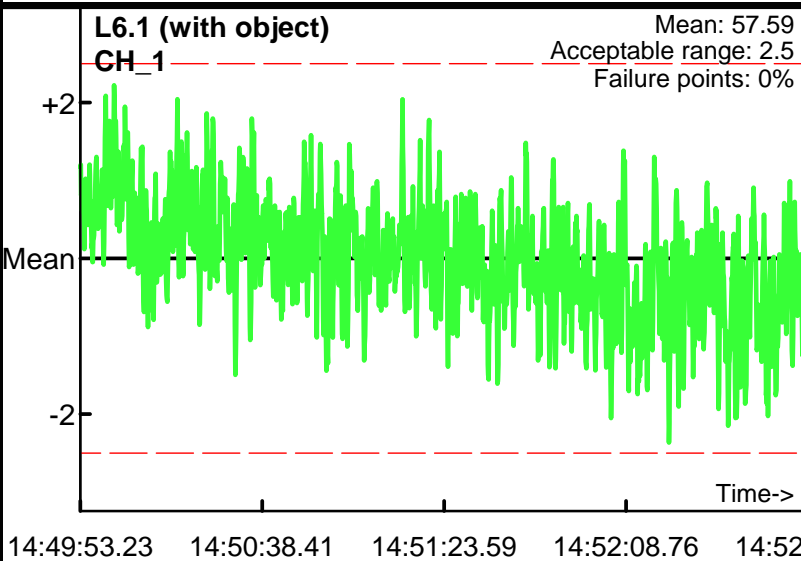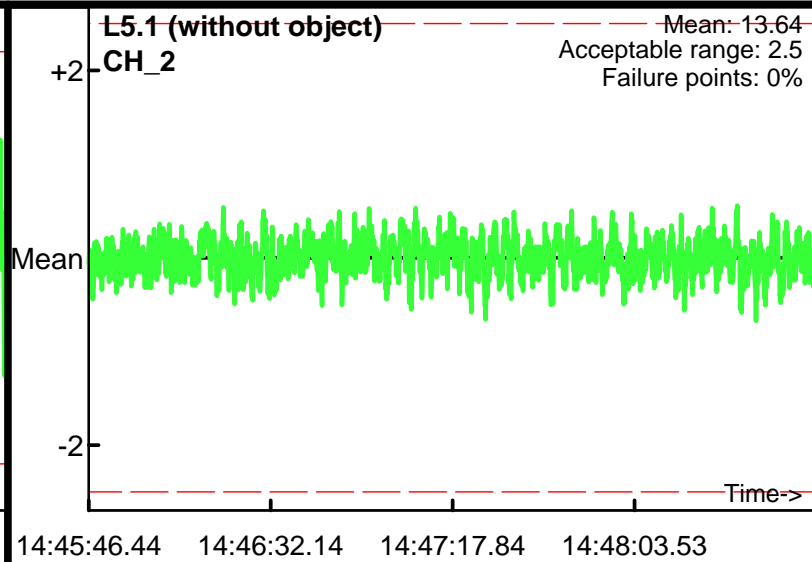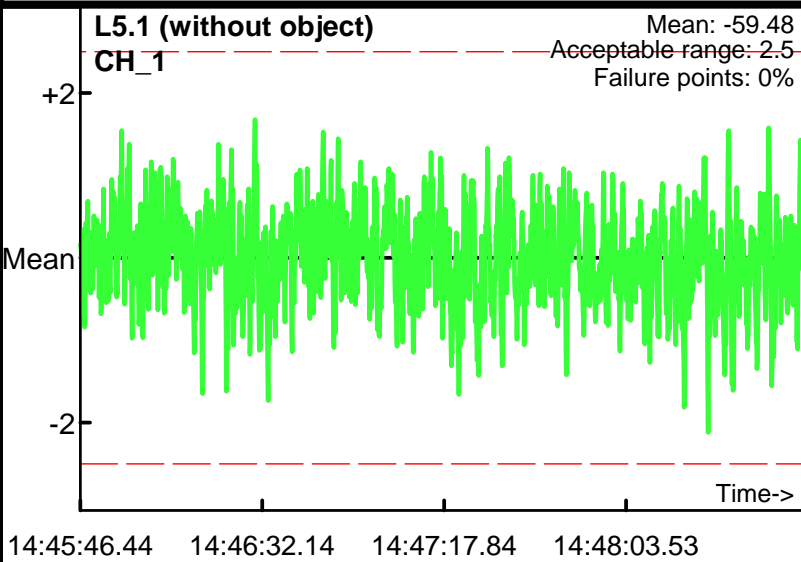
Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009

L5.1 (without object)
CH_3
Mean: 14.43
Acceptable range: 2.5
Failure points: 0%

L5.1 (without object)
CH_4
Mean: 3.1
Acceptable range: 2.5
Failure points: 0%

14:45:46.44   14:46:32.14   14:47:17.84   14:48:03.53

14:45:46.44   14:46:32.14   14:47:17.84   14:48:03.53

L6.1 (with object)
CH_3
Mean: 71.33
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_4
Mean: 33.68
Acceptable range: 2.5
Failure points: 0%

14:49:53.23   14:50:38.41   14:51:23.59   14:52:08.76   14:52

14:49:53.23   14:50:38.41   14:51:23.59   14:52:08.76   14:52

L7.1 (without object)
CH_3
Mean: 14.48
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_4
Mean: 3.13
Acceptable range: 2.5
Failure points: 0%

14:53:28.03   14:53:43.73   14:53:59.43   14:54:15.13

14:53:28.03   14:53:43.73   14:53:59.43   14:54:15.13

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L5.1 L6.1 L7.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
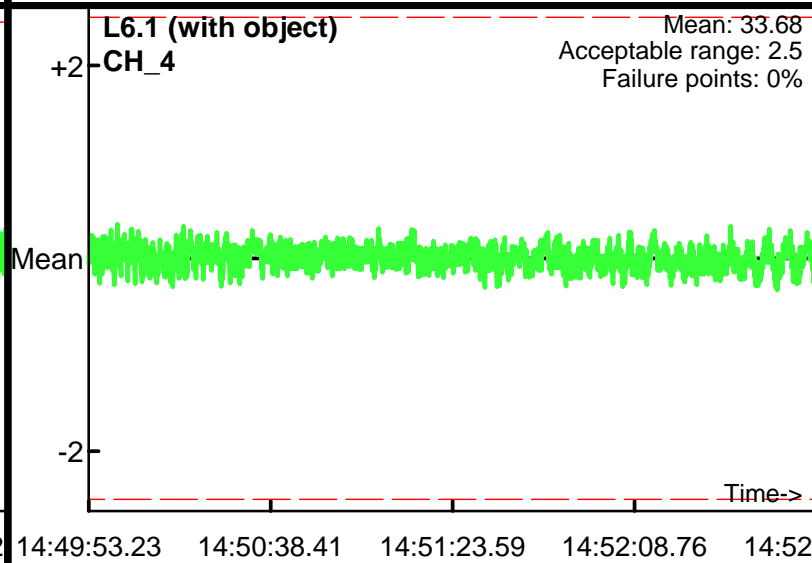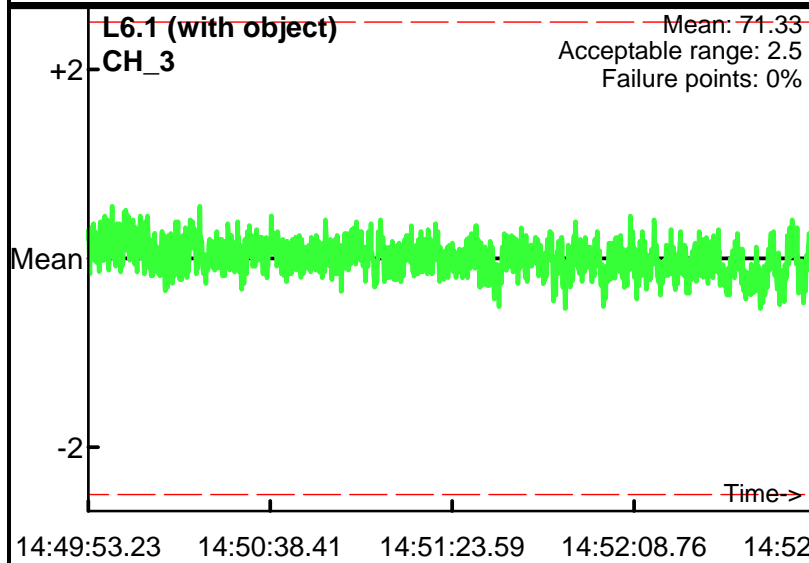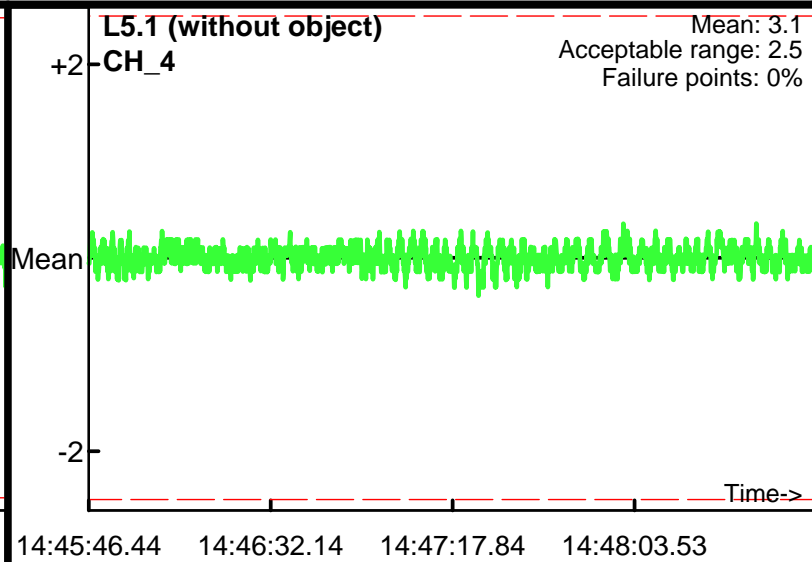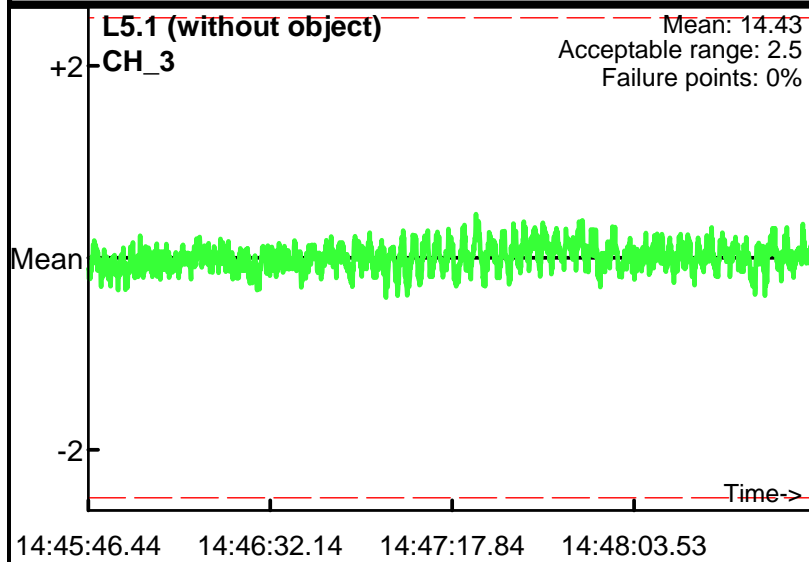Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009

L5.2 (without object)
CH_1
Mean: -41.05
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_2
Mean: 11.19
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_1
Mean: 47.74
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_2
Mean: 66.35
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_1
Mean: -42.13
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_2
Mean: 11.03
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develoment Areas
Equipment: EM-61 Mark II
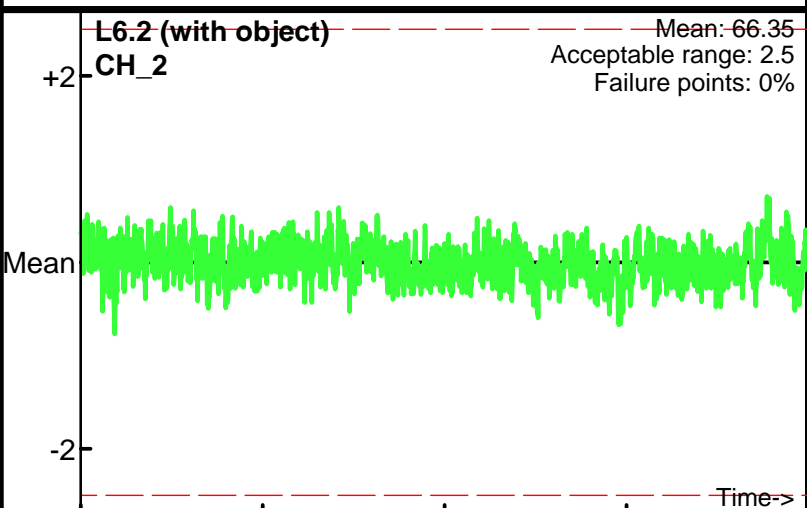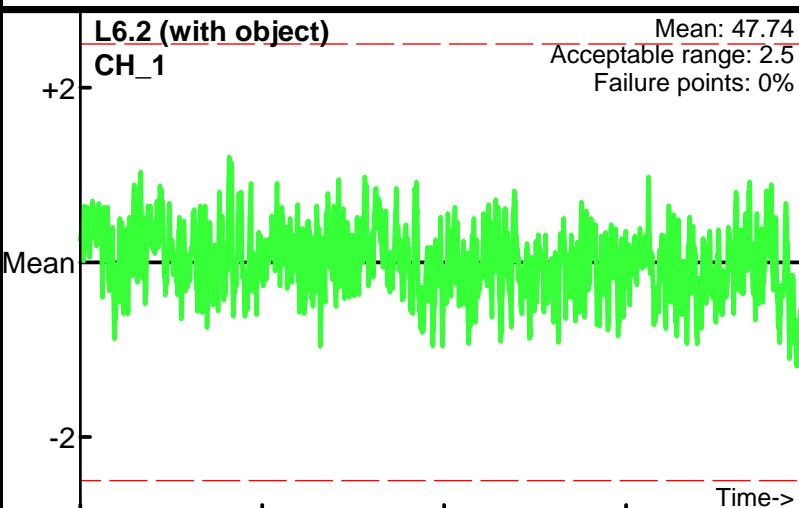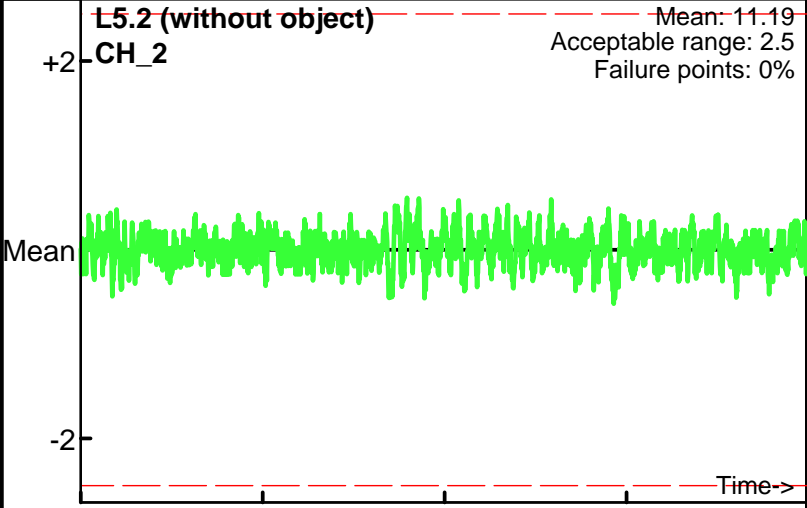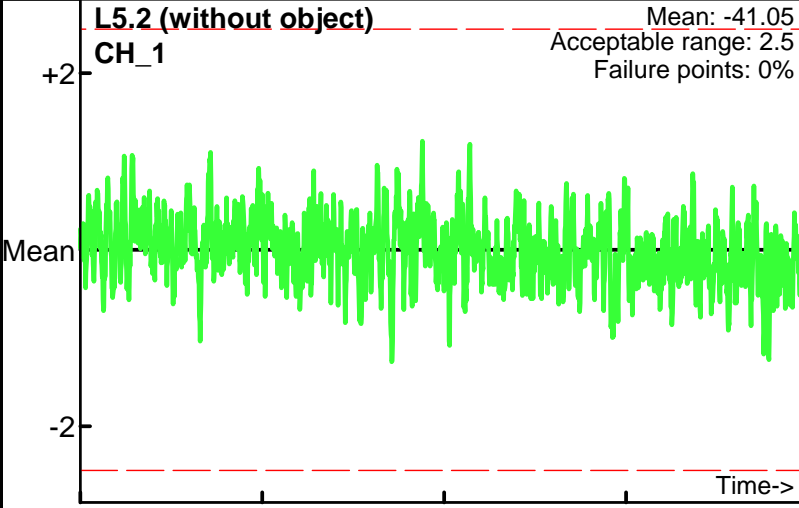Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/13/2009

L5.2 (without object)
CH_3
Mean: 8.74
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_4
Mean: 0.11
Acceptable range: 2.5
Failure points: 0%

14:45:46.50   14:46:32.18   14:47:17.85   14:48:03.53

14:45:46.50   14:46:32.18   14:47:17.85   14:48:03.53

L6.2 (with object)
CH_3
Mean: 37.23
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_4
Mean: 12.46
Acceptable range: 2.5
Failure points: 0%

14:49:53.20   14:50:38.40   14:51:23.60   14:52:08.80   14:52

14:49:53.20   14:50:38.40   14:51:23.60   14:52:08.80   14:52

L7.2 (without object)
CH_3
Mean: 8.7
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_4
Mean: 0.051
Acceptable range: 2.5
Failure points: 0%

14:53:28.00   14:53:43.72   14:53:59.45   14:54:15.17

14:53:28.00   14:53:43.72   14:53:59.45   14:54:15.17

Database: D:\Projects_QCReports_Ord_Data\111309\QC\111309_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

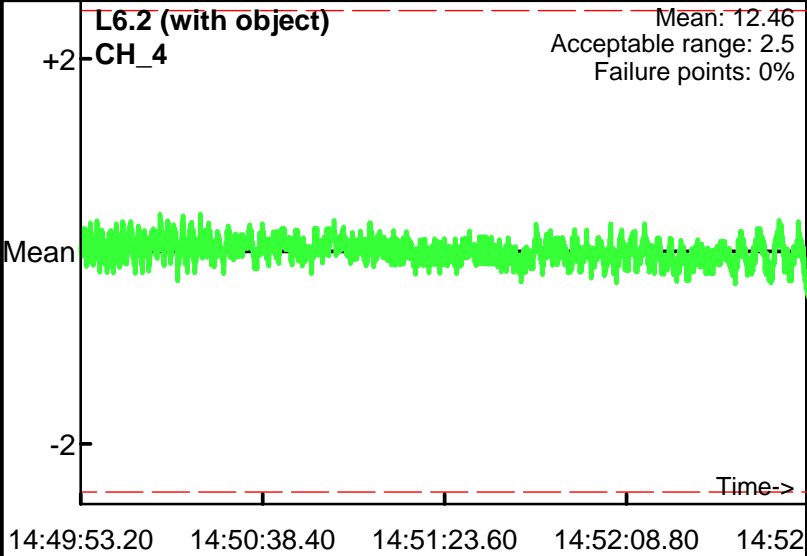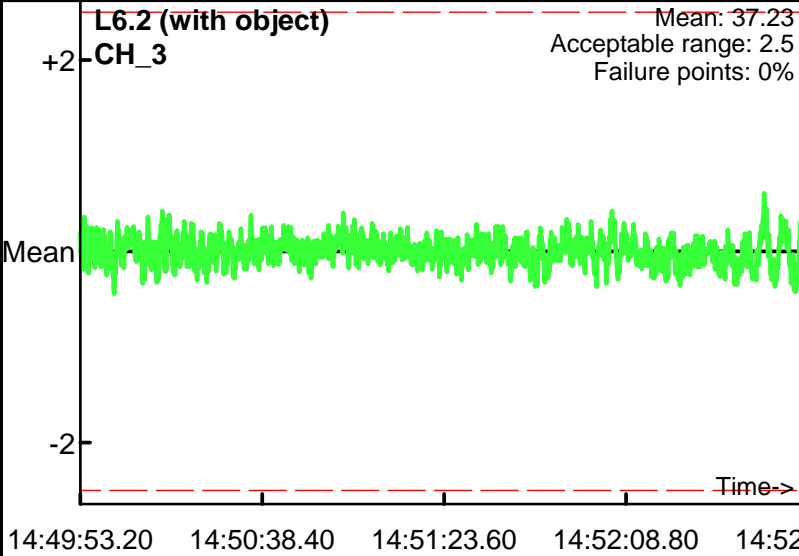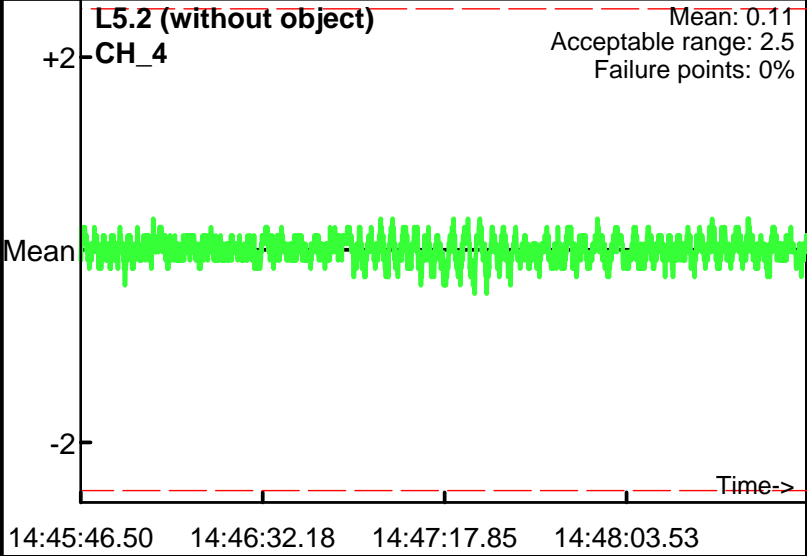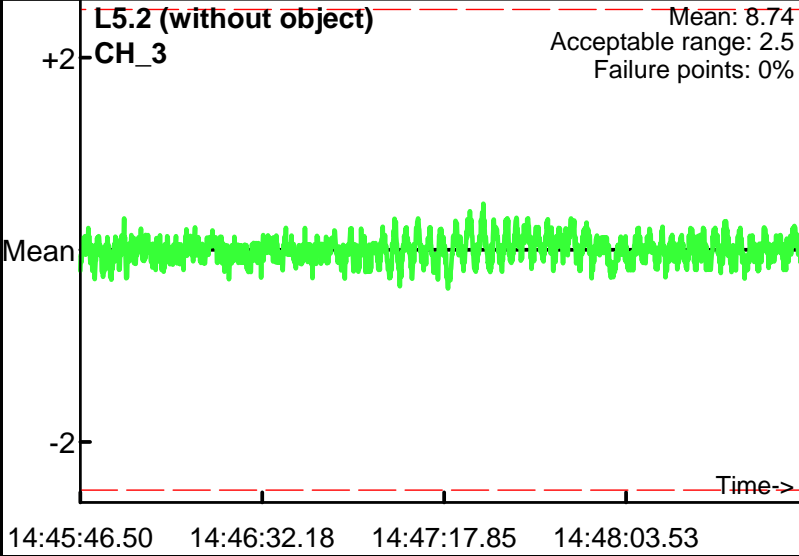● Outside range
– – Acceptable limits

AM test
Operator: PN & BR
Date: 11/30/2009

L0 (without object)
CH_1
Mean: -37.28
Acceptable range: 2.5
Failure points: 0%

Time->

14:19:50.08   14:20:36.78   14:21:23.48   14:22:10.18   14:22

L0 (without object)
CH_2
Mean: 8.11
Acceptable range: 2.5
Failure points: 0%

Time->

14:19:50.08   14:20:36.78   14:21:23.48   14:22:10.18   14:22

L1 (with object)
CH_1
Mean: 57.81
Acceptable range: 2.5
Failure points: 0%

Time->

14:23:47.89   14:24:33.81   14:25:19.73   14:26:05.66   14:26

L1 (with object)
CH_2
Mean: 66.89
Acceptable range: 2.5
Failure points: 0%

Time->

14:23:47.89   14:24:33.81   14:25:19.73   14:26:05.66   14:26

L2 (without object)
CH_1
Mean: -37.67
Acceptable range: 2.5
Failure points: 0%

Time->

14:27:30.69   14:27:46.14   14:28:01.59   14:28:17.03

L2 (without object)
CH_2
Mean: 7.86
Acceptable range: 2.5
Failure points: 0%

Time->

14:27:30.69   14:27:46.14   14:28:01.59   14:28:17.03

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
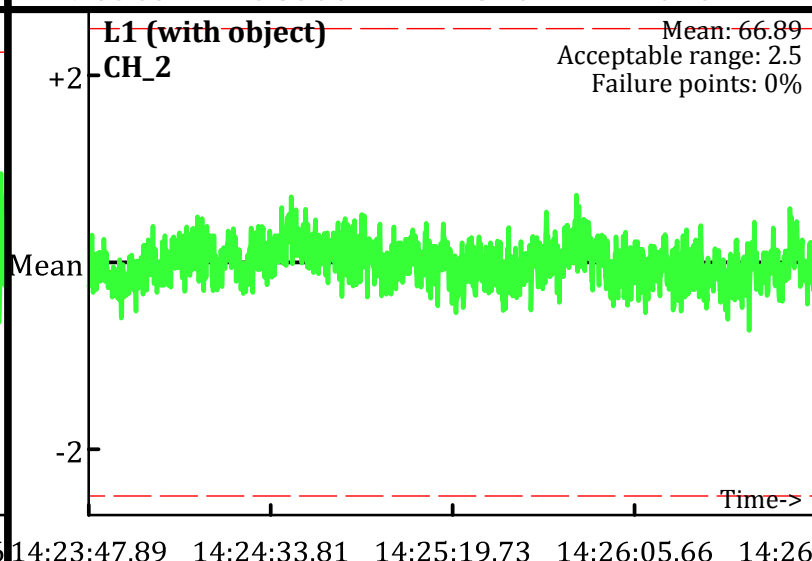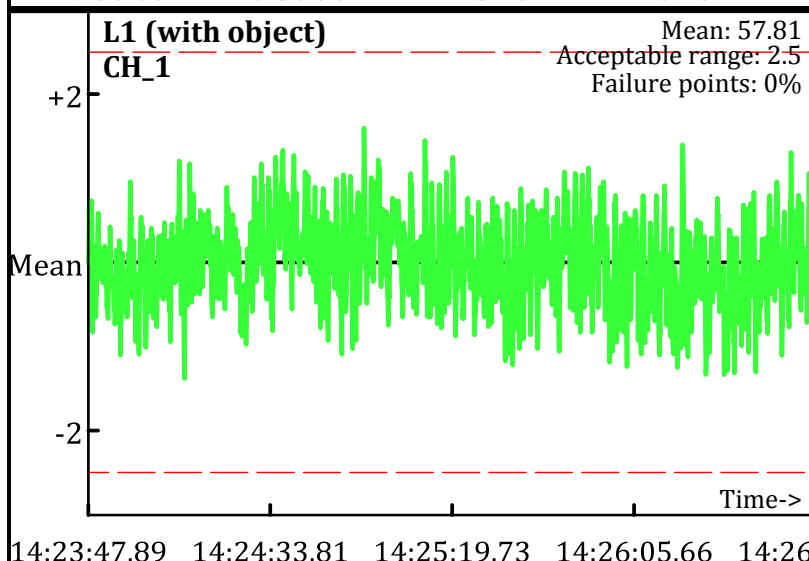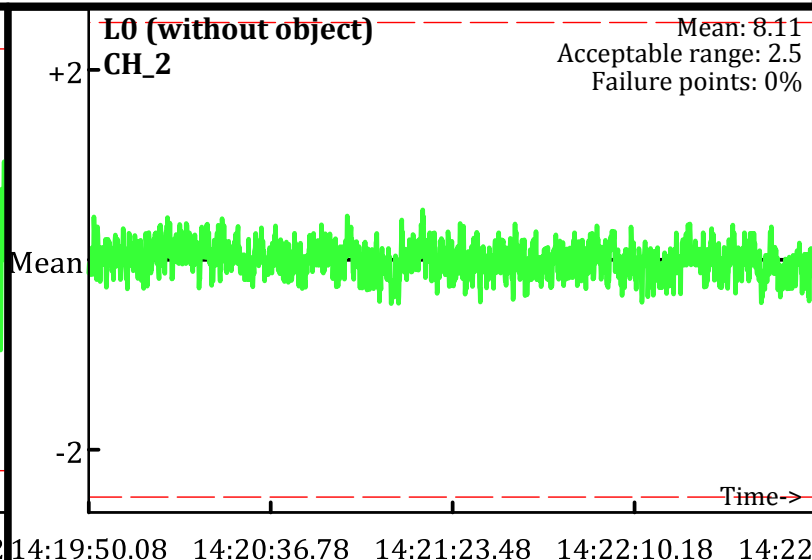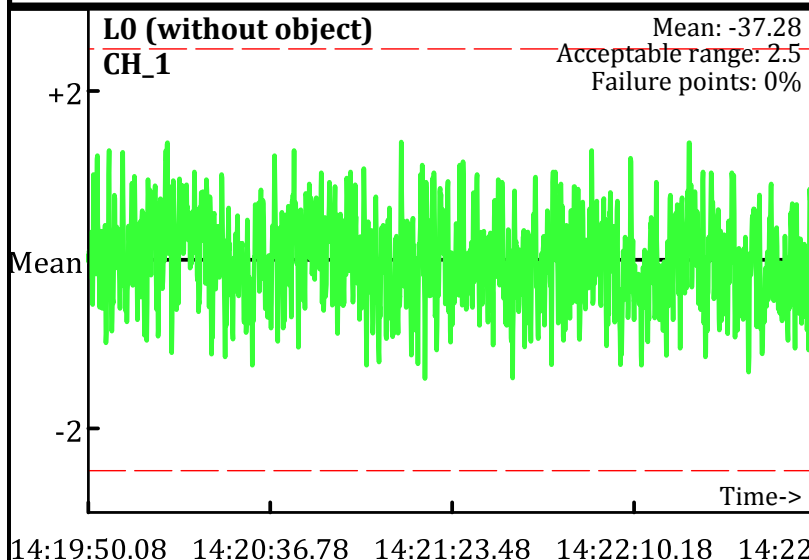Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
Date: 11/30/2009

L0 (without object)
CH_3

Mean: 6.58
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:19:50.08　14:20:36.78　14:21:23.48　14:22:10.18　14:22

L0 (without object)
CH_4

Mean: -1.48
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:19:50.08　14:20:36.78　14:21:23.48　14:22:10.18　14:22

L1 (with object)
CH_3

Mean: 37.09
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:23:47.89　14:24:33.81　14:25:19.73　14:26:05.66　14:26

L1 (with object)
CH_4

Mean: 11.86
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:23:47.89　14:24:33.81　14:25:19.73　14:26:05.66　14:26

L2 (without object)
CH_3

Mean: 6.54
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:27:30.69　14:27:46.14　14:28:01.59　14:28:17.03

L2 (without object)
CH_4

Mean: -1.51
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

14:27:30.69　14:27:46.14　14:28:01.59　14:28:17.03

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L0 L1 L2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
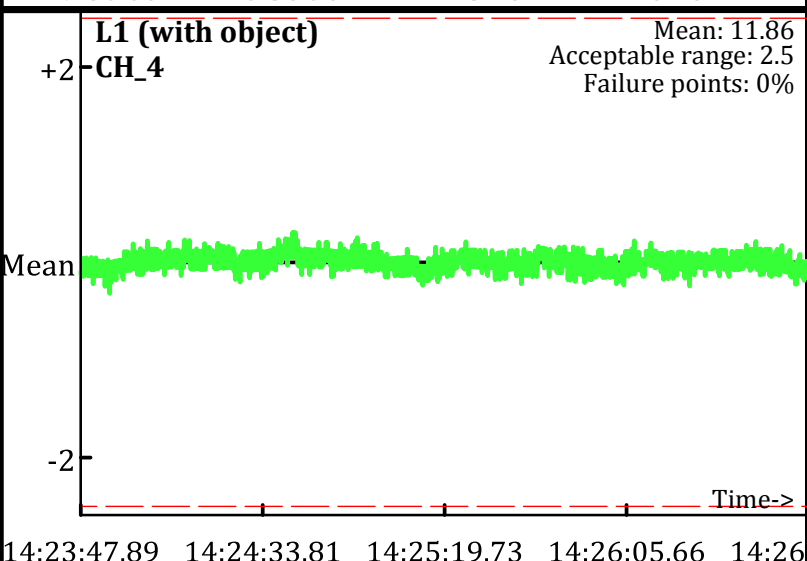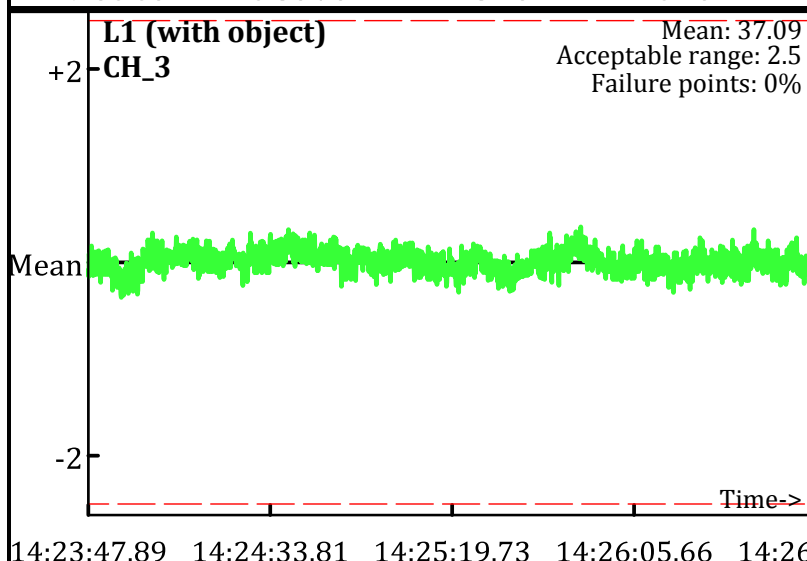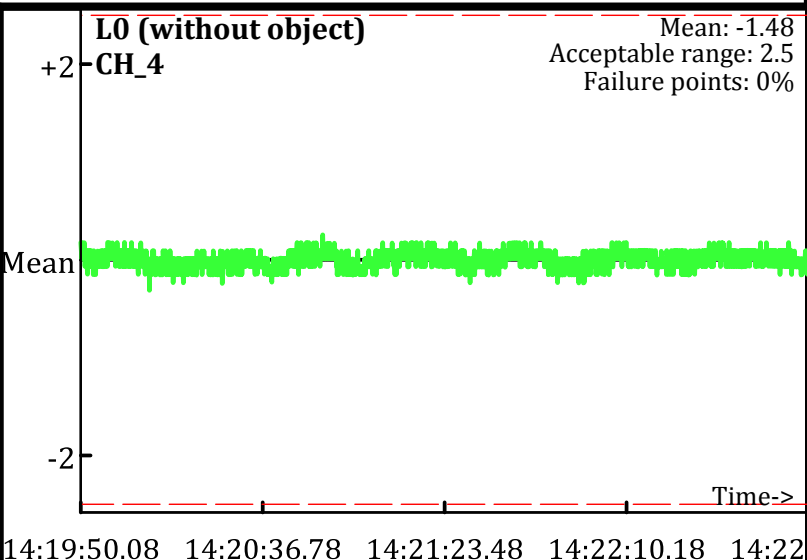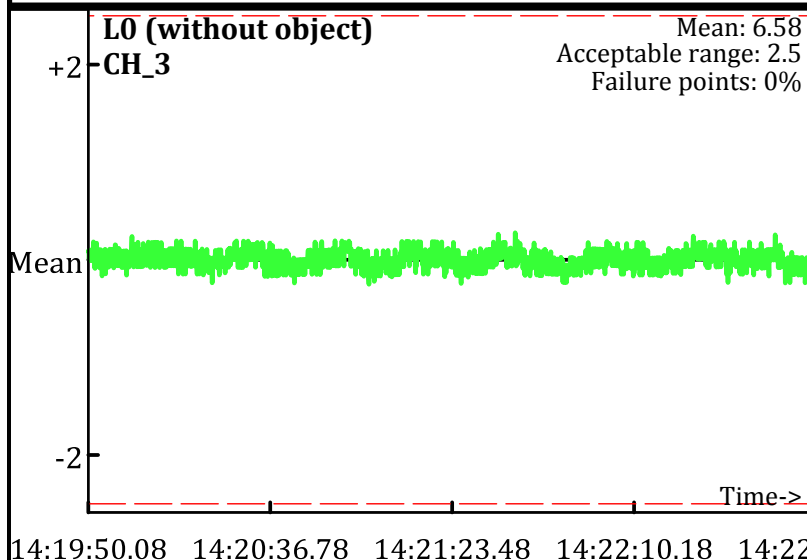Grid/Location: QC Area

● Outside range
-- -- Acceptable limits

AM test
Operator: PN & BR
Date: 11/30/2009

L0.1 (without object) CH_1 — Mean: -70.32, Acceptable range: 2.5, Failure points: 0%

L0.1 (without object) CH_2 — Mean: 11.63, Acceptable range: 2.5, Failure points: 0%

L1.1 (with object) CH_1 — Mean: 48.6, Acceptable range: 2.5, Failure points: 0%

L1.1 (with object) CH_2 — Mean: 101.06, Acceptable range: 2.5, Failure points: 0%

L2.1 (without object) CH_1 — Mean: -70.58, Acceptable range: 2.5, Failure points: 0%

L2.1 (without object) CH_2 — Mean: 11.33, Acceptable range: 2.5, Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

L0.1 (without object)
CH_3
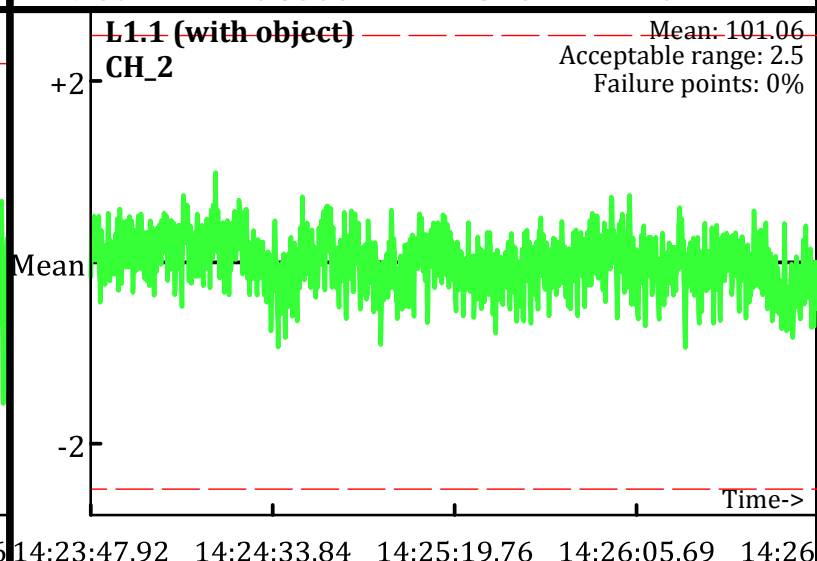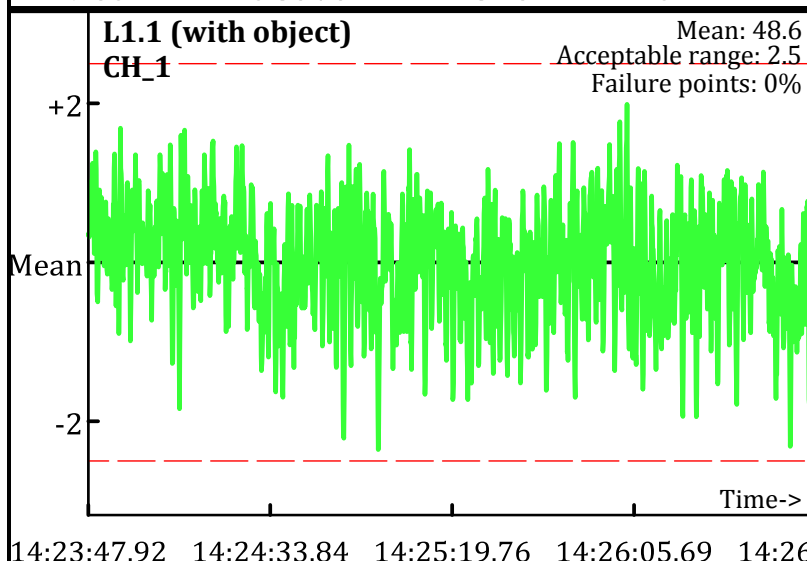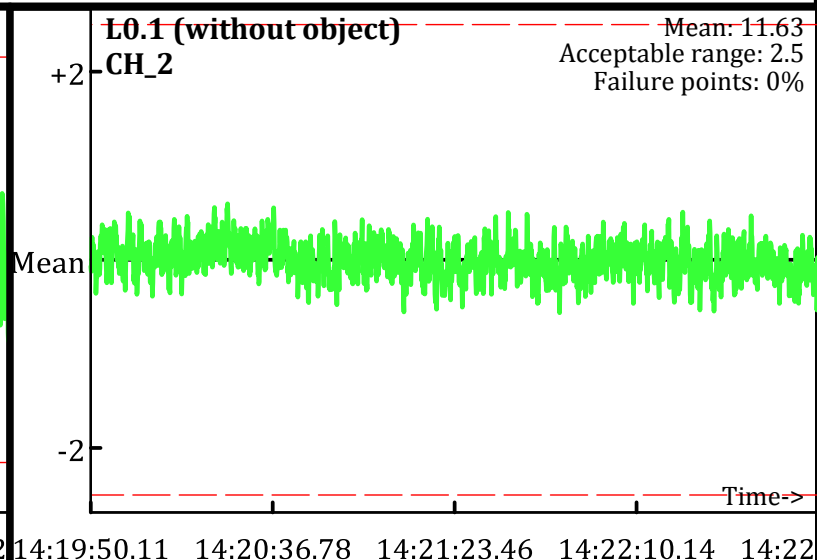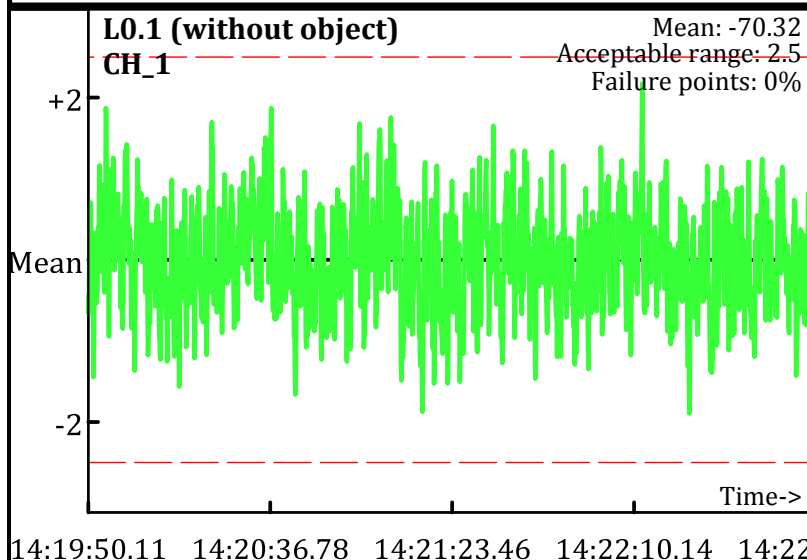Mean: 14.23
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:19:50.11   14:20:36.78   14:21:23.46   14:22:10.14   14:22

L0.1 (without object)
CH_4
Mean: 3.43
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:19:50.11   14:20:36.78   14:21:23.46   14:22:10.14   14:22

L1.1 (with object)
CH_3
Mean: 71.46
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:23:47.92   14:24:33.84   14:25:19.76   14:26:05.69   14:26

L1.1 (with object)
CH_4
Mean: 34.03
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:23:47.92   14:24:33.84   14:25:19.76   14:26:05.69   14:26

L2.1 (without object)
CH_3
Mean: 14.12
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:27:30.72   14:27:46.17   14:28:01.62   14:28:17.07

L2.1 (without object)
CH_4
Mean: 3.31
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:27:30.72   14:27:46.17   14:28:01.62   14:28:17.07

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
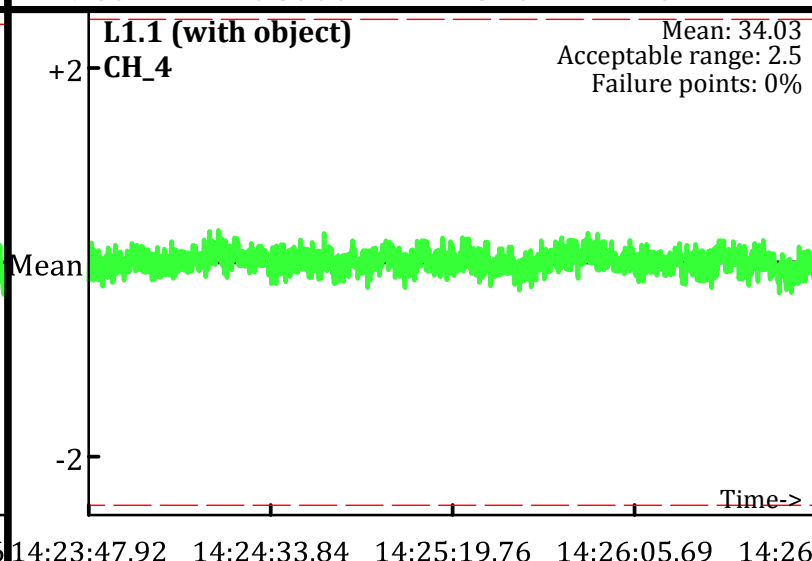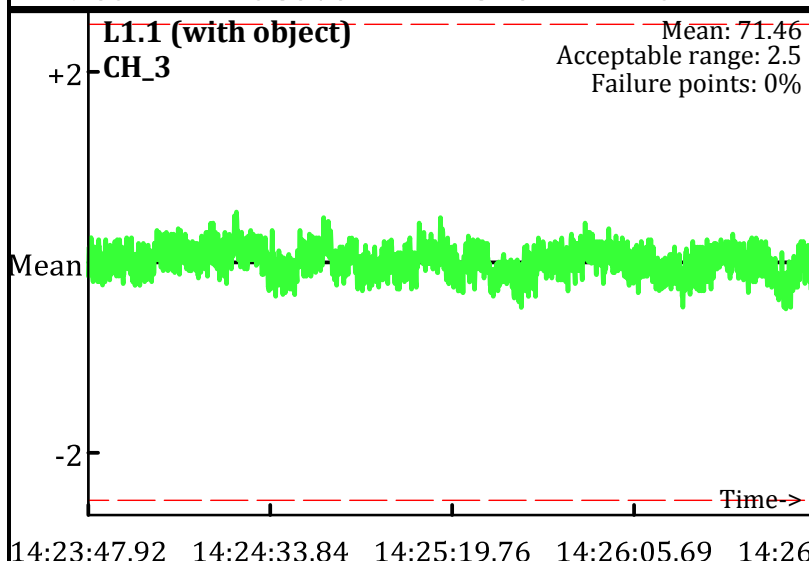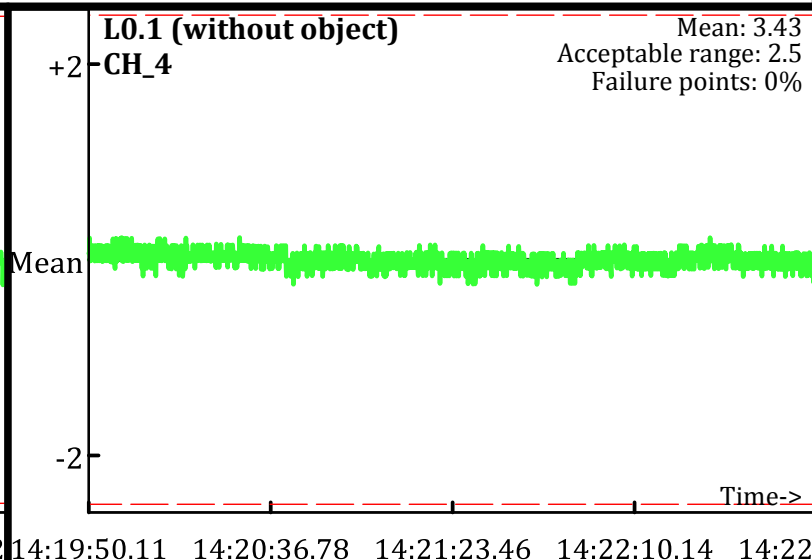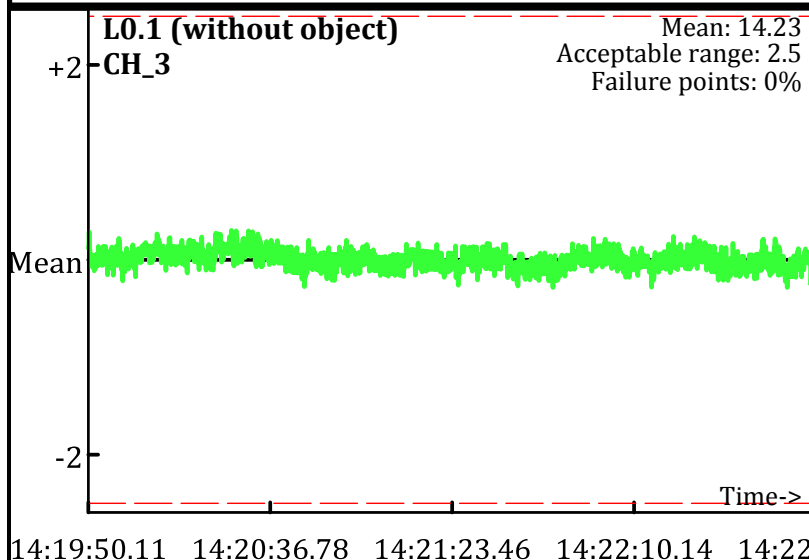Grid/Location: QC Area

● Outside range
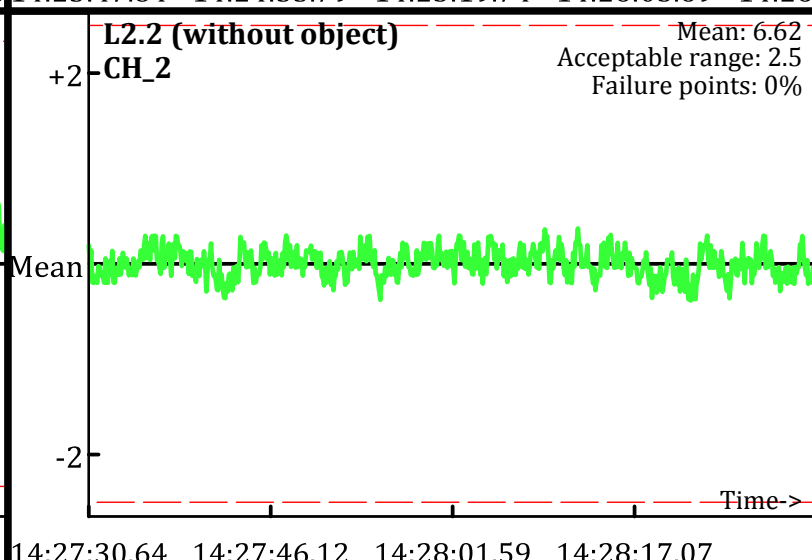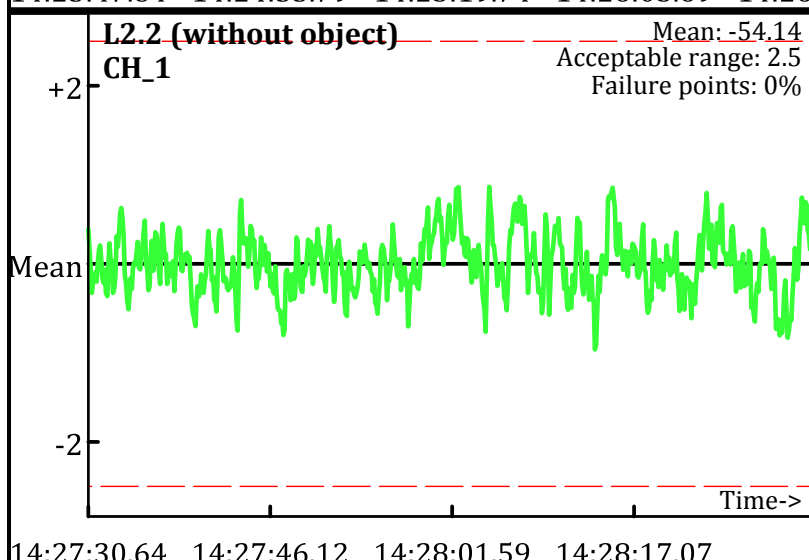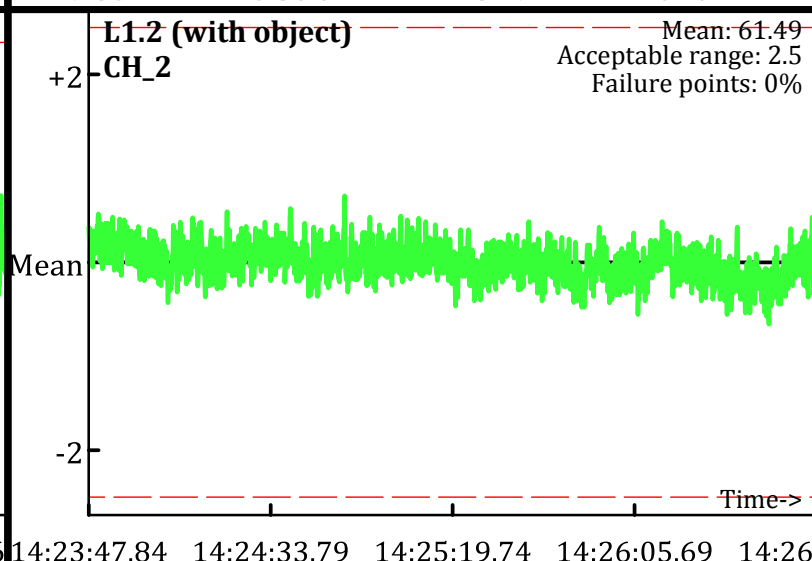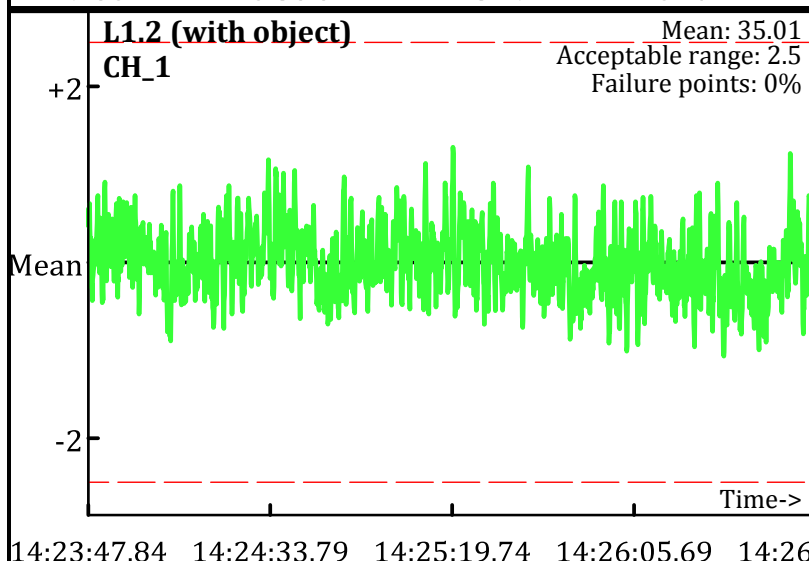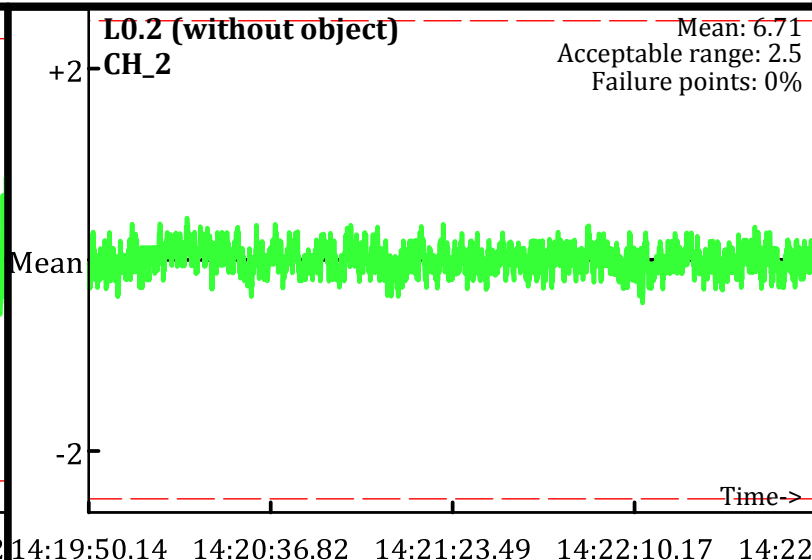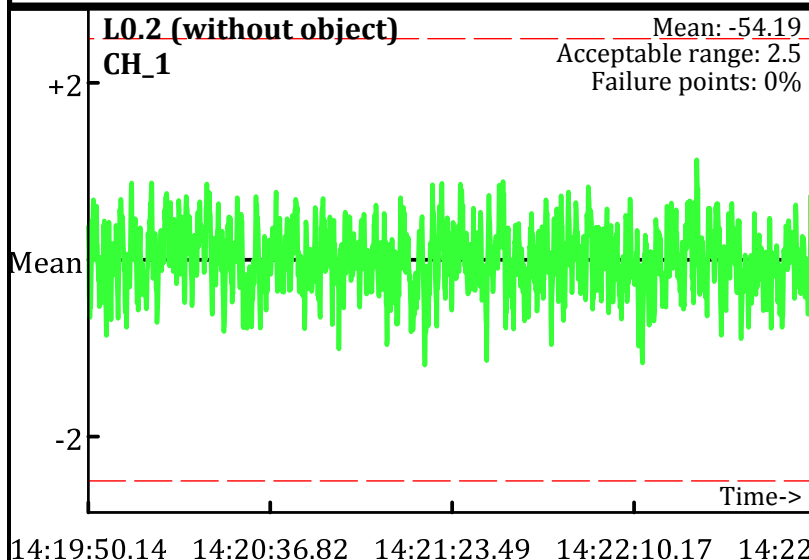--- Acceptable limits

AM test
Operator: PN & BR
Date: 11/30/2009

L0.2 (without object) CH_1 — Mean: -54.19, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:19:50.14 · 14:20:36.82 · 14:21:23.49 · 14:22:10.17 · 14:22

L0.2 (without object) CH_2 — Mean: 6.71, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:19:50.14 · 14:20:36.82 · 14:21:23.49 · 14:22:10.17 · 14:22

L1.2 (with object) CH_1 — Mean: 35.01, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:23:47.84 · 14:24:33.79 · 14:25:19.74 · 14:26:05.69 · 14:26

L1.2 (with object) CH_2 — Mean: 61.49, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:23:47.84 · 14:24:33.79 · 14:25:19.74 · 14:26:05.69 · 14:26

L2.2 (without object) CH_1 — Mean: -54.14, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:27:30.64 · 14:27:46.12 · 14:28:01.59 · 14:28:17.07

L2.2 (without object) CH_2 — Mean: 6.62, Acceptable range: 2.5, Failure points: 0%
Time axis: 14:27:30.64 · 14:27:46.12 · 14:28:01.59 · 14:28:17.07

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

● Outside range
– – Acceptable limits

L0.2 (without object)
CH_3
Mean: 6.82
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:19:50.14   14:20:36.82   14:21:23.49   14:22:10.17   14:22

L0.2 (without object)
CH_4
Mean: -0.51
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:19:50.14   14:20:36.82   14:21:23.49   14:22:10.17   14:22

L1.2 (with object)
CH_3
Mean: 34.91
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:23:47.84   14:24:33.79   14:25:19.74   14:26:05.69   14:26

L1.2 (with object)
CH_4
Mean: 11.56
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:23:47.84   14:24:33.79   14:25:19.74   14:26:05.69   14:26

L2.2 (without object)
CH_3
Mean: 6.8
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:27:30.64   14:27:46.12   14:28:01.59   14:28:17.07

L2.2 (without object)
CH_4
Mean: -0.54
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:27:30.64   14:27:46.12   14:28:01.59   14:28:17.07

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
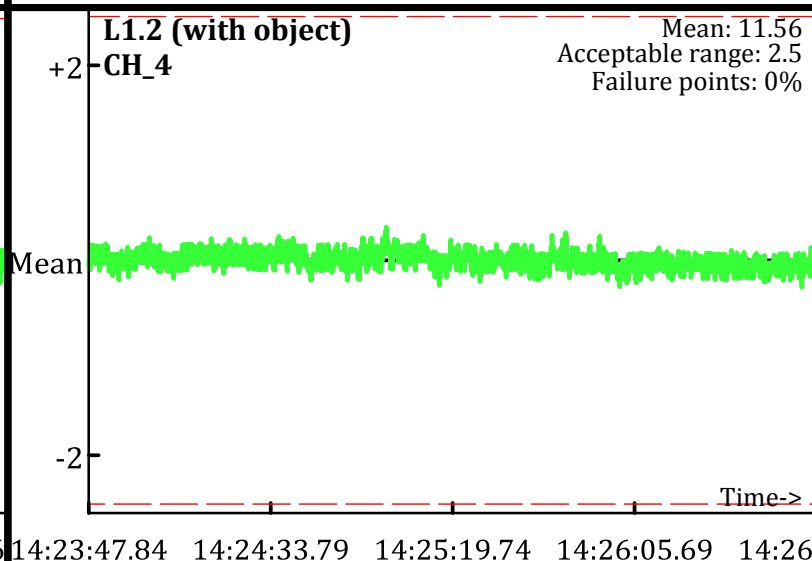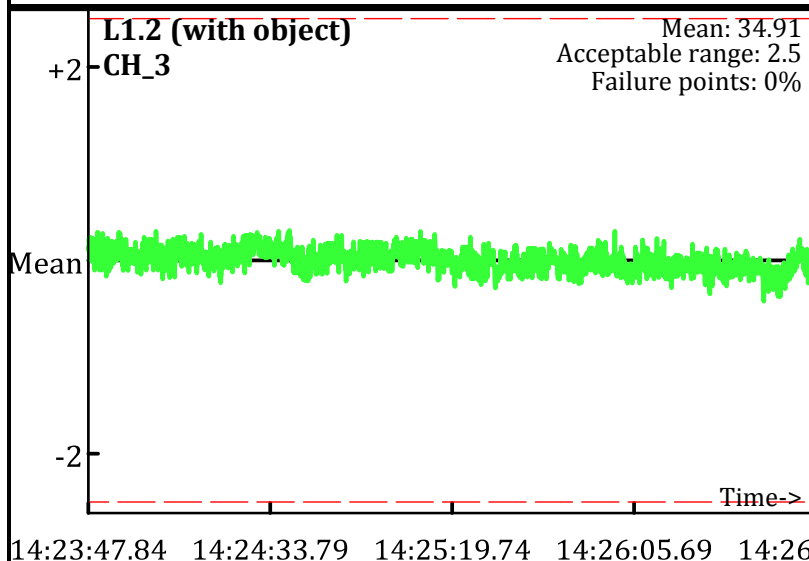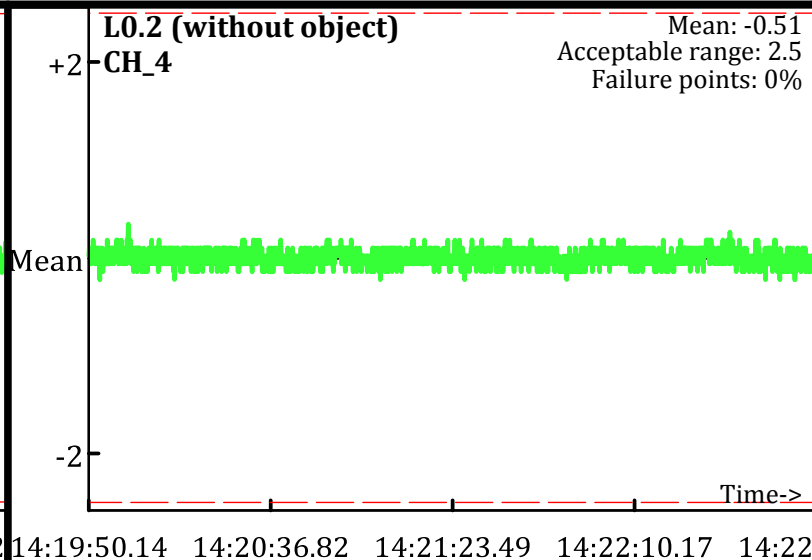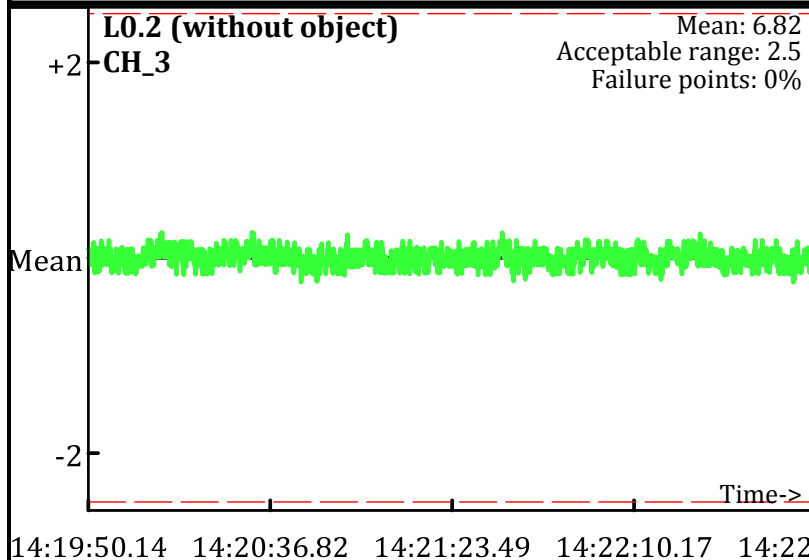Grid/Location: QC Area

● Outside range
– – – Acceptable limits

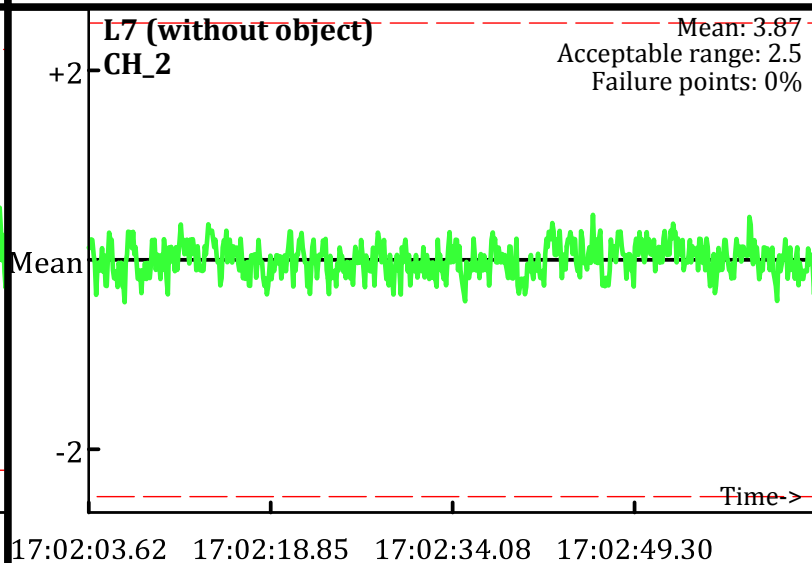PM test
Operator: PN & BR
Date: 11/30/2009

L5 (without object) CH_1 — Mean: -47.99, Acceptable range: 2.5, Failure points: 0%

L5 (without object) CH_2 — Mean: 3.88, Acceptable range: 2.5, Failure points: 0%

L6 (with object) CH_1 — Mean: 47.03, Acceptable range: 2.5, Failure points: 0%

L6 (with object) CH_2 — Mean: 63.01, Acceptable range: 2.5, Failure points: 0%

L7 (without object) CH_1 — Mean: -48.74, Acceptable range: 2.5, Failure points: 0%

L7 (without object) CH_2 — Mean: 3.87, Acceptable range: 2.5, Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits
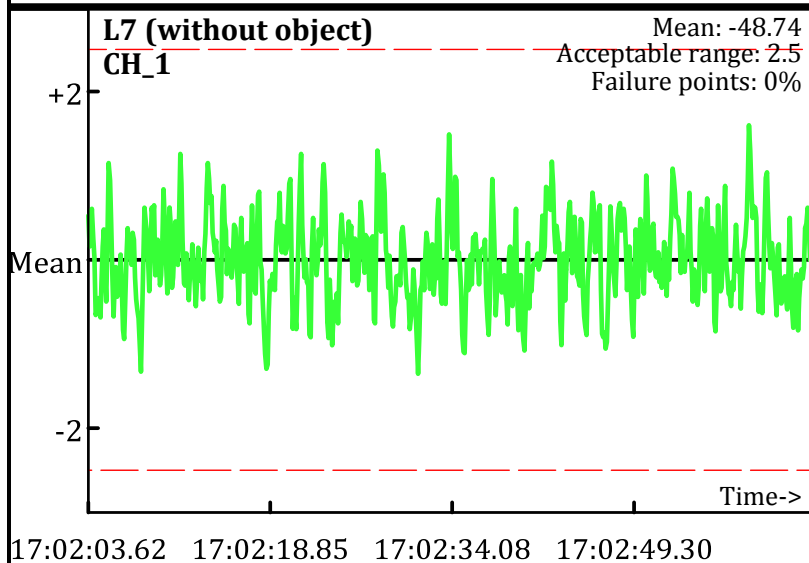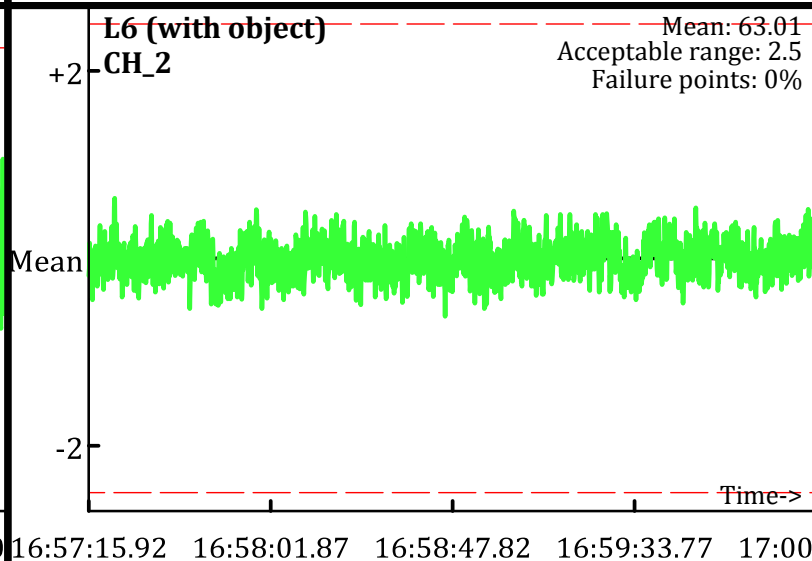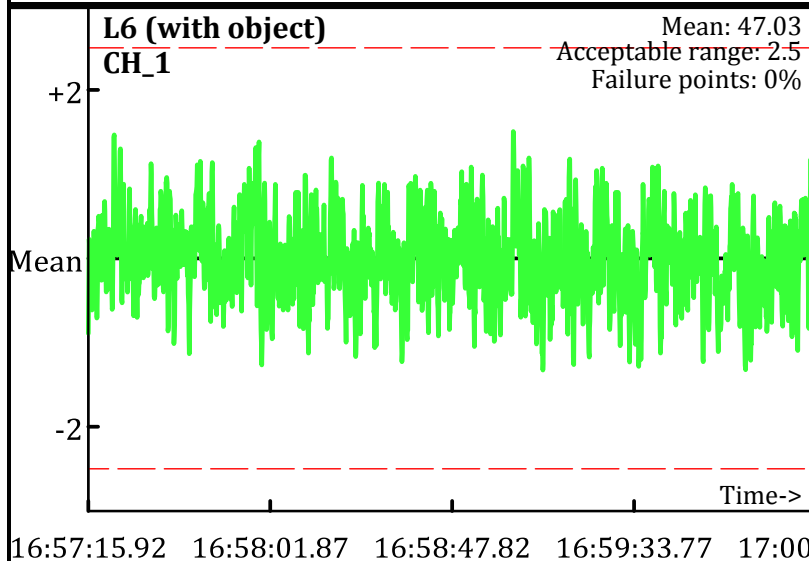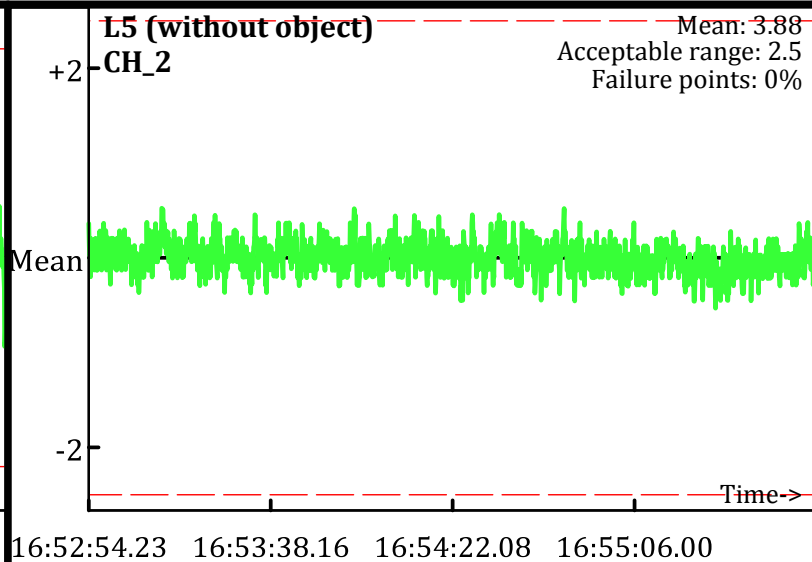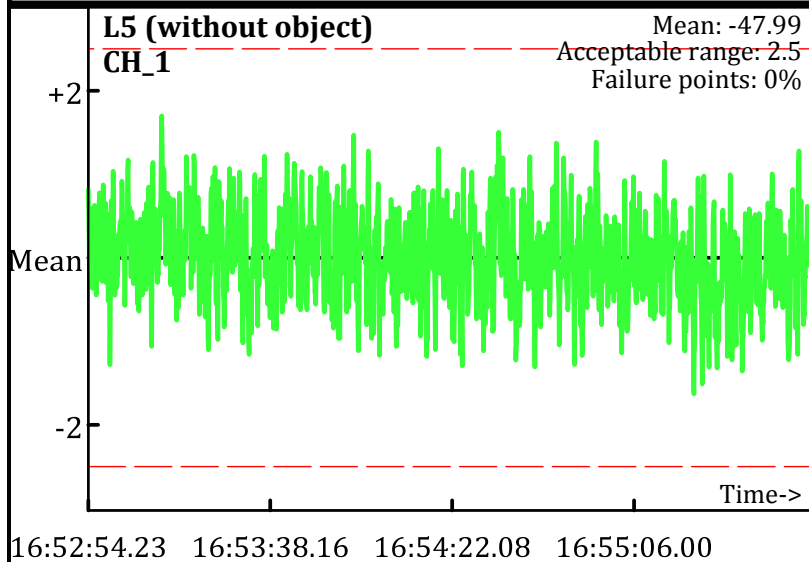
PM test
Operator: PN & BR
Date: 11/30/2009

L5 (without object)
CH_3
Mean: 5.21
Acceptable range: 2.5
Failure points: 0%

16:52:54.23   16:53:38.16   16:54:22.08   16:55:06.00

L5 (without object)
CH_4
Mean: -2.09
Acceptable range: 2.5
Failure points: 0%

16:52:54.23   16:53:38.16   16:54:22.08   16:55:06.00

L6 (with object)
CH_3
Mean: 36.07
Acceptable range: 2.5
Failure points: 0%

16:57:15.92   16:58:01.87   16:58:47.82   16:59:33.77   17:00

L6 (with object)
CH_4
Mean: 11.45
Acceptable range: 2.5
Failure points: 0%

16:57:15.92   16:58:01.87   16:58:47.82   16:59:33.77   17:00

L7 (without object)
CH_3
Mean: 5.39
Acceptable range: 2.5
Failure points: 0%

17:02:03.62   17:02:18.85   17:02:34.08   17:02:49.30

L7 (without object)
CH_4
Mean: -1.97
Acceptable range: 2.5
Failure points: 0%

17:02:03.62   17:02:18.85   17:02:34.08   17:02:49.30

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L5 L6 L7

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/30/2009
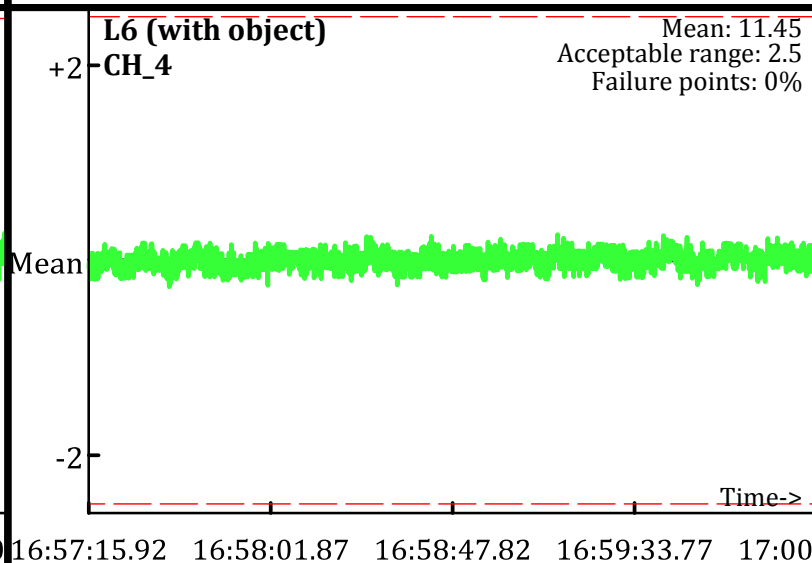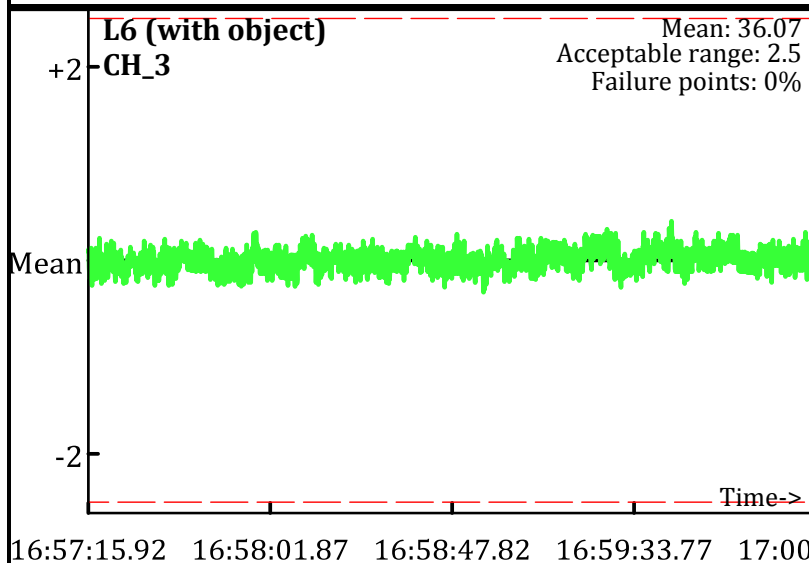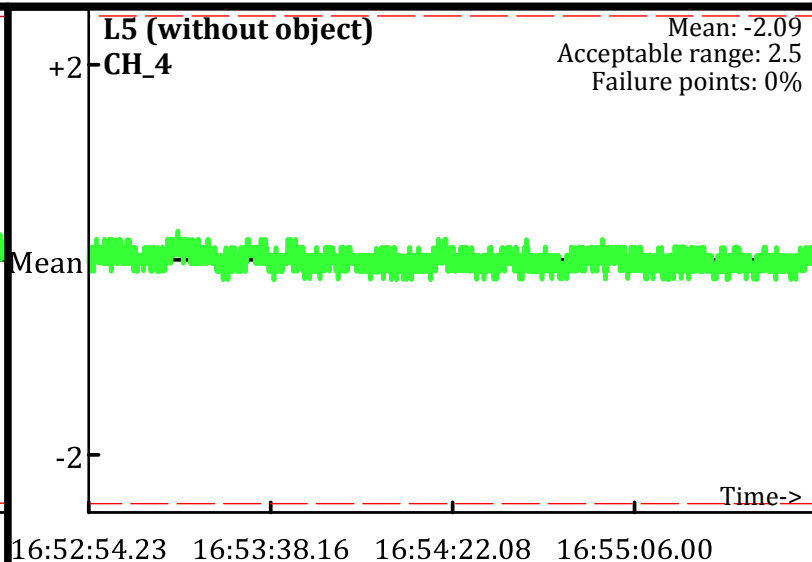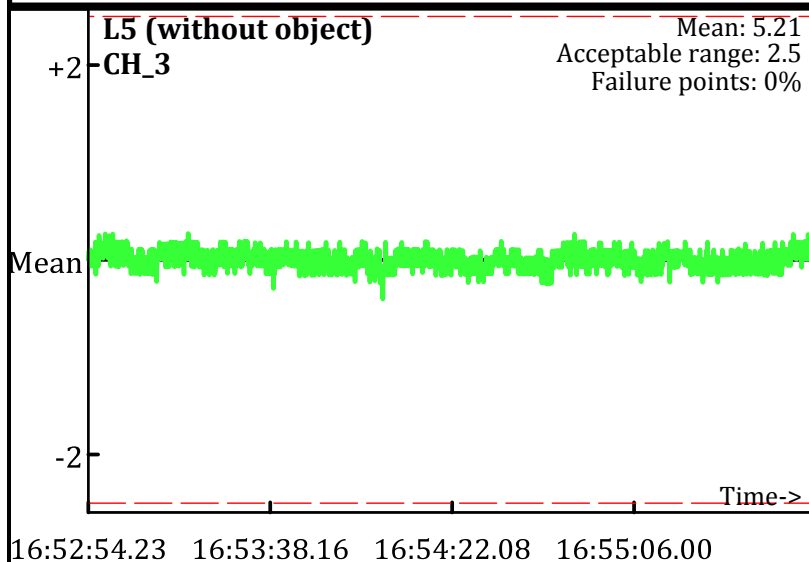

L5.1 (without object)
CH_1
Mean: -76.23
Acceptable range: 2.5
Failure points: 0%

L5.1 (without object)
CH_2
Mean: 9.89
Acceptable range: 2.5
Failure points: 0%

16:52:54.26   16:53:38.19   16:54:22.12   16:55:06.04

L6.1 (with object)
CH_1
Mean: 46.26
Acceptable range: 2.5
Failure points: 0.0544%

L6.1 (with object)
CH_2
Mean: 102.45
Acceptable range: 2.5
Failure points: 0%

16:57:15.97   16:58:01.89   16:58:47.81   16:59:33.73   17:00

L7.1 (without object)
CH_1
Mean: -77.89
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_2
Mean: 9.68
Acceptable range: 2.5
Failure points: 0%

17:02:03.66   17:02:18.88   17:02:34.11   17:02:49.34

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L5.1 L6.1 L7.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits
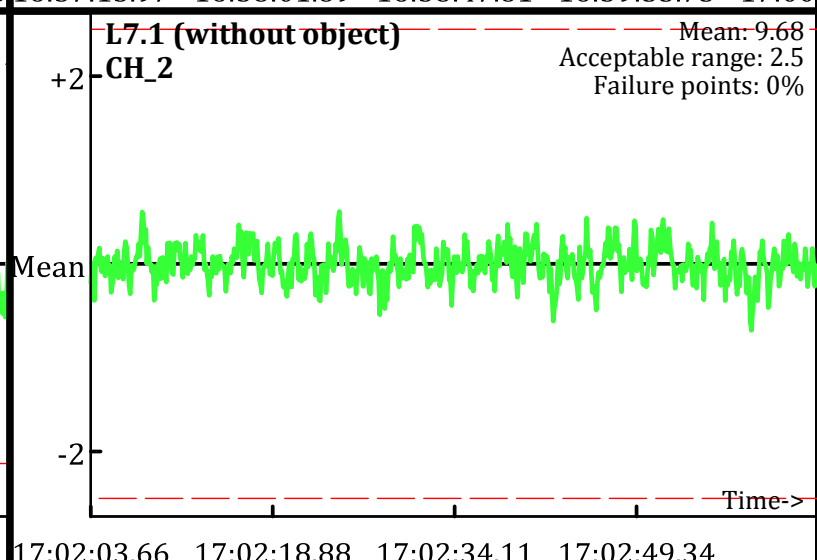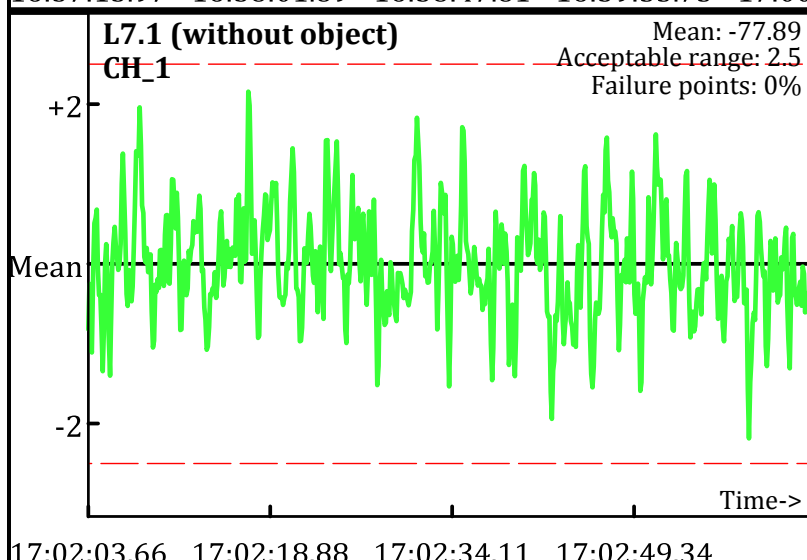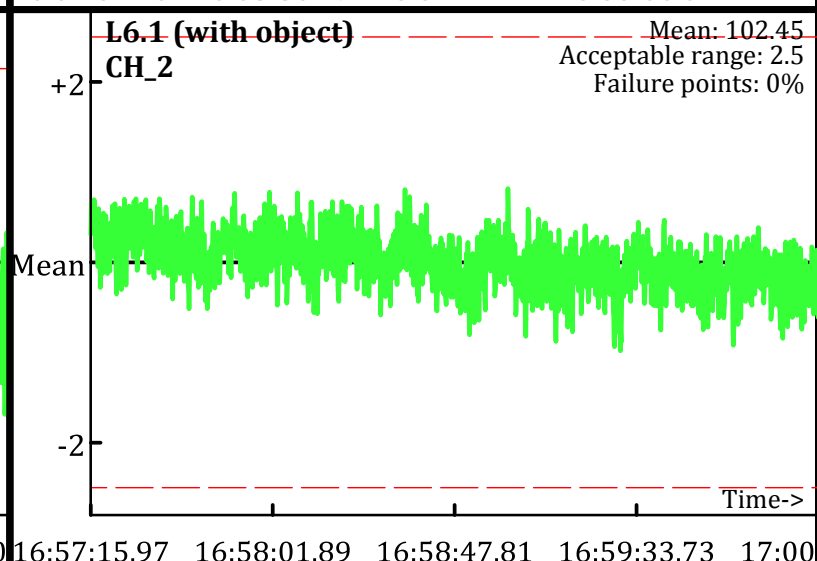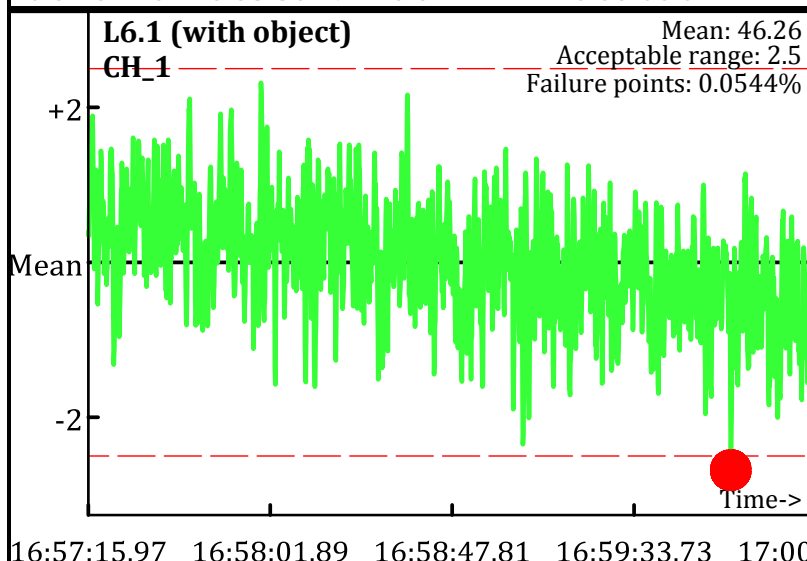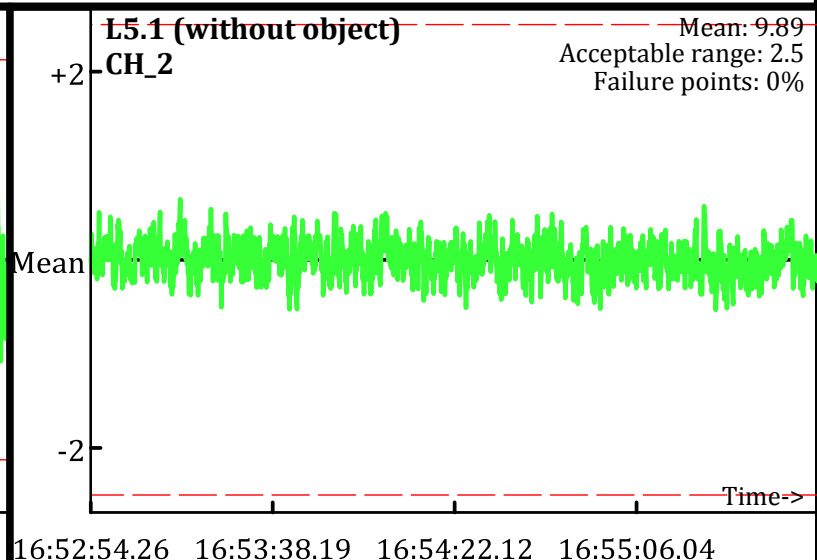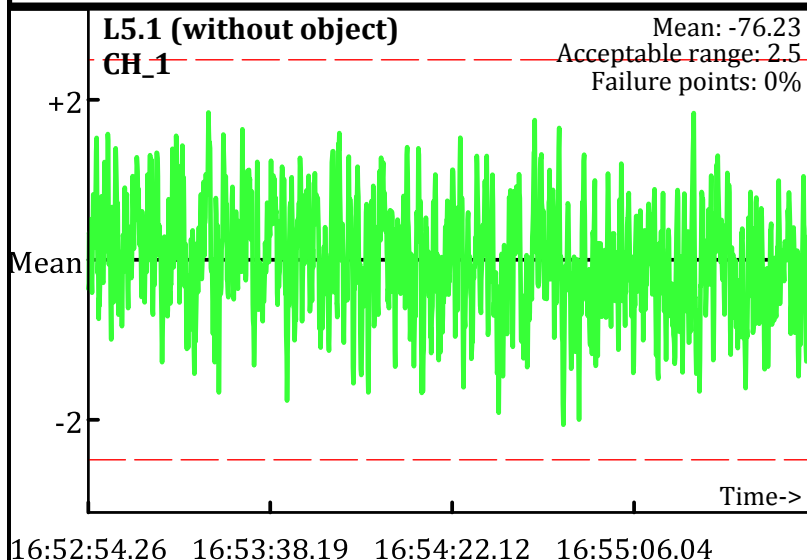
PM test
Operator: PN & BR
Date: 11/30/2009

L5.1 (without object) CH_3 — Mean: 13.76, Acceptable range: 2.5, Failure points: 0%
Time-> 16:52:54.26 16:53:38.19 16:54:22.12 16:55:06.04

L5.1 (without object) CH_4 — Mean: 3.07, Acceptable range: 2.5, Failure points: 0%
Time-> 16:52:54.26 16:53:38.19 16:54:22.12 16:55:06.04

L6.1 (with object) CH_3 — Mean: 72.96, Acceptable range: 2.5, Failure points: 0%
Time-> 16:57:15.97 16:58:01.89 16:58:47.81 16:59:33.73 17:00

L6.1 (with object) CH_4 — Mean: 34.66, Acceptable range: 2.5, Failure points: 0%
Time-> 16:57:15.97 16:58:01.89 16:58:47.81 16:59:33.73 17:00

L7.1 (without object) CH_3 — Mean: 13.9, Acceptable range: 2.5, Failure points: 0%
Time-> 17:02:03.66 17:02:18.88 17:02:34.11 17:02:49.34

L7.1 (without object) CH_4 — Mean: 3.13, Acceptable range: 2.5, Failure points: 0%
Time-> 17:02:03.66 17:02:18.88 17:02:34.11 17:02:49.34

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
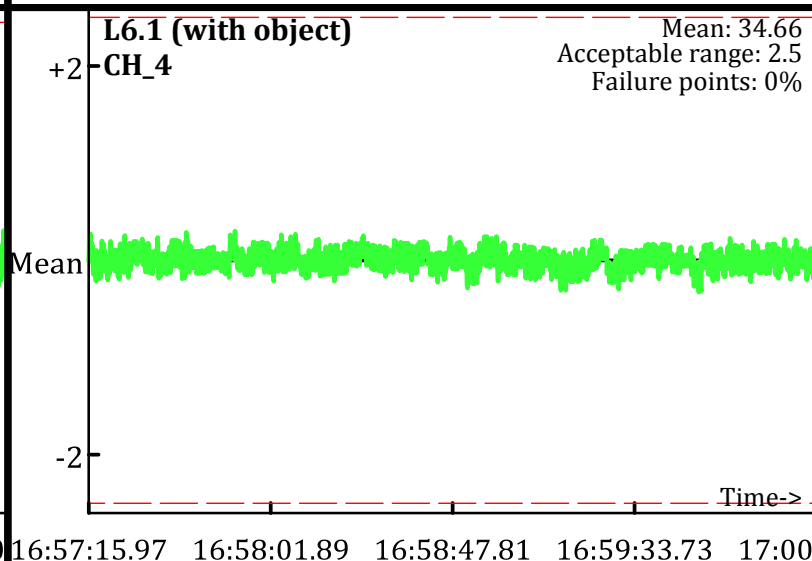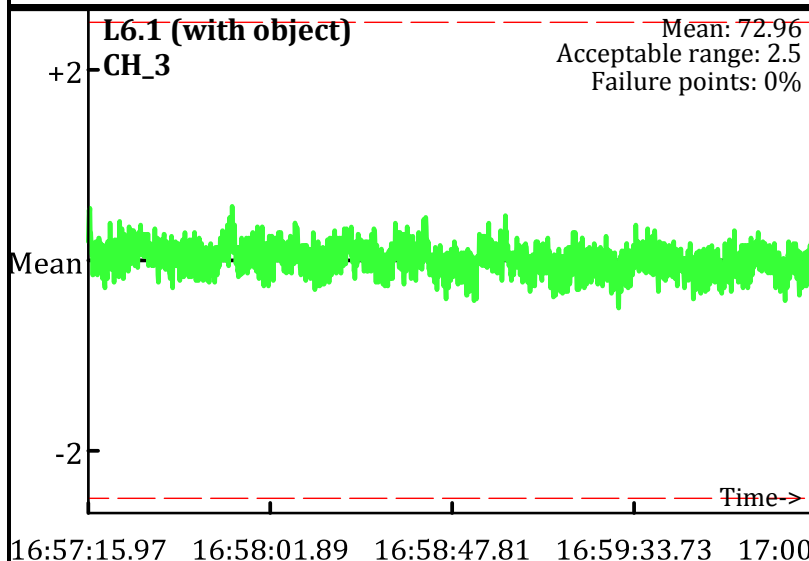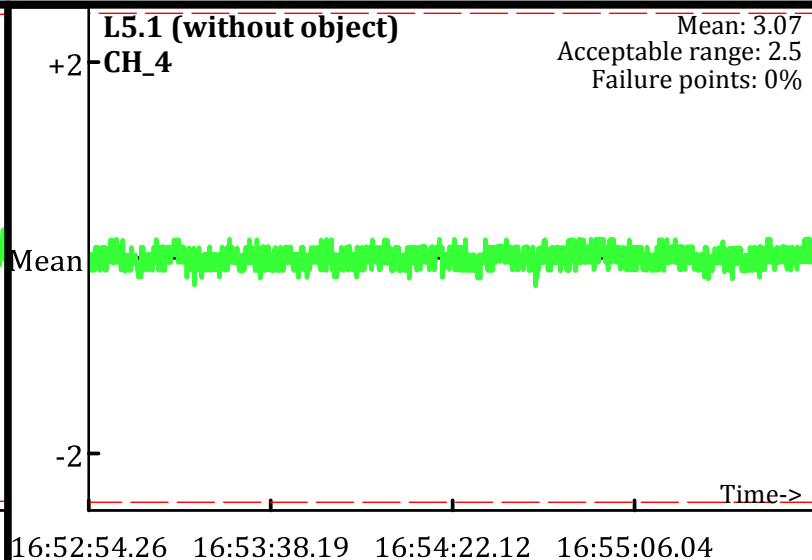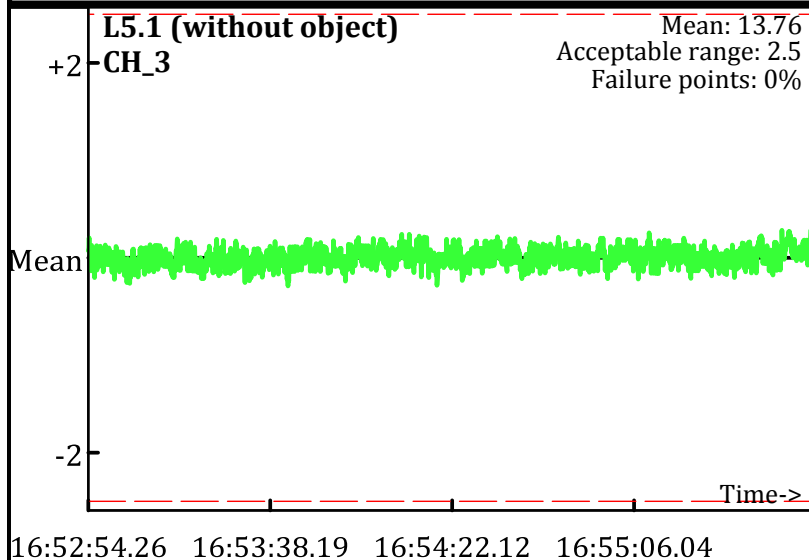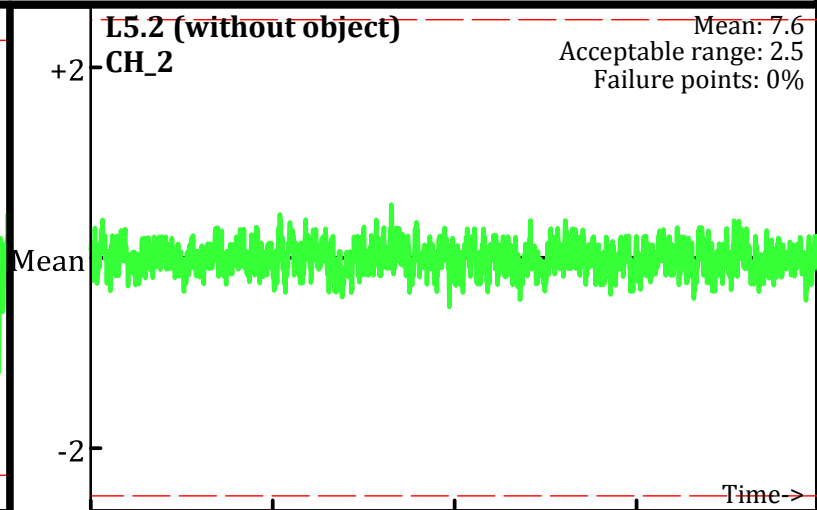Line Name: L5.1 L6.1 L7.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/30/2009

L5.2 (without object)
CH_1
Mean: -57.38
Acceptable range: 2.5
Failure points: 0%

Time->

16:52:54.19   16:53:38.14   16:54:22.09   16:55:06.03

L5.2 (without object)
CH_2
Mean: 7.6
Acceptable range: 2.5
Failure points: 0%

Time->

16:52:54.19   16:53:38.14   16:54:22.09   16:55:06.03

L6.2 (with object)
CH_1
Mean: 32.53
Acceptable range: 2.5
Failure points: 0%

Time->

16:57:15.98   16:58:01.91   16:58:47.84   16:59:33.76

L6.2 (with object)
CH_2
Mean: 63.42
Acceptable range: 2.5
Failure points: 0%

Time->

16:57:15.98   16:58:01.91   16:58:47.84   16:59:33.76

L7.2 (without object)
CH_1
Mean: -58.67
Acceptable range: 2.5
Failure points: 0%

Time->

17:02:03.69   17:02:18.89   17:02:34.09   17:02:49.28   17:03

L7.2 (without object)
CH_2
Mean: 7.44
Acceptable range: 2.5
Failure points: 0%

Time->

17:02:03.69   17:02:18.89   17:02:34.09   17:02:49.28   17:03

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
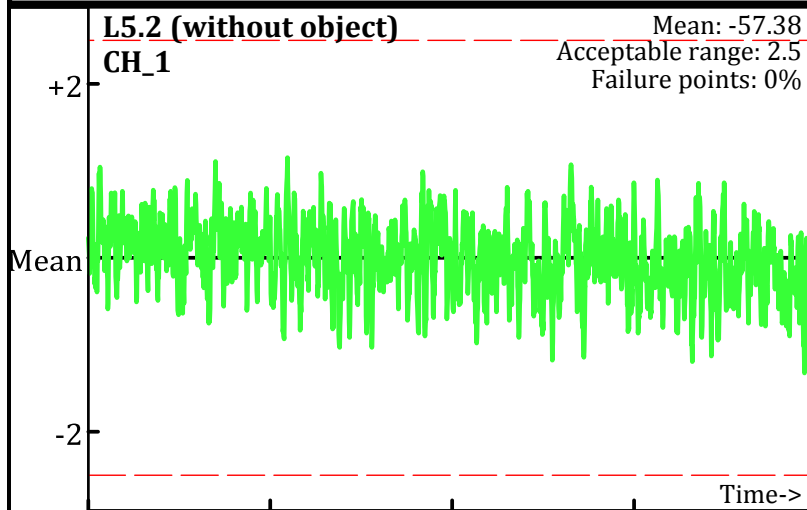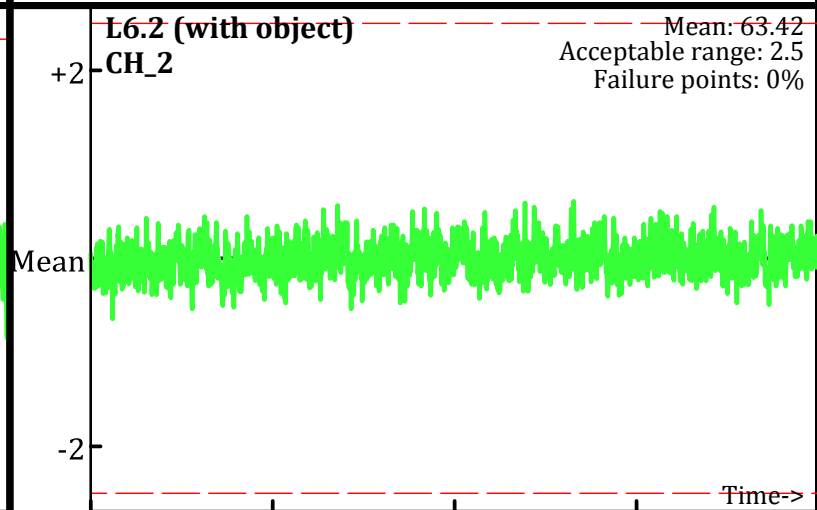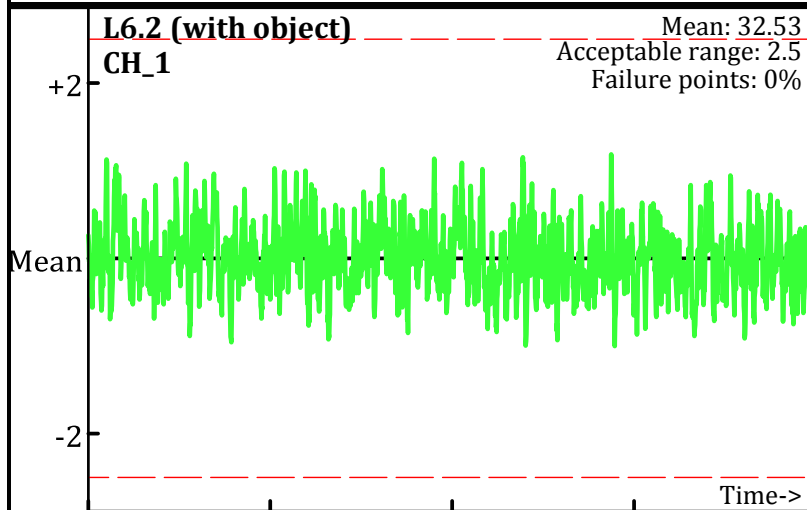– – – Acceptable limits

PM test
Operator: PN & BR
Date: 11/30/2009

L5.2 (without object)
CH_3
Mean: 7.8
Acceptable range: 2.5
Failure points: 0%

Time->

16:52:54.19   16:53:38.14   16:54:22.09   16:55:06.03

L5.2 (without object)
CH_4
Mean: -0.14
Acceptable range: 2.5
Failure points: 0%

Time->

16:52:54.19   16:53:38.14   16:54:22.09   16:55:06.03

L6.2 (with object)
CH_3
Mean: 36.61
Acceptable range: 2.5
Failure points: 0%

Time->

16:57:15.98   16:58:01.91   16:58:47.84   16:59:33.76

L6.2 (with object)
CH_4
Mean: 12.3
Acceptable range: 2.5
Failure points: 0%

Time->

16:57:15.98   16:58:01.91   16:58:47.84   16:59:33.76
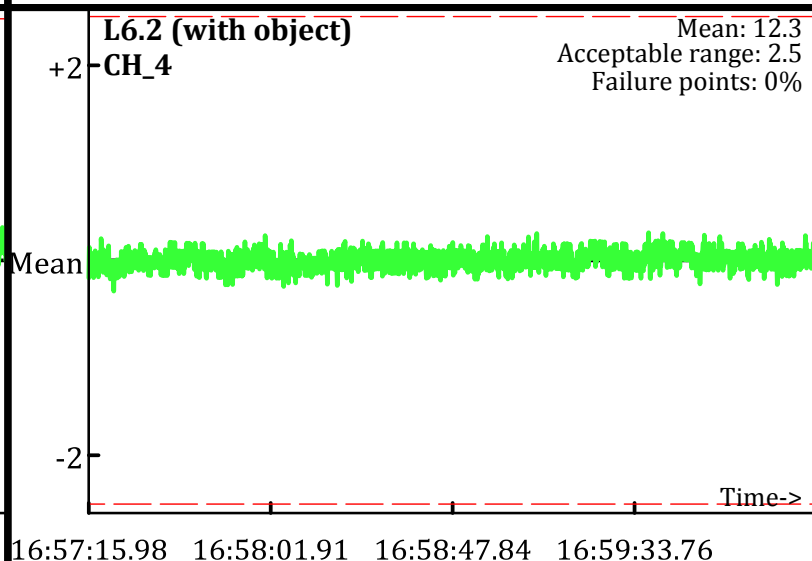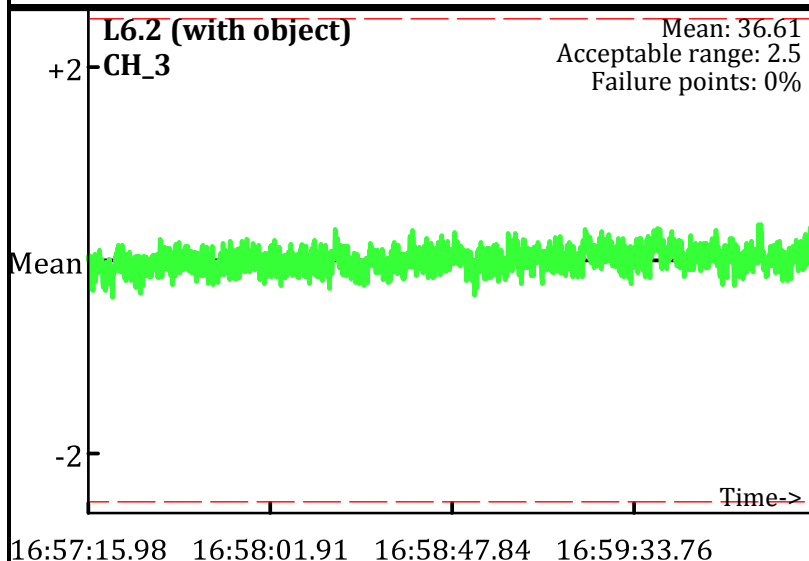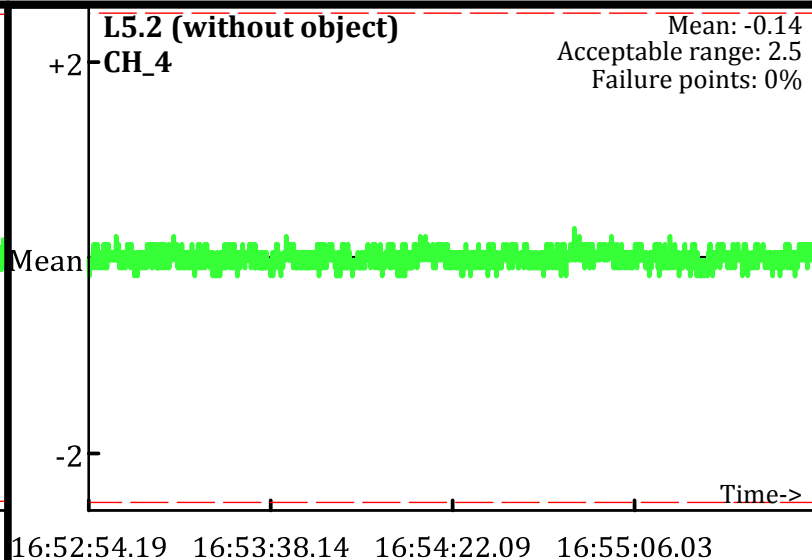
L7.2 (without object)
CH_3
Mean: 7.87
Acceptable range: 2.5
Failure points: 0%

Time->

17:02:03.69   17:02:18.89   17:02:34.09   17:02:49.28   17:03

L7.2 (without object)
CH_4
Mean: -0.12
Acceptable range: 2.5
Failure points: 0%

Time->

17:02:03.69   17:02:18.89   17:02:34.09   17:02:49.28   17:03

Database: D:\Projects_QCReports_Ord_Data\113009\QC\113009_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
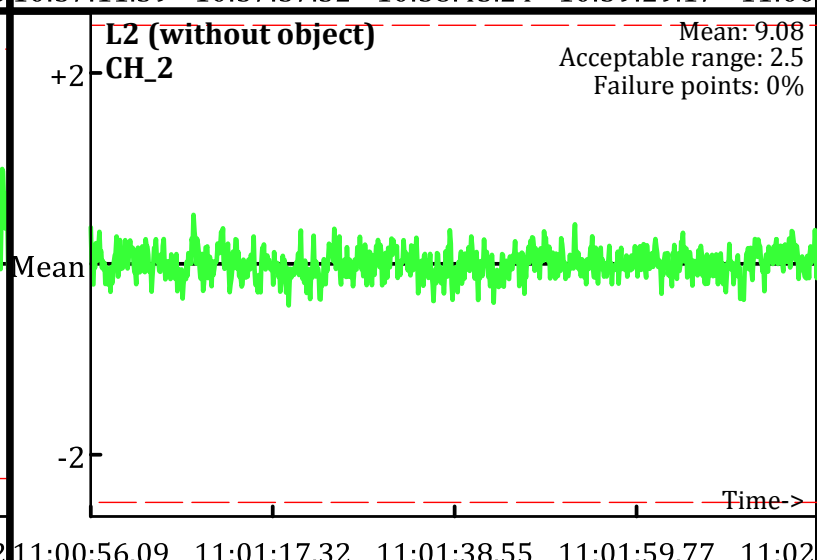Operator: PN & BS
Date: 12/1/2009

L0 (without object)
CH_1
Mean: -37.92
Acceptable range: 2.5
Failure points: 0%

10:53:00.59   10:53:45.77   10:54:30.94   10:55:16.11

L0 (without object)
CH_2
Mean: 9.17
Acceptable range: 2.5
Failure points: 0%

10:53:00.59   10:53:45.77   10:54:30.94   10:55:16.11

L1 (with object)
CH_1
Mean: 57.67
Acceptable range: 2.5
Failure points: 0%

10:57:11.39   10:57:57.32   10:58:43.24   10:59:29.17   11:00

L1 (with object)
CH_2
Mean: 67.66
Acceptable range: 2.5
Failure points: 0%

10:57:11.39   10:57:57.32   10:58:43.24   10:59:29.17   11:00

L2 (without object)
CH_1
Mean: -37.11
Acceptable range: 2.5
Failure points: 0%

11:00:56.09   11:01:17.32   11:01:38.55   11:01:59.77   11:02

L2 (without object)
CH_2
Mean: 9.08
Acceptable range: 2.5
Failure points: 0%

11:00:56.09   11:01:17.32   11:01:38.55   11:01:59.77   11:02

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

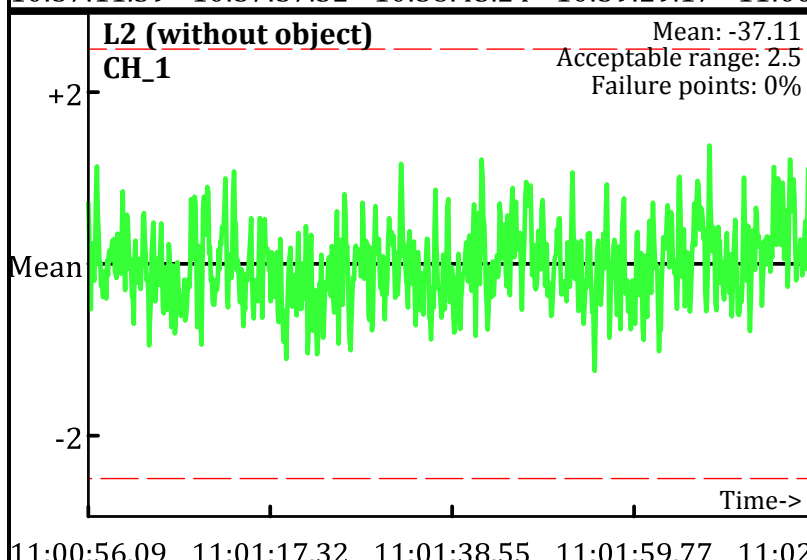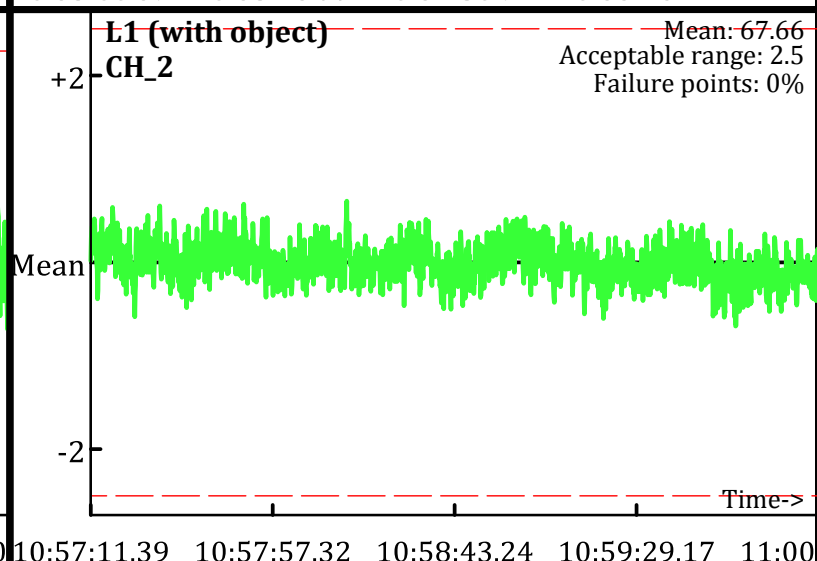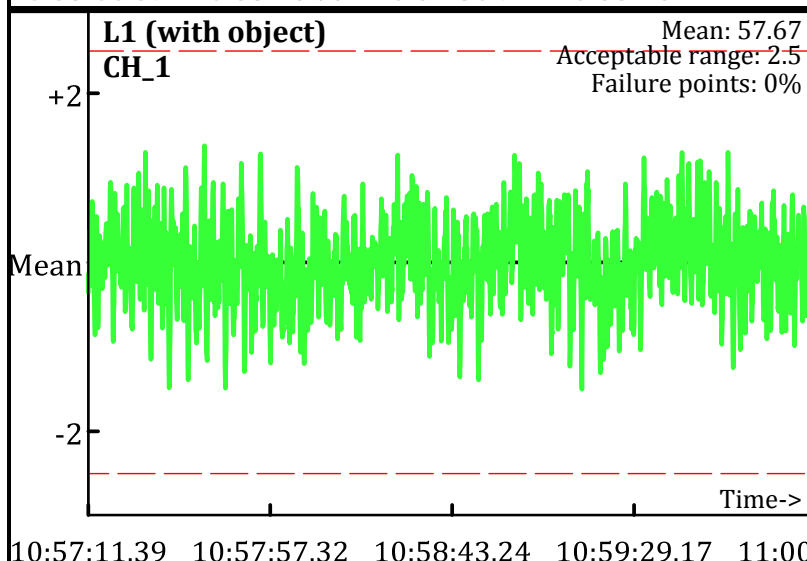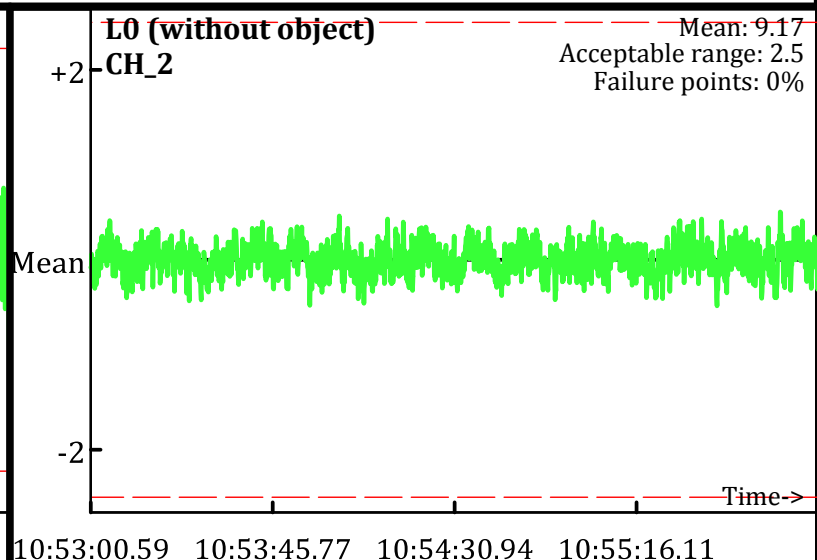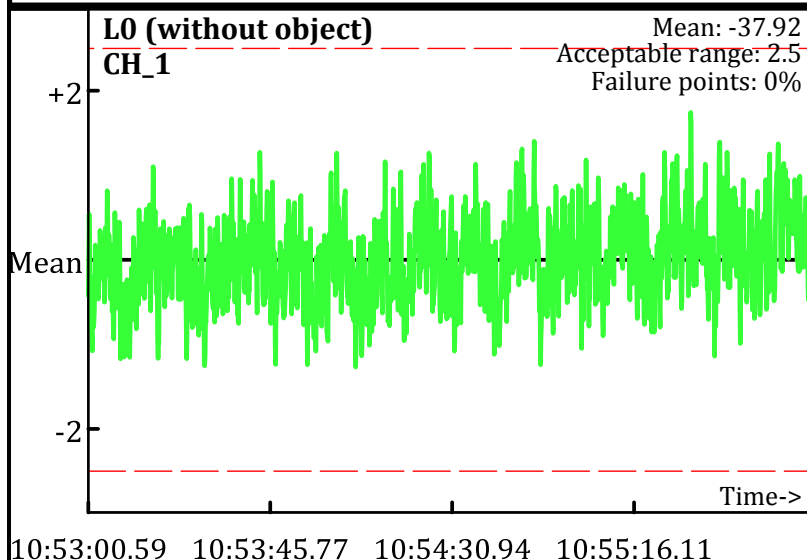AM test
Operator: PN & BS
Date: 12/1/2009

L0 (without object)
CH_3
Mean: 7.64
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:53:00.59   10:53:45.77   10:54:30.94   10:55:16.11

L0 (without object)
CH_4
Mean: -0.73
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:53:00.59   10:53:45.77   10:54:30.94   10:55:16.11

L1 (with object)
CH_3
Mean: 37.86
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:57:11.39   10:57:57.32   10:58:43.24   10:59:29.17   11:00

L1 (with object)
CH_4
Mean: 12.43
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:57:11.39   10:57:57.32   10:58:43.24   10:59:29.17   11:00

L2 (without object)
CH_3
Mean: 7.61
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:00:56.09   11:01:17.32   11:01:38.55   11:01:59.77   11:02

L2 (without object)
CH_4
Mean: -0.77
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:00:56.09   11:01:17.32   11:01:38.55   11:01:59.77   11:02

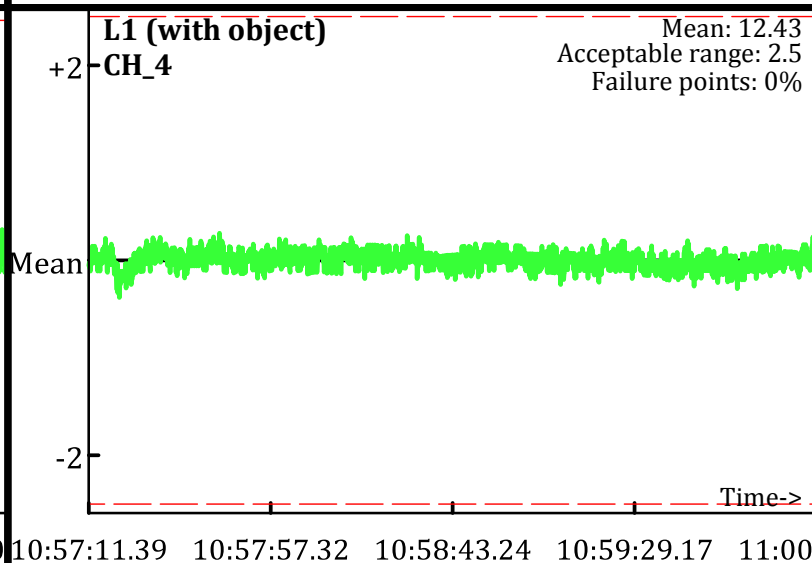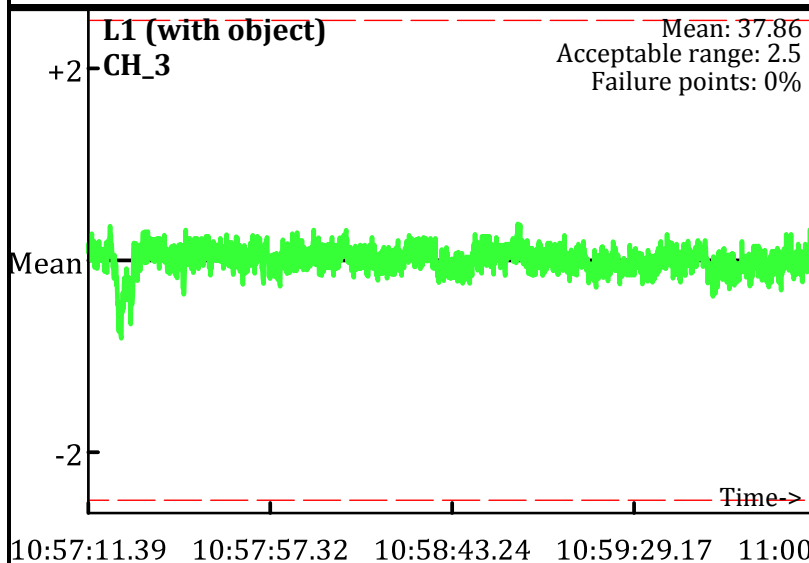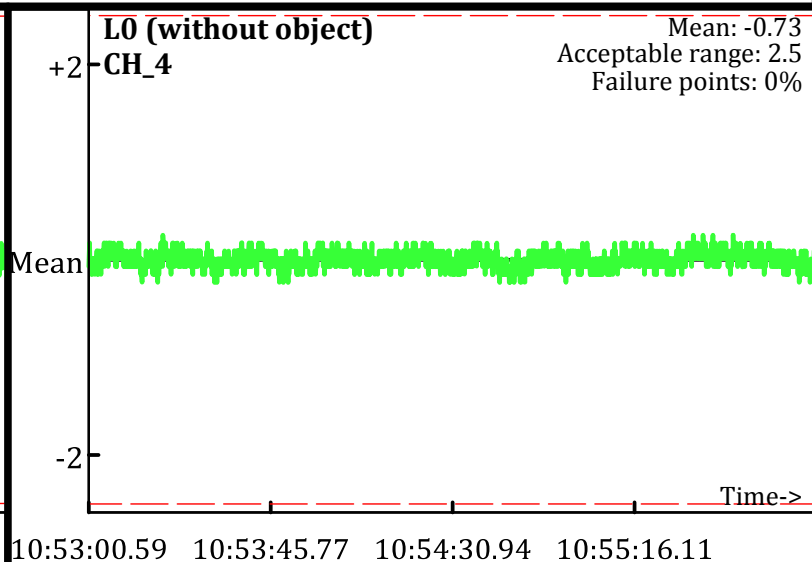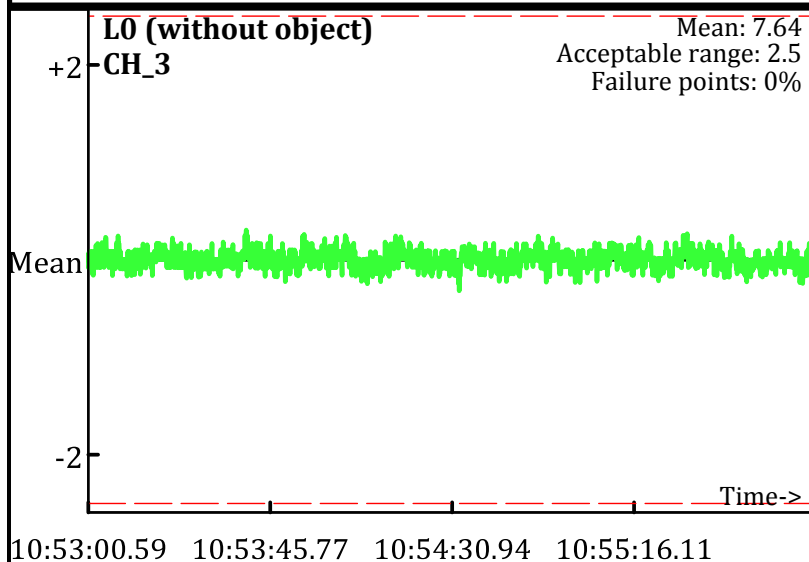Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
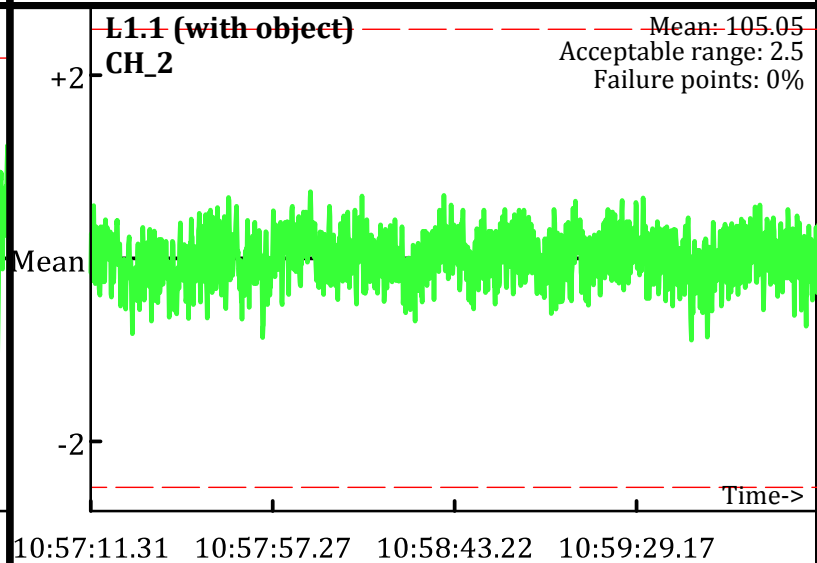Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BS
Date: 12/1/2009

L0.1 (without object)
CH_1
Mean: -70.03
Acceptable range: 2.5
Failure points: 0%

10:53:00.63 10:53:45.80 10:54:30.97 10:55:16.14

L0.1 (without object)
CH_2
Mean: 12.36
Acceptable range: 2.5
Failure points: 0%

10:53:00.63 10:53:45.80 10:54:30.97 10:55:16.14

L1.1 (with object)
CH_1
Mean: 53.73
Acceptable range: 2.5
Failure points: 0%

10:57:11.31 10:57:57.27 10:58:43.22 10:59:29.17

L1.1 (with object)
CH_2
Mean: 105.05
Acceptable range: 2.5
Failure points: 0%

10:57:11.31 10:57:57.27 10:58:43.22 10:59:29.17

L2.1 (without object)
CH_1
Mean: -69.37
Acceptable range: 2.5
Failure points: 0%

11:00:56.12 11:01:17.32 11:01:38.52 11:01:59.71

L2.1 (without object)
CH_2
Mean: 12.32
Acceptable range: 2.5
Failure points: 0%

11:00:56.12 11:01:17.32 11:01:38.52 11:01:59.71

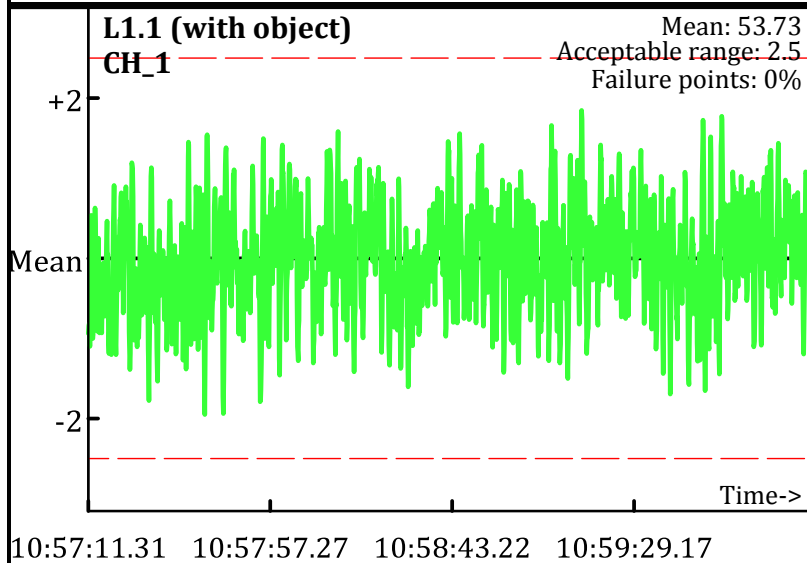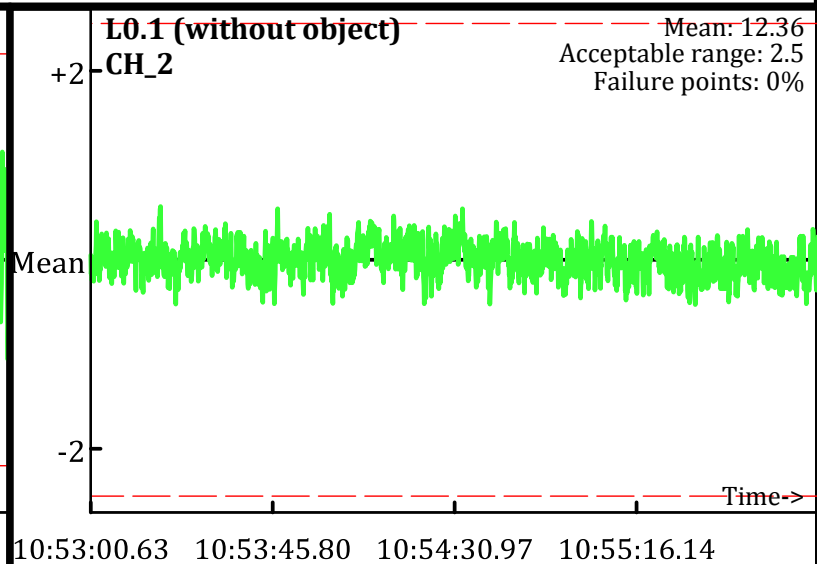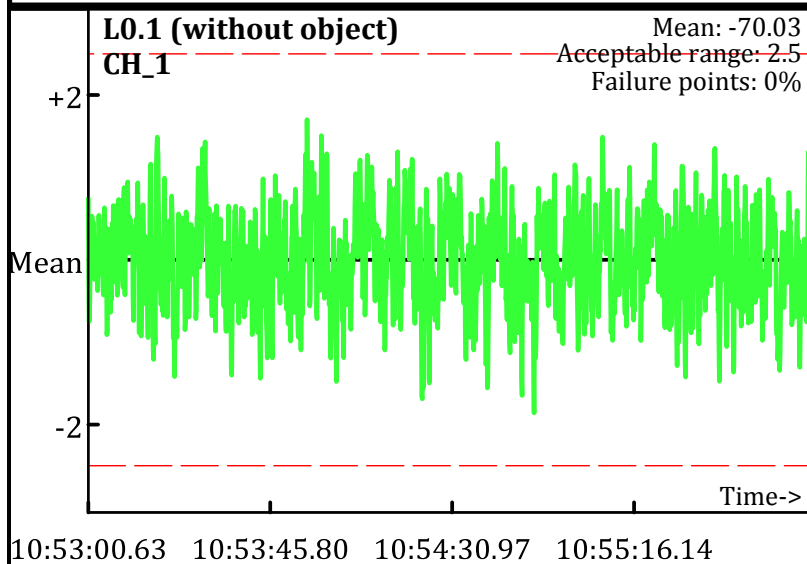# Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
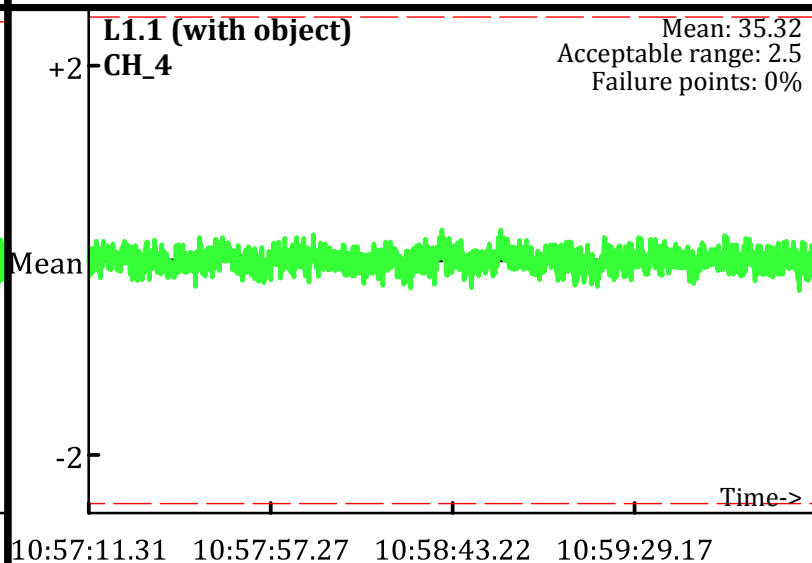Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BS
Date: 12/1/2009

L0.1 (without object)
CH_3
Mean: 14.62
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
10:53:00.63   10:53:45.80   10:54:30.97   10:55:16.14

L0.1 (without object)
CH_4
Mean: 3.65
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
10:53:00.63   10:53:45.80   10:54:30.97   10:55:16.14

L1.1 (with object)
CH_3
Mean: 73.85
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
10:57:11.31   10:57:57.27   10:58:43.22   10:59:29.17

L1.1 (with object)
CH_4
Mean: 35.32
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
10:57:11.31   10:57:57.27   10:58:43.22   10:59:29.17

L2.1 (without object)
CH_3
Mean: 14.58
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:00:56.12   11:01:17.32   11:01:38.52   11:01:59.71

L2.1 (without object)
CH_4
Mean: 3.63
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:00:56.12   11:01:17.32   11:01:38.52   11:01:59.71

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
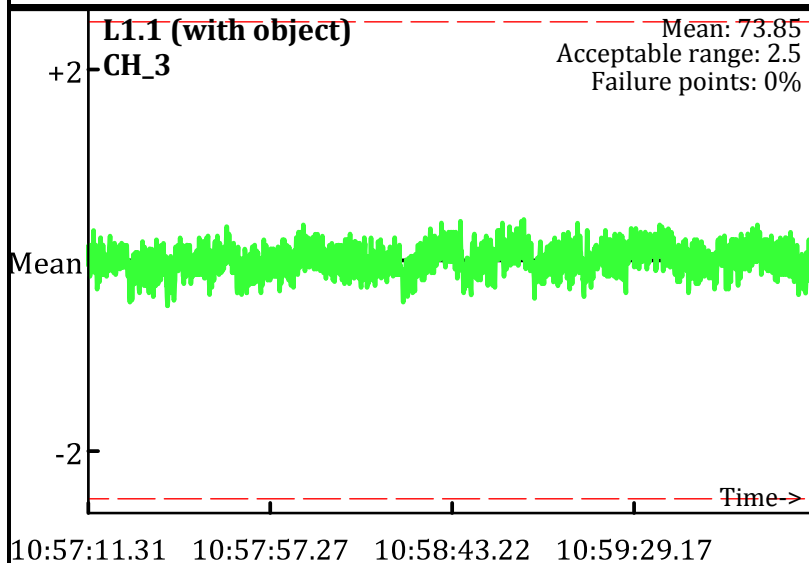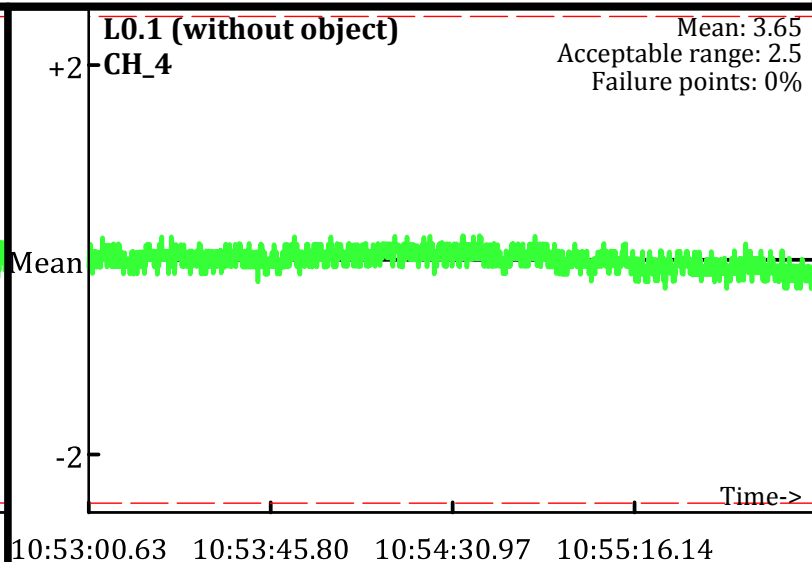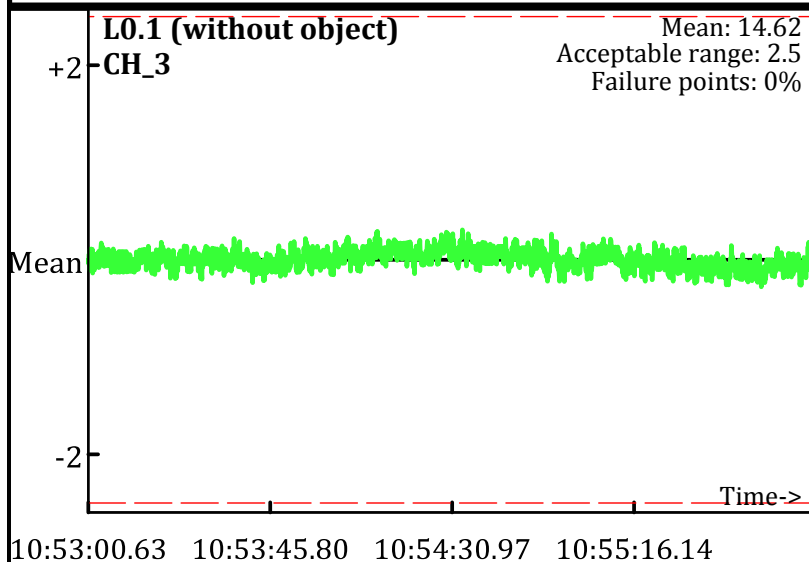Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
-- -- Acceptable limits
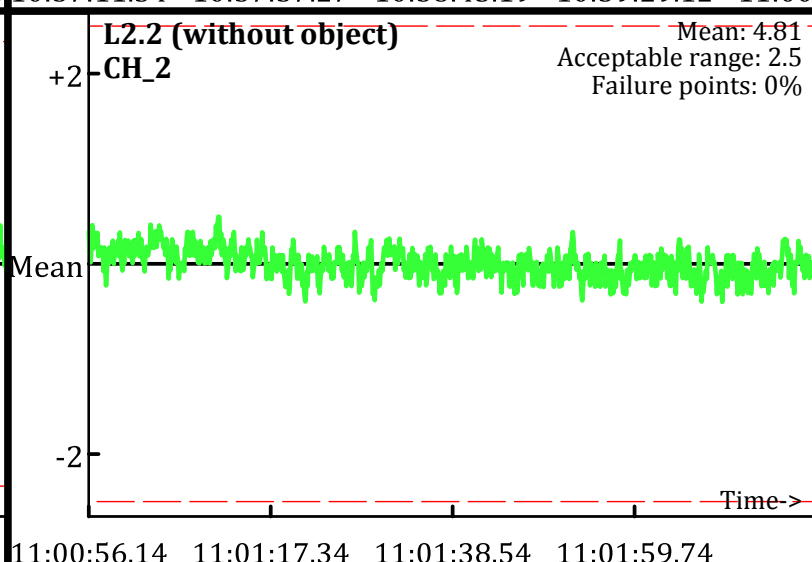
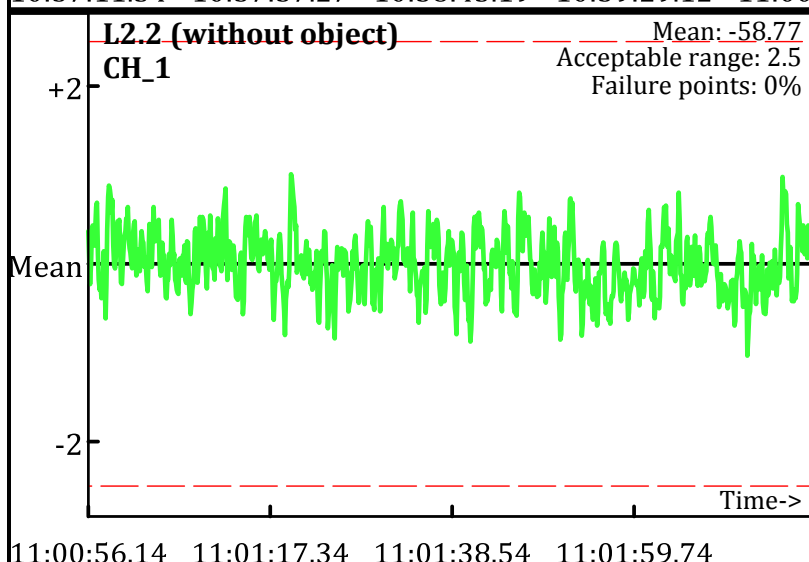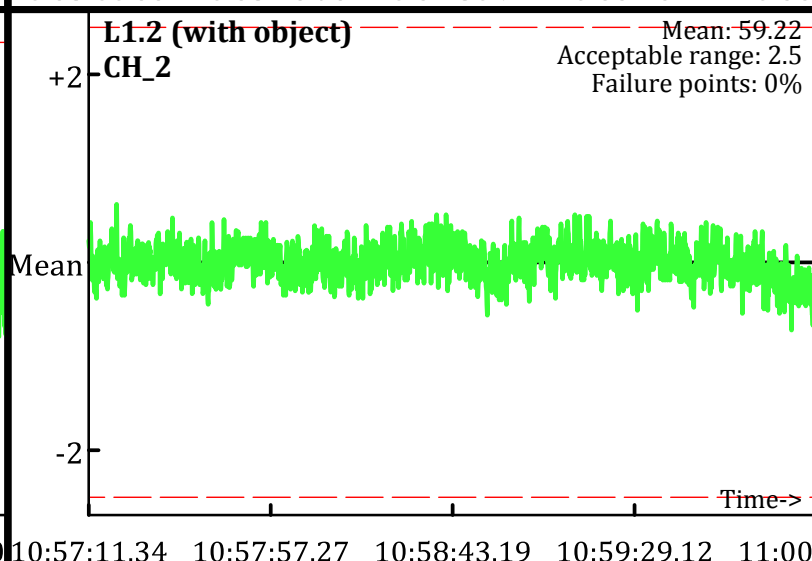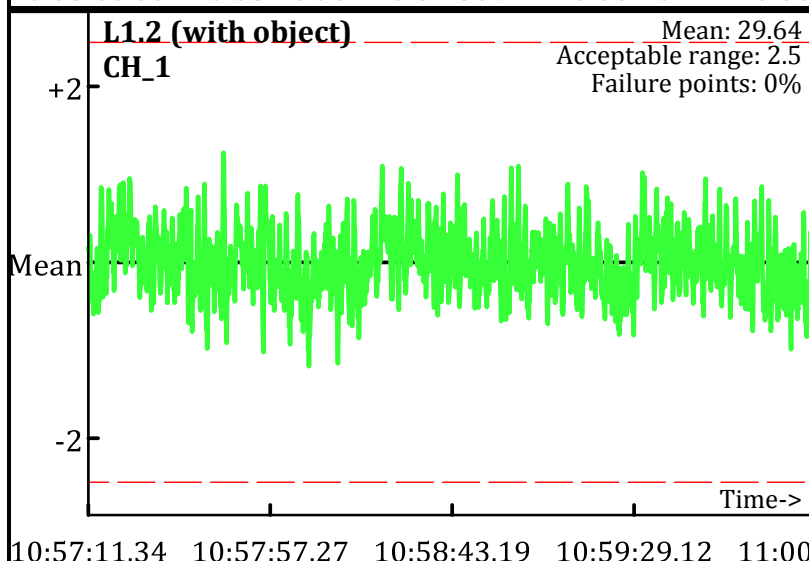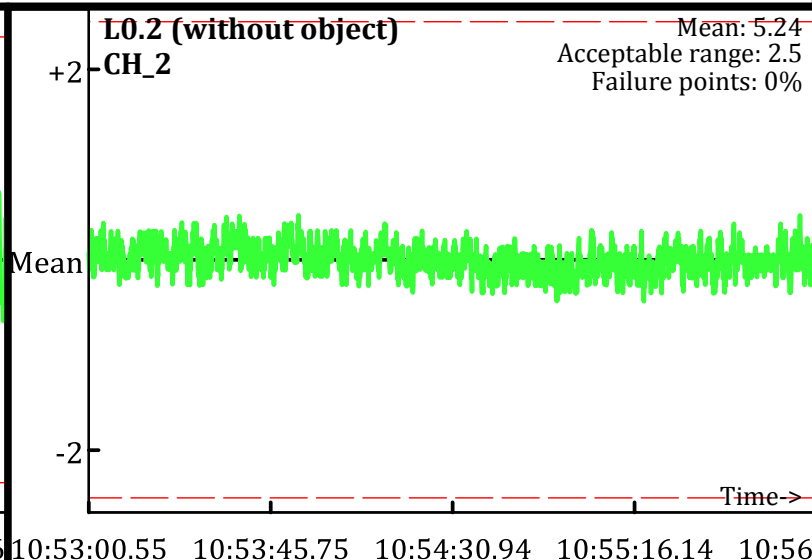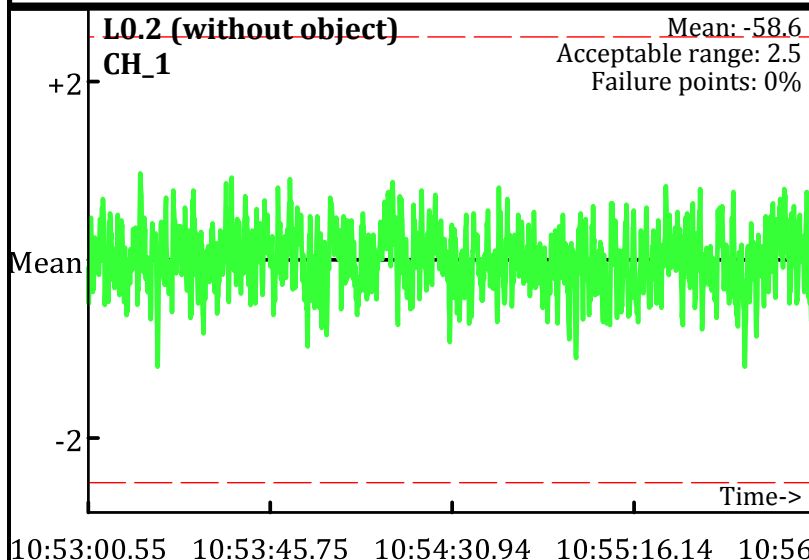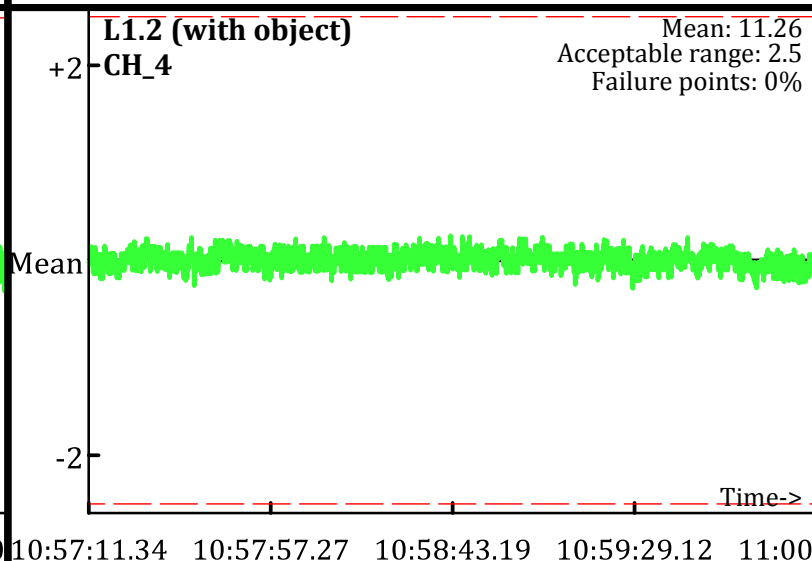AM test
Operator: PN & BS
Date: 12/1/2009

L0.2 (without object)
CH_1
Mean: -58.6
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

10:53:00.55   10:53:45.75   10:54:30.94   10:55:16.14   10:56

L0.2 (without object)
CH_2
Mean: 5.24
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

10:53:00.55   10:53:45.75   10:54:30.94   10:55:16.14   10:56

L1.2 (with object)
CH_1
Mean: 29.64
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

10:57:11.34   10:57:57.27   10:58:43.19   10:59:29.12   11:00

L1.2 (with object)
CH_2
Mean: 59.22
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

10:57:11.34   10:57:57.27   10:58:43.19   10:59:29.12   11:00

L2.2 (without object)
CH_1
Mean: -58.77
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:00:56.14   11:01:17.34   11:01:38.54   11:01:59.74

L2.2 (without object)
CH_2
Mean: 4.81
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:00:56.14   11:01:17.34   11:01:38.54   11:01:59.74

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

L0.2 (without object)
CH_3
Mean: 6.29
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:53:00.55 10:53:45.75 10:54:30.94 10:55:16.14 10:56

L0.2 (without object)
CH_4
Mean: -0.66
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:53:00.55 10:53:45.75 10:54:30.94 10:55:16.14 10:56

L1.2 (with object)
CH_3
Mean: 33.95
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:57:11.34 10:57:57.27 10:58:43.19 10:59:29.12 11:00

L1.2 (with object)
CH_4
Mean: 11.26
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

10:57:11.34 10:57:57.27 10:58:43.19 10:59:29.12 11:00

L2.2 (without object)
CH_3
Mean: 6.04
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

11:00:56.14 11:01:17.34 11:01:38.54 11:01:59.74

L2.2 (without object)
CH_4
Mean: -0.93
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

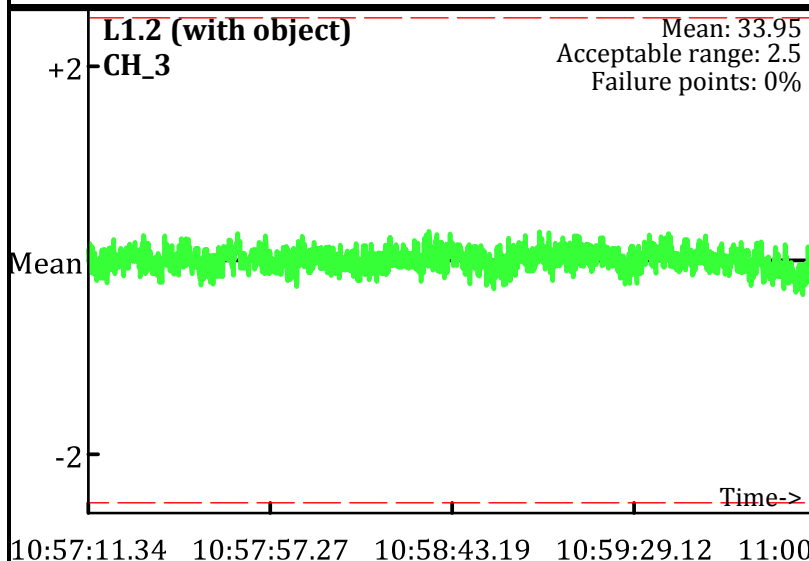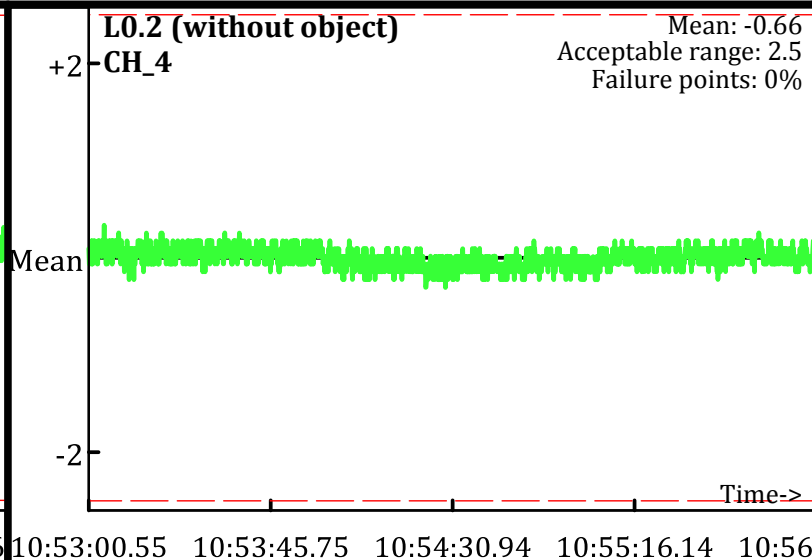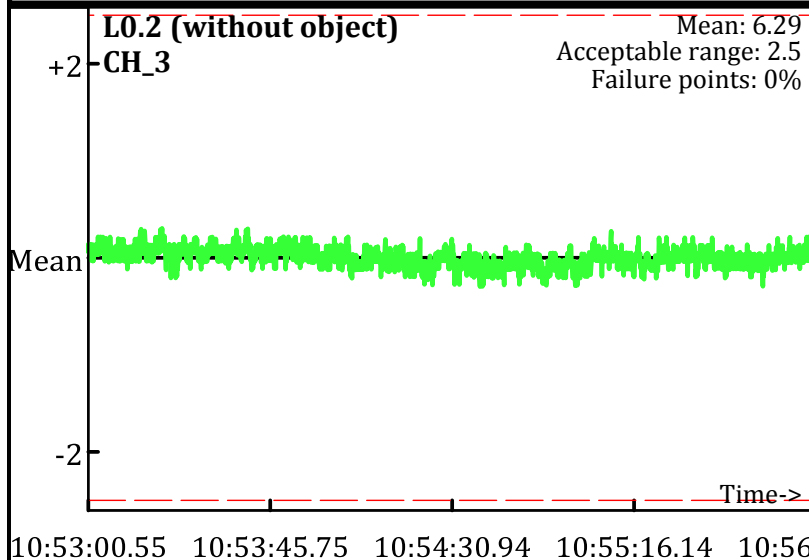11:00:56.14 11:01:17.34 11:01:38.54 11:01:59.74

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits
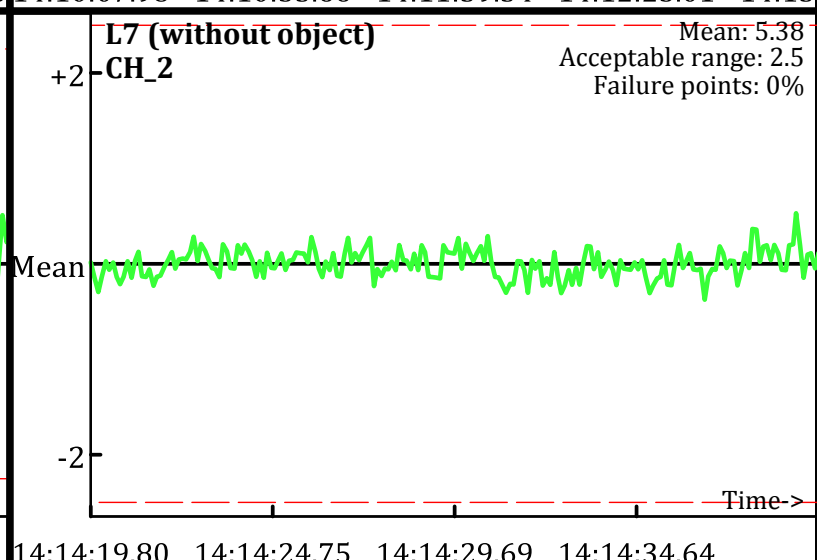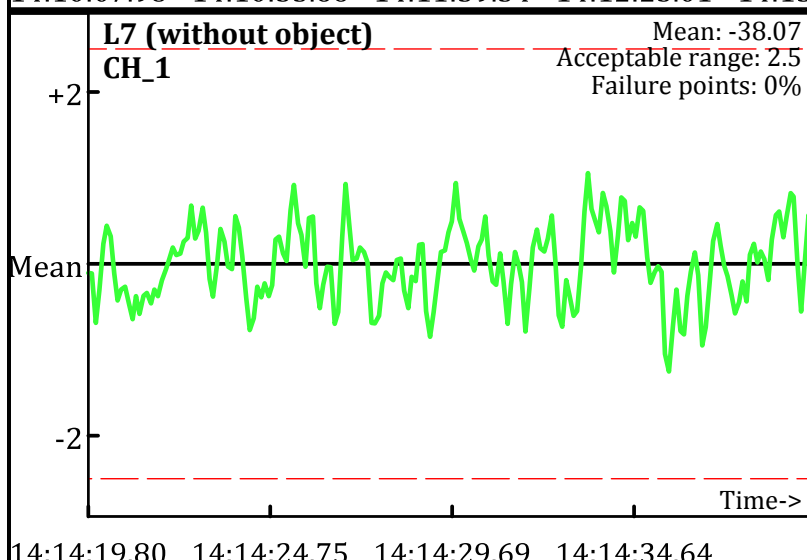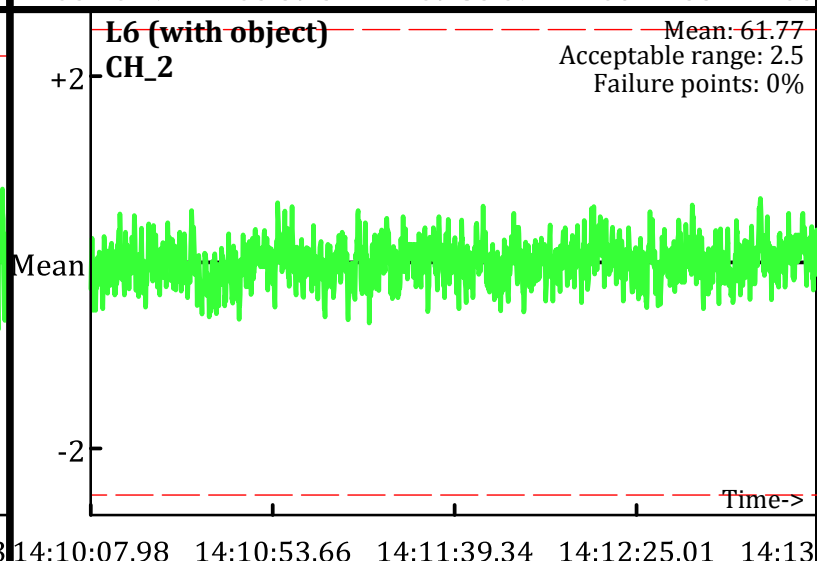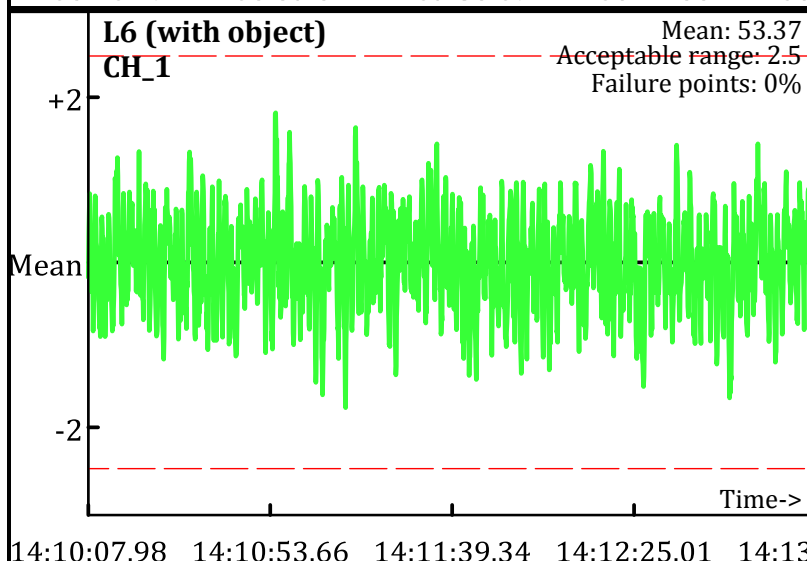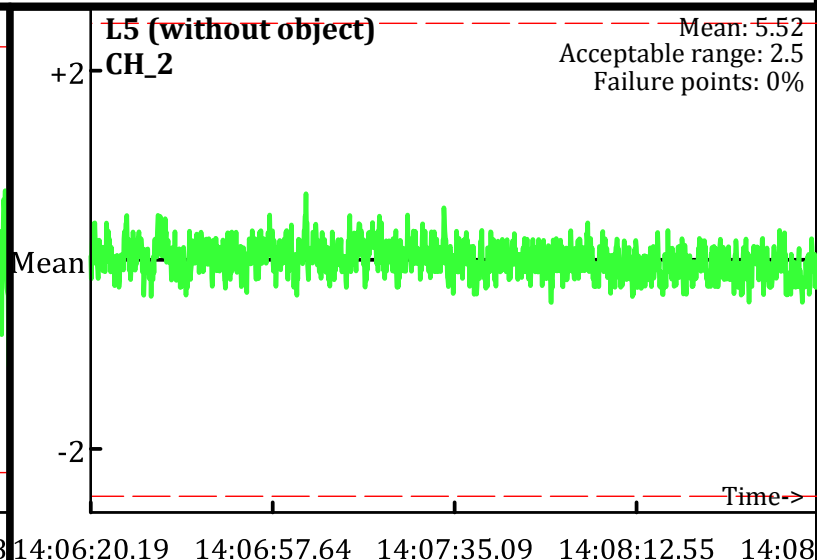
PM test
Operator: PN & BS
Date: 12/1/2009

L5 (without object)
CH_1
Mean: -37.38
Acceptable range: 2.5
Failure points: 0%

L5 (without object)
CH_2
Mean: 5.52
Acceptable range: 2.5
Failure points: 0%

14:06:20.19 14:06:57.64 14:07:35.09 14:08:12.55 14:08

L6 (with object)
CH_1
Mean: 53.37
Acceptable range: 2.5
Failure points: 0%

L6 (with object)
CH_2
Mean: 61.77
Acceptable range: 2.5
Failure points: 0%

14:10:07.98 14:10:53.66 14:11:39.34 14:12:25.01 14:13

L7 (without object)
CH_1
Mean: -38.07
Acceptable range: 2.5
Failure points: 0%

L7 (without object)
CH_2
Mean: 5.38
Acceptable range: 2.5
Failure points: 0%

14:14:19.80 14:14:24.75 14:14:29.69 14:14:34.64

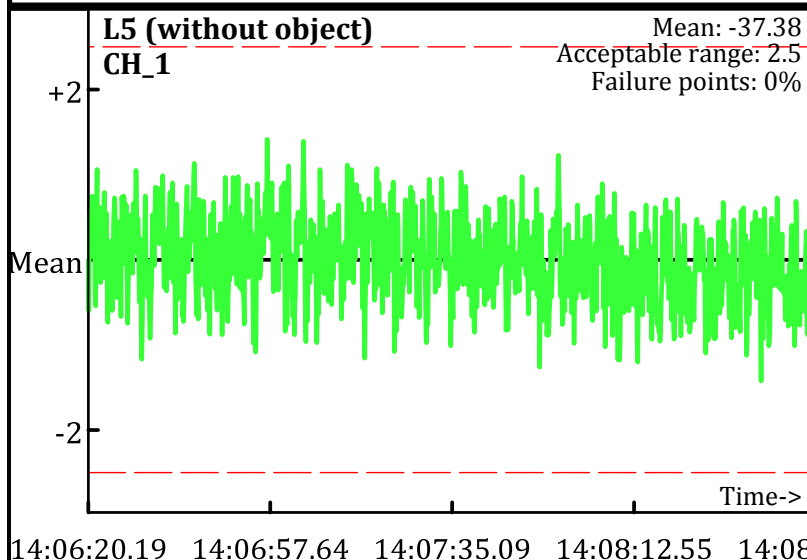Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
Line Name: L5 L6 L7

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
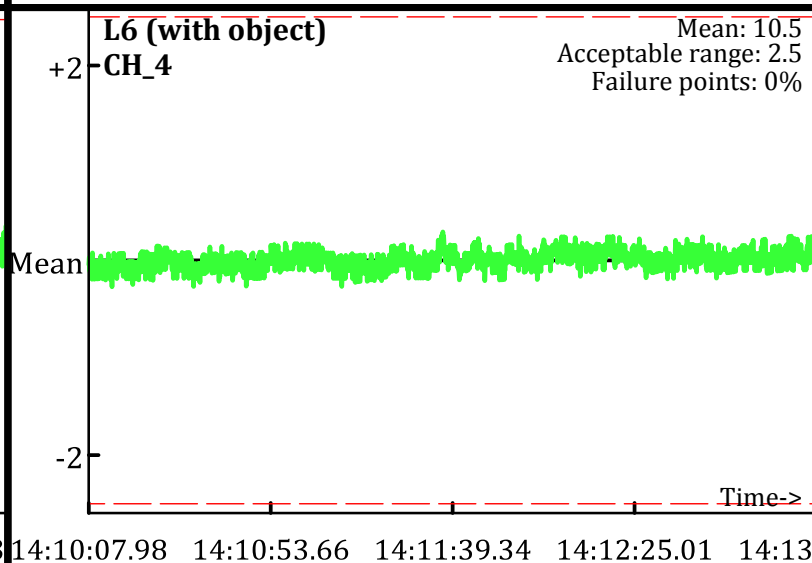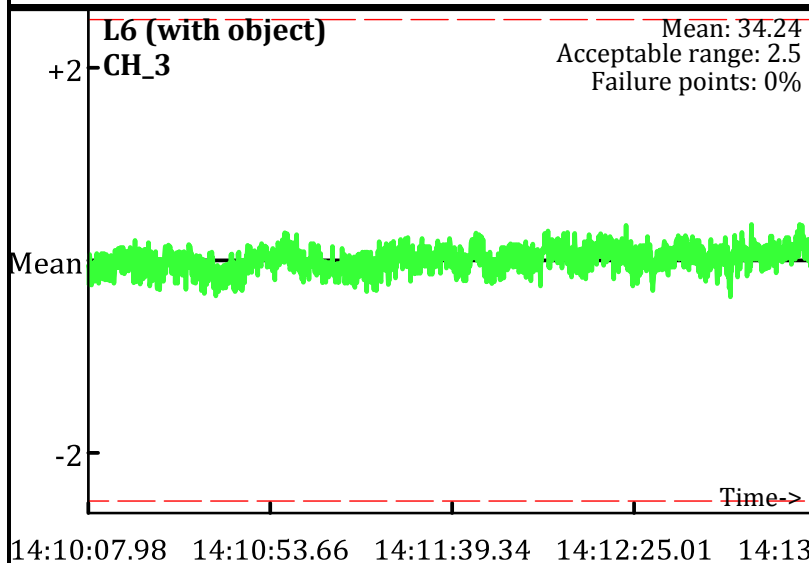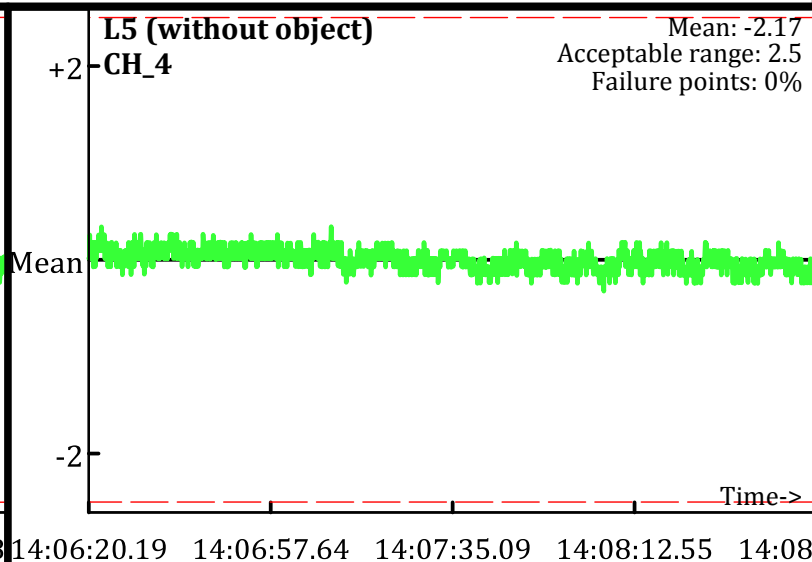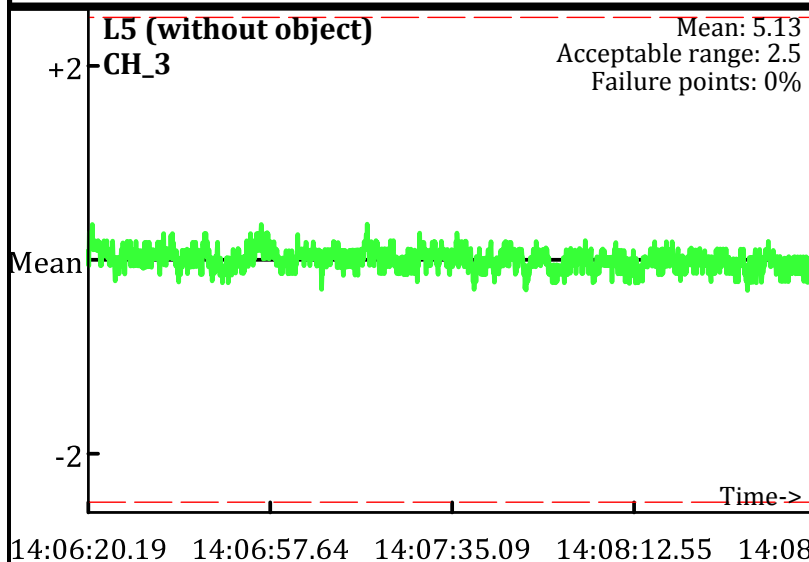Grid/Location: QC Area

🔴 Outside range
-- -- Acceptable limits

PM test
Operator: PN & BS
Date: 12/1/2009

L5 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 5.13
Acceptable range: 2.5
Failure points: 0%

14:06:20.19   14:06:57.64   14:07:35.09   14:08:12.55   14:08

L5 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.17
Acceptable range: 2.5
Failure points: 0%

14:06:20.19   14:06:57.64   14:07:35.09   14:08:12.55   14:08

L6 (with object)
CH_3
+2
Mean
-2
Time->

Mean: 34.24
Acceptable range: 2.5
Failure points: 0%

14:10:07.98   14:10:53.66   14:11:39.34   14:12:25.01   14:13

L6 (with object)
CH_4
+2
Mean
-2
Time->

Mean: 10.5
Acceptable range: 2.5
Failure points: 0%

14:10:07.98   14:10:53.66   14:11:39.34   14:12:25.01   14:13

L7 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 5.14
Acceptable range: 2.5
Failure points: 0%

14:14:19.80   14:14:24.75   14:14:29.69   14:14:34.64

L7 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.13
Acceptable range: 2.5
Failure points: 0%

14:14:19.80   14:14:24.75   14:14:29.69   14:14:34.64

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
Line Name: L5 L6 L7

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits
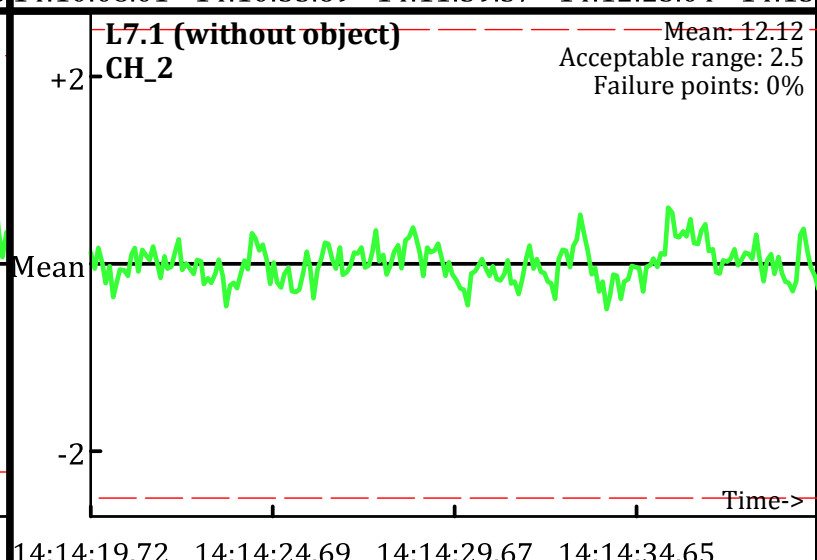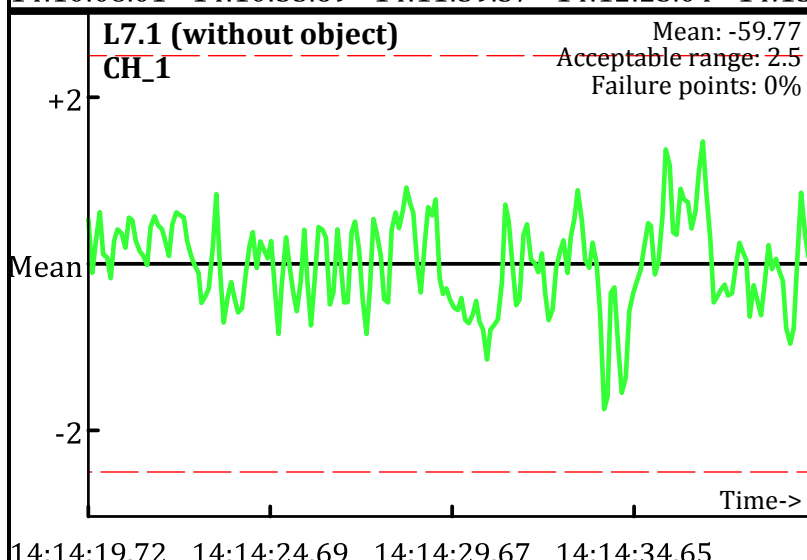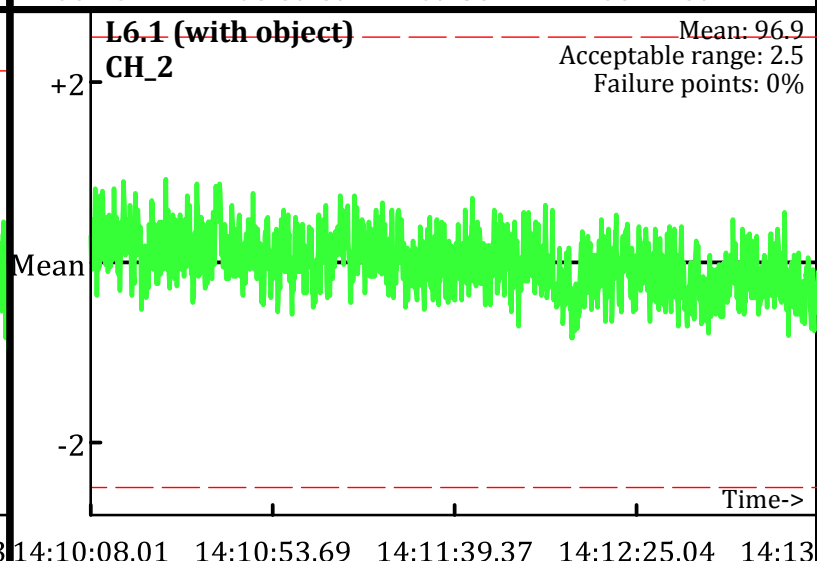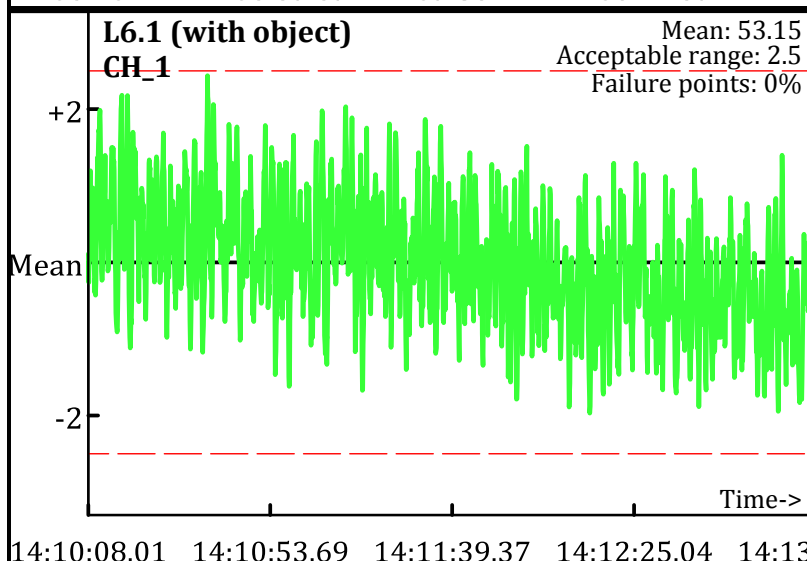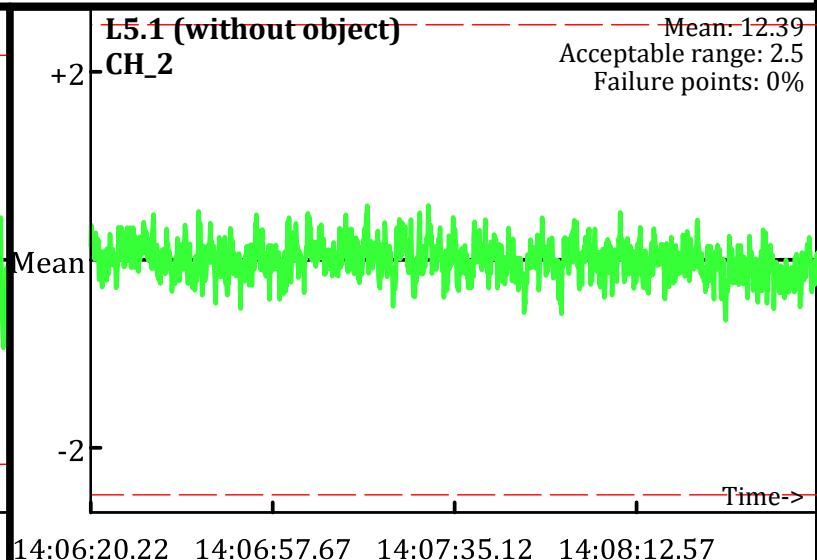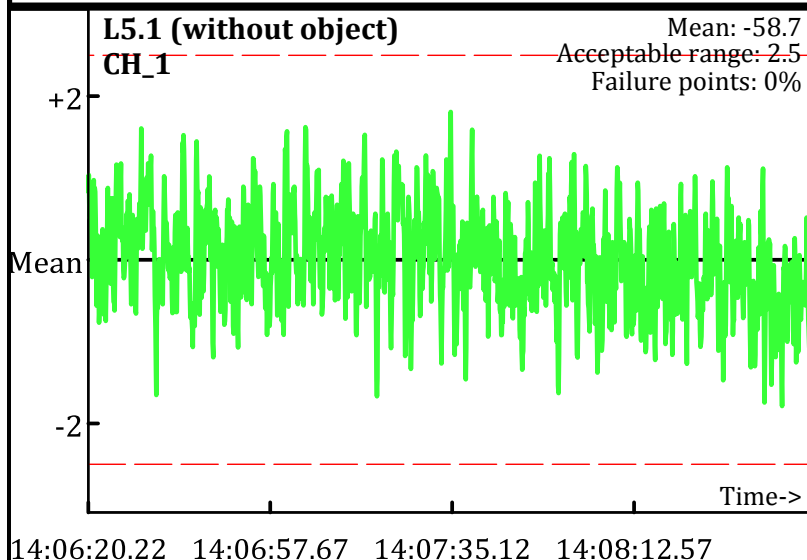
PM test
Operator: PN & BS
Date: 12/1/2009

L5.1 (without object)
CH_1

Mean: -58.7
Acceptable range: 2.5
Failure points: 0%

L5.1 (without object)
CH_2

Mean: 12.39
Acceptable range: 2.5
Failure points: 0%

14:06:20.22   14:06:57.67   14:07:35.12   14:08:12.57

L6.1 (with object)
CH_1

Mean: 53.15
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_2

Mean: 96.9
Acceptable range: 2.5
Failure points: 0%

14:10:08.01   14:10:53.69   14:11:39.37   14:12:25.04   14:13

L7.1 (without object)
CH_1

Mean: -59.77
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_2

Mean: 12.12
Acceptable range: 2.5
Failure points: 0%

14:14:19.72   14:14:24.69   14:14:29.67   14:14:34.65

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
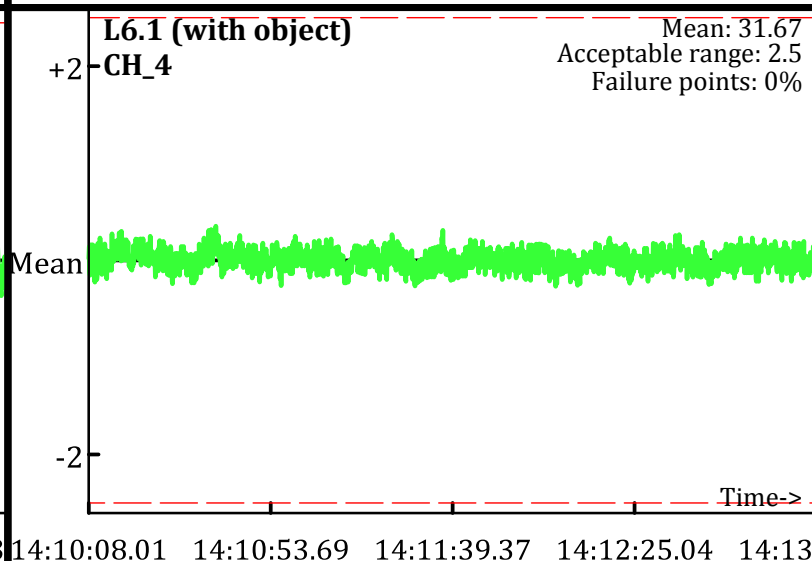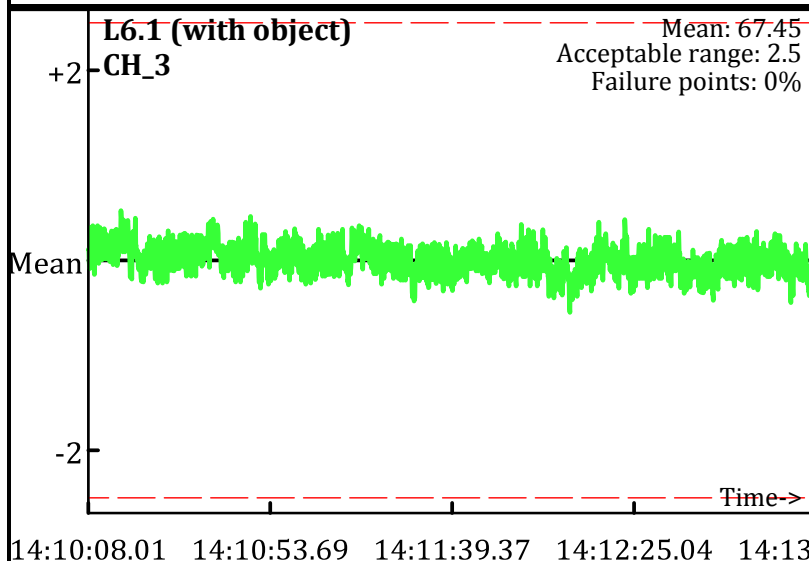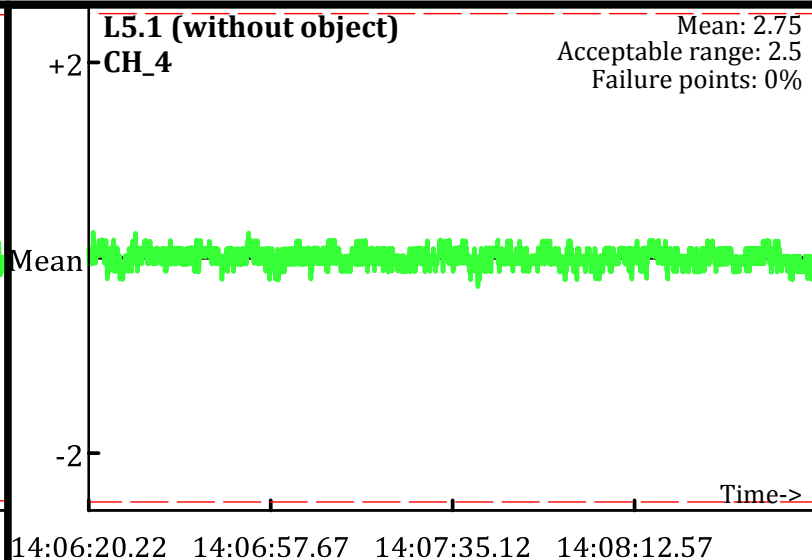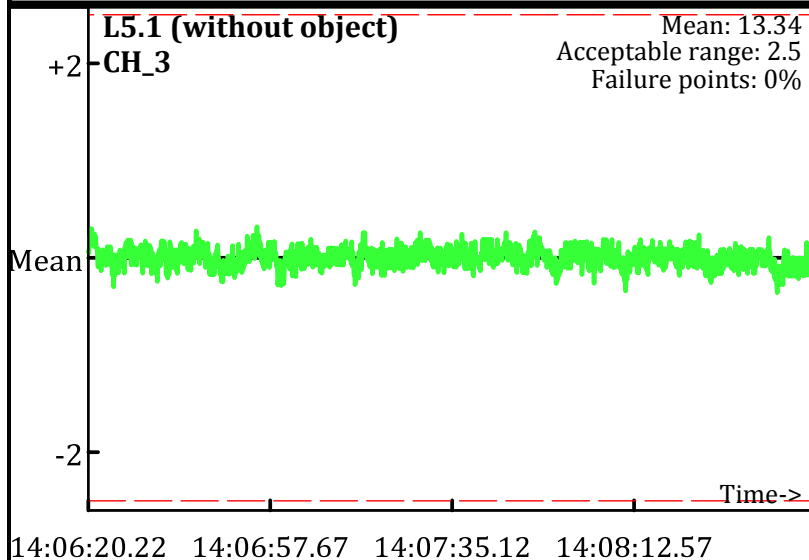Line Name: L5.1 L6.1 L7.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BS
Date: 12/1/2009

L5.1 (without object)
CH_3
Mean: 13.34
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:06:20.22   14:06:57.67   14:07:35.12   14:08:12.57

L5.1 (without object)
CH_4
Mean: 2.75
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:06:20.22   14:06:57.67   14:07:35.12   14:08:12.57

L6.1 (with object)
CH_3
Mean: 67.45
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:10:08.01   14:10:53.69   14:11:39.37   14:12:25.04   14:13

L6.1 (with object)
CH_4
Mean: 31.67
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:10:08.01   14:10:53.69   14:11:39.37   14:12:25.04   14:13

L7.1 (without object)
CH_3
Mean: 13.27
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:14:19.72   14:14:24.69   14:14:29.67   14:14:34.65

L7.1 (without object)
CH_4
Mean: 2.7
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:14:19.72   14:14:24.69   14:14:29.67   14:14:34.65

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits
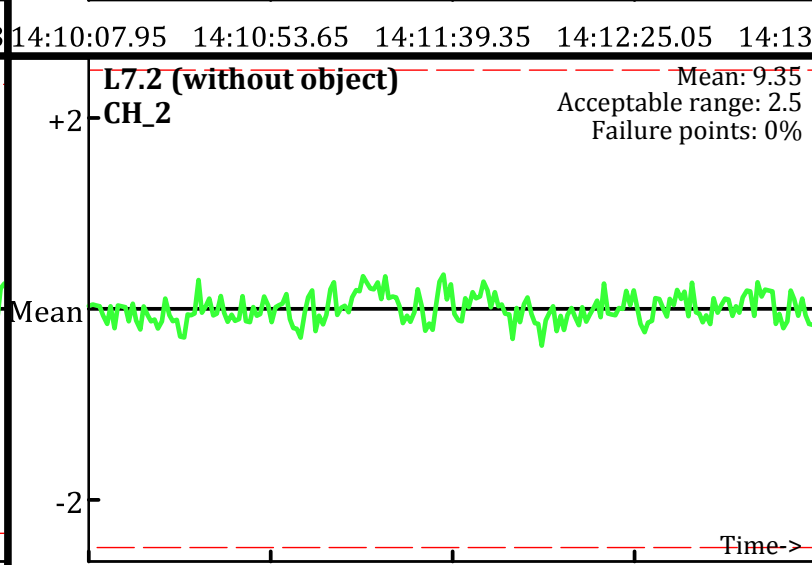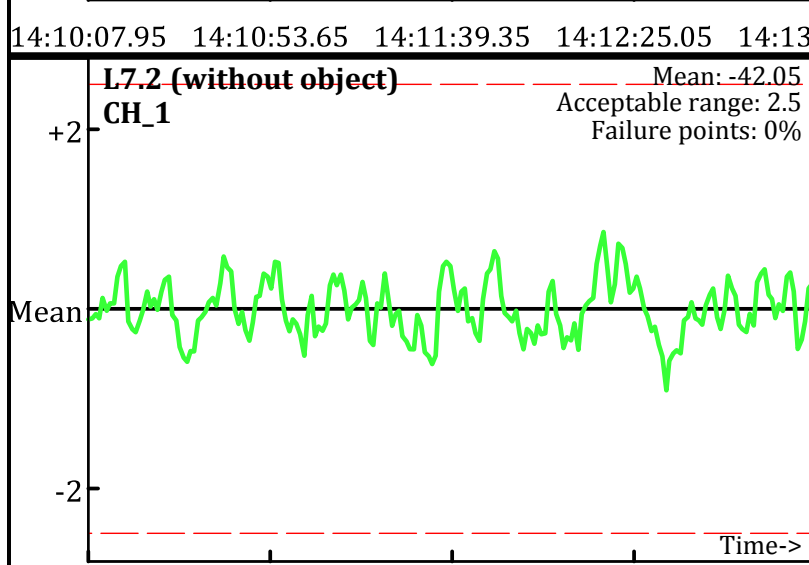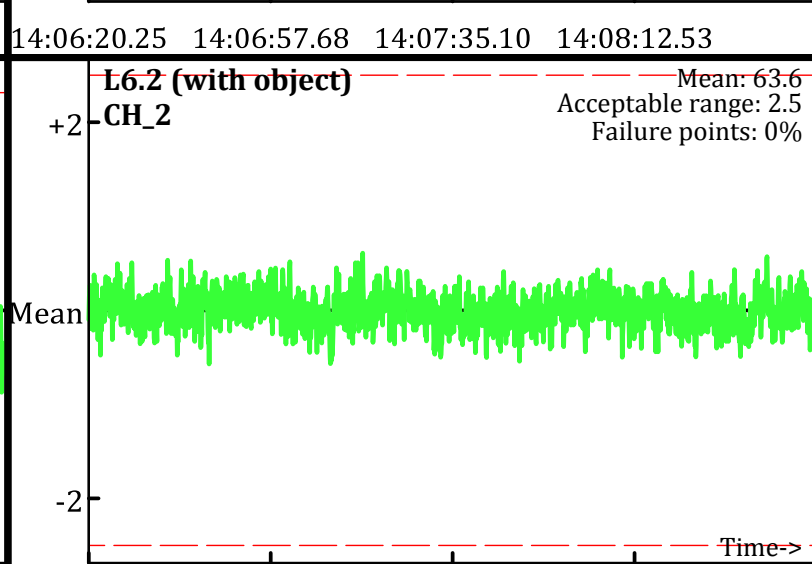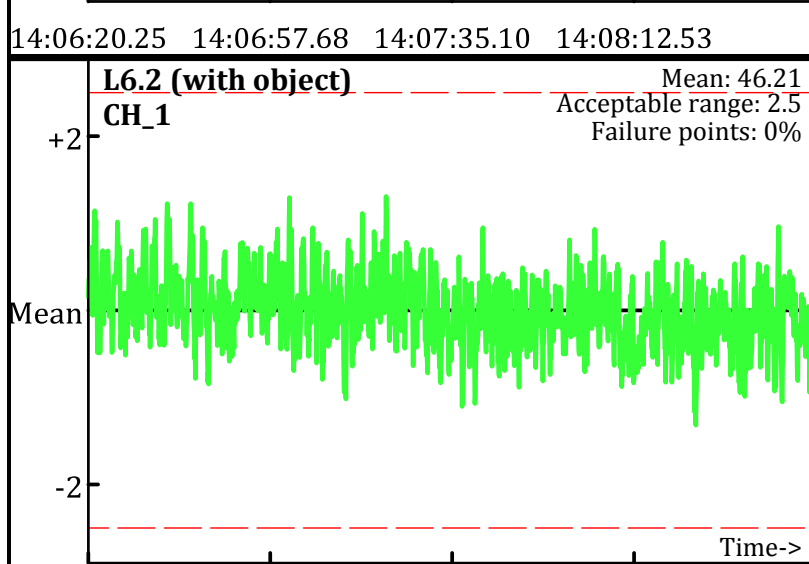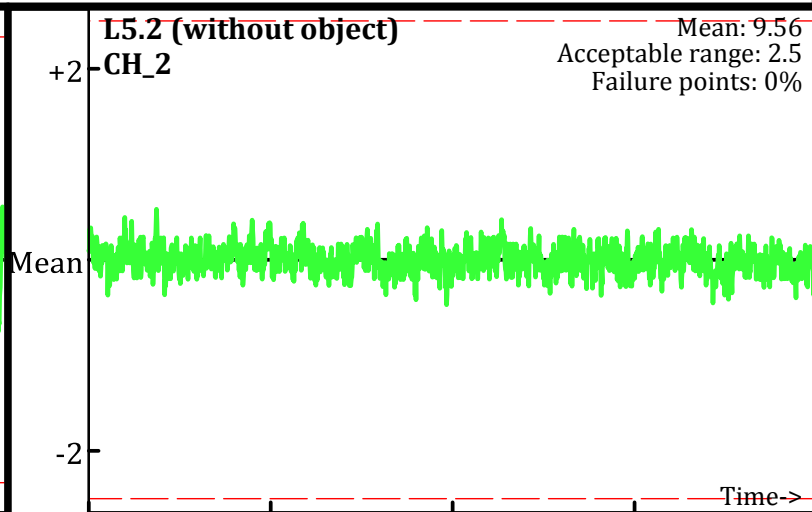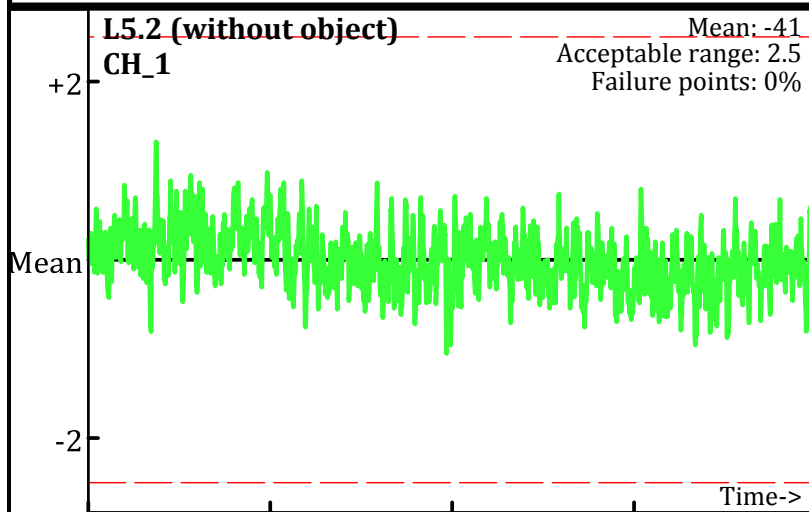
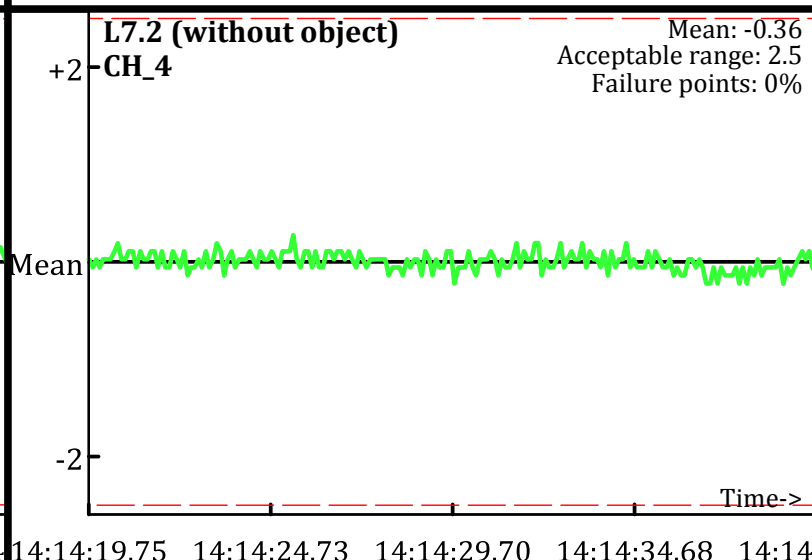PM test
Operator: PN & BS
Date: 12/1/2009

L5.2 (without object)
CH_1
Mean: -41
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:06:20.25   14:06:57.68   14:07:35.10   14:08:12.53

L5.2 (without object)
CH_2
Mean: 9.56
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:06:20.25   14:06:57.68   14:07:35.10   14:08:12.53

L6.2 (with object)
CH_1
Mean: 46.21
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:10:07.95   14:10:53.65   14:11:39.35   14:12:25.05   14:13

L6.2 (with object)
CH_2
Mean: 63.6
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:10:07.95   14:10:53.65   14:11:39.35   14:12:25.05   14:13

L7.2 (without object)
CH_1
Mean: -42.05
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:14:19.75   14:14:24.73   14:14:29.70   14:14:34.68   14:14

L7.2 (without object)
CH_2
Mean: 9.35
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:14:19.75   14:14:24.73   14:14:29.70   14:14:34.68   14:14

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

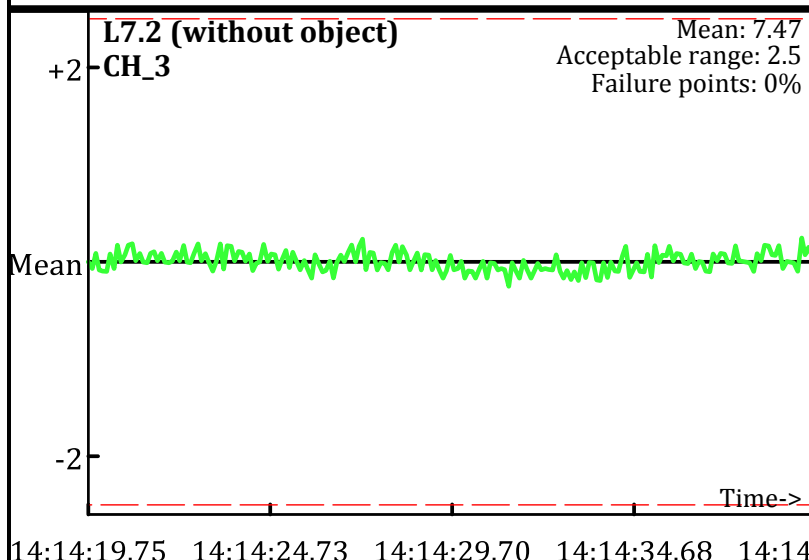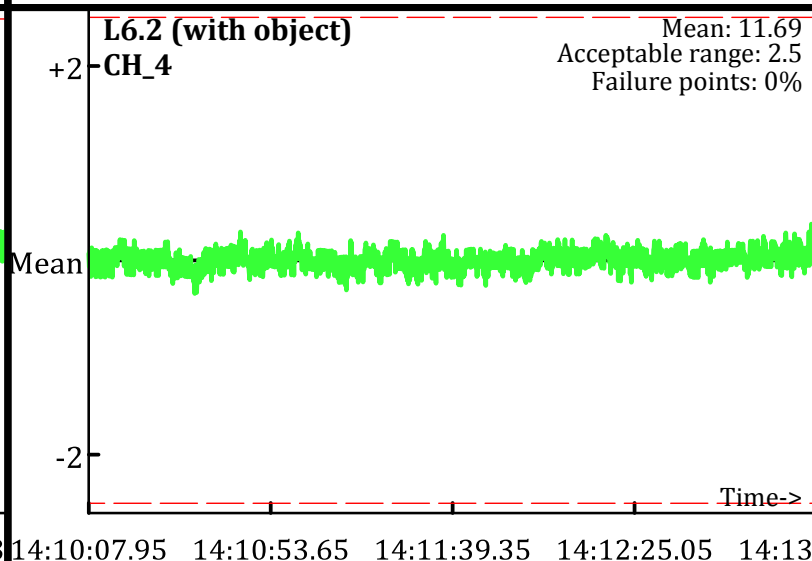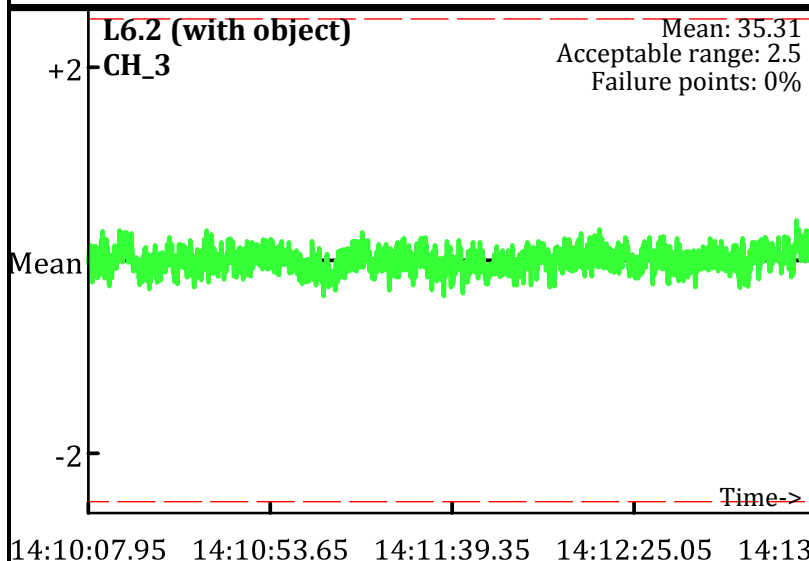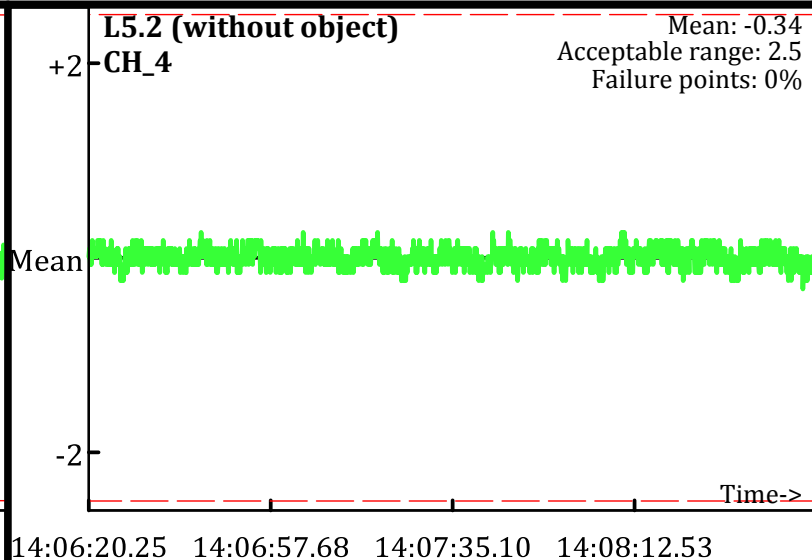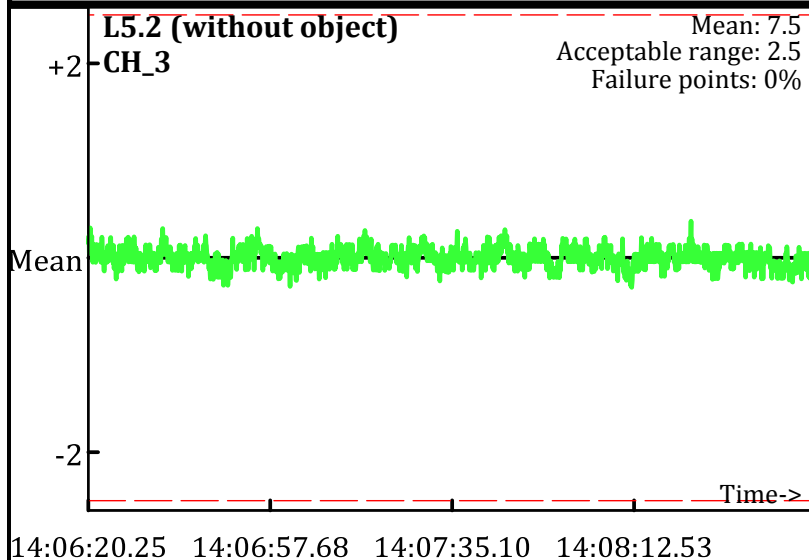PM test
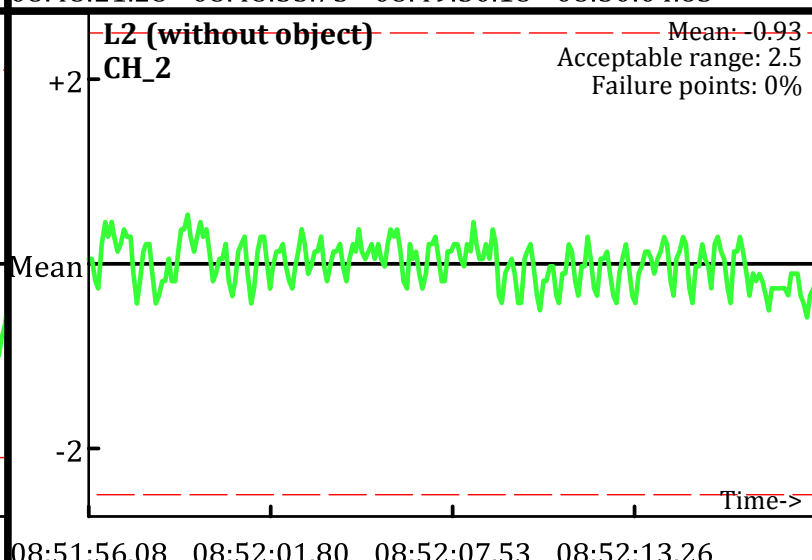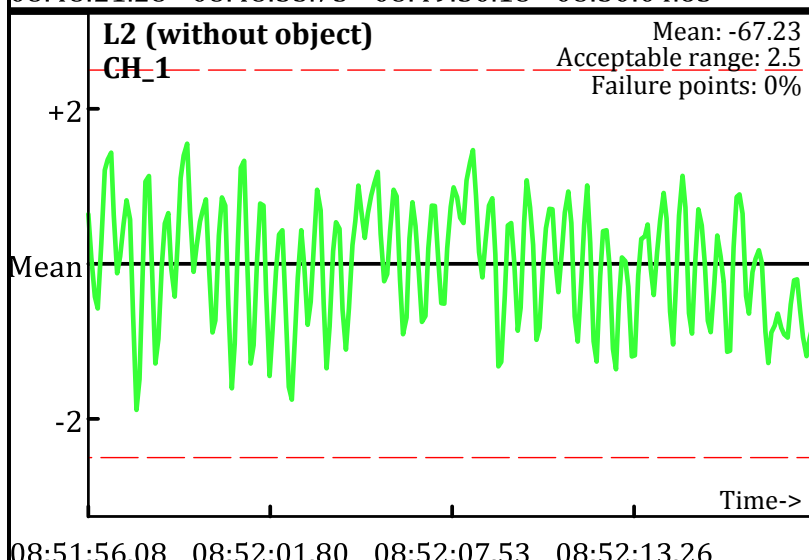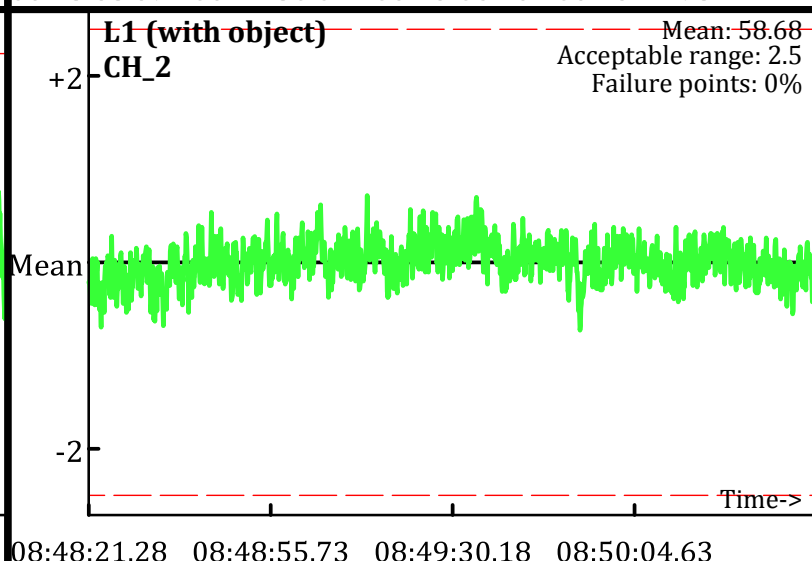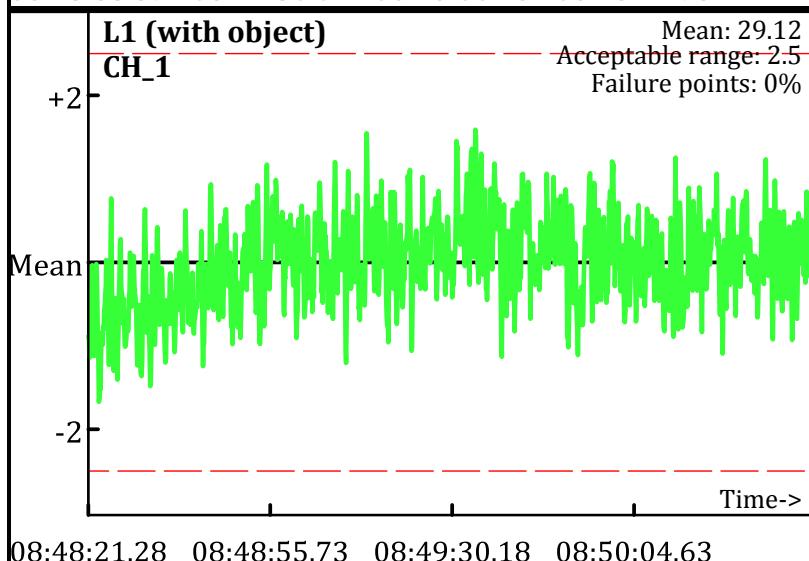Operator: PN & BS
Date: 12/1/2009

L5.2 (without object)
CH_3
Mean: 7.5
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_4
Mean: -0.34
Acceptable range: 2.5
Failure points: 0%

14:06:20.25   14:06:57.68   14:07:35.10   14:08:12.53

14:06:20.25   14:06:57.68   14:07:35.10   14:08:12.53

L6.2 (with object)
CH_3
Mean: 35.31
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_4
Mean: 11.69
Acceptable range: 2.5
Failure points: 0%

14:10:07.95   14:10:53.65   14:11:39.35   14:12:25.05   14:13

14:10:07.95   14:10:53.65   14:11:39.35   14:12:25.05   14:13

L7.2 (without object)
CH_3
Mean: 7.47
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_4
Mean: -0.36
Acceptable range: 2.5
Failure points: 0%

14:14:19.75   14:14:24.73   14:14:29.70   14:14:34.68   14:14

14:14:19.75   14:14:24.73   14:14:29.70   14:14:34.68   14:14

Database: D:\Projects_QCReports_Ord_Data\120109\QC\120109_TA_QC.gdb
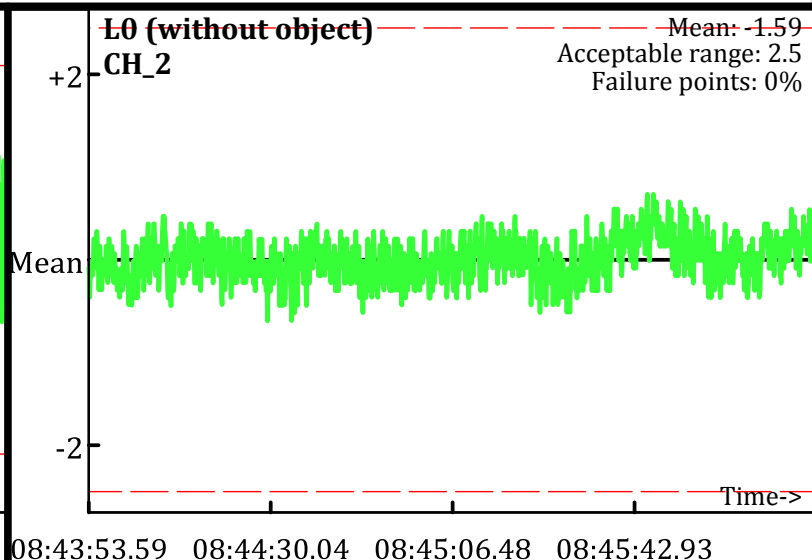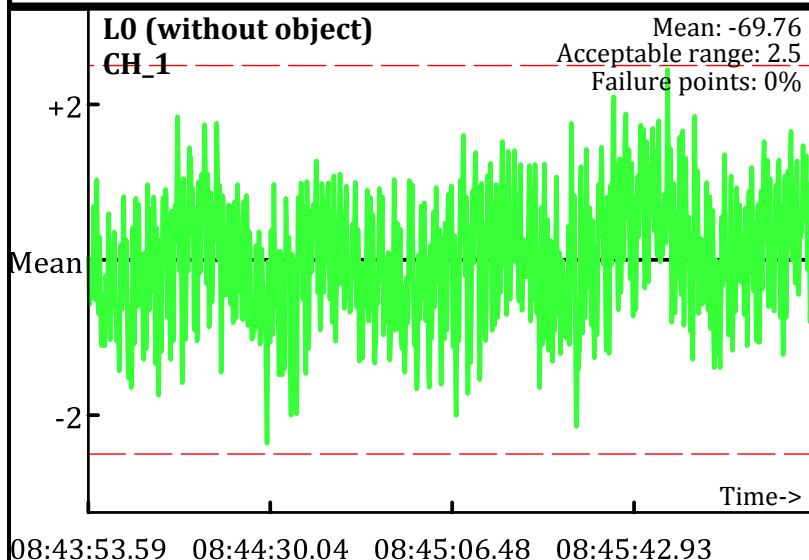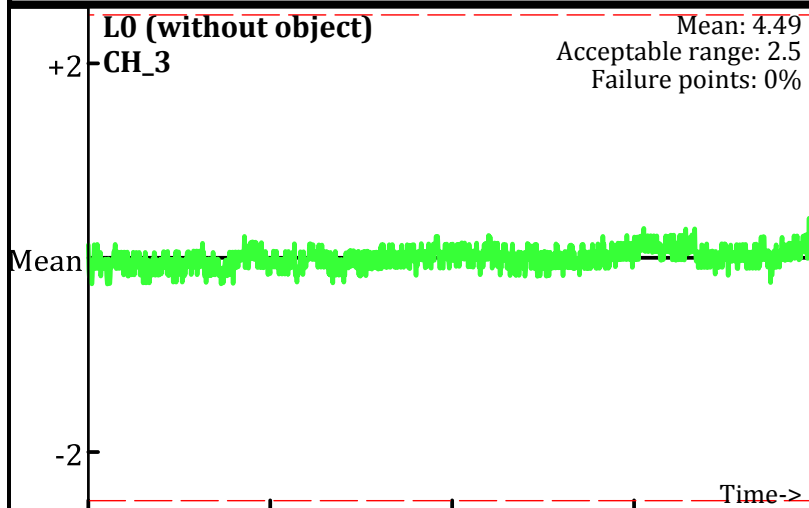Line Name: L5.2 L6.2 L7.2

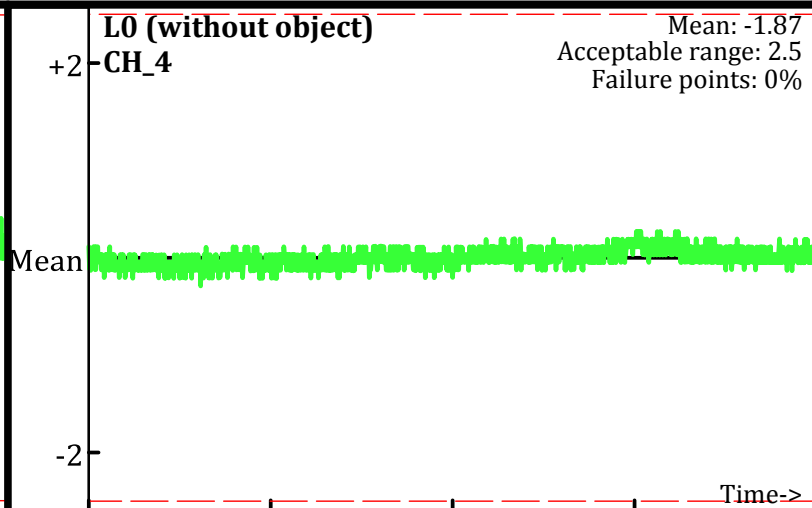Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
Date: 12/10/2009

L0 (without object)
CH_1
Mean: -69.76
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH_2
Mean: -1.59
Acceptable range: 2.5
Failure points: 0%

08:43:53.59 08:44:30.04 08:45:06.48 08:45:42.93

L1 (with object)
CH_1
Mean: 29.12
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_2
Mean: 58.68
Acceptable range: 2.5
Failure points: 0%

08:48:21.28 08:48:55.73 08:49:30.18 08:50:04.63

L2 (without object)
CH_1
Mean: -67.23
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_2
Mean: -0.93
Acceptable range: 2.5
Failure points: 0%

08:51:56.08 08:52:01.80 08:52:07.53 08:52:13.26

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area
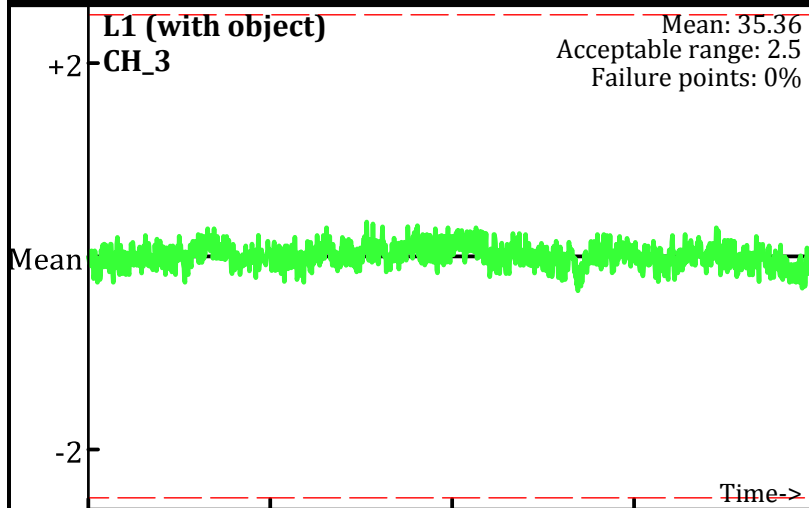
● Outside range
– – – Acceptable limits

AM test
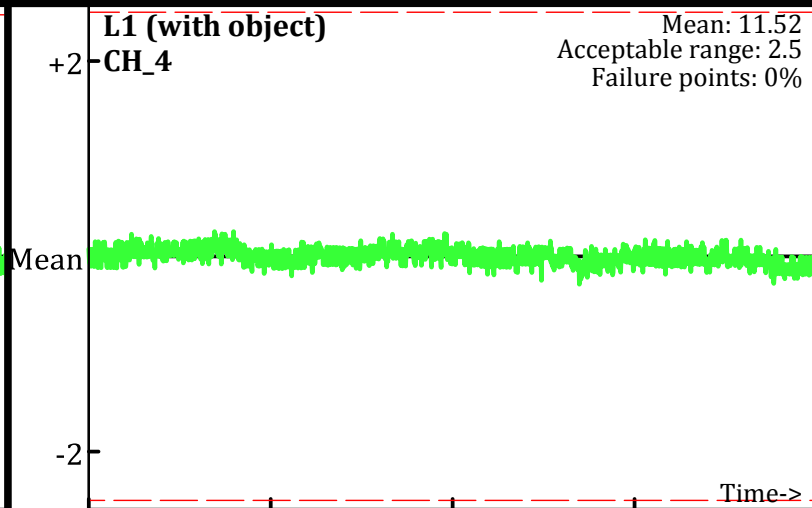Operator: PN & BR
Date: 12/10/2009

L0 (without object)
CH_3
Mean: 4.49
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:43:53.59   08:44:30.04   08:45:06.48   08:45:42.93

L0 (without object)
CH_4
Mean: -1.87
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:43:53.59   08:44:30.04   08:45:06.48   08:45:42.93

L1 (with object)
CH_3
Mean: 35.36
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:48:21.28   08:48:55.73   08:49:30.18   08:50:04.63

L1 (with object)
CH_4
Mean: 11.52
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:48:21.28   08:48:55.73   08:49:30.18   08:50:04.63

L2 (without object)
CH_3
Mean: 4.61
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:51:56.08   08:52:01.80   08:52:07.53   08:52:13.26

L2 (without object)
CH_4
Mean: -1.86
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
08:51:56.08   08:52:01.80   08:52:07.53   08:52:13.26

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
Operator: PN & BR
Date: 12/10/2009

L0.1 (without object)
CH_1
Mean: -112.51
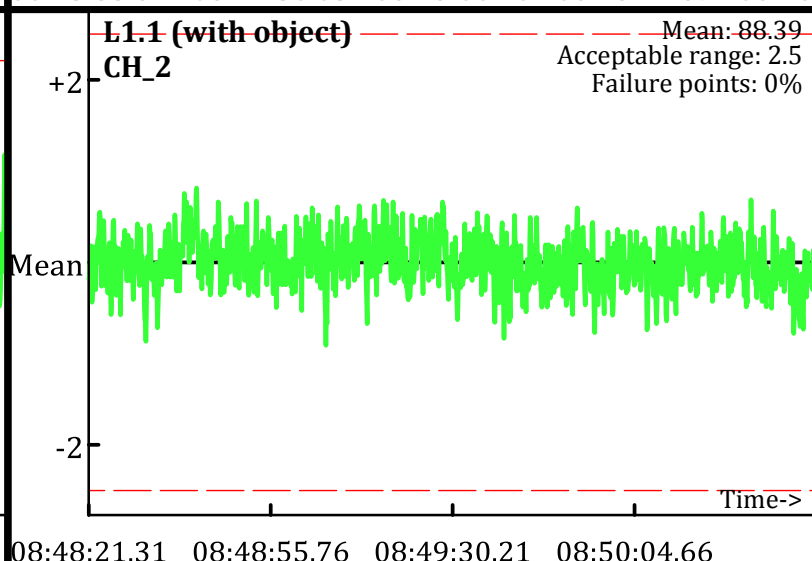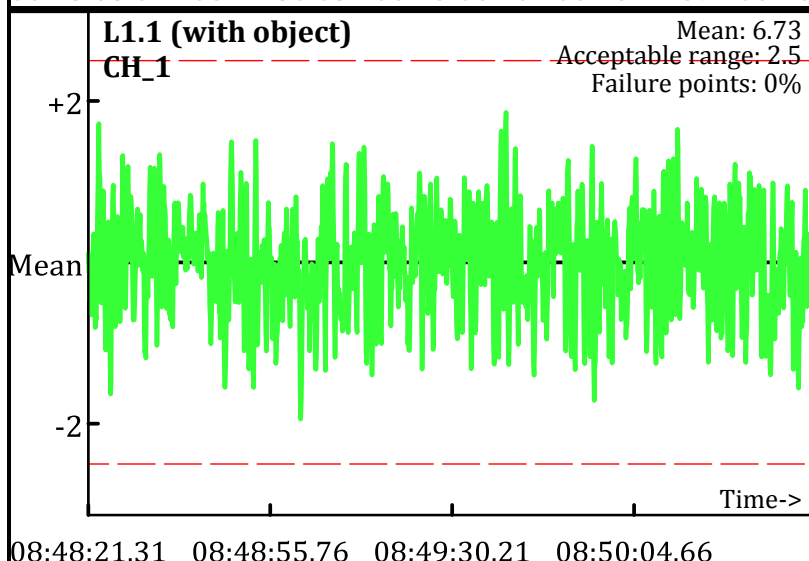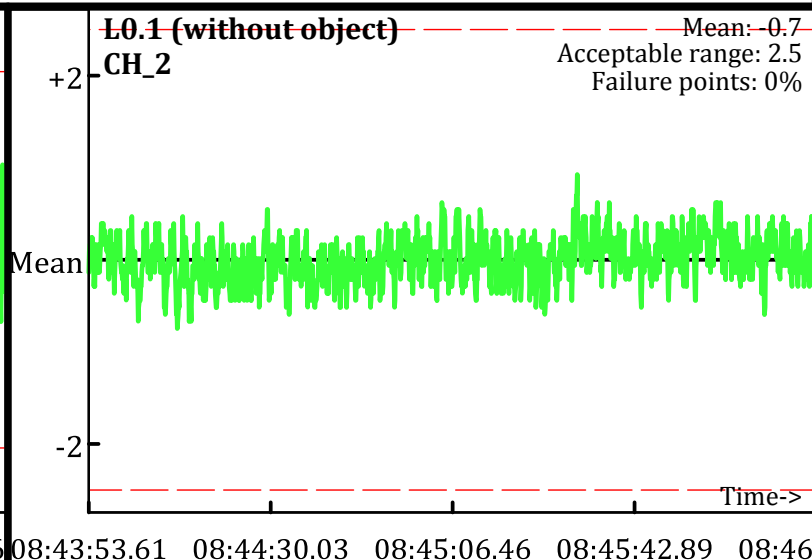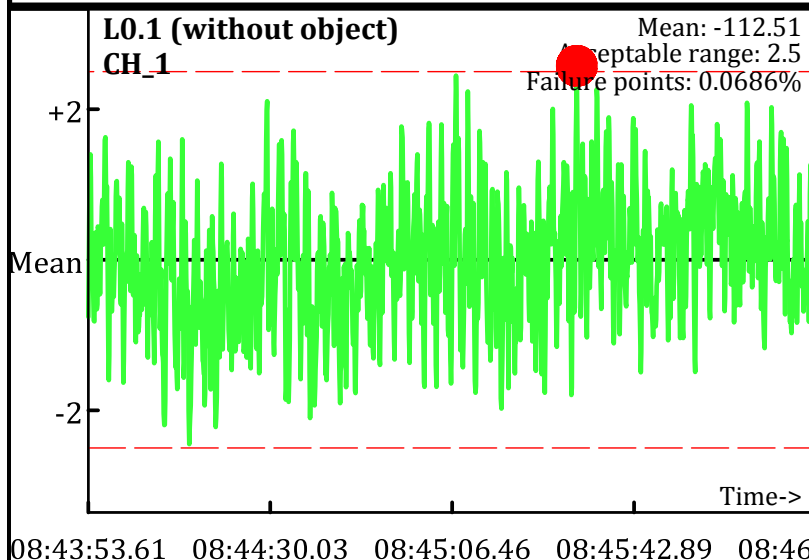Acceptable range: 2.5
Failure points: 0.0686%

L0.1 (without object)
CH_2
Mean: -0.7
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_1
Mean: 6.73
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_2
Mean: 88.39
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_1
Mean: -110.06
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_2
Mean: -0.41
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
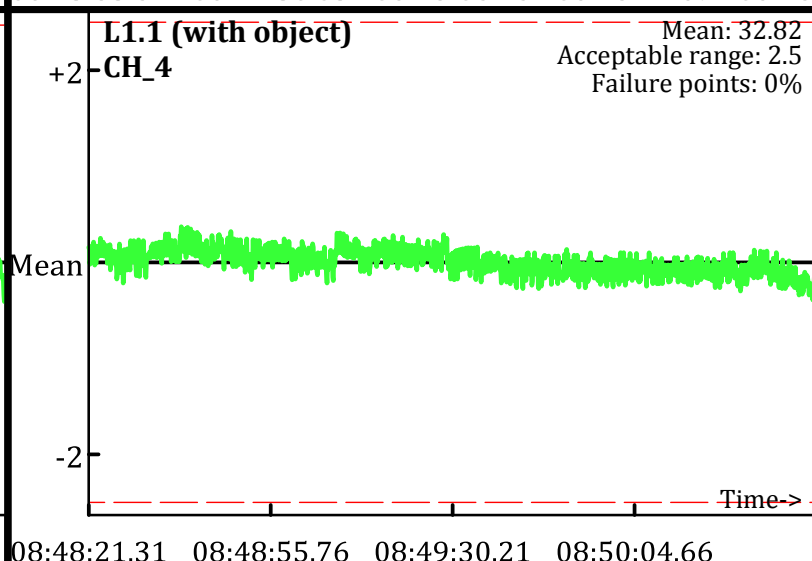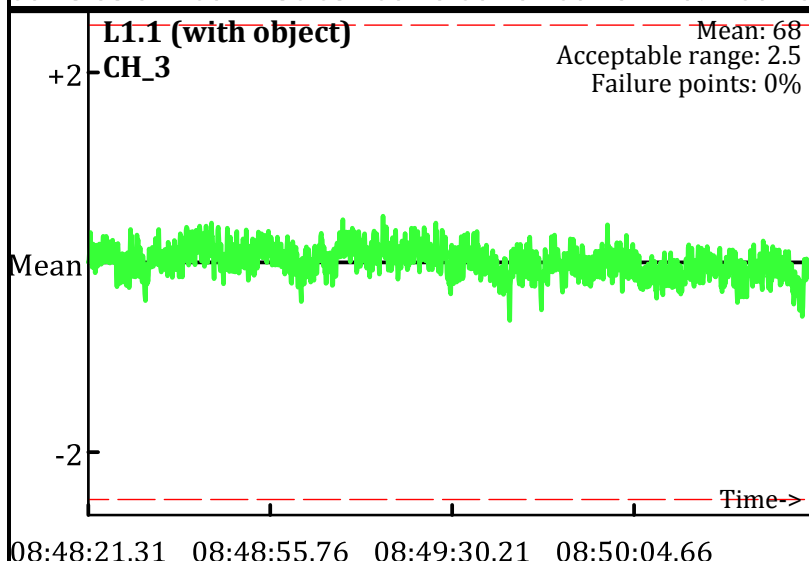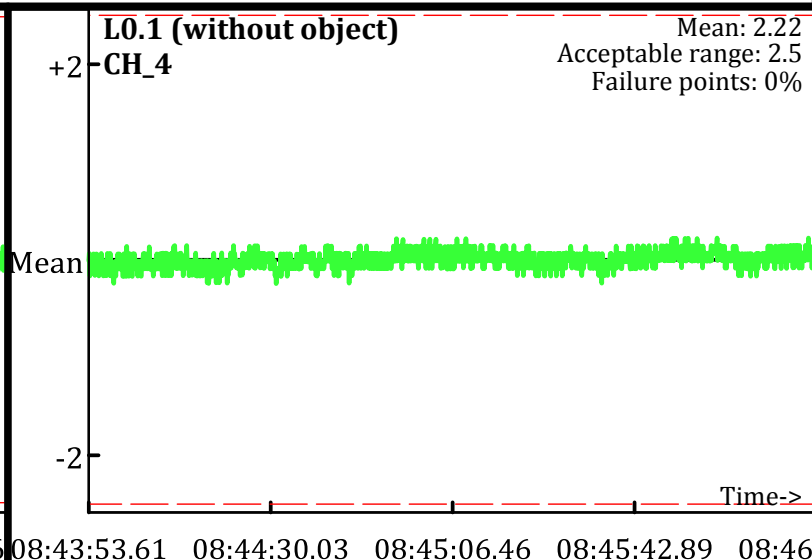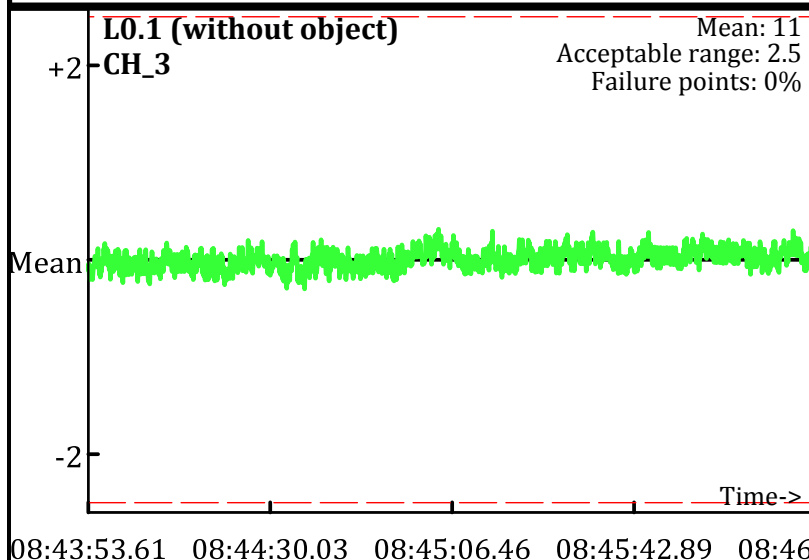Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

AM test
Operator: PN & BR
Date: 12/10/2009

L0.1 (without object)
CH_3
Mean: 11
Acceptable range: 2.5
Failure points: 0%

L0.1 (without object)
CH_4
Mean: 2.22
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_3
Mean: 68
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_4
Mean: 32.82
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_3
Mean: 10.68
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_4
Mean: 1.78
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
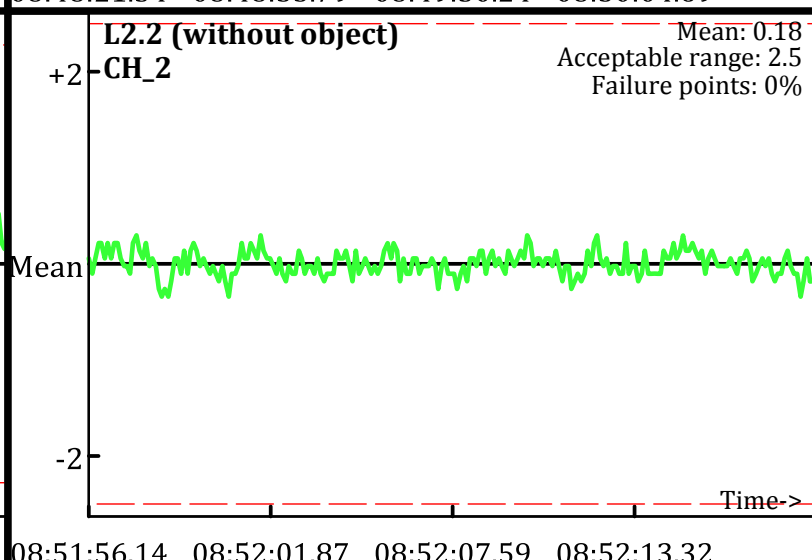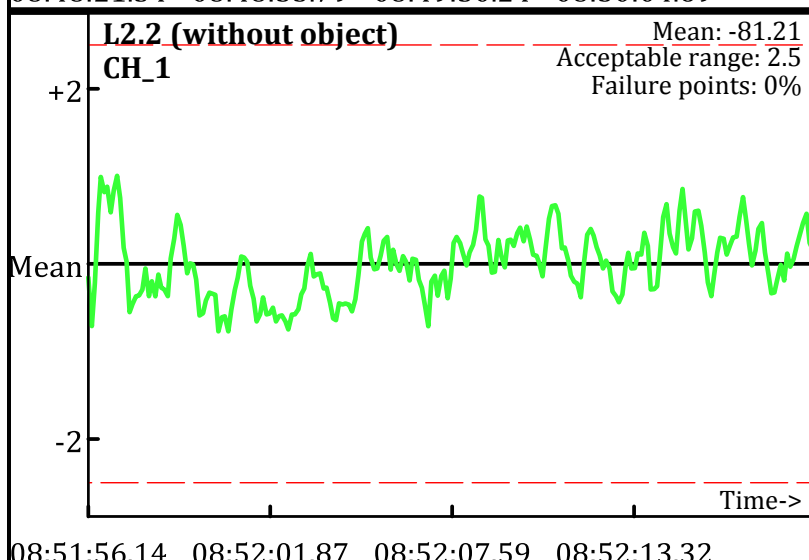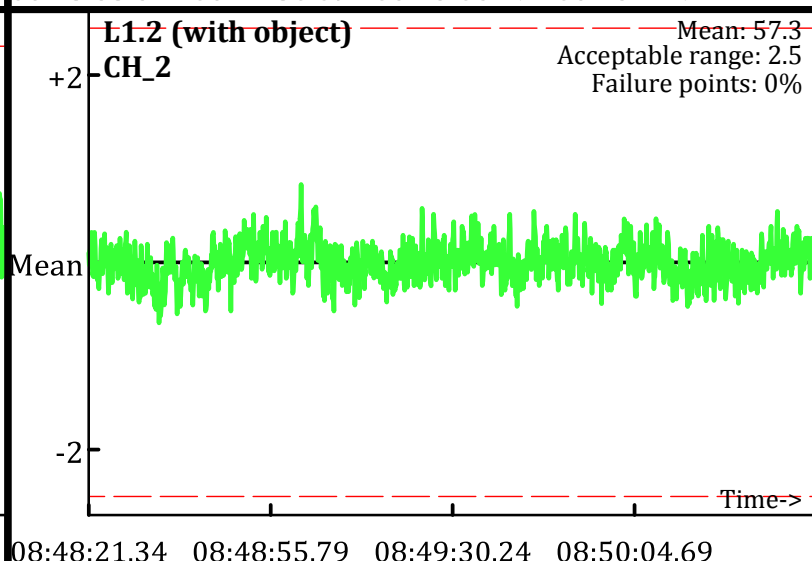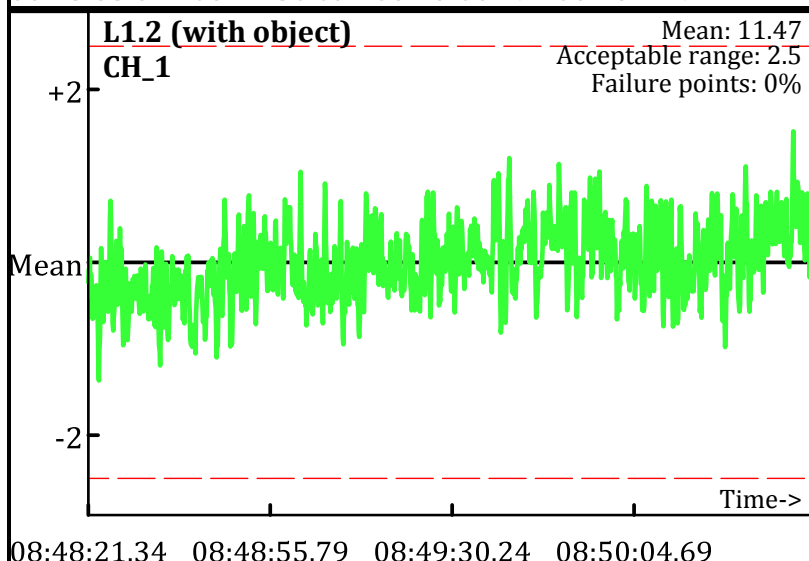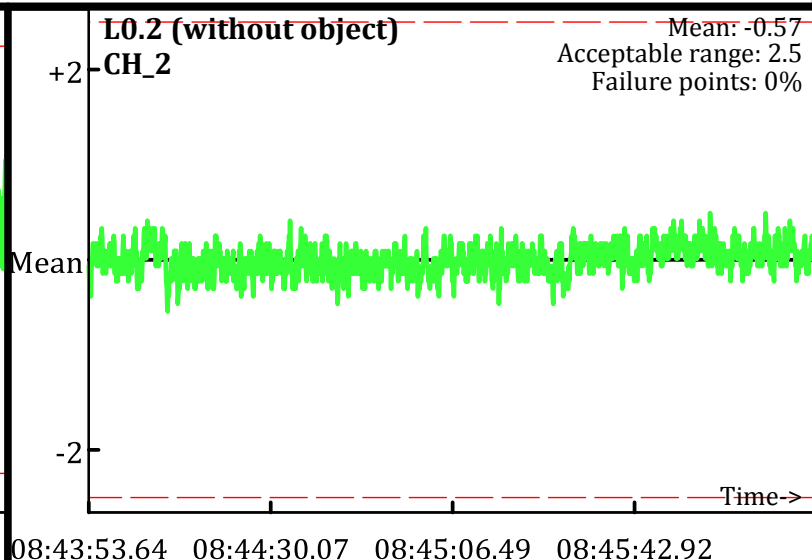–– Acceptable limits

AM test
Operator: PN & BR
Date: 12/10/2009

L0.2 (without object)
CH_1
Mean: -83.89
Acceptable range: 2.5
Failure points: 0%

Time->

08:43:53.64   08:44:30.07   08:45:06.49   08:45:42.92

L0.2 (without object)
CH_2
Mean: -0.57
Acceptable range: 2.5
Failure points: 0%

Time->

08:43:53.64   08:44:30.07   08:45:06.49   08:45:42.92

L1.2 (with object)
CH_1
Mean: 11.47
Acceptable range: 2.5
Failure points: 0%

Time->

08:48:21.34   08:48:55.79   08:49:30.24   08:50:04.69

L1.2 (with object)
CH_2
Mean: 57.3
Acceptable range: 2.5
Failure points: 0%

Time->

08:48:21.34   08:48:55.79   08:49:30.24   08:50:04.69

L2.2 (without object)
CH_1
Mean: -81.21
Acceptable range: 2.5
Failure points: 0%

Time->

08:51:56.14   08:52:01.87   08:52:07.59   08:52:13.32

L2.2 (without object)
CH_2
Mean: 0.18
Acceptable range: 2.5
Failure points: 0%

Time->

08:51:56.14   08:52:01.87   08:52:07.59   08:52:13.32

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L0.2 L1.2 L2.2

Page: 1

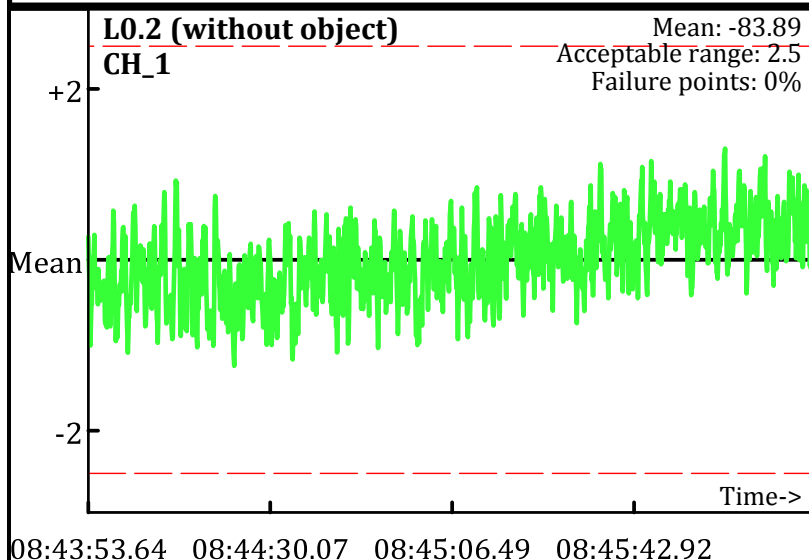# Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
Date: 12/10/2009
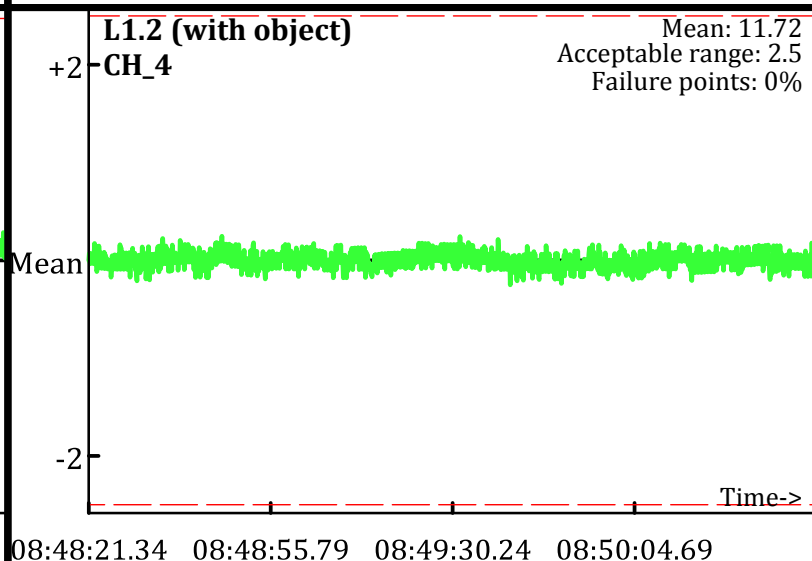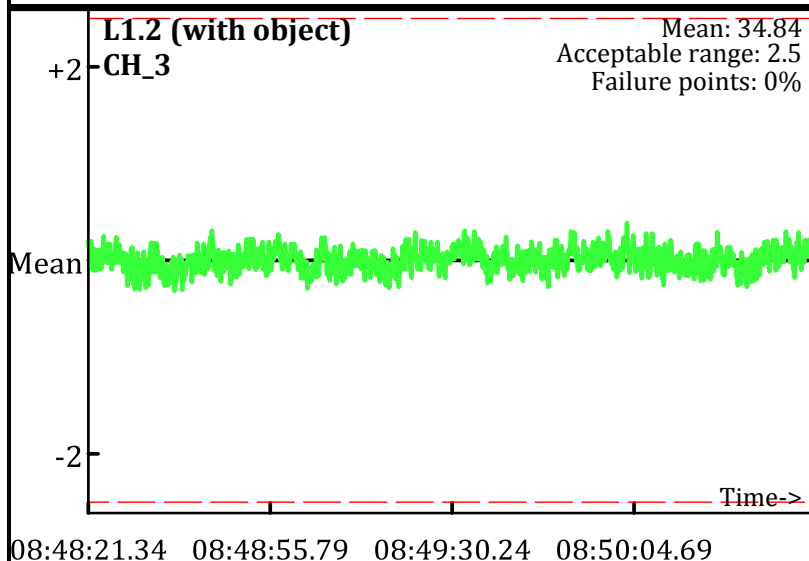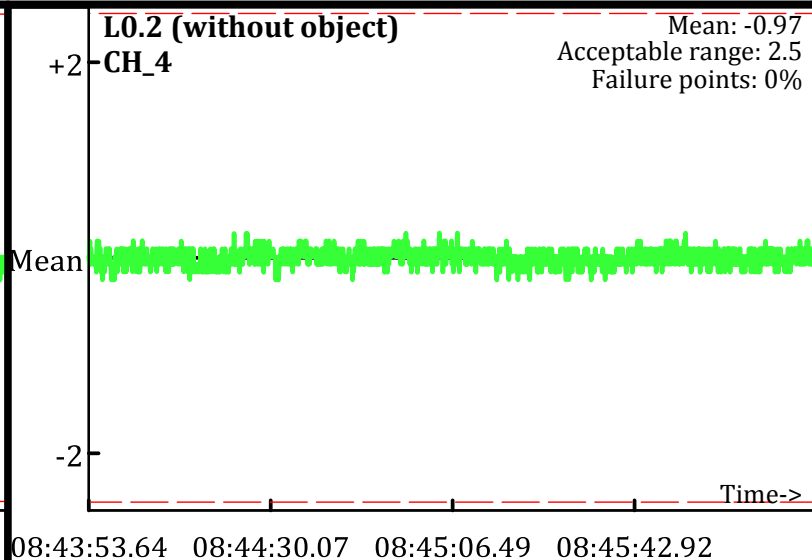
L0.2 (without object)
CH_3
Mean: 5.32
Acceptable range: 2.5
Failure points: 0%

L0.2 (without object)
CH_4
Mean: -0.97
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_3
Mean: 34.84
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_4
Mean: 11.72
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_3
Mean: 5.47
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_4
Mean: -0.95
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
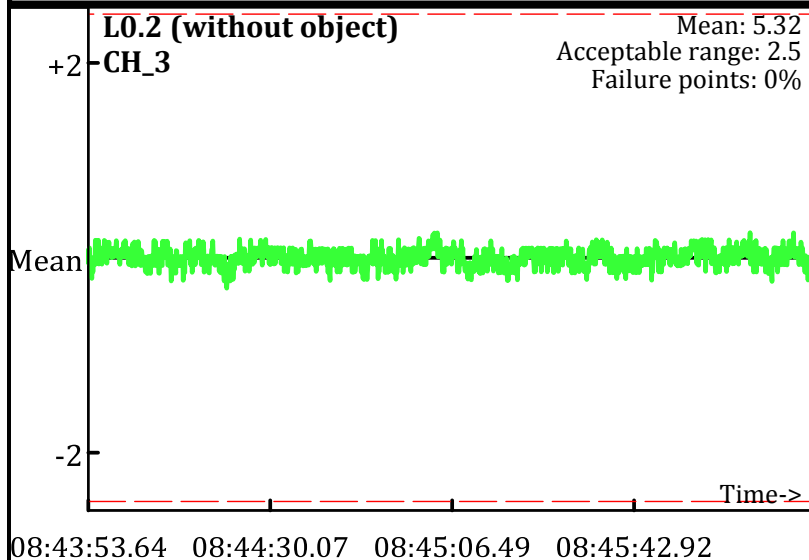Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
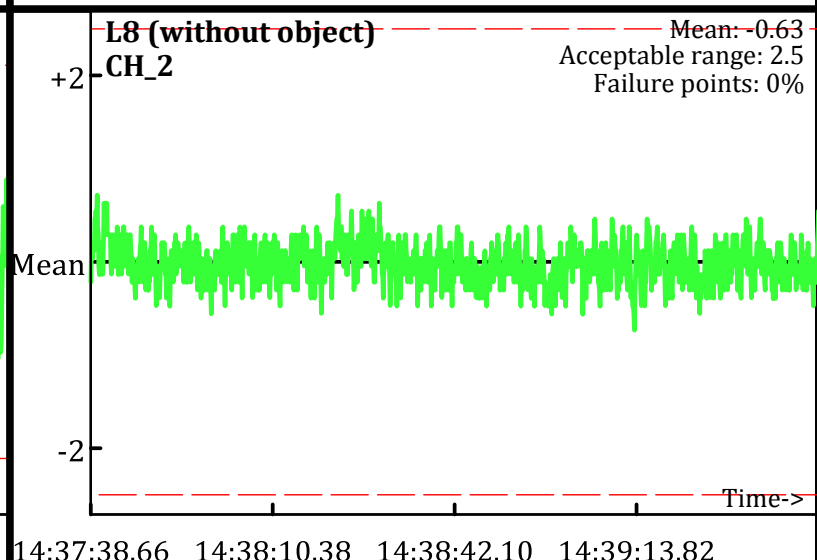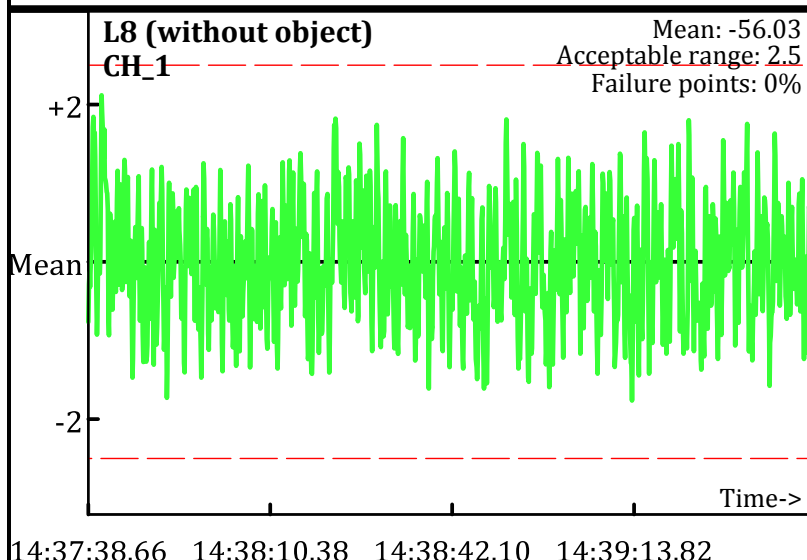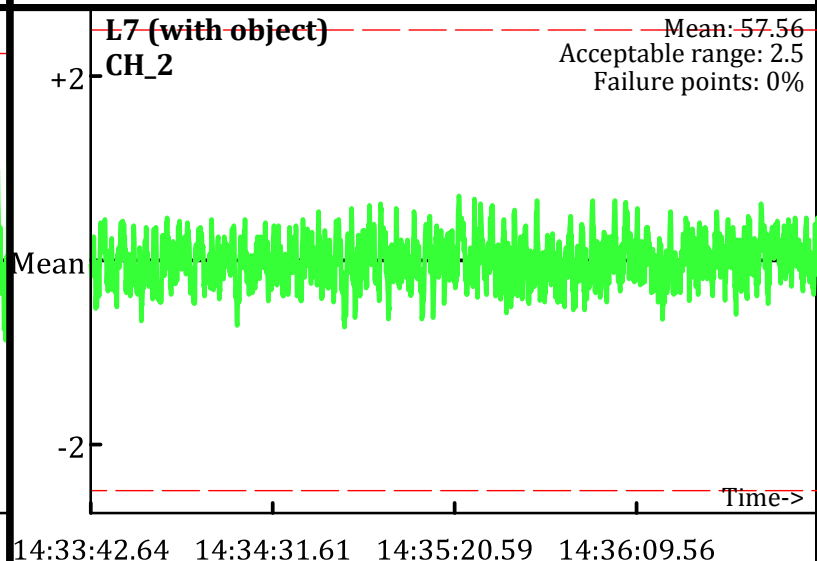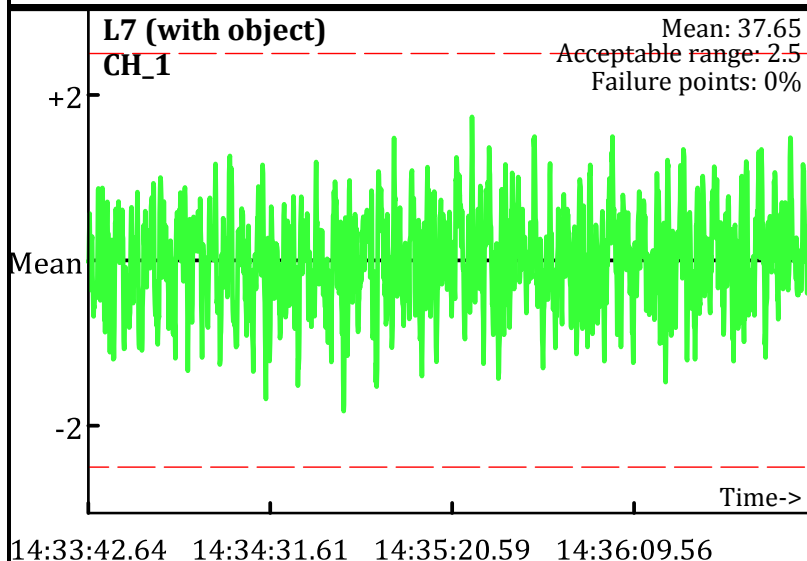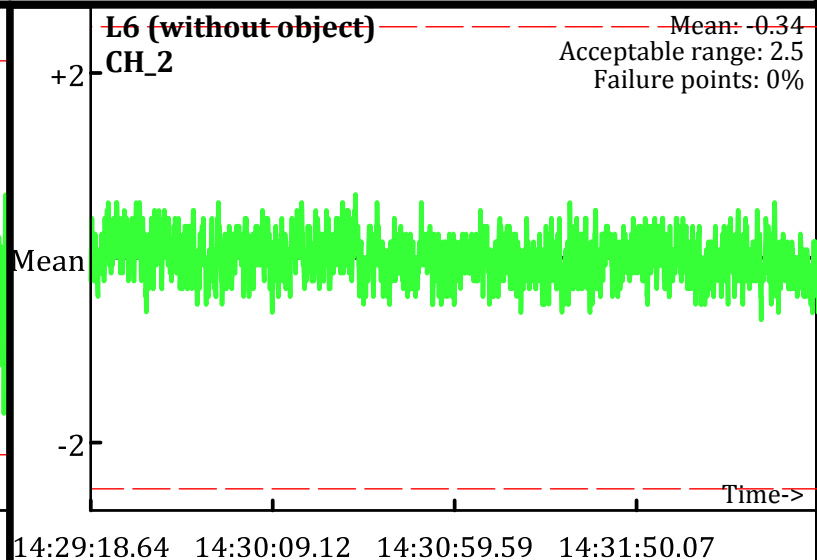— — Acceptable limits

PM test
Operator: PN & BR
Date: 12/10/2009

L6 (without object)
CH_1
Mean: -55.34
Acceptable range: 2.5
Failure points: 0%

Time->

14:29:18.64   14:30:09.12   14:30:59.59   14:31:50.07

L6 (without object)
CH_2
Mean: -0.34
Acceptable range: 2.5
Failure points: 0%

Time->

14:29:18.64   14:30:09.12   14:30:59.59   14:31:50.07

L7 (with object)
CH_1
Mean: 37.65
Acceptable range: 2.5
Failure points: 0%

Time->

14:33:42.64   14:34:31.61   14:35:20.59   14:36:09.56

L7 (with object)
CH_2
Mean: 57.56
Acceptable range: 2.5
Failure points: 0%

Time->

14:33:42.64   14:34:31.61   14:35:20.59   14:36:09.56

L8 (without object)
CH_1
Mean: -56.03
Acceptable range: 2.5
Failure points: 0%

Time->

14:37:38.66   14:38:10.38   14:38:42.10   14:39:13.82

L8 (without object)
CH_2
Mean: -0.63
Acceptable range: 2.5
Failure points: 0%

Time->

14:37:38.66   14:38:10.38   14:38:42.10   14:39:13.82

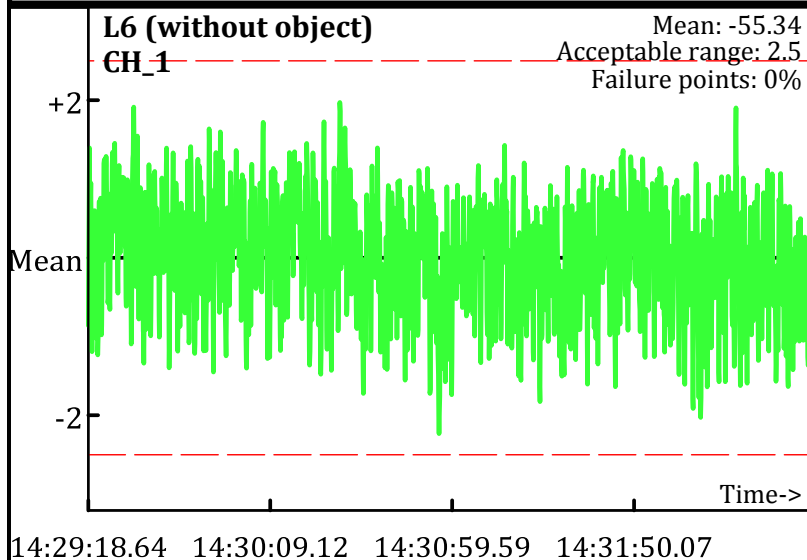Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L6 L7 L8

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 12/10/2009
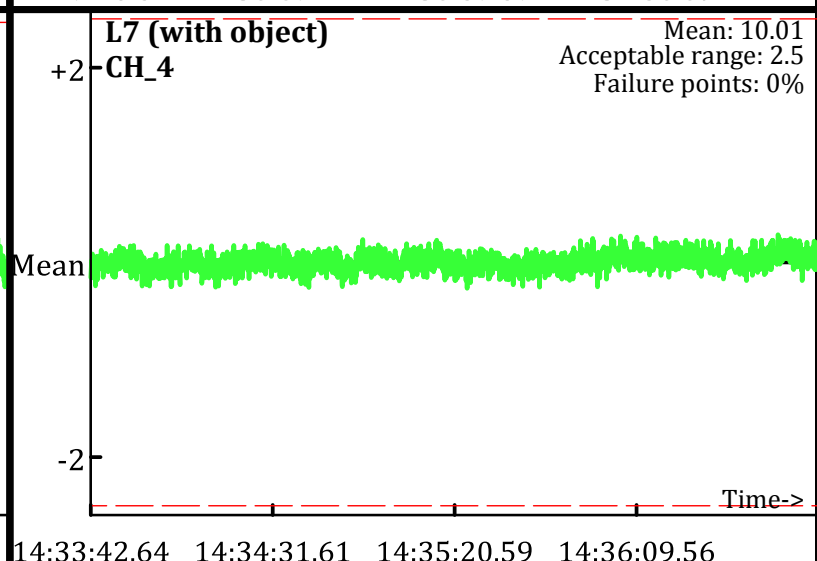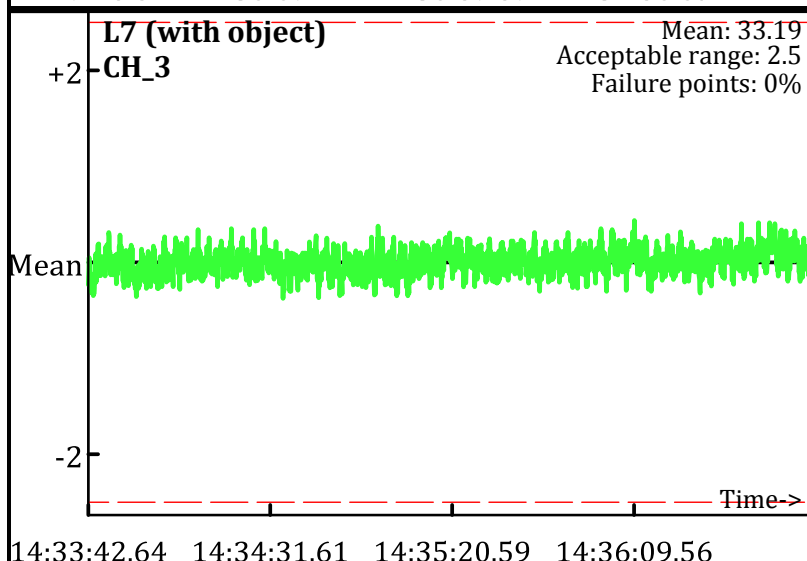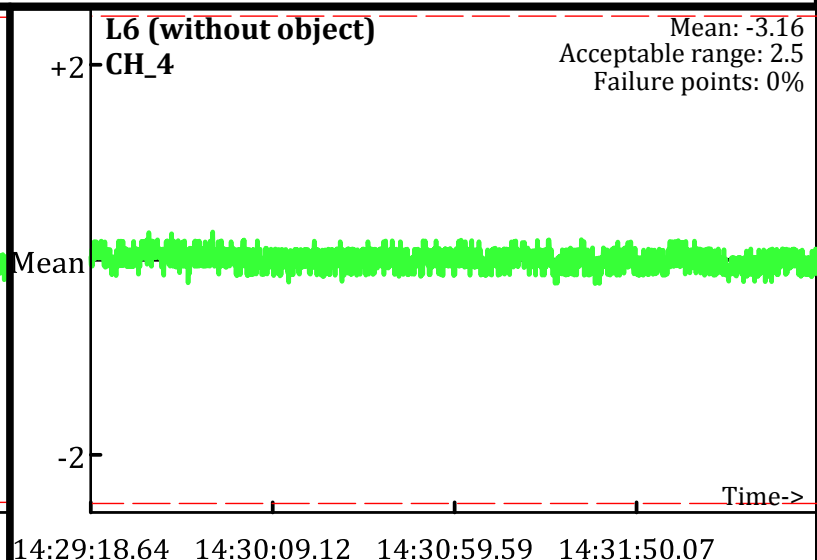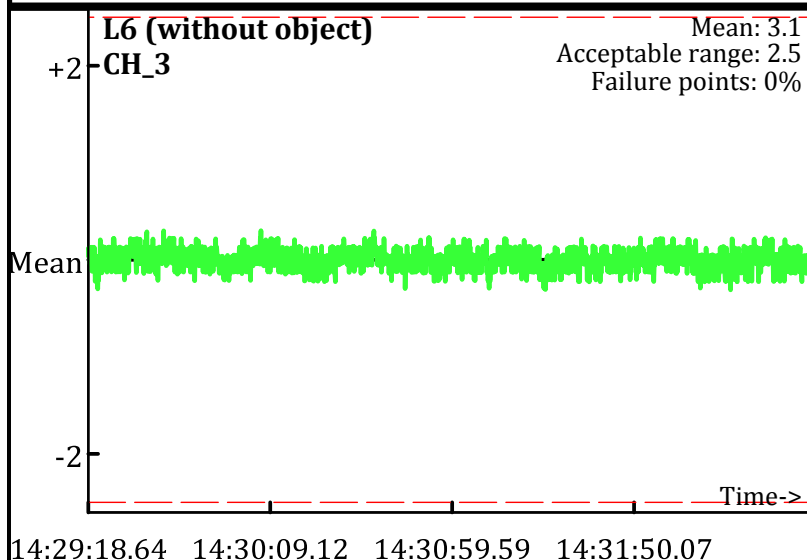
L6 (without object)
CH_3
Mean: 3.1
Acceptable range: 2.5
Failure points: 0%

L6 (without object)
CH_4
Mean: -3.16
Acceptable range: 2.5
Failure points: 0%

14:29:18.64   14:30:09.12   14:30:59.59   14:31:50.07

14:29:18.64   14:30:09.12   14:30:59.59   14:31:50.07

L7 (with object)
CH_3
Mean: 33.19
Acceptable range: 2.5
Failure points: 0%

L7 (with object)
CH_4
Mean: 10.01
Acceptable range: 2.5
Failure points: 0%

14:33:42.64   14:34:31.61   14:35:20.59   14:36:09.56

14:33:42.64   14:34:31.61   14:35:20.59   14:36:09.56

L8 (without object)
CH_3
Mean: 3.05
Acceptable range: 2.5
Failure points: 0%

L8 (without object)
CH_4
Mean: -3.2
Acceptable range: 2.5
Failure points: 0%

14:37:38.66   14:38:10.38   14:38:42.10   14:39:13.82

14:37:38.66   14:38:10.38   14:38:42.10   14:39:13.82

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L6 L7 L8

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits
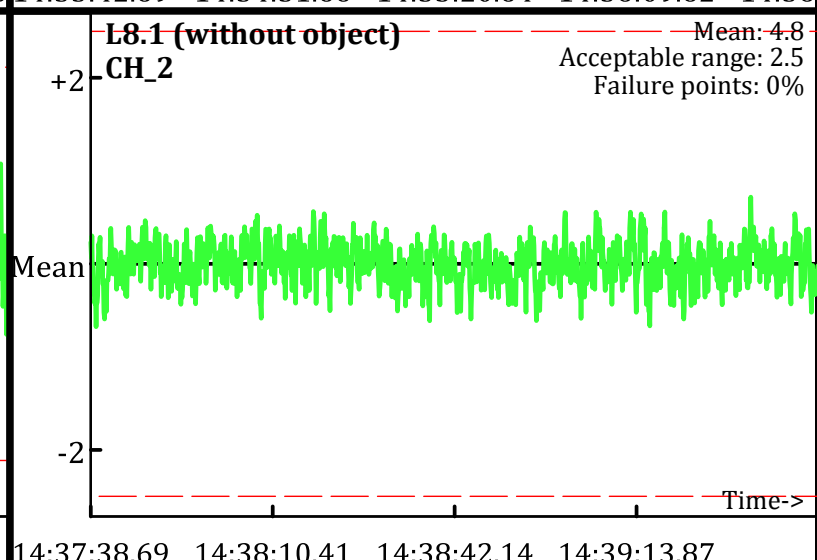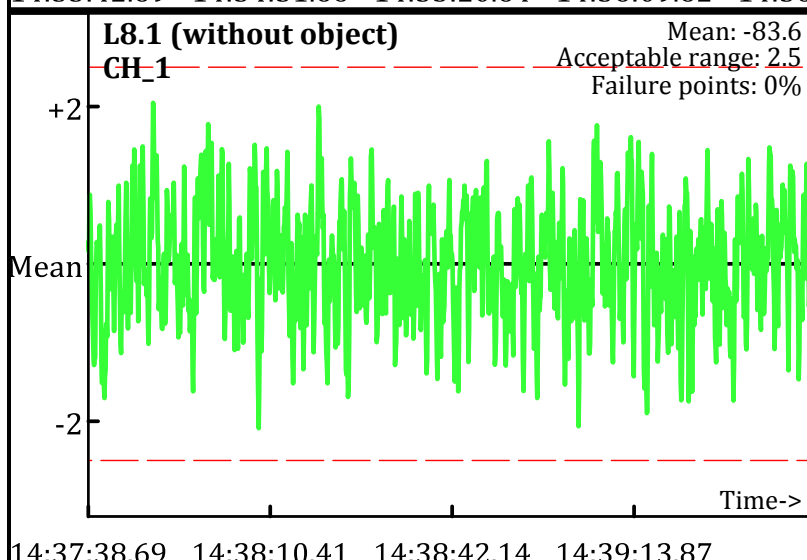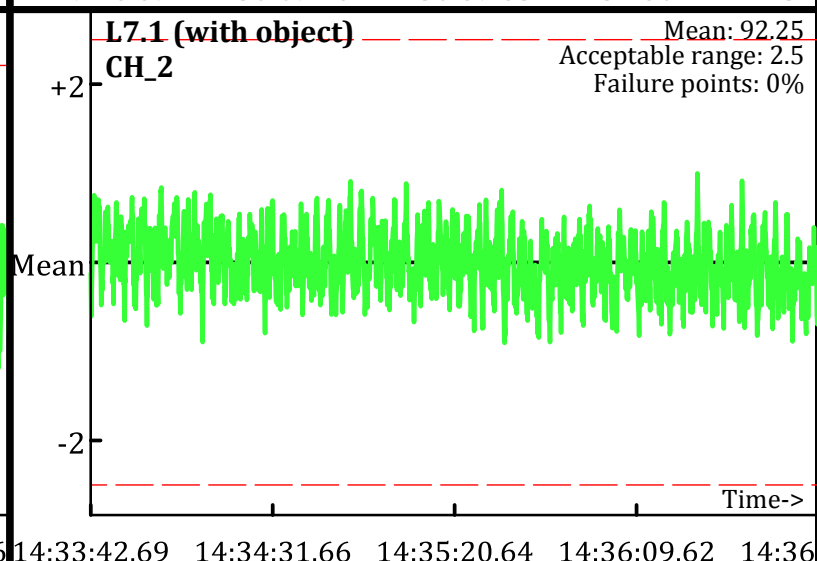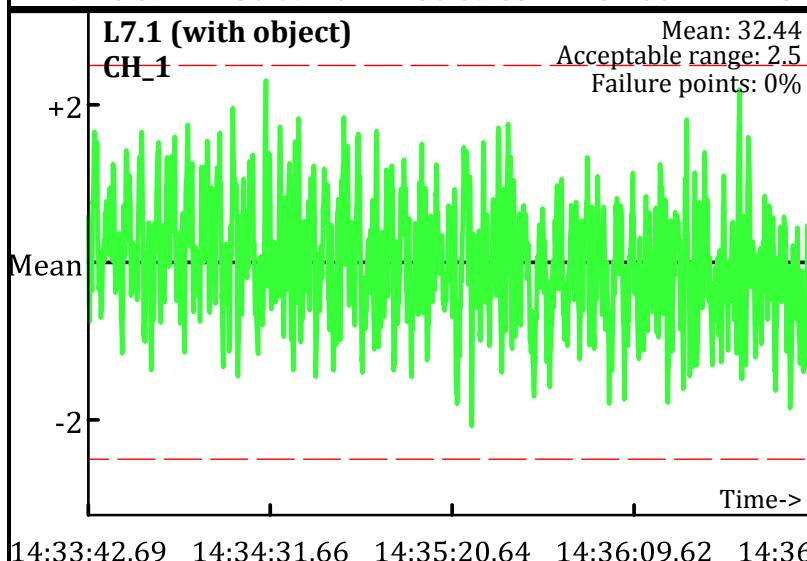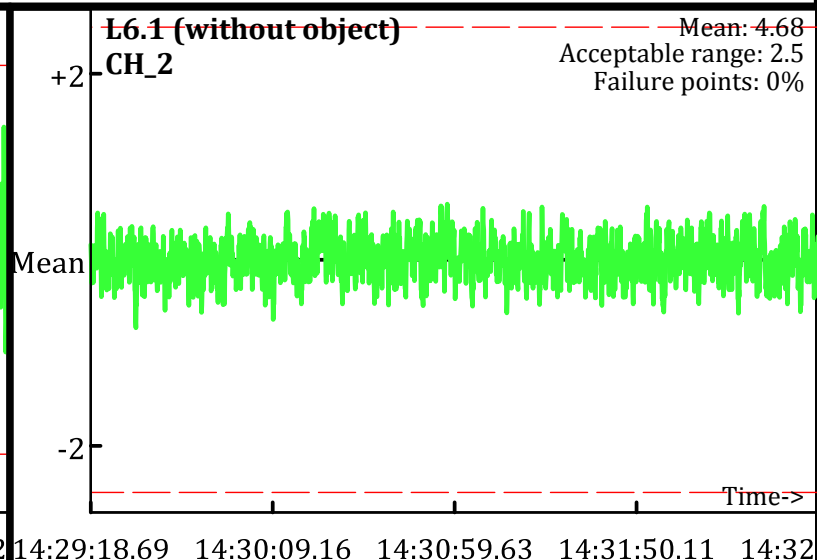
PM test
Operator: PN & BR
Date: 12/10/2009

L6.1 (without object)
CH_1
Mean: -83.59
Acceptable range: 2.5
Failure points: 0%

L6.1 (without object)
CH_2
Mean: 4.68
Acceptable range: 2.5
Failure points: 0%

L7.1 (with object)
CH_1
Mean: 32.44
Acceptable range: 2.5
Failure points: 0%

L7.1 (with object)
CH_2
Mean: 92.25
Acceptable range: 2.5
Failure points: 0%

L8.1 (without object)
CH_1
Mean: -83.6
Acceptable range: 2.5
Failure points: 0%

L8.1 (without object)
CH_2
Mean: 4.8
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
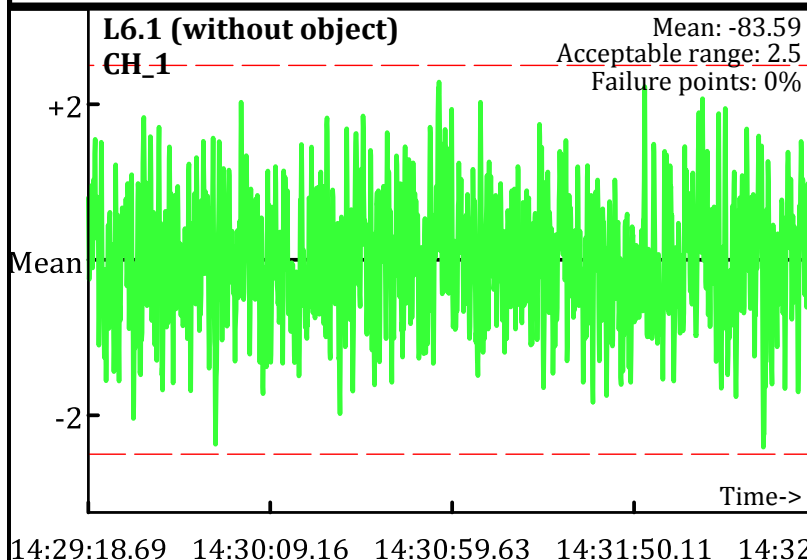Line Name: L6.1 L7.1 L8.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
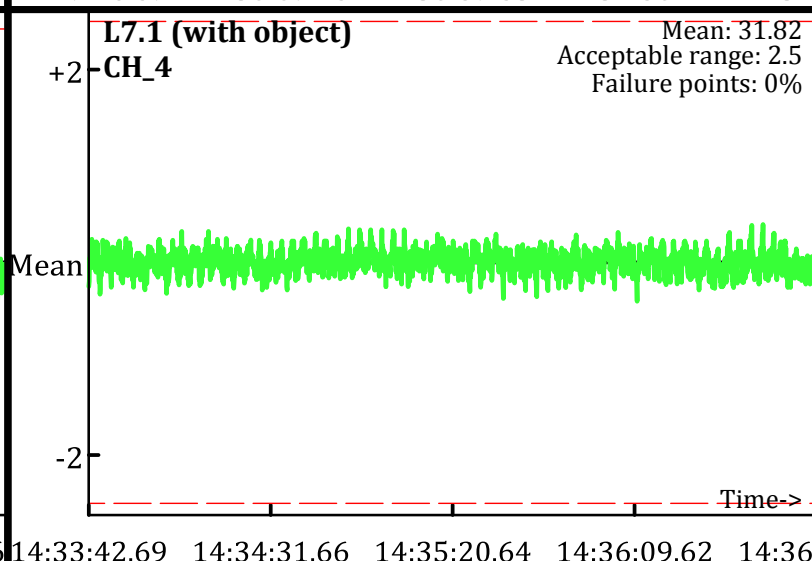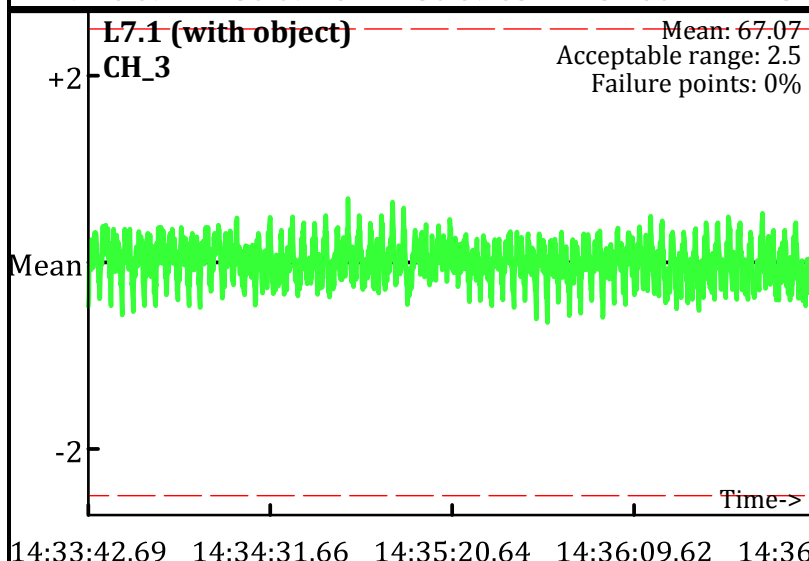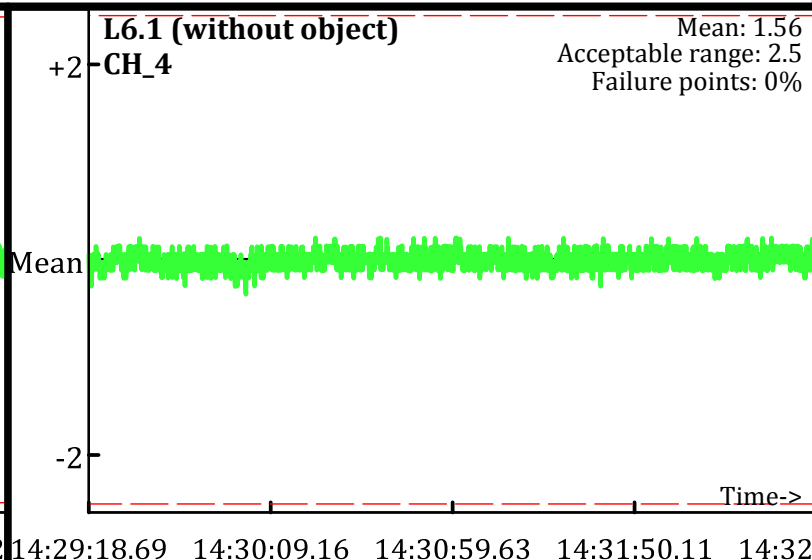Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 12/10/2009

L6.1 (without object)
CH_3
Mean: 10.82
Acceptable range: 2.5
Failure points: 0%

Time->

14:29:18.69   14:30:09.16   14:30:59.63   14:31:50.11   14:32

L6.1 (without object)
CH_4
Mean: 1.56
Acceptable range: 2.5
Failure points: 0%

Time->

14:29:18.69   14:30:09.16   14:30:59.63   14:31:50.11   14:32

L7.1 (with object)
CH_3
Mean: 67.07
Acceptable range: 2.5
Failure points: 0%

Time->

14:33:42.69   14:34:31.66   14:35:20.64   14:36:09.62   14:36

L7.1 (with object)
CH_4
Mean: 31.82
Acceptable range: 2.5
Failure points: 0%

Time->

14:33:42.69   14:34:31.66   14:35:20.64   14:36:09.62   14:36

L8.1 (without object)
CH_3
Mean: 10.92
Acceptable range: 2.5
Failure points: 0%

Time->

14:37:38.69   14:38:10.41   14:38:42.14   14:39:13.87

L8.1 (without object)
CH_4
Mean: 1.6
Acceptable range: 2.5
Failure points: 0%

Time->

14:37:38.69   14:38:10.41   14:38:42.14   14:39:13.87

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
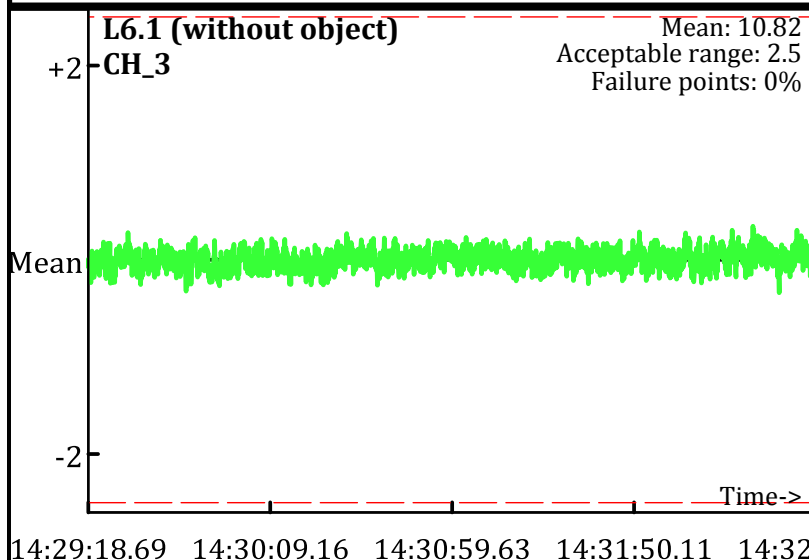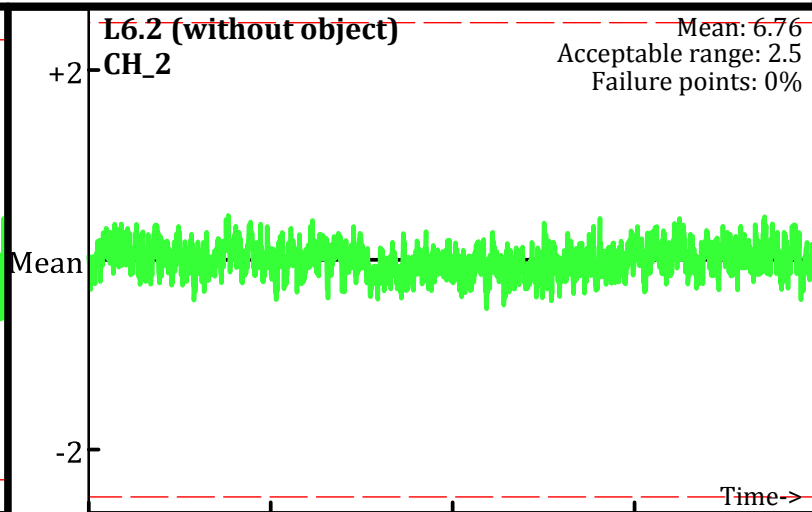Line Name: L6.1 L7.1 L8.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
-- -- Acceptable limits

PM test
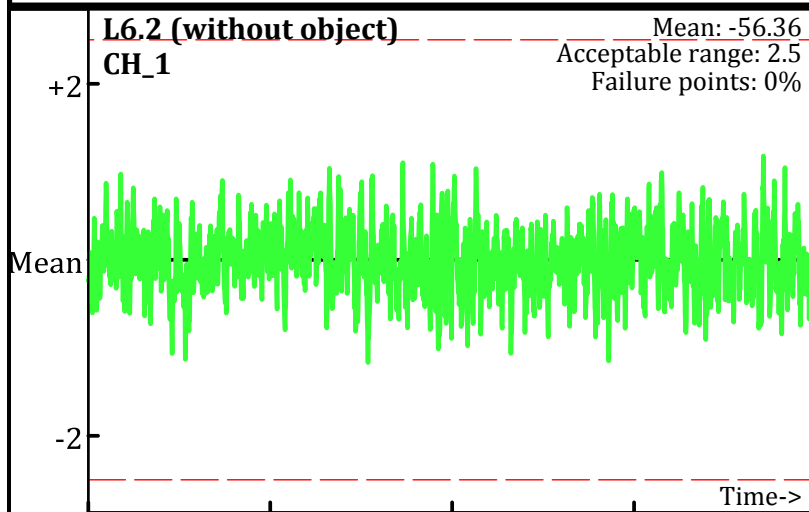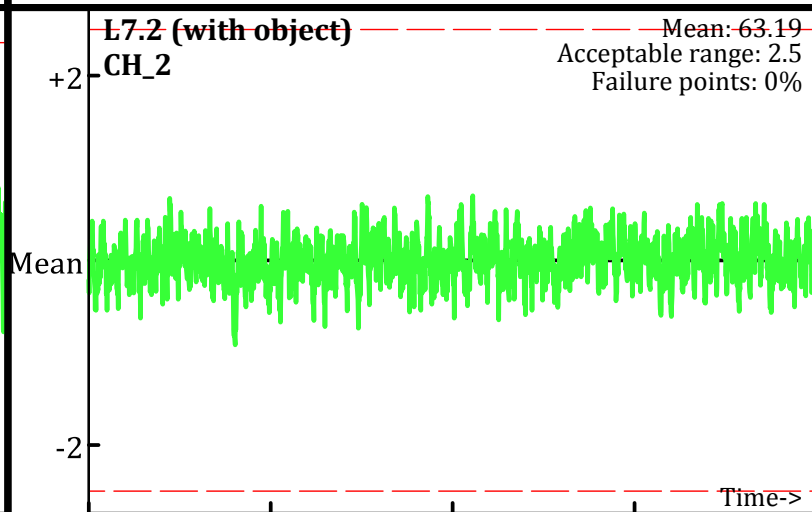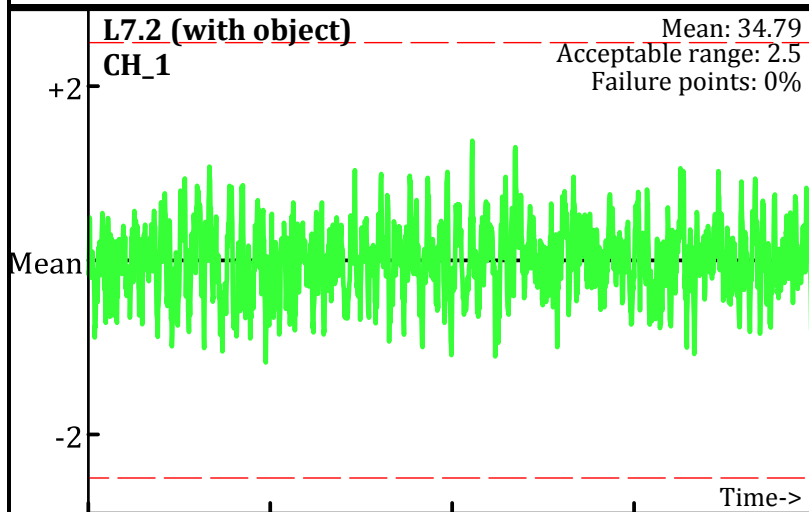Operator: PN & BR
Date: 12/10/2009

L6.2 (without object)
CH_1
Mean: -56.36
Acceptable range: 2.5
Failure points: 0%

L6.2 (without object)
CH_2
Mean: 6.76
Acceptable range: 2.5
Failure points: 0%

Time->

14:29:18.62   14:30:09.13   14:30:59.63   14:31:50.13

L7.2 (with object)
CH_1
Mean: 34.79
Acceptable range: 2.5
Failure points: 0%

L7.2 (with object)
CH_2
Mean: 63.19
Acceptable range: 2.5
Failure points: 0%

Time->

14:33:42.63   14:34:31.62   14:35:20.62   14:36:09.62   14:36

L8.2 (without object)
CH_1
Mean: -56.36
Acceptable range: 2.5
Failure points: 0%

L8.2 (without object)
CH_2
Mean: 6.83
Acceptable range: 2.5
Failure points: 0%

Time->
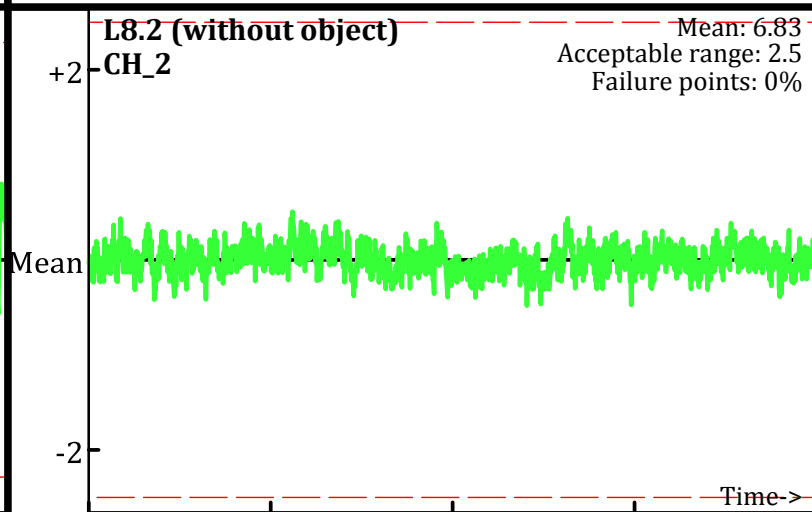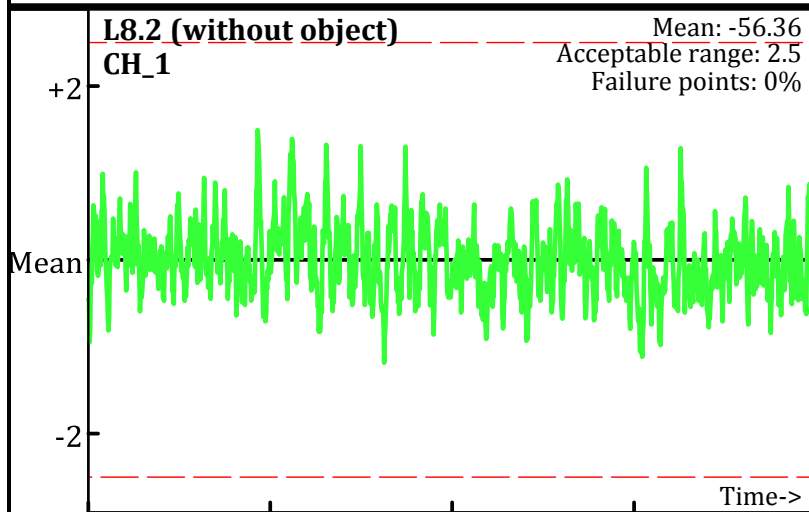
14:37:38.72   14:38:10.44   14:38:42.17   14:39:13.90

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L6.2 L7.2 L8.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
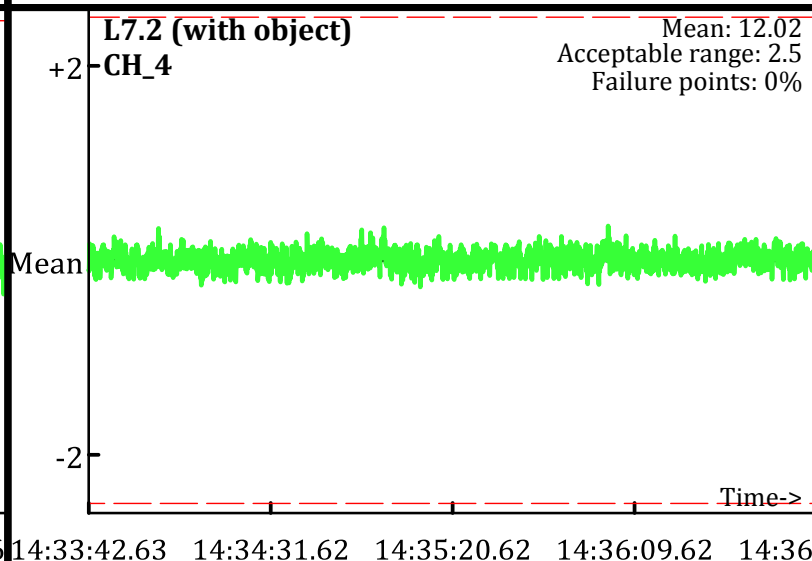- - - Acceptable limits

PM test
Operator: PN & BR
Date: 12/10/2009

L6.2 (without object) CH_3 — Mean: 7, Acceptable range: 2.5, Failure points: 0%
Time range: 14:29:18.62 — 14:31:50.13

L6.2 (without object) CH_4 — Mean: -0.72, Acceptable range: 2.5, Failure points: 0%
Time range: 14:29:18.62 — 14:31:50.13

L7.2 (with object) CH_3 — Mean: 36.18, Acceptable range: 2.5, Failure points: 0%
Time range: 14:33:42.63 — 14:36

L7.2 (with object) CH_4 — Mean: 12.02, Acceptable range: 2.5, Failure points: 0%
Time range: 14:33:42.63 — 14:36

L8.2 (without object) CH_3 — Mean: 7.05, Acceptable range: 2.5, Failure points: 0%
Time range: 14:37:38.72 — 14:39:13.90

L8.2 (without object) CH_4 — Mean: -0.7, Acceptable range: 2.5, Failure points: 0%
Time range: 14:37:38.72 — 14:39:13.90

Database: D:\Projects_QCReports_Ord_Data\121009\QC\121009_TA_QC.gdb
Line Name: L6.2 L7.2 L8.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
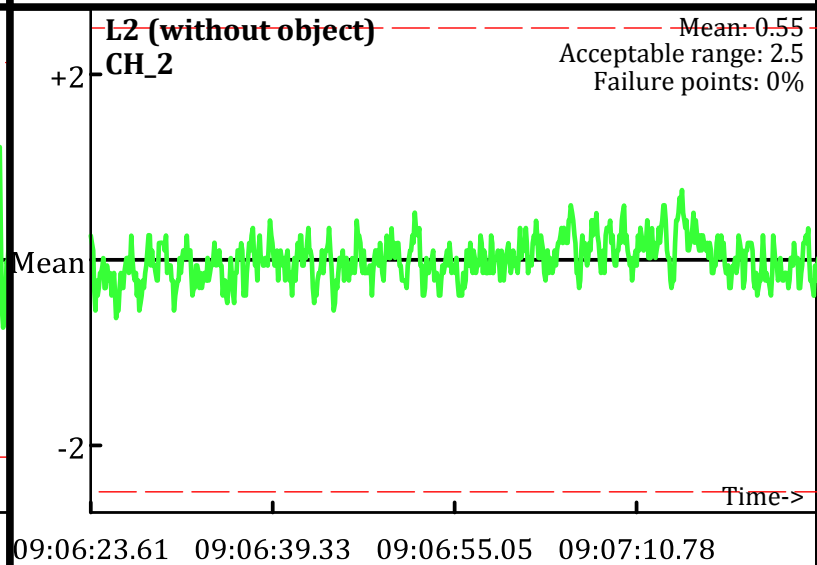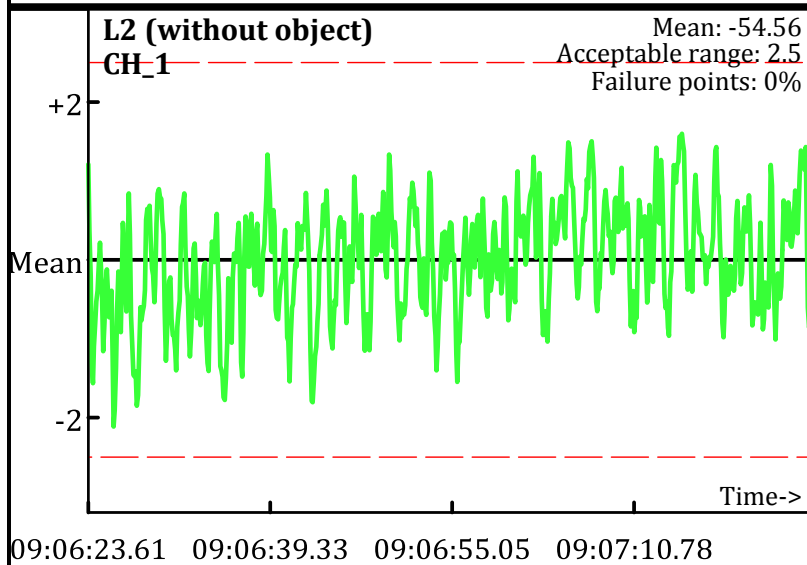– – – Acceptable limits

AM test
Operator: PN & BR
Date: 12/29/2009

L0 (without object)
CH_1
Mean: -60.16
Acceptable range: 2.5
Failure points: 0.529%

L0 (without object)
CH_2
Mean: -1.15
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_1
Mean: 37.37
Acceptable range: 2.5
Failure points: 0.0996%

L1 (with object)
CH_2
Mean: 58.2
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_1
Mean: -54.56
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_2
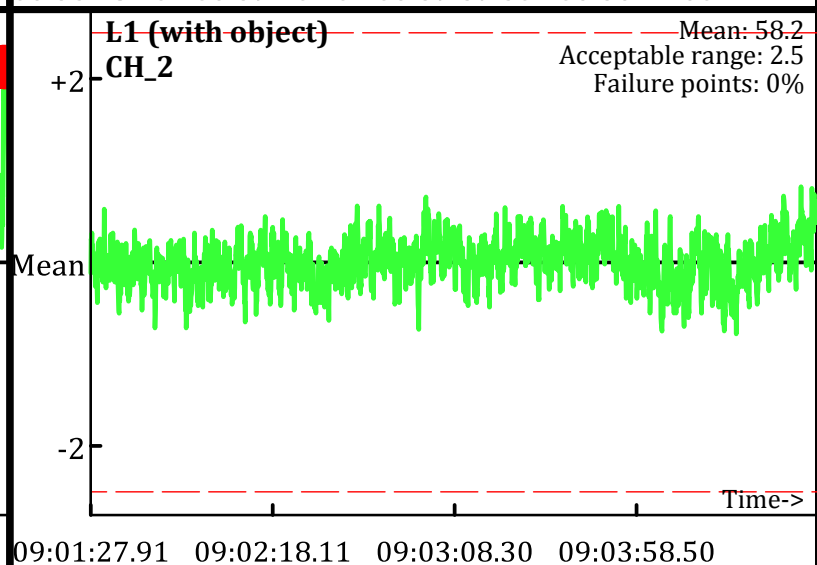Mean: 0.55
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
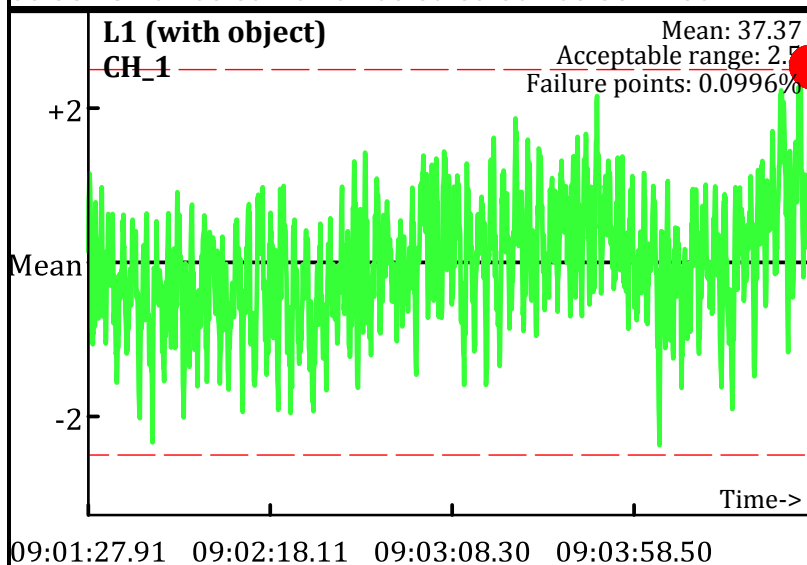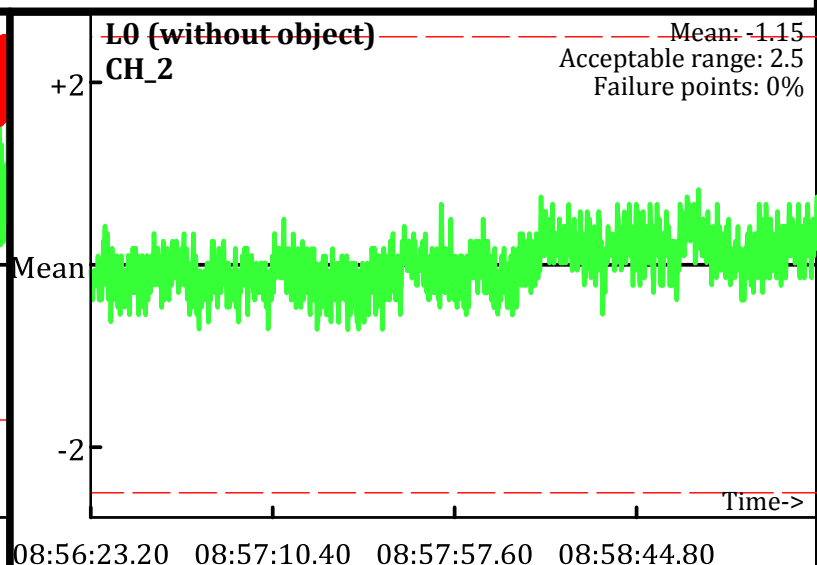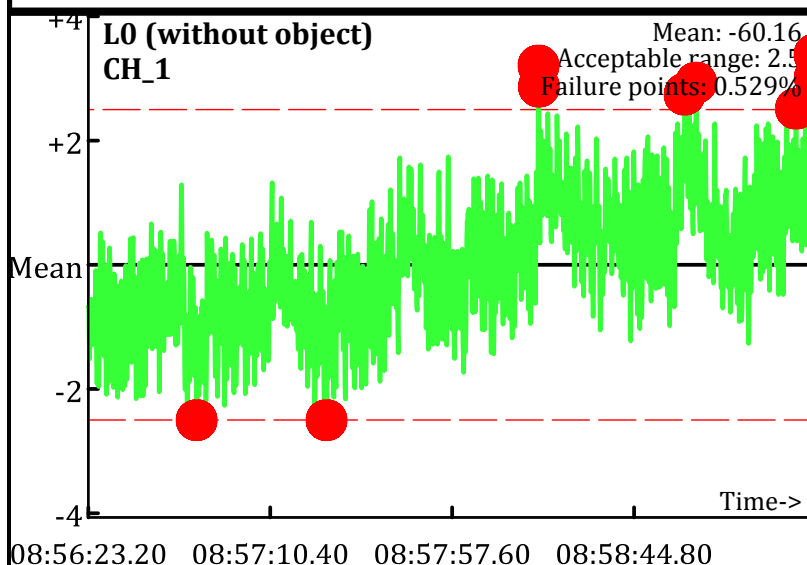-- Acceptable limits

AM test
Operator: PN & BR
Date: 12/29/2009

L0 (without object)
CH_3
Mean: 3.74
Acceptable range: 2.5
Failure points: 0%

08:56:23.20   08:57:10.40   08:57:57.60   08:58:44.80

L0 (without object)
CH_4
Mean: -2.29
Acceptable range: 2.5
Failure points: 0%

08:56:23.20   08:57:10.40   08:57:57.60   08:58:44.80

L1 (with object)
CH_3
Mean: 34.13
Acceptable range: 2.5
Failure points: 0%

09:01:27.91   09:02:18.11   09:03:08.30   09:03:58.50

L1 (with object)
CH_4
Mean: 10.98
Acceptable range: 2.5
Failure points: 0%

09:01:27.91   09:02:18.11   09:03:08.30   09:03:58.50

L2 (without object)
CH_3
Mean: 3.99
Acceptable range: 2.5
Failure points: 0%

09:06:23.61   09:06:39.33   09:06:55.05   09:07:10.78

L2 (without object)
CH_4
Mean: -2.22
Acceptable range: 2.5
Failure points: 0%

09:06:23.61   09:06:39.33   09:06:55.05   09:07:10.78

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
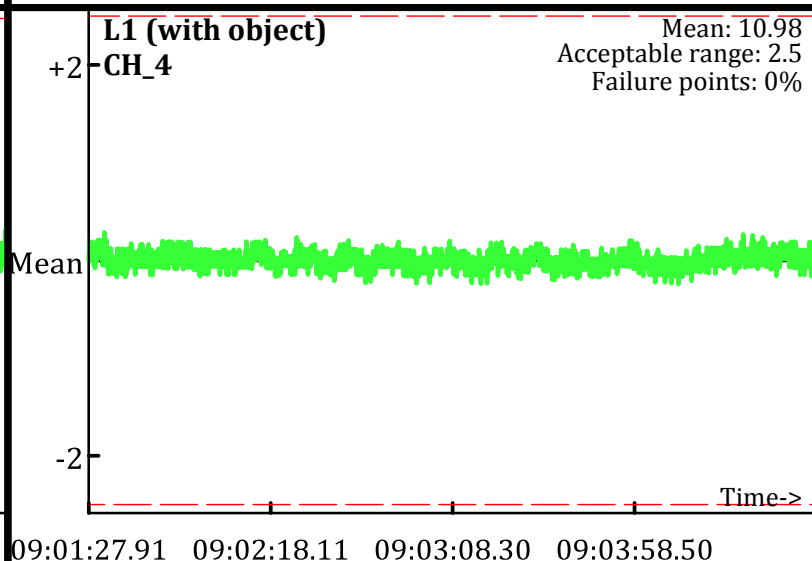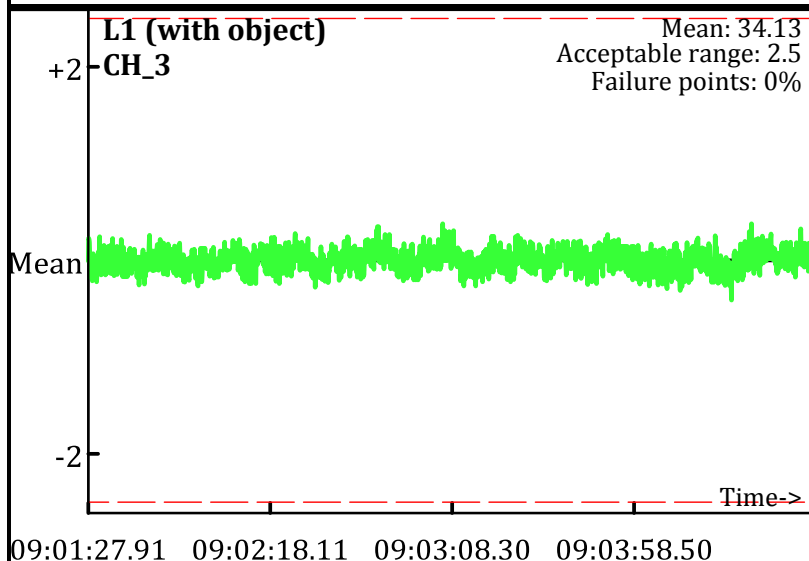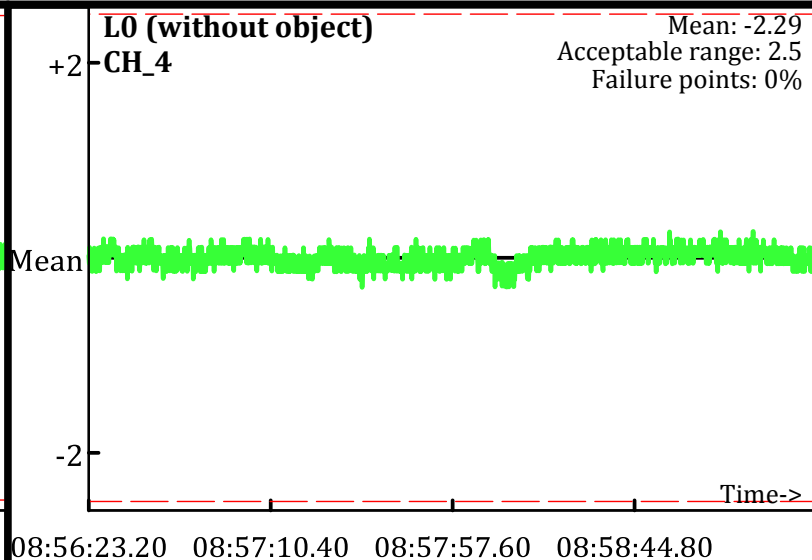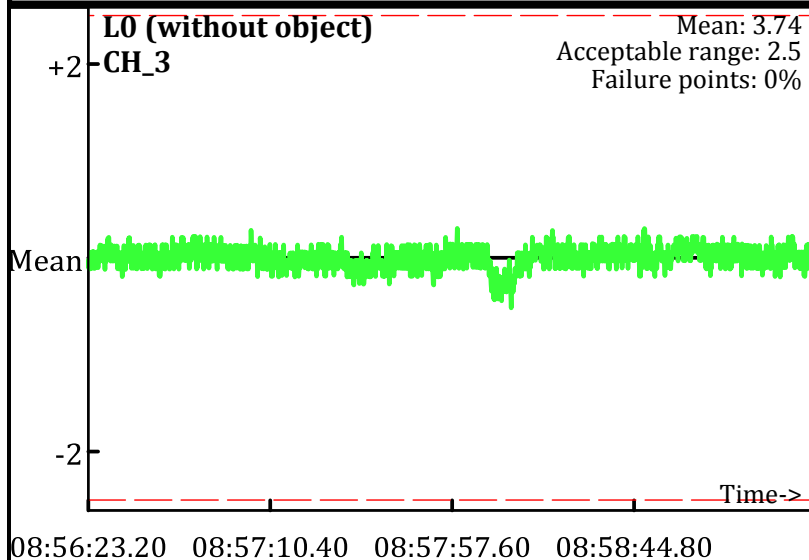Grid/Location: QC Area

⬤ Outside range
--- Acceptable limits

AM test
Operator: PN & BR
Date: 12/29/2009

L0.1 (without object)
CH_1
Mean: -121.48
Acceptable range: 2.5
Failure points: 1.43%

L0.1 (without object)
CH_2
Mean: -6.27
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_1
Mean: -3.17
Acceptable range: 2.5
Failure points: 3.44%

L1.1 (with object)
CH_2
Mean: 81.41
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_1
Mean: -114.75
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_2
Mean: -4.06
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

L0.1 (without object)
CH_3
Mean: 8.87
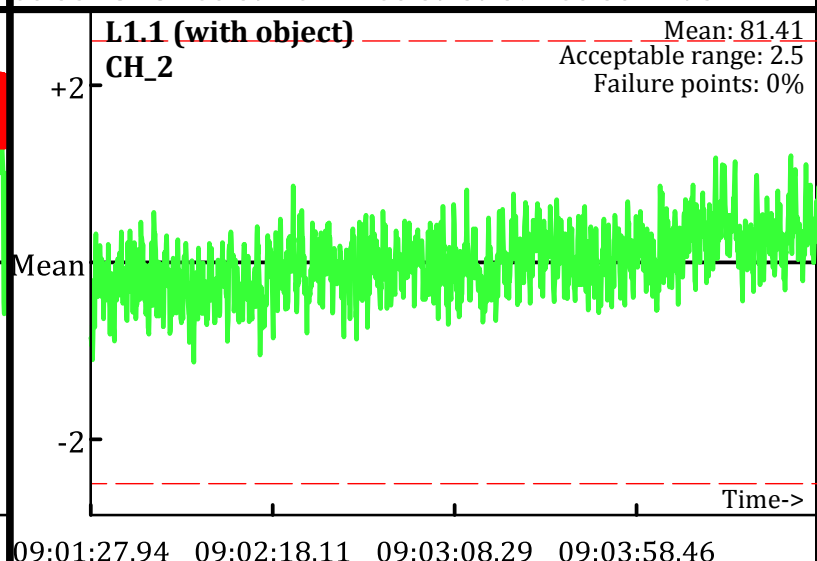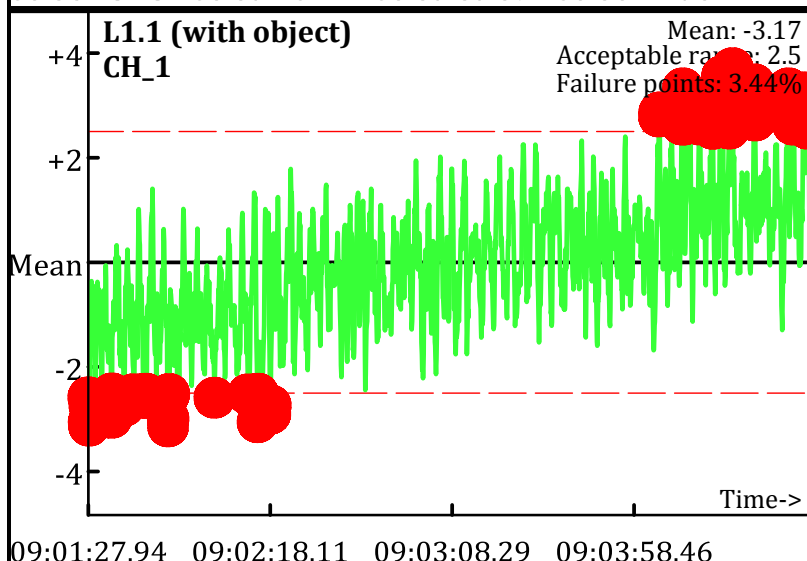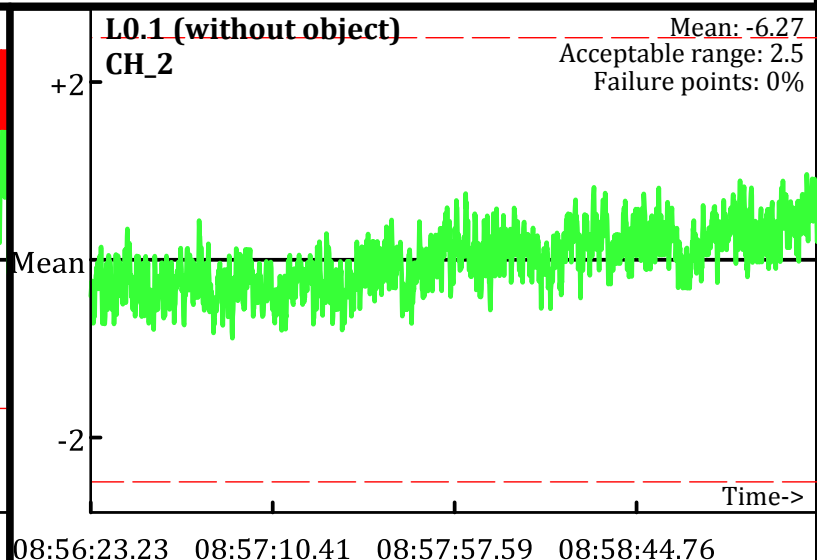Acceptable range: 2.5
Failure points: 0%

L0.1 (without object)
CH_4
Mean: 1.58
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_3
Mean: 64.66
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_4
Mean: 31.48
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_3
Mean: 9.35
Acceptable range: 2.5
Failure points: 0%

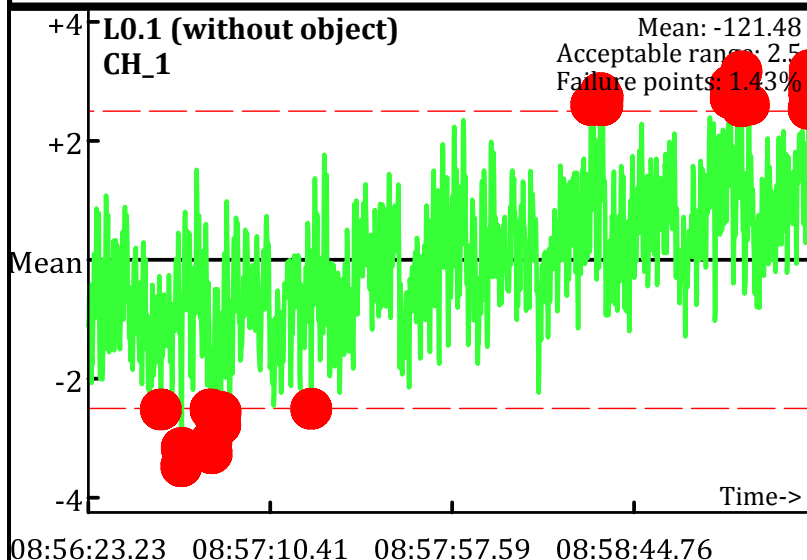L2.1 (without object)
CH_4
Mean: 1.59
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - Develpment Areas
Equipment: EM-61 Mark II
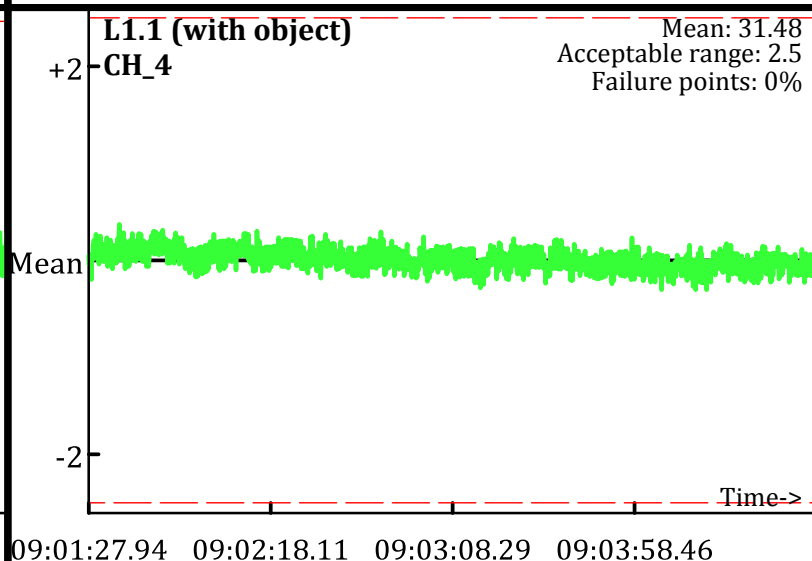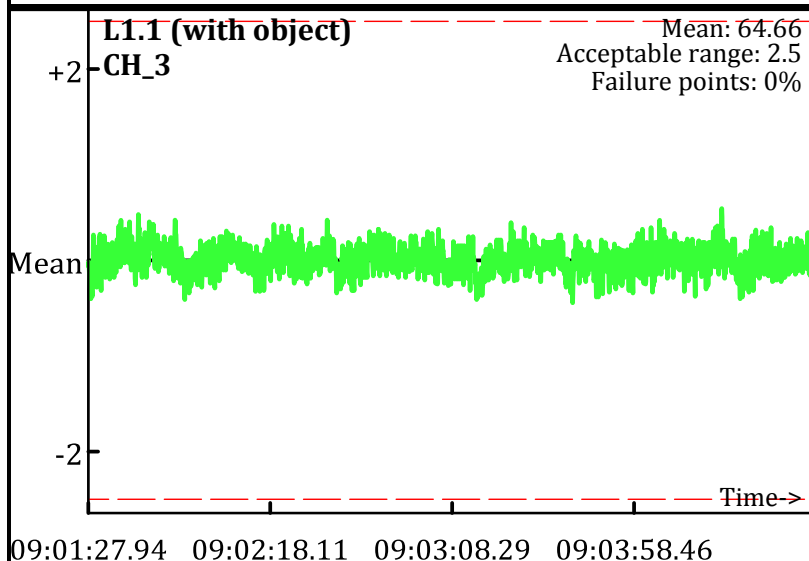Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & BR
Date: 12/29/2009

L0.2 (without object)
CH_1
Mean: -79.03
Acceptable range: 2.5
Failure points: 0%

08:56:23.25   08:57:10.43   08:57:57.61   08:58:44.79

L0.2 (without object)
CH_2
Mean: 0.96
Acceptable range: 2.5
Failure points: 0%

08:56:23.25   08:57:10.43   08:57:57.61   08:58:44.79

L1.2 (with object)
CH_1
Mean: 13.69
Acceptable range: 2.5
Failure points: 0%

09:01:27.95   09:02:18.13   09:03:08.30   09:03:58.48

L1.2 (with object)
CH_2
Mean: 57.27
Acceptable range: 2.5
Failure points: 0%

09:01:27.95   09:02:18.13   09:03:08.30   09:03:58.48

L2.2 (without object)
CH_1
Mean: -76.93
Acceptable range: 2.5
Failure points: 0%

09:06:23.66   09:06:39.38   09:06:55.10   09:07:10.82   09:07

L2.2 (without object)
CH_2
Mean: 1.24
Acceptable range: 2.5
Failure points: 0%

09:06:23.66   09:06:39.38   09:06:55.10   09:07:10.82   09:07

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
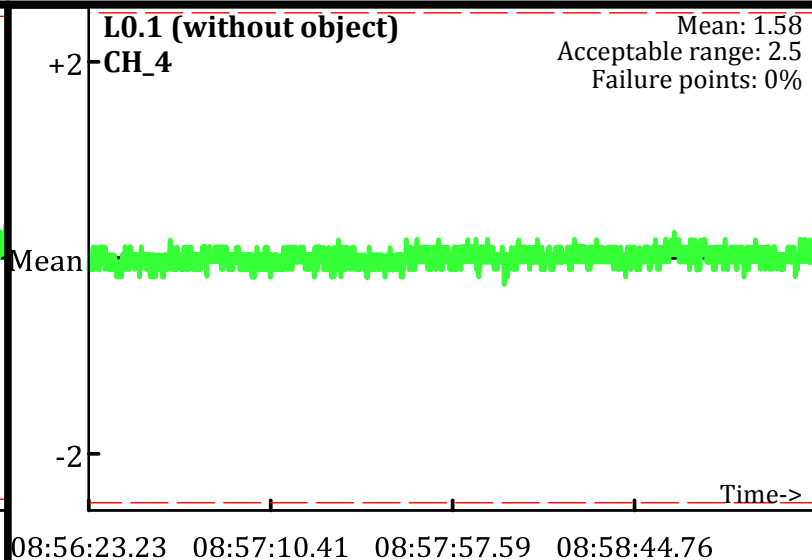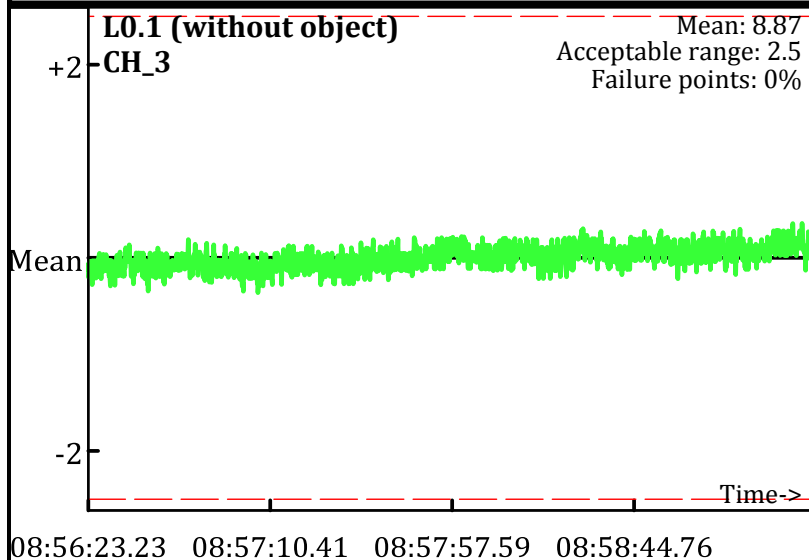Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

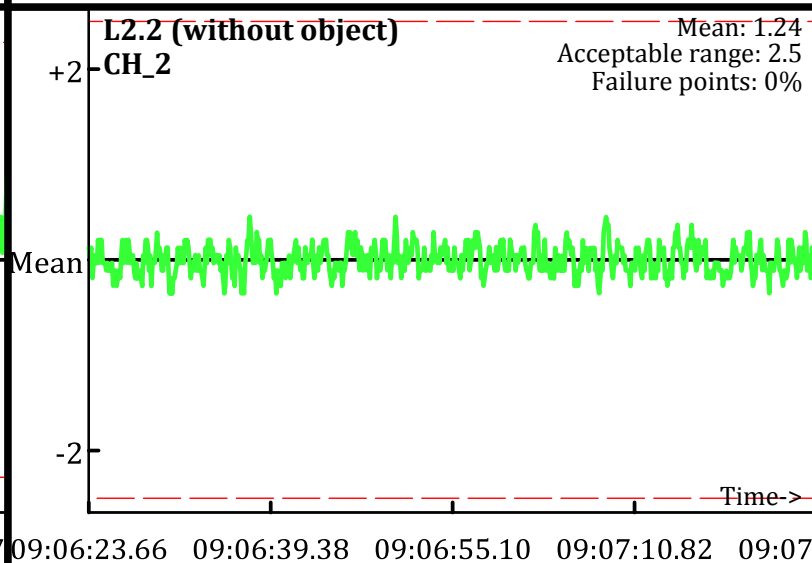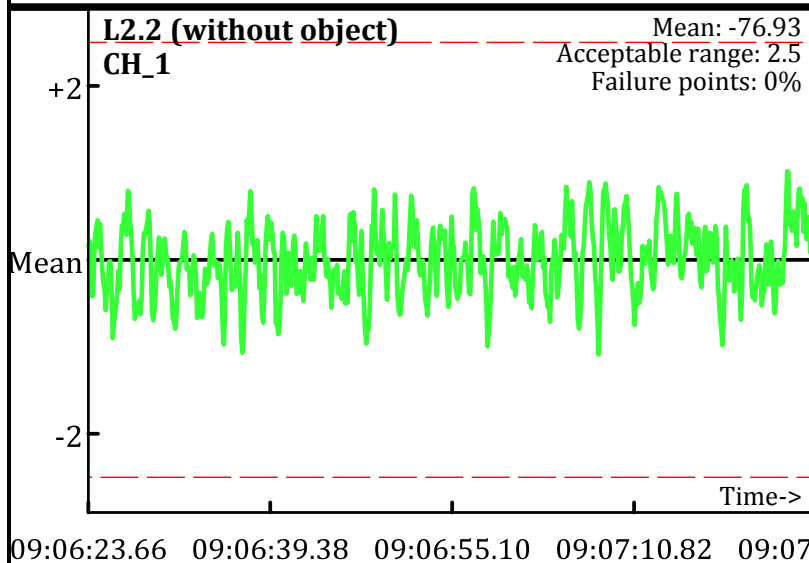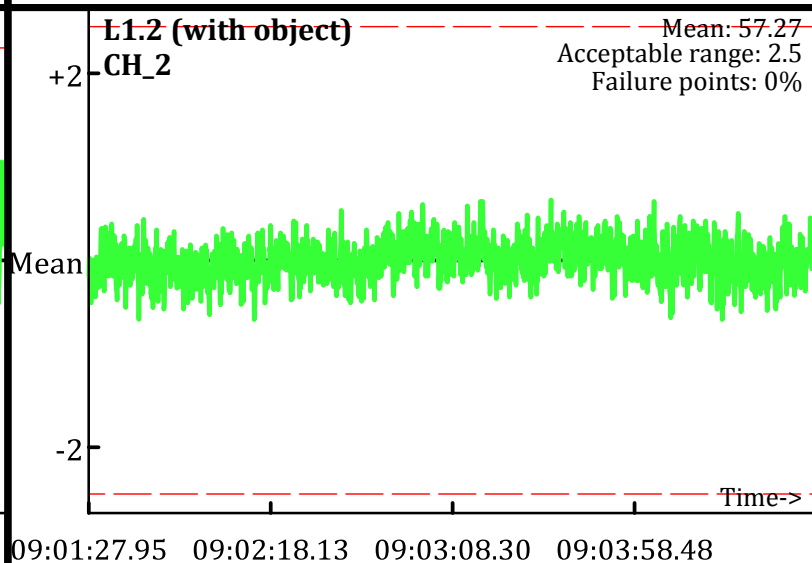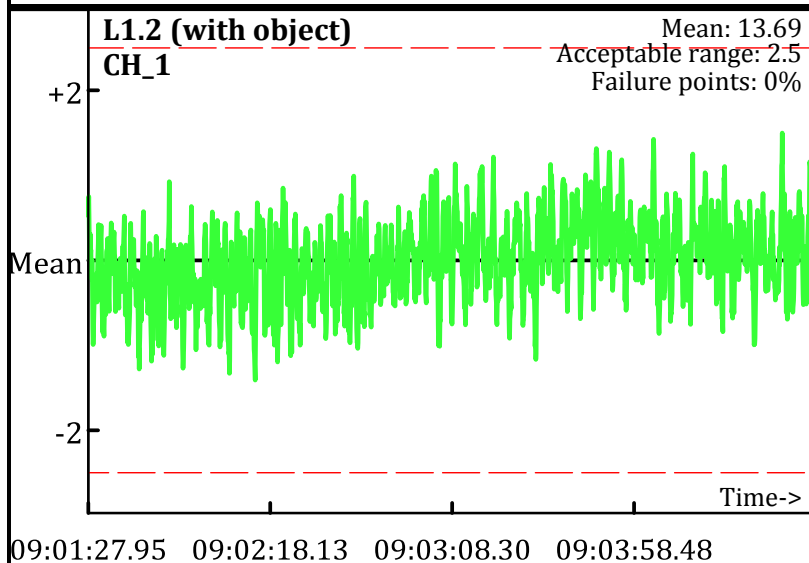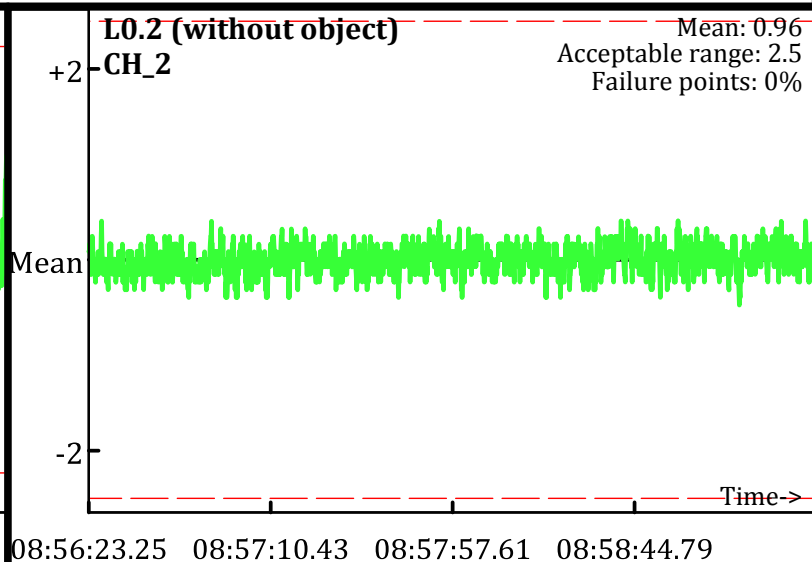AM test
Operator: PN & BR
Date: 12/29/2009

L0.2 (without object)
CH_3
+2
Mean
-2
Time->
Mean: 5.9
Acceptable range: 2.5
Failure points: 0%

08:56:23.25   08:57:10.43   08:57:57.61   08:58:44.79

L0.2 (without object)
CH_4
+2
Mean
-2
Time->
Mean: -0.73
Acceptable range: 2.5
Failure points: 0%

08:56:23.25   08:57:10.43   08:57:57.61   08:58:44.79

L1.2 (with object)
CH_3
+2
Mean
-2
Time->
Mean: 34.71
Acceptable range: 2.5
Failure points: 0%

09:01:27.95   09:02:18.13   09:03:08.30   09:03:58.48

L1.2 (with object)
CH_4
+2
Mean
-2
Time->
Mean: 11.69
Acceptable range: 2.5
Failure points: 0%

09:01:27.95   09:02:18.13   09:03:08.30   09:03:58.48

L2.2 (without object)
CH_3
+2
Mean
-2
Time->
Mean: 5.84
Acceptable range: 2.5
Failure points: 0%

09:06:23.66   09:06:39.38   09:06:55.10   09:07:10.82   09:07

L2.2 (without object)
CH_4
+2
Mean
-2
Time->
Mean: -0.76
Acceptable range: 2.5
Failure points: 0%
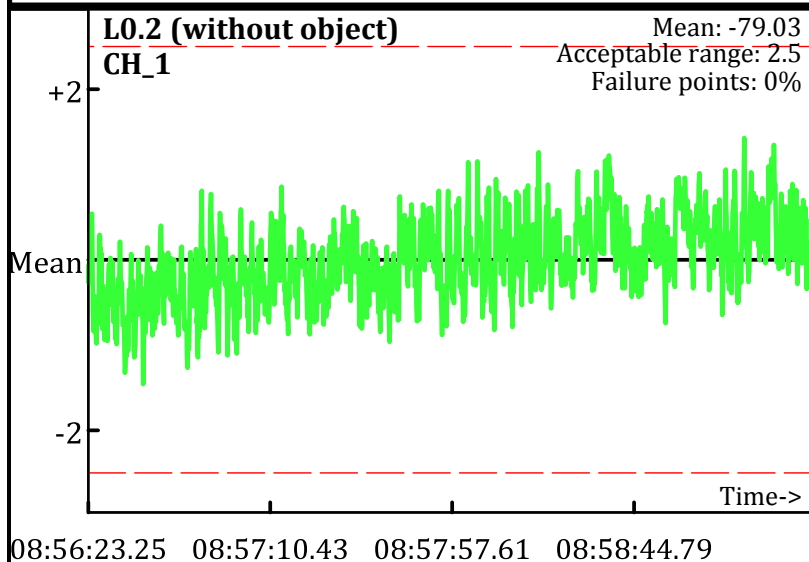
09:06:23.66   09:06:39.38   09:06:55.10   09:07:10.82   09:07

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
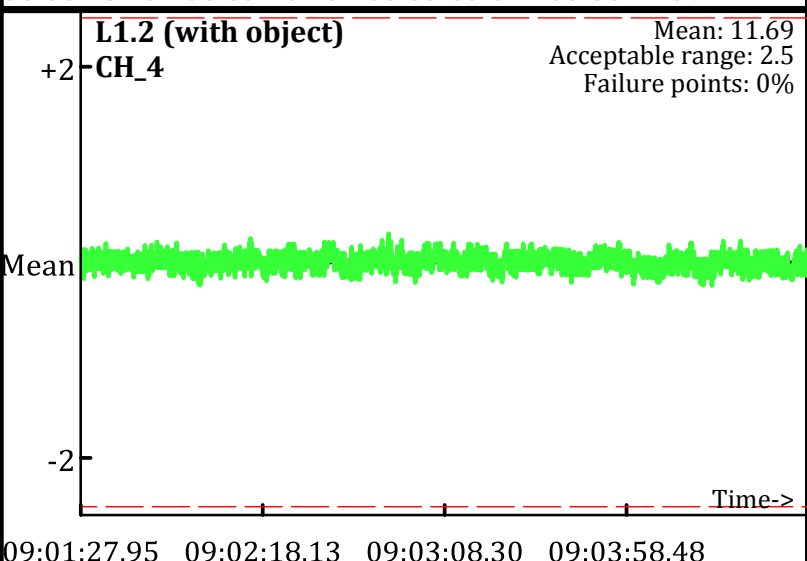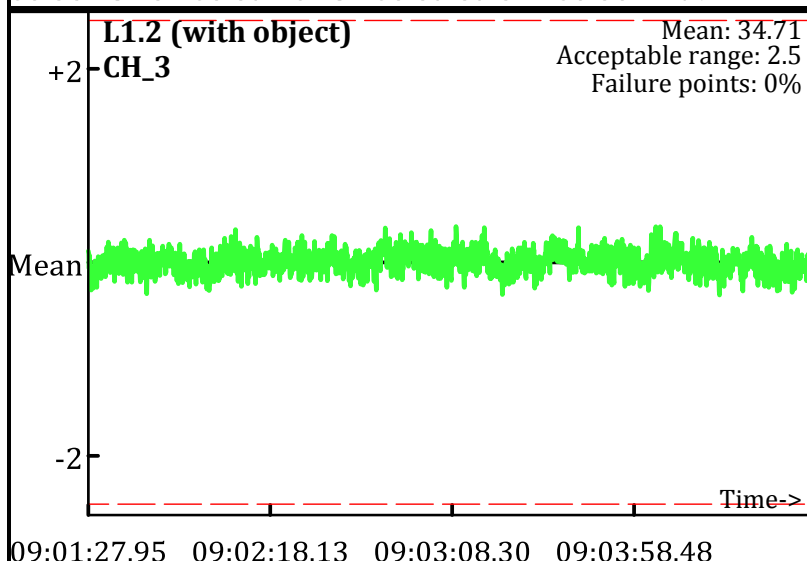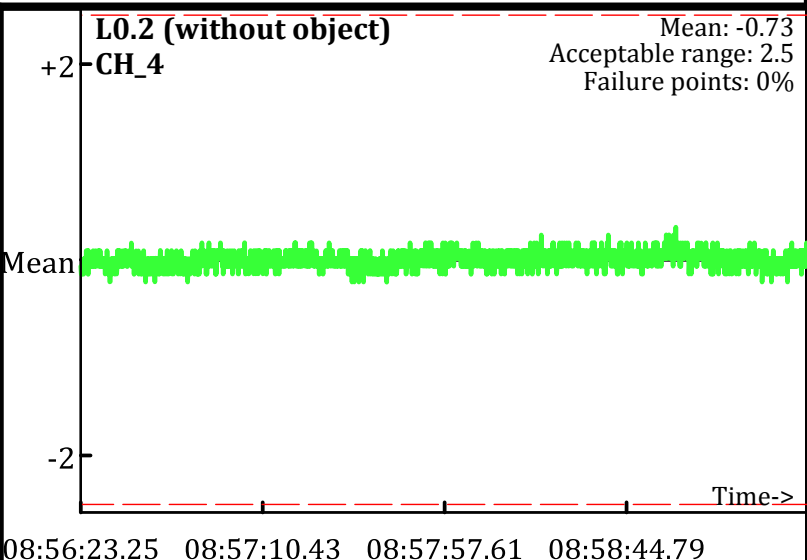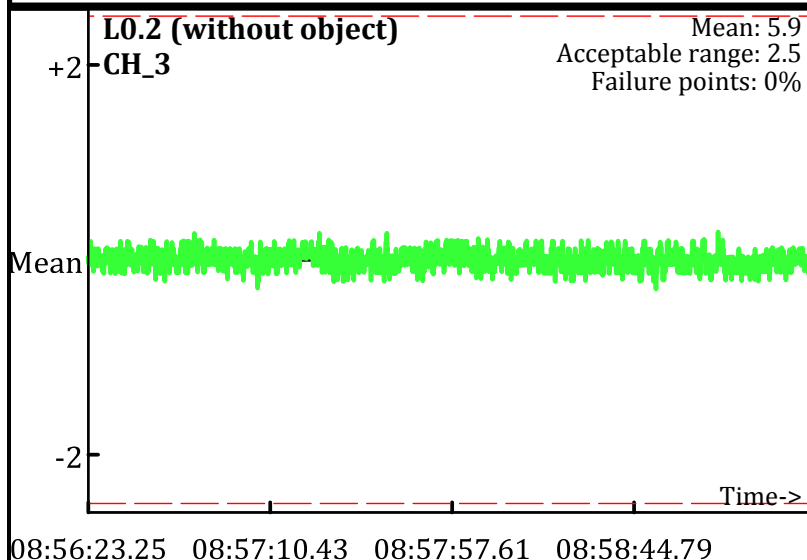Grid/Location: QC Area

● Outside range
- - - Acceptable limits

PM test
Operator: PN & BR
Date: 12/29/2009

L6 (without object)
CH_1
Mean: -58.92
Acceptable range: 2.5
Failure points: 0%

L6 (without object)
CH_2
Mean: -1.19
Acceptable range: 2.5
Failure points: 0%

16:47:25.73   16:48:12.18   16:48:58.63   16:49:45.08   16:50

16:47:25.73   16:48:12.18   16:48:58.63   16:49:45.08   16:50

L7 (with object)
CH_1
Mean: 35.12
Acceptable range: 2.5
Failure points: 0%

L7 (with object)
CH_2
Mean: 57.04
Acceptable range: 2.5
Failure points: 0%

16:52:14.53   16:53:00.71   16:53:46.88   16:54:33.06

16:52:14.53   16:53:00.71   16:53:46.88   16:54:33.06

L8 (without object)
CH_1
Mean: -59.02
Acceptable range: 2.5
Failure points: 0%

L8 (without object)
CH_2
Mean: -1.11
Acceptable range: 2.5
Failure points: 0%

16:56:05.33   16:56:27.03   16:56:48.73   16:57:10.43

16:56:05.33   16:56:27.03   16:56:48.73   16:57:10.43

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
Line Name: L6 L7 L8

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
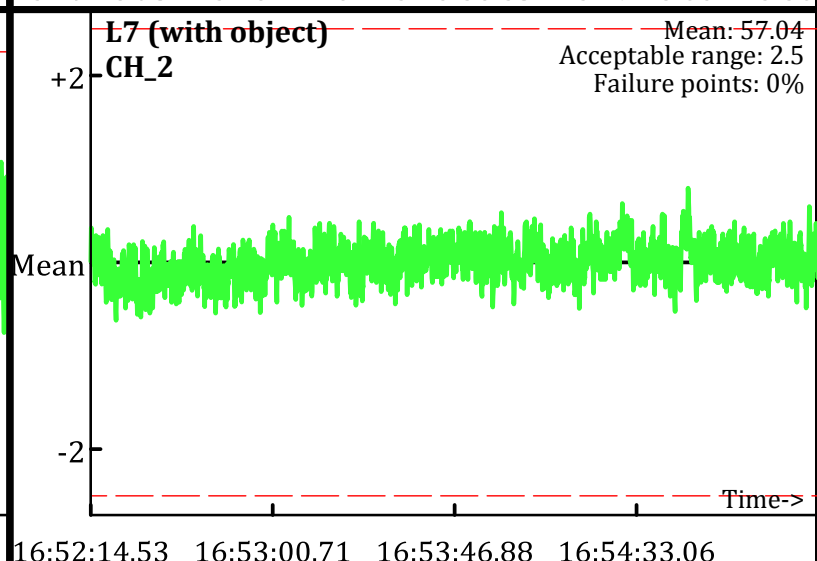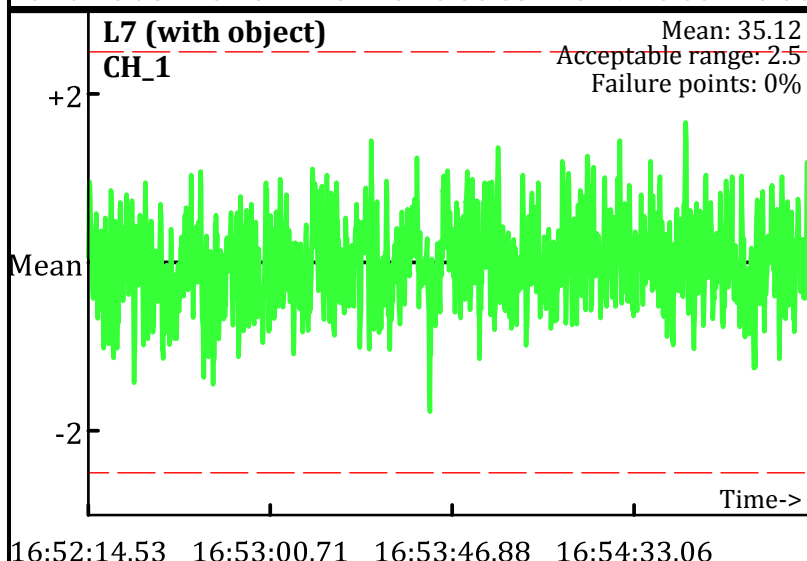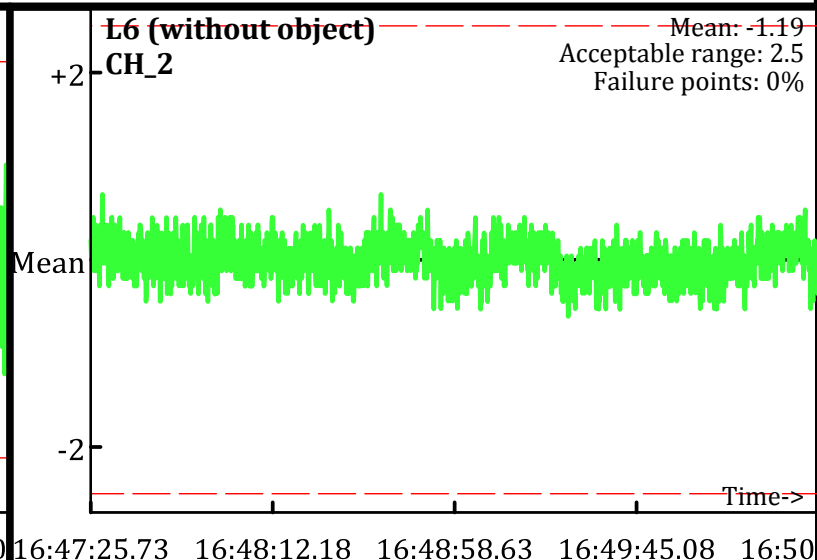Grid/Location: QC Area

● Outside range
− − − Acceptable limits

PM test
Operator: PN & BR
Date: 12/29/2009

L6 (without object) CH_3
Mean: 3.22
Acceptable range: 2.5
Failure points: 0%

L6 (without object) CH_4
Mean: -2.75
Acceptable range: 2.5
Failure points: 0%

L7 (with object) CH_3
Mean: 33.37
Acceptable range: 2.5
Failure points: 0%

L7 (with object) CH_4
Mean: 10.44
Acceptable range: 2.5
Failure points: 0%

L8 (without object) CH_3
Mean: 3.39
Acceptable range: 2.5
Failure points: 0%

L8 (without object) CH_4
Mean: -2.62
Acceptable range: 2.5
Failure points: 0%

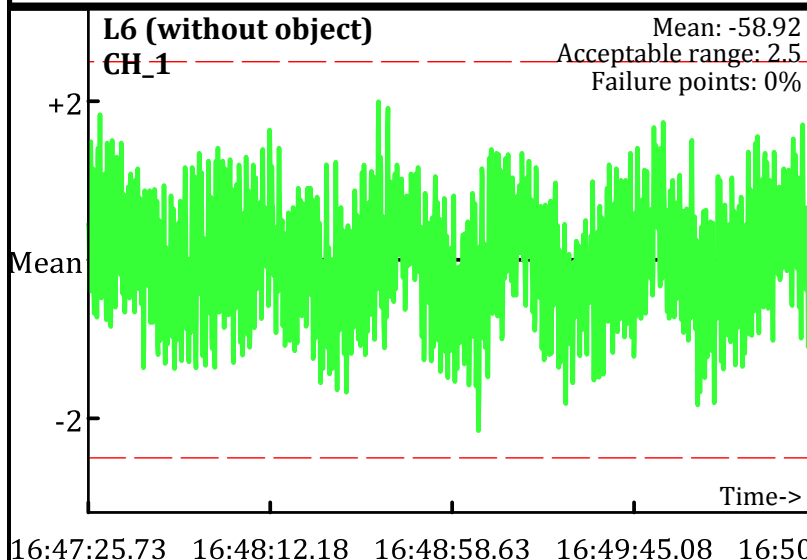# Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
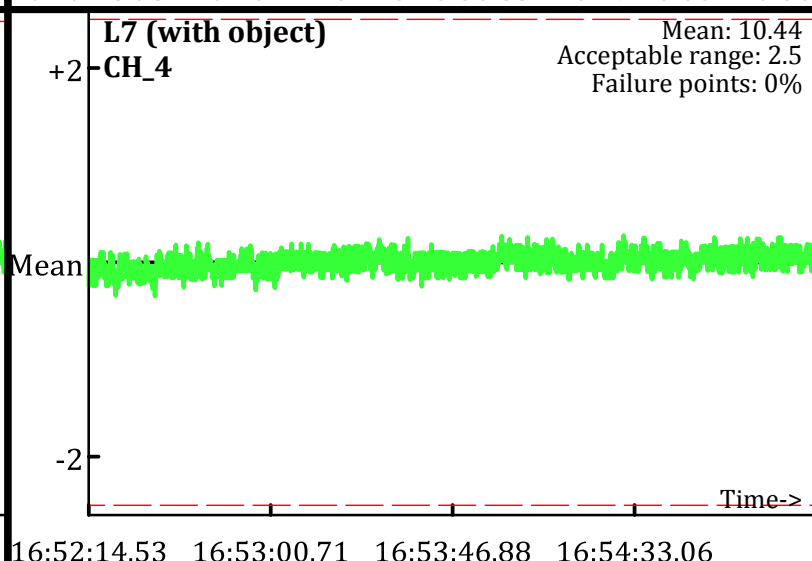Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & BR
Date: 12/29/2009

L6.1 (without object)
CH_1
Mean: -89.14
Acceptable range: 2.5
Failure points: 0%

L6.1 (without object)
CH_2
Mean: 3.86
Acceptable range: 2.5
Failure points: 0%

16:47:25.75   16:48:12.18   16:48:58.60   16:49:45.03

L7.1 (with object)
CH_1
Mean: 26.22
Acceptable range: 2.5
Failure points: 0.0541%

L7.1 (with object)
CH_2
Mean: 91
Acceptable range: 2.5
Failure points: 0%

16:52:14.45   16:53:00.66   16:53:46.86   16:54:33.06   16:55

L8.1 (without object)
CH_1
Mean: -89.38
Acceptable range: 2.5
Failure points: 0%

L8.1 (without object)
CH_2
Mean: 3.8
Acceptable range: 2.5
Failure points: 0%

16:56:05.36   16:56:27.06   16:56:48.76   16:57:10.46

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
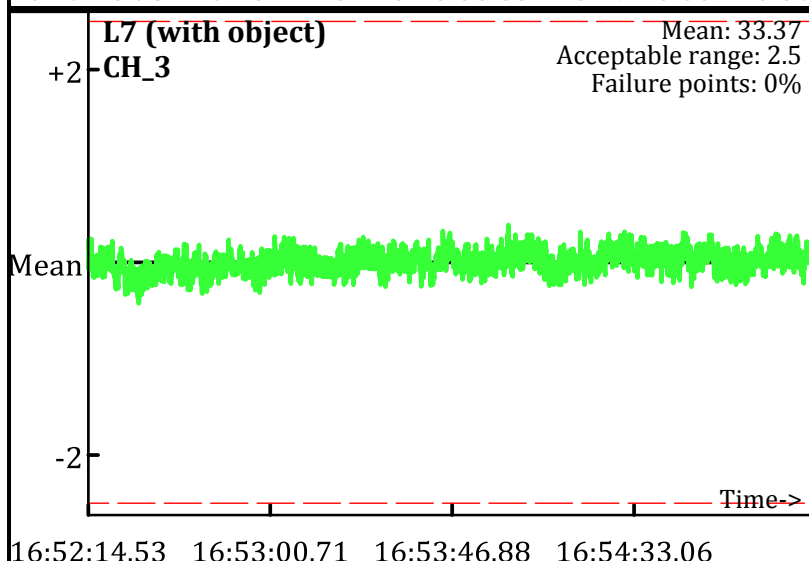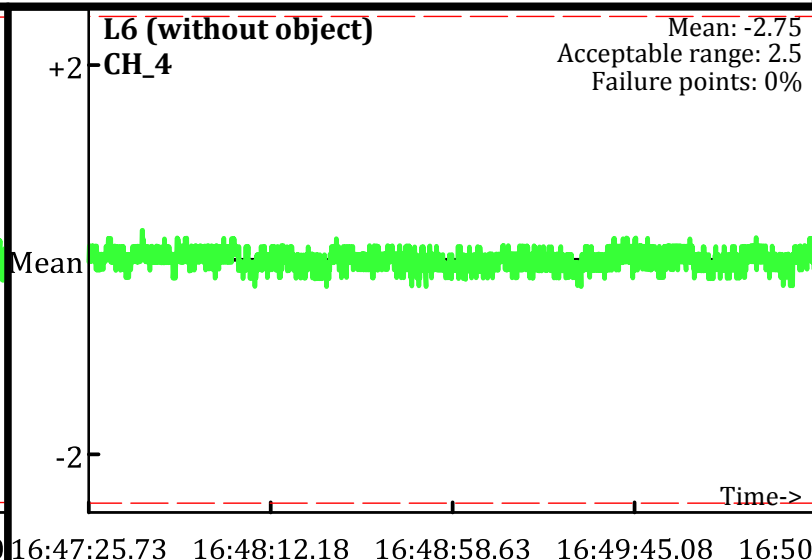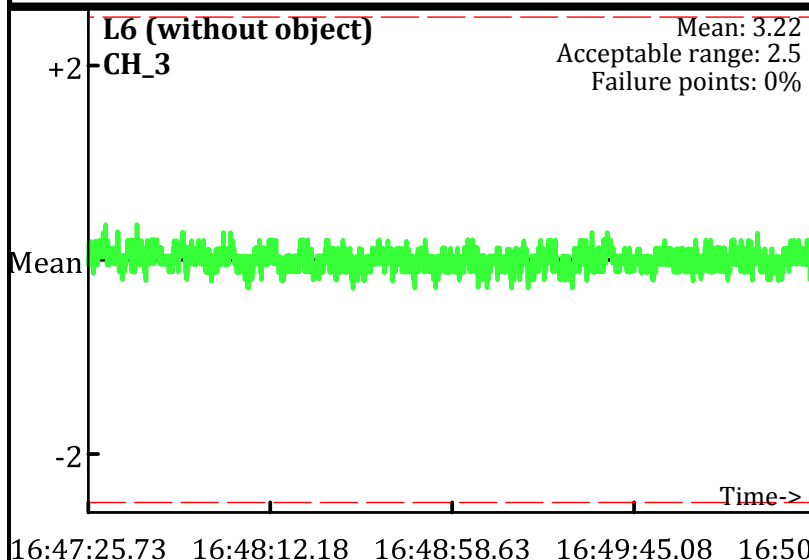Line Name: L6.1 L7.1 L8.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits

PM test
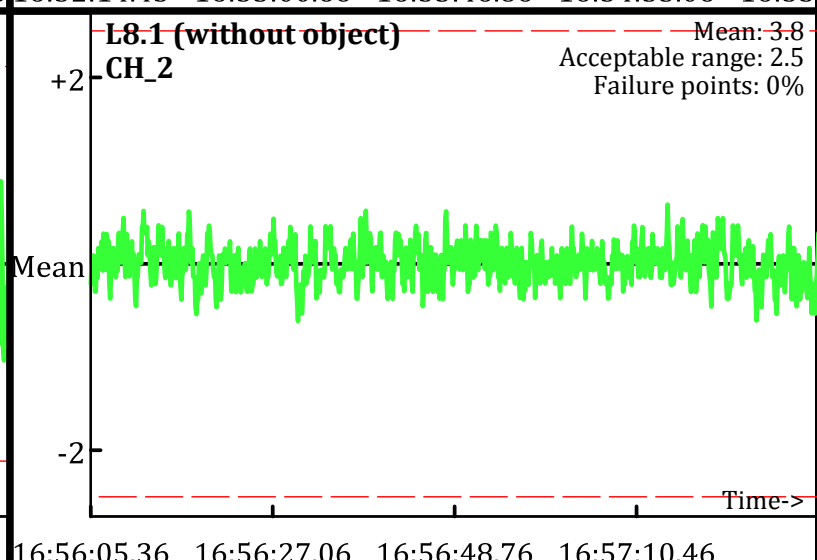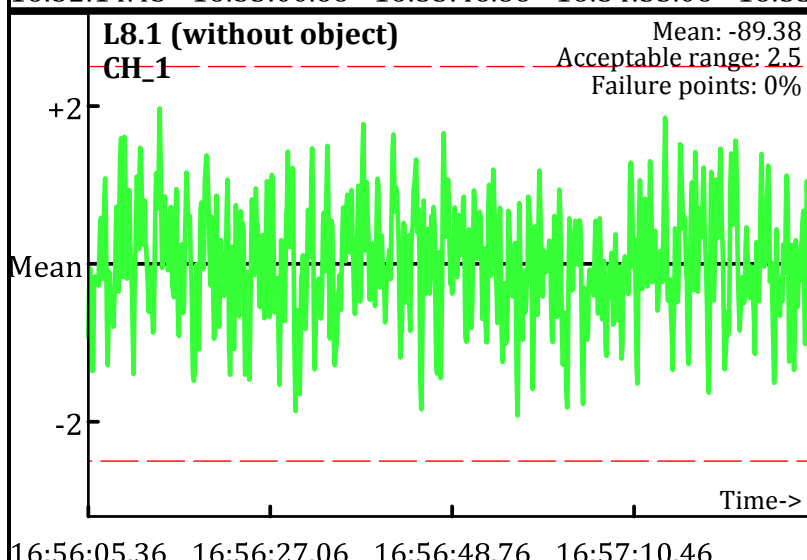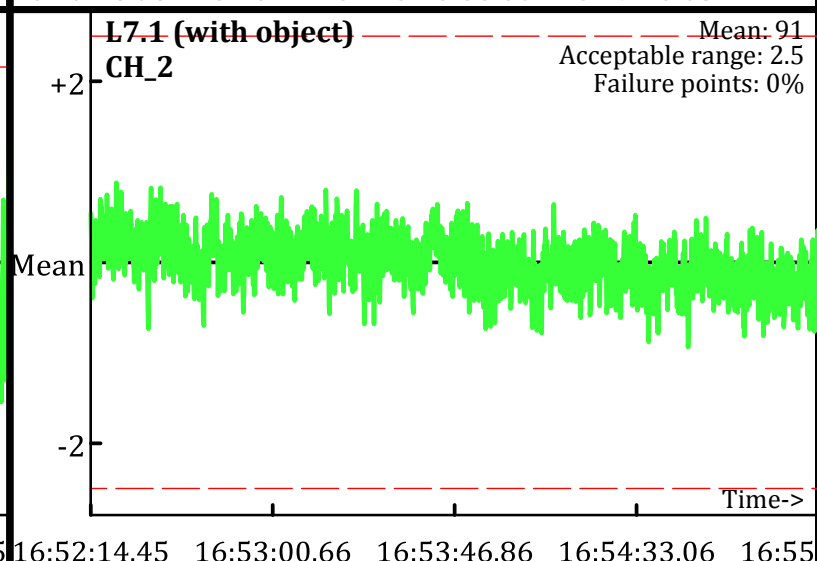Operator: PN & BR
Date: 12/29/2009

L6.1 (without object)
CH_3
Mean: 11.01
Acceptable range: 2.5
Failure points: 0%

L6.1 (without object)
CH_4
Mean: 1.87
Acceptable range: 2.5
Failure points: 0%

L7.1 (with object)
CH_3
Mean: 66.97
Acceptable range: 2.5
Failure points: 0%

L7.1 (with object)
CH_4
Mean: 31.94
Acceptable range: 2.5
Failure points: 0%

L8.1 (without object)
CH_3
Mean: 11.04
Acceptable range: 2.5
Failure points: 0%

L8.1 (without object)
CH_4
Mean: 1.87
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
Line Name: L6.1 L7.1 L8.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
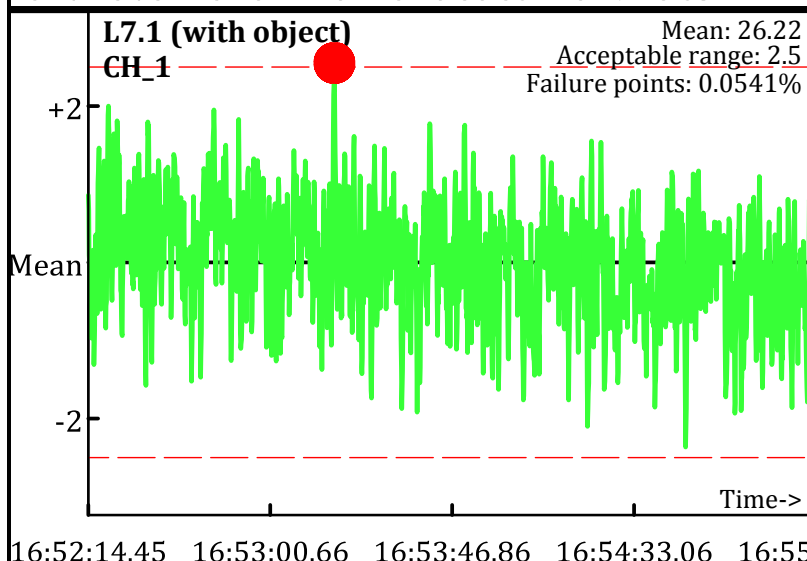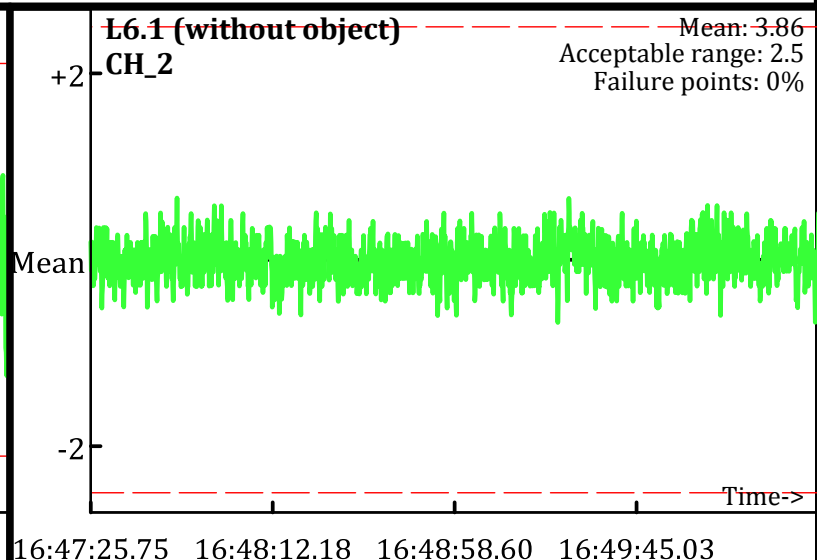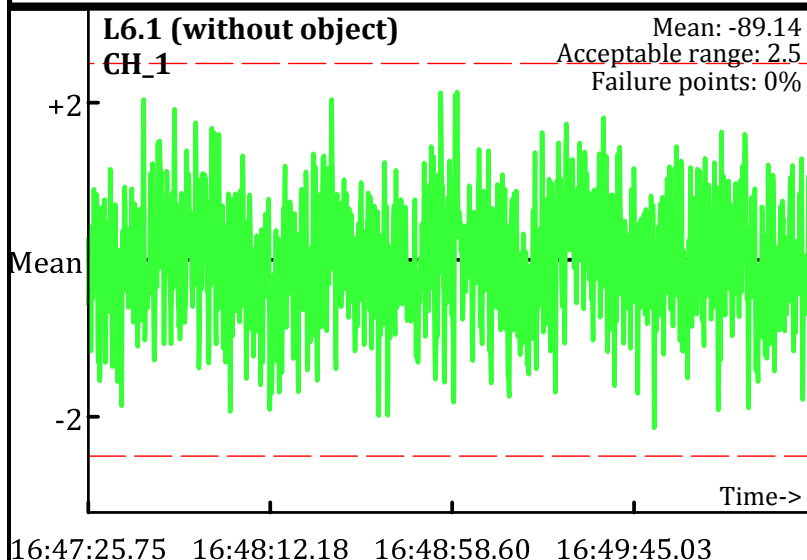-- Acceptable limits

PM test
Operator: PN & BR
Date: 12/29/2009

L6.2 (without object)
CH_1
Mean: -59.63
Acceptable range: 2.5
Failure points: 0%

16:47:25.78   16:48:12.21   16:48:58.63   16:49:45.06

L6.2 (without object)
CH_2
Mean: 6.96
Acceptable range: 2.5
Failure points: 0%

16:47:25.78   16:48:12.21   16:48:58.63   16:49:45.06

L7.2 (with object)
CH_1
Mean: 30.47
Acceptable range: 2.5
Failure points: 0%

16:52:14.48   16:53:00.68   16:53:46.88   16:54:33.08

L7.2 (with object)
CH_2
Mean: 62.5
Acceptable range: 2.5
Failure points: 0%

16:52:14.48   16:53:00.68   16:53:46.88   16:54:33.08

L8.2 (without object)
CH_1
Mean: -60.23
Acceptable range: 2.5
Failure points: 0%

16:56:05.28   16:56:26.98   16:56:48.68   16:57:10.38

L8.2 (without object)
CH_2
Mean: 6.73
Acceptable range: 2.5
Failure points: 0%

16:56:05.28   16:56:26.98   16:56:48.68   16:57:10.38

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
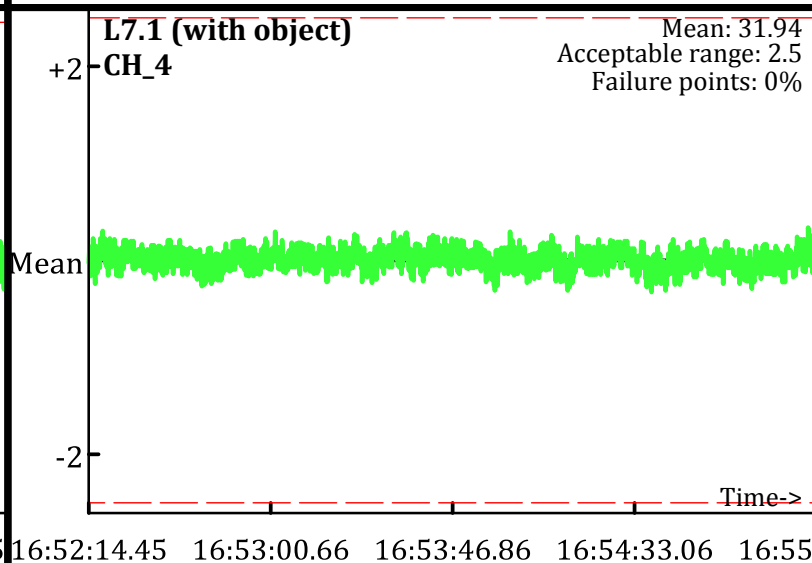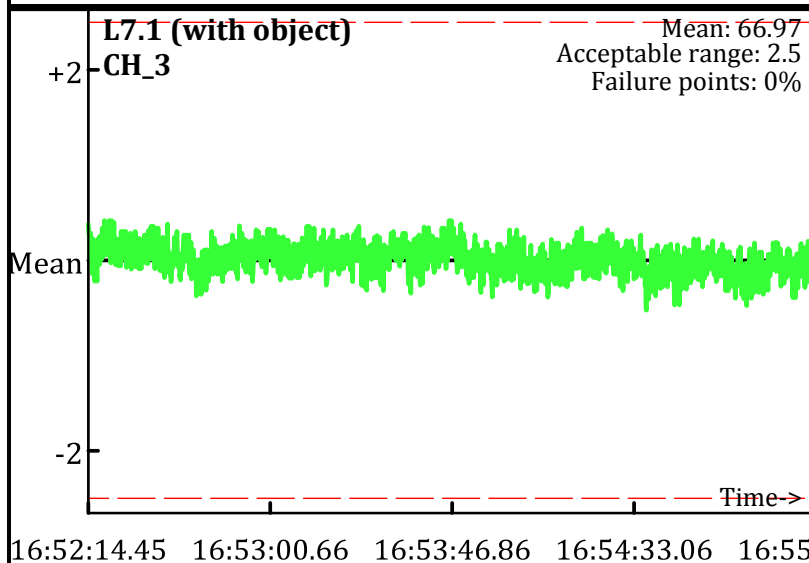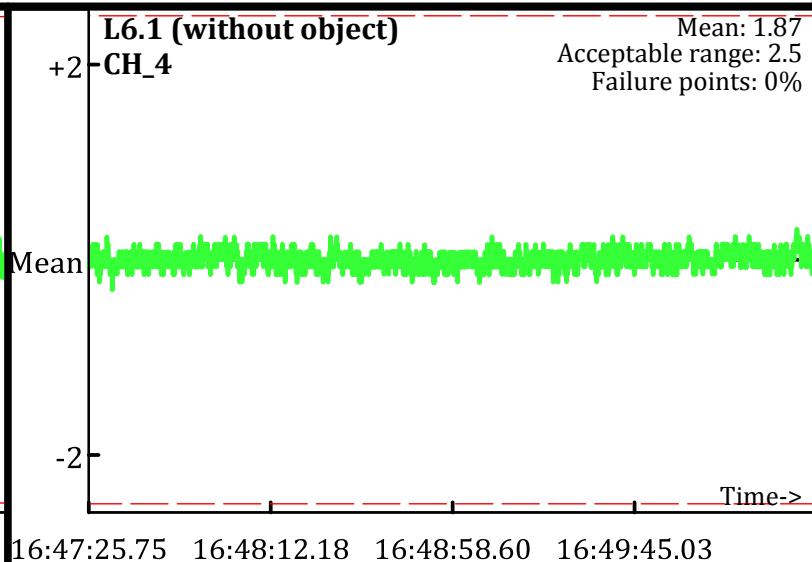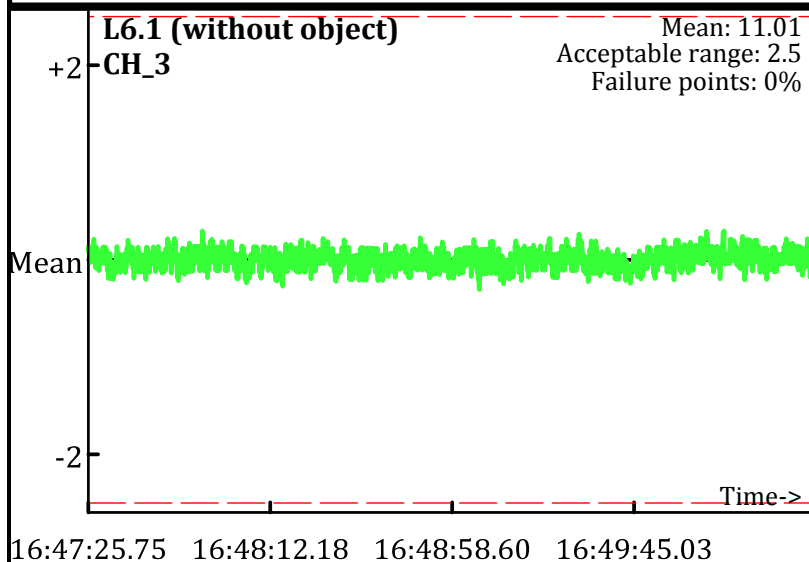Line Name: L6.2 L7.2 L8.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - Develpoment Areas
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

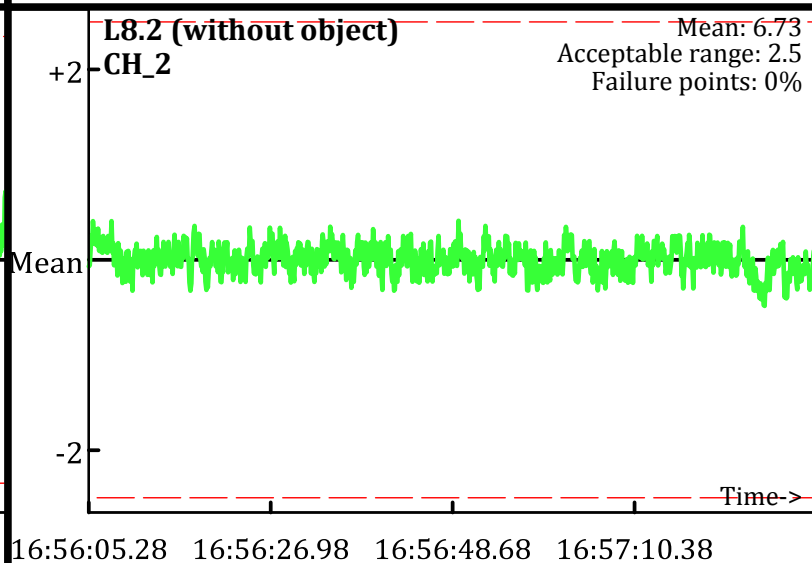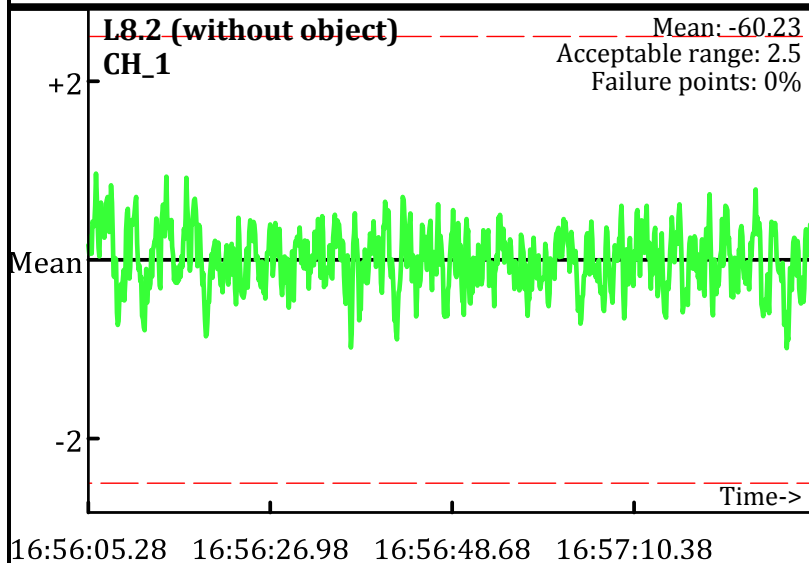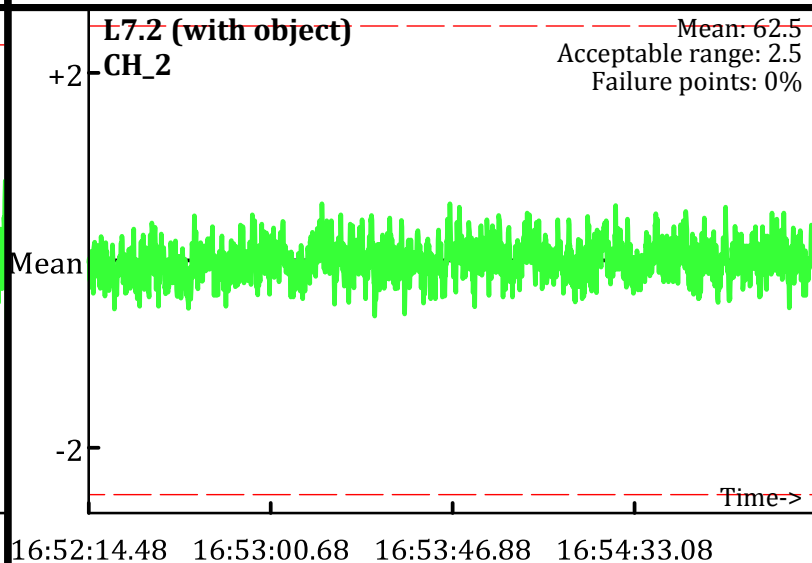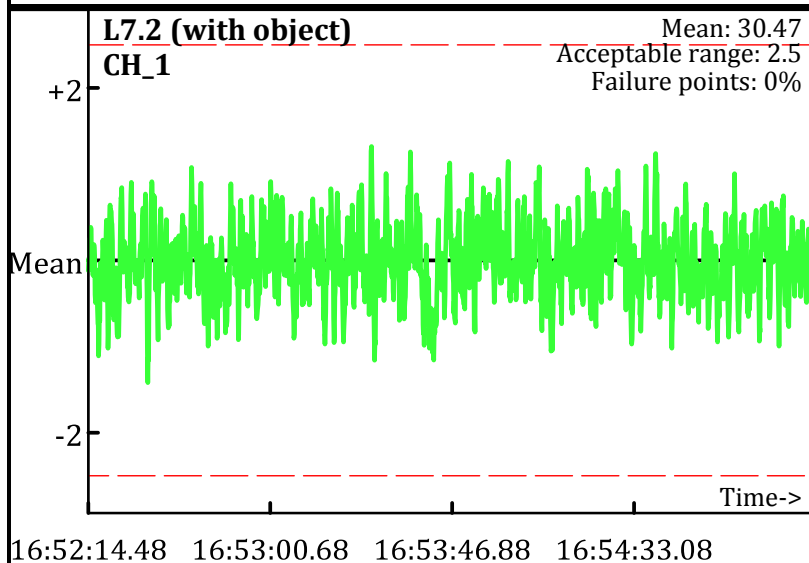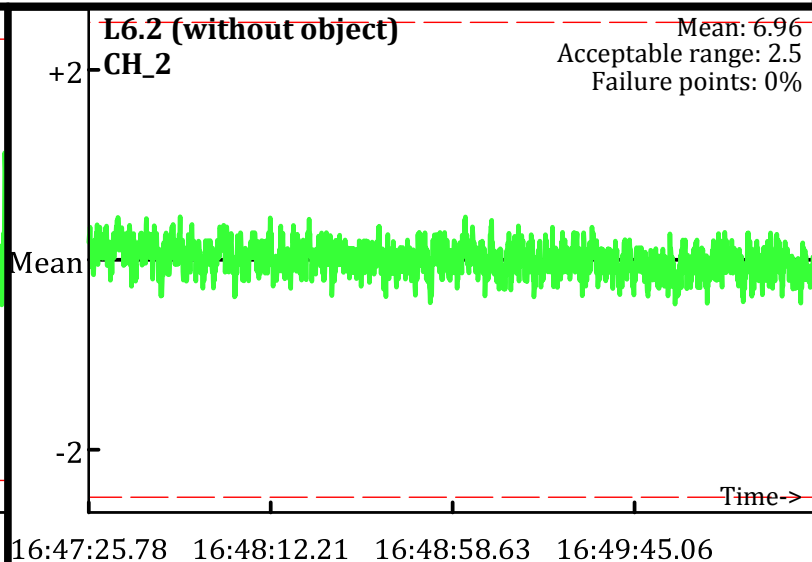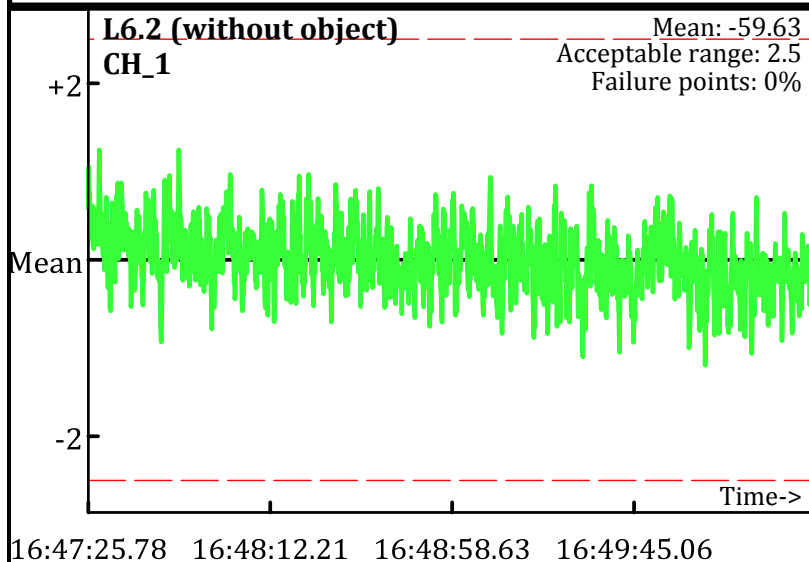PM test
Operator: PN & BR
Date: 12/29/2009

L6.2 (without object)
CH_3
Mean: 7.59
Acceptable range: 2.5
Failure points: 0%

L6.2 (without object)
CH_4
Mean: -0.18
Acceptable range: 2.5
Failure points: 0%

16:47:25.78   16:48:12.21   16:48:58.63   16:49:45.06
16:47:25.78   16:48:12.21   16:48:58.63   16:49:45.06

L7.2 (with object)
CH_3
Mean: 36.16
Acceptable range: 2.5
Failure points: 0%

L7.2 (with object)
CH_4
Mean: 12.17
Acceptable range: 2.5
Failure points: 0%

16:52:14.48   16:53:00.68   16:53:46.88   16:54:33.08
16:52:14.48   16:53:00.68   16:53:46.88   16:54:33.08

L8.2 (without object)
CH_3
Mean: 7.53
Acceptable range: 2.5
Failure points: 0%

L8.2 (without object)
CH_4
Mean: -0.23
Acceptable range: 2.5
Failure points: 0%

16:56:05.28   16:56:26.98   16:56:48.68   16:57:10.38
16:56:05.28   16:56:26.98   16:56:48.68   16:57:10.38

Database: D:\Projects_QCReports_Ord_Data\122909\QC\122909_TA_QC.gdb
Line Name: L6.2 L7.2 L8.2

Page: 2

Static Calibration Test

Data collected using the single unit EM61 cart. Therefore this series will only have 2 pages for AM & 2 pages for PM

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
Operator: PN
Date: 12/30/2009

L0 (without object)
CH1
Mean: -1.88
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:12:33.00   17:13:18.71   17:14:04.41   17:14:50.12

L0 (without object)
CH2
Mean: -0.8
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:12:33.00   17:13:18.71   17:14:04.41   17:14:50.12

L1 (with object)
CH1
Mean: 82.59
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:16:30.02   17:17:16.51   17:18:03.00   17:18:49.48

L1 (with object)
CH2
Mean: 51.38
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:16:30.02   17:17:16.51   17:18:03.00   17:18:49.48

L2 (without object)
CH1
Mean: -1.5
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:19:55.98   17:20:12.19   17:20:28.40   17:20:44.61

L2 (without object)
CH2
Mean: -0.68
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

17:19:55.98   17:20:12.19   17:20:28.40   17:20:44.61

Database: D:\Projects_QCReports_Ord_Data\123009\123009AM.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Data collected using the single unit EM61 cart. Therefore this series will only have 2 pages for AM & 2 pages for PM

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
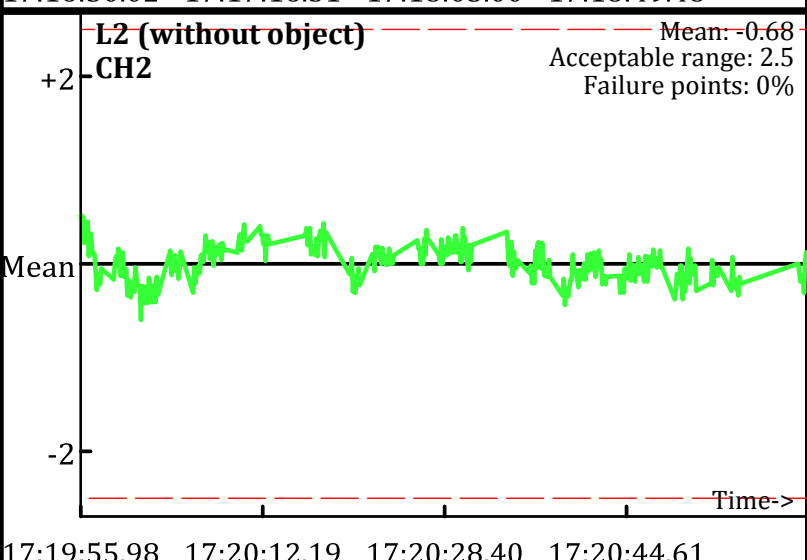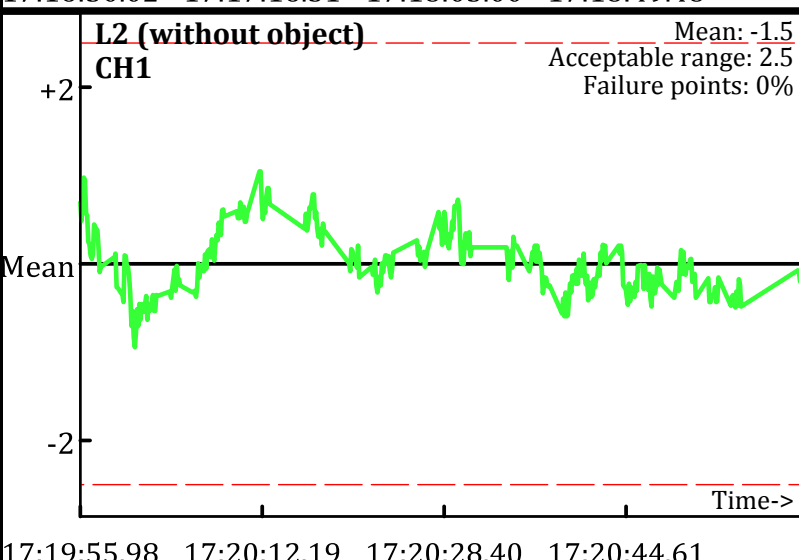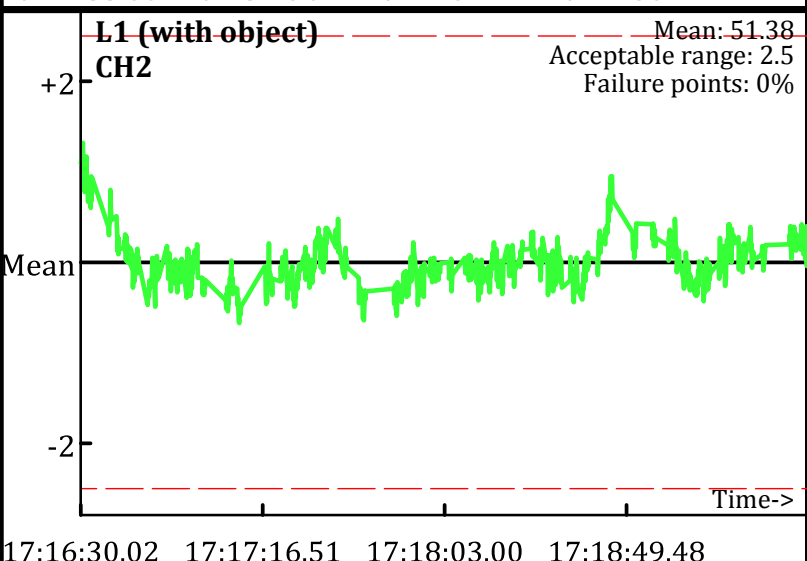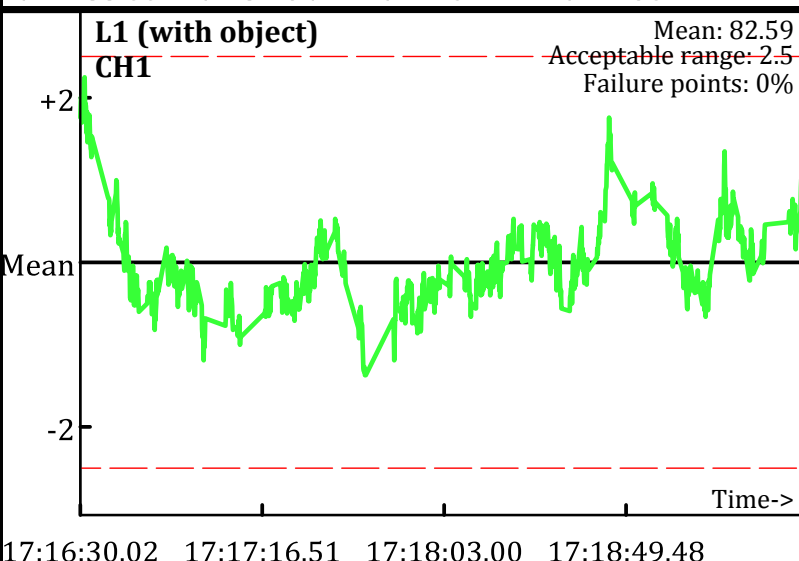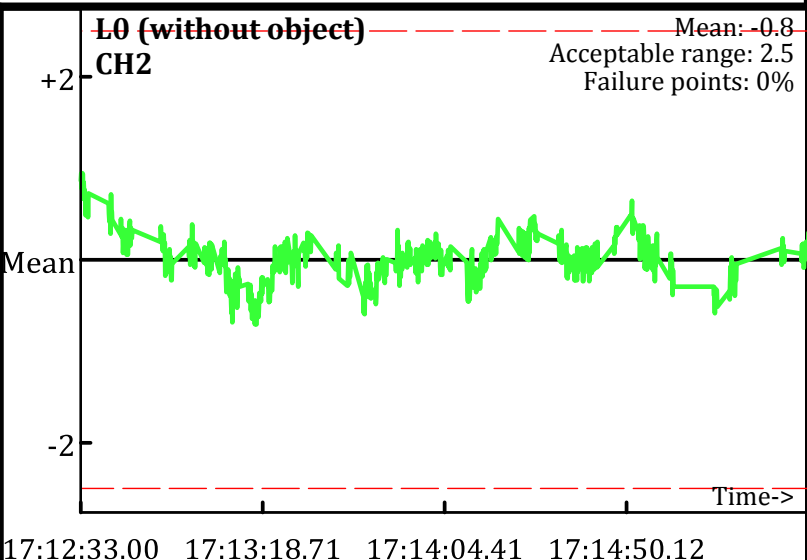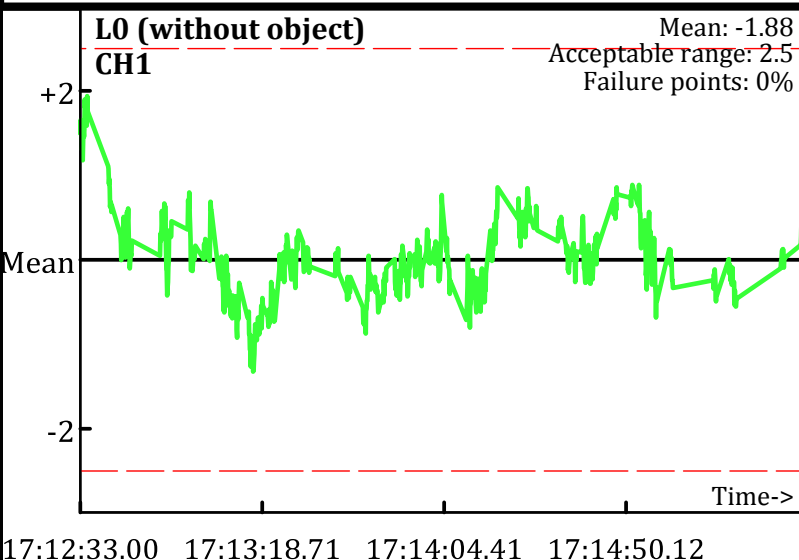– – – Acceptable limits

AM test
Operator: PN
Date: 12/30/2009

L0 (without object) CH3
Mean: -0.23
Acceptable range: 2.5
Failure points: 0%

17:12:33.00   17:13:18.71   17:14:04.41   17:14:50.12

L0 (without object) CH4
Mean: -0.027
Acceptable range: 2.5
Failure points: 0%

17:12:33.00   17:13:18.71   17:14:04.41   17:14:50.12

L1 (with object) CH3
Mean: 26.73
Acceptable range: 2.5
Failure points: 0%

17:16:30.02   17:17:16.51   17:18:03.00   17:18:49.48

L1 (with object) CH4
Mean: 11.56
Acceptable range: 2.5
Failure points: 0%

17:16:30.02   17:17:16.51   17:18:03.00   17:18:49.48

L2 (without object) CH3
Mean: -0.18
Acceptable range: 2.5
Failure points: 0%

17:19:55.98   17:20:12.19   17:20:28.40   17:20:44.61

L2 (without object) CH4
Mean: -0.081
Acceptable range: 2.5
Failure points: 0%

17:19:55.98   17:20:12.19   17:20:28.40   17:20:44.61

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
-- Acceptable limits

PM test
Operator: PN
Date: 12/30/2009

L0 (without object)
CH1
Mean: -1.47
Acceptable range: 2.5
Failure points: 2.72%

L0 (without object)
CH2
Mean: -0.99
Acceptable range: 2.5
Failure points: 0%

18:24:36.20 18:25:26.43 18:26:16.66 18:27:06.89
18:24:36.20 18:25:26.43 18:26:16.66 18:27:06.89

L1 (with object)
CH1
Mean: 74.77
Acceptable range: 2.5
Failure points: 2.16%

L1 (with object)
CH2
Mean: 44.83
Acceptable range: 2.5
Failure points: 0%

18:29:12.41 18:30:01.88 18:30:51.35 18:31:40.82 18:32
18:29:12.41 18:30:01.88 18:30:51.35 18:31:40.82 18:32

L2 (without object)
CH1
Mean: -5.42
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH2
Mean: -2.72
Acceptable range: 2.5
Failure points: 0%

18:32:53.44 18:33:10.41 18:33:27.38 18:33:44.35 18:34
18:32:53.44 18:33:10.41 18:33:27.38 18:33:44.35 18:34

Database: D:\Projects_QCReports_Ord_Data\123009\123009PM.gdb
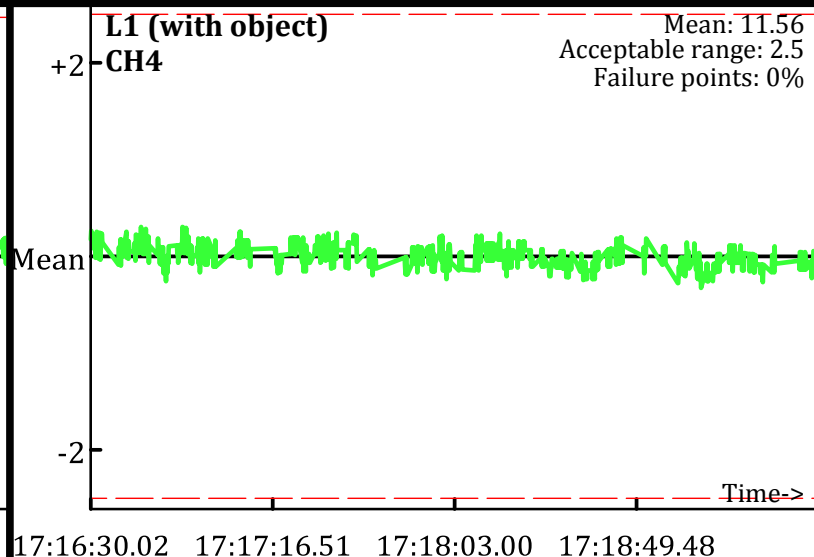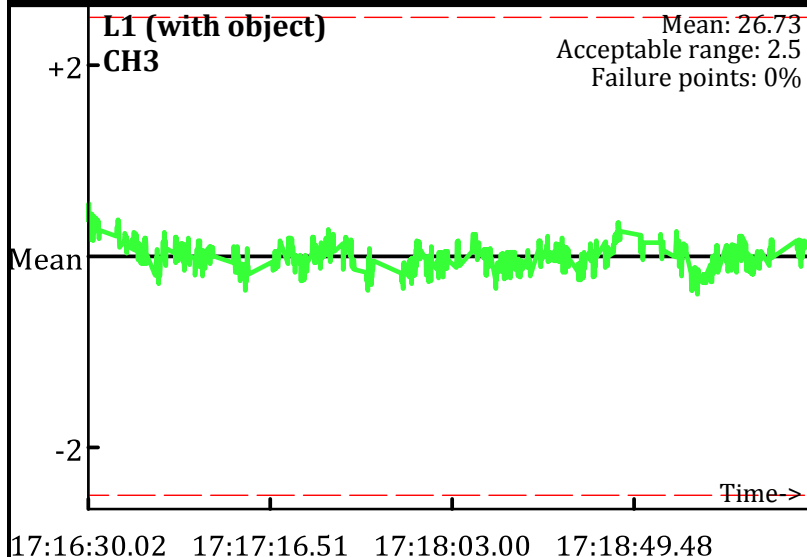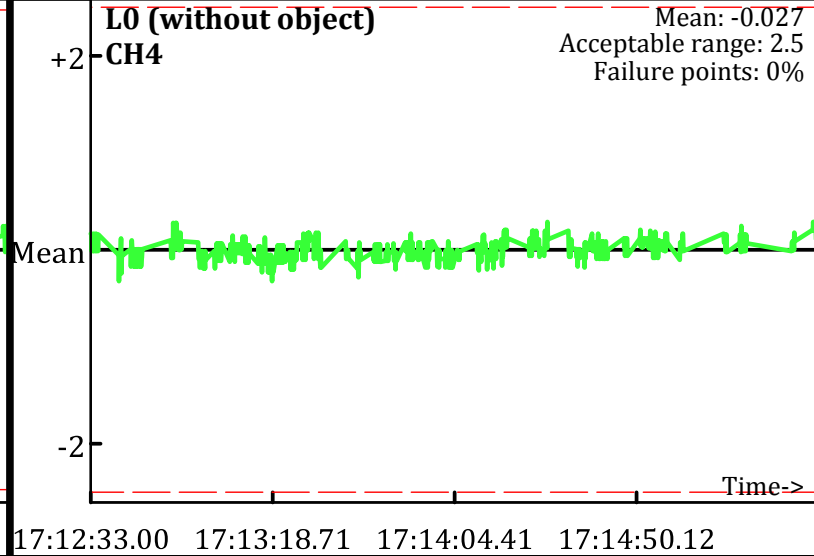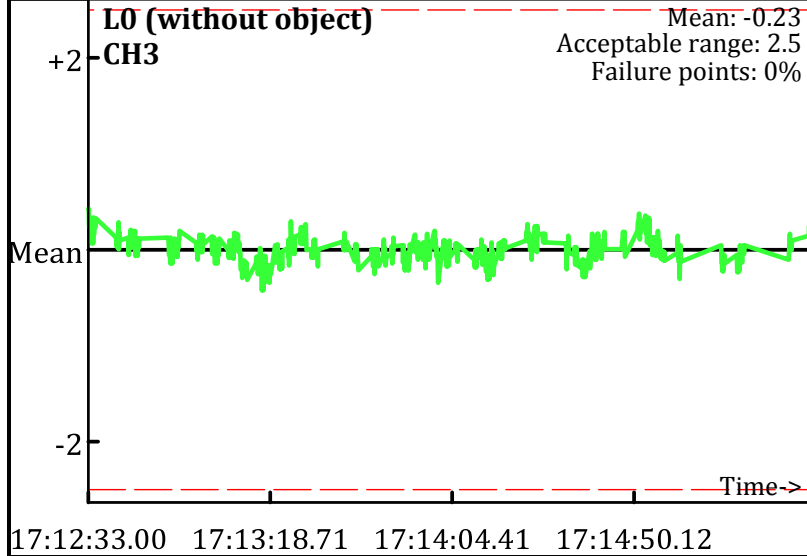Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Data collected using the single unit EM61 cart. Therefore this series will only have 2 pages for AM & 2 pages for PM

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN
Date: 12/30/2009
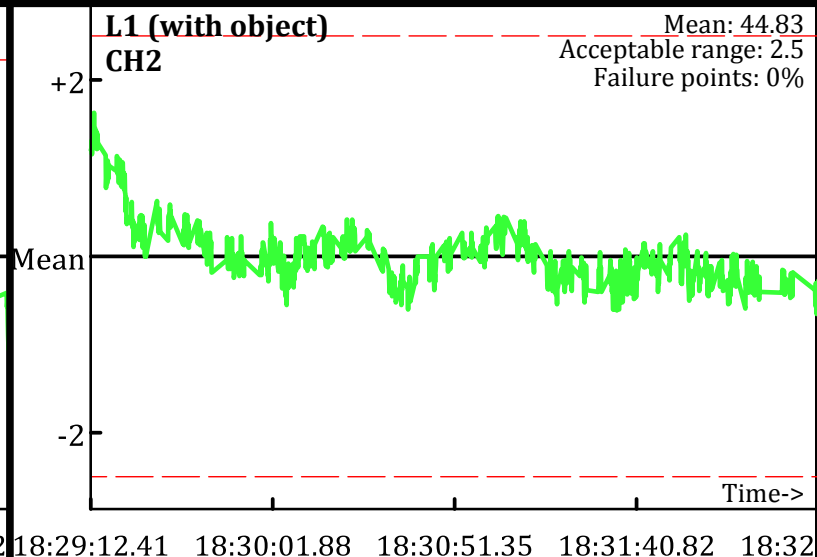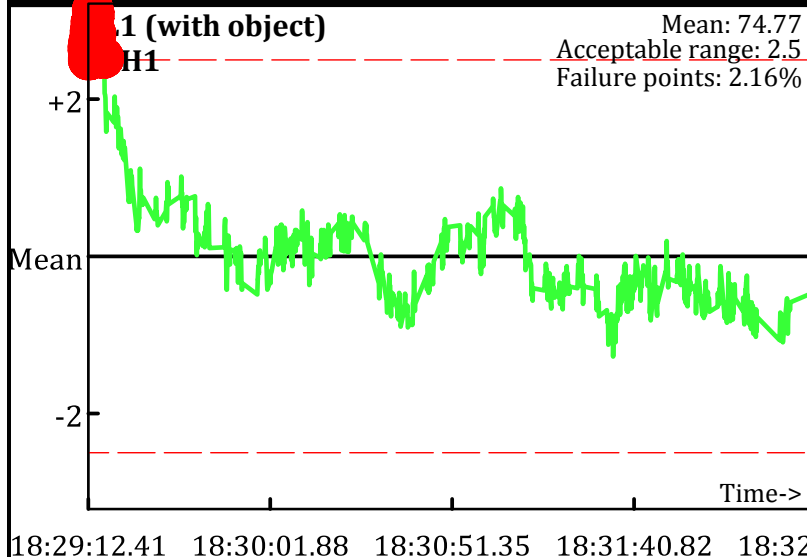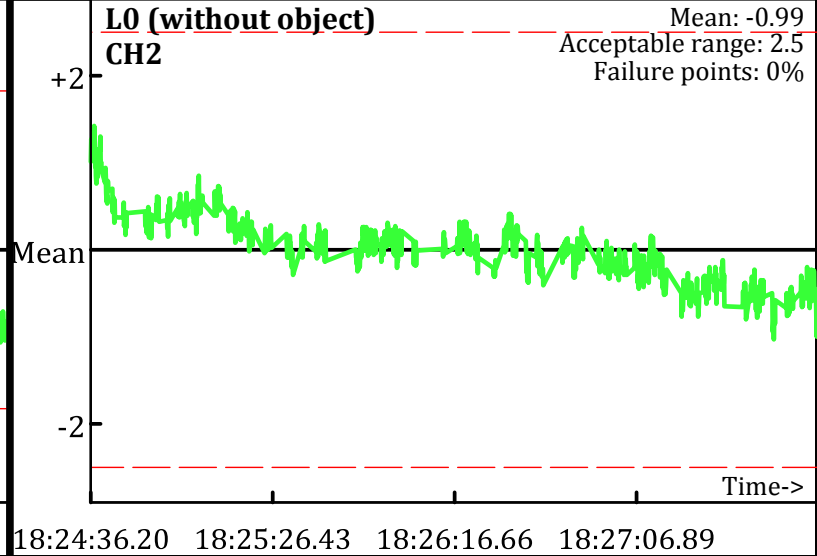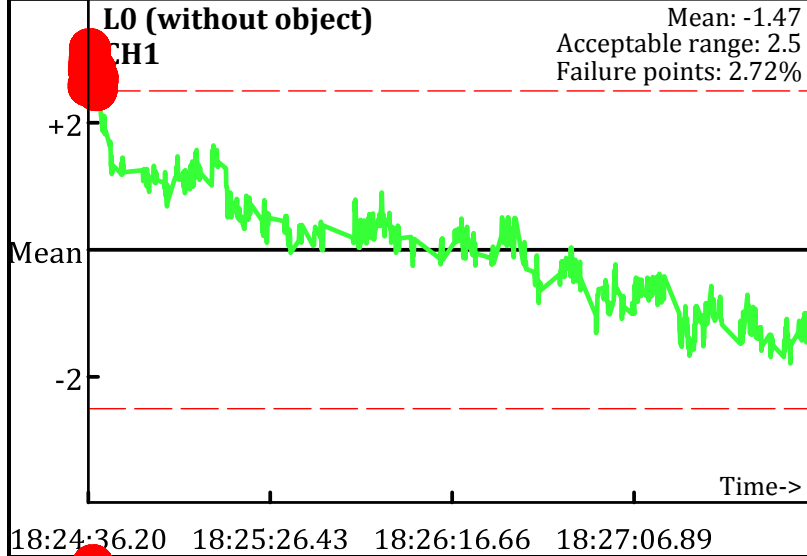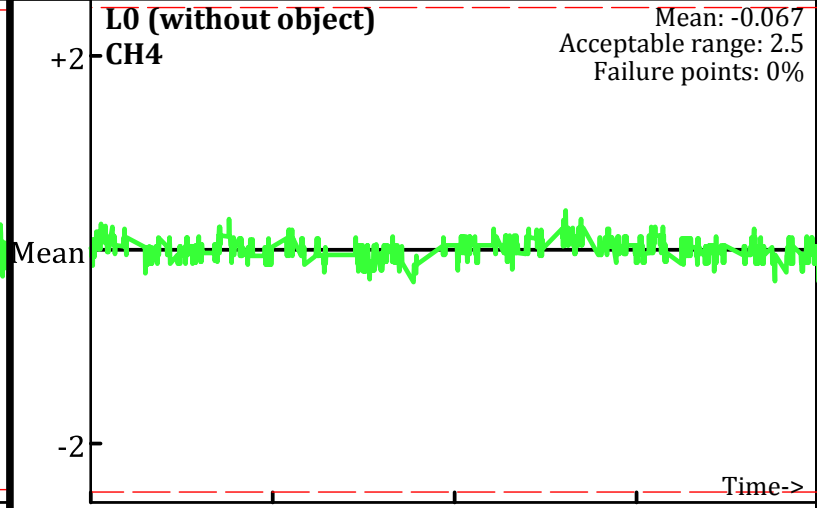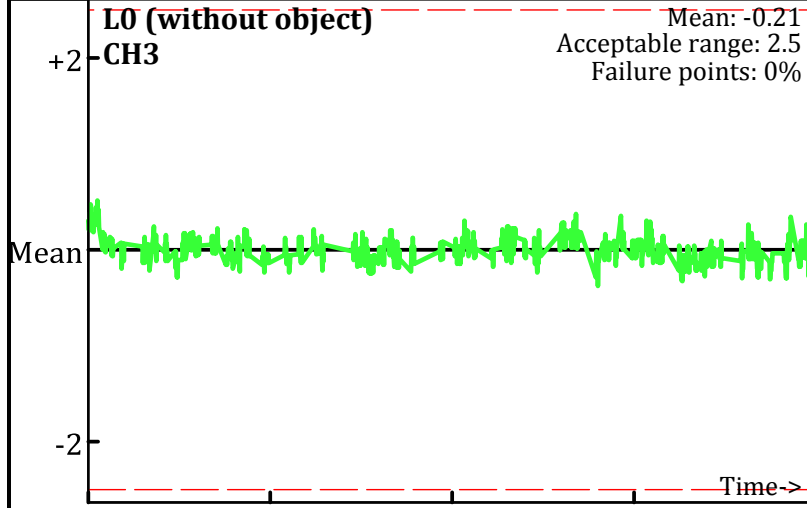
L0 (without object)
CH3
+2
Mean
-2

Mean: -0.21
Acceptable range: 2.5
Failure points: 0%

Time->

18:24:36.20   18:25:26.43   18:26:16.66   18:27:06.89

L0 (without object)
CH4
+2
Mean
-2

Mean: -0.067
Acceptable range: 2.5
Failure points: 0%

Time->

18:24:36.20   18:25:26.43   18:26:16.66   18:27:06.89

L1 (with object)
CH3
+2
Mean
-2

Mean: 22.65
Acceptable range: 2.5
Failure points: 0%

Time->

18:29:12.41   18:30:01.88   18:30:51.35   18:31:40.82   18:32

L1 (with object)
CH4
+2
Mean
-2

Mean: 9.23
Acceptable range: 2.5
Failure points: 0%

Time->

18:29:12.41   18:30:01.88   18:30:51.35   18:31:40.82   18:32

L2 (without object)
CH3
+2
Mean
-2

Mean: -0.56
Acceptable range: 2.5
Failure points: 0%

Time->

18:32:53.44   18:33:10.41   18:33:27.38   18:33:44.35   18:34

L2 (without object)
CH4
+2
Mean
-2

Mean: -0.24
Acceptable range: 2.5
Failure points: 0%

Time->

18:32:53.44   18:33:10.41   18:33:27.38   18:33:44.35   18:34

Database: D:\Projects_QCReports_Ord_Data\123009\123009PM.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH1
Mean: -2.27
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH2
Mean: -1.35
Acceptable range: 2.5
Failure points: 0%

09:47:50.31   09:48:39.54   09:49:28.78   09:50:18.01

09:47:50.31   09:48:39.54   09:49:28.78   09:50:18.01

L1 (with object)
CH1
Mean: 131.33
Acceptable range: 2.5
Failure points: 2.43%

L1 (with object)
CH2
Mean: 86.72
Acceptable range: 2.5
Failure points: 0%

09:51:59.39   09:52:52.37   09:53:45.34   09:54:38.31   09:55

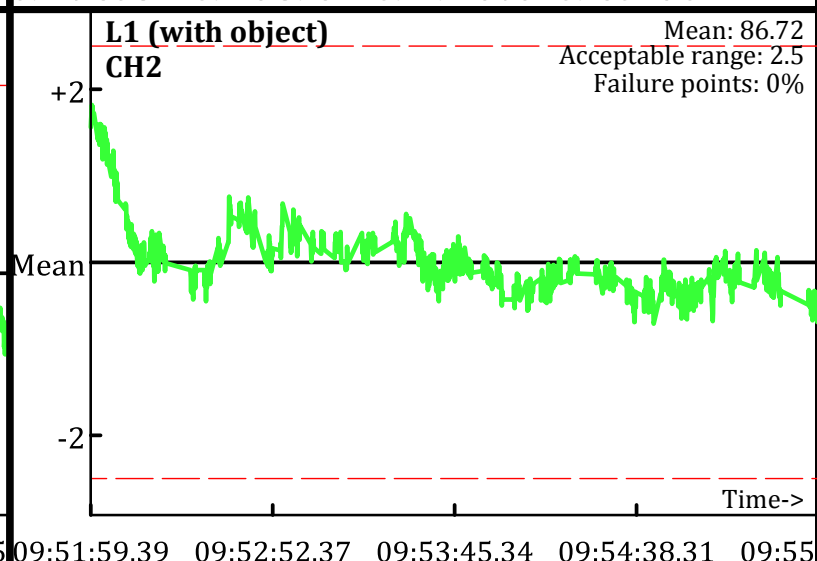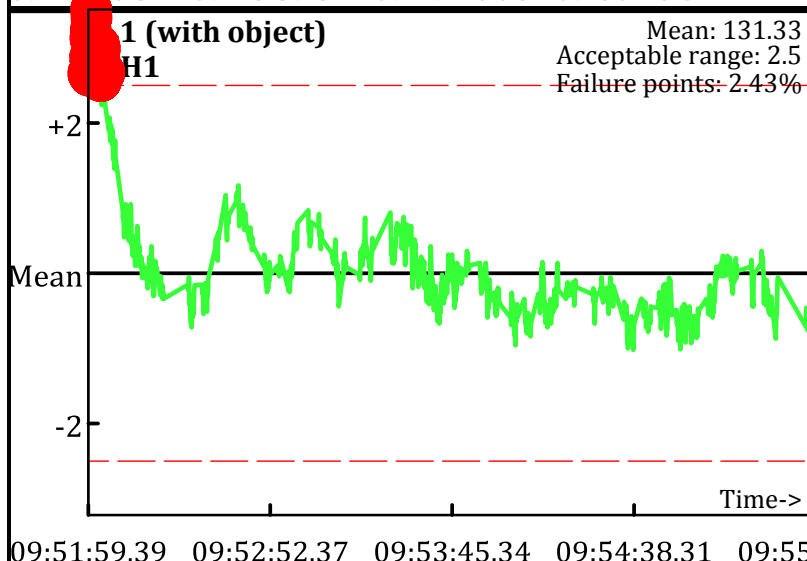09:51:59.39   09:52:52.37   09:53:45.34   09:54:38.31   09:55

L2 (without object)
CH1
Mean: -3.59
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH2
Mean: -2.44
Acceptable range: 2.5
Failure points: 0%

09:56:01.37   09:56:16.59   09:56:31.82   09:56:47.05   09:57

09:56:01.37   09:56:16.59   09:56:31.82   09:56:47.05   09:57

Database: D:\Projects_QCReports_Ord_Data\112509\112509AM.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
— — Acceptable limits

AM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH3

Mean: -0.38
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:47:50.31   09:48:39.54   09:49:28.78   09:50:18.01

L0 (without object)
CH4

Mean: -0.13
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:47:50.31   09:48:39.54   09:49:28.78   09:50:18.01

L1 (with object)
CH3

Mean: 49.34
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:51:59.39   09:52:52.37   09:53:45.34   09:54:38.31   09:55

L1 (with object)
CH4

Mean: 23.21
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:51:59.39   09:52:52.37   09:53:45.34   09:54:38.31   09:55

L2 (without object)
CH3

Mean: -0.59
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:56:01.37   09:56:16.59   09:56:31.82   09:56:47.05   09:57

L2 (without object)
CH4

Mean: -0.19
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

09:56:01.37   09:56:16.59   09:56:31.82   09:56:47.05   09:57

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN
Date: 1/7/2010
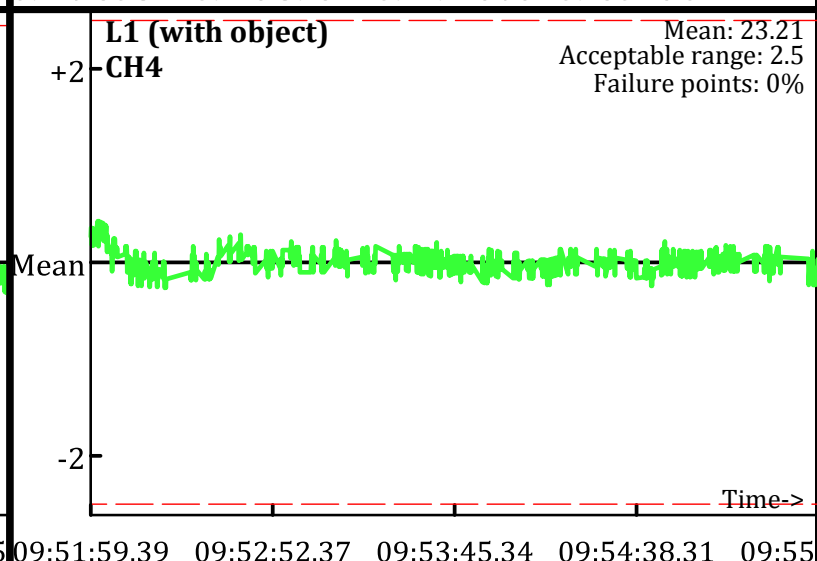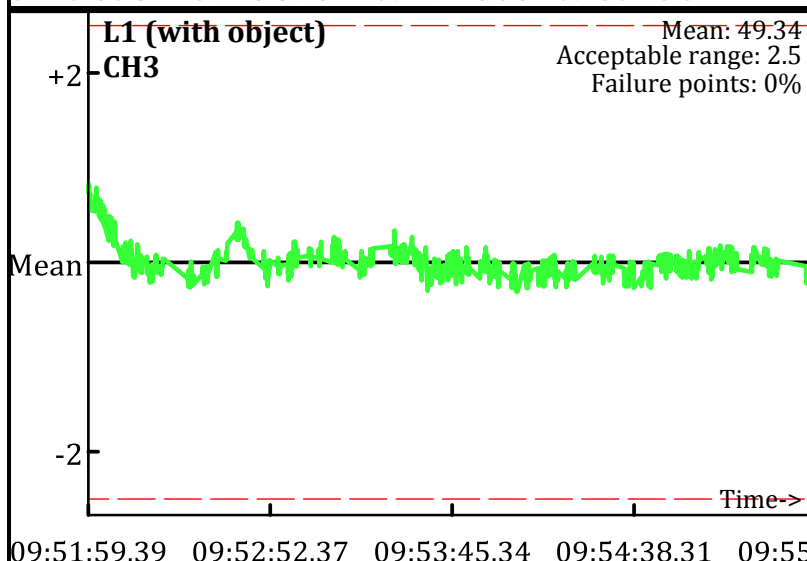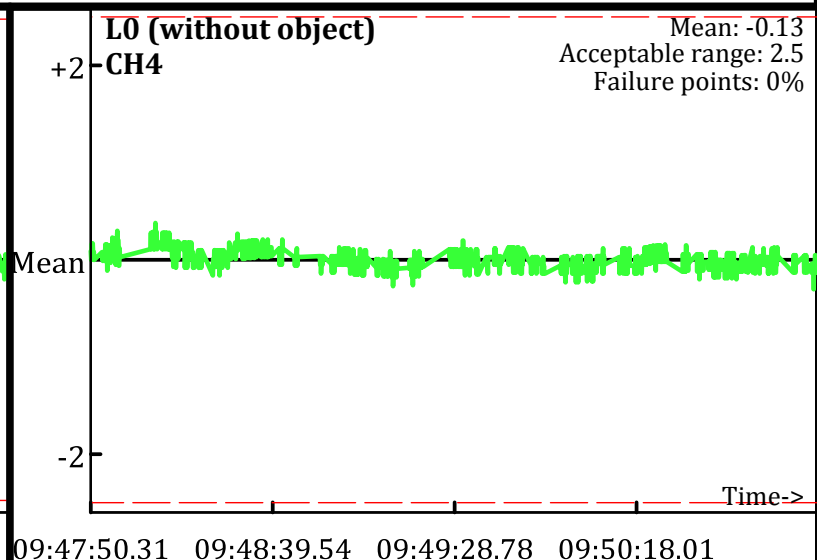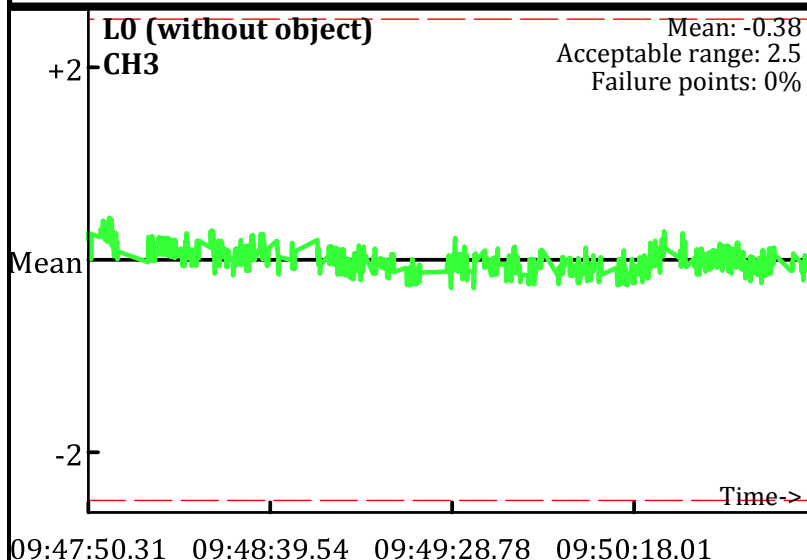
L0 (without object)
CH3
+2
Mean
-2
Time->

Mean: -0.5
Acceptable range: 2.5
Failure points: 0%

11:11:27.66   11:12:20.13   11:13:12.60   11:14:05.06   11:14

L0 (without object)
CH4
+2
Mean
-2
Time->

Mean: -0.22
Acceptable range: 2.5
Failure points: 0%

11:11:27.66   11:12:20.13   11:13:12.60   11:14:05.06   11:14

L1 (with object)
CH3
+2
Mean
-2
Time->

Mean: 30.14
Acceptable range: 2.5
Failure points: 0%

11:15:38.11   11:16:26.57   11:17:15.02   11:18:03.48   11:18

L1 (with object)
CH4
+2
Mean
-2
Time->

Mean: 13.21
Acceptable range: 2.5
Failure points: 0%

11:15:38.11   11:16:26.57   11:17:15.02   11:18:03.48   11:18

L2 (without object)
CH3
+2
Mean
-2
Time->

Mean: -0.59
Acceptable range: 2.5
Failure points: 0%

11:19:19.97   11:19:35.93   11:19:51.89   11:20:07.85

L2 (without object)
CH4
+2
Mean
-2
Time->

Mean: -0.27
Acceptable range: 2.5
Failure points: 0%

11:19:19.97   11:19:35.93   11:19:51.89   11:20:07.85

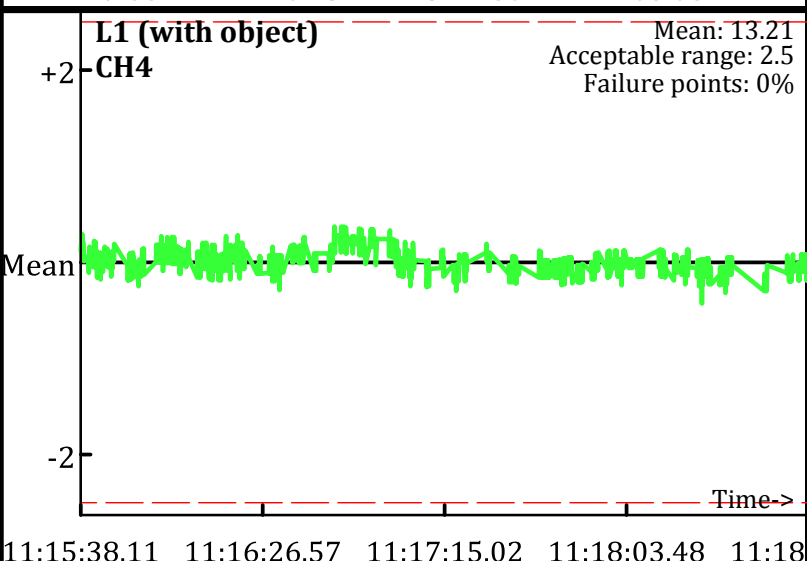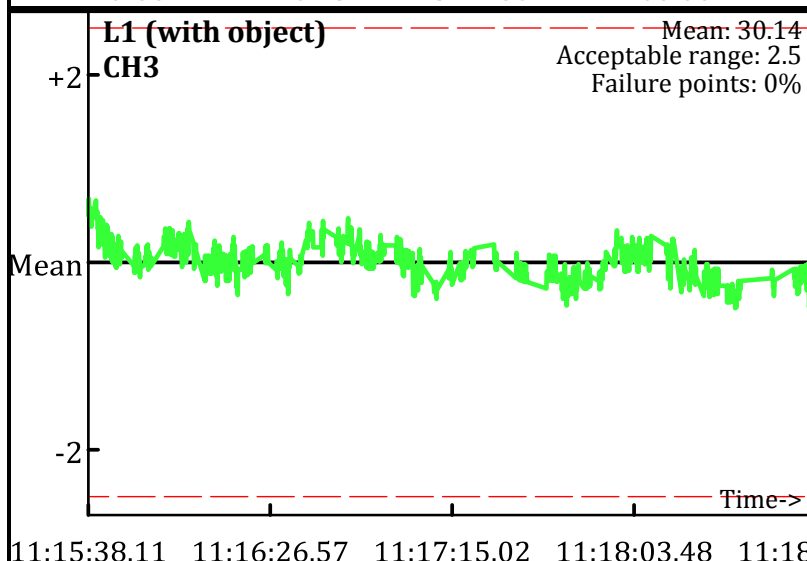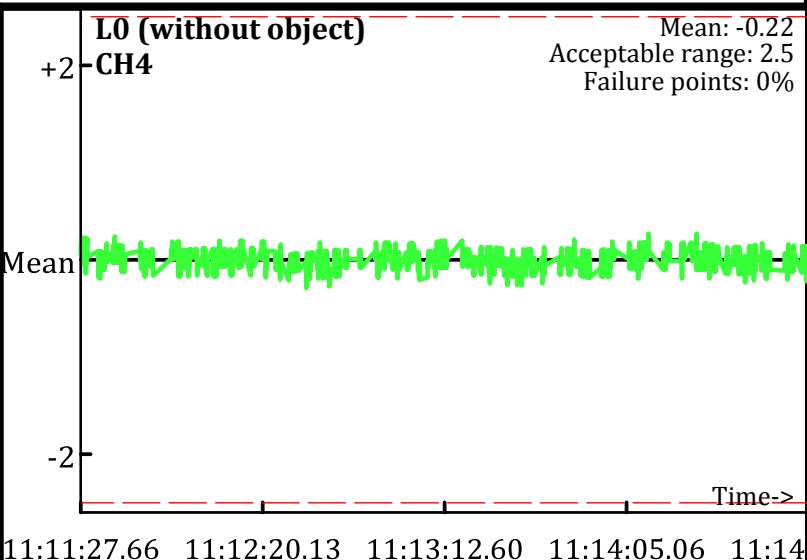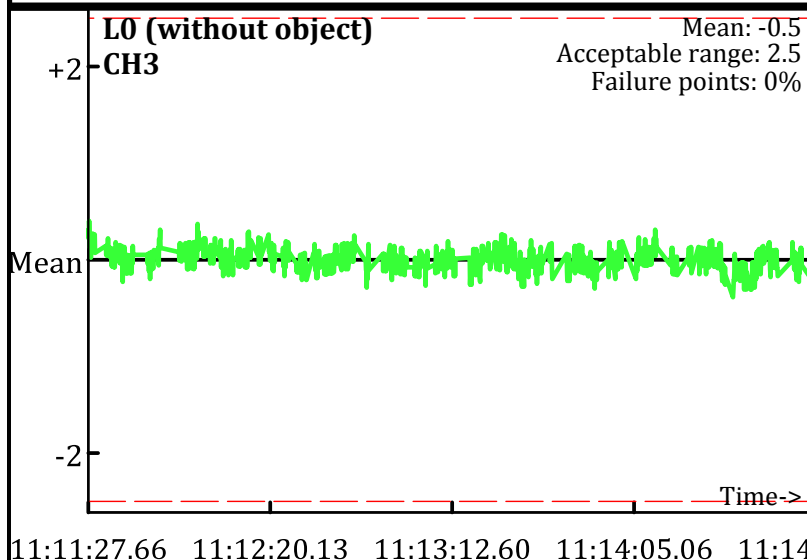Database: D:\Projects_QCReports_Ord_Data\120809\120809AM.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
- - - Acceptable limits

AM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH1
Mean: -2.51
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH2
Mean: -1.6
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH1
Mean: 91.59
Acceptable range: 2.5
Failure points: 0.978%

L1 (with object)
CH2
Mean: 56.64
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH1
Mean: -1.63
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH2
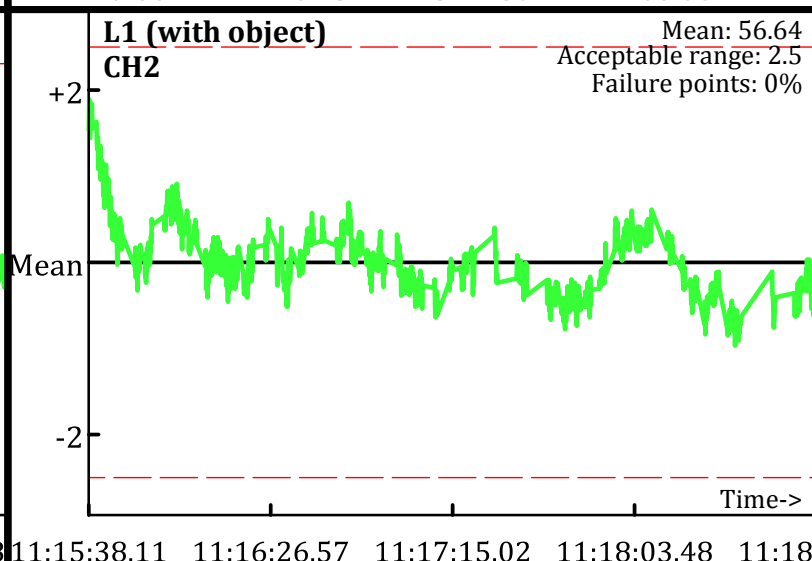Mean: -2.1
Acceptable range: 2.5
Failure points: 0%

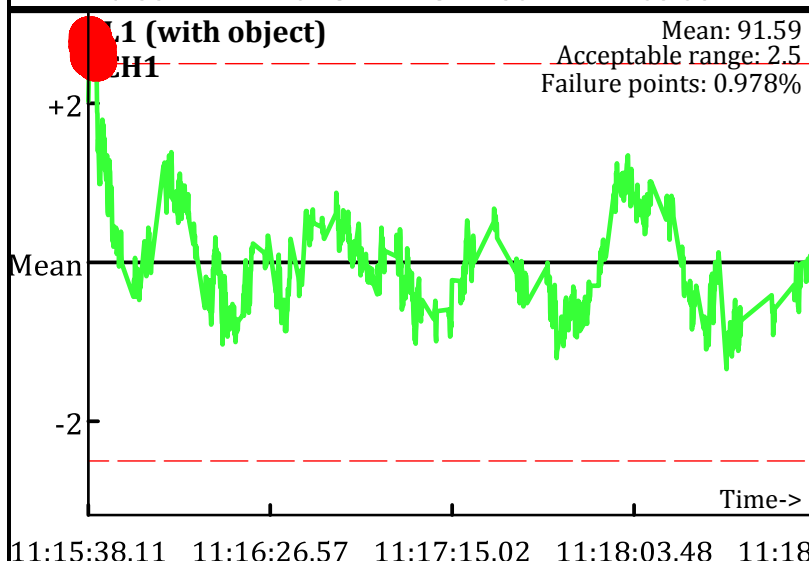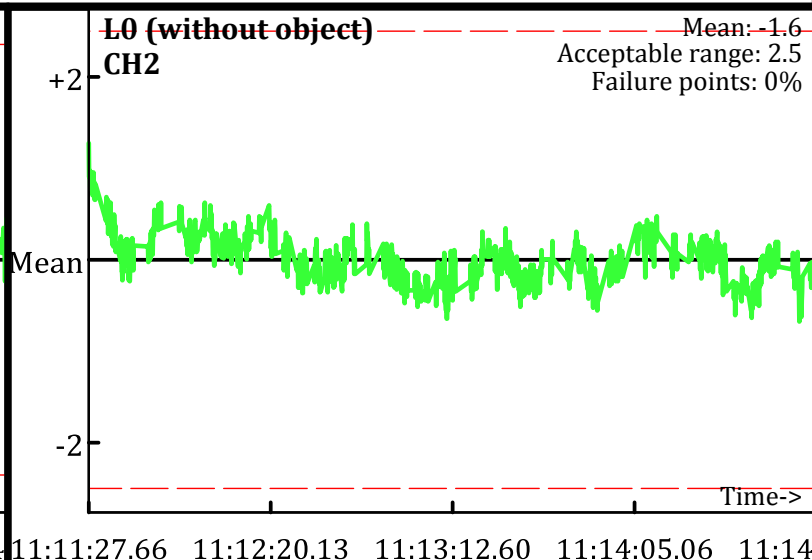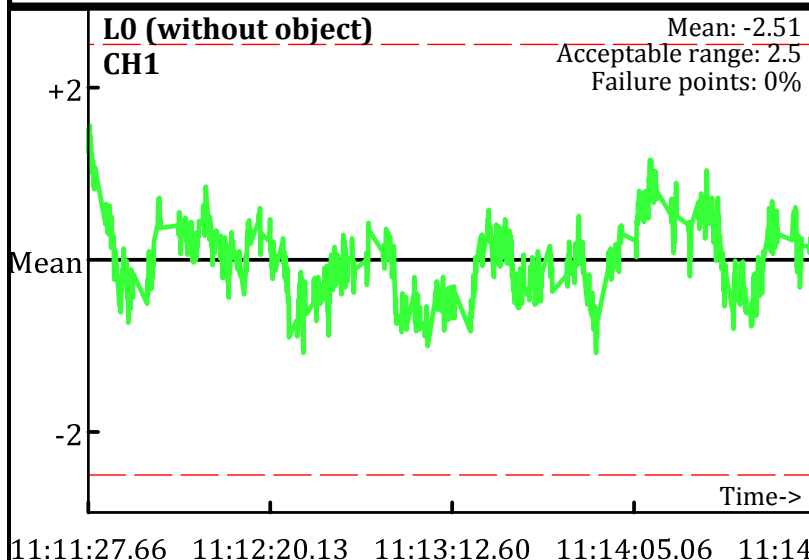# Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
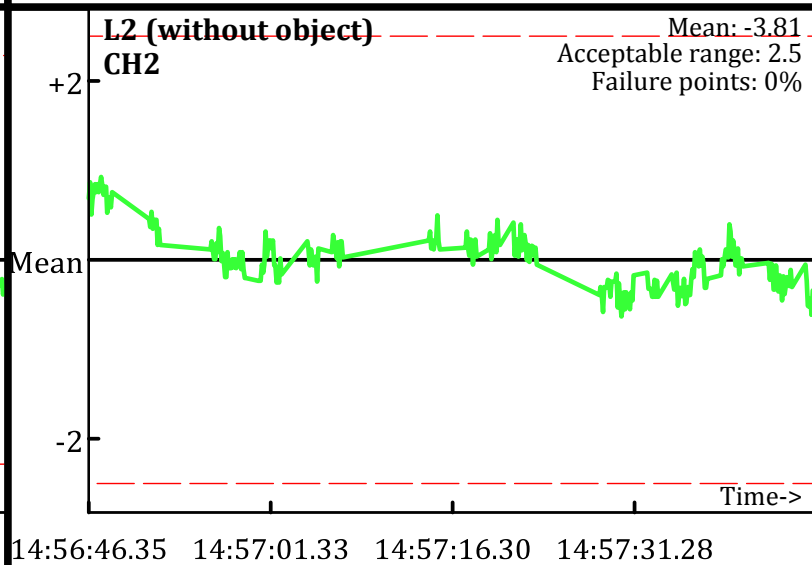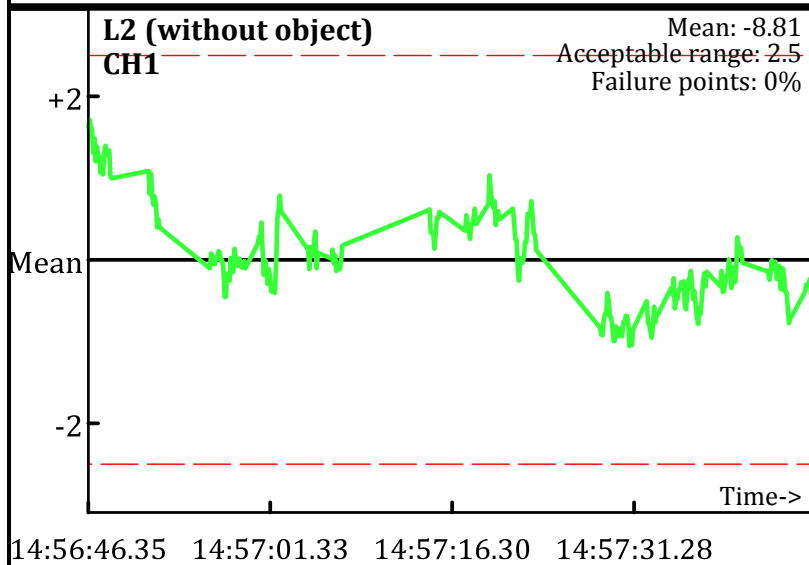Grid/Location: QC Area

● Outside range
- - - Acceptable limits

AM test
Operator: PN
Date: 1/7/2010

L0 (without object) CH1

Mean: -3.29
Acceptable range: 2.5
Failure points: 3.71%

14:45:31.43 14:46:18.40 14:47:05.37 14:47:52.35 14:48

L0 (without object) CH2

Mean: -1.19
Acceptable range: 2.5
Failure points: 0%

14:45:31.43 14:46:18.40 14:47:05.37 14:47:52.35 14:48

L1 (with object) CH1

Mean: 131.97
Acceptable range: 2.5
Failure points: 2.66%

14:49:36.69 14:50:22.14 14:51:07.59 14:51:53.05

L1 (with object) CH2

Mean: 89.15
Acceptable range: 2.5
Failure points: 0%

14:49:36.69 14:50:22.14 14:51:07.59 14:51:53.05

L2 (without object) CH1

Mean: -8.81
Acceptable range: 2.5
Failure points: 0%

14:56:46.35 14:57:01.33 14:57:16.30 14:57:31.28

L2 (without object) CH2

Mean: -3.81
Acceptable range: 2.5
Failure points: 0%

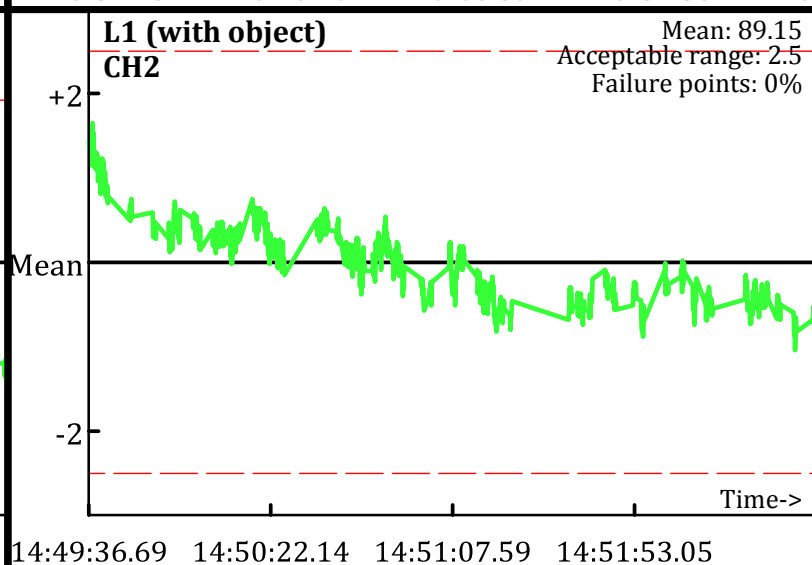14:56:46.35 14:57:01.33 14:57:16.30 14:57:31.28

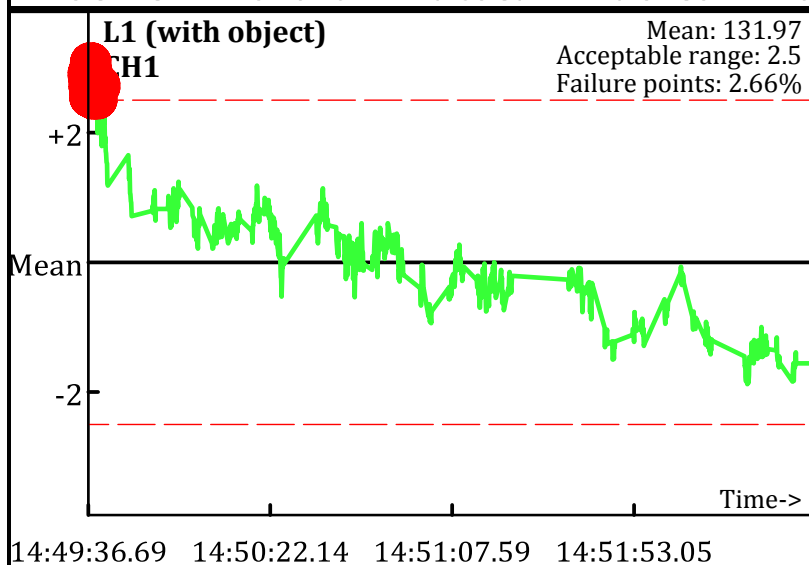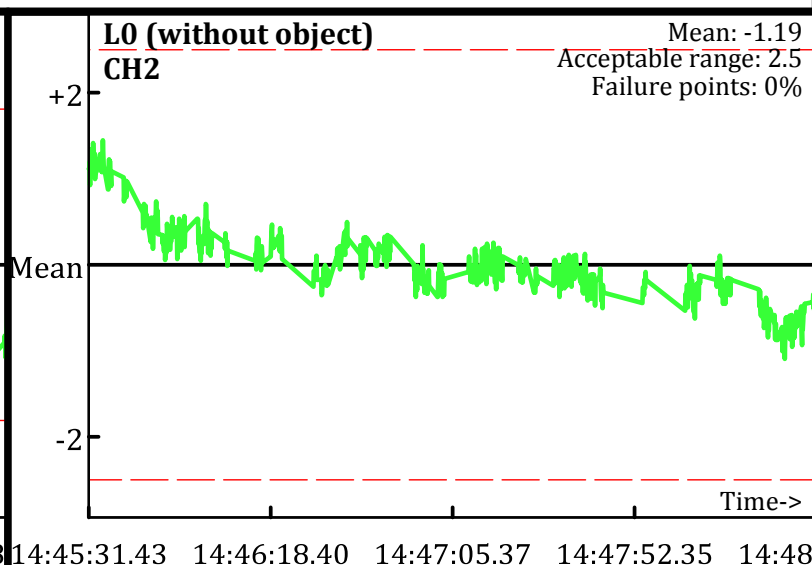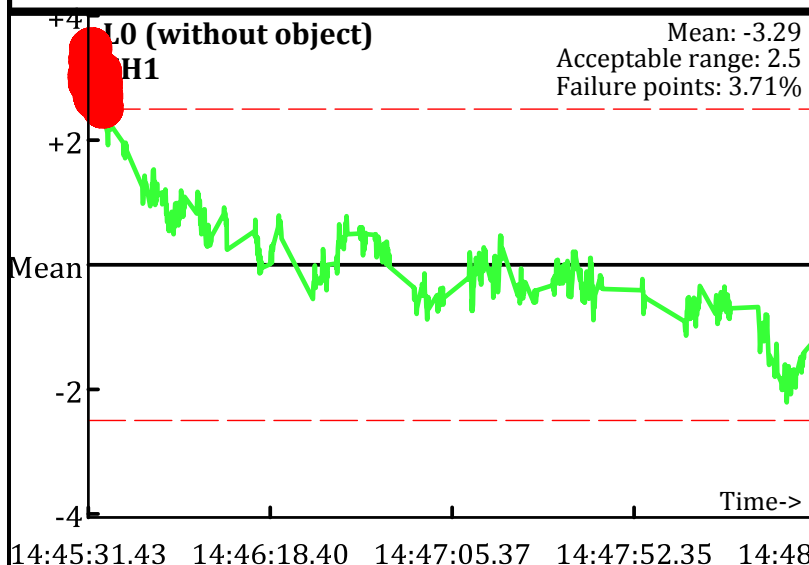# Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
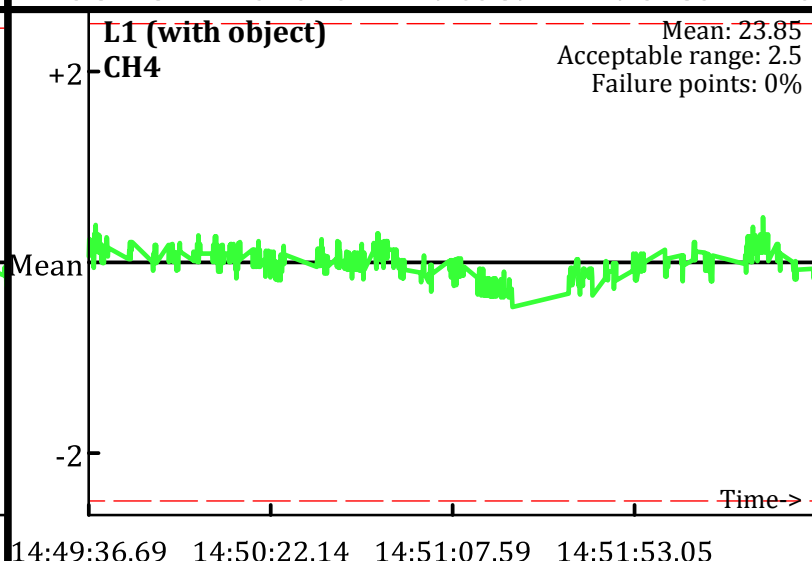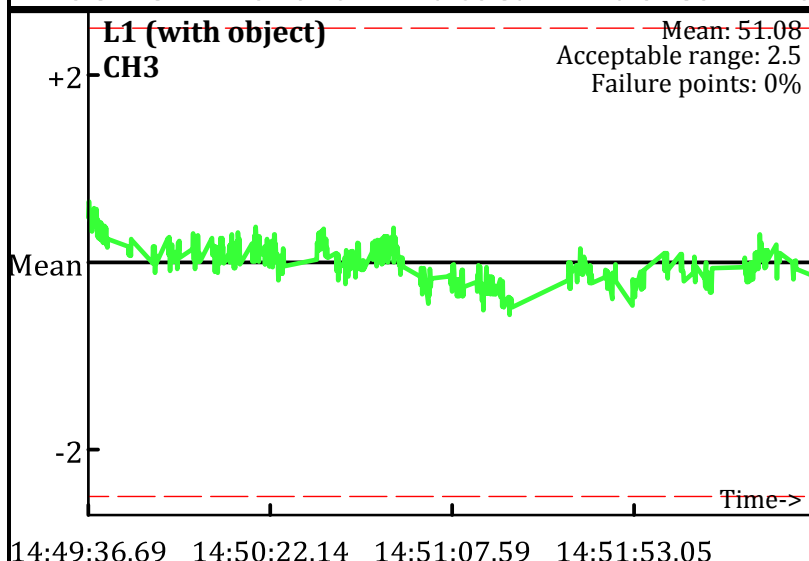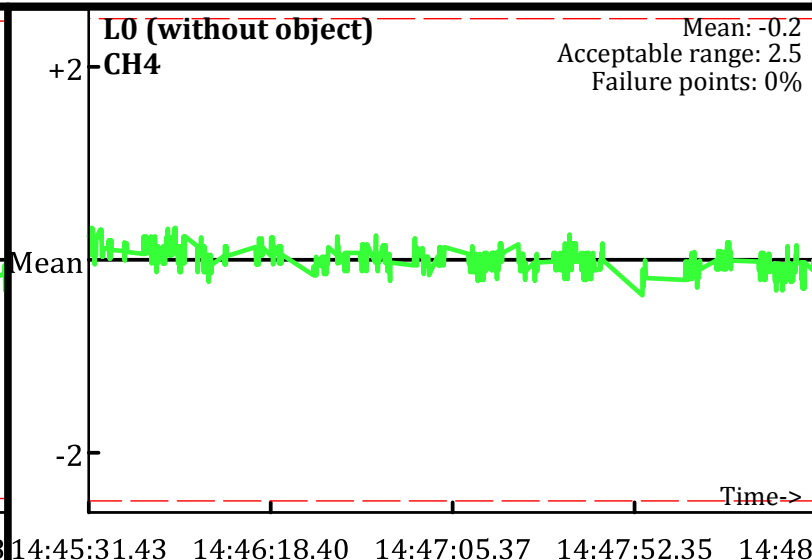Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH3
+2
Mean
-2

Mean: -0.32
Acceptable range: 2.5
Failure points: 0%

Time->

14:45:31.43   14:46:18.40   14:47:05.37   14:47:52.35   14:48

L0 (without object)
CH4
+2
Mean
-2

Mean: -0.2
Acceptable range: 2.5
Failure points: 0%

Time->

14:45:31.43   14:46:18.40   14:47:05.37   14:47:52.35   14:48

L1 (with object)
CH3
+2
Mean
-2

Mean: 51.08
Acceptable range: 2.5
Failure points: 0%

Time->

14:49:36.69   14:50:22.14   14:51:07.59   14:51:53.05

L1 (with object)
CH4
+2
Mean
-2

Mean: 23.85
Acceptable range: 2.5
Failure points: 0%

Time->

14:49:36.69   14:50:22.14   14:51:07.59   14:51:53.05

L2 (without object)
CH3
+2
Mean
-2

Mean: -0.81
Acceptable range: 2.5
Failure points: 0%

Time->

14:56:46.35   14:57:01.33   14:57:16.30   14:57:31.28

L2 (without object)
CH4
+2
Mean
-2

Mean: -0.67
Acceptable range: 2.5
Failure points: 0%

Time->

14:56:46.35   14:57:01.33   14:57:16.30   14:57:31.28

Database: D:\Projects_QCReports_Ord_Data\112409\112409AM.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

L0 (without object)
CH1
Mean: -2.77
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:14:55.41   17:15:53.17   17:16:50.92   17:17:48.68

L0 (without object)
CH2
Mean: -1.23
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:14:55.41   17:15:53.17   17:16:50.92   17:17:48.68

L1 (with object)
CH1
Mean: 93.71
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:20:22.88   17:21:12.36   17:22:01.83   17:22:51.30   17:23

L1 (with object)
CH2
Mean: 59.56
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:20:22.88   17:21:12.36   17:22:01.83   17:22:51.30   17:23

L2 (without object)
CH1
Mean: -2.72
Acceptable range: 2.5
Failure points: 3.91%

+2

Mean

-2

Time->

17:23:58.12   17:24:14.59   17:24:31.06   17:24:47.54   17:25

L2 (without object)
CH2
Mean: -1.37
Acceptable range: 2.5
Failure points: 0%

+2

Mean

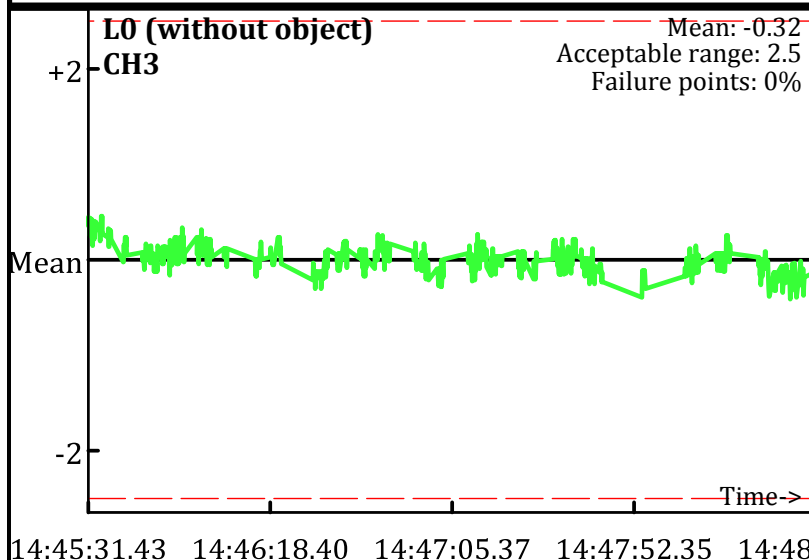-2

Time->

17:23:58.12   17:24:14.59   17:24:31.06   17:24:47.54   17:25

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
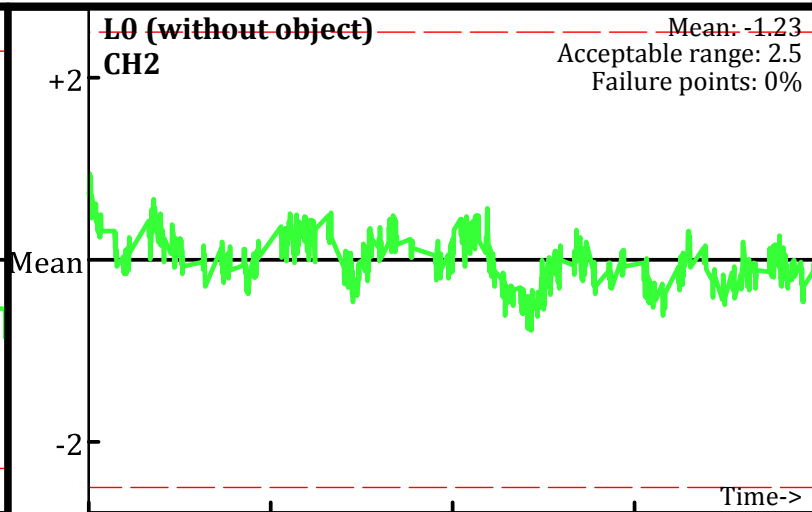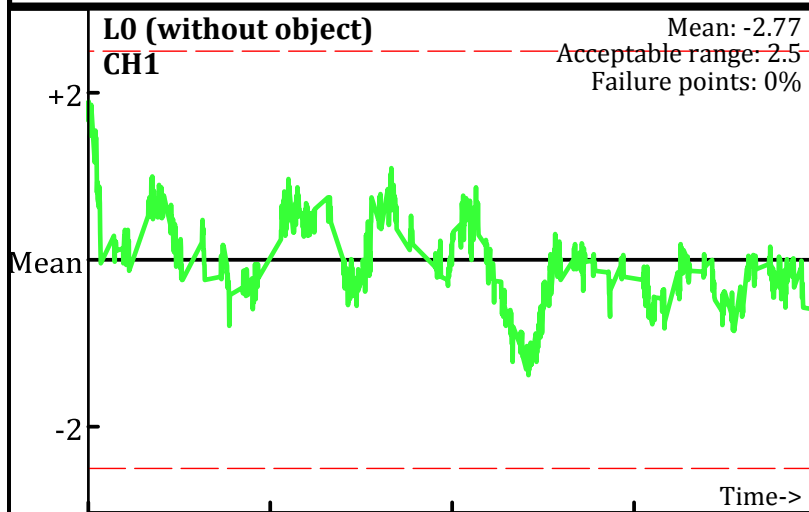– – – Acceptable limits

PM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH3
Mean: -0.27
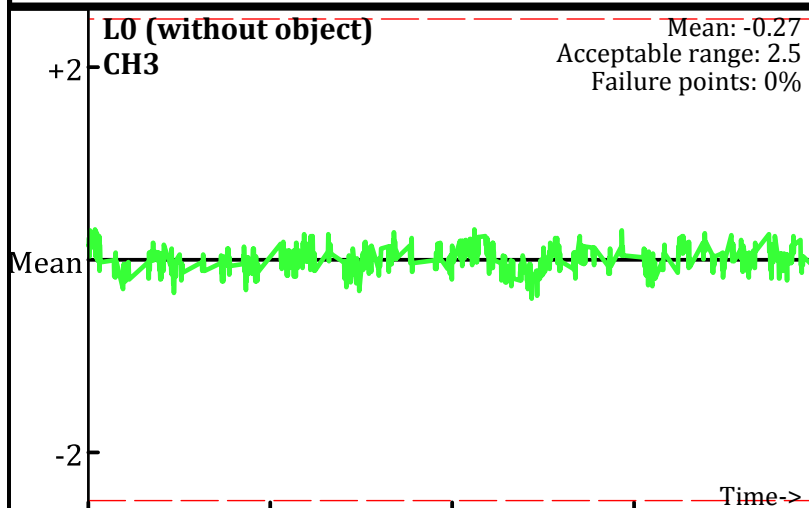Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:14:55.41   17:15:53.17   17:16:50.92   17:17:48.68

L0 (without object)
CH4
Mean: -0.057
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:14:55.41   17:15:53.17   17:16:50.92   17:17:48.68

L1 (with object)
CH3
Mean: 32.09
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:20:22.88   17:21:12.36   17:22:01.83   17:22:51.30   17:23

L1 (with object)
CH4
Mean: 14.29
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:20:22.88   17:21:12.36   17:22:01.83   17:22:51.30   17:23

L2 (without object)
CH3
Mean: -0.23
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:23:58.12   17:24:14.59   17:24:31.06   17:24:47.54   17:25

L2 (without object)
CH4
Mean: -0.11
Acceptable range: 2.5
Failure points: 0%
+2
Mean
-2
Time->
17:23:58.12   17:24:14.59   17:24:31.06   17:24:47.54   17:25

Database: D:\Projects_QCReports_Ord_Data\120809\120809PM.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

● Outside range
- - - Acceptable limits

L0 (without object)
CH1
Mean: -1.73
Acceptable range: 2.5
Failure points: 2.49%

+2

Mean

-2

Time->

17:49:33.19   17:50:19.93   17:51:06.67   17:51:53.41

L0 (without object)
CH2
Mean: -0.54
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:49:33.19   17:50:19.93   17:51:06.67   17:51:53.41

L1 (with object)
CH1
Mean: 136.5
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:55:51.38   17:56:35.85   17:57:20.32   17:58:04.79   17:58

L1 (with object)
CH2
Mean: 92.18
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:55:51.38   17:56:35.85   17:57:20.32   17:58:04.79   17:58

L2 (without object)
CH1
Mean: -3.23
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:59:26.61   17:59:42.09   17:59:57.57   18:00:13.05

L2 (without object)
CH2
Mean: -0.89
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

17:59:26.61   17:59:42.09   17:59:57.57   18:00:13.05

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
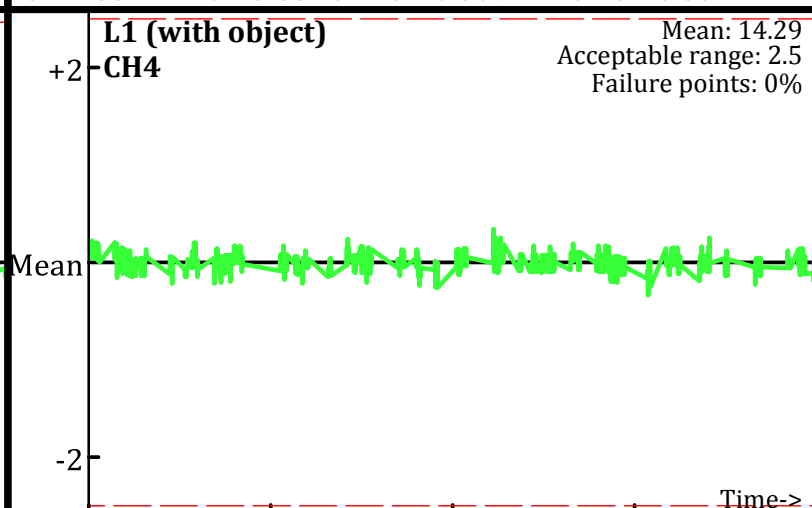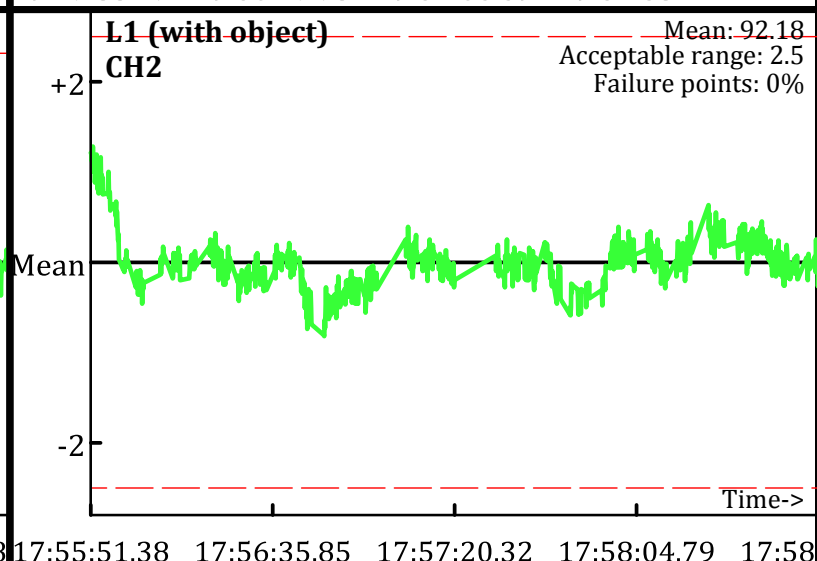Grid/Location: QC Area

⬤ Outside range
--- Acceptable limits

PM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH3
Mean: -0.067
Acceptable range: 2.5
Failure points: 0%

17:49:33.19   17:50:19.93   17:51:06.67   17:51:53.41

L0 (without object)
CH4
Mean: 0.045
Acceptable range: 2.5
Failure points: 0%

17:49:33.19   17:50:19.93   17:51:06.67   17:51:53.41

L1 (with object)
CH3
Mean: 52.67
Acceptable range: 2.5
Failure points: 0%

17:55:51.38   17:56:35.85   17:57:20.32   17:58:04.79   17:58

L1 (with object)
CH4
Mean: 25.07
Acceptable range: 2.5
Failure points: 0%

17:55:51.38   17:56:35.85   17:57:20.32   17:58:04.79   17:58

L2 (without object)
CH3
Mean: -0.016
Acceptable range: 2.5
Failure points: 0%

17:59:26.61   17:59:42.09   17:59:57.57   18:00:13.05

L2 (without object)
CH4
Mean: 0.078
Acceptable range: 2.5
Failure points: 0%

17:59:26.61   17:59:42.09   17:59:57.57   18:00:13.05

Database: D:\Projects_QCReports_Ord_Data\112409\112409PM.gdb
Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN
Date: 1/7/2010
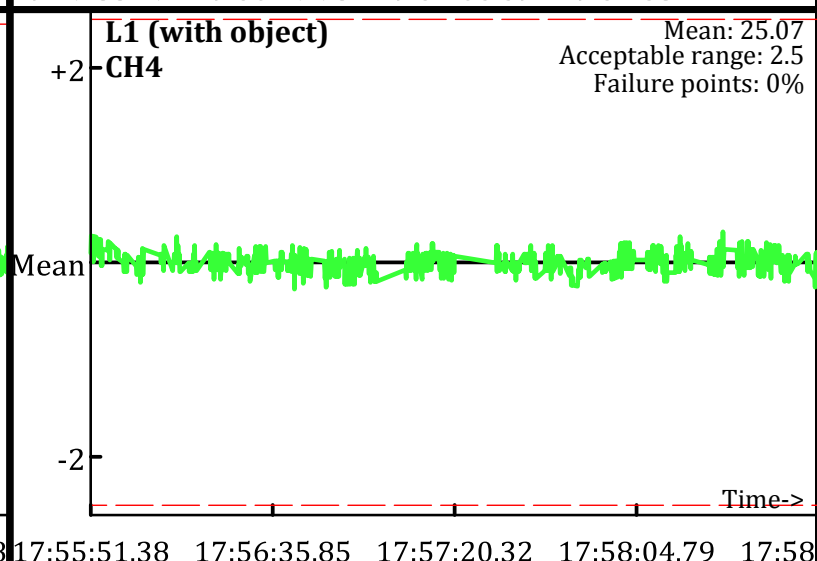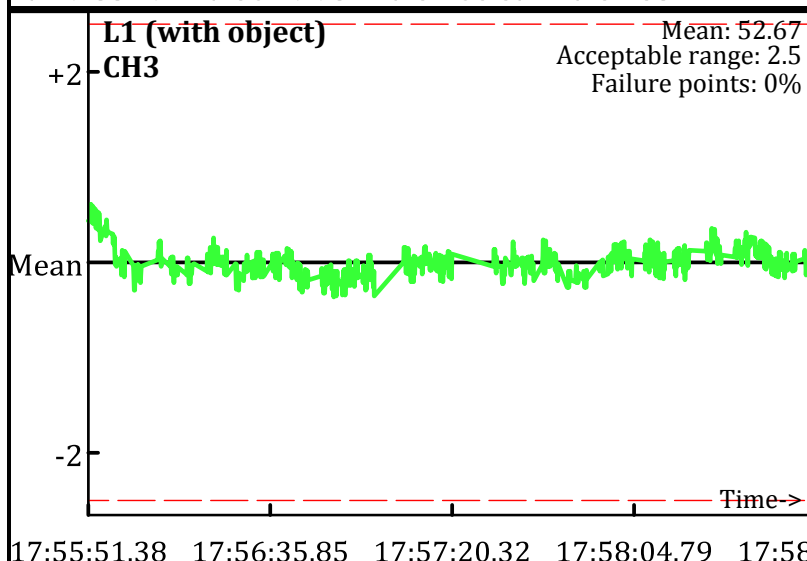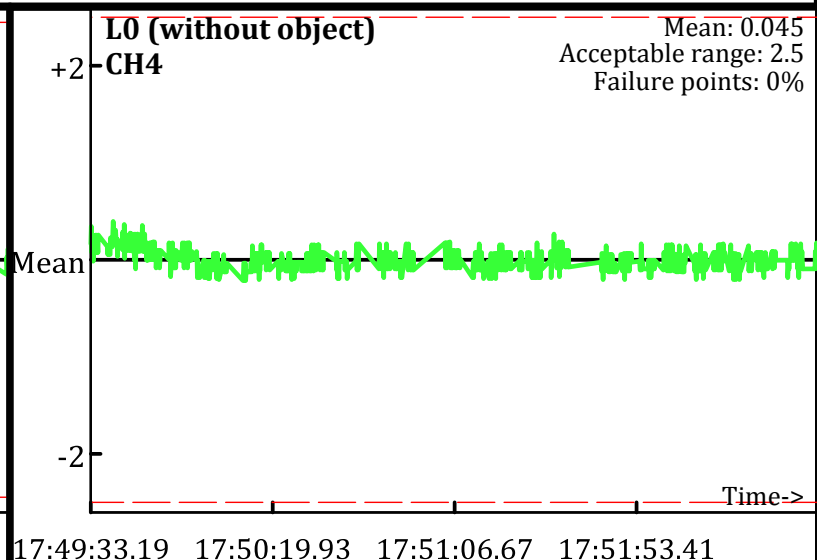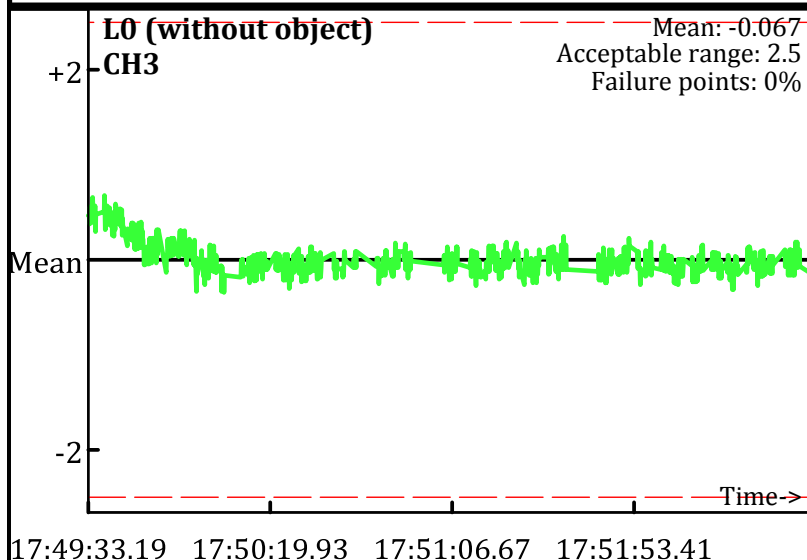
L0 (without object)
CH1
Mean: 1.59
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH2
Mean: 1.15
Acceptable range: 2.5
Failure points: 0%

Time->

18:14:08.21   18:14:54.42   18:15:40.63   18:16:26.85

18:14:08.21   18:14:54.42   18:15:40.63   18:16:26.85

L1 (with object)
CH1
Mean: 121.57
Acceptable range: 2.5
Failure points: 1.36%

L1 (with object)
CH2
Mean: 80.33
Acceptable range: 2.5
Failure points: 0%

Time->

18:18:32.92   18:19:20.37   18:20:07.82   18:20:55.28

18:18:32.92   18:19:20.37   18:20:07.82   18:20:55.28

L2 (without object)
CH1
Mean: 1.55
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH2
Mean: 1.58
Acceptable range: 2.5
Failure points: 0%

Time->

18:22:06.92   18:22:20.89   18:22:34.86   18:22:48.83   18:23

18:22:06.92   18:22:20.89   18:22:34.86   18:22:48.83   18:23

Database: D:\Projects_QCReports_Ord_Data\112509\112509PM.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: FortOrd-E20c.2
Equipment: EM-61 Mark II
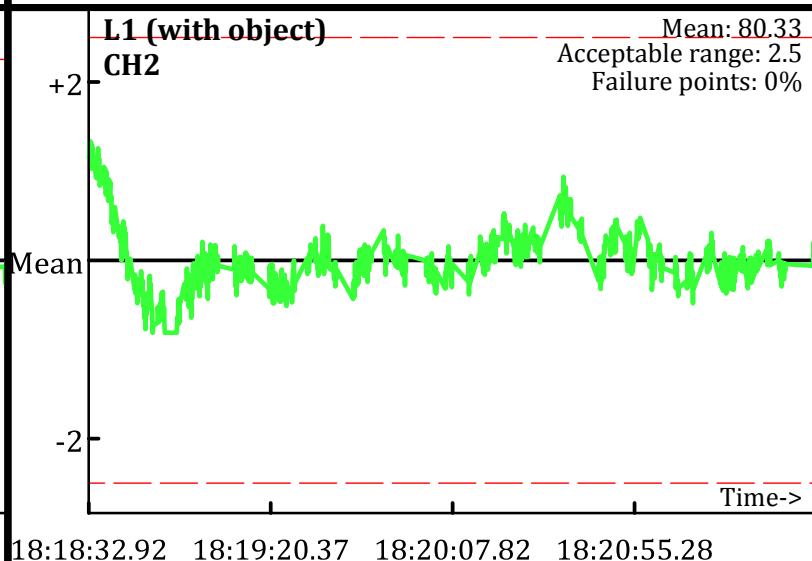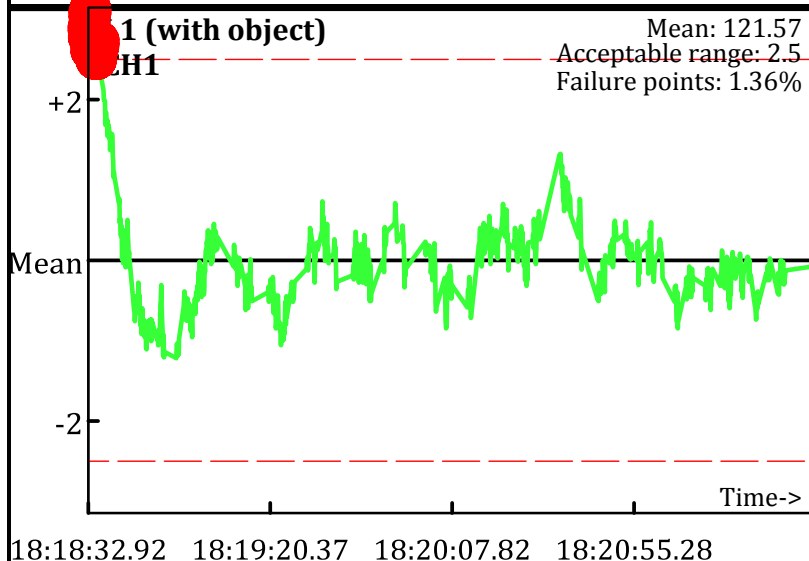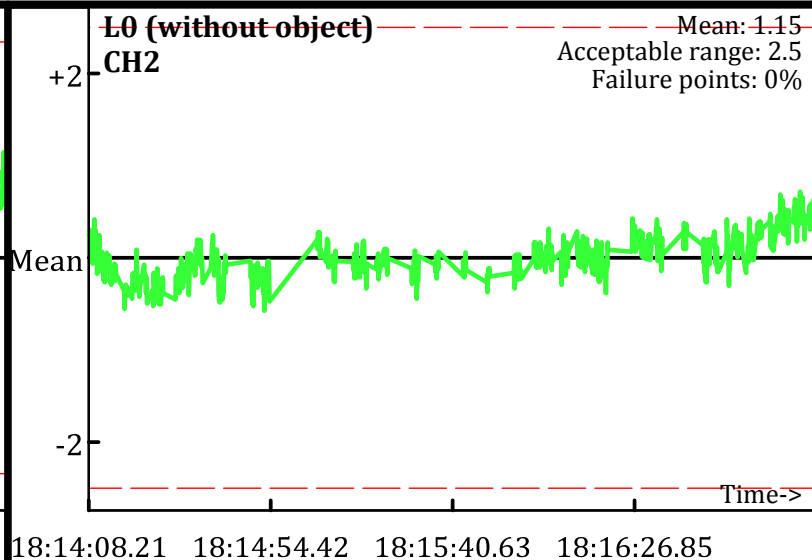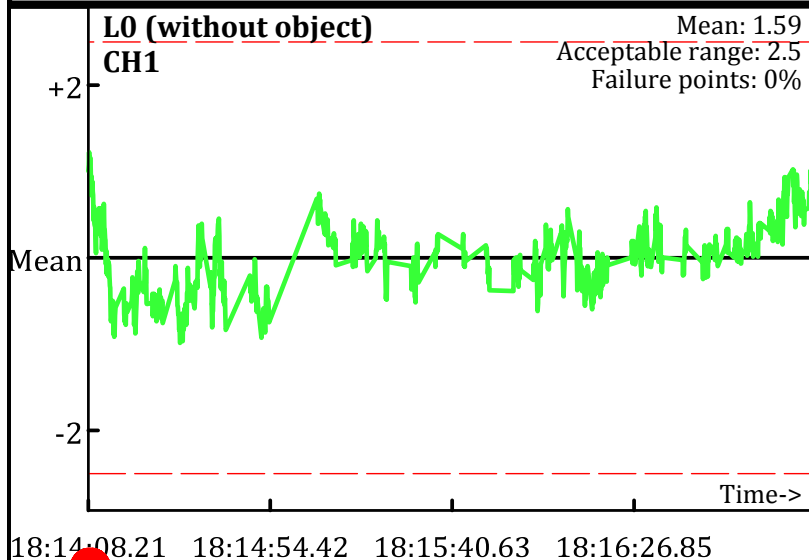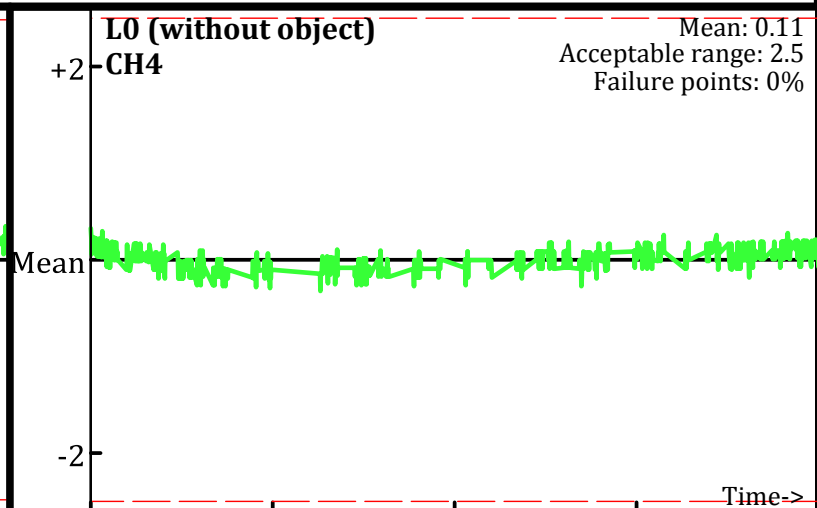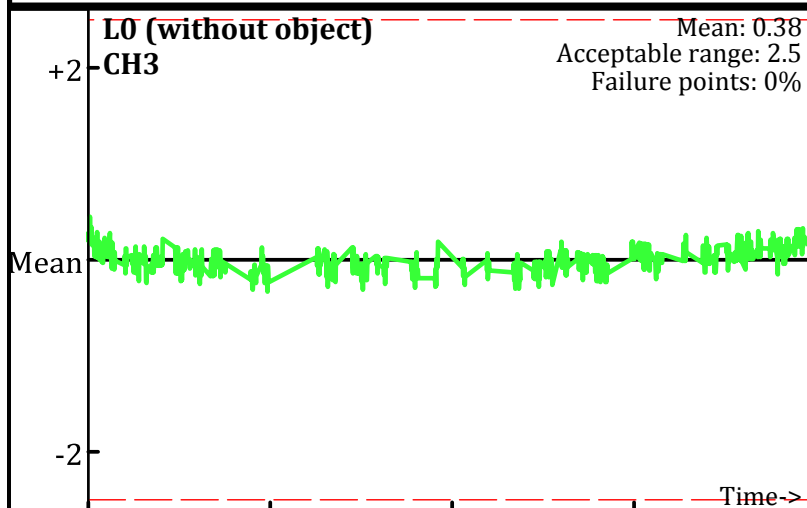Grid/Location: QC Area

● Outside range
— — Acceptable limits

PM test
Operator: PN
Date: 1/7/2010

L0 (without object)
CH3
Mean: 0.38
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH4
Mean: 0.11
Acceptable range: 2.5
Failure points: 0%

18:14:08.21　18:14:54.42　18:15:40.63　18:16:26.85

18:14:08.21　18:14:54.42　18:15:40.63　18:16:26.85

L1 (with object)
CH3
Mean: 44.58
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH4
Mean: 20.78
Acceptable range: 2.5
Failure points: 0%

18:18:32.92　18:19:20.37　18:20:07.82　18:20:55.28

18:18:32.92　18:19:20.37　18:20:07.82　18:20:55.28

L2 (without object)
CH3
Mean: 0.52
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH4
Mean: 0.17
Acceptable range: 2.5
Failure points: 0%

18:22:06.92　18:22:20.89　18:22:34.86　18:22:48.83　18:23

18:22:06.92　18:22:20.89　18:22:34.86　18:22:48.83　18:23

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
- - - Acceptable limits

AM test
Operator: PN & SH
Date: 1/11/2010

L0 (without object)
CH_1
Mean: -105.99
Acceptable range: 2.5
Failure points: 9.5%

Time->

12:54:56.67   12:55:35.84   12:56:15.02   12:56:54.19

L0 (without object)
CH_2
Mean: -2.04
Acceptable range: 2.5
Failure points: 0%

Time->

12:54:56.67   12:55:35.84   12:56:15.02   12:56:54.19

L1 (with object)
CH_1
Mean: -8.19
Acceptable range: 2.5
Failure points: 0%

Time->

13:00:25.36   13:01:05.78   13:01:46.21   13:02:26.64   13:03

L1 (with object)
CH_2
Mean: 58.78
Acceptable range: 2.5
Failure points: 0%

Time->

13:00:25.36   13:01:05.78   13:01:46.21   13:02:26.64   13:03

L2 (without object)
CH_1
Mean: -107.41
Acceptable range: 2.5
Failure points: 0%

Time->

13:03:39.17   13:04:00.62   13:04:22.07   13:04:43.52   13:05

L2 (without object)
CH_2
Mean: -2.49
Acceptable range: 2.5
Failure points: 0%

Time->

13:03:39.17   13:04:00.62   13:04:22.07   13:04:43.52   13:05

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & SH
Date: 1/11/2010

L0 (without object)
CH_3
Mean: 5.22
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:54:56.67   12:55:35.84   12:56:15.02   12:56:54.19

L0 (without object)
CH_4
Mean: -2.21
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:54:56.67   12:55:35.84   12:56:15.02   12:56:54.19

L1 (with object)
CH_3
Mean: 36.39
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:00:25.36   13:01:05.78   13:01:46.21   13:02:26.64   13:03

L1 (with object)
CH_4
Mean: 11.17
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:00:25.36   13:01:05.78   13:01:46.21   13:02:26.64   13:03

L2 (without object)
CH_3
Mean: 5.12
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:03:39.17   13:04:00.62   13:04:22.07   13:04:43.52   13:05

L2 (without object)
CH_4
Mean: -2.3
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:03:39.17   13:04:00.62   13:04:22.07   13:04:43.52   13:05

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
- - - Acceptable limits

AM test
Operator: PN & SH
Date: 1/11/2010
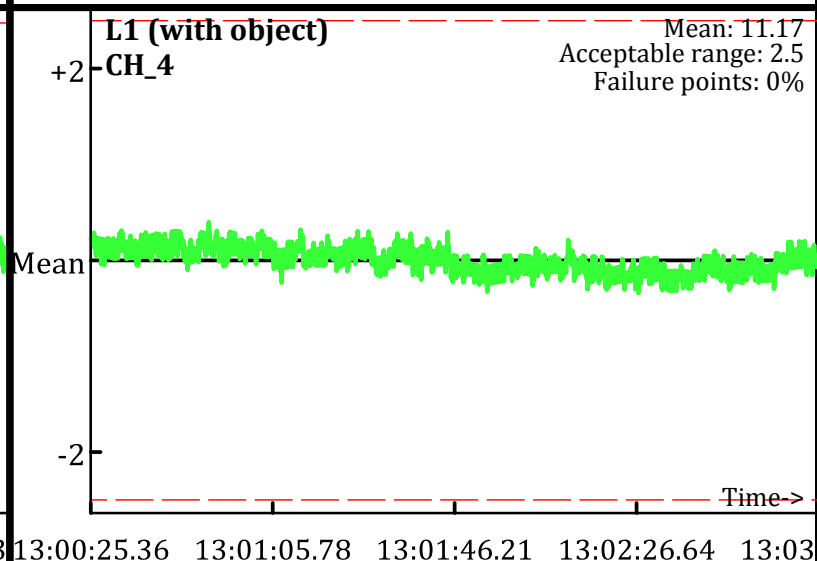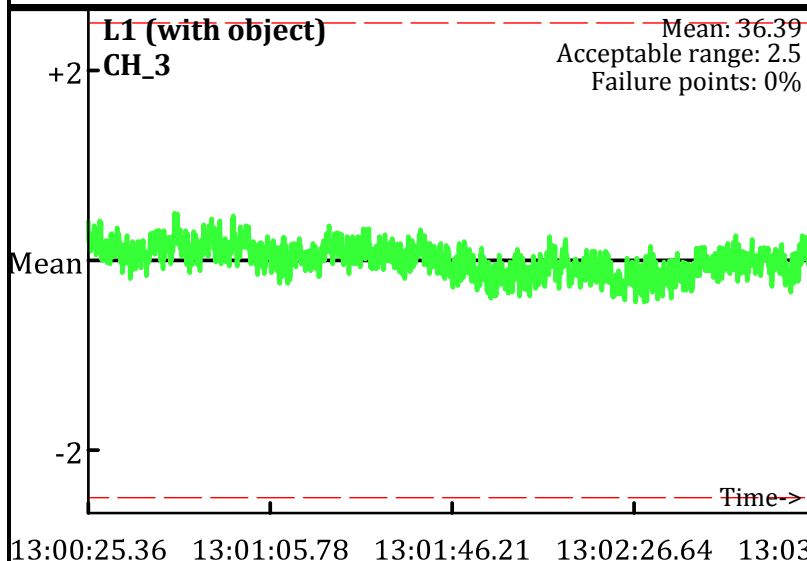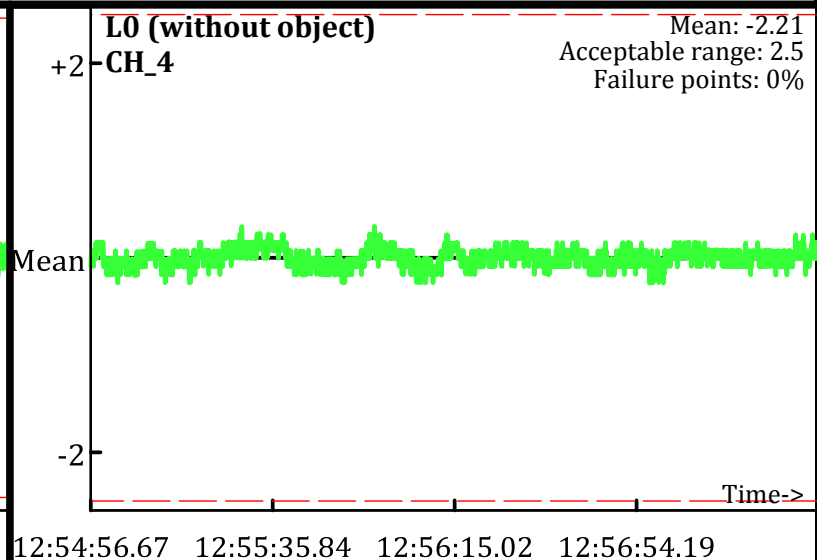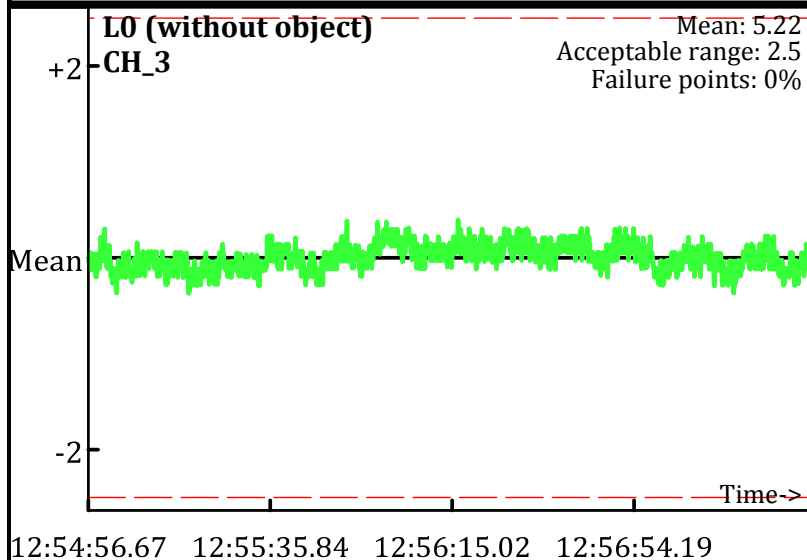
L0.1 (without object)
CH_1
Mean: -69.56
Acceptable range: 2.5
Failure points: 3.7%

L0.1 (without object)
CH_2
Mean: 6.71
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_1
Mean: 126.62
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_2
Mean: 145.68
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_1
Mean: -68.33
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_2
Mean: 7.16
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
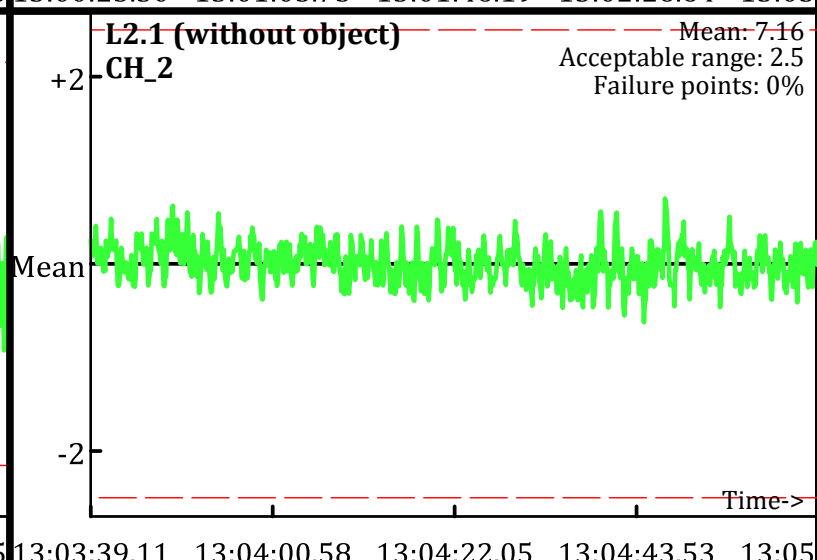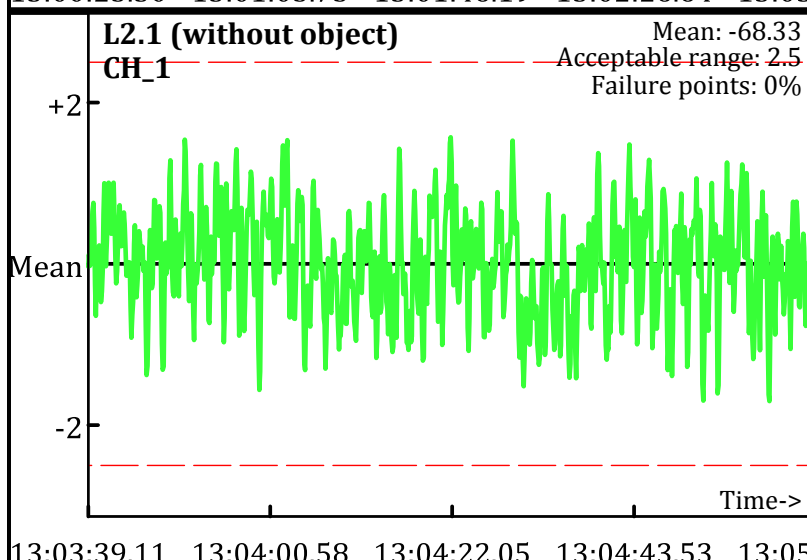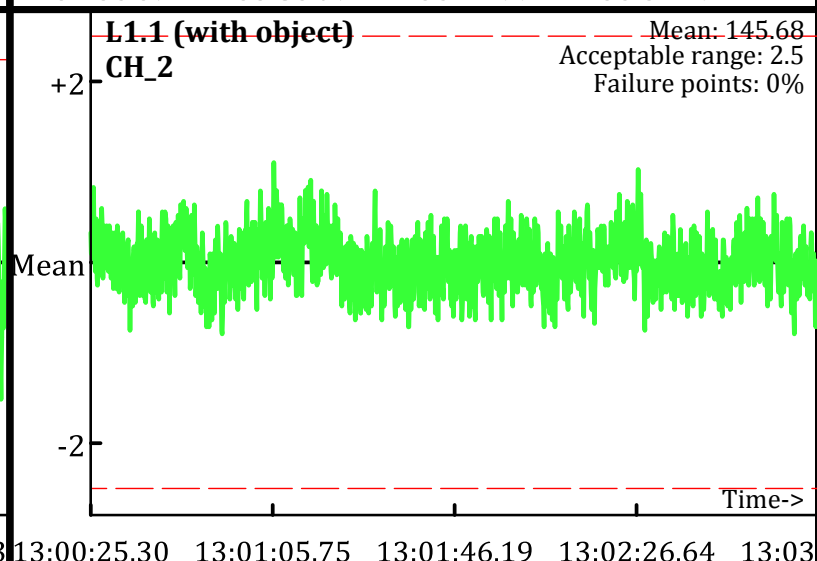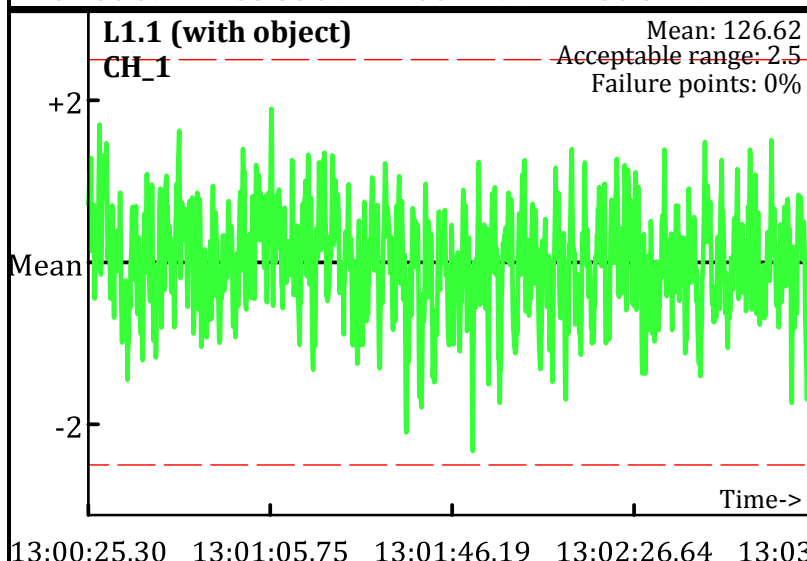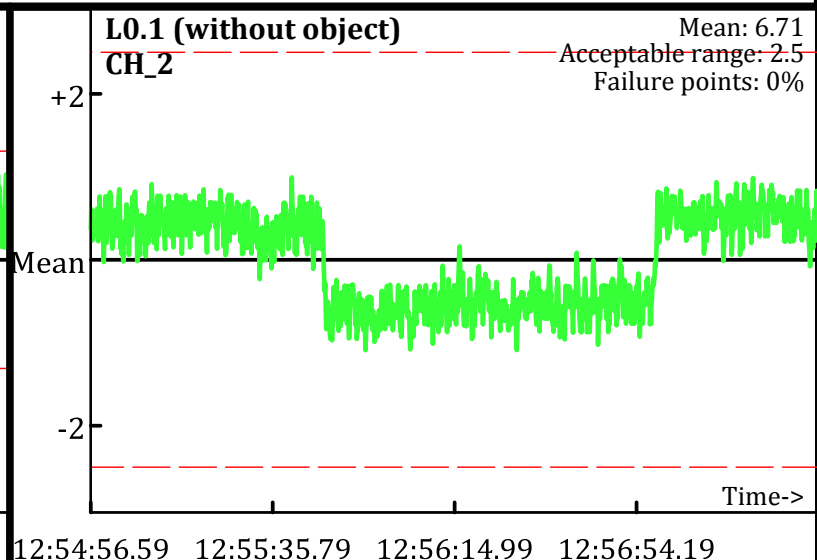- - - Acceptable limits

AM test
Operator: PN & SH
Date: 1/11/2010

L0.1 (without object)
CH_3
Mean: 10.62
Acceptable range: 2.5
Failure points: 0%

12:54:56.59   12:55:35.79   12:56:14.99   12:56:54.19

L0.1 (without object)
CH_4
Mean: 1.72
Acceptable range: 2.5
Failure points: 0%

12:54:56.59   12:55:35.79   12:56:14.99   12:56:54.19

L1.1 (with object)
CH_3
Mean: 93.76
Acceptable range: 2.5
Failure points: 0%

13:00:25.30   13:01:05.75   13:01:46.19   13:02:26.64   13:03

L1.1 (with object)
CH_4
Mean: 44.13
Acceptable range: 2.5
Failure points: 0%

13:00:25.30   13:01:05.75   13:01:46.19   13:02:26.64   13:03

L2.1 (without object)
CH_3
Mean: 10.74
Acceptable range: 2.5
Failure points: 0%

13:03:39.11   13:04:00.58   13:04:22.05   13:04:43.53   13:05

L2.1 (without object)
CH_4
Mean: 1.75
Acceptable range: 2.5
Failure points: 0%
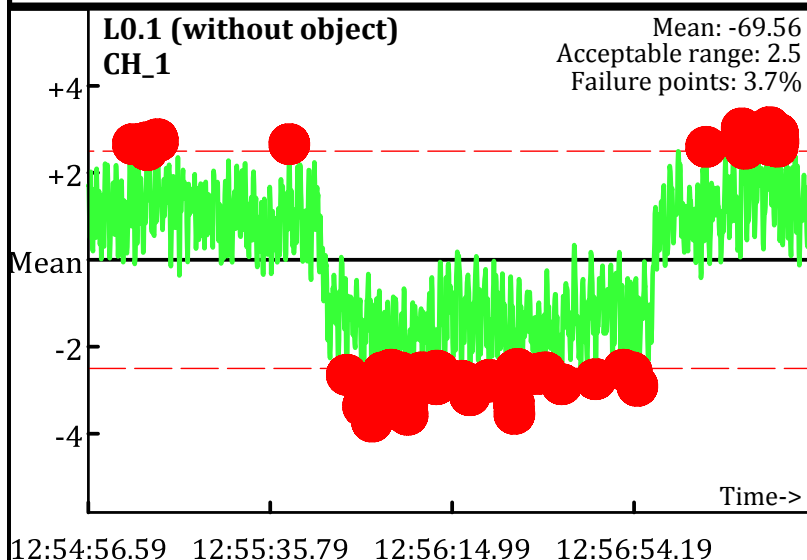
13:03:39.11   13:04:00.58   13:04:22.05   13:04:43.53   13:05

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
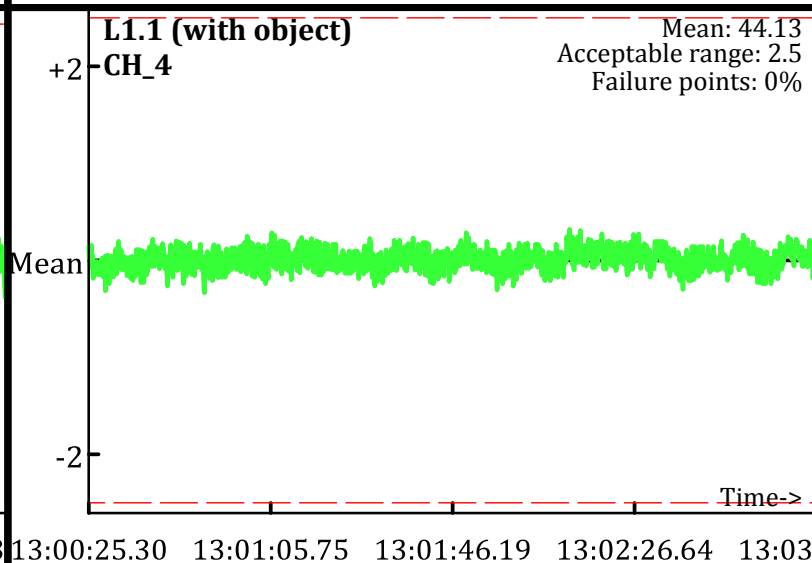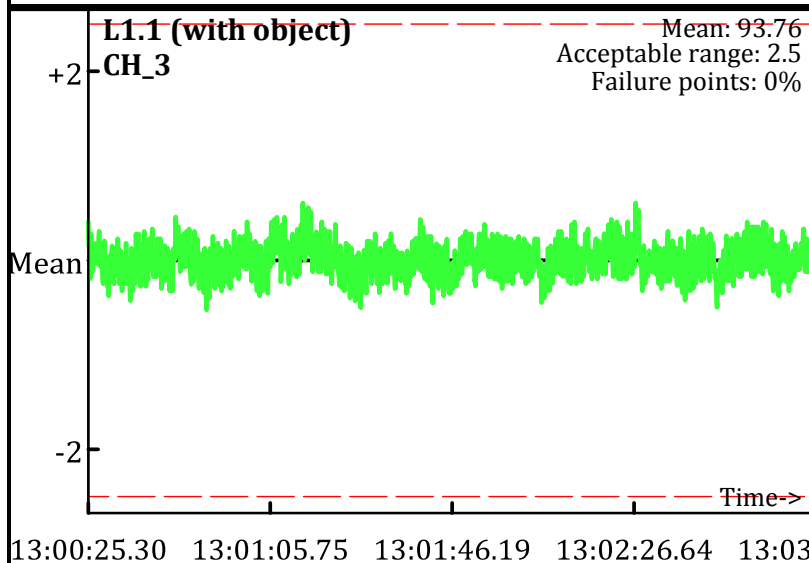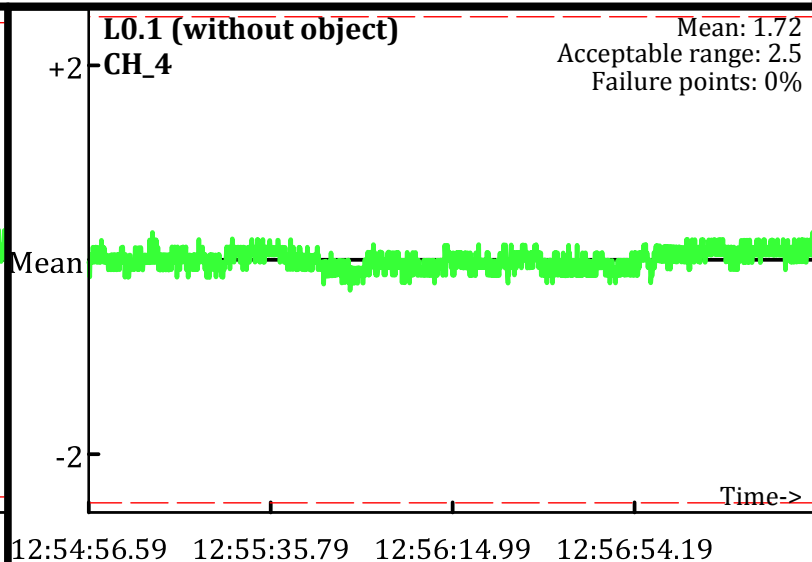Grid/Location: QC Area

● Outside range
- - - Acceptable limits

AM test
Operator: PN & SH
Date: 1/11/2010

L0.2 (without object)
CH_1
Mean: -50
Acceptable range: 2.5
Failure points: 0%

L0.2 (without object)
CH_2
Mean: 6.35
Acceptable range: 2.5
Failure points: 0%

12:54:56.61   12:55:35.81   12:56:15.02   12:56:54.22

L1.2 (with object)
CH_1
Mean: 39.11
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_2
Mean: 61.05
Acceptable range: 2.5
Failure points: 0%

13:00:25.31   13:01:05.77   13:01:46.22   13:02:26.67

L2.2 (without object)
CH_1
Mean: -50.47
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_2
Mean: 6.25
Acceptable range: 2.5
Failure points: 0%

13:03:39.11   13:04:00.59   13:04:22.06   13:04:43.54

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
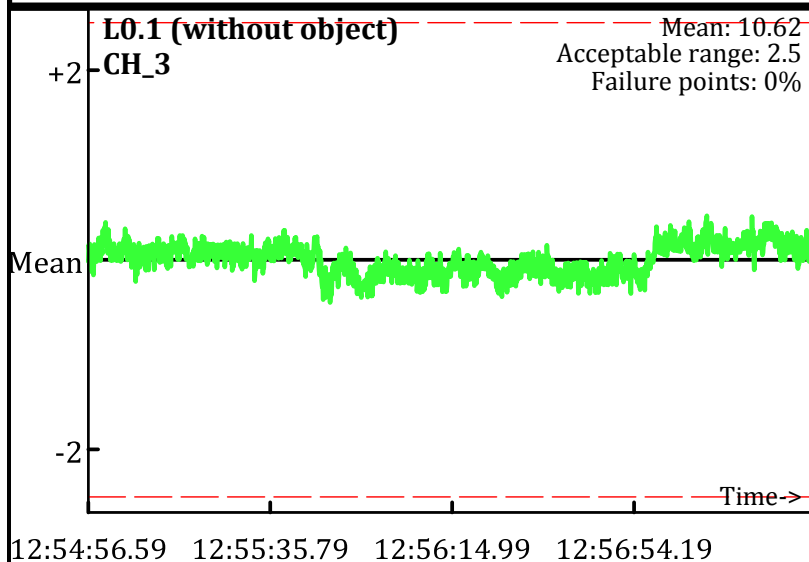Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
— — Acceptable limits
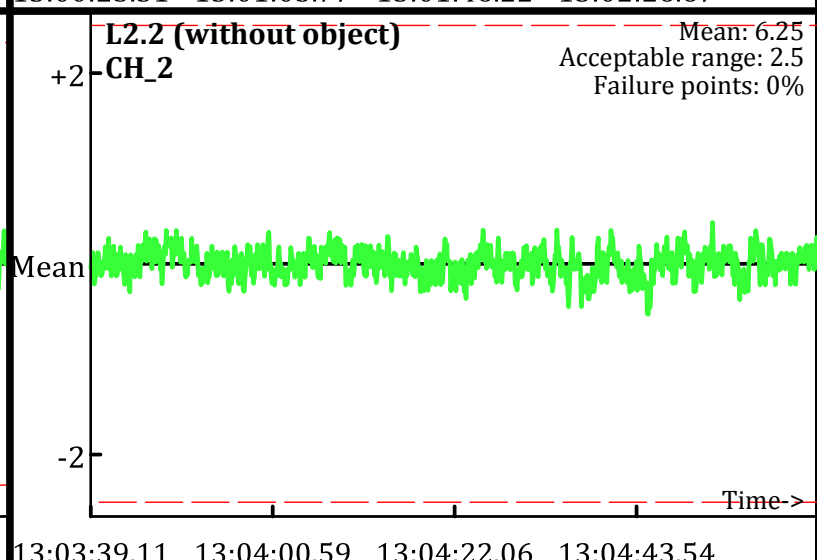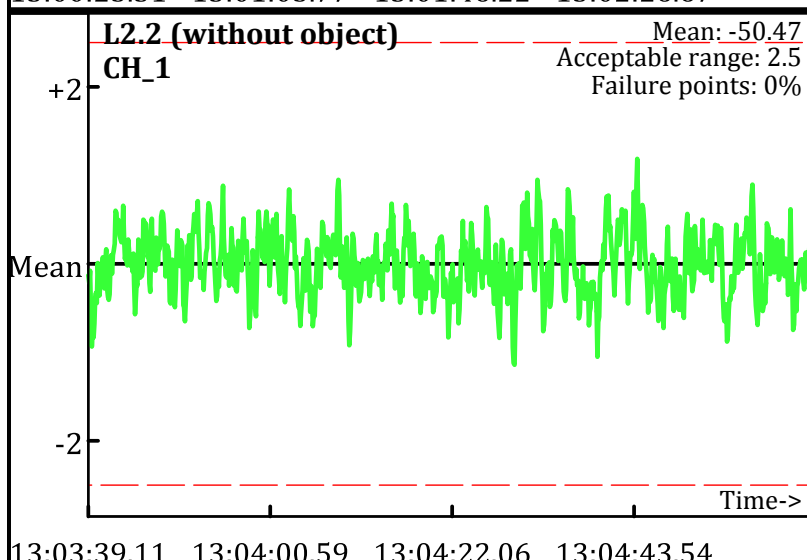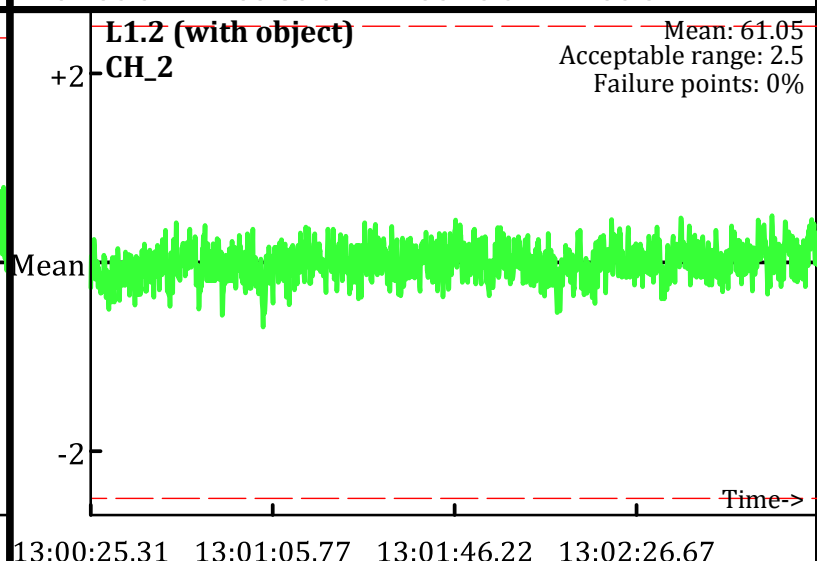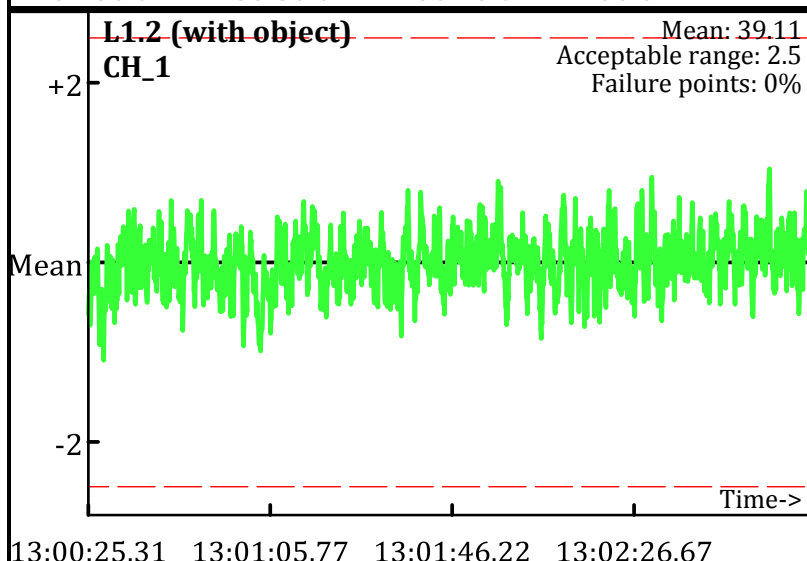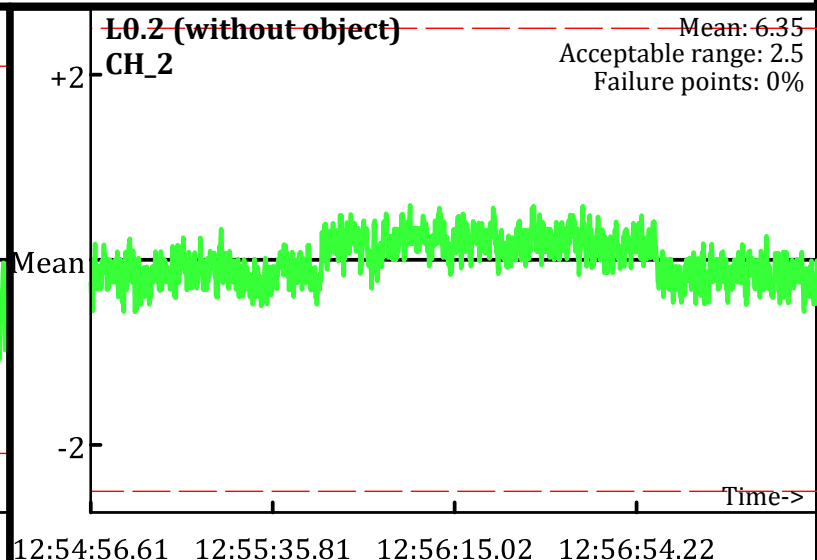
AM test
Operator: PN & SH
Date: 1/11/2010

L0.2 (without object)
CH_3
Mean: 7.03
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

12:54:56.61   12:55:35.81   12:56:15.02   12:56:54.22

L0.2 (without object)
CH_4
Mean: -0.26
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

12:54:56.61   12:55:35.81   12:56:15.02   12:56:54.22

L1.2 (with object)
CH_3
Mean: 35.17
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

13:00:25.31   13:01:05.77   13:01:46.22   13:02:26.67

L1.2 (with object)
CH_4
Mean: 11.78
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

13:00:25.31   13:01:05.77   13:01:46.22   13:02:26.67

L2.2 (without object)
CH_3
Mean: 7.08
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

13:03:39.11   13:04:00.59   13:04:22.06   13:04:43.54

L2.2 (without object)
CH_4
Mean: -0.22
Acceptable range: 2.5
Failure points: 0%

+2

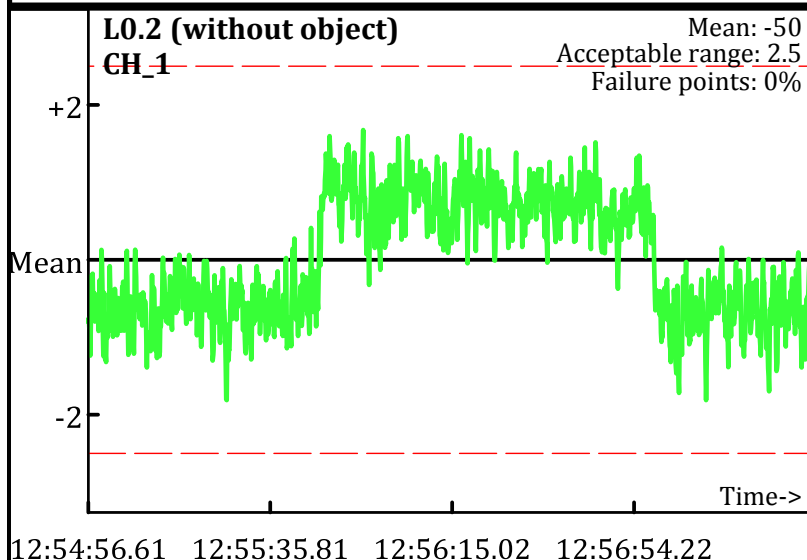Mean

-2

Time->

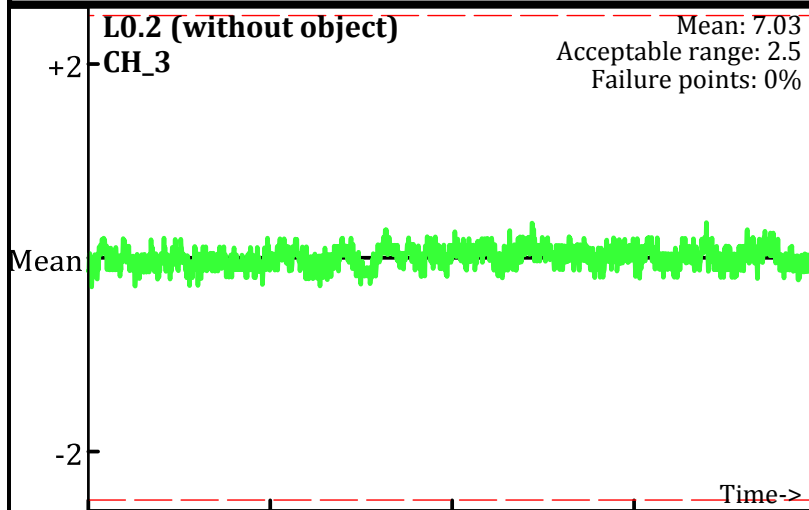13:03:39.11   13:04:00.59   13:04:22.06   13:04:43.54
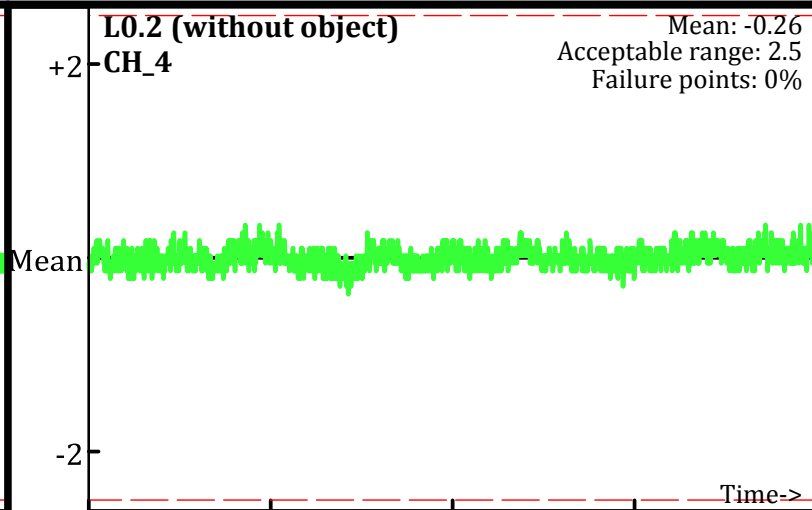
Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

PM test
Operator: PN & SH
Date: 1/11/2010

L5 (without object) CH_1
Mean: -115.01
Acceptable range: 2.5
Failure points: 0%

16:32:06.00   16:32:52.17   16:33:38.34   16:34:24.52

L5 (without object) CH_2
Mean: -6.15
Acceptable range: 2.5
Failure points: 0%

16:32:06.00   16:32:52.17   16:33:38.34   16:34:24.52

L6 (with object) CH_1
Mean: -15.63
Acceptable range: 2.5
Failure points: 0%

16:36:40.69   16:37:46.61   16:38:52.54   16:39:58.46

L6 (with object) CH_2
Mean: 55.97
Acceptable range: 2.5
Failure points: 0%

16:36:40.69   16:37:46.61   16:38:52.54   16:39:58.46

L7 (without object) CH_1
Mean: -116.93
Acceptable range: 2.5
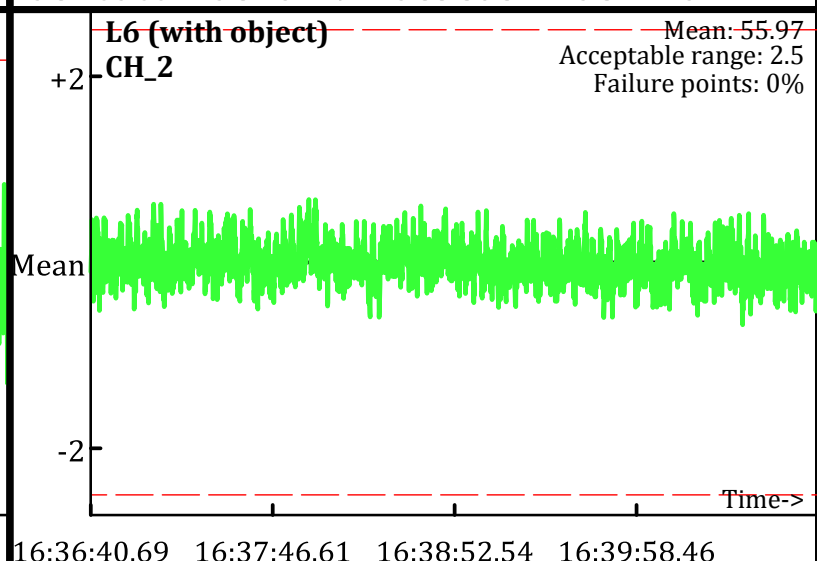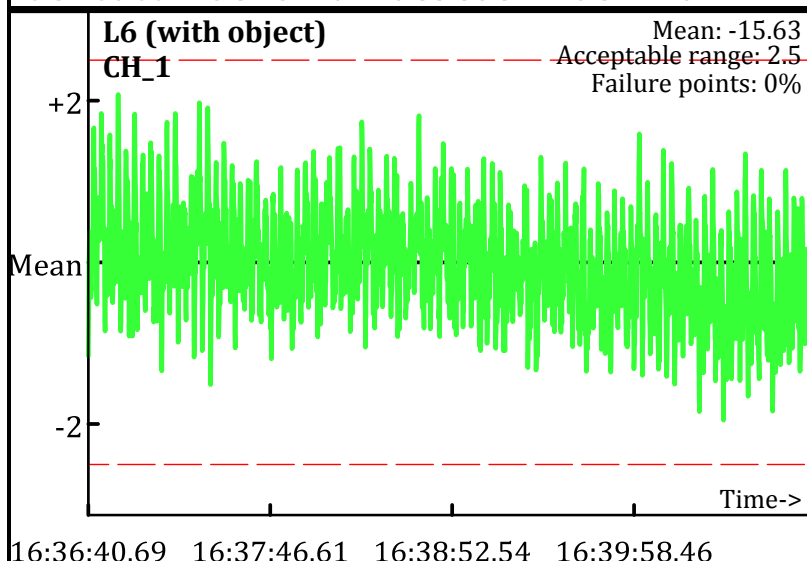Failure points: 0%

16:41:43.39   16:42:00.36   16:42:17.34   16:42:34.31

L7 (without object) CH_2
Mean: -6.61
Acceptable range: 2.5
Failure points: 0%

16:41:43.39   16:42:00.36   16:42:17.34   16:42:34.31

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L5 L6 L7

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
— — — Acceptable limits

PM test
Operator: PN & SH
Date: 1/11/2010

L5 (without object)
CH_3
Mean: 4.03
Acceptable range: 2.5
Failure points: 0%

16:32:06.00 16:32:52.17 16:33:38.34 16:34:24.52

L5 (without object)
CH_4
Mean: -2.67
Acceptable range: 2.5
Failure points: 0%

16:32:06.00 16:32:52.17 16:33:38.34 16:34:24.52

L6 (with object)
CH_3
Mean: 36.03
Acceptable range: 2.5
Failure points: 0%

16:36:40.69 16:37:46.61 16:38:52.54 16:39:58.46

L6 (with object)
CH_4
Mean: 11.17
Acceptable range: 2.5
Failure points: 0%

16:36:40.69 16:37:46.61 16:38:52.54 16:39:58.46

L7 (without object)
CH_3
Mean: 3.95
Acceptable range: 2.5
Failure points: 0%

16:41:43.39 16:42:00.36 16:42:17.34 16:42:34.31

L7 (without object)
CH_4
Mean: -2.7
Acceptable range: 2.5
Failure points: 0%

16:41:43.39 16:42:00.36 16:42:17.34 16:42:34.31

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L5 L6 L7

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

PM test
Operator: PN & SH
Date: 1/11/2010
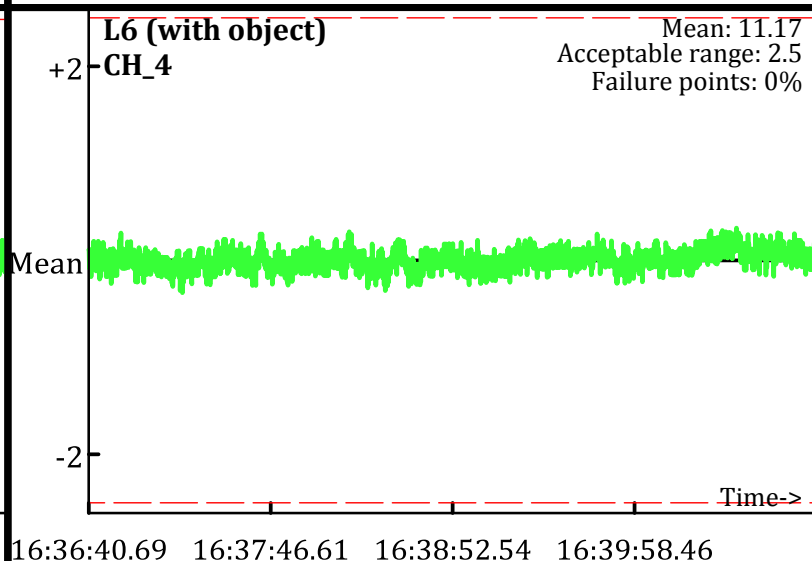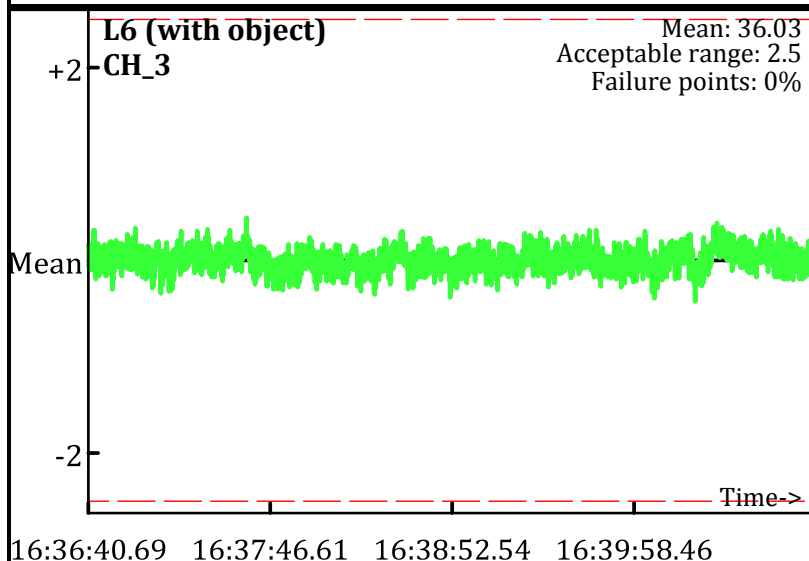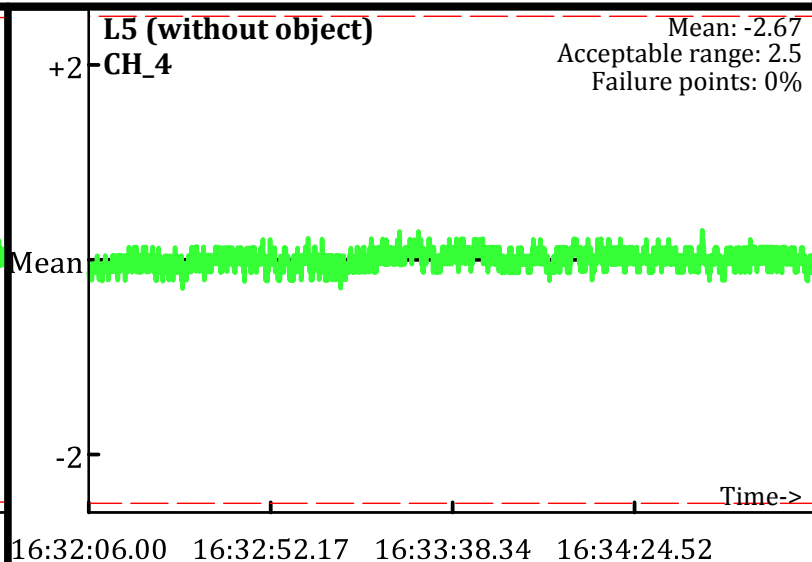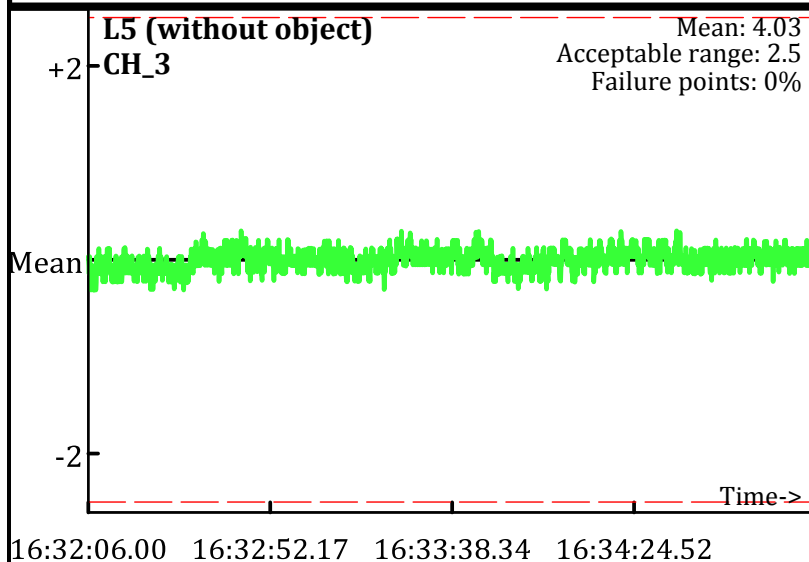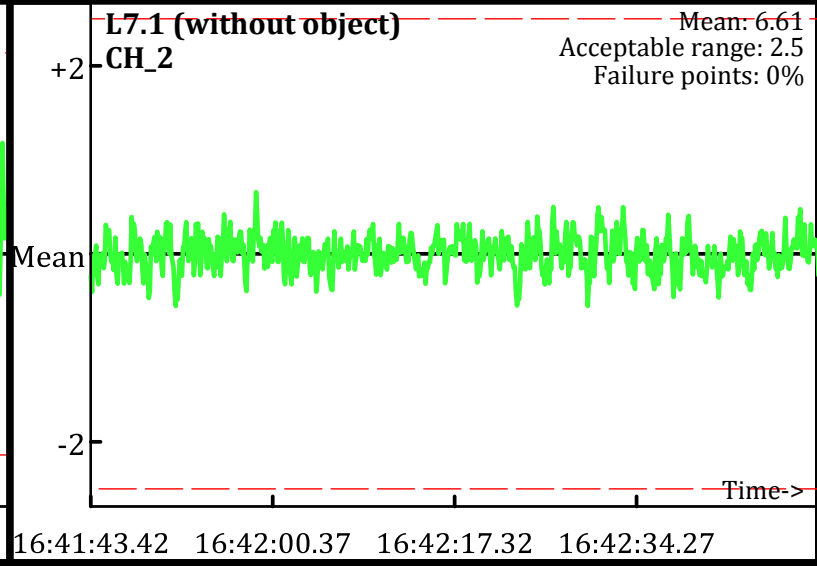
L5.1 (without object)
CH_1
Mean: -67.56
Acceptable range: 2.5
Failure points: 0%

16:32:05.92   16:32:52.12   16:33:38.32   16:34:24.52

L5.1 (without object)
CH_2
Mean: 6.61
Acceptable range: 2.5
Failure points: 0%

16:32:05.92   16:32:52.12   16:33:38.32   16:34:24.52

L6.1 (with object)
CH_1
Mean: 131.57
Acceptable range: 2.5
Failure points: 0.0758%

16:36:40.72   16:37:46.62   16:38:52.52   16:39:58.43

L6.1 (with object)
CH_2
Mean: 148.62
Acceptable range: 2.5
Failure points: 0%

16:36:40.72   16:37:46.62   16:38:52.52   16:39:58.43

L7.1 (without object)
CH_1
Mean: -68.03
Acceptable range: 2.5
Failure points: 0%

16:41:43.42   16:42:00.37   16:42:17.32   16:42:34.27

L7.1 (without object)
CH_2
Mean: 6.61
Acceptable range: 2.5
Failure points: 0%

16:41:43.42   16:42:00.37   16:42:17.32   16:42:34.27

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L5.1 L6.1 L7.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

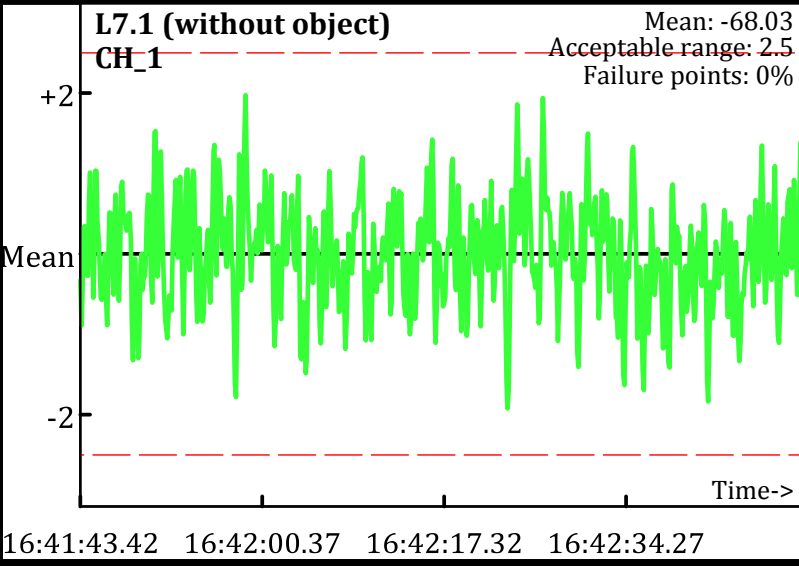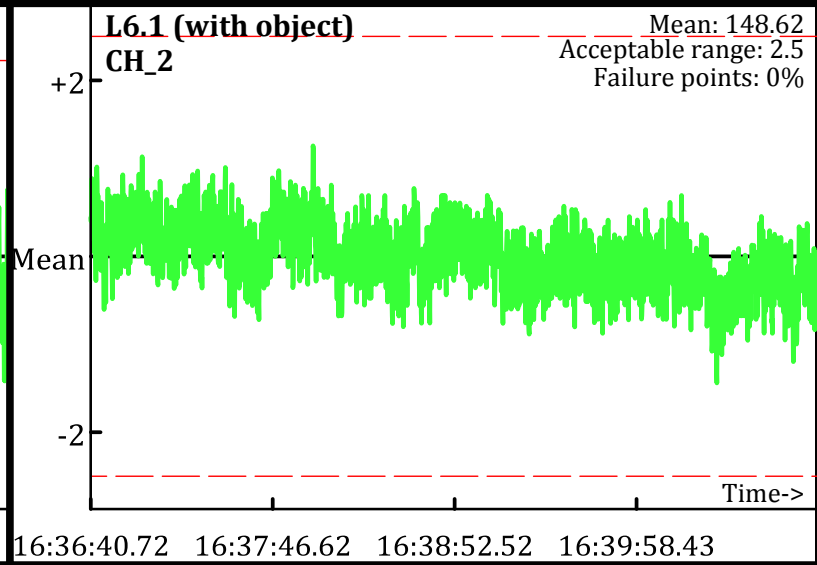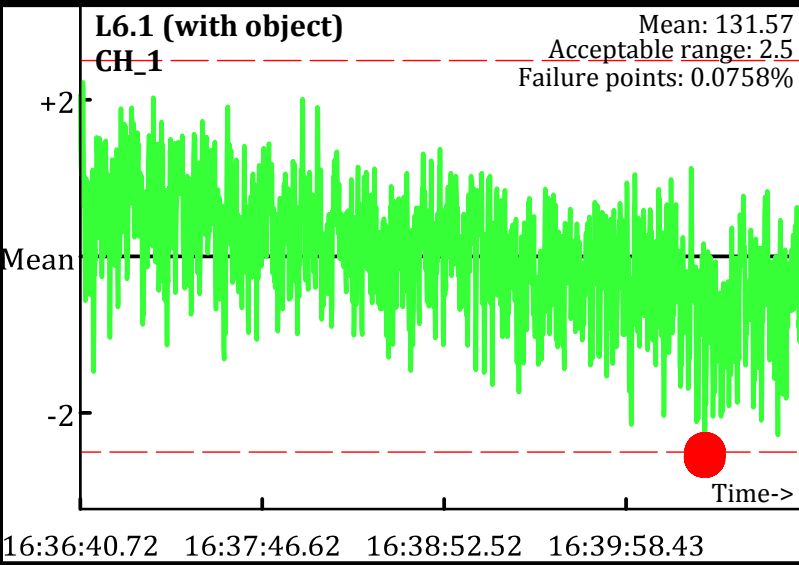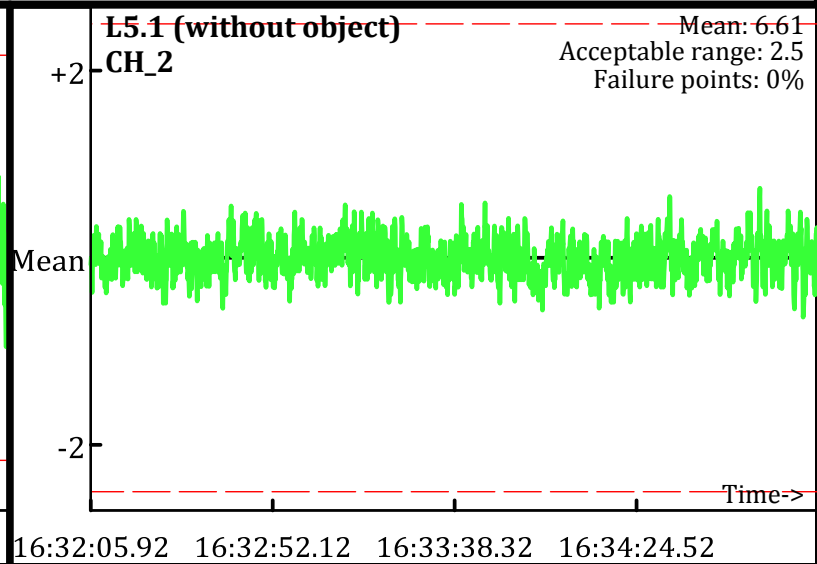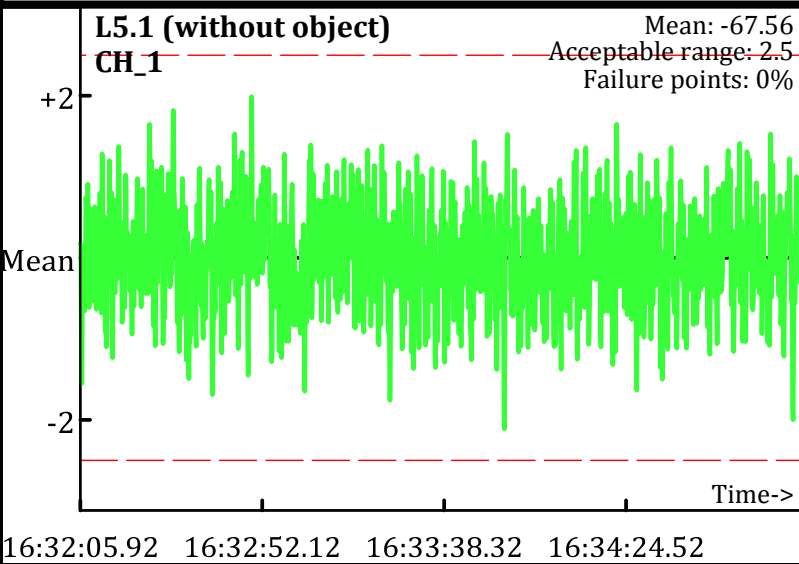PM test
Operator: PN & SH
Date: 1/11/2010

L5.1 (without object)
CH_3
Mean: 10.18
Acceptable range: 2.5
Failure points: 0%

16:32:05.92   16:32:52.12   16:33:38.32   16:34:24.52

L5.1 (without object)
CH_4
Mean: 1.24
Acceptable range: 2.5
Failure points: 0%

16:32:05.92   16:32:52.12   16:33:38.32   16:34:24.52

L6.1 (with object)
CH_3
Mean: 95.5
Acceptable range: 2.5
Failure points: 0%

16:36:40.72   16:37:46.62   16:38:52.52   16:39:58.43

L6.1 (with object)
CH_4
Mean: 44.88
Acceptable range: 2.5
Failure points: 0%

16:36:40.72   16:37:46.62   16:38:52.52   16:39:58.43

L7.1 (without object)
CH_3
Mean: 10.24
Acceptable range: 2.5
Failure points: 0%

16:41:43.42   16:42:00.37   16:42:17.32   16:42:34.27

L7.1 (without object)
CH_4
Mean: 1.25
Acceptable range: 2.5
Failure points: 0%

16:41:43.42   16:42:00.37   16:42:17.32   16:42:34.27

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
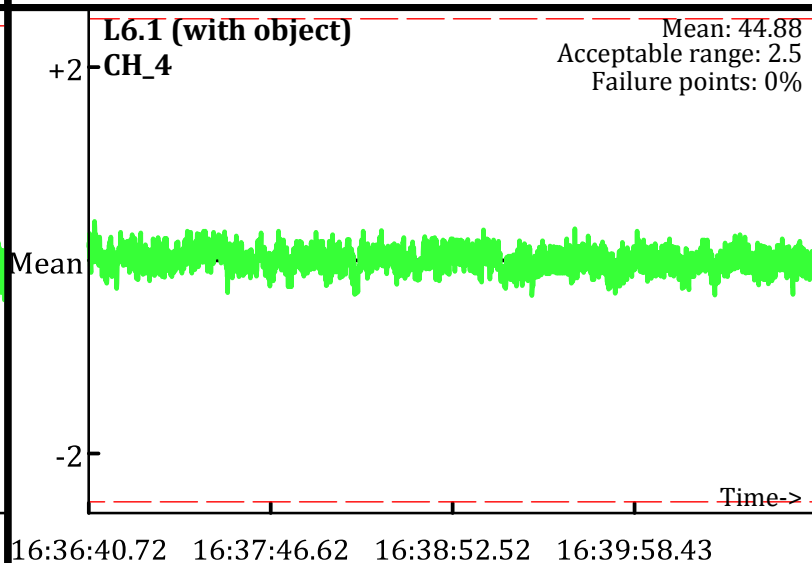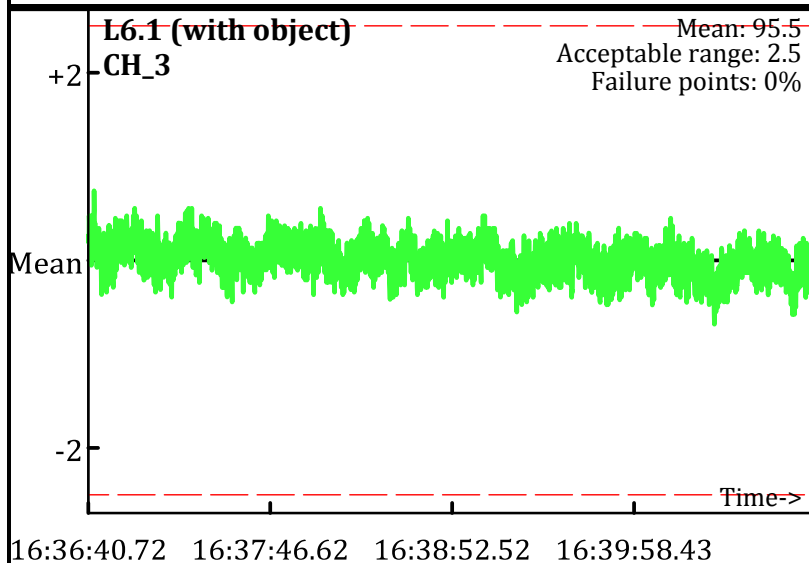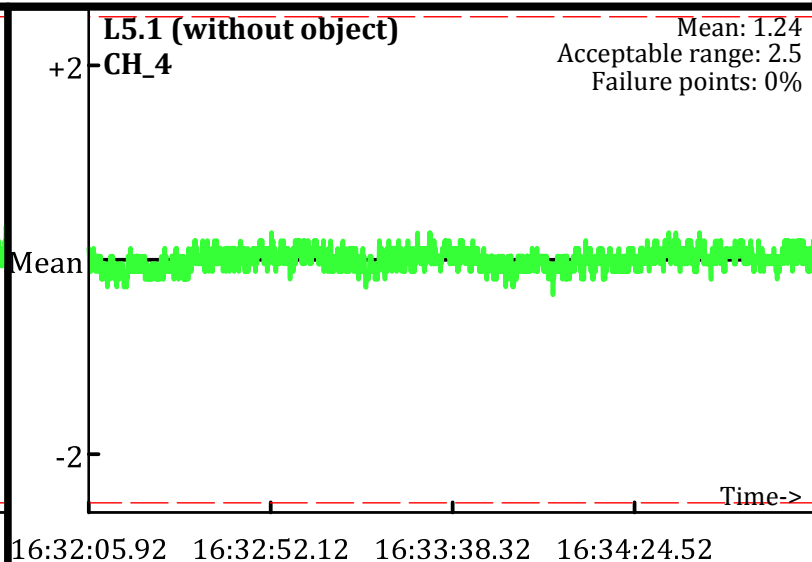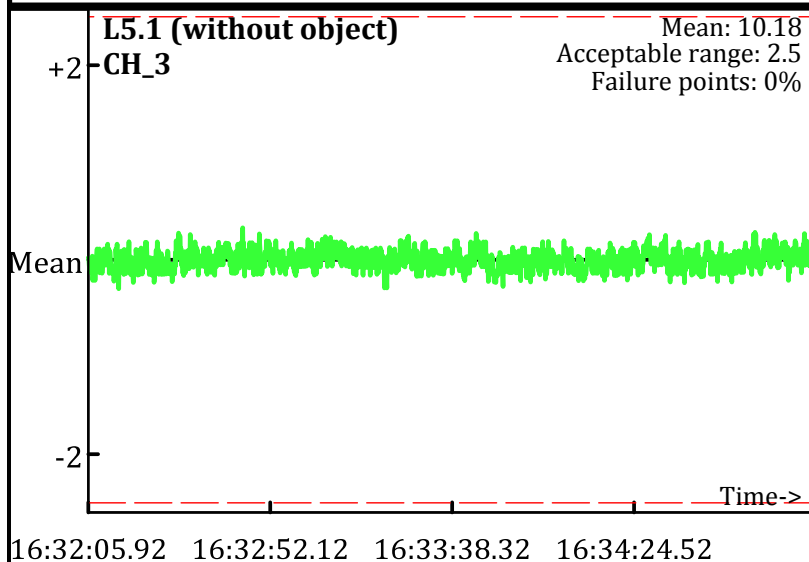Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits

PM test
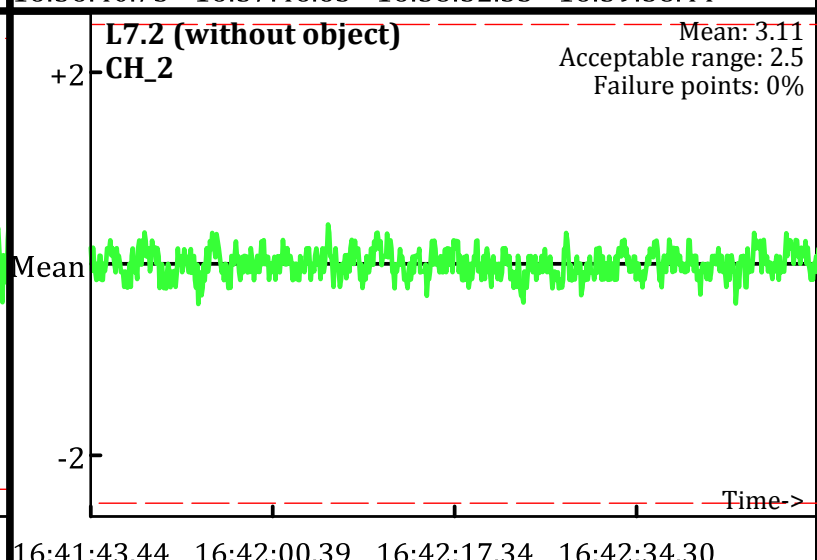Operator: PN & SH
Date: 1/11/2010

L5.2 (without object)
CH_1
Mean: -53.93
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_2
Mean: 3.16
Acceptable range: 2.5
Failure points: 0%

16:32:05.94   16:32:52.12   16:33:38.30   16:34:24.48   16:35

L6.2 (with object)
CH_1
Mean: 37.28
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_2
Mean: 59.69
Acceptable range: 2.5
Failure points: 0%

16:36:40.75   16:37:46.65   16:38:52.55   16:39:58.44

L7.2 (without object)
CH_1
Mean: -54.44
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_2
Mean: 3.11
Acceptable range: 2.5
Failure points: 0%

16:41:43.44   16:42:00.39   16:42:17.34   16:42:34.30

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
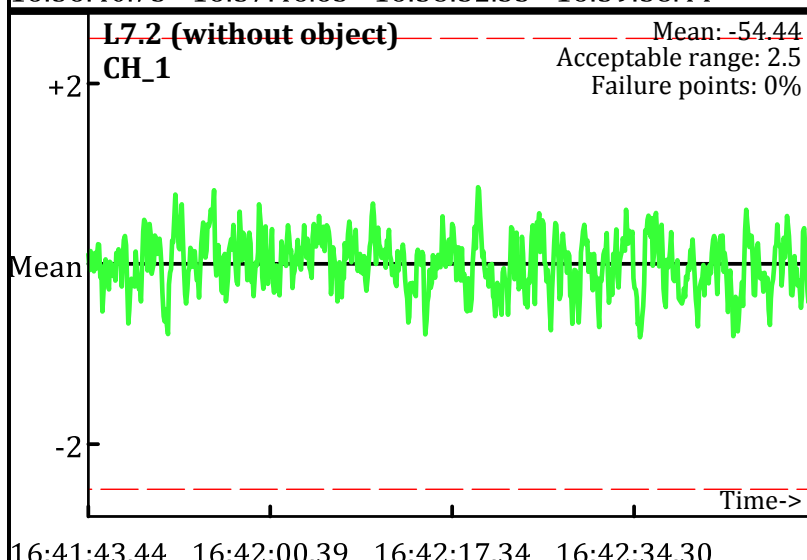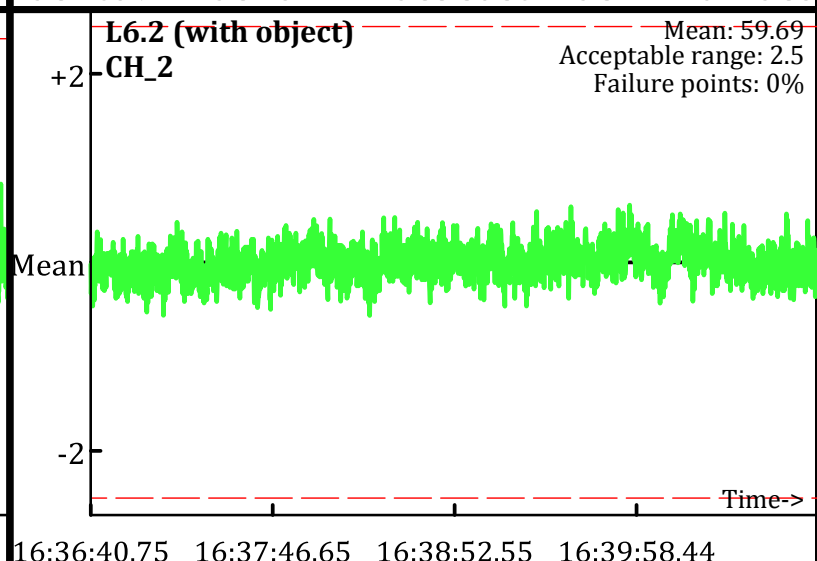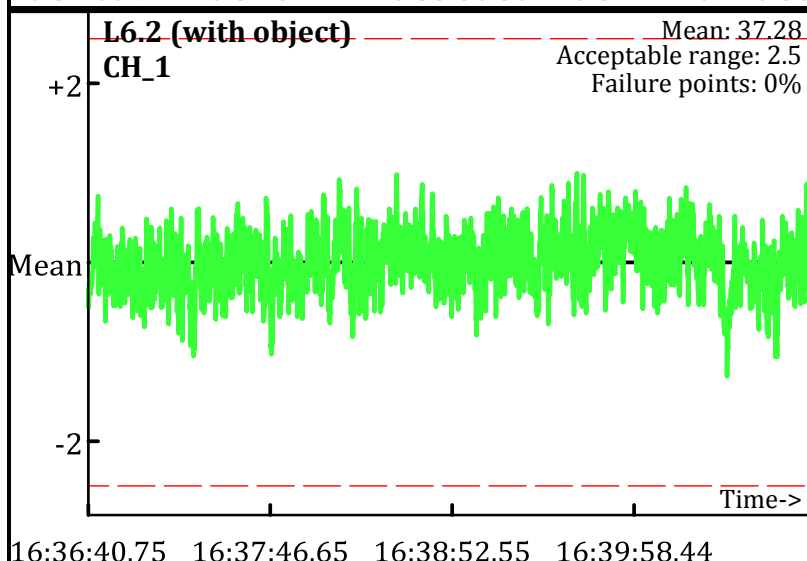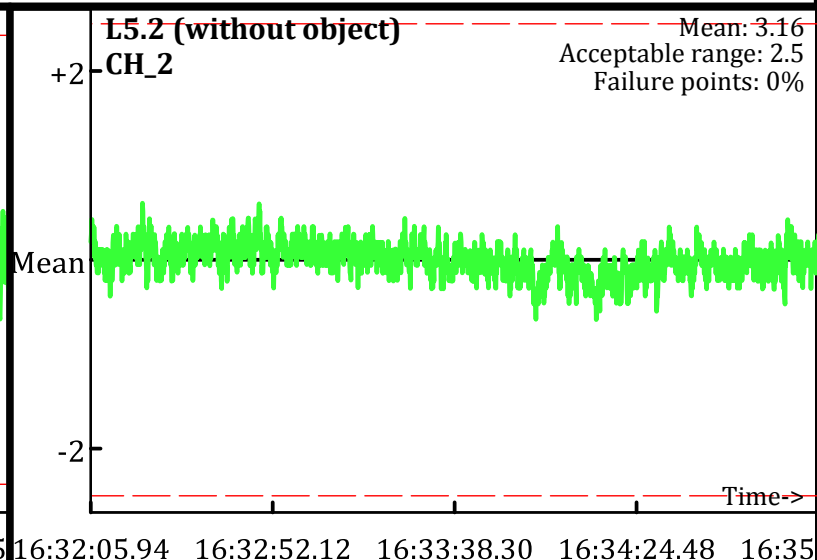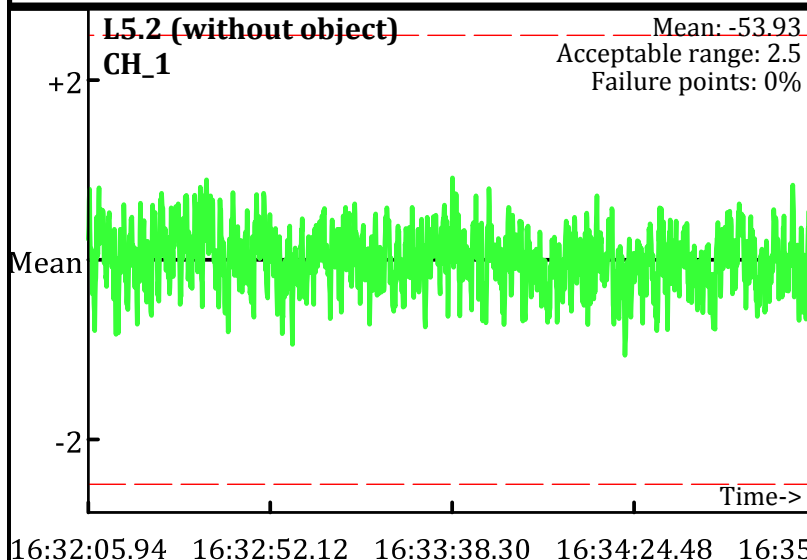Operator: PN & SH
Date: 1/11/2010

L5.2 (without object)
CH_3
Mean: 5.05
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:32:05.94   16:32:52.12   16:33:38.30   16:34:24.48   16:35

L5.2 (without object)
CH_4
Mean: -1.45
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:32:05.94   16:32:52.12   16:33:38.30   16:34:24.48   16:35

L6.2 (with object)
CH_3
Mean: 34.45
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:36:40.75   16:37:46.65   16:38:52.55   16:39:58.44

L6.2 (with object)
CH_4
Mean: 11.27
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:36:40.75   16:37:46.65   16:38:52.55   16:39:58.44

L7.2 (without object)
CH_3
Mean: 5.2
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:41:43.44   16:42:00.39   16:42:17.34   16:42:34.30

L7.2 (without object)
CH_4
Mean: -1.33
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
16:41:43.44   16:42:00.39   16:42:17.34   16:42:34.30

Database: D:\Projects_QCReports_Ord_Data\011110\QC\011110_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
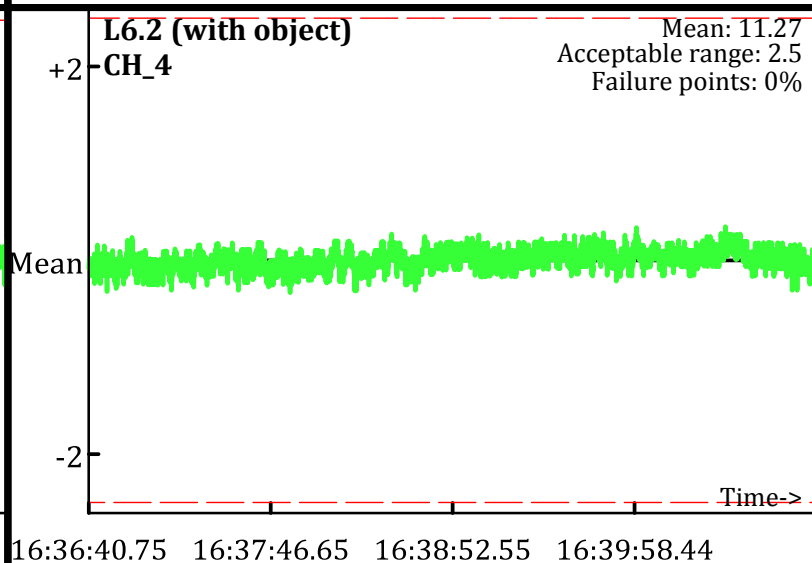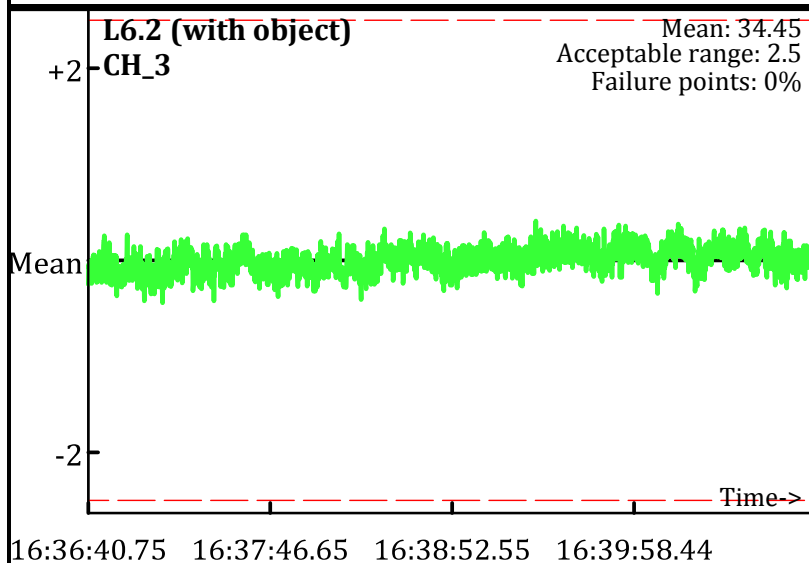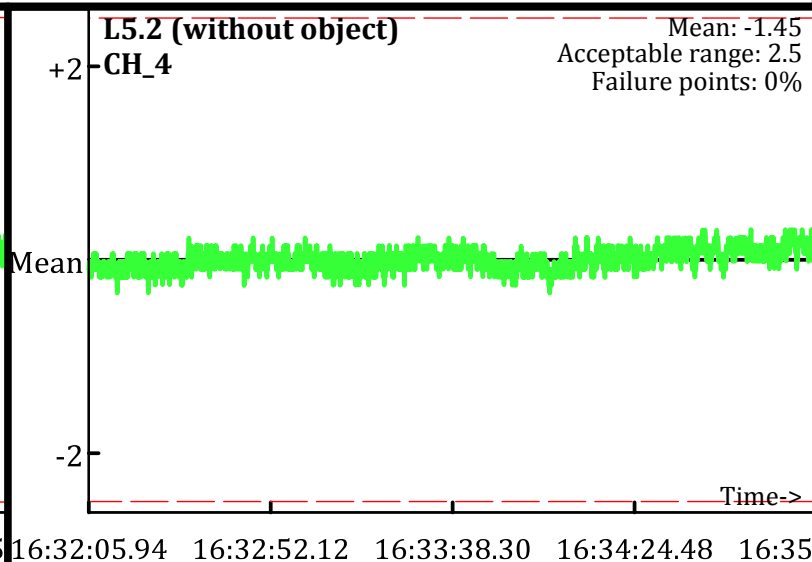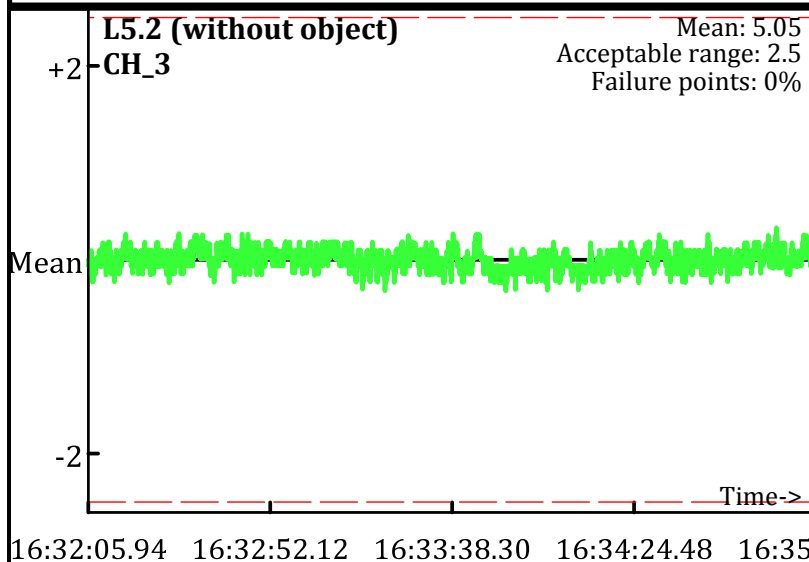Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
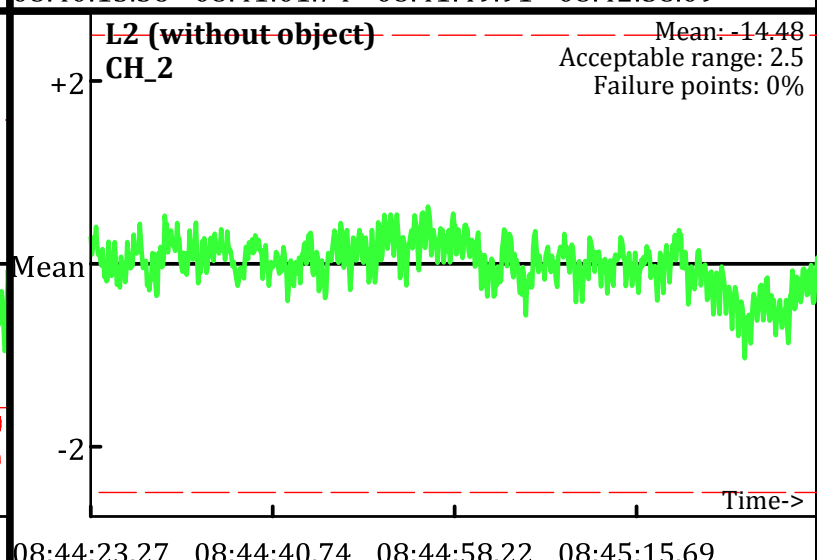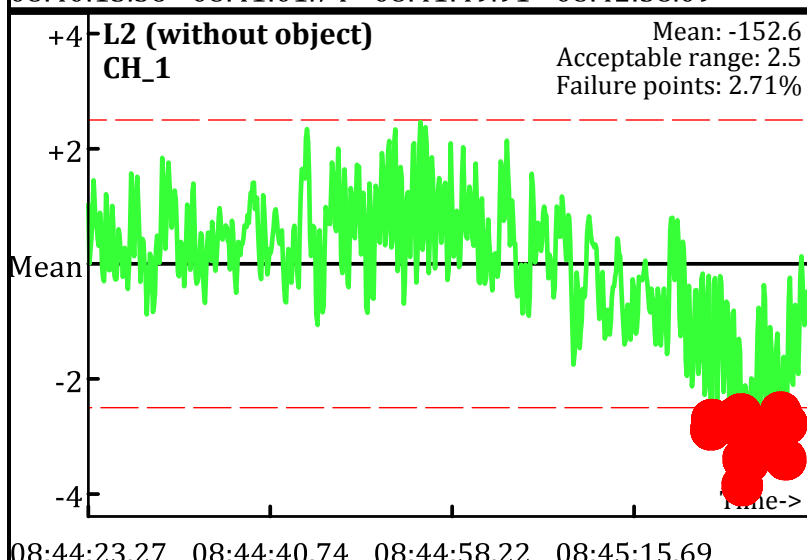Operator: PN & SH
Date: 1/12/2010

L0 (without object)
CH_1
Mean: -161.44
Acceptable range: 2.5
Failure points: 3.16%

L0 (without object)
CH_2
Mean: -17.57
Acceptable range: 2.5
Failure points: 0%

08:35:50.76   08:36:39.71   08:37:28.66   08:38:17.61

L1 (with object)
CH_1
Mean: -57.08
Acceptable range: 2.5
Failure points: 4.72%

L1 (with object)
CH_2
Mean: 44.92
Acceptable range: 2.5
Failure points: 0%

08:40:13.56   08:41:01.74   08:41:49.91   08:42:38.09

L2 (without object)
CH_1
Mean: -152.6
Acceptable range: 2.5
Failure points: 2.71%

L2 (without object)
CH_2
Mean: -14.48
Acceptable range: 2.5
Failure points: 0%

08:44:23.27   08:44:40.74   08:44:58.22   08:45:15.69

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
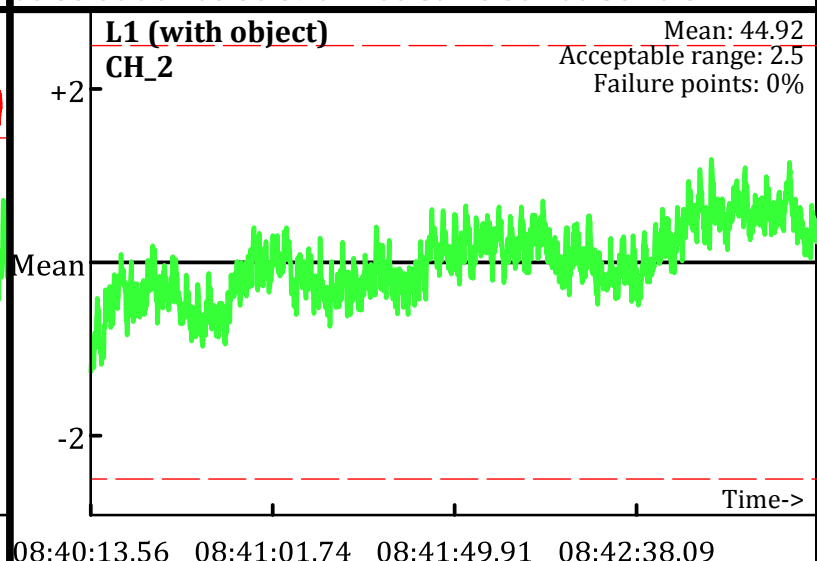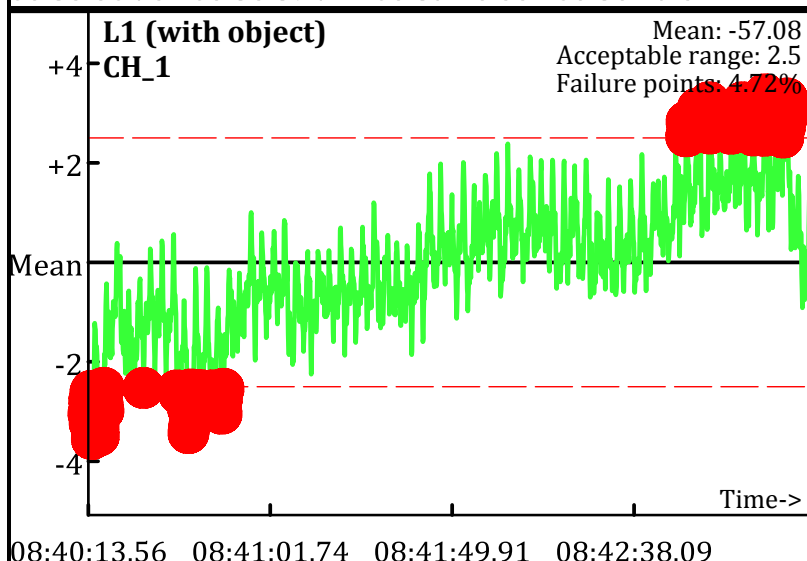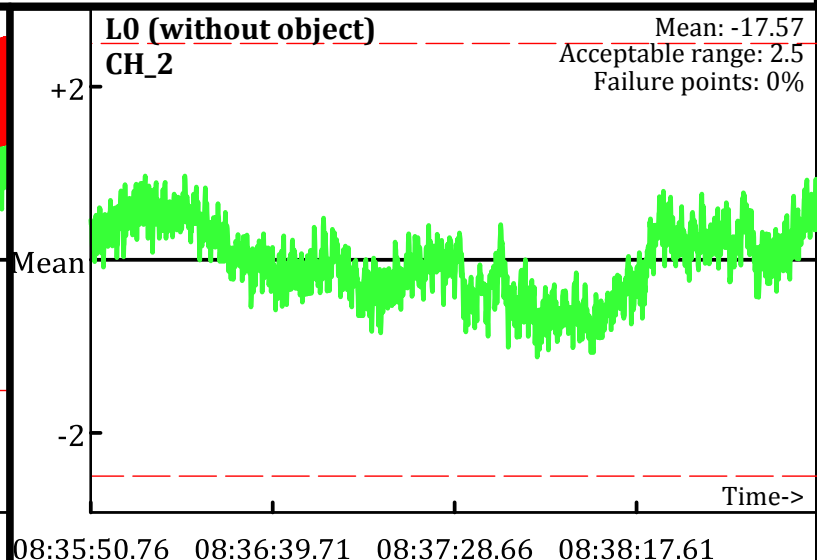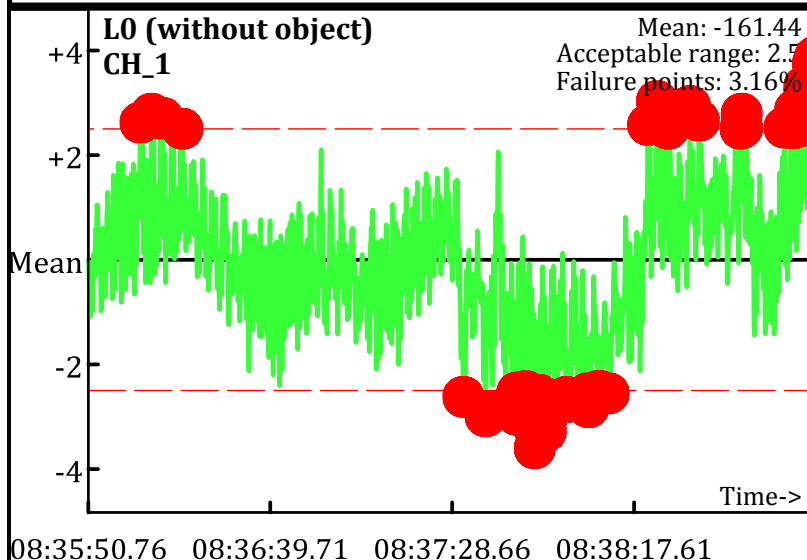Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
– – – Acceptable limits

AM test
Operator: PN & SH
Date: 1/12/2010

L0 (without object)
CH_3
Mean: 1.77
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH_4
Mean: -2.77
Acceptable range: 2.5
Failure points: 0%

Time->
08:35:50.76   08:36:39.71   08:37:28.66   08:38:17.61

Time->
08:35:50.76   08:36:39.71   08:37:28.66   08:38:17.61

L1 (with object)
CH_3
Mean: 33.38
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_4
Mean: 10.83
Acceptable range: 2.5
Failure points: 0%

Time->
08:40:13.56   08:41:01.74   08:41:49.91   08:42:38.09

Time->
08:40:13.56   08:41:01.74   08:41:49.91   08:42:38.09

L2 (without object)
CH_3
Mean: 2.62
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_4
Mean: -2.58
Acceptable range: 2.5
Failure points: 0%

Time->
08:44:23.27   08:44:40.74   08:44:58.22   08:45:15.69

Time->
08:44:23.27   08:44:40.74   08:44:58.22   08:45:15.69

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
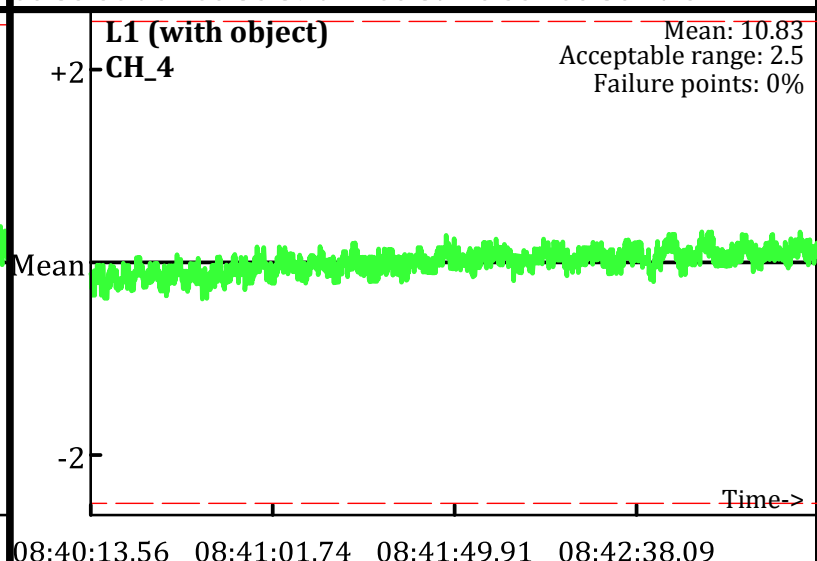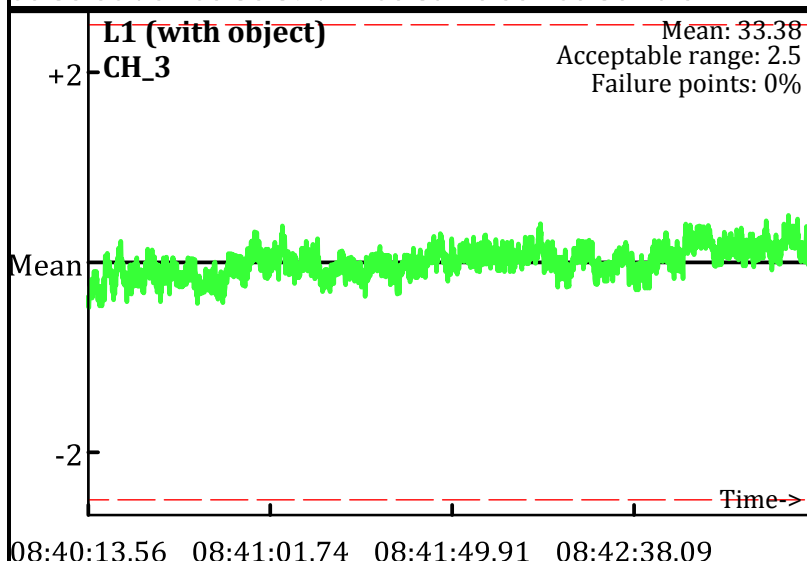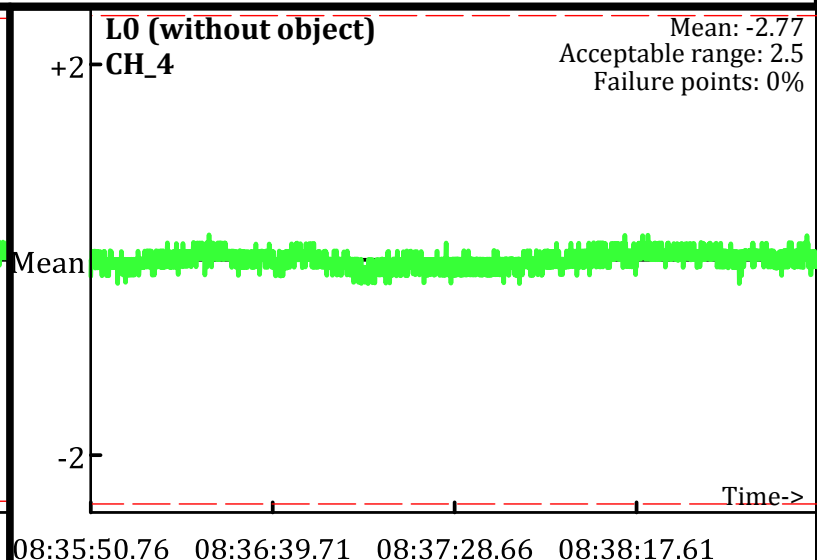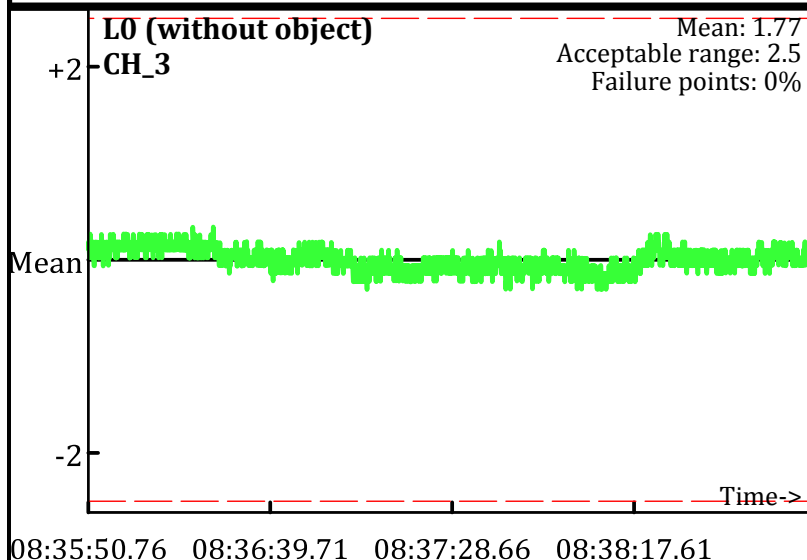Line Name: L0 L1 L2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

AM test
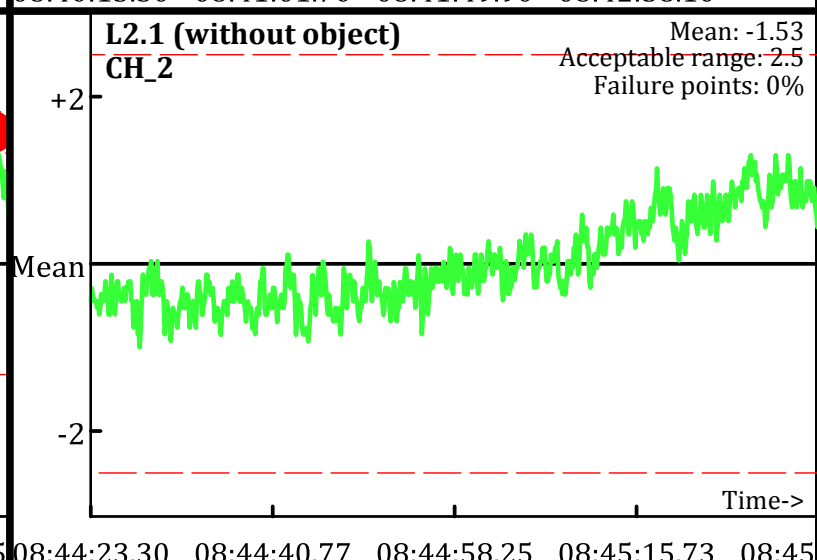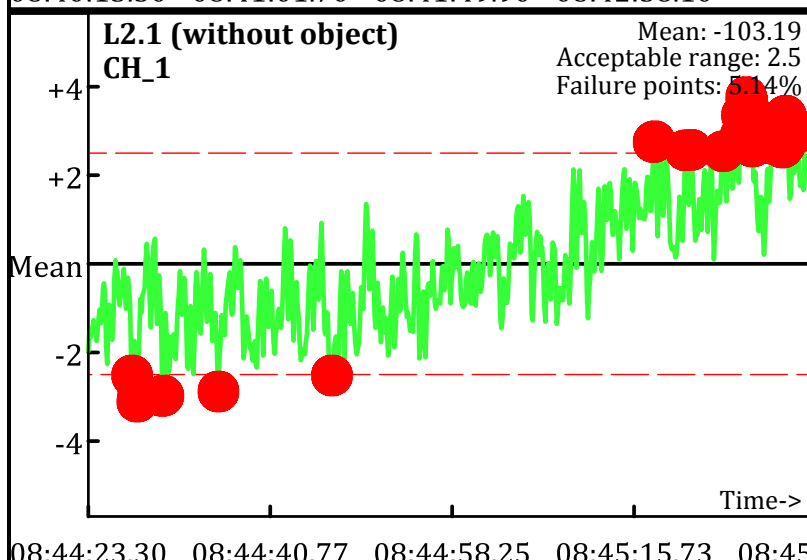Operator: PN & SH
Date: 1/12/2010

L0.1 (without object)
CH_1
Mean: -105.78
Acceptable range: 2.5
Failure points: 2.25%

L0.1 (without object)
CH_2
Mean: -2.21
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_1
Mean: 9.68
Acceptable range: 2
Failure points: 0.881%

L1.1 (with object)
CH_2
Mean: 84.8
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_1
Mean: -103.19
Acceptable range: 2.5
Failure points: 5.14%

L2.1 (without object)
CH_2
Mean: -1.53
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
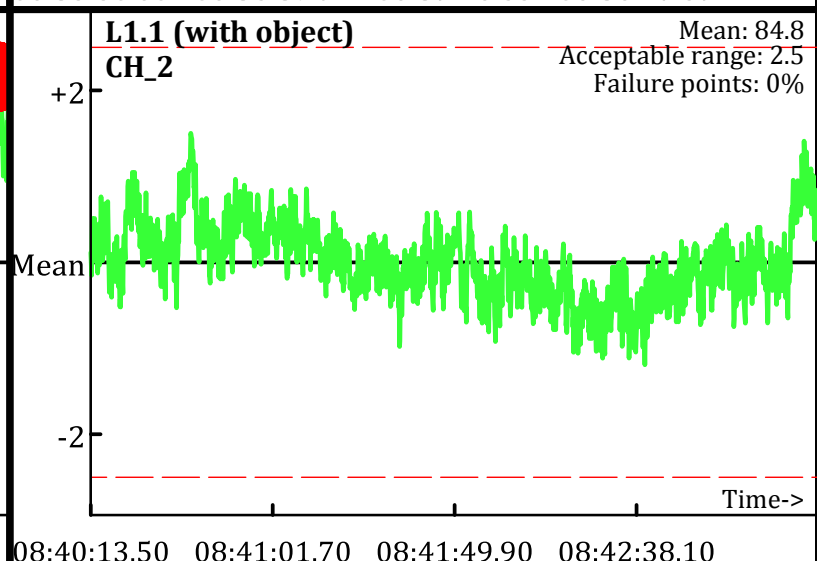Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits
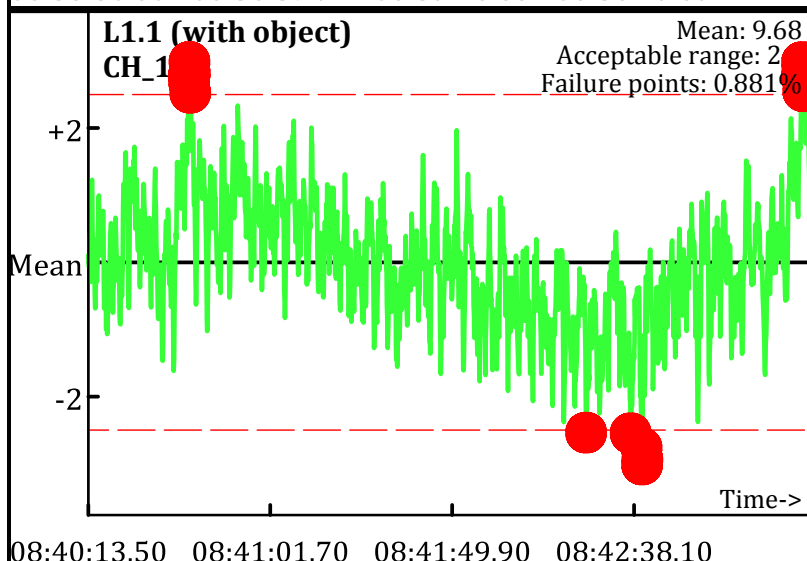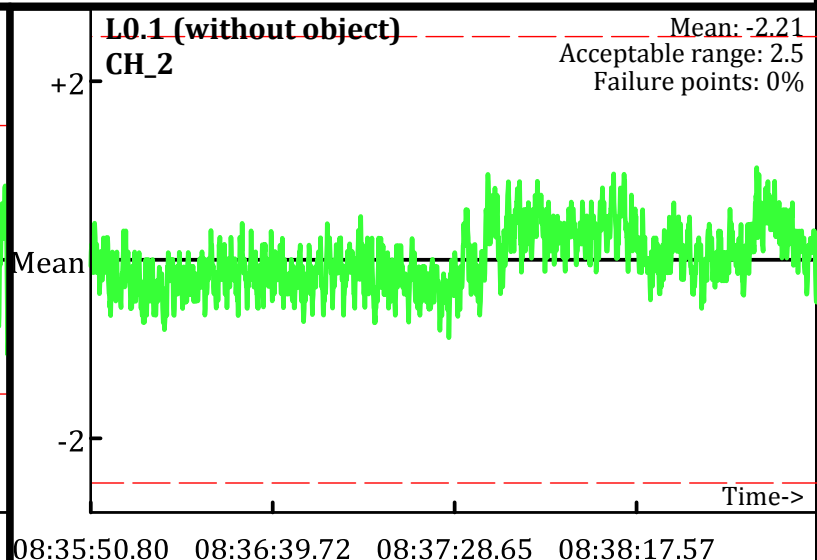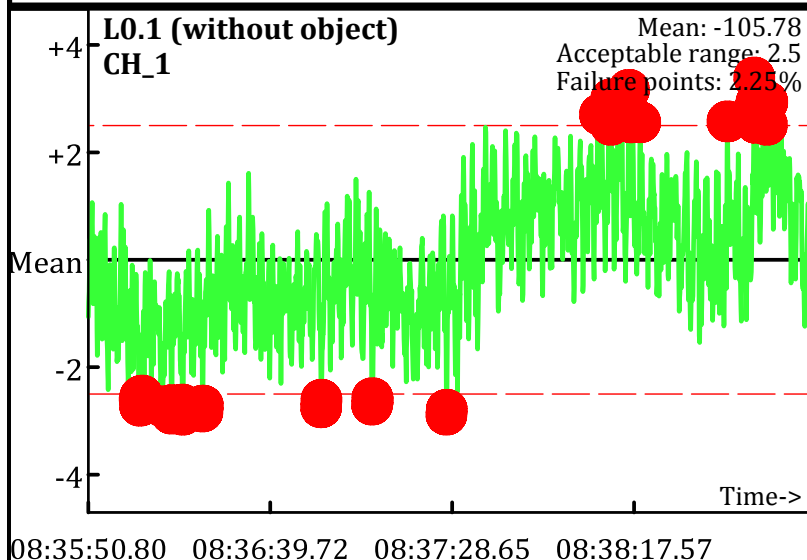
AM test
Operator: PN & SH
Date: 1/12/2010

L0.1 (without object)
CH_3
Mean: 9.48
Acceptable range: 2.5
Failure points: 0%

08:35:50.80   08:36:39.72   08:37:28.65   08:38:17.57

L0.1 (without object)
CH_4
Mean: 1.72
Acceptable range: 2.5
Failure points: 0%

08:35:50.80   08:36:39.72   08:37:28.65   08:38:17.57

L1.1 (with object)
CH_3
Mean: 65.46
Acceptable range: 2.5
Failure points: 0%

08:40:13.50   08:41:01.70   08:41:49.90   08:42:38.10

L1.1 (with object)
CH_4
Mean: 31.78
Acceptable range: 2.5
Failure points: 0%

08:40:13.50   08:41:01.70   08:41:49.90   08:42:38.10

L2.1 (without object)
CH_3
Mean: 9.64
Acceptable range: 2.5
Failure points: 0%

08:44:23.30   08:44:40.77   08:44:58.25   08:45:15.73   08:45

L2.1 (without object)
CH_4
Mean: 1.69
Acceptable range: 2.5
Failure points: 0%

08:44:23.30   08:44:40.77   08:44:58.25   08:45:15.73   08:45

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

AM test
Operator: PN & SH
Date: 1/12/2010
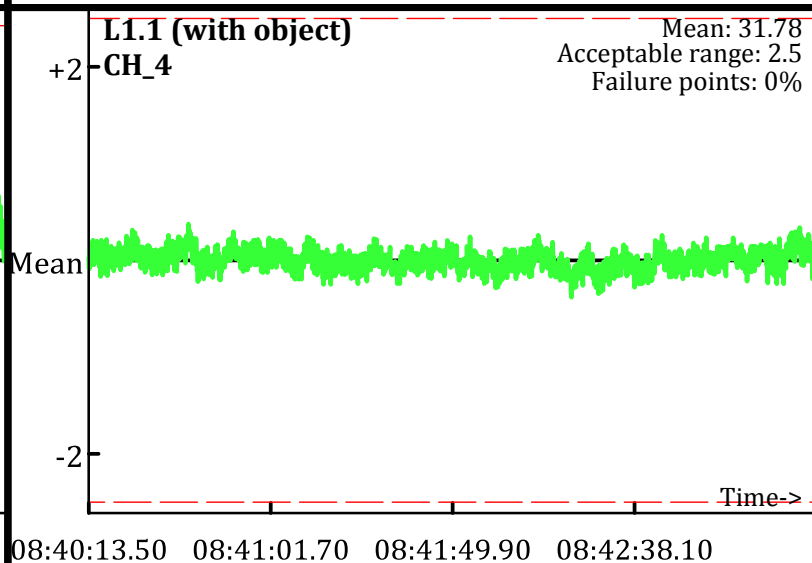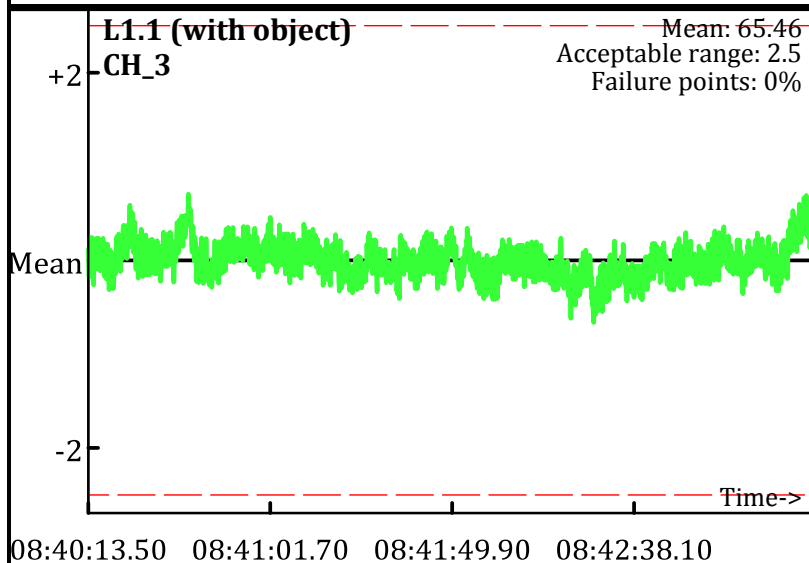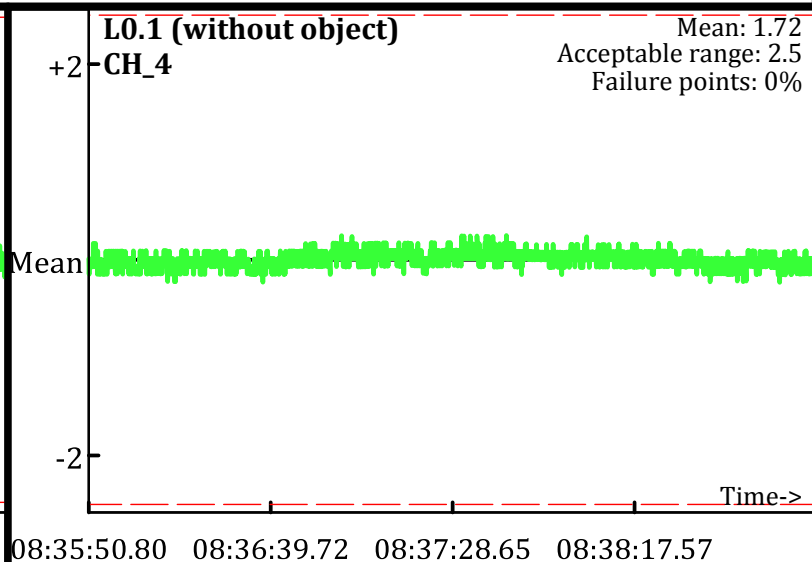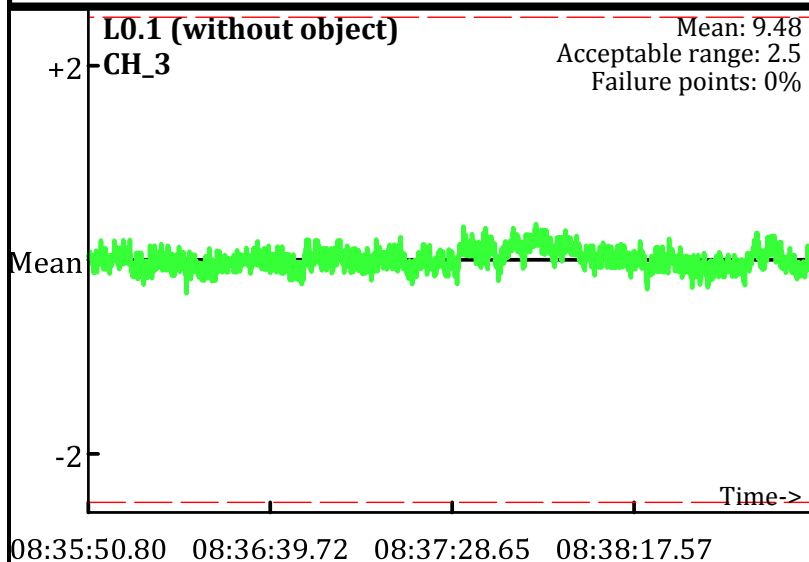

L0.2 (without object)
CH_1
Mean: -64.54
Acceptable range: 2.5
Failure points: 0%

L0.2 (without object)
CH_2
Mean: 3.55
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_1
Mean: 28.88
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_2
Mean: 60.95
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_1
Mean: -64.25
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_2
Mean: 3.2
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits
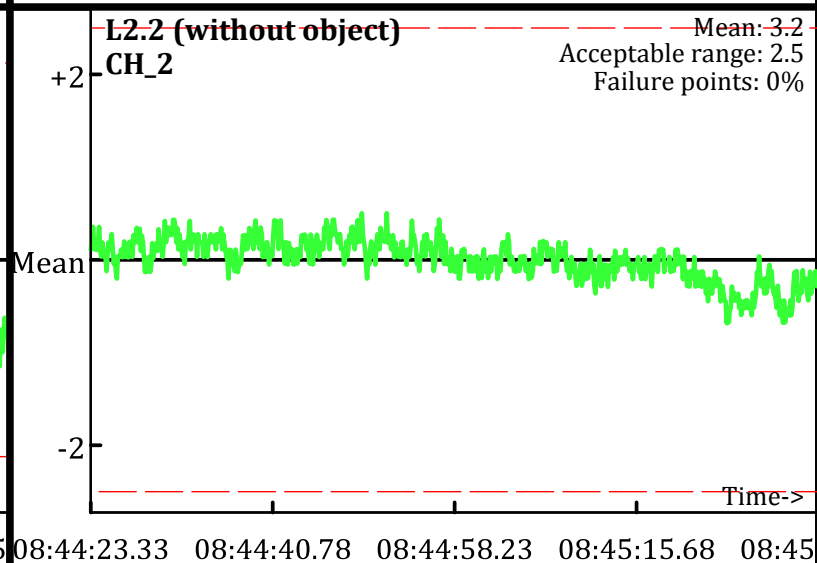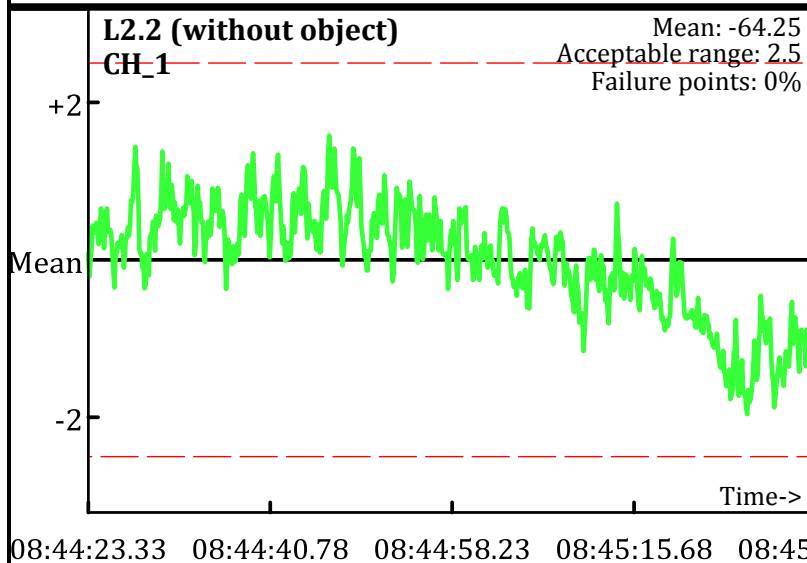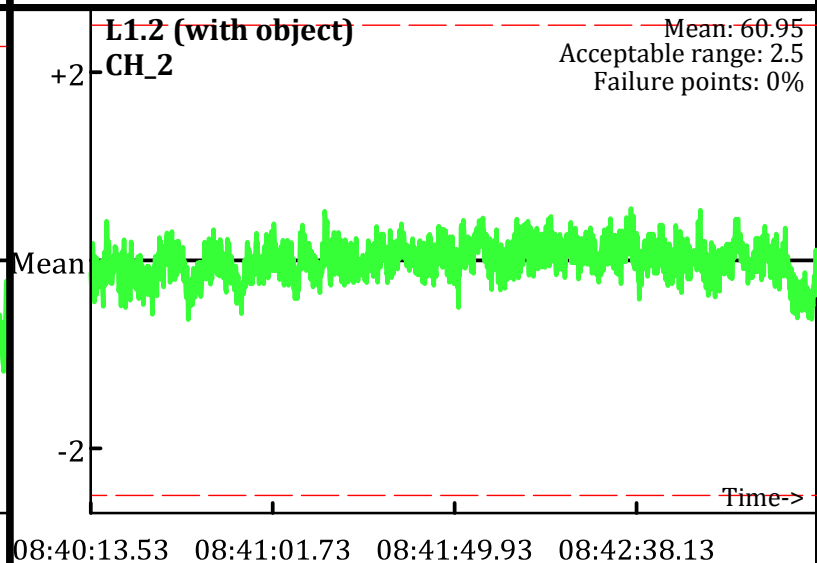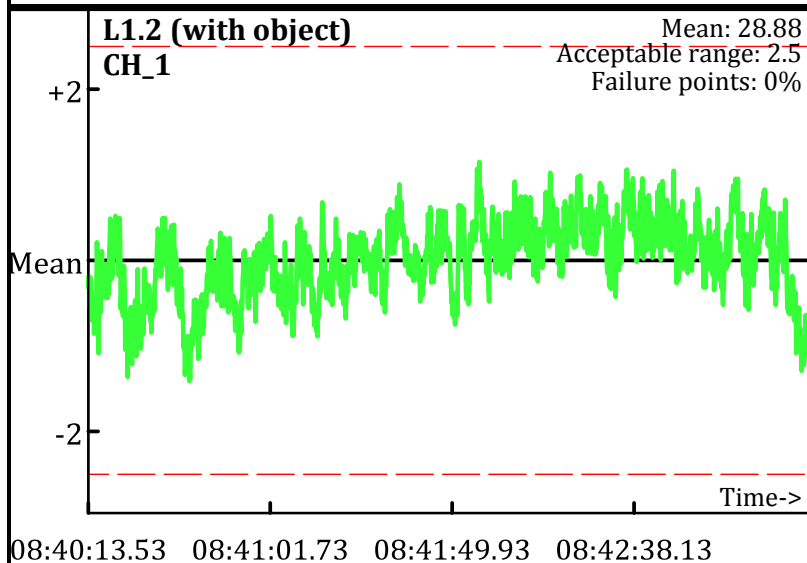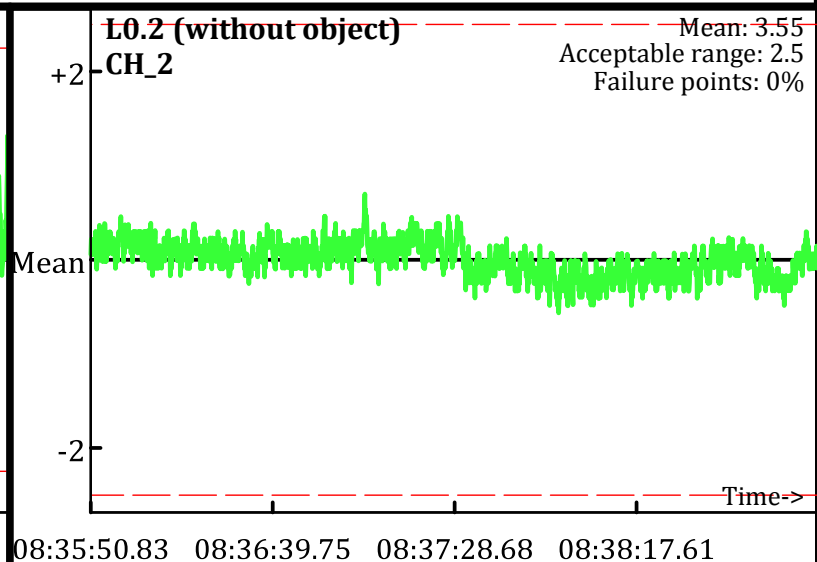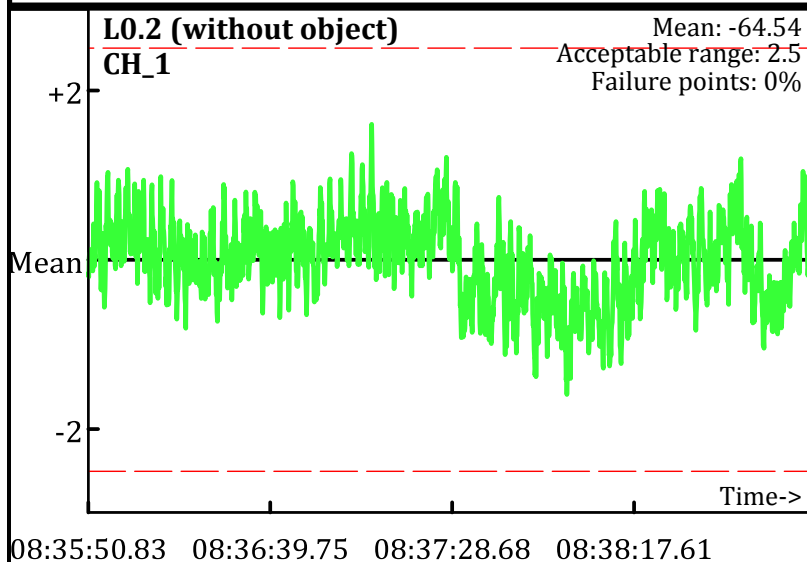
AM test
Operator: PN & SH
Date: 1/12/2010

L0.2 (without object)
CH_3
Mean: 6.4
Acceptable range: 2.5
Failure points: 0%

08:35:50.83 08:36:39.75 08:37:28.68 08:38:17.61

L0.2 (without object)
CH_4
Mean: -0.44
Acceptable range: 2.5
Failure points: 0%

08:35:50.83 08:36:39.75 08:37:28.68 08:38:17.61

L1.2 (with object)
CH_3
Mean: 36.59
Acceptable range: 2.5
Failure points: 0%

08:40:13.53 08:41:01.73 08:41:49.93 08:42:38.13

L1.2 (with object)
CH_4
Mean: 12.86
Acceptable range: 2.5
Failure points: 0%

08:40:13.53 08:41:01.73 08:41:49.93 08:42:38.13

L2.2 (without object)
CH_3
Mean: 6.17
Acceptable range: 2.5
Failure points: 0%

08:44:23.33 08:44:40.78 08:44:58.23 08:45:15.68 08:45

L2.2 (without object)
CH_4
Mean: -0.63
Acceptable range: 2.5
Failure points: 0%

08:44:23.33 08:44:40.78 08:44:58.23 08:45:15.68 08:45

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits
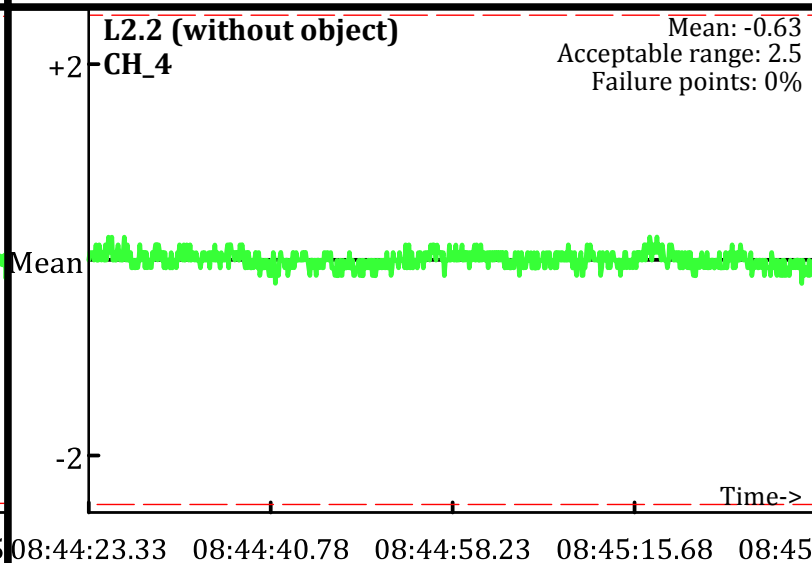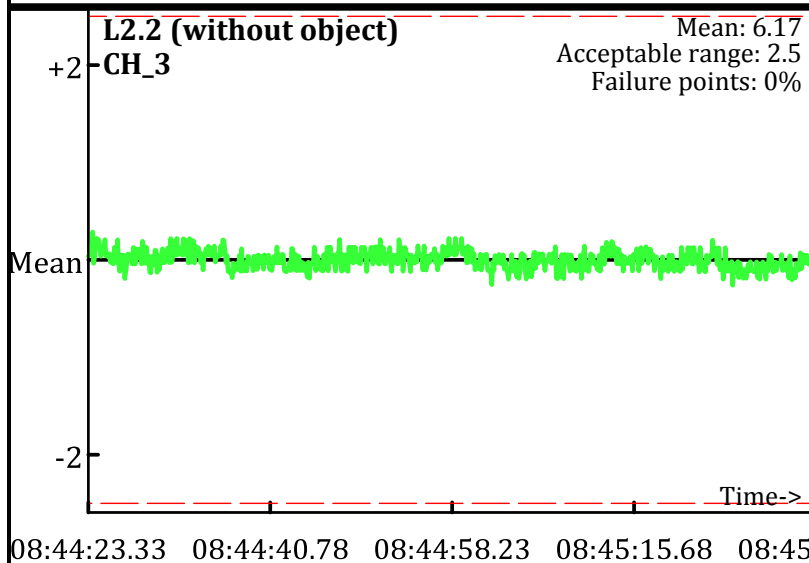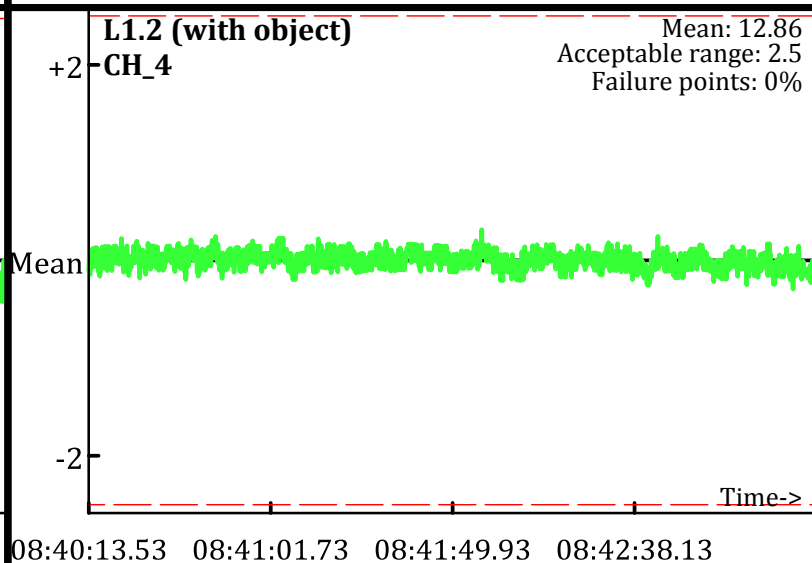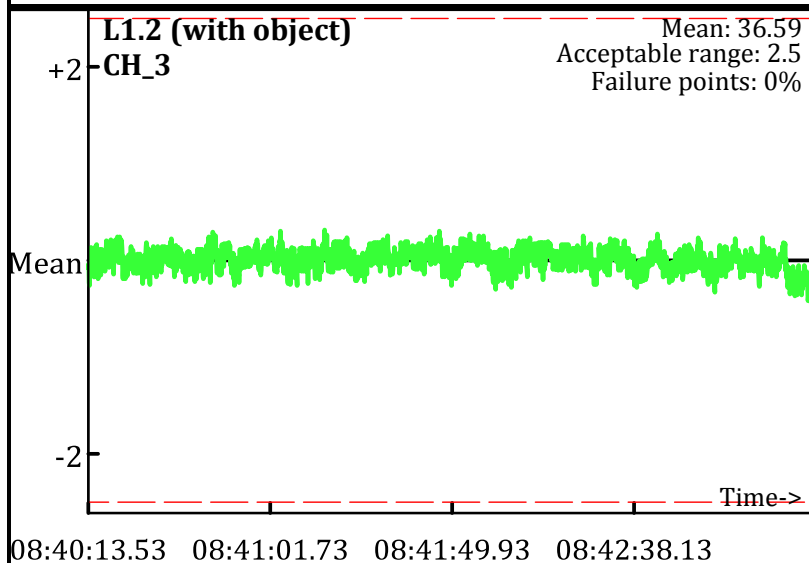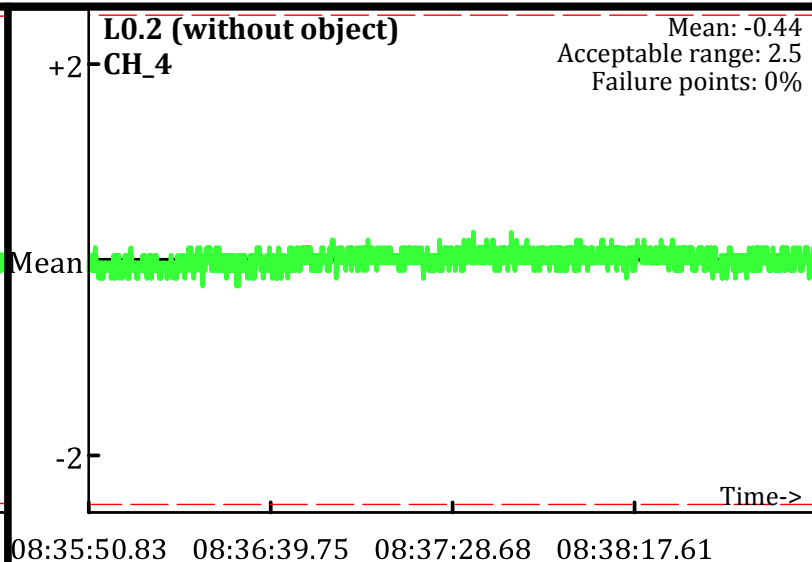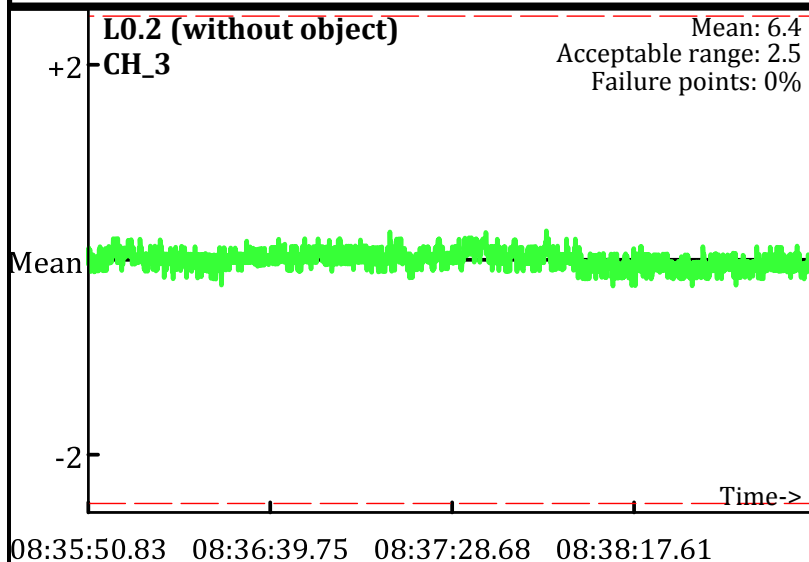
PM test
Operator: PN & SH
Date: 1/12/2010

L5 (without object)
CH_1
Mean: -128.58
Acceptable range: 2.5
Failure points: 0%

L5 (without object)
CH_2
Mean: -12.1
Acceptable range: 2.5
Failure points: 0%

16:48:41.73   16:49:27.41   16:50:13.08   16:50:58.75   16:51

L7 (with object)
CH_1
Mean: -38.51
Acceptable range: 2.5
Failure points: 0%

L7 (with object)
CH_2
Mean: 44.34
Acceptable range: 2.5
Failure points: 0%

16:54:36.42   16:55:22.85   16:56:09.27   16:56:55.70   16:57

L8 (without object)
CH_1
Mean: -129.95
Acceptable range: 2.5
Failure points: 0%

L8 (without object)
CH_2
Mean: -12.61
Acceptable range: 2.5
Failure points: 0%

16:58:52.12   16:59:07.60   16:59:23.08   16:59:38.55   16:59

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
Line Name: L5 L7 L8

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

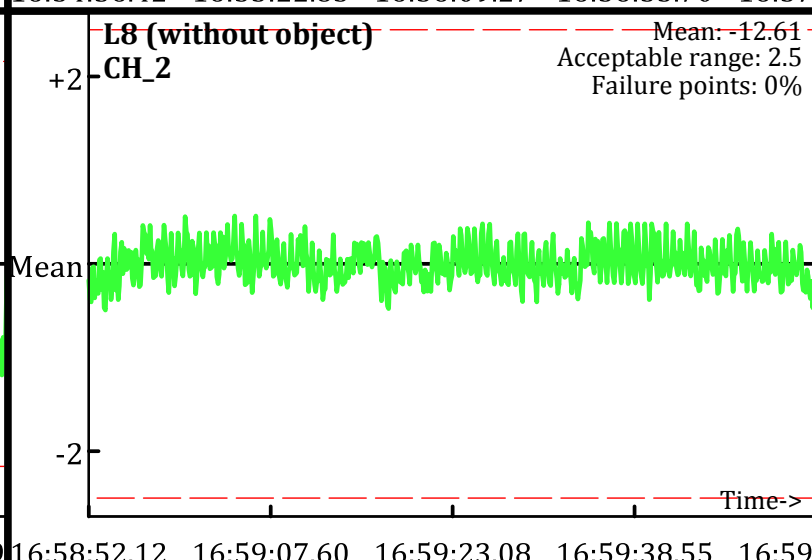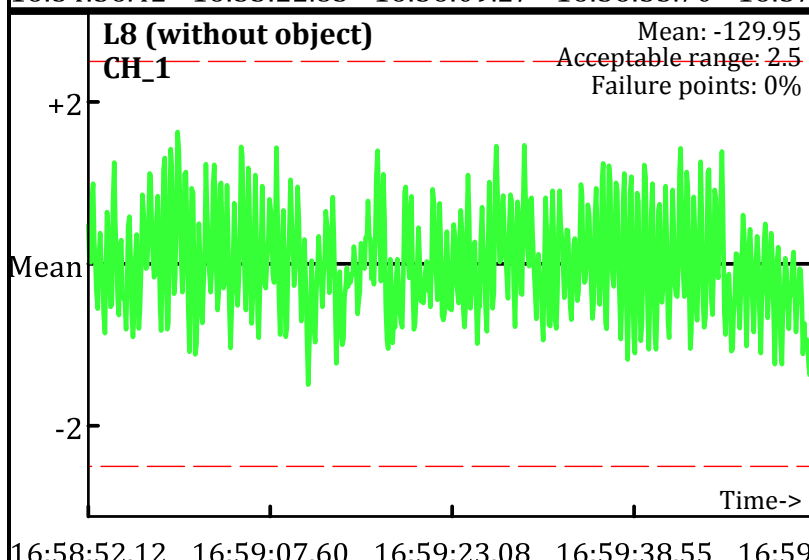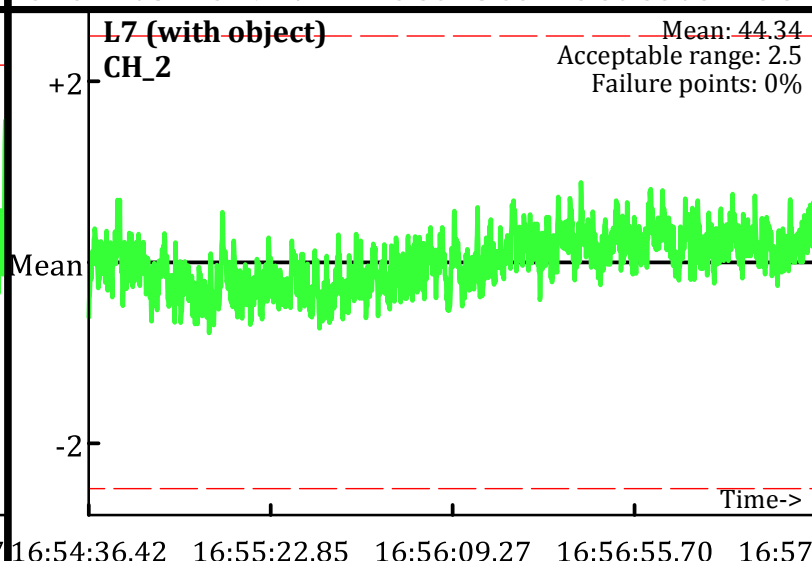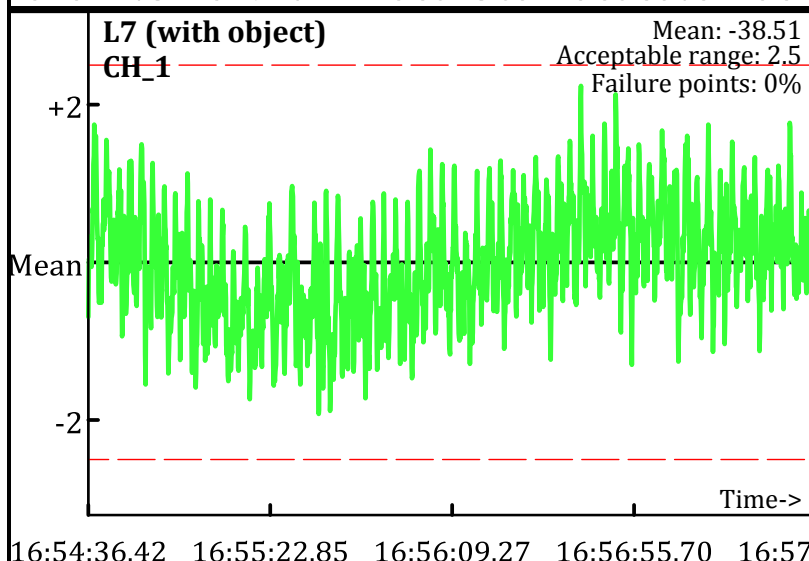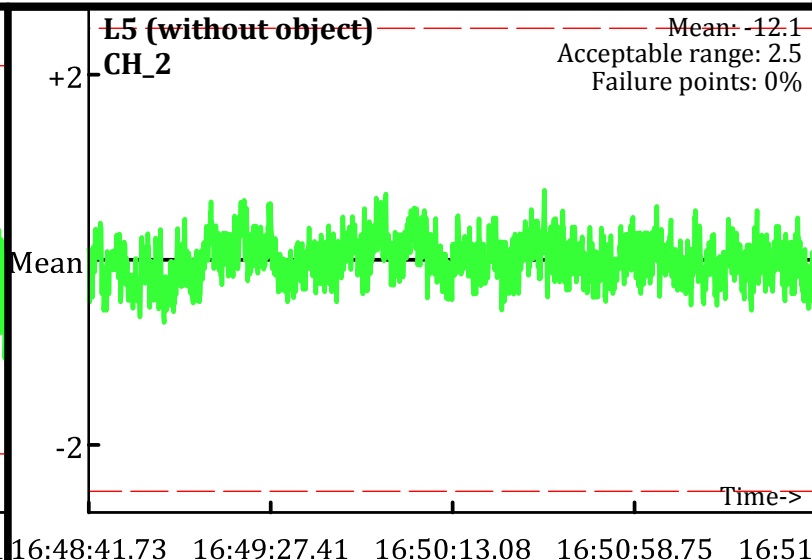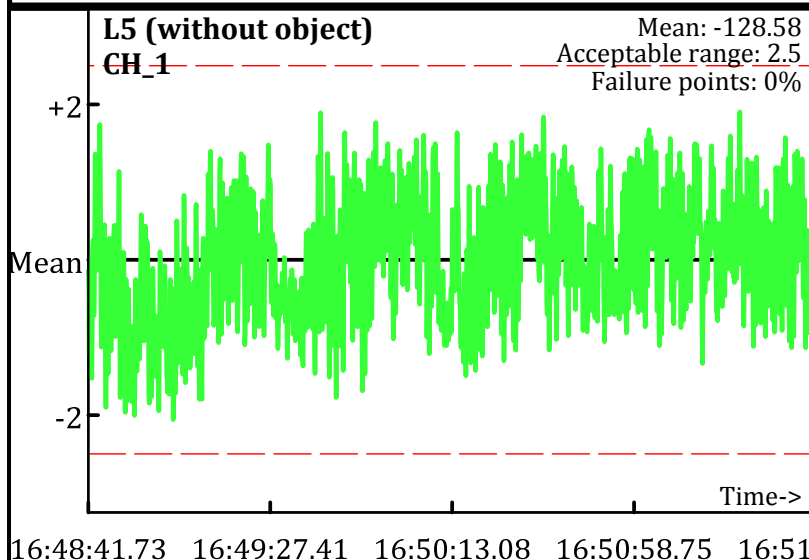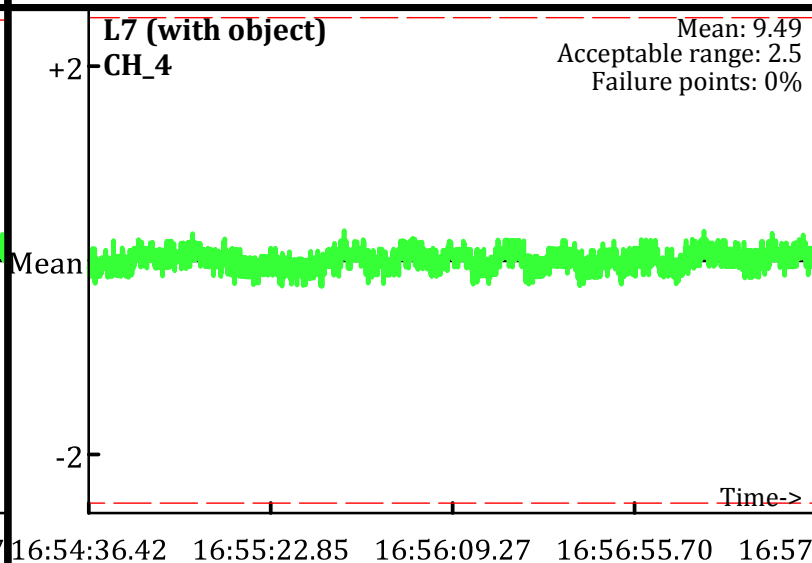PM test
Operator: PN & SH
Date: 1/12/2010

L5 (without object)
CH_3
Mean: 2.06
Acceptable range: 2.5
Failure points: 0%

L5 (without object)
CH_4
Mean: -3.39
Acceptable range: 2.5
Failure points: 0%

16:48:41.73 16:49:27.41 16:50:13.08 16:50:58.75 16:51
16:48:41.73 16:49:27.41 16:50:13.08 16:50:58.75 16:51

L7 (with object)
CH_3
Mean: 31.53
Acceptable range: 2.5
Failure points: 0%

L7 (with object)
CH_4
Mean: 9.49
Acceptable range: 2.5
Failure points: 0%

16:54:36.42 16:55:22.85 16:56:09.27 16:56:55.70 16:57
16:54:36.42 16:55:22.85 16:56:09.27 16:56:55.70 16:57

L8 (without object)
CH_3
Mean: 1.81
Acceptable range: 2.5
Failure points: 0%

L8 (without object)
CH_4
Mean: -3.6
Acceptable range: 2.5
Failure points: 0%

16:58:52.12 16:59:07.60 16:59:23.08 16:59:38.55 16:59
16:58:52.12 16:59:07.60 16:59:23.08 16:59:38.55 16:59

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
Line Name: L5 L7 L8

Page: 2

Static Calibration Test

● Outside range
– – – Acceptable limits

L5.1 (without object)
CH_1
Mean: -85.8
Acceptable range: 2.5
Failure points: 0.0547%

+2
Mean
-2
Time->

16:48:41.75 16:49:27.43 16:50:13.10 16:50:58.78 16:51

L5.1 (without object)
CH_2
Mean: 0.29
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:48:41.75 16:49:27.43 16:50:13.10 16:50:58.78 16:51

L7.1 (with object)
CH_1
Mean: 36.01
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:54:36.36 16:55:22.81 16:56:09.26 16:56:55.71

L7.1 (with object)
CH_2
Mean: 91.39
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:54:36.36 16:55:22.81 16:56:09.26 16:56:55.71

L8.1 (without object)
CH_1
Mean: -83.9
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:58:52.16 16:59:07.63 16:59:23.11 16:59:38.59 16:59

L8.1 (without object)
CH_2
Mean: 1.33
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

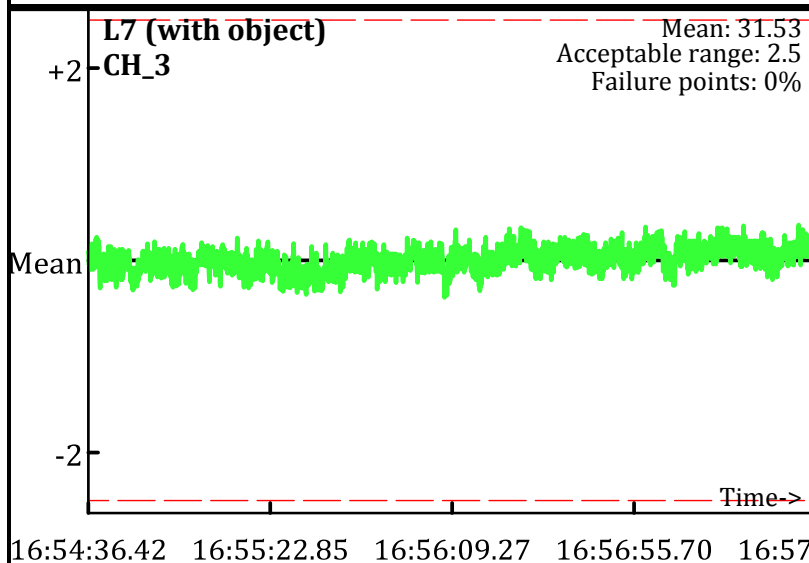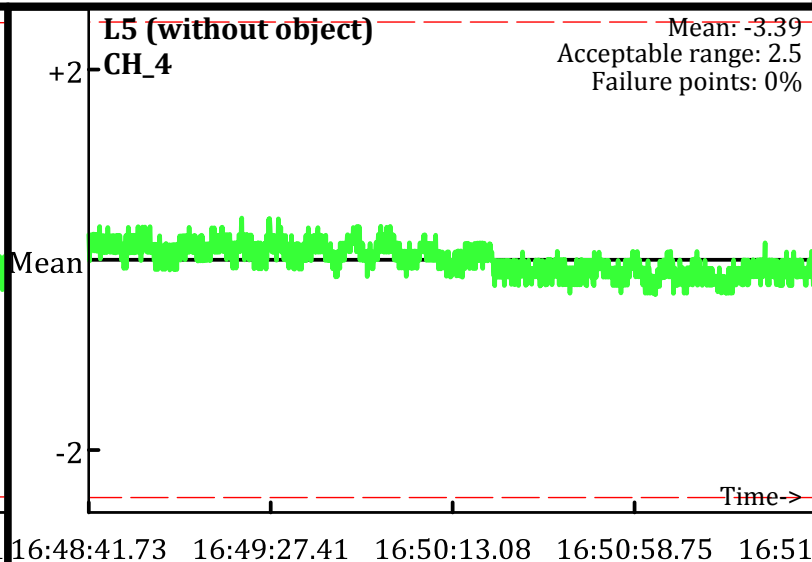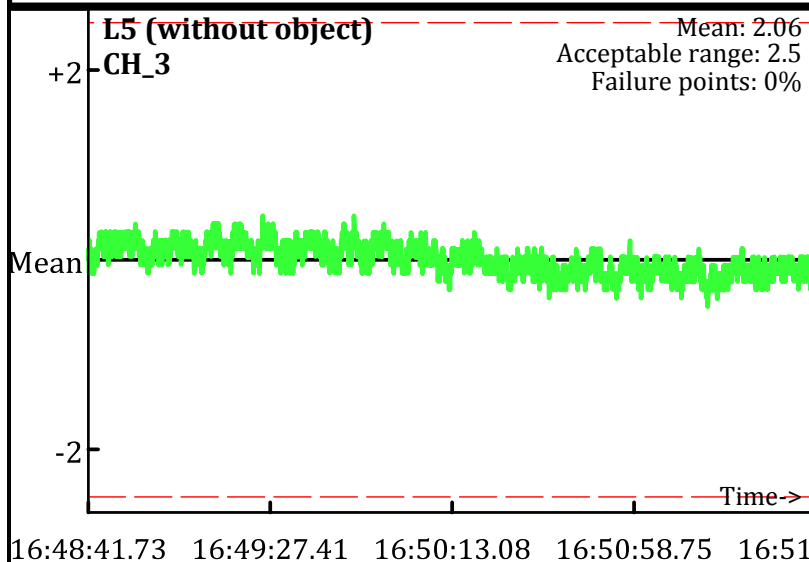16:58:52.16 16:59:07.63 16:59:23.11 16:59:38.59 16:59

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

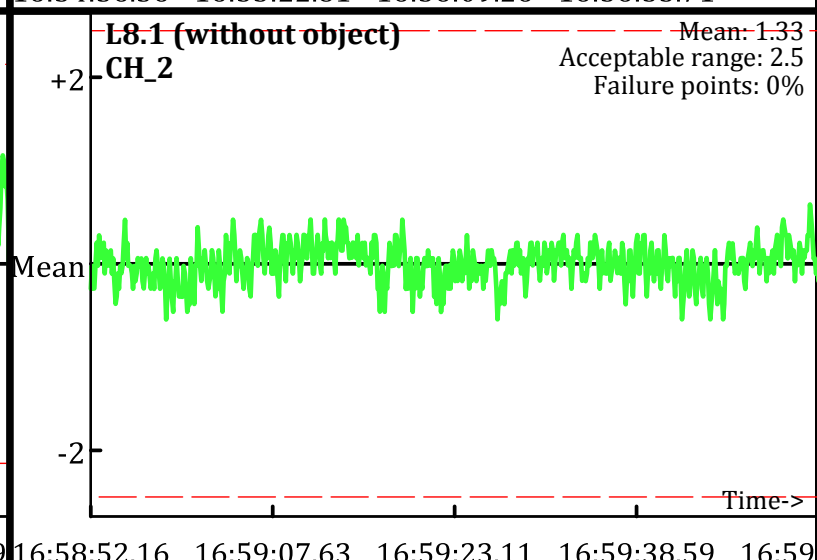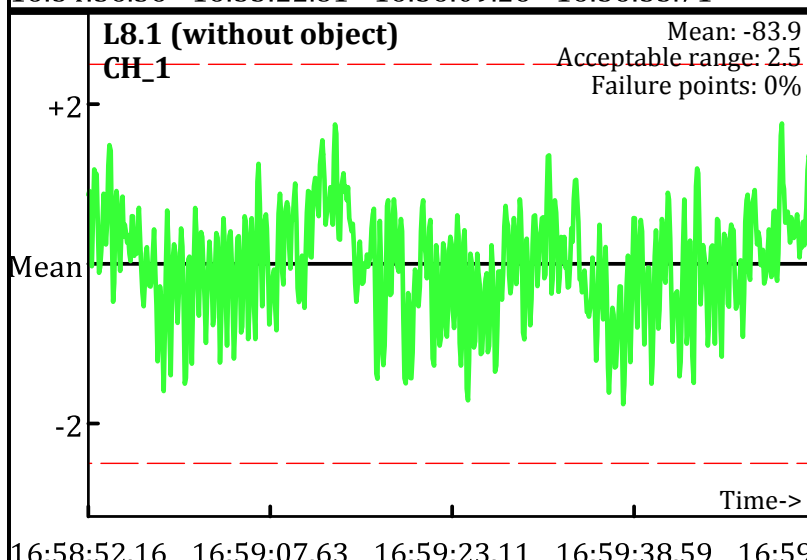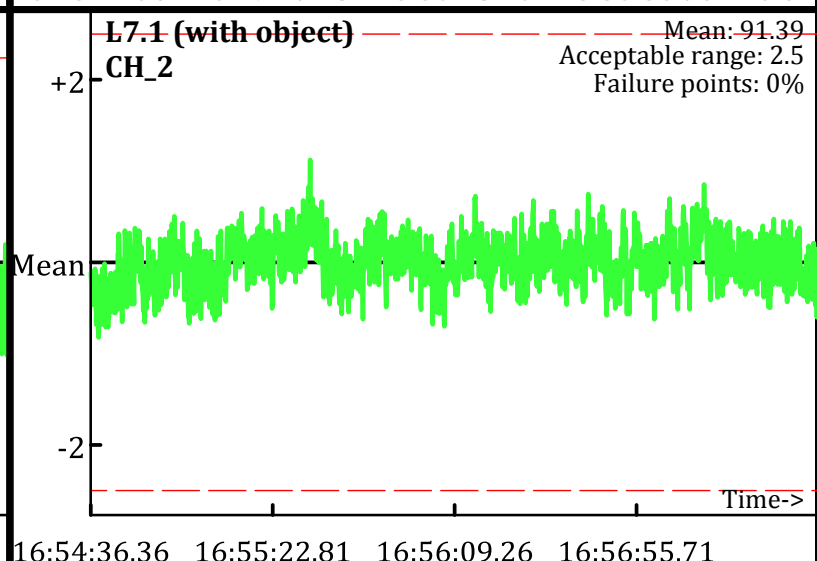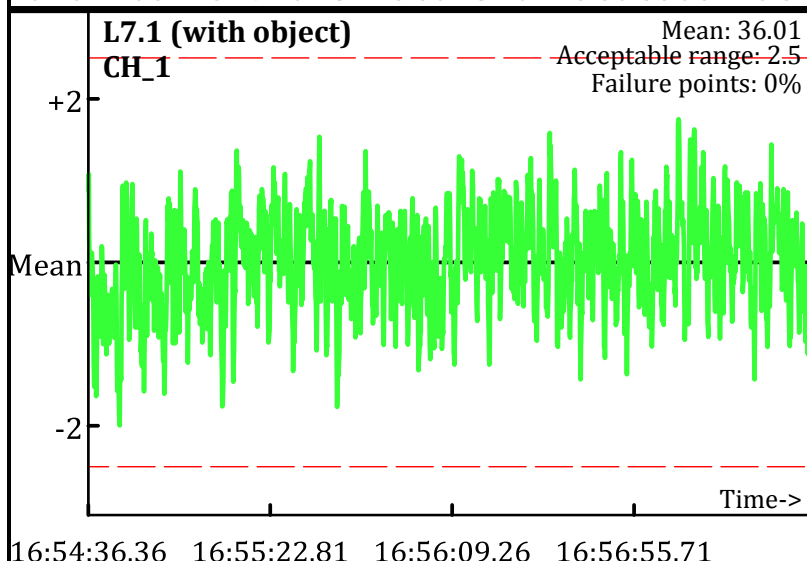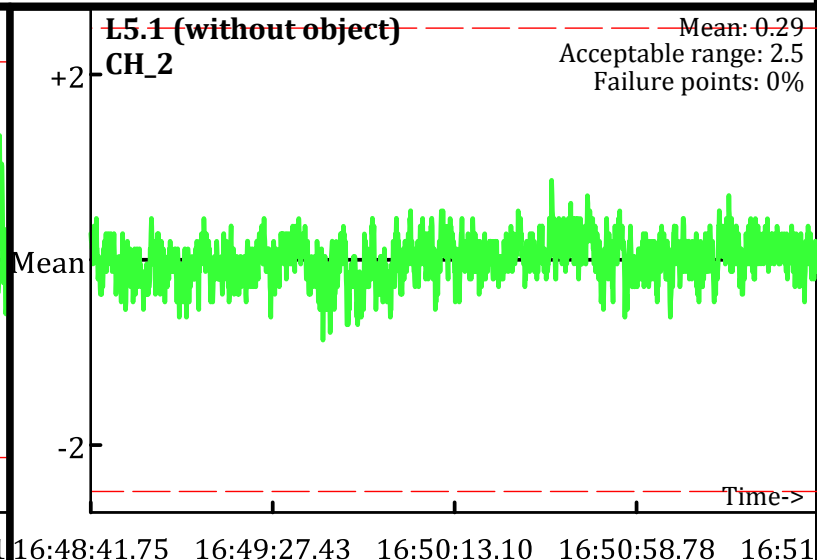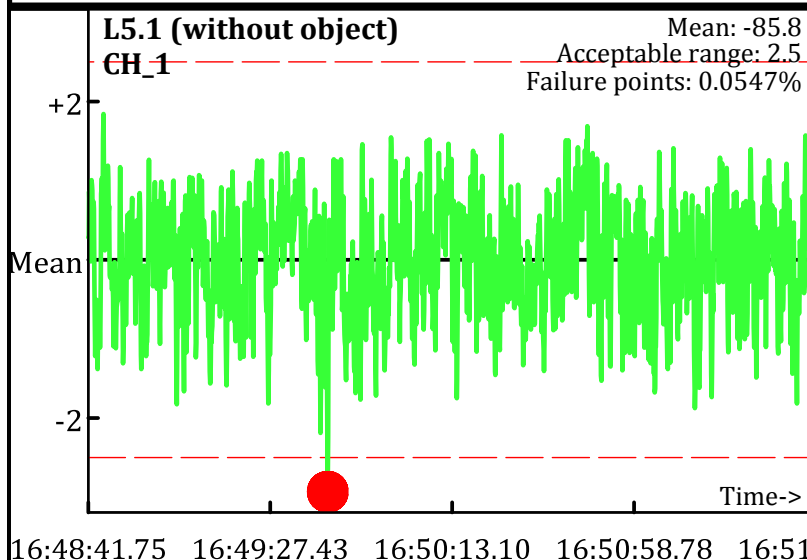PM test
Operator: PN & SH
Date: 1/12/2010

L5.1 (without object)
CH_3
Mean: 8.65
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:48:41.75   16:49:27.43   16:50:13.10   16:50:58.78   16:51

L5.1 (without object)
CH_4
Mean: 0.75
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:48:41.75   16:49:27.43   16:50:13.10   16:50:58.78   16:51

L7.1 (with object)
CH_3
Mean: 66.66
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:36.36   16:55:22.81   16:56:09.26   16:56:55.71

L7.1 (with object)
CH_4
Mean: 31.75
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:36.36   16:55:22.81   16:56:09.26   16:56:55.71

L8.1 (without object)
CH_3
Mean: 9.09
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:58:52.16   16:59:07.63   16:59:23.11   16:59:38.59   16:59

L8.1 (without object)
CH_4
Mean: 0.87
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:58:52.16   16:59:07.63   16:59:23.11   16:59:38.59   16:59

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
Line Name: L5.1 L7.1 L8.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
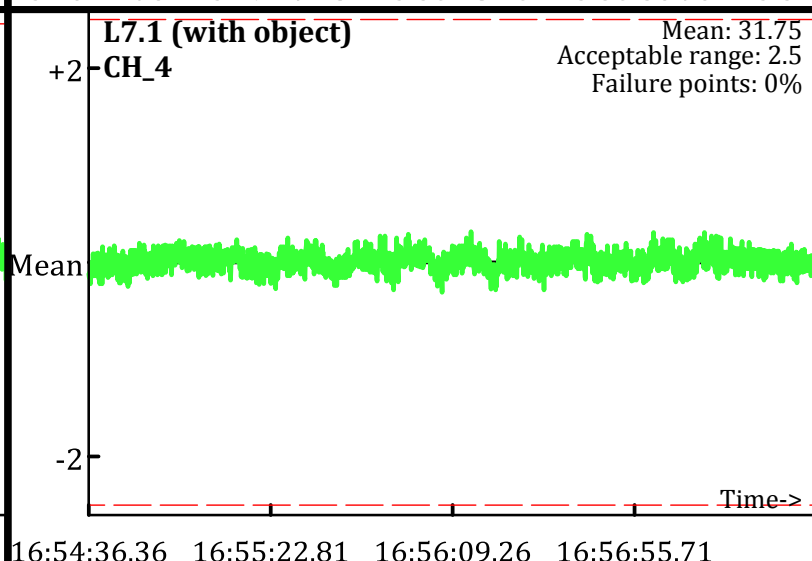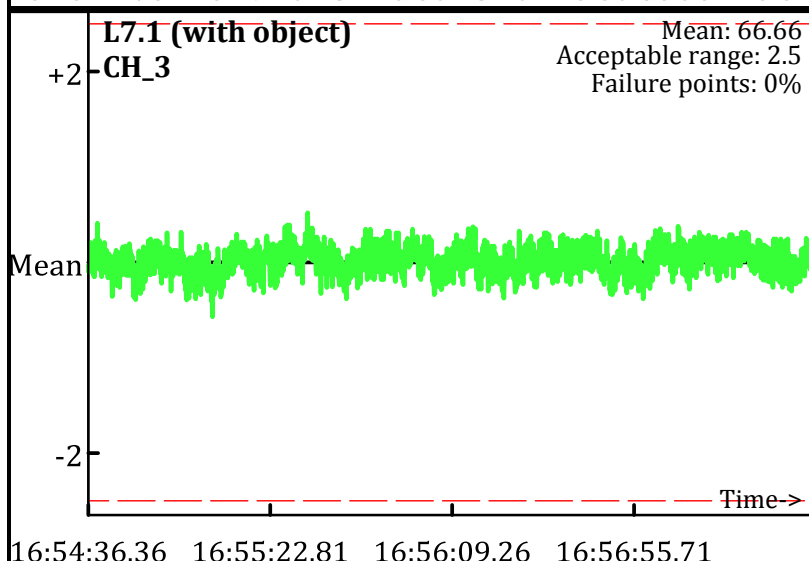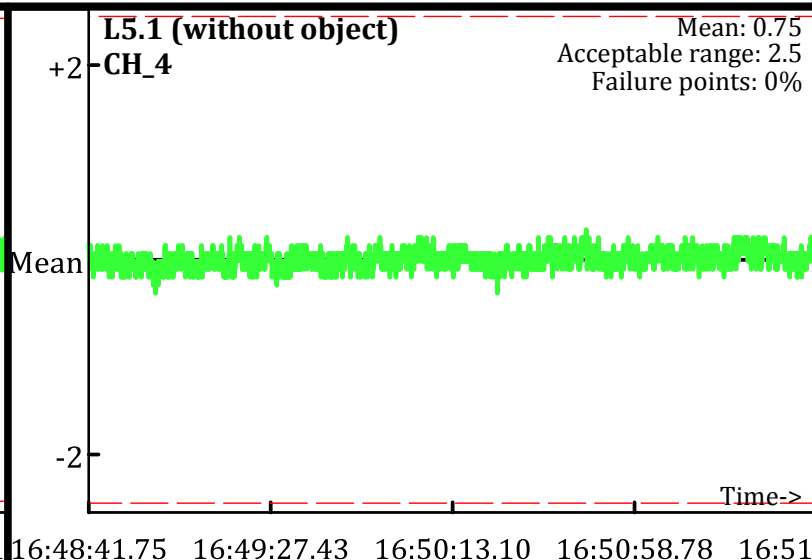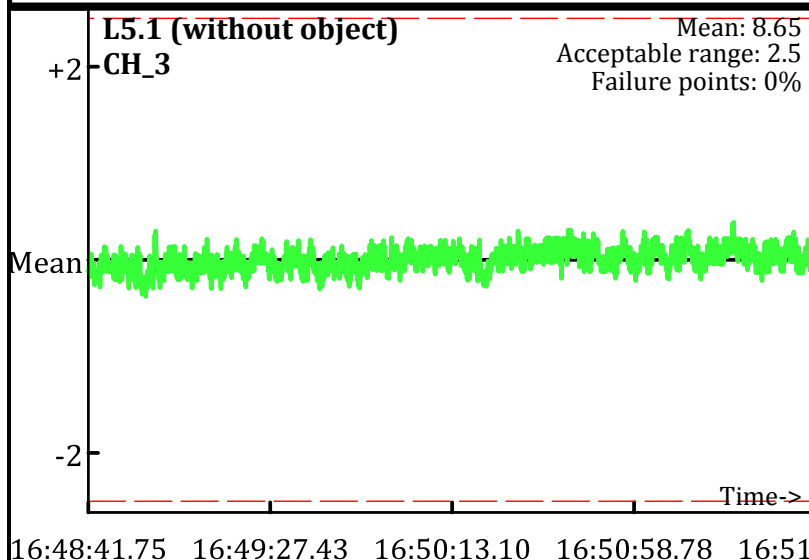Grid/Location: QC Area

⬤ Outside range
– – – Acceptable limits

PM test
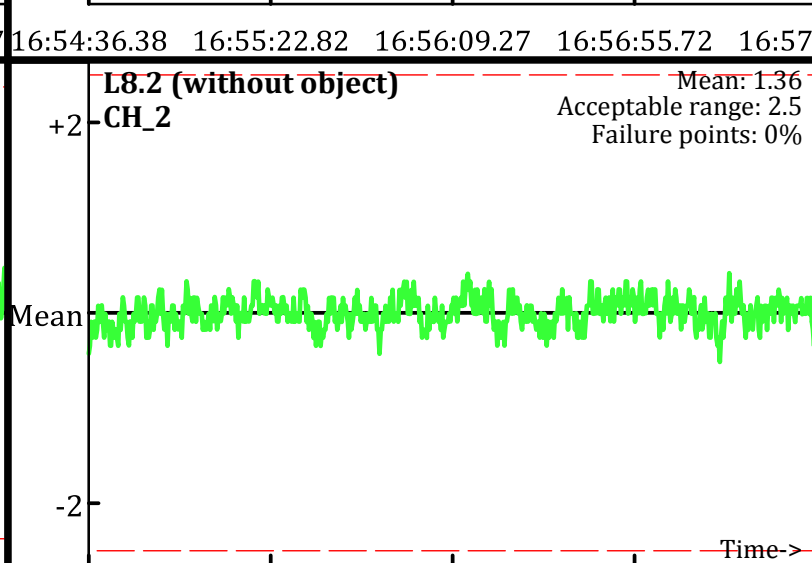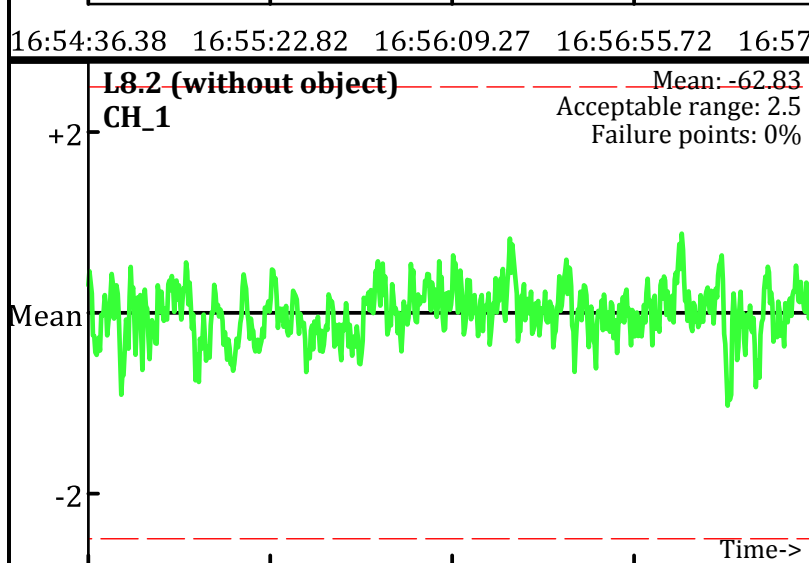Operator: PN & SH
Date: 1/12/2010

L5.2 (without object)
CH_1
Mean: -62.46
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:48:41.69   16:49:27.39   16:50:13.09   16:50:58.78   16:51

L5.2 (without object)
CH_2
Mean: 1.3
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:48:41.69   16:49:27.39   16:50:13.09   16:50:58.78   16:51

L7.2 (with object)
CH_1
Mean: 20.61
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:54:36.38   16:55:22.82   16:56:09.27   16:56:55.72   16:57

L7.2 (with object)
CH_2
Mean: 52.99
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:54:36.38   16:55:22.82   16:56:09.27   16:56:55.72   16:57

L8.2 (without object)
CH_1
Mean: -62.83
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:58:52.19   16:59:07.64   16:59:23.09   16:59:38.53

L8.2 (without object)
CH_2
Mean: 1.36
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

16:58:52.19   16:59:07.64   16:59:23.09   16:59:38.53

Database: D:\Projects_QCReports_Ord_Data\011210\QC\011210_TA_QC.gdb
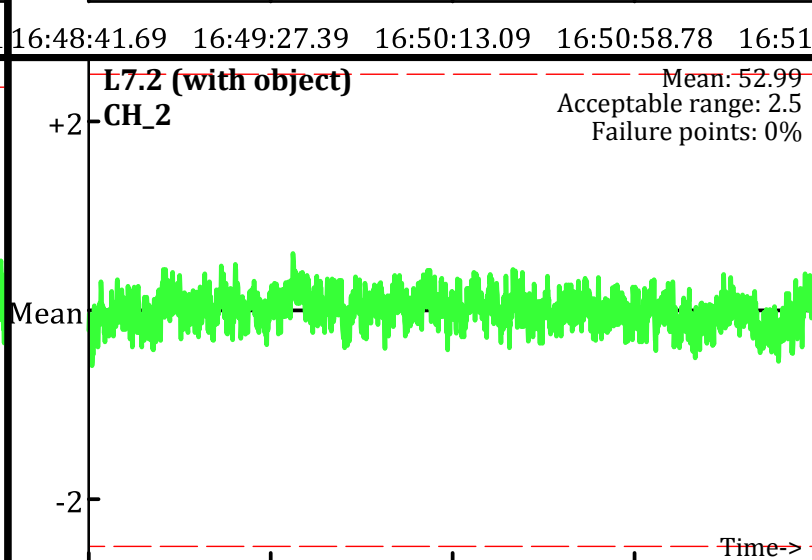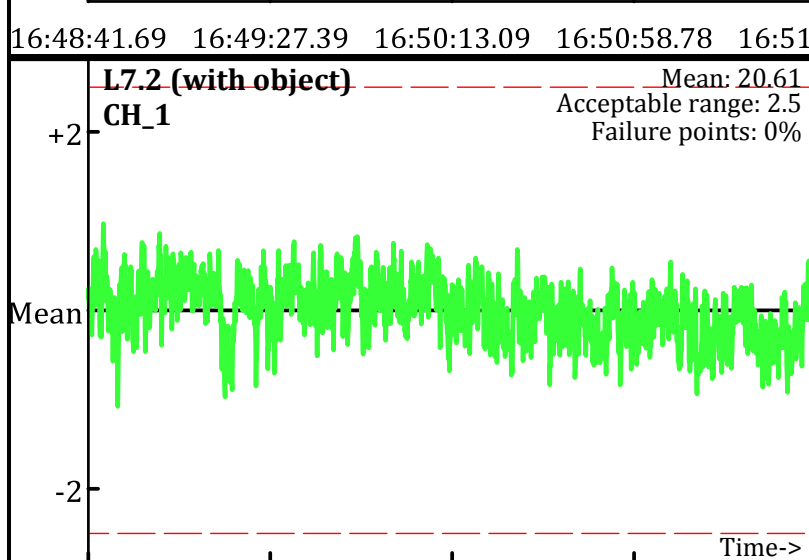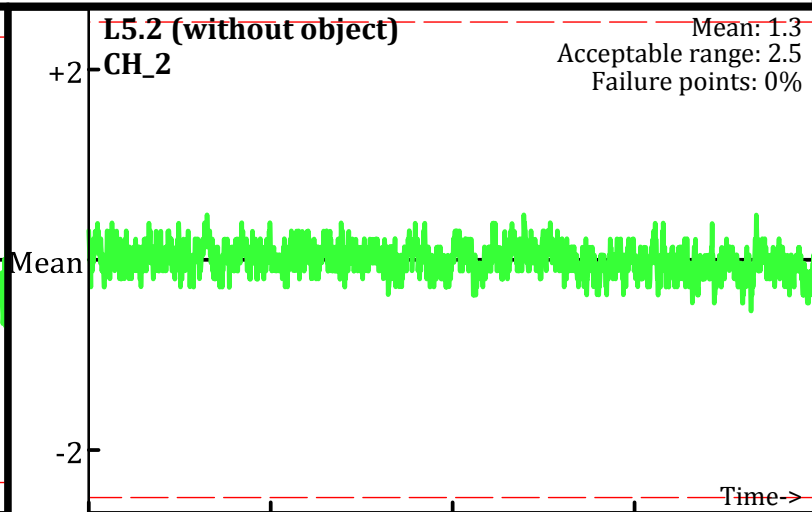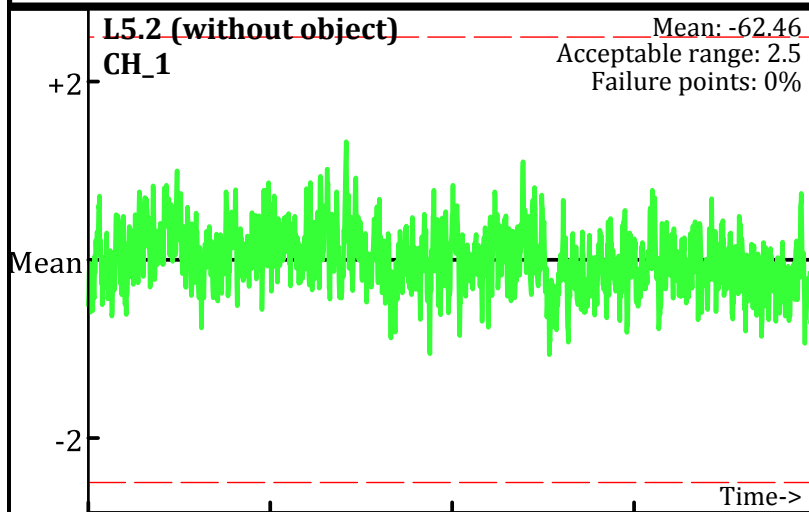Line Name: L5.2 L7.2 L8.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/12/2010

L5.2 (without object)
CH_3

Mean: 5.69
Acceptable range: 2.5
Failure points: 0%

Time->

16:48:41.69   16:49:27.39   16:50:13.09   16:50:58.78   16:51

L5.2 (without object)
CH_4

Mean: -0.79
Acceptable range: 2.5
Failure points: 0%

Time->

16:48:41.69   16:49:27.39   16:50:13.09   16:50:58.78   16:51

L7.2 (with object)
CH_3

Mean: 32.82
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:36.38   16:55:22.82   16:56:09.27   16:56:55.72   16:57

L7.2 (with object)
CH_4

Mean: 11.07
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:36.38   16:55:22.82   16:56:09.27   16:56:55.72   16:57

L8.2 (without object)
CH_3

Mean: 5.74
Acceptable range: 2.5
Failure points: 0%

Time->

16:58:52.19   16:59:07.64   16:59:23.09   16:59:38.53

L8.2 (without object)
CH_4

Mean: -0.72
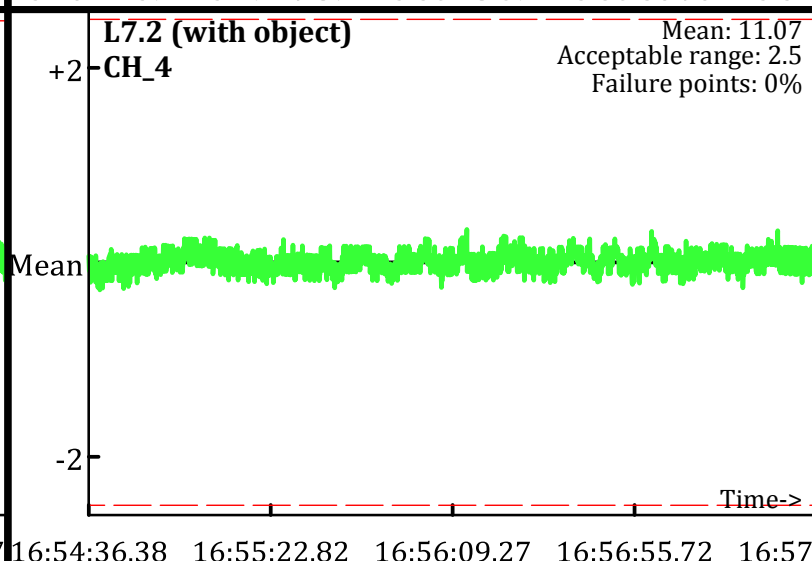Acceptable range: 2.5
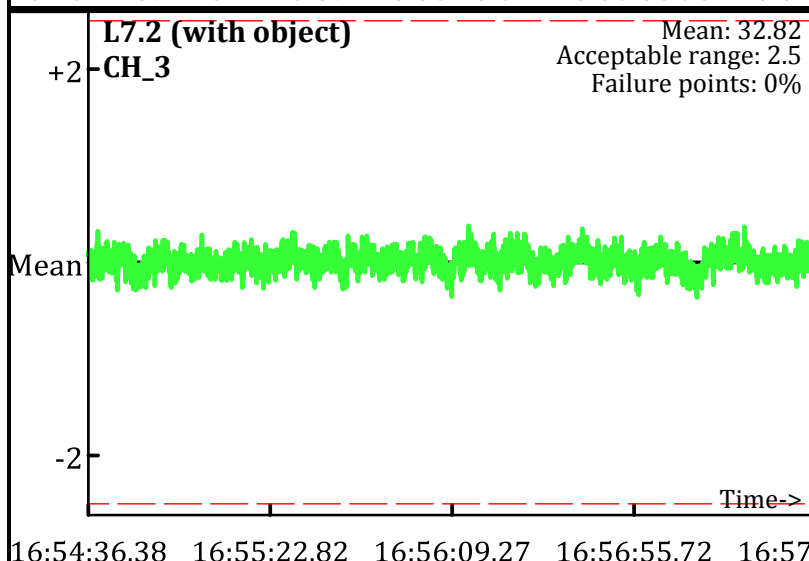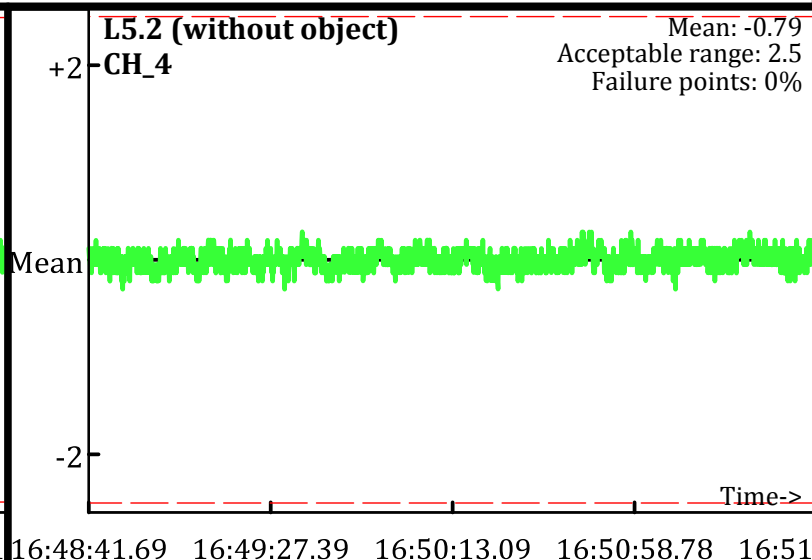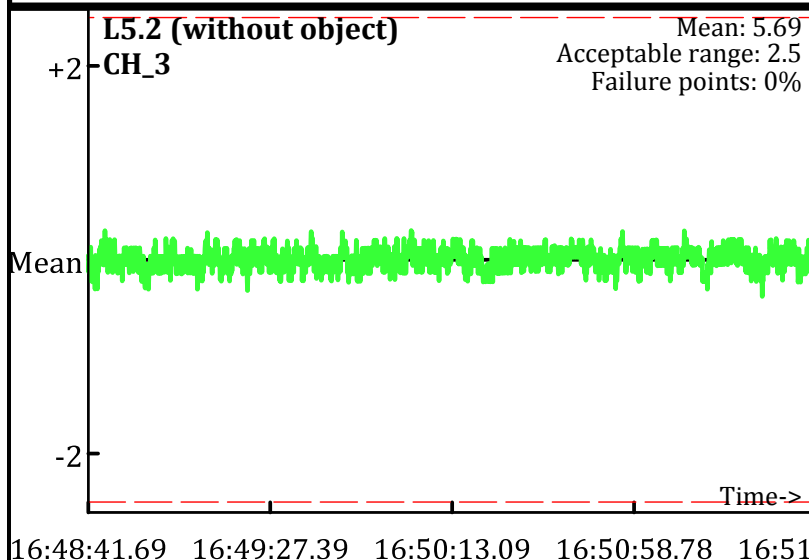Failure points: 0%

Time->

16:58:52.19   16:59:07.64   16:59:23.09   16:59:38.53

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

AM test
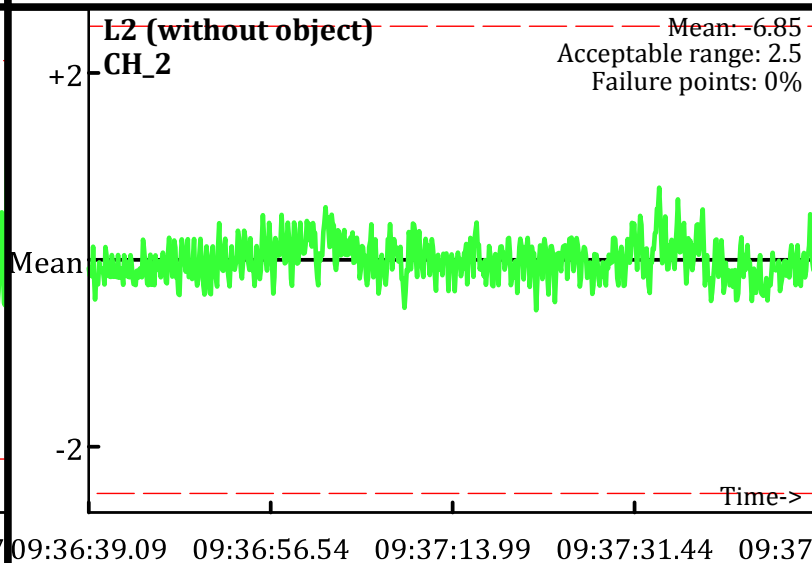Operator: PN & SH
Date: 1/13/2010

L0 (without object)
CH_1
Mean: -118.84
Acceptable range: 2.5
Failure points: 0%

Time->

09:28:42.58   09:29:28.01   09:30:13.44   09:30:58.87

L0 (without object)
CH_2
Mean: -6.69
Acceptable range: 2.5
Failure points: 0%

Time->

09:28:42.58   09:29:28.01   09:30:13.44   09:30:58.87

L1 (with object)
CH_1
Mean: -26.96
Acceptable range: 2.5
Failure points: 0%

Time->

09:32:55.30   09:33:41.22   09:34:27.14   09:35:13.06   09:35

L1 (with object)
CH_2
Mean: 50.74
Acceptable range: 2.5
Failure points: 0%

Time->

09:32:55.30   09:33:41.22   09:34:27.14   09:35:13.06   09:35

L2 (without object)
CH_1
Mean: -119.42
Acceptable range: 2.5
Failure points: 0%

Time->

09:36:39.09   09:36:56.54   09:37:13.99   09:37:31.44   09:37

L2 (without object)
CH_2
Mean: -6.85
Acceptable range: 2.5
Failure points: 0%

Time->

09:36:39.09   09:36:56.54   09:37:13.99   09:37:31.44   09:37

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
‒ ‒ ‒ Acceptable limits

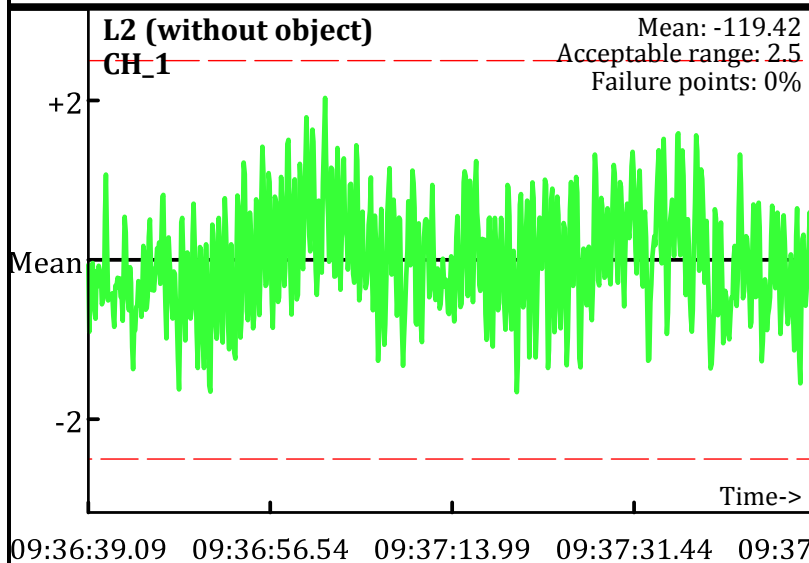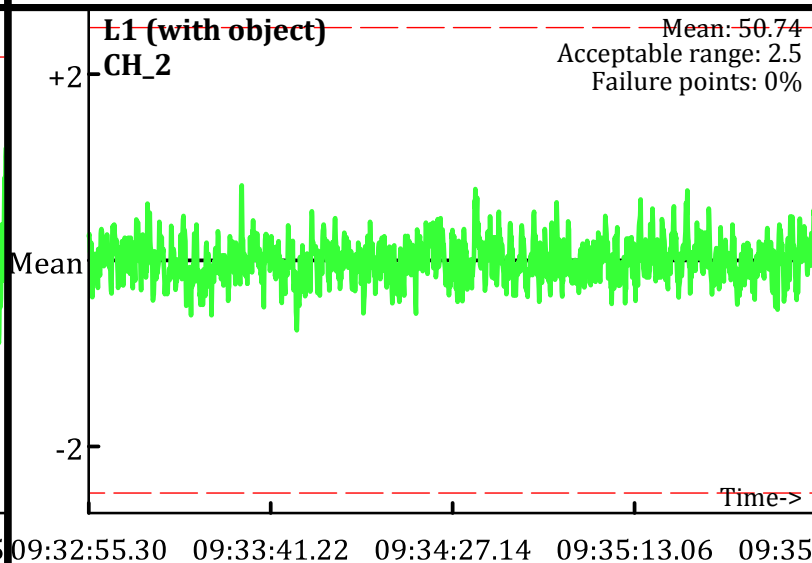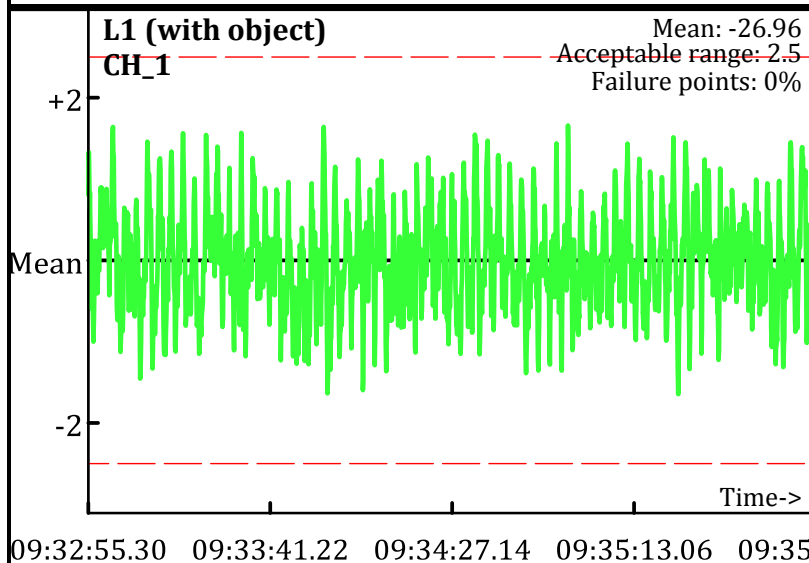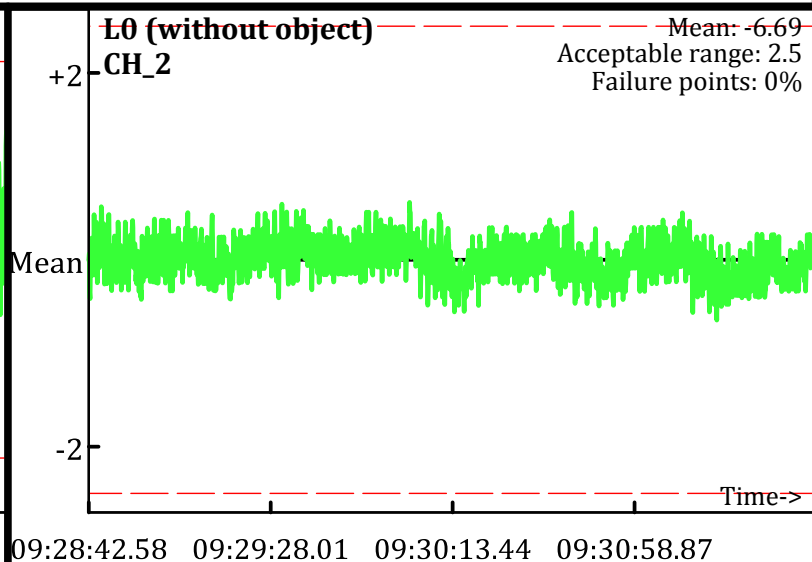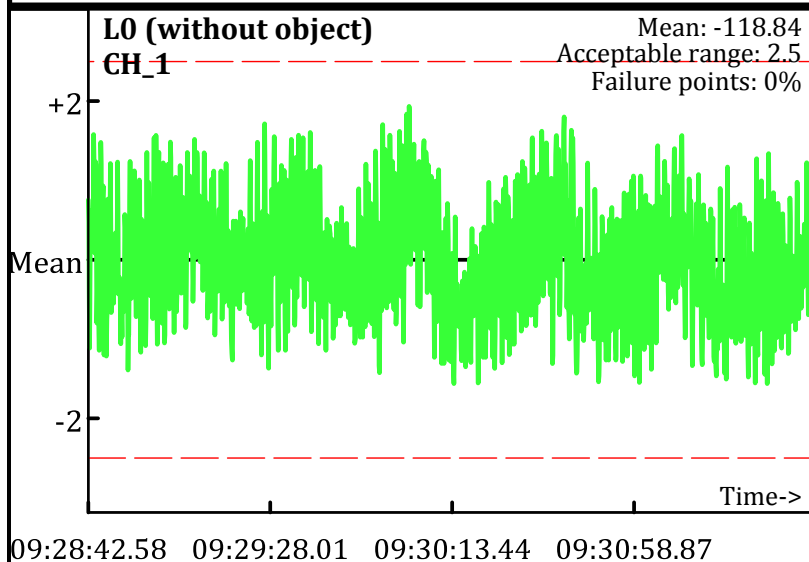AM test
Operator: PN & SH
Date: 1/13/2010

L0 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 4.26
Acceptable range: 2.5
Failure points: 0%

09:28:42.58   09:29:28.01   09:30:13.44   09:30:58.87

L0 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.26
Acceptable range: 2.5
Failure points: 0%

09:28:42.58   09:29:28.01   09:30:13.44   09:30:58.87

L1 (with object)
CH_3
+2
Mean
-2
Time->

Mean: 34.09
Acceptable range: 2.5
Failure points: 0%

09:32:55.30   09:33:41.22   09:34:27.14   09:35:13.06   09:35

L1 (with object)
CH_4
+2
Mean
-2
Time->

Mean: 10.71
Acceptable range: 2.5
Failure points: 0%

09:32:55.30   09:33:41.22   09:34:27.14   09:35:13.06   09:35

L2 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 4.21
Acceptable range: 2.5
Failure points: 0%

09:36:39.09   09:36:56.54   09:37:13.99   09:37:31.44   09:37

L2 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.39
Acceptable range: 2.5
Failure points: 0%

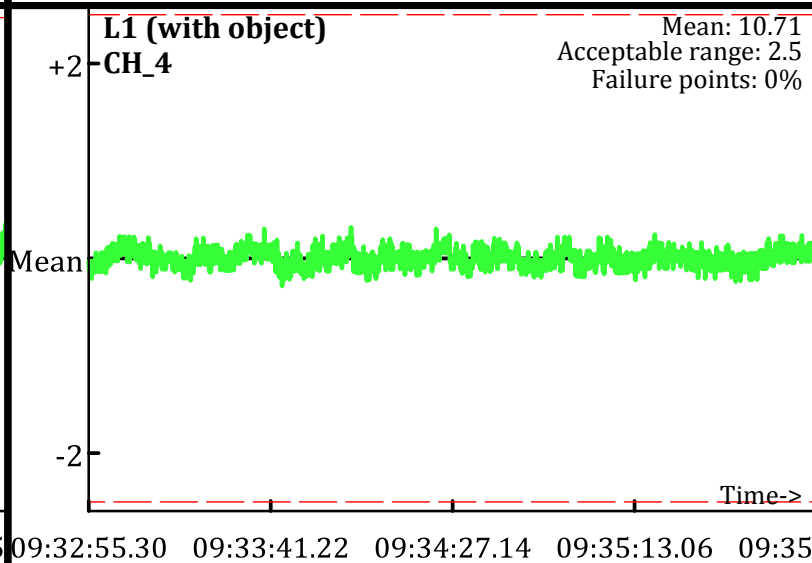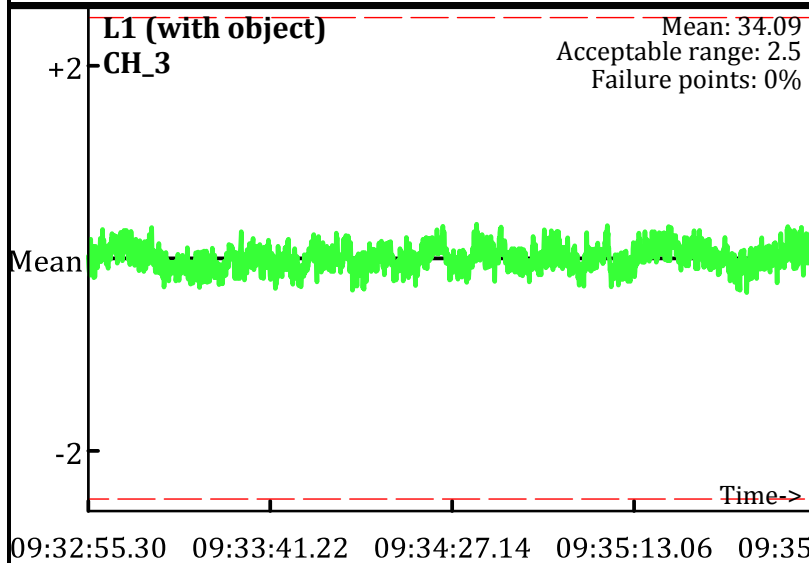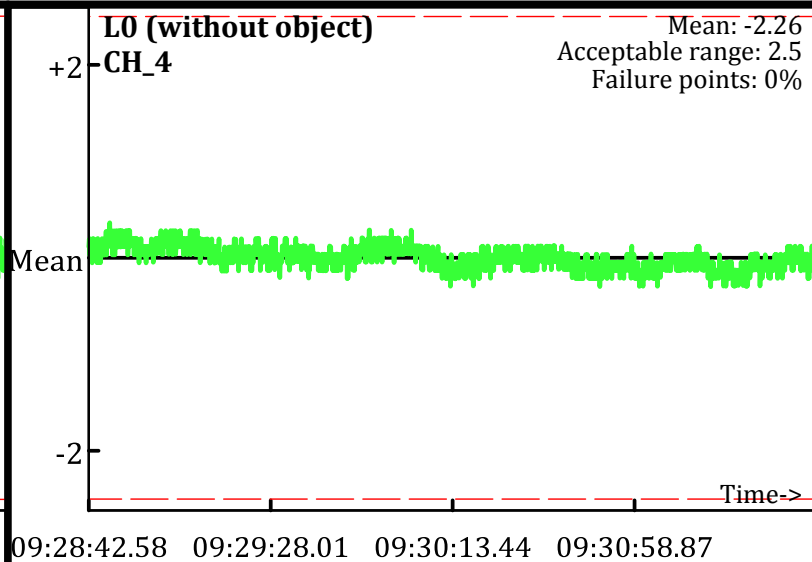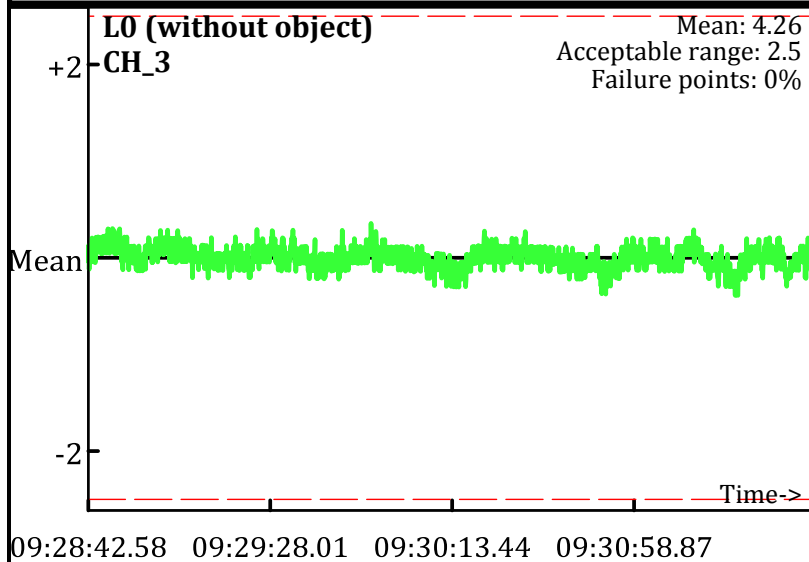09:36:39.09   09:36:56.54   09:37:13.99   09:37:31.44   09:37

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
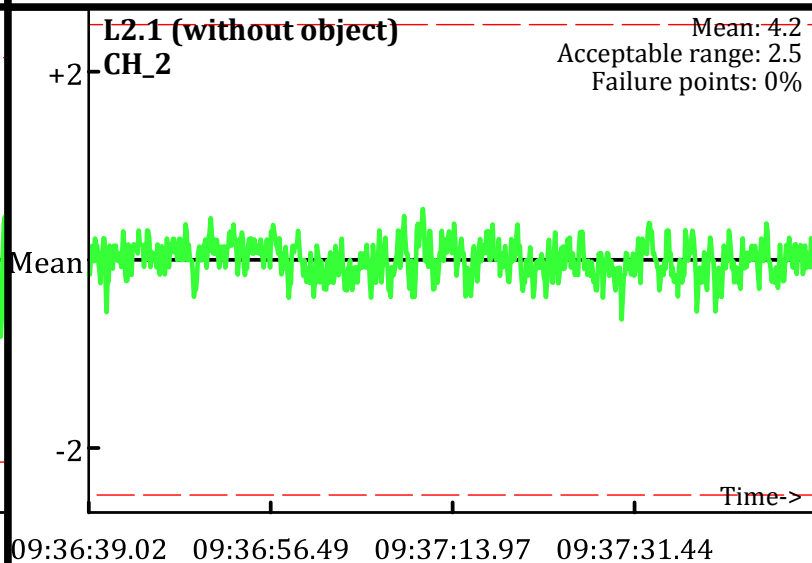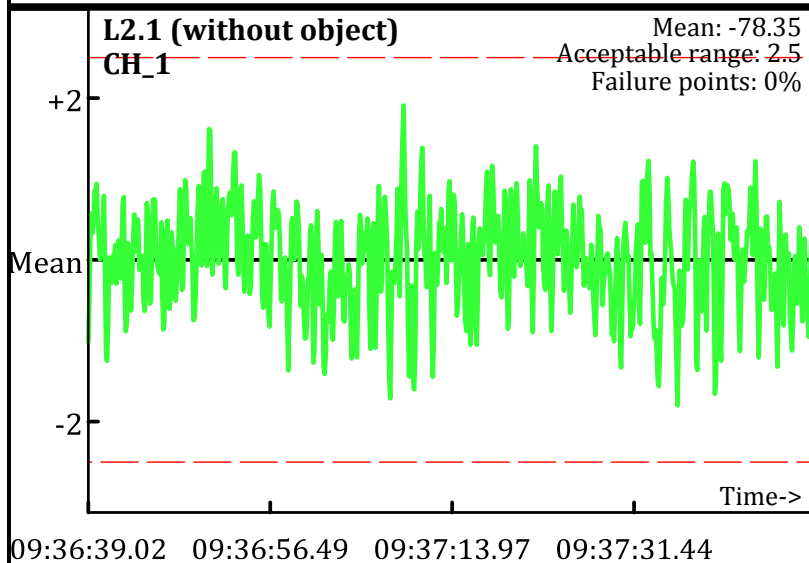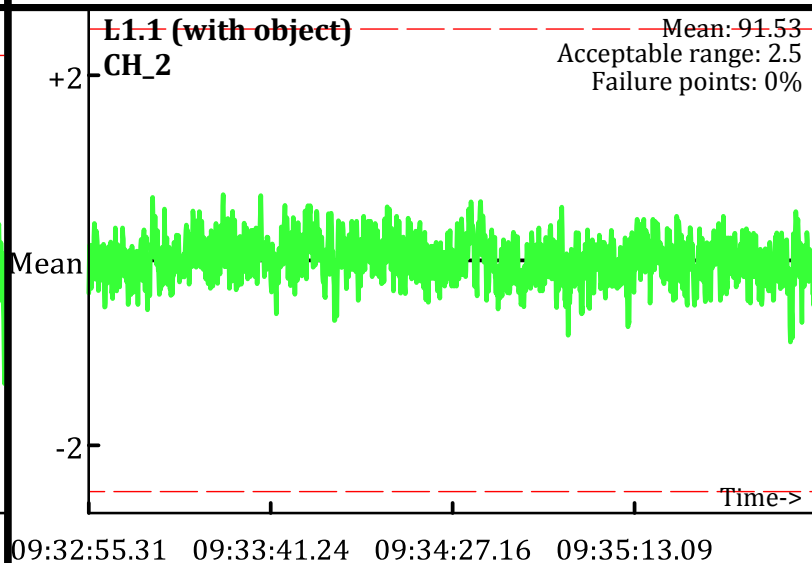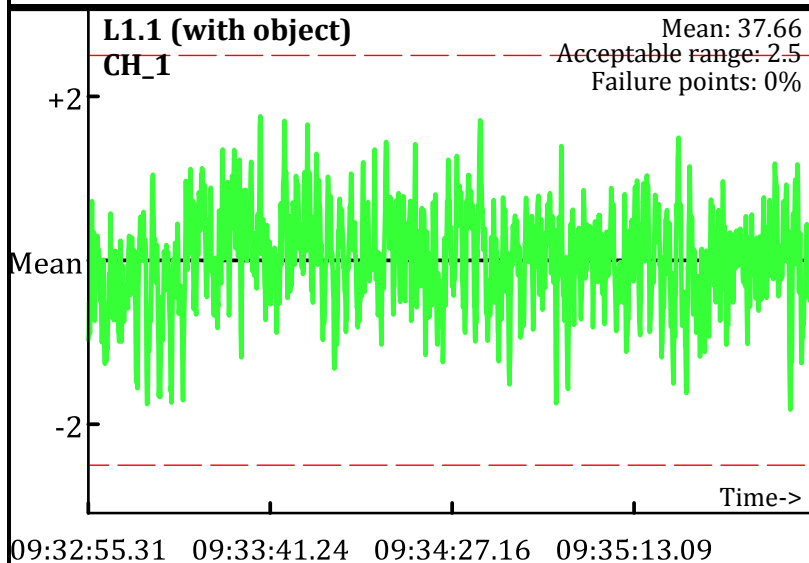Operator: PN & SH
Date: 1/13/2010

L0.1 (without object)
CH_1

Mean: -79.41
Acceptable range: 2.5
Failure points: 0%

Time->

09:28:42.52   09:29:27.96   09:30:13.41   09:30:58.86

L0.1 (without object)
CH_2

Mean: 3.99
Acceptable range: 2.5
Failure points: 0%

Time->

09:28:42.52   09:29:27.96   09:30:13.41   09:30:58.86

L1.1 (with object)
CH_1

Mean: 37.66
Acceptable range: 2.5
Failure points: 0%

Time->

09:32:55.31   09:33:41.24   09:34:27.16   09:35:13.09

L1.1 (with object)
CH_2

Mean: 91.53
Acceptable range: 2.5
Failure points: 0%

Time->

09:32:55.31   09:33:41.24   09:34:27.16   09:35:13.09

L2.1 (without object)
CH_1

Mean: -78.35
Acceptable range: 2.5
Failure points: 0%

Time->

09:36:39.02   09:36:56.49   09:37:13.97   09:37:31.44

L2.1 (without object)
CH_2

Mean: 4.2
Acceptable range: 2.5
Failure points: 0%

Time->

09:36:39.02   09:36:56.49   09:37:13.97   09:37:31.44

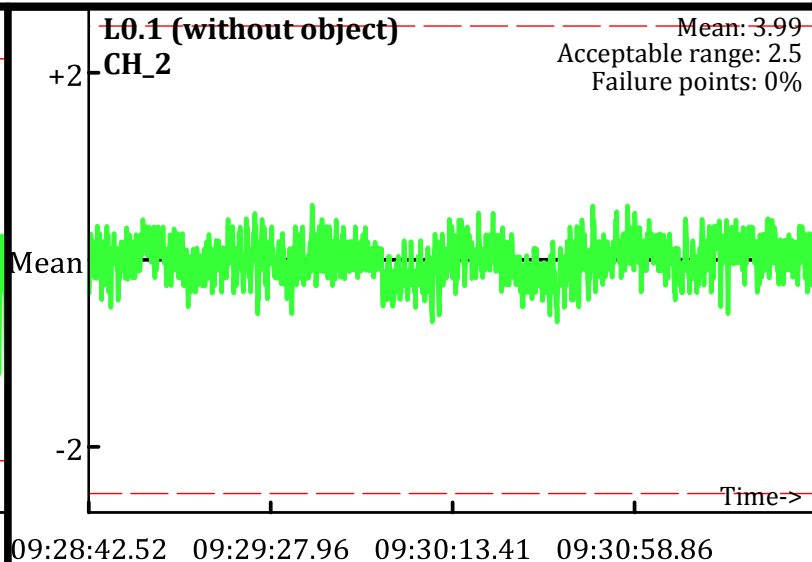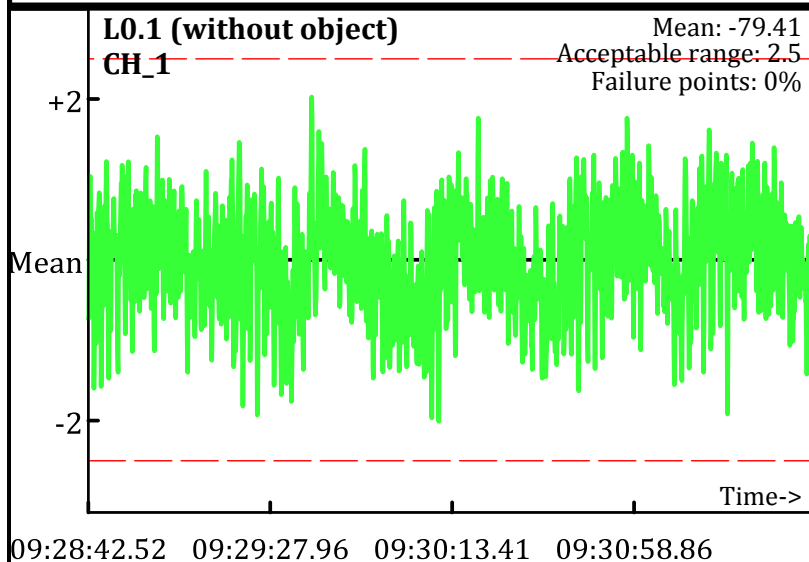Database: D:\Projects_QCReports_Ord_Data\011310\QC\011310_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
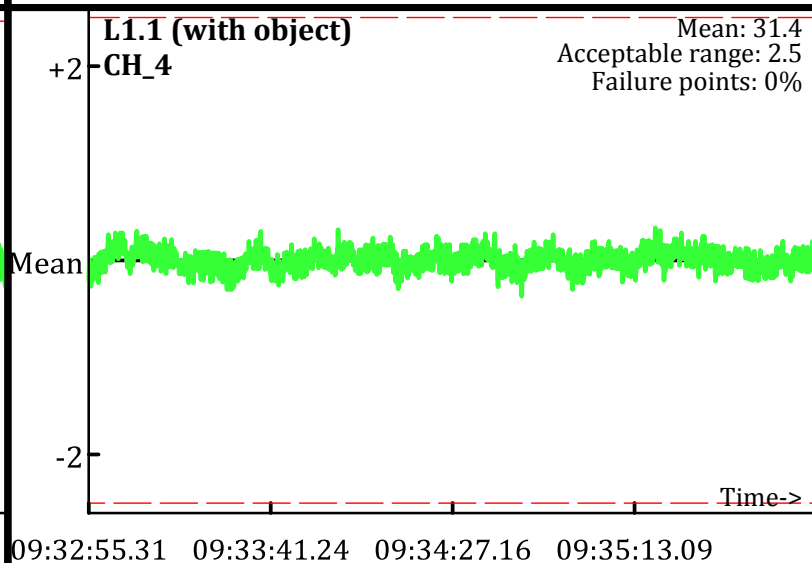Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

L0.1 (without object)
CH_3
Mean: 9.98
Acceptable range: 2.5
Failure points: 0%

09:28:42.52   09:29:27.96   09:30:13.41   09:30:58.86

L0.1 (without object)
CH_4
Mean: 1.43
Acceptable range: 2.5
Failure points: 0%

09:28:42.52   09:29:27.96   09:30:13.41   09:30:58.86

L1.1 (with object)
CH_3
Mean: 65.92
Acceptable range: 2.5
Failure points: 0%

09:32:55.31   09:33:41.24   09:34:27.16   09:35:13.09

L1.1 (with object)
CH_4
Mean: 31.4
Acceptable range: 2.5
Failure points: 0%

09:32:55.31   09:33:41.24   09:34:27.16   09:35:13.09

L2.1 (without object)
CH_3
Mean: 10.06
Acceptable range: 2.5
Failure points: 0%

09:36:39.02   09:36:56.49   09:37:13.97   09:37:31.44

L2.1 (without object)
CH_4
Mean: 1.45
Acceptable range: 2.5
Failure points: 0%

09:36:39.02   09:36:56.49   09:37:13.97   09:37:31.44
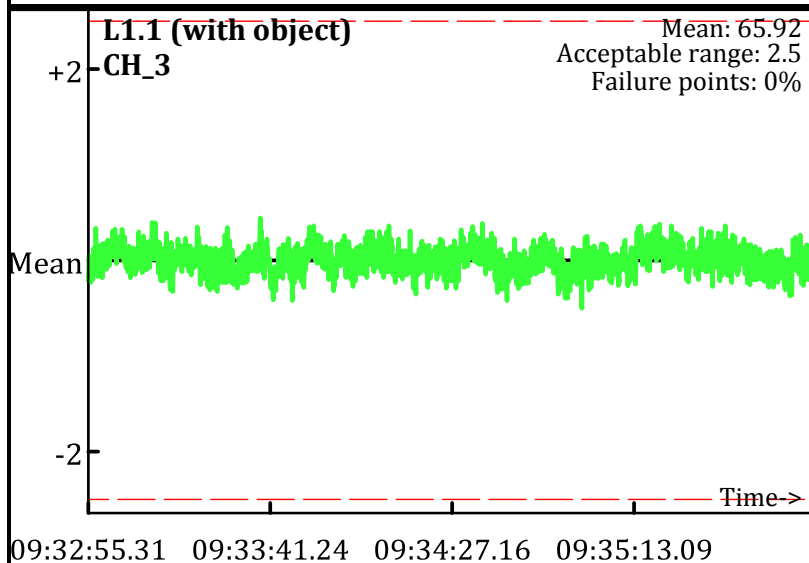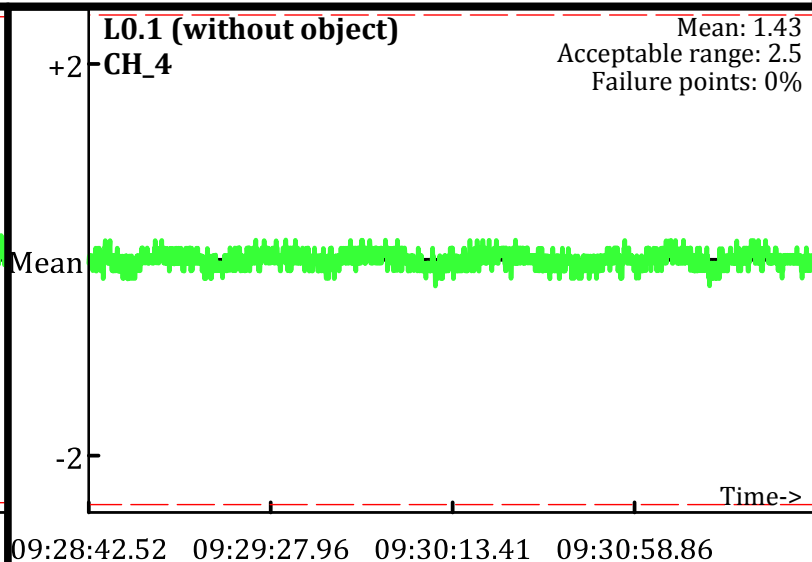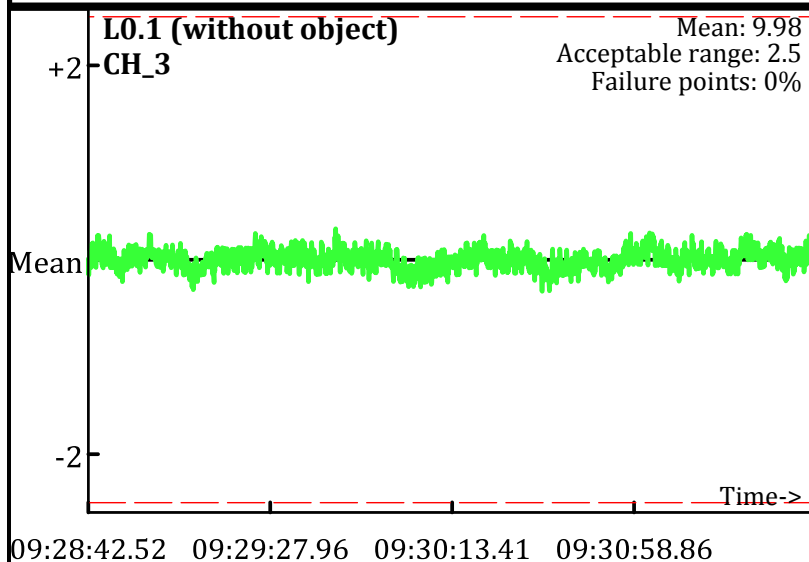
Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
– – – Acceptable limits

AM test
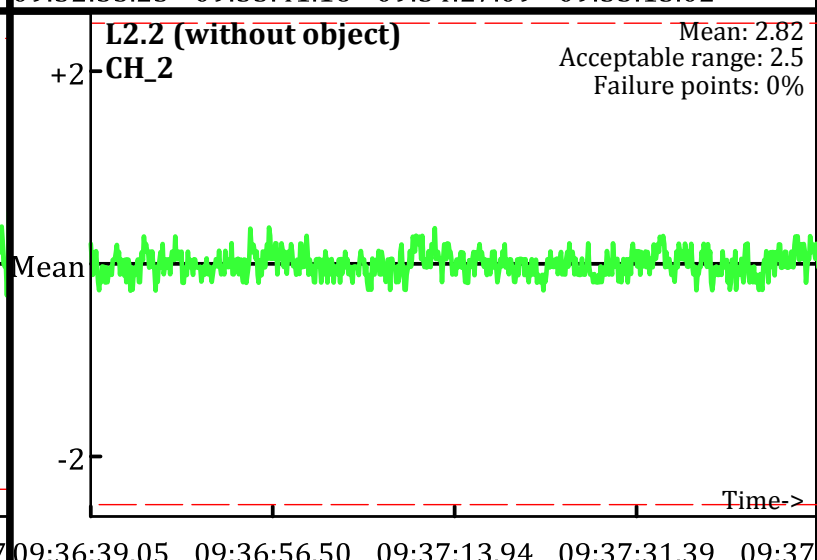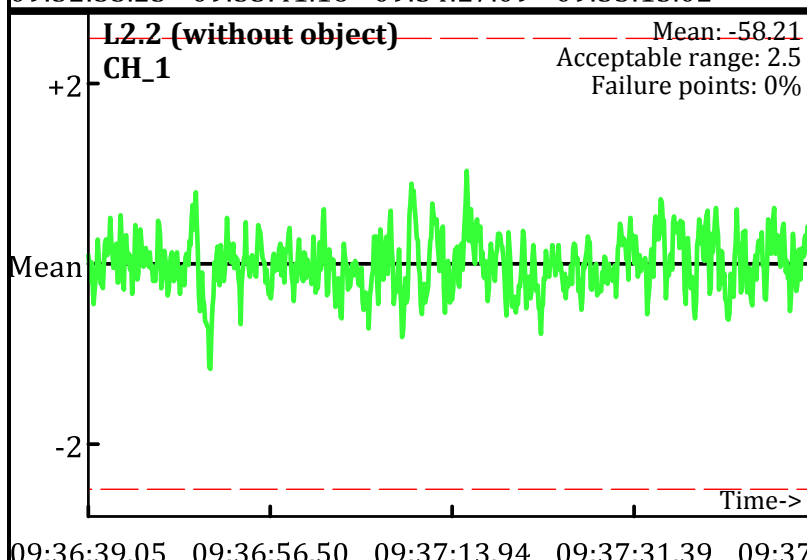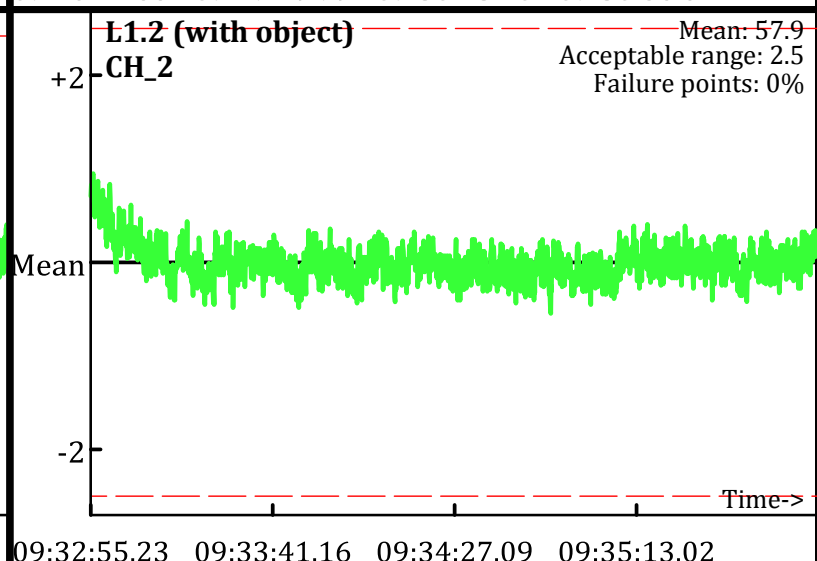Operator: PN & SH
Date: 1/13/2010

L0.2 (without object)
CH_1
Mean: -58.75
Acceptable range: 2.5
Failure points: 0%

09:28:42.55 09:29:27.97 09:30:13.40 09:30:58.82

L0.2 (without object)
CH_2
Mean: 2.59
Acceptable range: 2.5
Failure points: 0%

09:28:42.55 09:29:27.97 09:30:13.40 09:30:58.82

L1.2 (with object)
CH_1
Mean: 30.46
Acceptable range: 2.5
Failure points: 0%

09:32:55.23 09:33:41.16 09:34:27.09 09:35:13.02

L1.2 (with object)
CH_2
Mean: 57.9
Acceptable range: 2.5
Failure points: 0%

09:32:55.23 09:33:41.16 09:34:27.09 09:35:13.02

L2.2 (without object)
CH_1
Mean: -58.21
Acceptable range: 2.5
Failure points: 0%

09:36:39.05 09:36:56.50 09:37:13.94 09:37:31.39 09:37

L2.2 (without object)
CH_2
Mean: 2.82
Acceptable range: 2.5
Failure points: 0%

09:36:39.05 09:36:56.50 09:37:13.94 09:37:31.39 09:37

Database: D:\Projects_QCReports_Ord_Data\011310\QC\011310_TA_QC.gdb
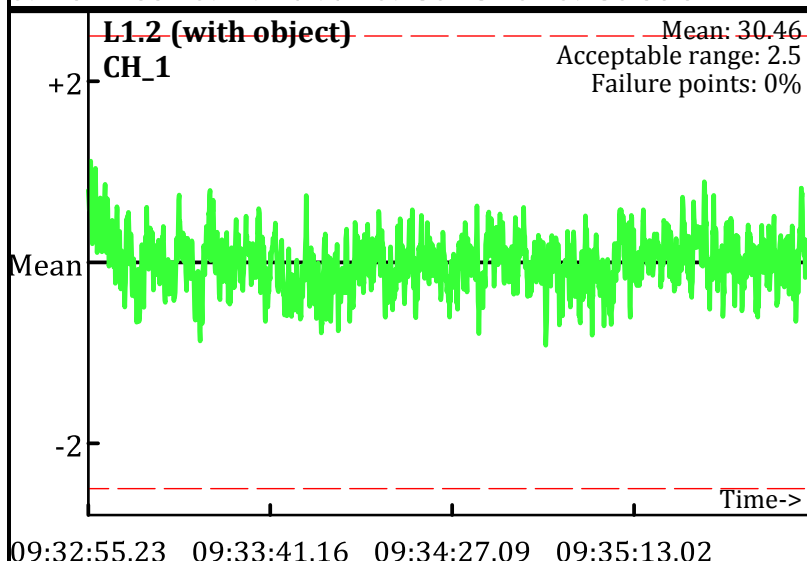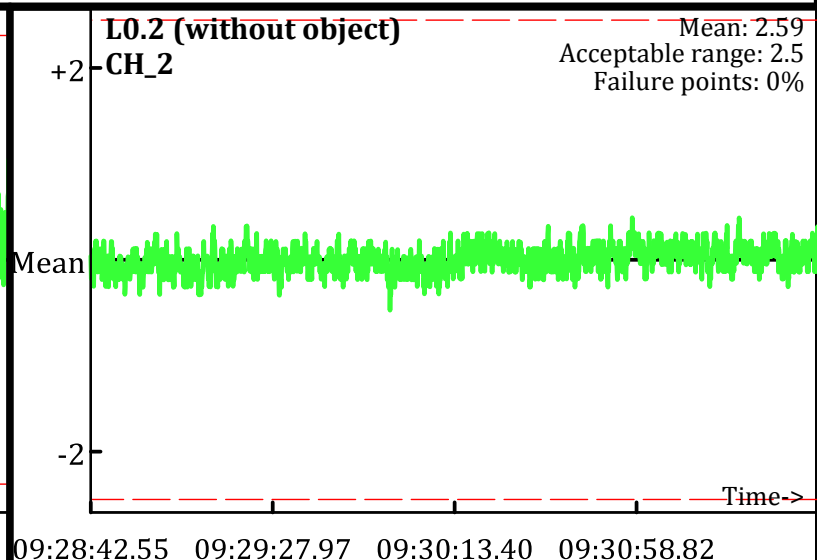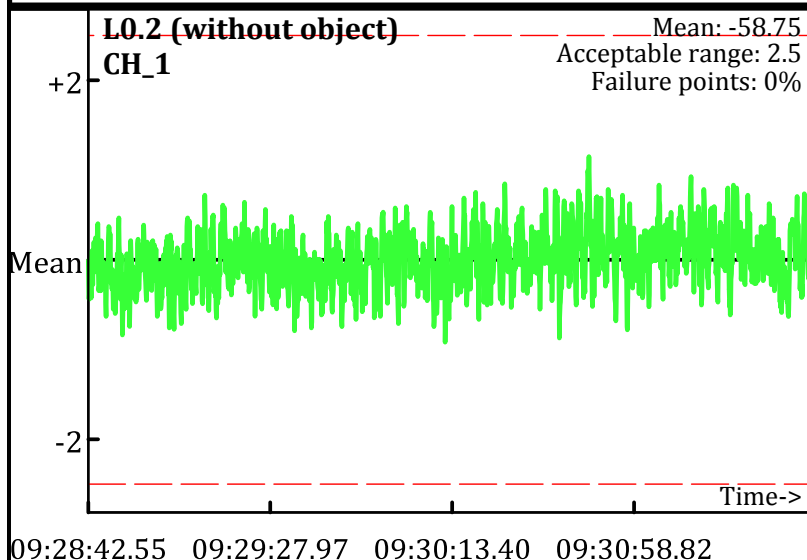Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

AM test
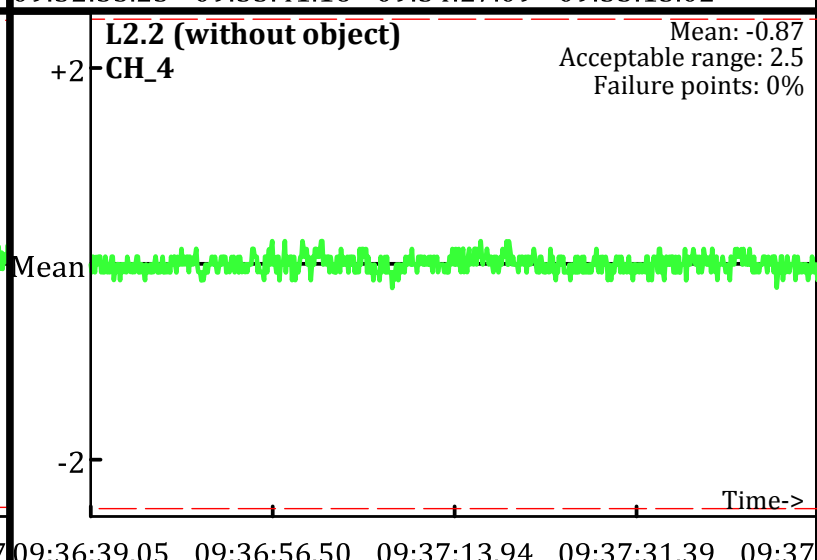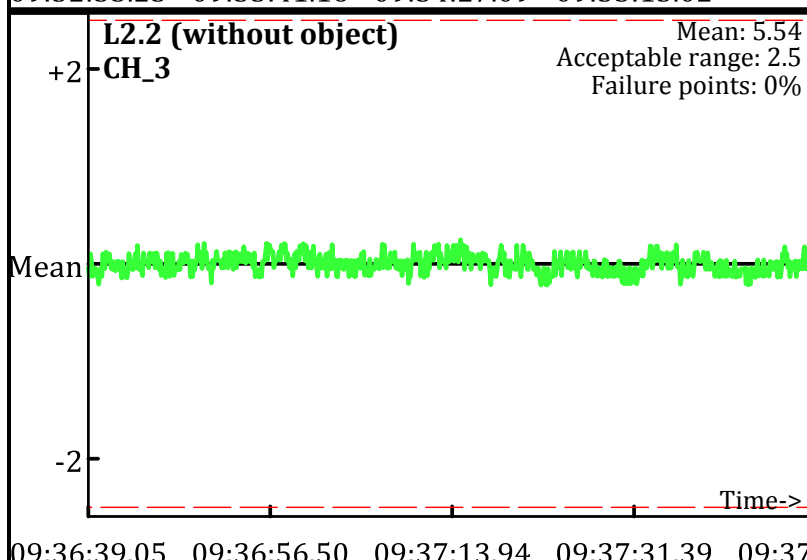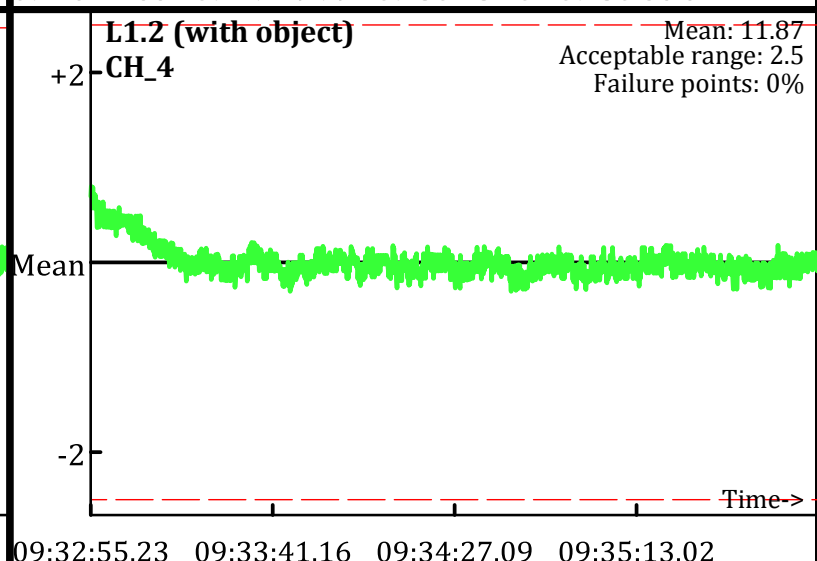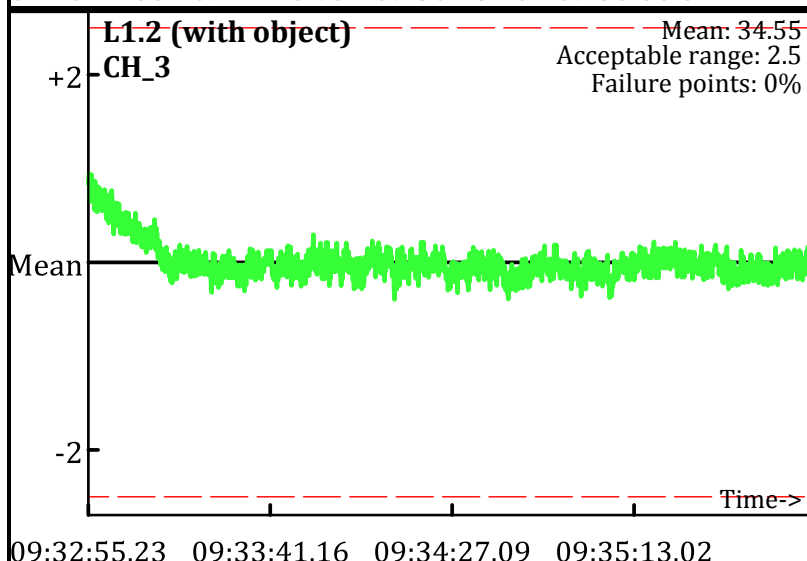Operator: PN & SH
Date: 1/13/2010

L0.2 (without object)
CH_3
Mean: 5.41
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:28:42.55 09:29:27.97 09:30:13.40 09:30:58.82

L0.2 (without object)
CH_4
Mean: -0.94
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:28:42.55 09:29:27.97 09:30:13.40 09:30:58.82

L1.2 (with object)
CH_3
Mean: 34.55
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:32:55.23 09:33:41.16 09:34:27.09 09:35:13.02

L1.2 (with object)
CH_4
Mean: 11.87
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:32:55.23 09:33:41.16 09:34:27.09 09:35:13.02

L2.2 (without object)
CH_3
Mean: 5.54
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:36:39.05 09:36:56.50 09:37:13.94 09:37:31.39 09:37

L2.2 (without object)
CH_4
Mean: -0.87
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
09:36:39.05 09:36:56.50 09:37:13.94 09:37:31.39 09:37

Database: D:\Projects_QCReports_Ord_Data\011310\QC\011310_TA_QC.gdb
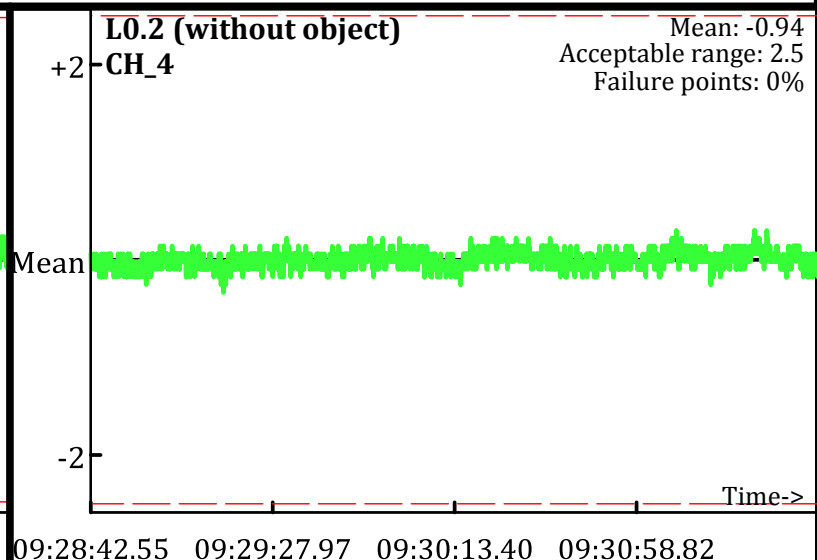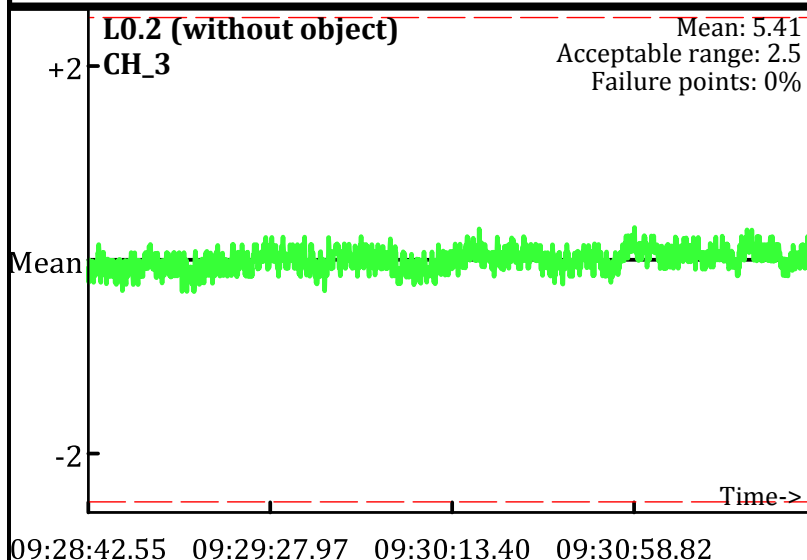Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits
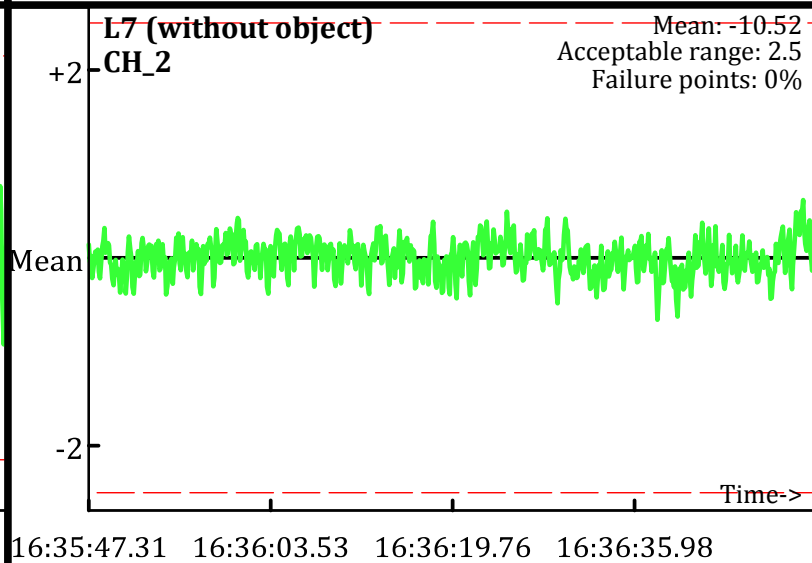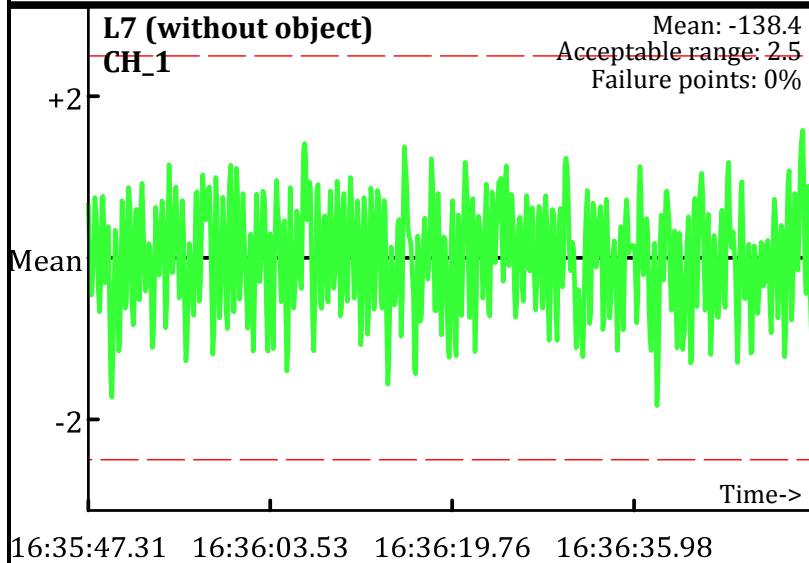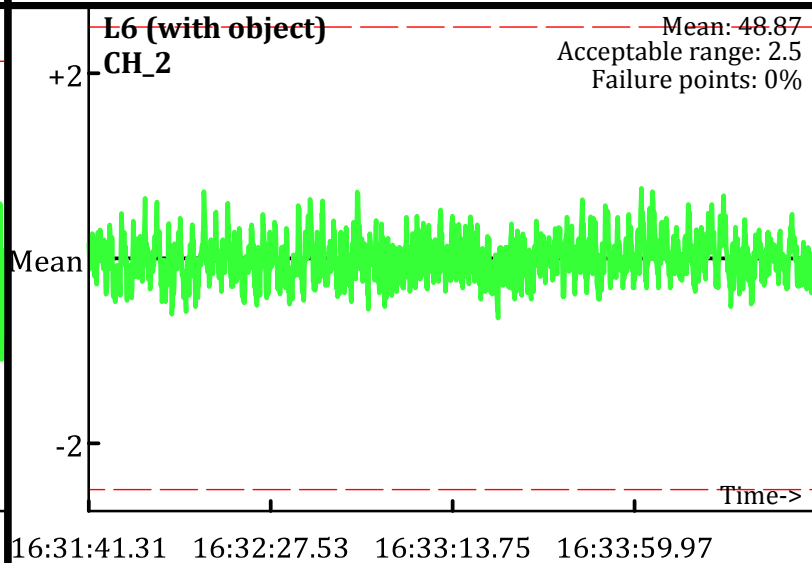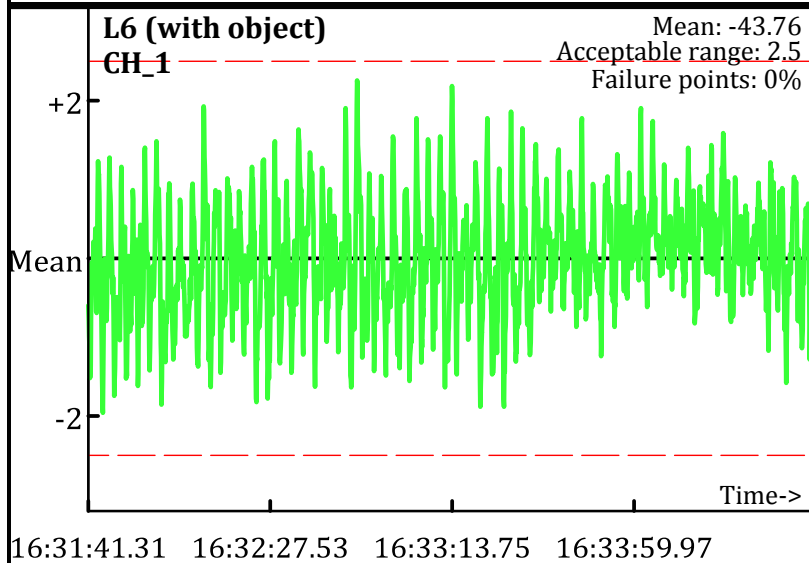
PM test
Operator: PN & SH
Date: 1/13/2010

L5 (without object)
CH_1
Mean: -140.13
Acceptable range: 2.5
Failure points: 0%

L5 (without object)
CH_2
Mean: -10.35
Acceptable range: 2.5
Failure points: 0%

L6 (with object)
CH_1
Mean: -43.76
Acceptable range: 2.5
Failure points: 0%

L6 (with object)
CH_2
Mean: 48.87
Acceptable range: 2.5
Failure points: 0%

L7 (without object)
CH_1
Mean: -138.4
Acceptable range: 2.5
Failure points: 0%

L7 (without object)
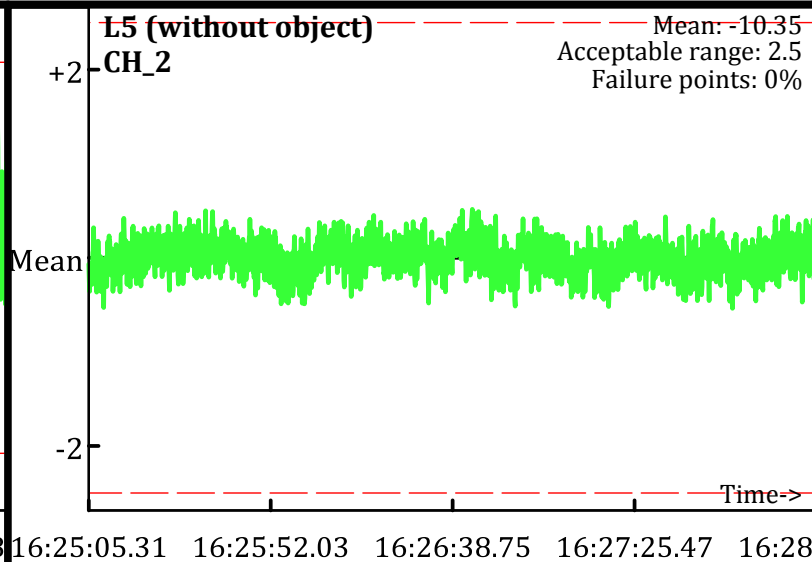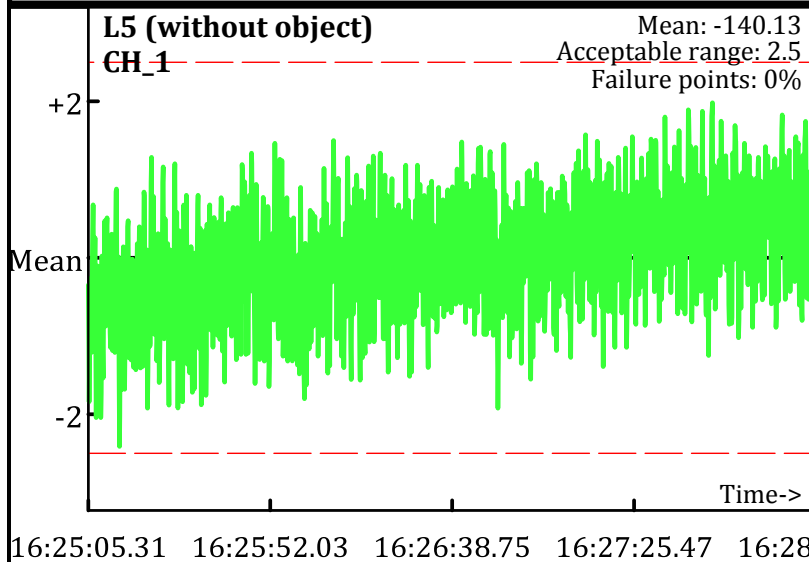**CH_2**
Mean: -10.52
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
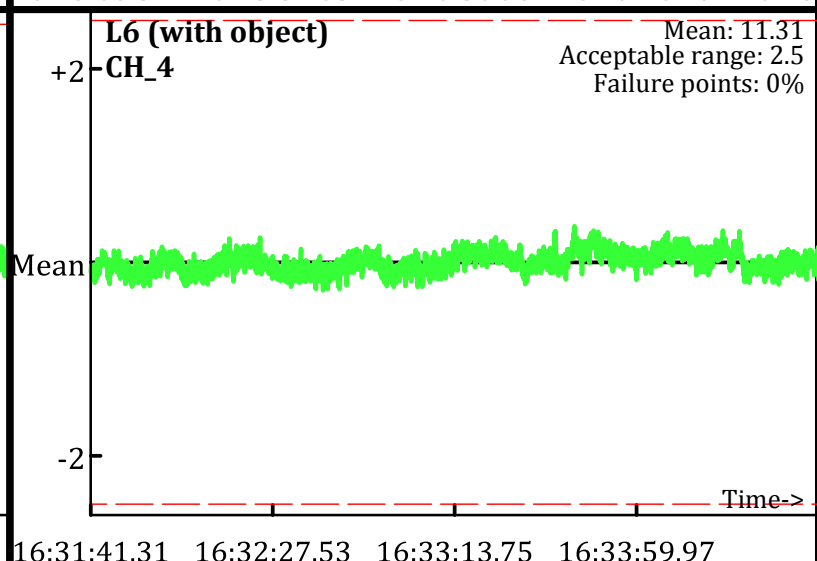Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/13/2010

L5 (without object)
CH_3
Mean: 3.37
Acceptable range: 2.5
Failure points: 0%

16:25:05.31 16:25:52.03 16:26:38.75 16:27:25.47 16:28

L5 (without object)
CH_4
Mean: -2.68
Acceptable range: 2.5
Failure points: 0%

16:25:05.31 16:25:52.03 16:26:38.75 16:27:25.47 16:28

L6 (with object)
CH_3
Mean: 34.49
Acceptable range: 2.5
Failure points: 0%

16:31:41.31 16:32:27.53 16:33:13.75 16:33:59.97

L6 (with object)
CH_4
Mean: 11.31
Acceptable range: 2.5
Failure points: 0%

16:31:41.31 16:32:27.53 16:33:13.75 16:33:59.97

L7 (without object)
CH_3
Mean: 3.3
Acceptable range: 2.5
Failure points: 0%

16:35:47.31 16:36:03.53 16:36:19.76 16:36:35.98

L7 (without object)
CH_4
Mean: -2.64
Acceptable range: 2.5
Failure points: 0%

16:35:47.31 16:36:03.53 16:36:19.76 16:36:35.98

Database: D:\Projects_QCReports_Ord_Data\011310\QC\011310_TA_QC.gdb
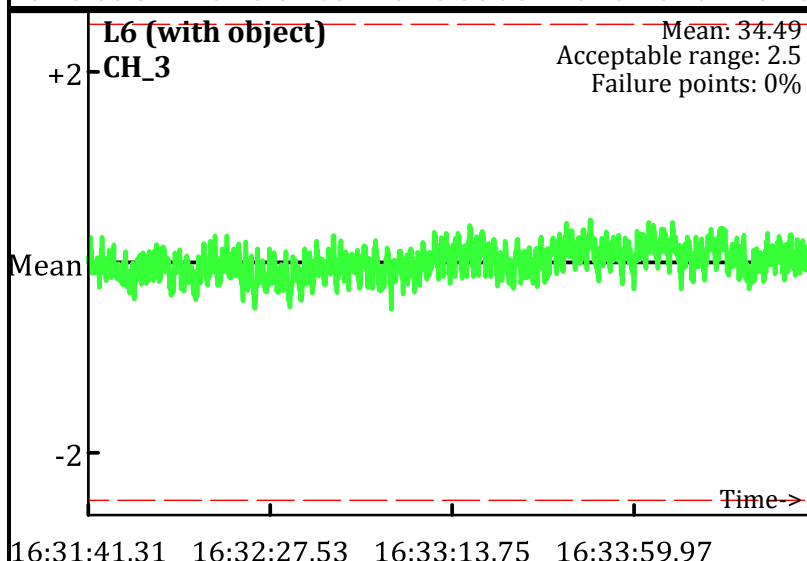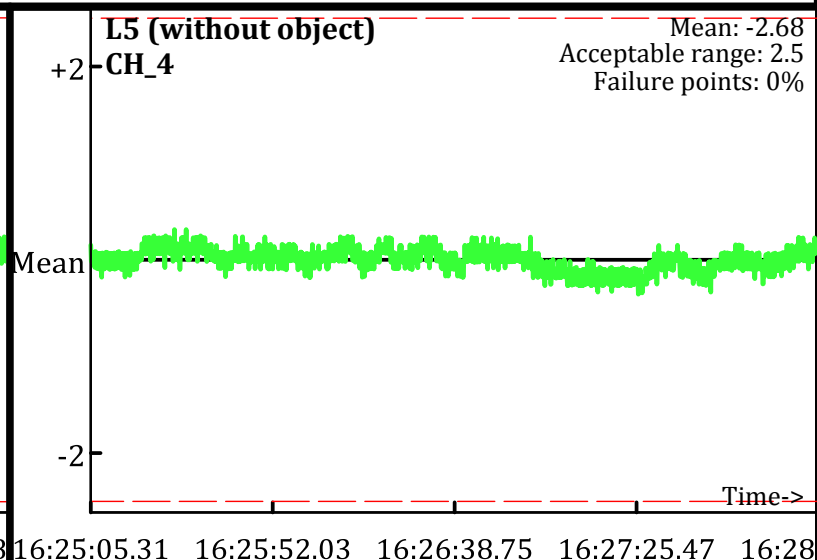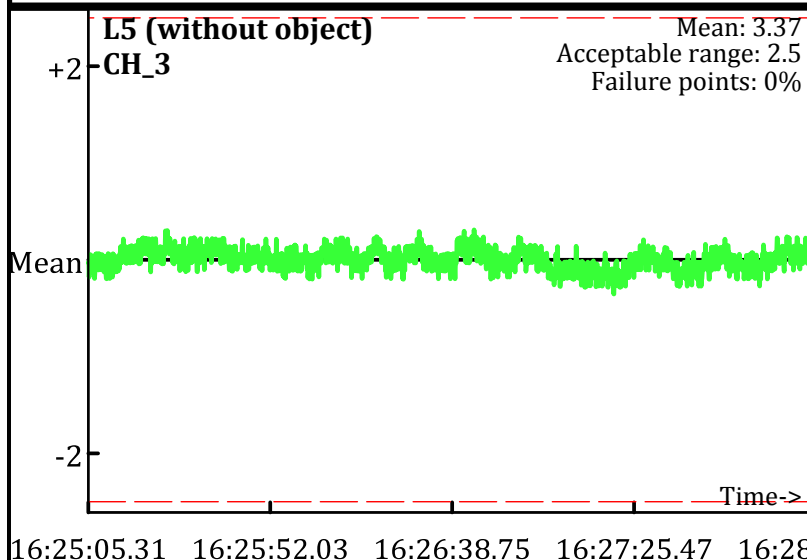Line Name: L5 L6 L7

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

PM test
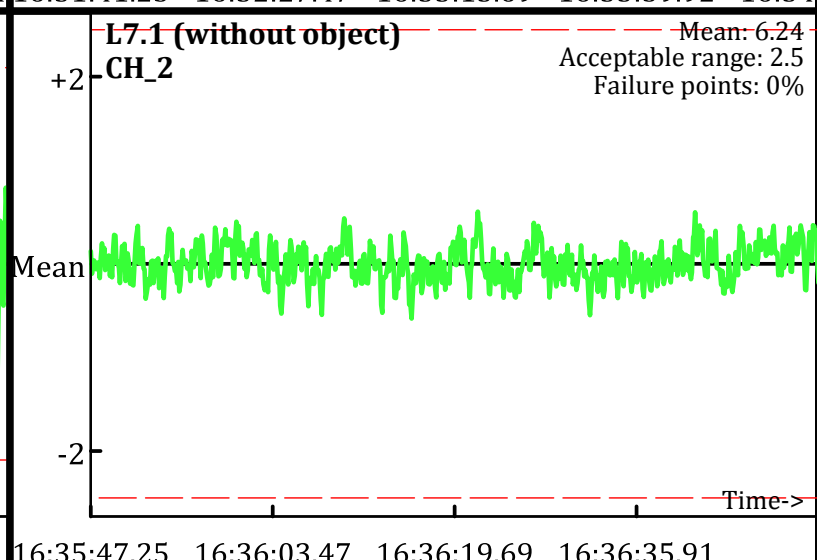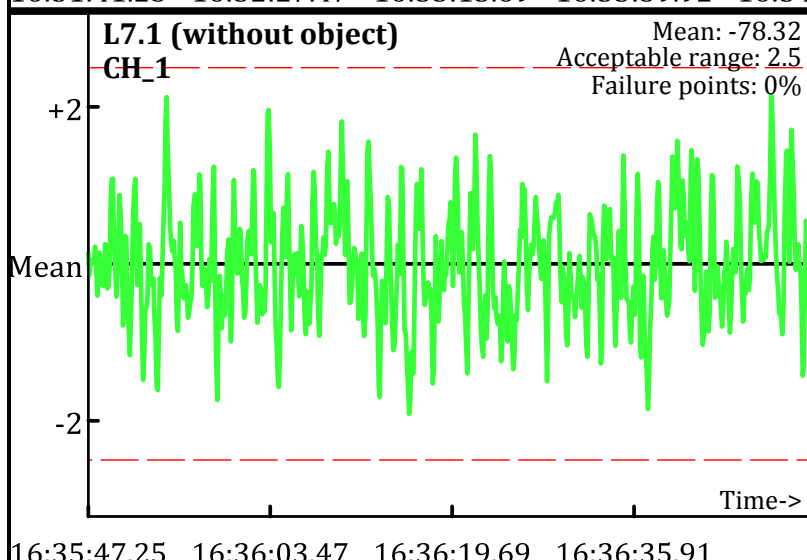Operator: PN & SH
Date: 1/13/2010

L5.1 (without object)
CH_1
Mean: -79.62
Acceptable range: 2.5
Failure points: 0%

L5.1 (without object)
CH_2
Mean: 6.39
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_1
Mean: 42.07
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_2
Mean: 98.55
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_1
Mean: -78.32
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
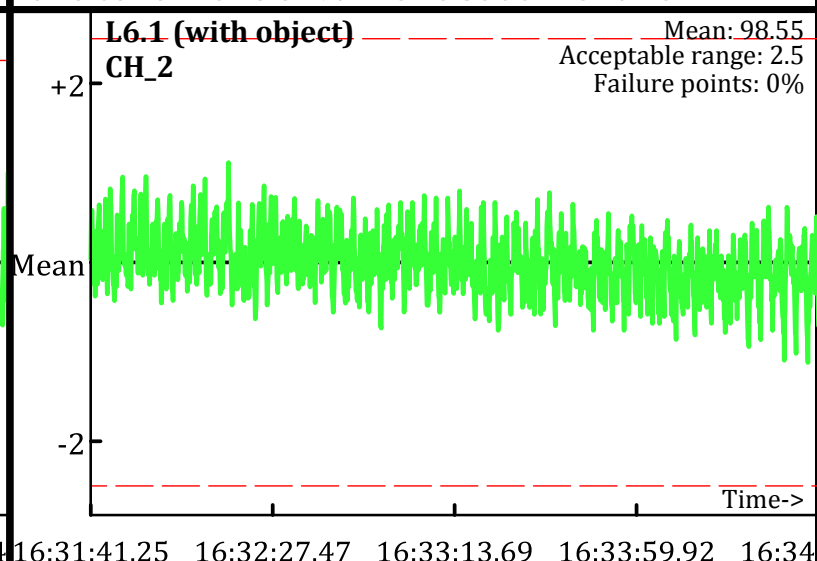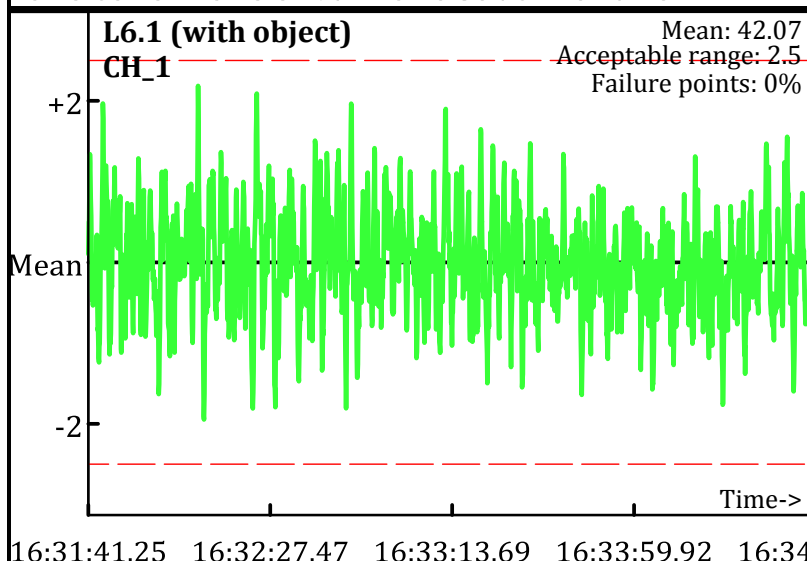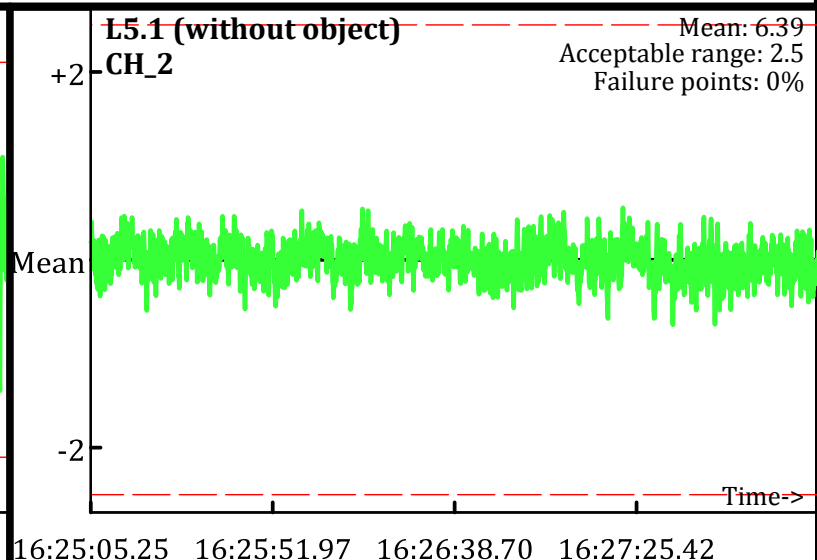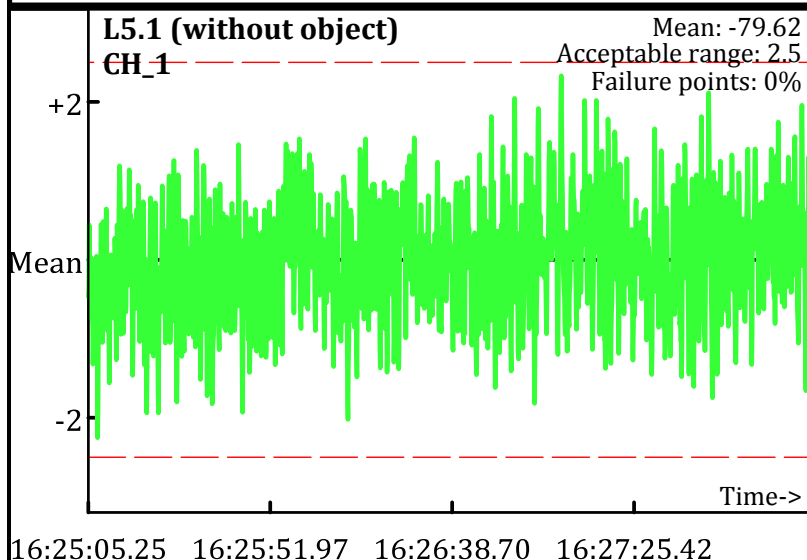CH_2
Mean: 6.24
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/13/2010

L5.1 (without object)
CH_3
Mean: 11.35
Acceptable range: 2.5
Failure points: 0%

L5.1 (without object)
CH_4
Mean: 2.21
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_3
Mean: 71.87
Acceptable range: 2.5
Failure points: 0%

L6.1 (with object)
CH_4
Mean: 35.23
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_3
Mean: 11.19
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_4
Mean: 2.09
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/13/2010
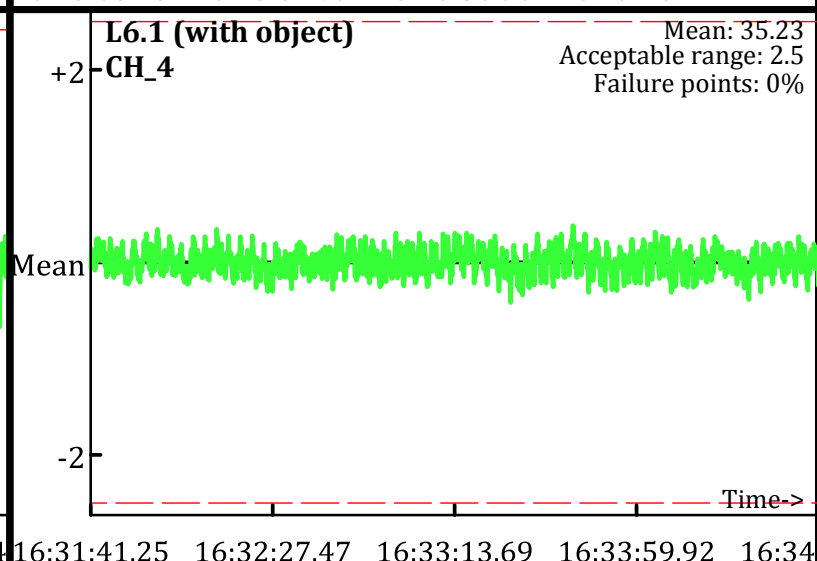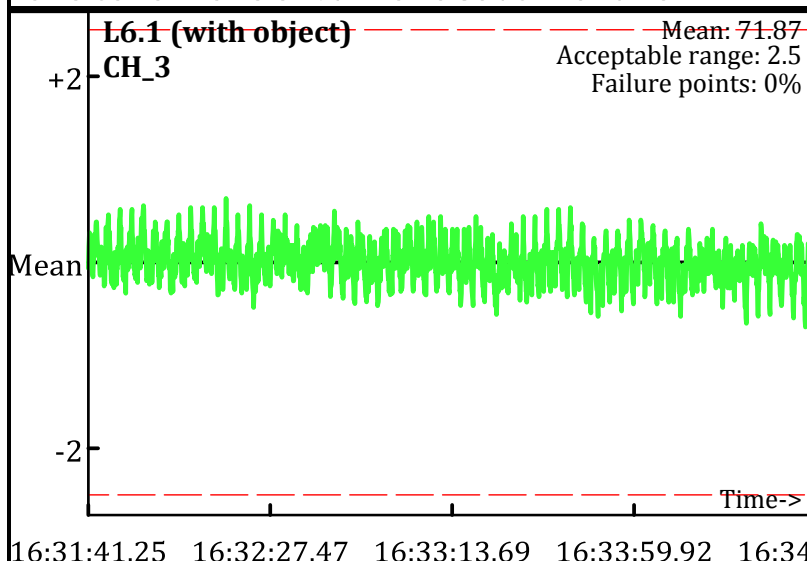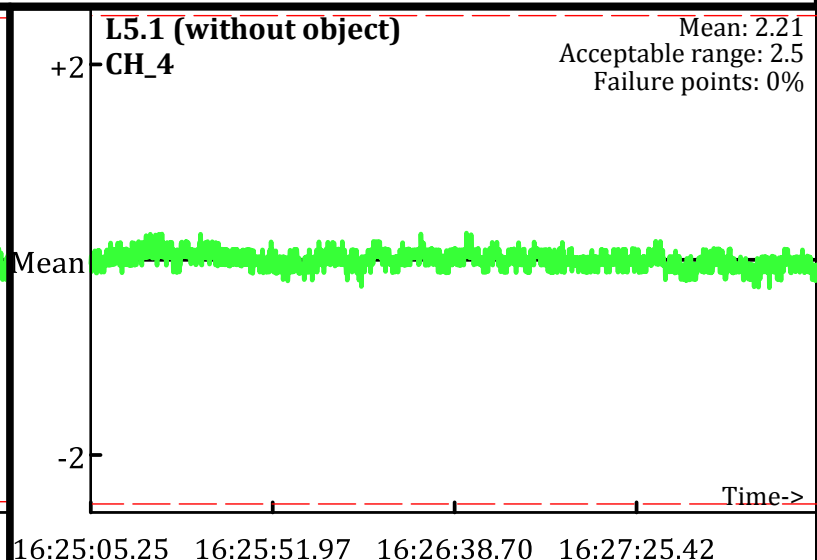

L5.2 (without object)
CH_1
Mean: -52.54
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_2
Mean: 7.15
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_1
Mean: 38.02
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_2
Mean: 63.68
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_1
Mean: -52.84
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_2
Mean: 6.81
Acceptable range: 2.5
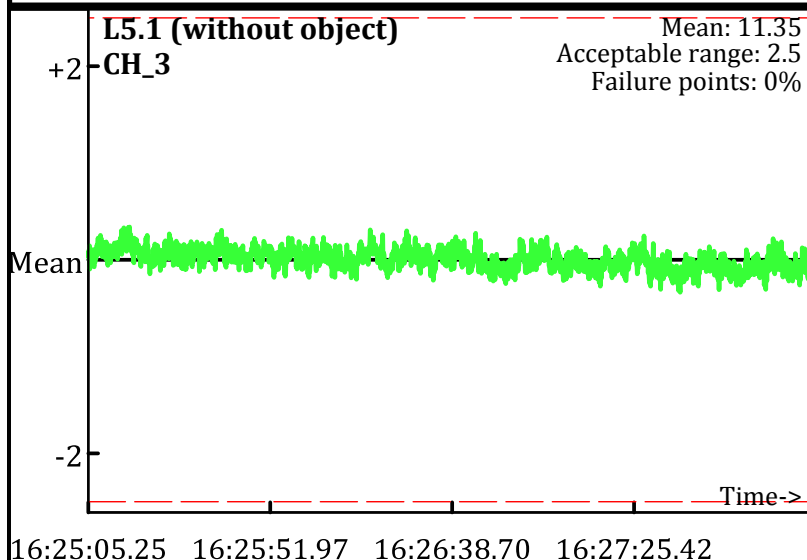Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
— — — Acceptable limits

PM test
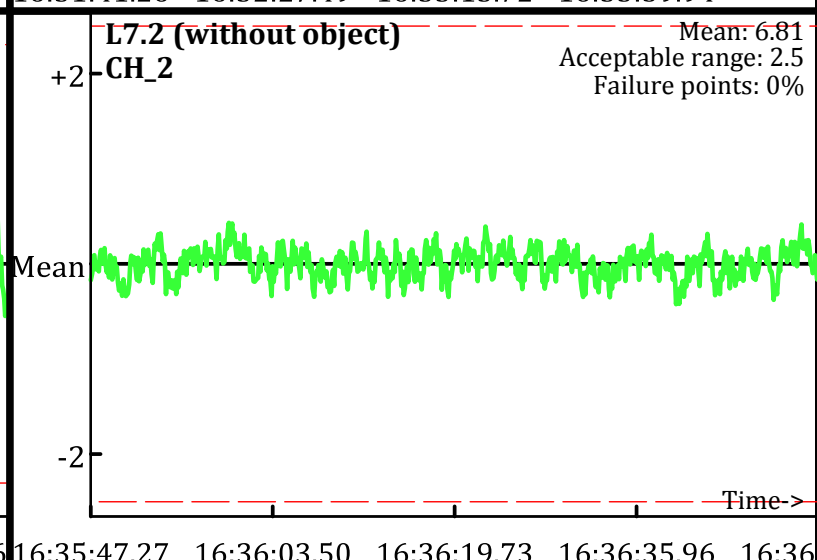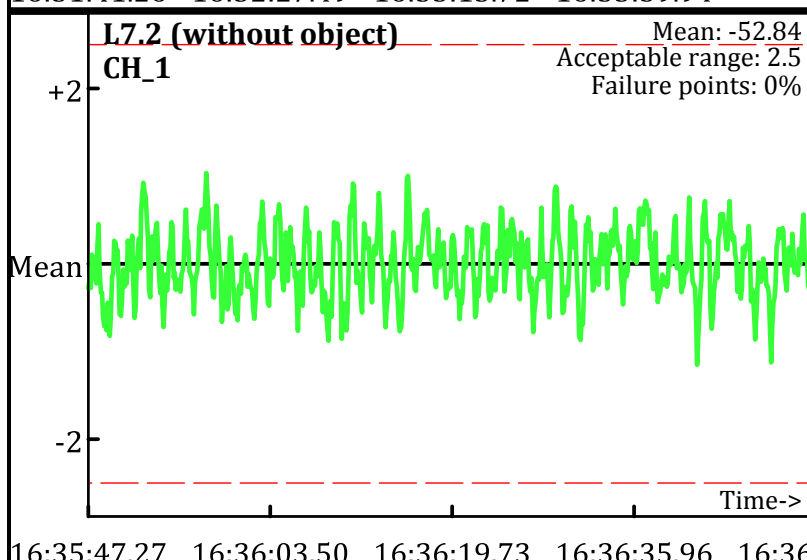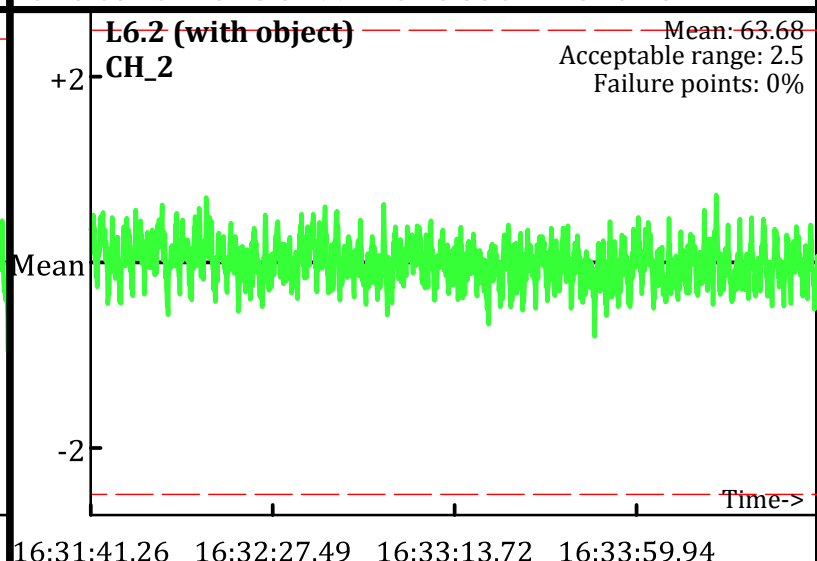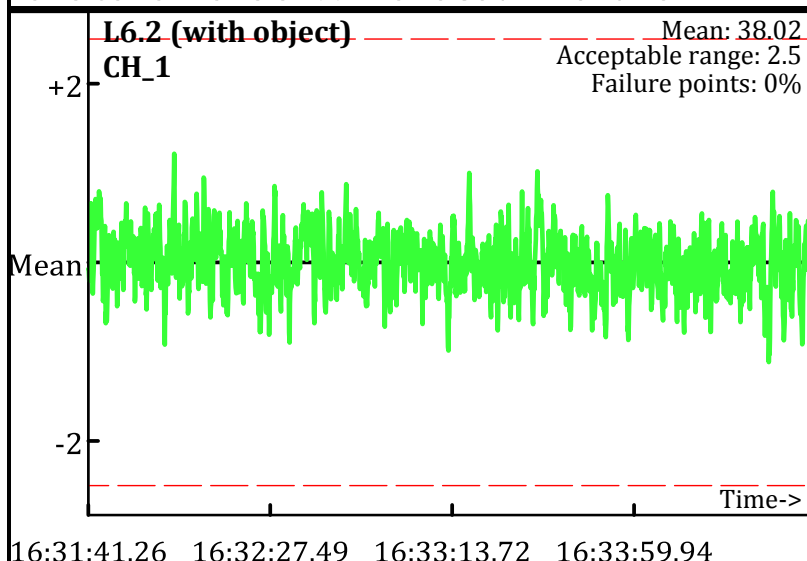Operator: PN & SH
Date: 1/13/2010

L5.2 (without object)
CH_3
Mean: 7.73
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_4
Mean: 0.33
Acceptable range: 2.5
Failure points: 0%

16:25:05.26 16:25:51.99 16:26:38.72 16:27:25.44
16:25:05.26 16:25:51.99 16:26:38.72 16:27:25.44

L6.2 (with object)
CH_3
Mean: 38.07
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_4
Mean: 13.77
Acceptable range: 2.5
Failure points: 0%

16:31:41.26 16:32:27.49 16:33:13.72 16:33:59.94
16:31:41.26 16:32:27.49 16:33:13.72 16:33:59.94

L7.2 (without object)
CH_3
Mean: 7.73
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_4
Mean: 0.34
Acceptable range: 2.5
Failure points: 0%

16:35:47.27 16:36:03.50 16:36:19.73 16:36:35.96 16:36
16:35:47.27 16:36:03.50 16:36:19.73 16:36:35.96 16:36

Database: D:\Projects_QCReports_Ord_Data\011310\QC\011310_TA_QC.gdb
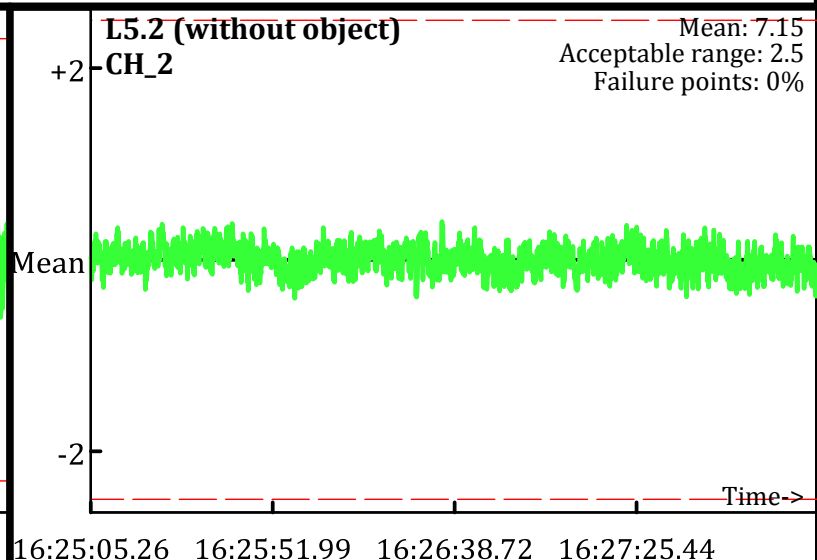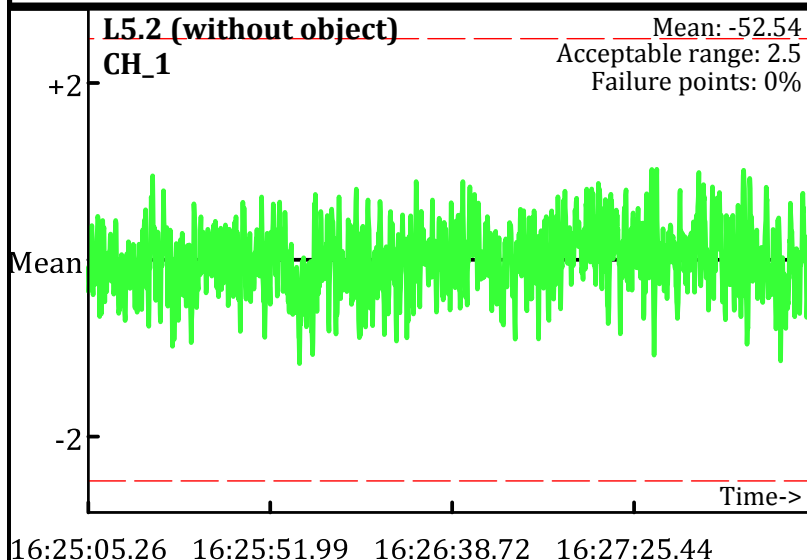Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
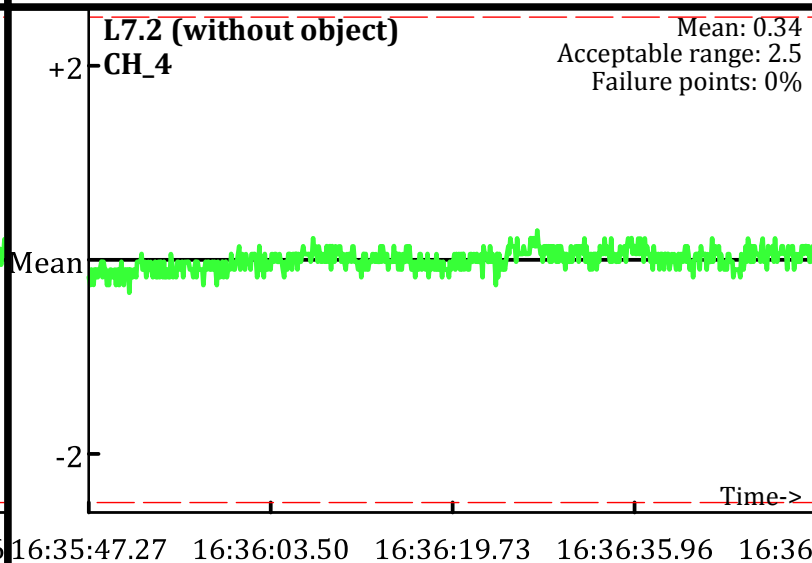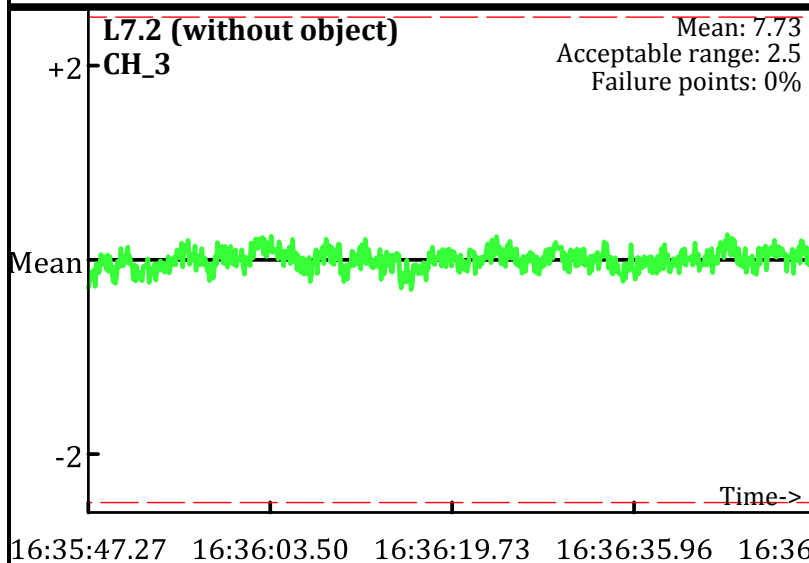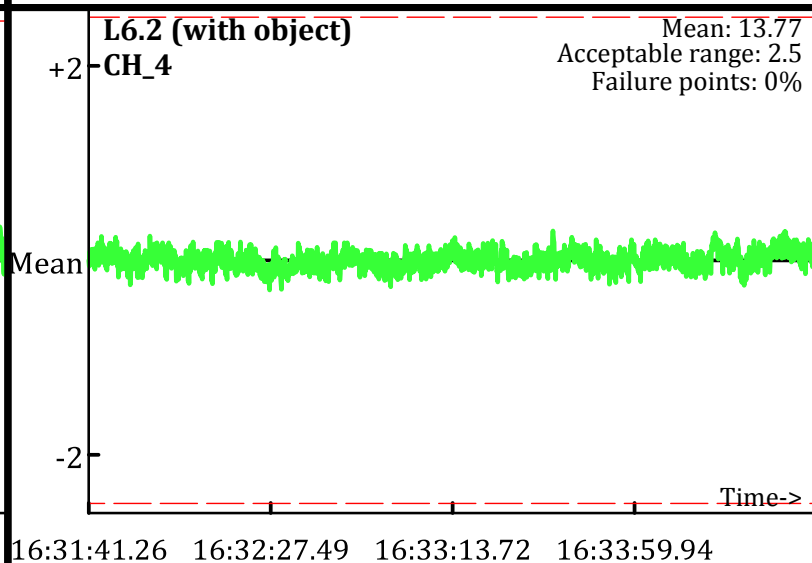--- Acceptable limits

AM test
Operator: PN & SH
Date: 1/14/2010

L0 (without object)
CH_1
Mean: -198.54
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH_2
Mean: -26.84
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_1
Mean: -86.93
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_2
Mean: 38.01
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_1
Mean: -182.77
Acceptable range: 2.5
Failure points: 1%

L2 (without object)
CH_2
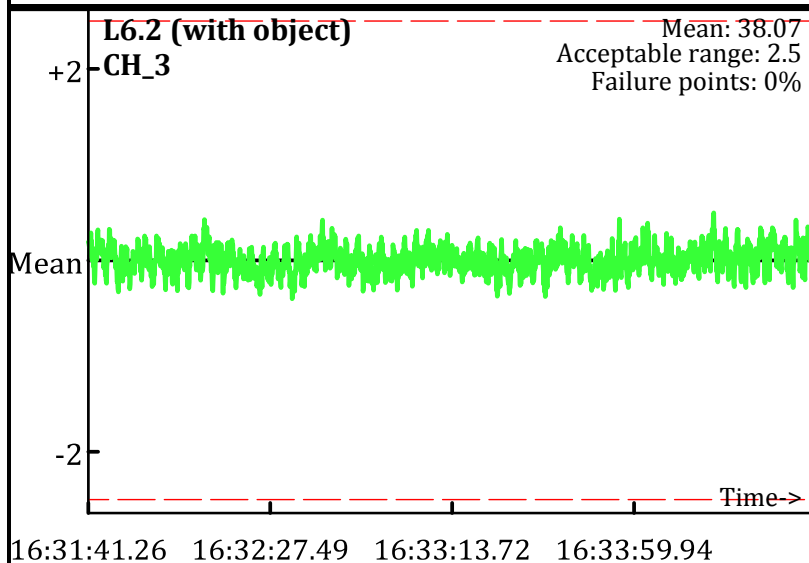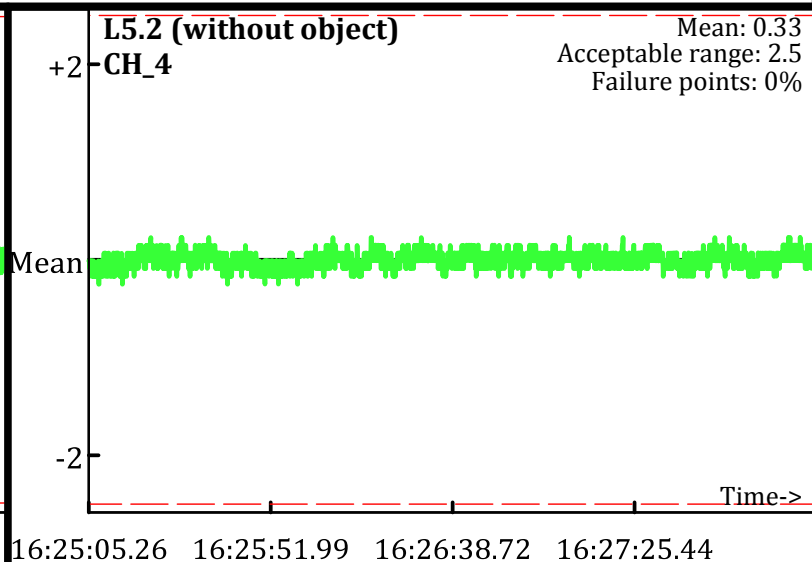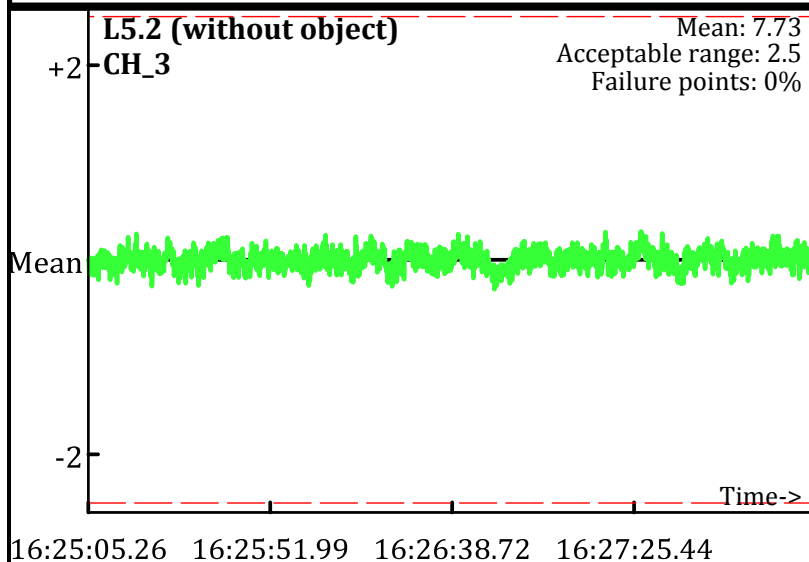Mean: -22.09
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
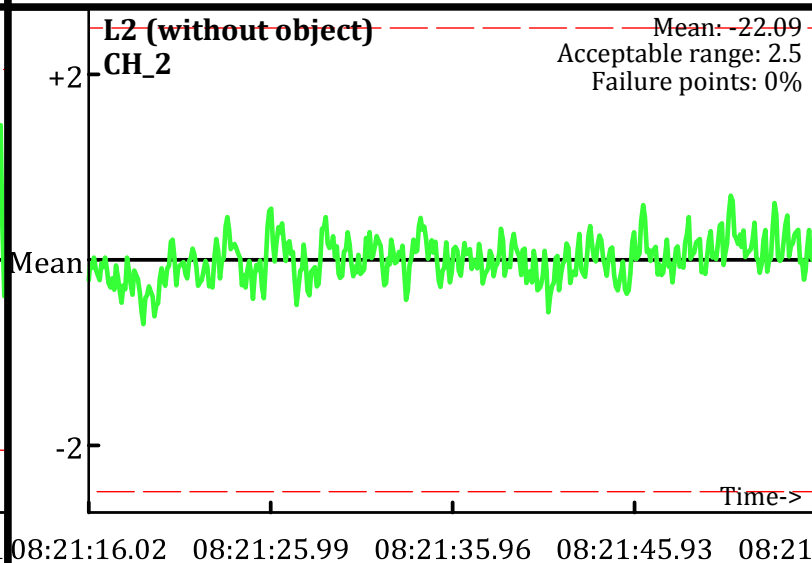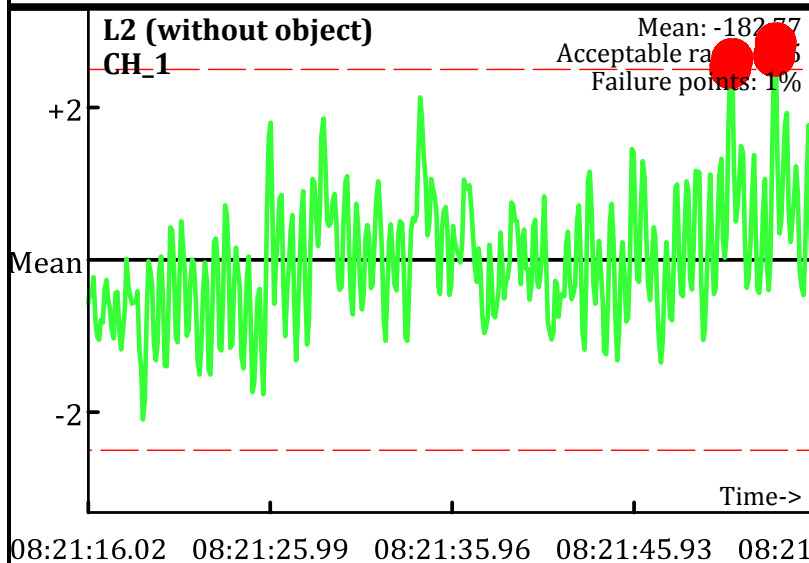Operator: PN & SH
Date: 1/14/2010

L0 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 0.79
Acceptable range: 2.5
Failure points: 0%

08:09:16.72   08:09:31.94   08:09:47.16   08:10:02.39

L0 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.5
Acceptable range: 2.5
Failure points: 0%

08:09:16.72   08:09:31.94   08:09:47.16   08:10:02.39

L1 (with object)
CH_3
+2
Mean
-2
Time->

Mean: 33.46
Acceptable range: 2.5
Failure points: 0%

08:19:29.11   08:19:43.83   08:19:58.55   08:20:13.28   08:20

L1 (with object)
CH_4
+2
Mean
-2
Time->

Mean: 11.79
Acceptable range: 2.5
Failure points: 0%

08:19:29.11   08:19:43.83   08:19:58.55   08:20:13.28   08:20

L2 (without object)
CH_3
+2
Mean
-2
Time->

Mean: 2.07
Acceptable range: 2.5
Failure points: 0%

08:21:16.02   08:21:25.99   08:21:35.96   08:21:45.93   08:21

L2 (without object)
CH_4
+2
Mean
-2
Time->

Mean: -2.09
Acceptable range: 2.5
Failure points: 0%
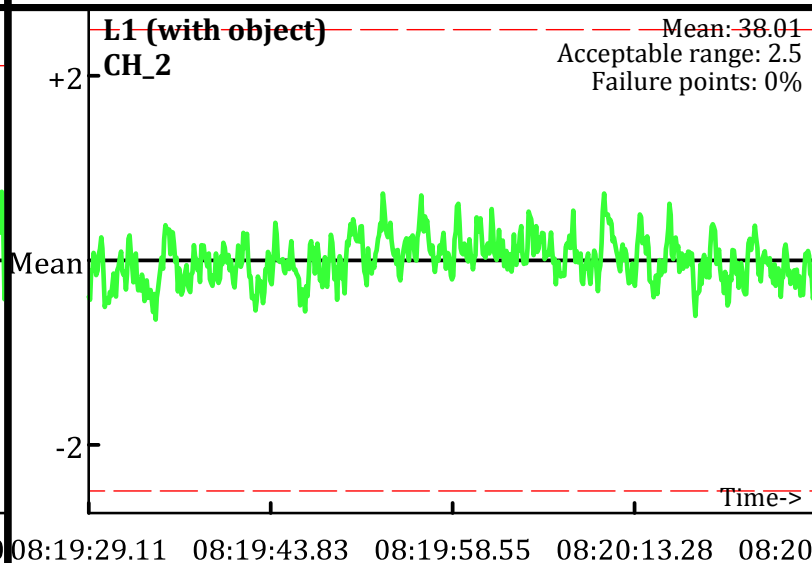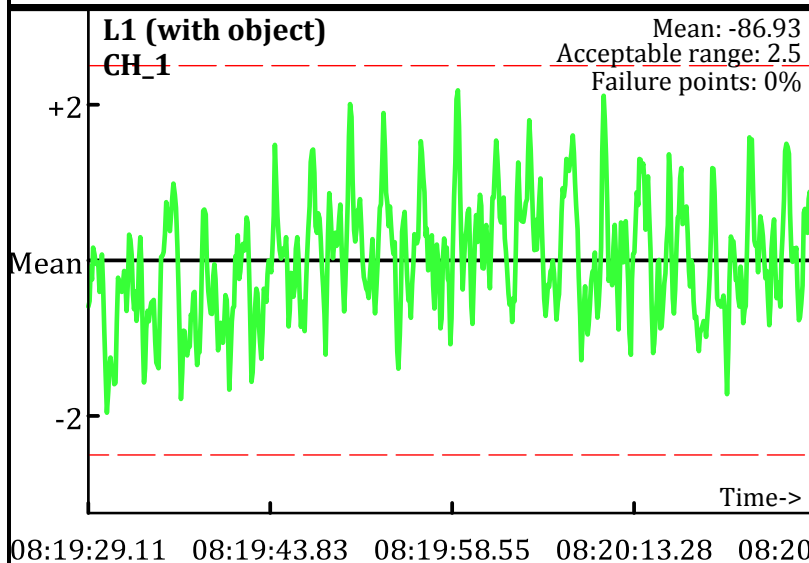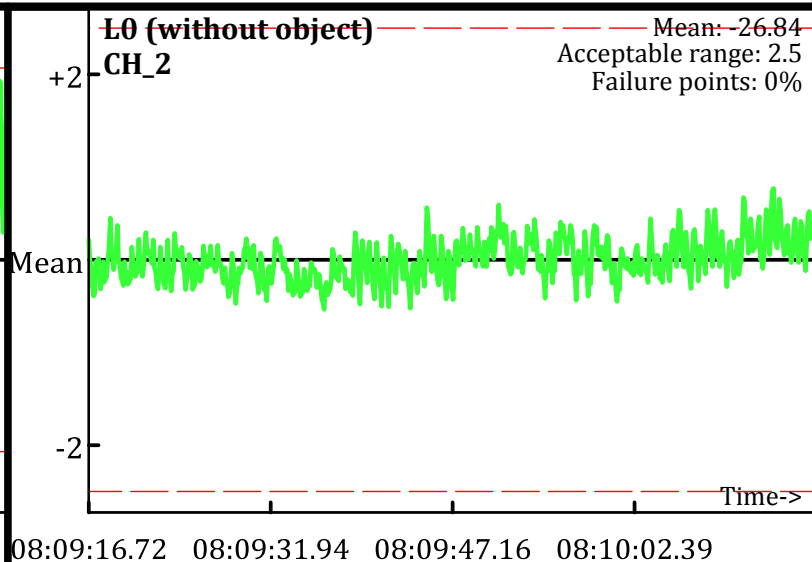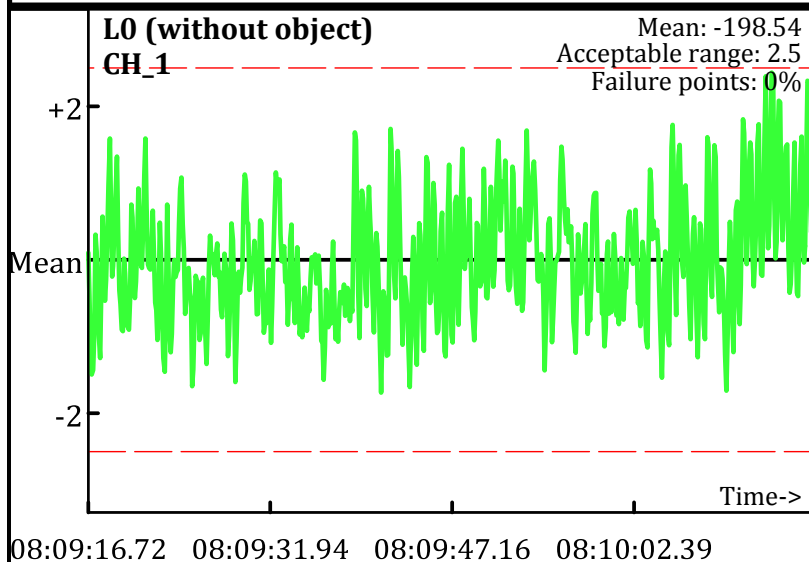
08:21:16.02   08:21:25.99   08:21:35.96   08:21:45.93   08:21

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & SH
Date: 1/14/2010

L0.1 (without object)
CH_1
Mean: -139.35
Acceptable range: 2.5
Failure points: 0.164%

L0.1 (without object)
CH_2
Mean: -12.14
Acceptable range: 2.5
Failure points: 0%

08:09:16.73 08:09:31.96 08:09:47.19 08:10:02.41

L1.1 (with object)
CH_1
Mean: -14.78
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_2
Mean: 80.26
Acceptable range: 2.5
Failure points: 0%

08:19:29.13 08:19:43.85 08:19:58.58 08:20:13.30

L2.1 (without object)
CH_1
Mean: -134.54
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_2
Mean: -10.57
Acceptable range: 2.5
Failure points: 0%

08:21:16.03 08:21:26.01 08:21:35.98 08:21:45.96

Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
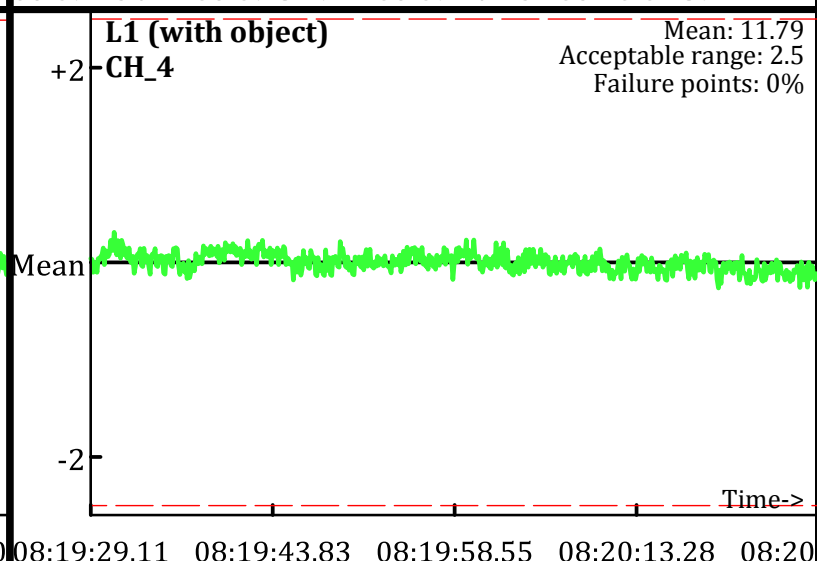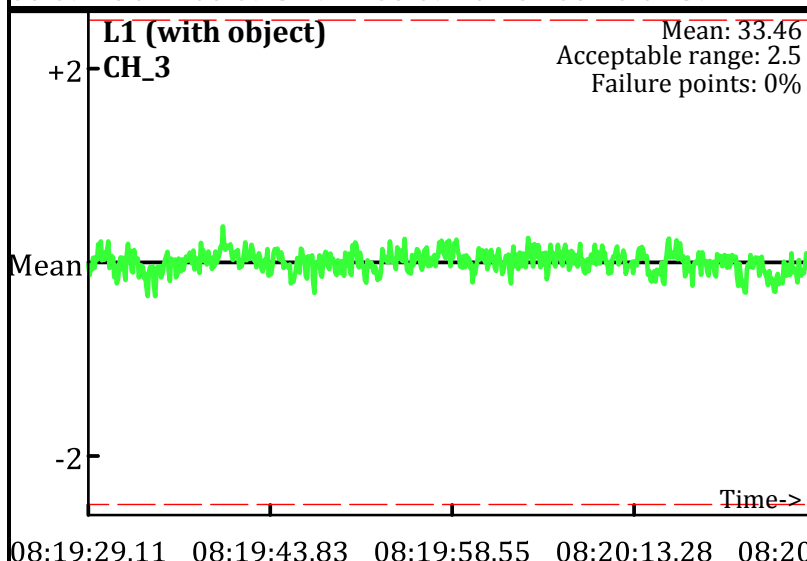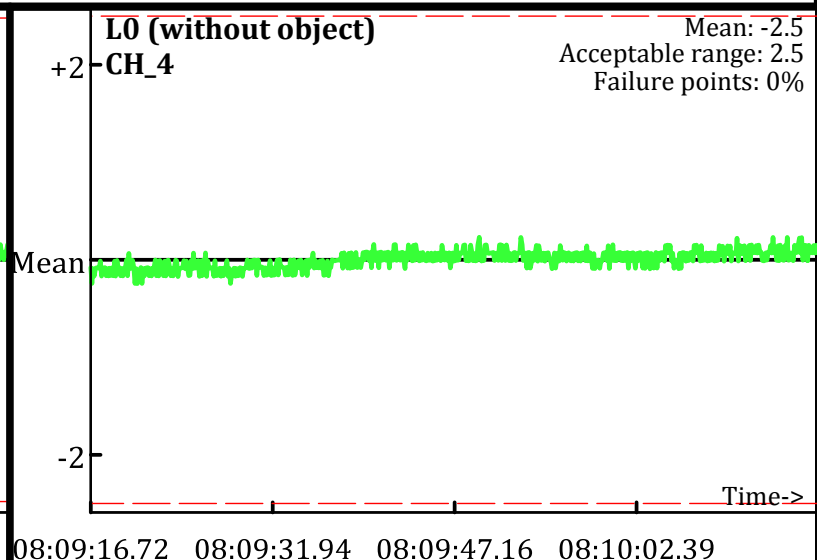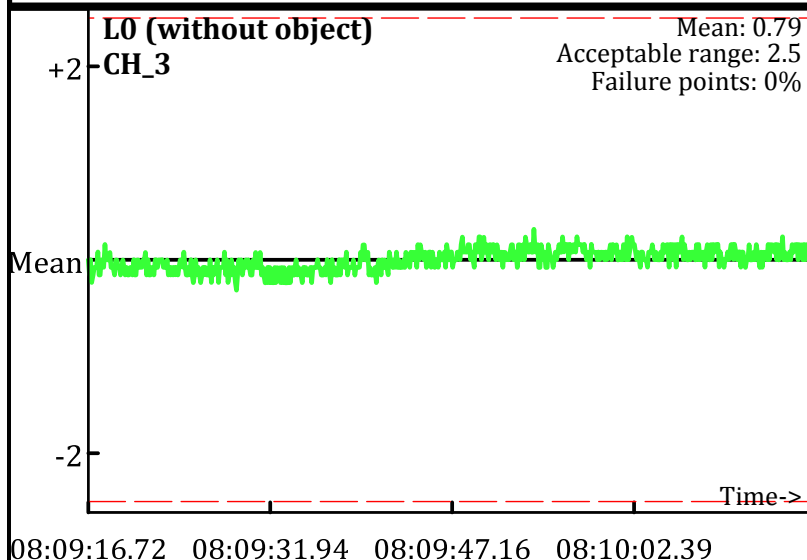Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits

AM test
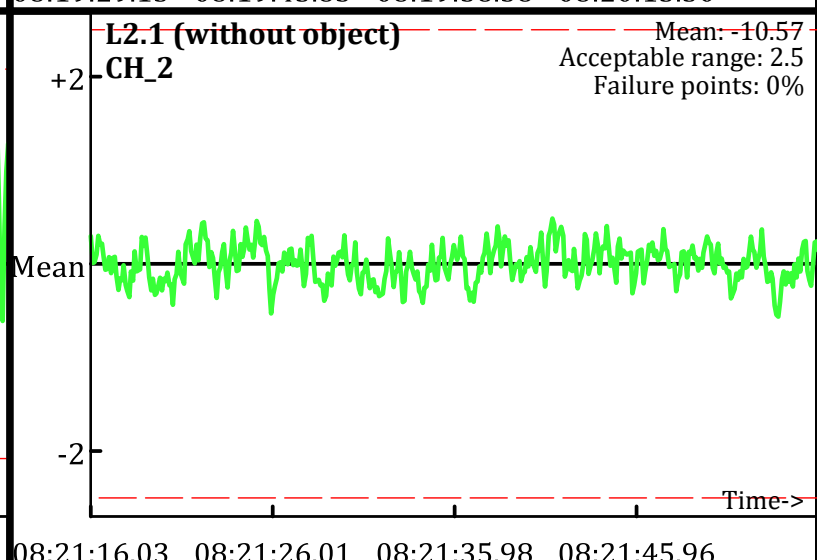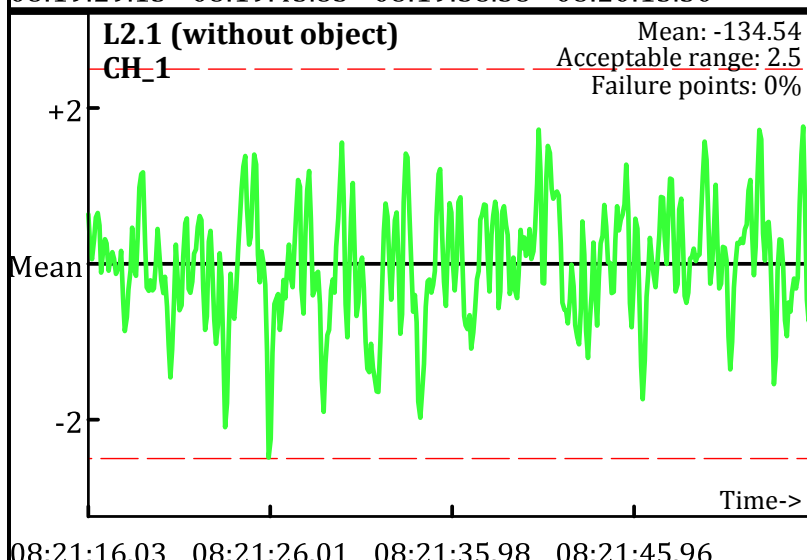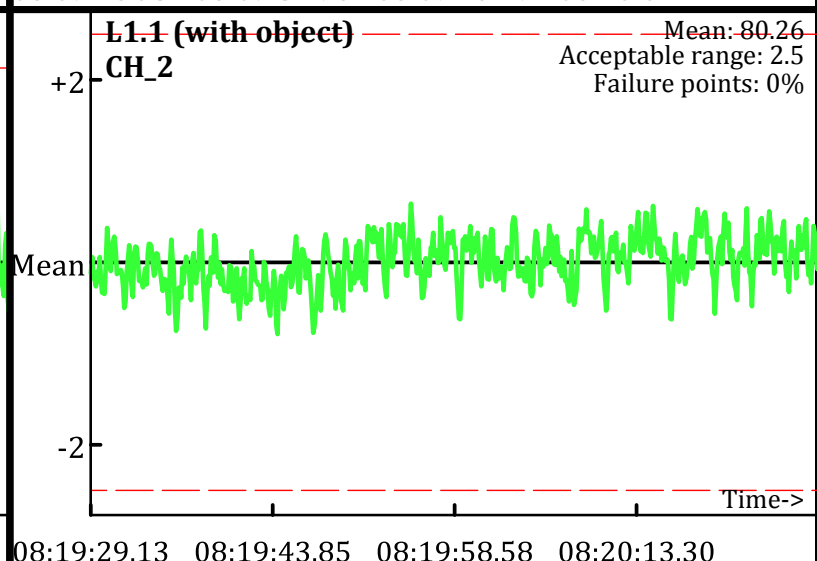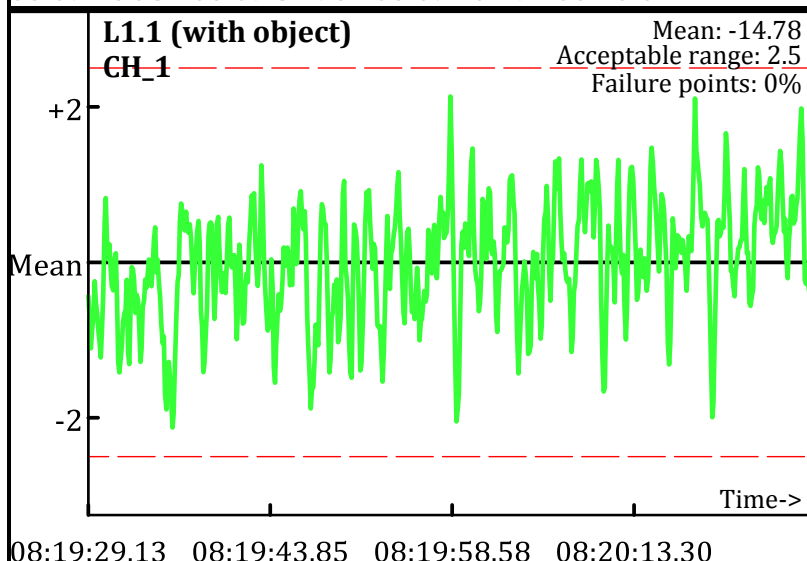Operator: PN & SH
Date: 1/14/2010

L0.1 (without object)
CH_3
Mean: 7.8
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:09:16.73   08:09:31.96   08:09:47.19   08:10:02.41

L0.1 (without object)
CH_4
Mean: 1.94
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:09:16.73   08:09:31.96   08:09:47.19   08:10:02.41

L1.1 (with object)
CH_3
Mean: 66.66
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:19:29.13   08:19:43.85   08:19:58.58   08:20:13.30

L1.1 (with object)
CH_4
Mean: 33.37
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:19:29.13   08:19:43.85   08:19:58.58   08:20:13.30

L2.1 (without object)
CH_3
Mean: 8.16
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:21:16.03   08:21:26.01   08:21:35.98   08:21:45.96

L2.1 (without object)
CH_4
Mean: 1.88
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
08:21:16.03   08:21:26.01   08:21:35.98   08:21:45.96

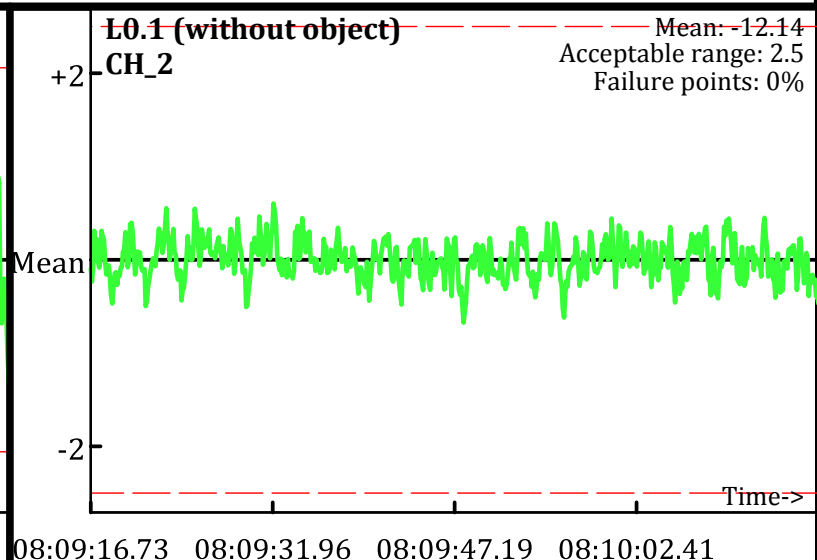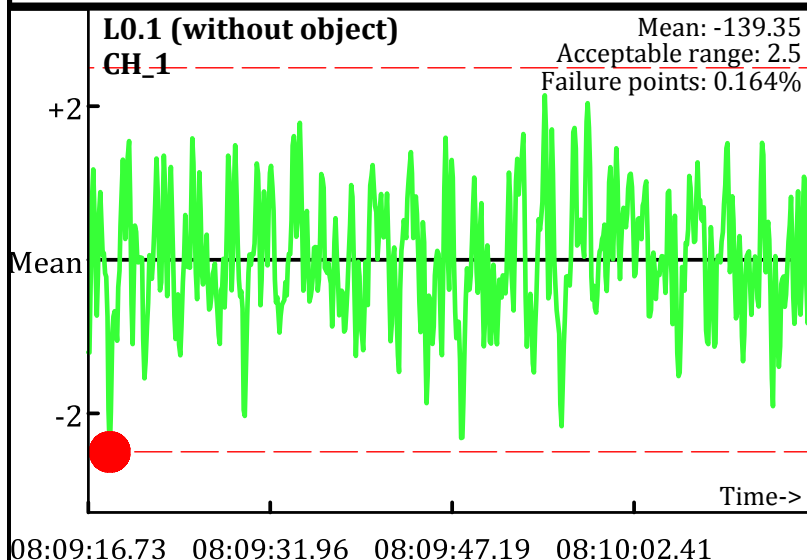Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
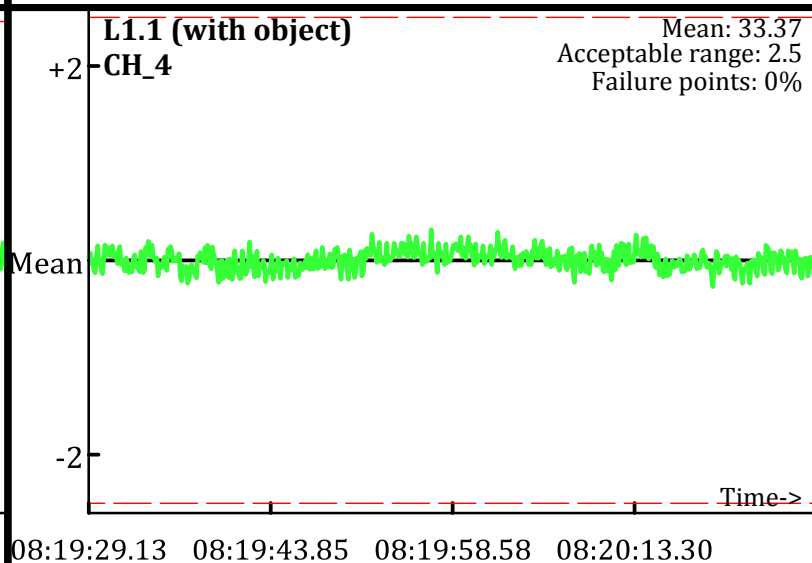Grid/Location: QC Area

🔴 Outside range
- - - Acceptable limits

AM test
Operator: PN & SH
Date: 1/14/2010

L0.2 (without object)
CH_1
Mean: -80.75
Acceptable range: 2.5
Failure points: 0%

L0.2 (without object)
CH_2
Mean: 1.11
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_1
Mean: 11.39
Acceptable range: 2.5
Failure points: 0%

L1.2 (with object)
CH_2
Mean: 56.18
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_1
Mean: -78.78
Acceptable range: 2.5
Failure points: 0%

L2.2 (without object)
CH_2
Mean: 0.44
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
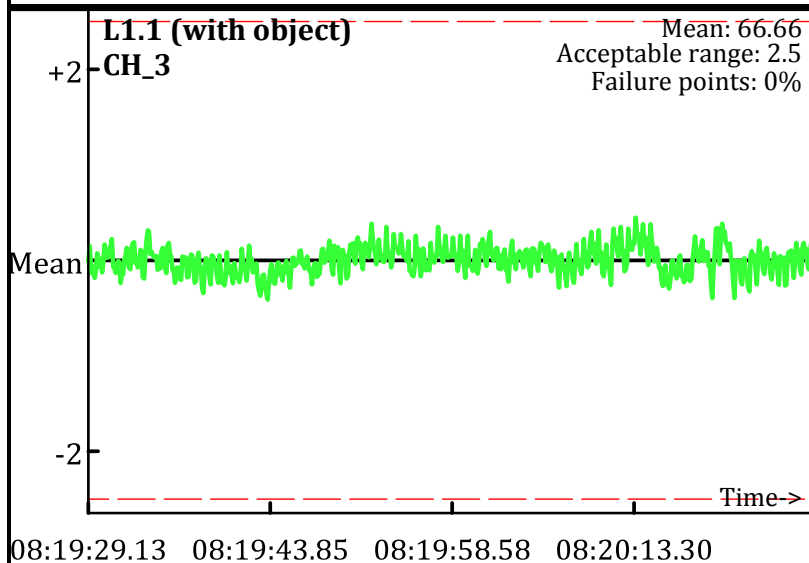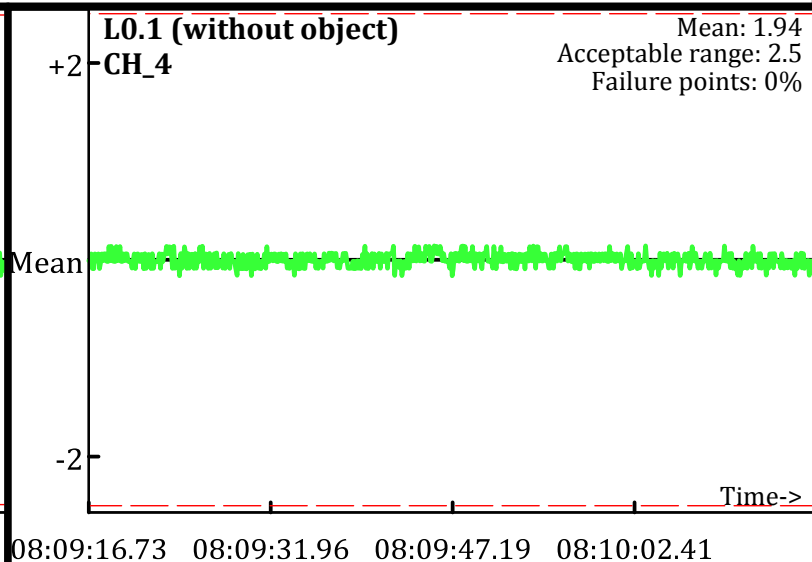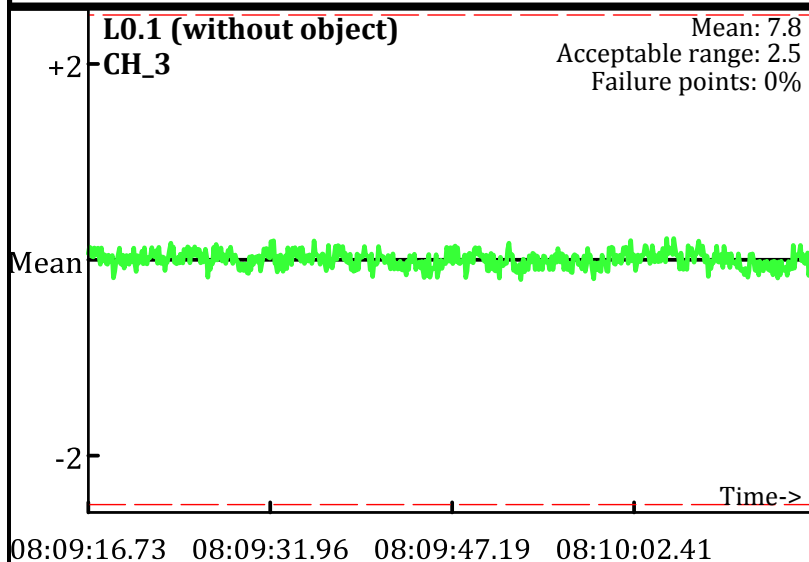Line Name: L0.2 L1.2 L2.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
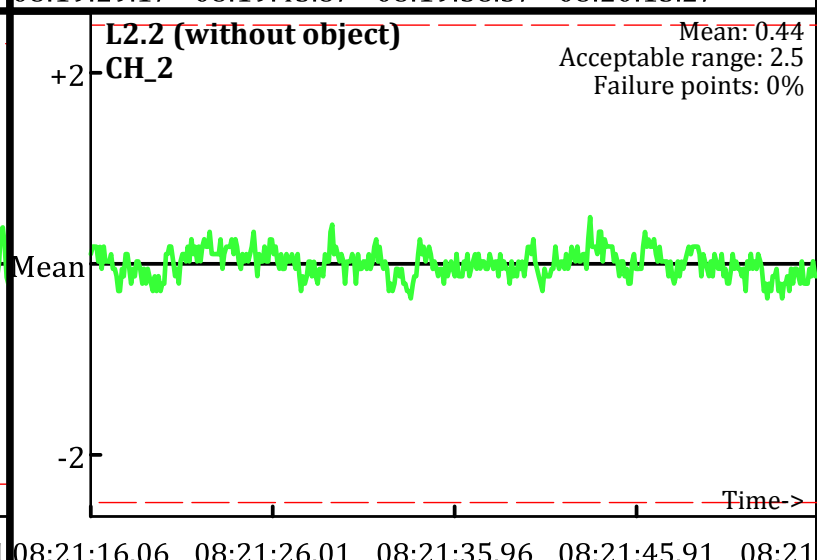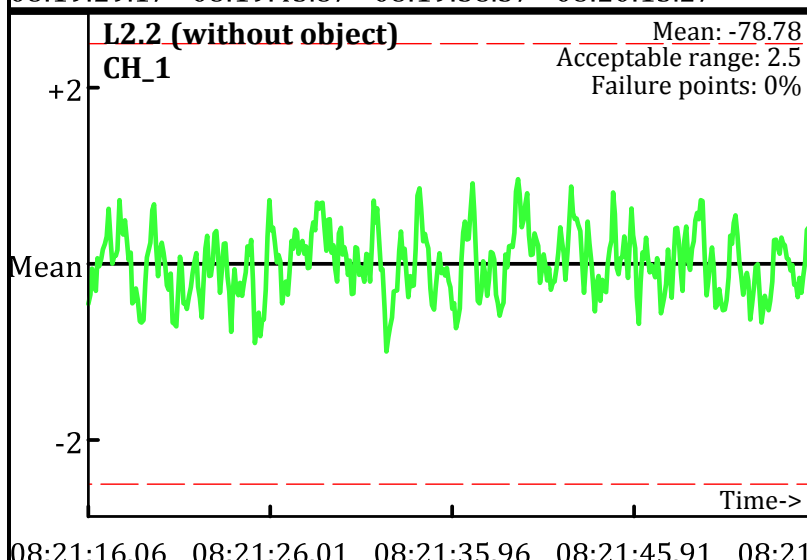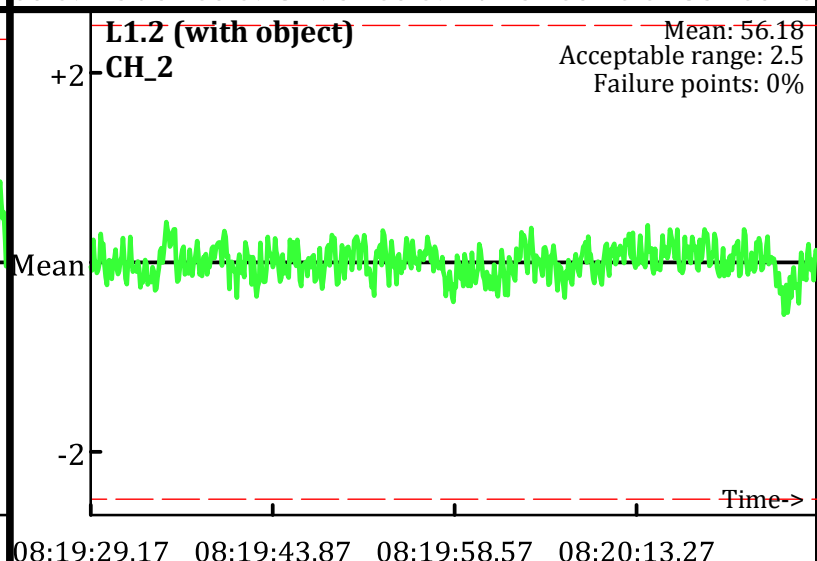Operator: PN & SH
Date: 1/14/2010

L0.2 (without object)
CH_3
Mean: 6.97
Acceptable range: 2.5
Failure points: 0%

08:09:16.76   08:09:31.96   08:09:47.16   08:10:02.36   08:10

L0.2 (without object)
CH_4
Mean: 0.29
Acceptable range: 2.5
Failure points: 0%

08:09:16.76   08:09:31.96   08:09:47.16   08:10:02.36   08:10

L1.2 (with object)
CH_3
Mean: 35.49
Acceptable range: 2.5
Failure points: 0%

08:19:29.17   08:19:43.87   08:19:58.57   08:20:13.27

L1.2 (with object)
CH_4
Mean: 12.46
Acceptable range: 2.5
Failure points: 0%

08:19:29.17   08:19:43.87   08:19:58.57   08:20:13.27

L2.2 (without object)
CH_3
Mean: 6.28
Acceptable range: 2.5
Failure points: 0%

08:21:16.06   08:21:26.01   08:21:35.96   08:21:45.91   08:21

L2.2 (without object)
CH_4
Mean: -0.31
Acceptable range: 2.5
Failure points: 0%

08:21:16.06   08:21:26.01   08:21:35.96   08:21:45.91   08:21

Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
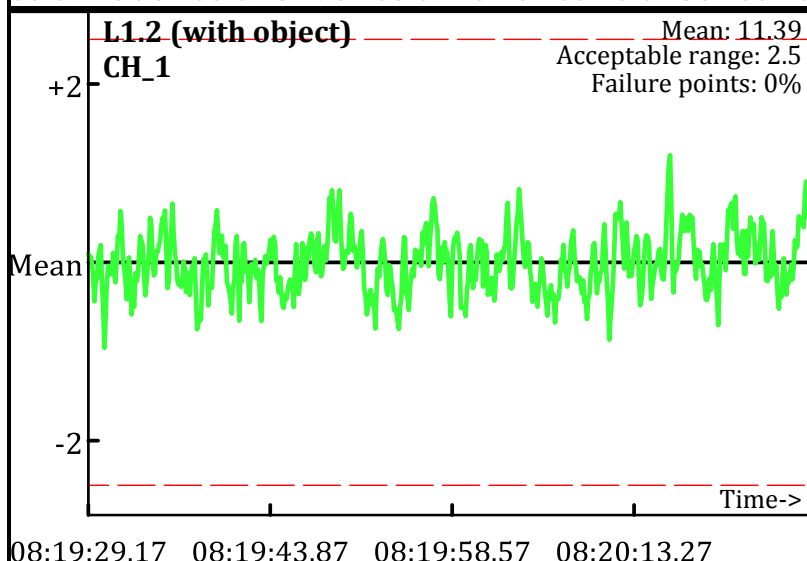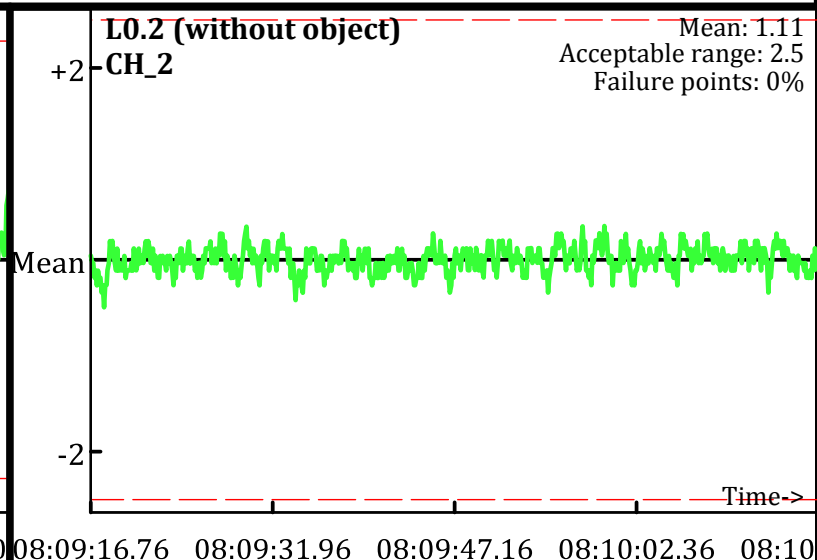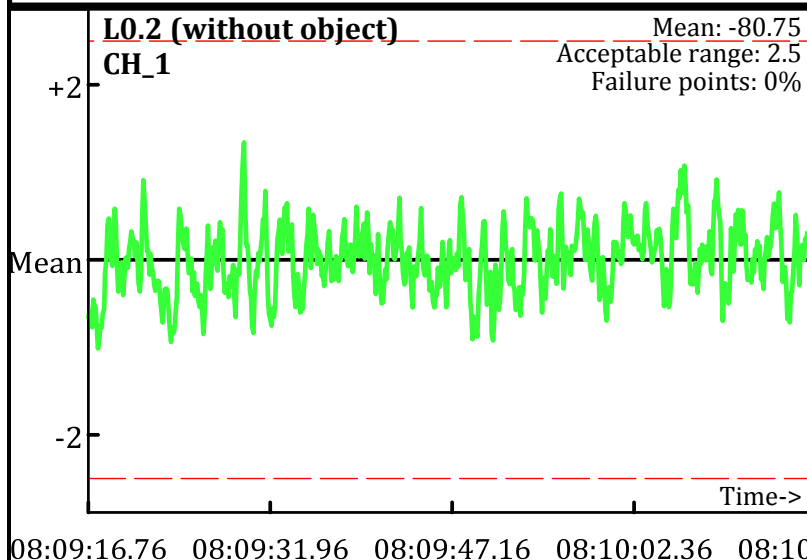Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
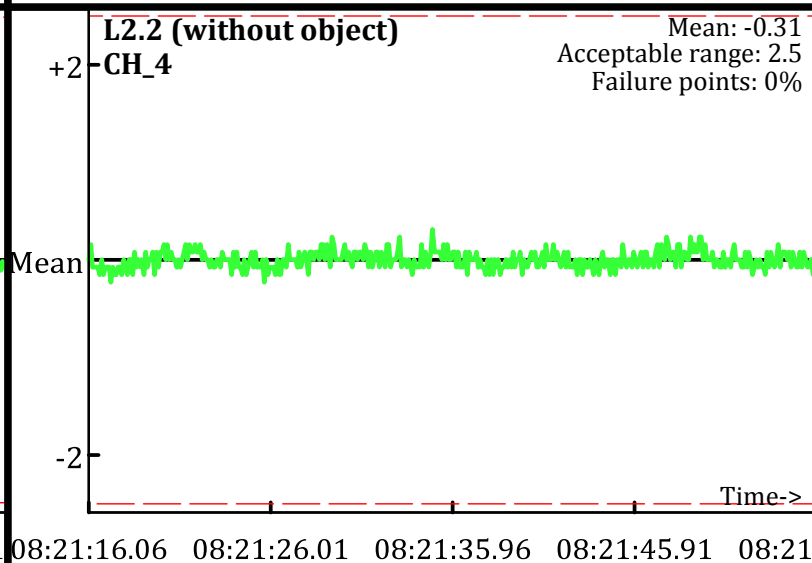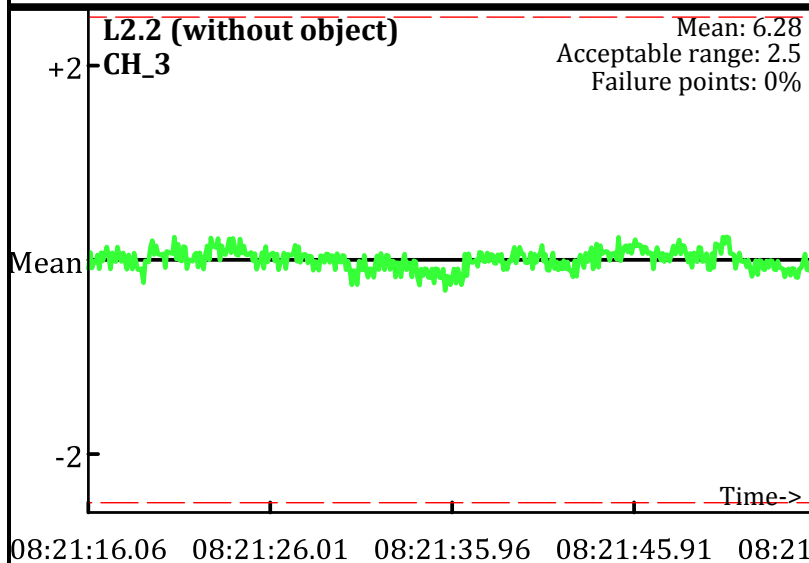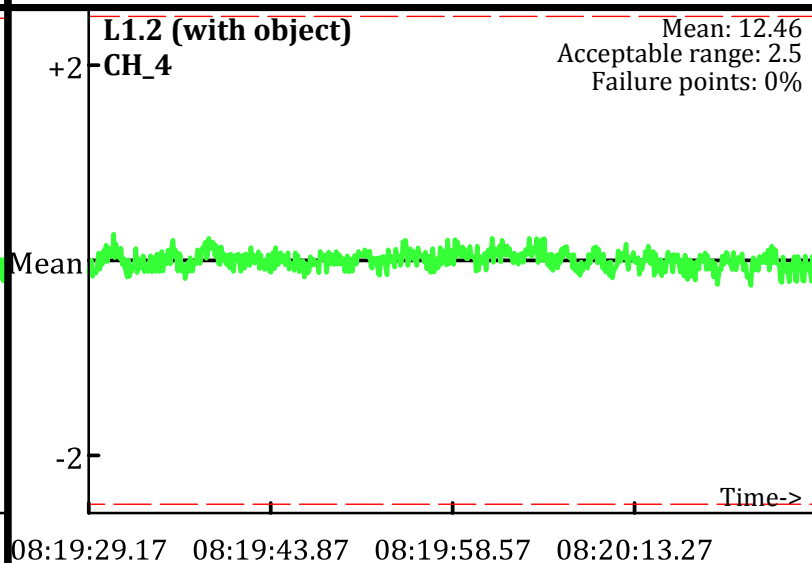Operator: PN & SH
Date: 1/14/2010

PM Cable Shake Test not performed – battery died

L6 (with object)
CH_1
Mean: -26.58
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2

Time->

16:54:46.13   16:55:25.57   16:56:05.02   16:56:44.47

L6 (with object)
CH_2
Mean: 50.75
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2

Time->

16:54:46.13   16:55:25.57   16:56:05.02   16:56:44.47

L5 (without object)
CH_1
Mean: -118.79
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2

Time->

16:50:41.31   16:51:26.76   16:52:12.21   16:52:57.66

L5 (without object)
CH_2
Mean: -6.74
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2

Time->

16:50:41.31   16:51:26.76   16:52:12.21   16:52:57.66
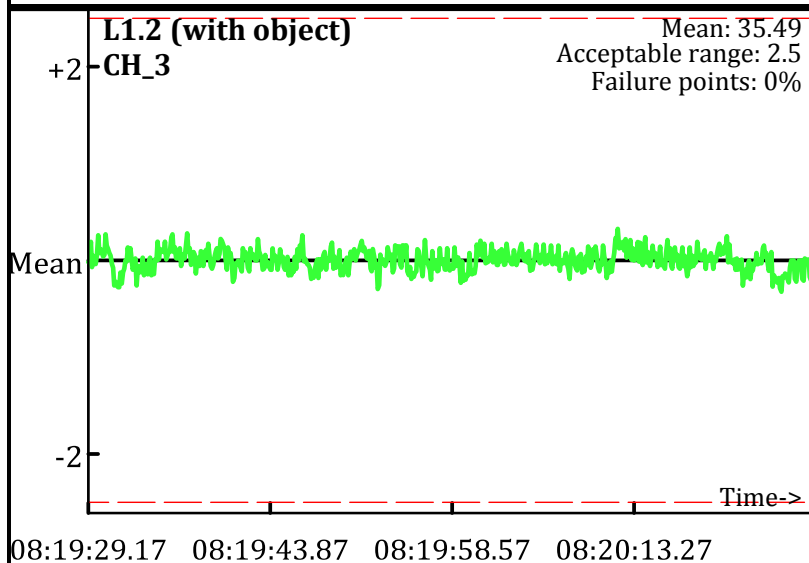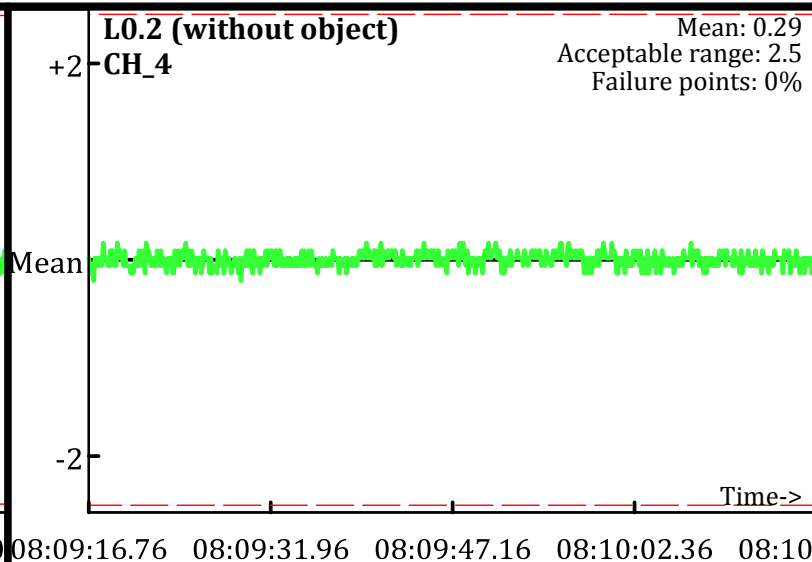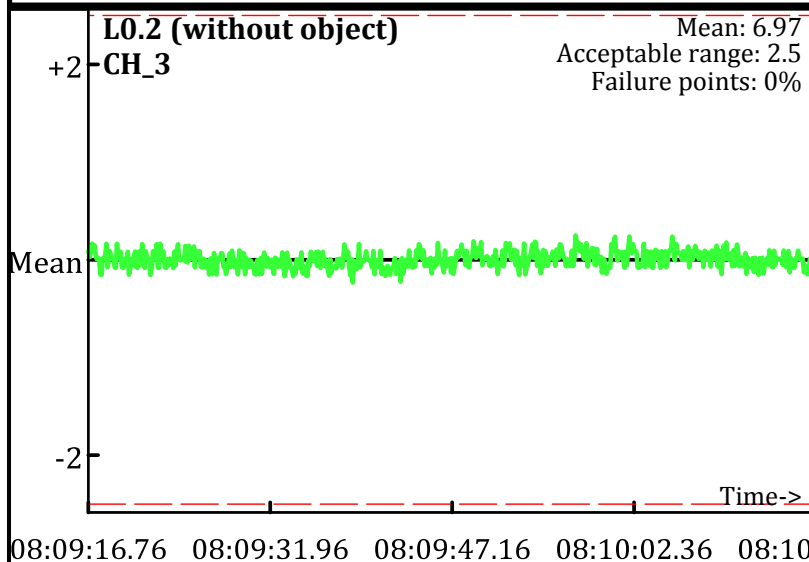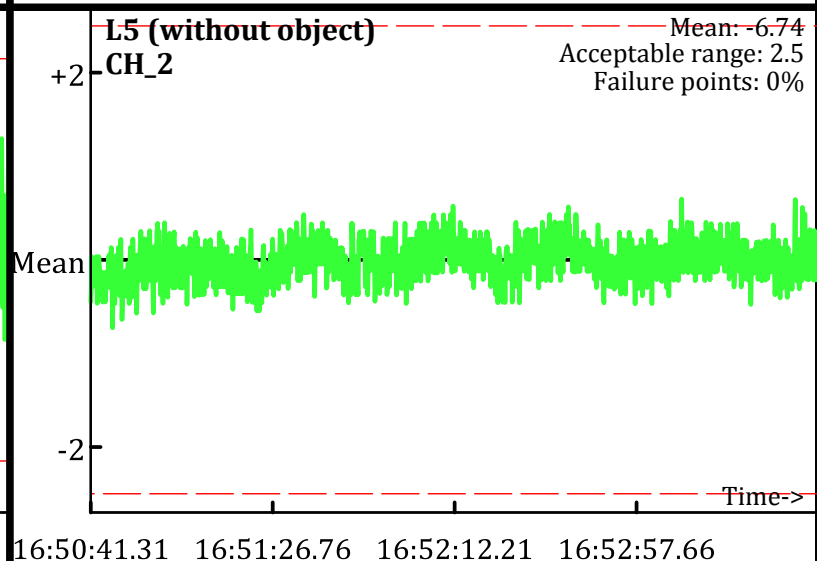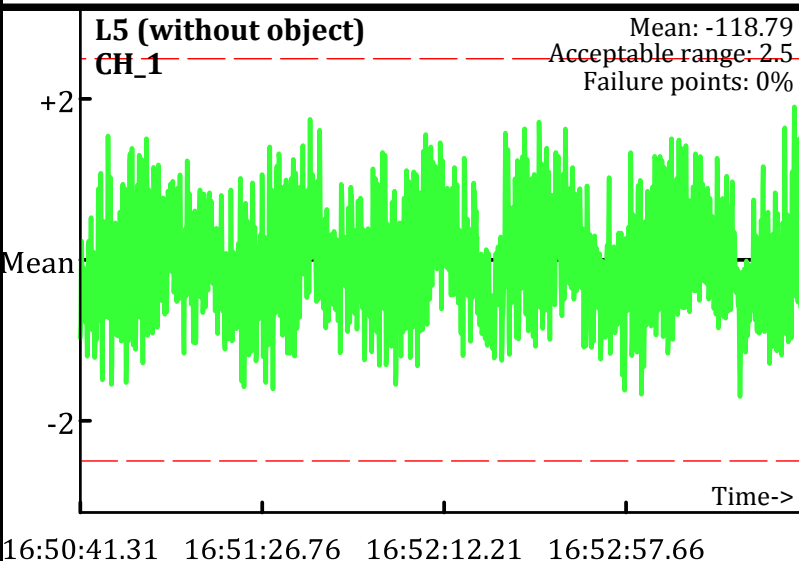
Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/14/2010

PM Cable Shake Test not performed – battery died

L6 (with object)
CH_3
+2
Mean
-2
Mean: 33.67
Acceptable range: 2.5
Failure points: 0%
Time->

16:54:46.13   16:55:25.57   16:56:05.02   16:56:44.47

L6 (with object)
CH_4
+2
Mean
-2
Mean: 10.22
Acceptable range: 2.5
Failure points: 0%
Time->

16:54:46.13   16:55:25.57   16:56:05.02   16:56:44.47

L5 (without object)
CH_3
+2
Mean
-2
Mean: 3.84
Acceptable range: 2.5
Failure points: 0%
Time->

16:50:41.31   16:51:26.76   16:52:12.21   16:52:57.66

L5 (without object)
CH_4
+2
Mean
-2
Mean: -2.76
Acceptable range: 2.5
Failure points: 0%
Time->

16:50:41.31   16:51:26.76   16:52:12.21   16:52:57.66

Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
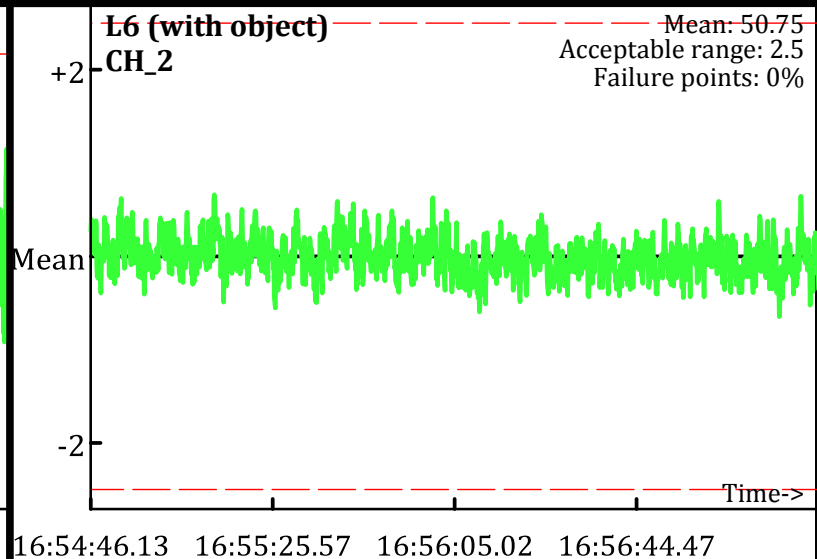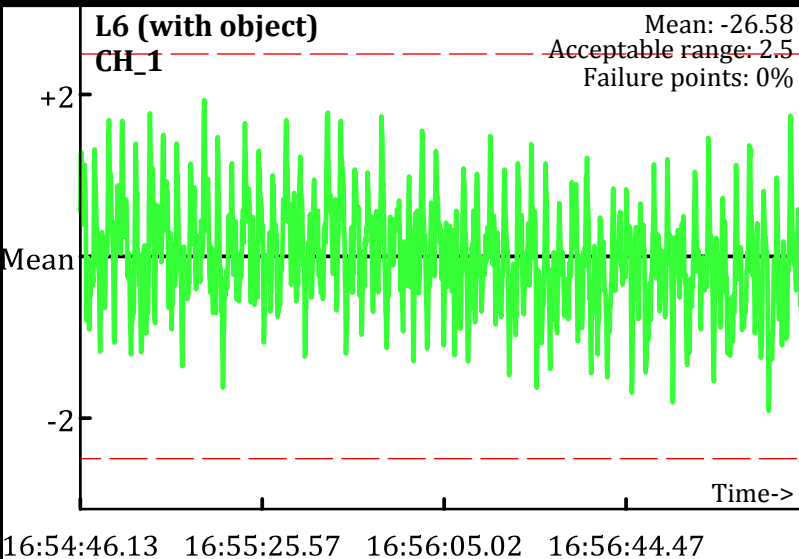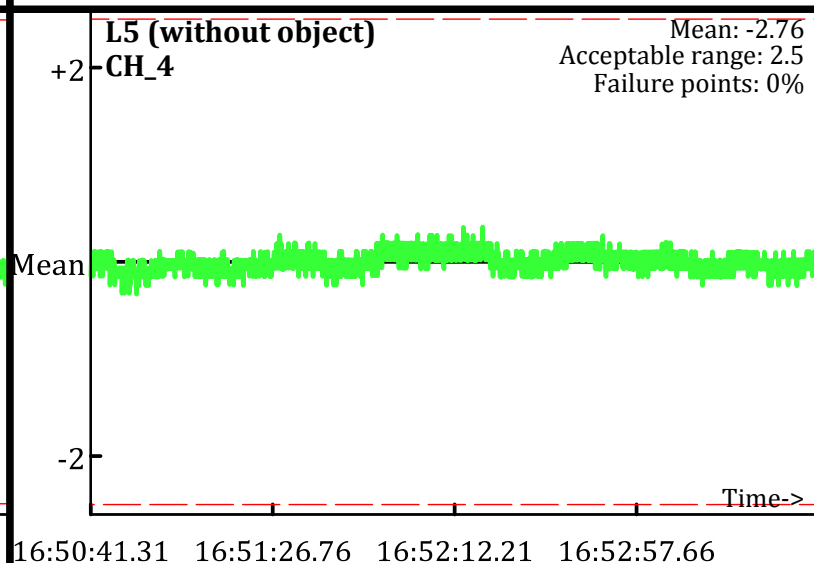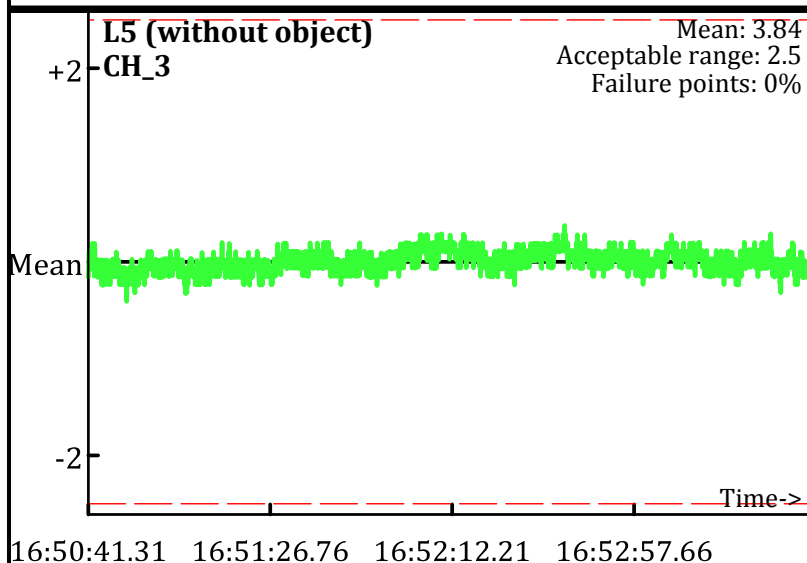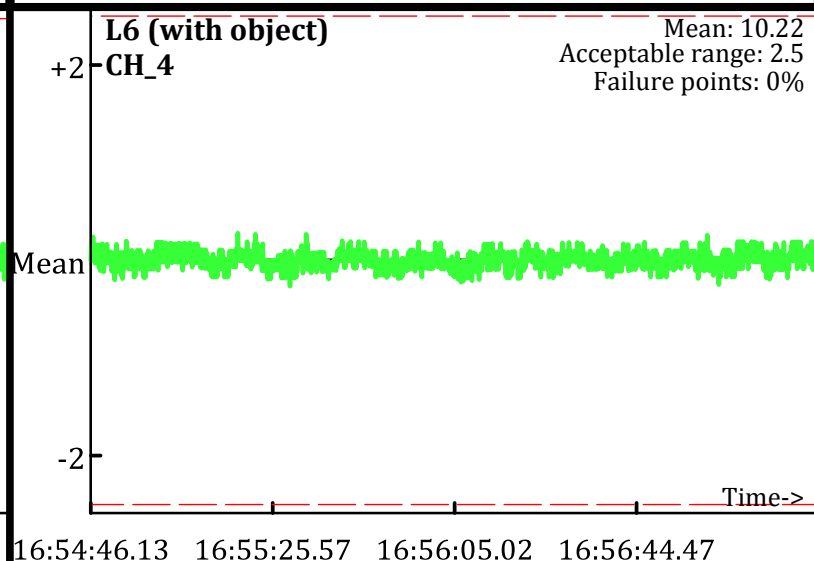Line Name: L5 L6 L5

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/14/2010
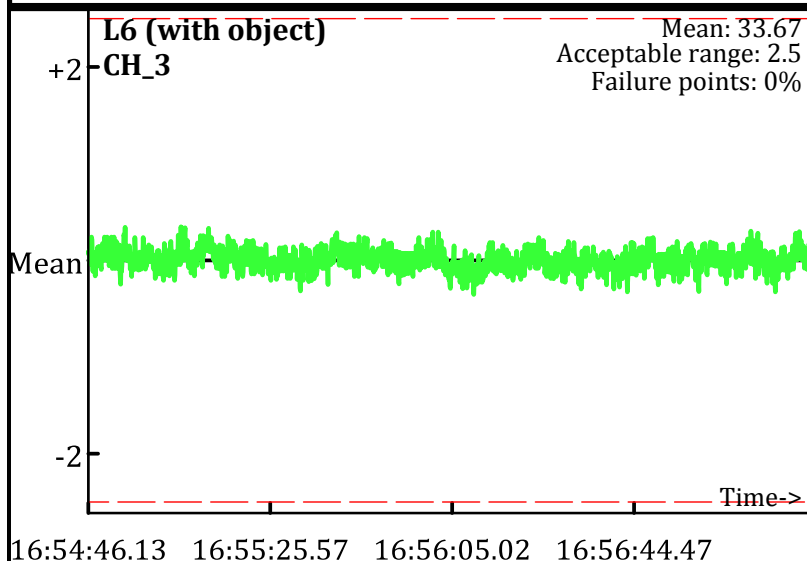
PM Cable Shake Test not performed – battery died

L6.1 (with object)
CH_1

Mean: 48.33
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:46.13   16:55:25.58   16:56:05.03   16:56:44.48

L6.1 (with object)
CH_2

Mean: 95.71
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:46.13   16:55:25.58   16:56:05.03   16:56:44.48

L5.1 (without object)
CH_1

Mean: -70.29
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:50:41.34   16:51:26.79   16:52:12.24   16:52:57.69

L5.1 (without object)
CH_2

Mean: 6.32
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

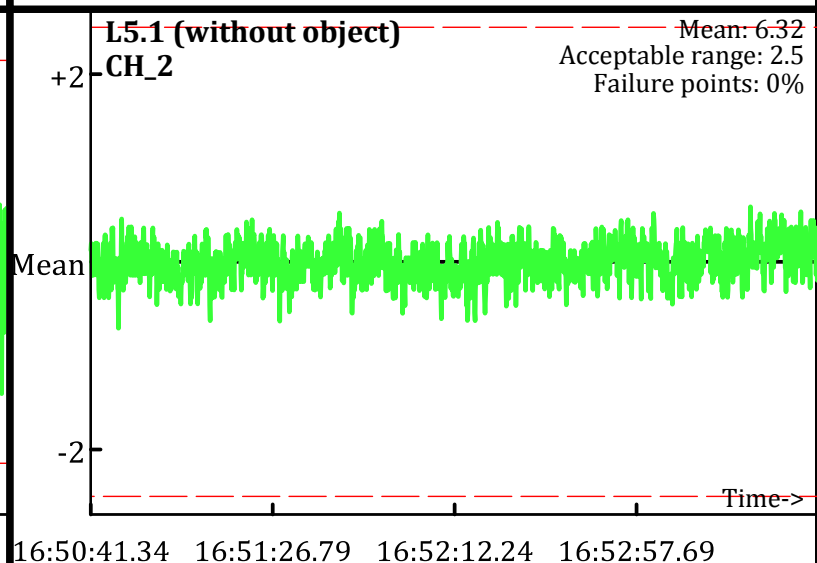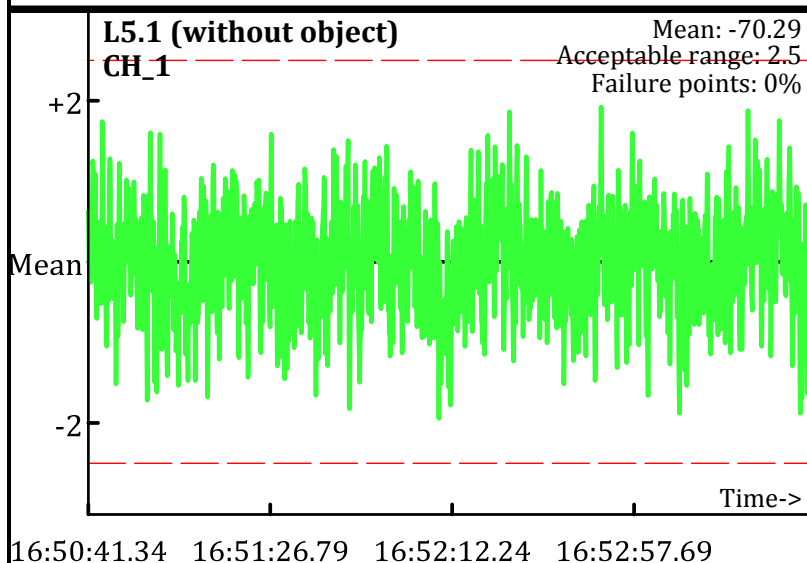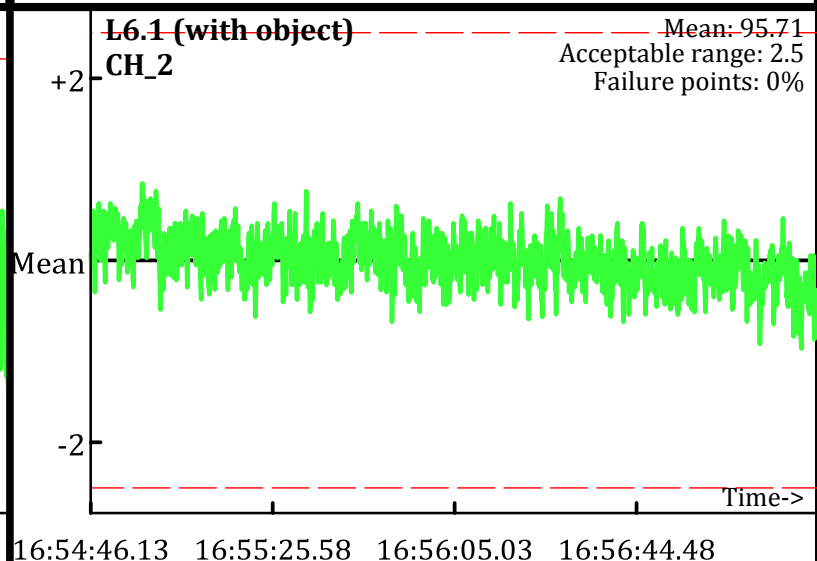16:50:41.34   16:51:26.79   16:52:12.24   16:52:57.69

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/14/2010
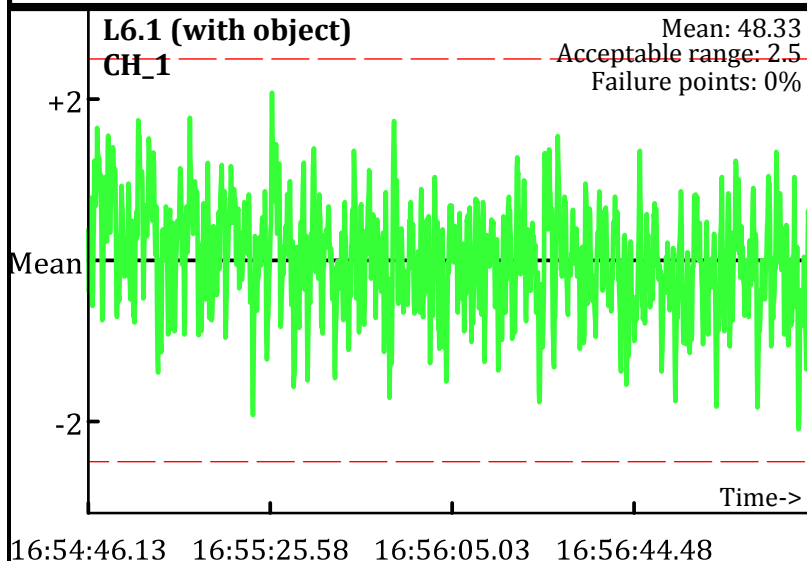
PM Cable Shake Test not performed – battery died

L6.1 (with object)
CH_3
+2
Mean
-2

Mean: 67.6
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:46.13 16:55:25.58 16:56:05.03 16:56:44.48

L6.1 (with object)
CH_4
+2
Mean
-2

Mean: 32
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:46.13 16:55:25.58 16:56:05.03 16:56:44.48

L5.1 (without object)
CH_3
+2
Mean
-2

Mean: 10.35
Acceptable range: 2.5
Failure points: 0%

Time->

16:50:41.34 16:51:26.79 16:52:12.24 16:52:57.69

L5.1 (without object)
CH_4
+2
Mean
-2

Mean: 1.3
Acceptable range: 2.5
Failure points: 0%

Time->

16:50:41.34 16:51:26.79 16:52:12.24 16:52:57.69

Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
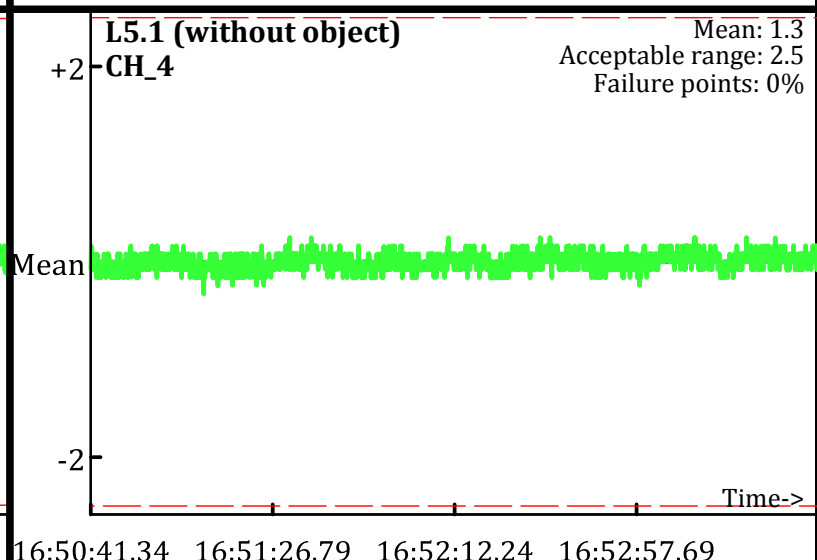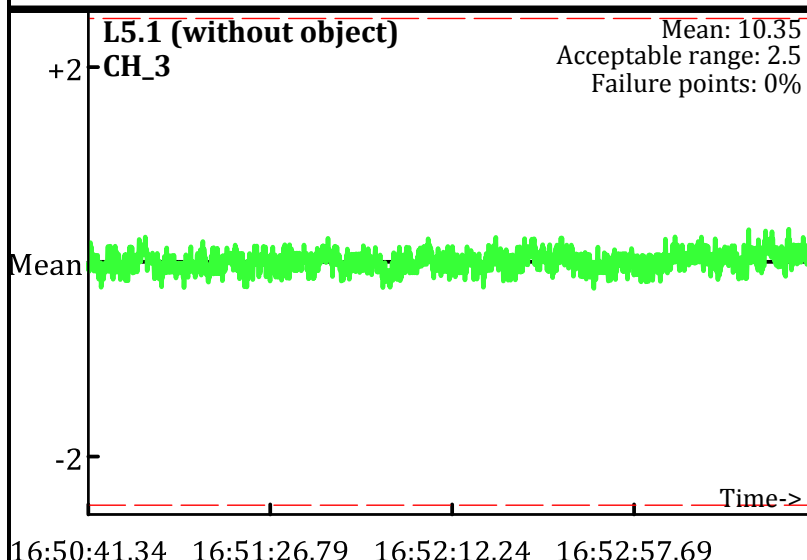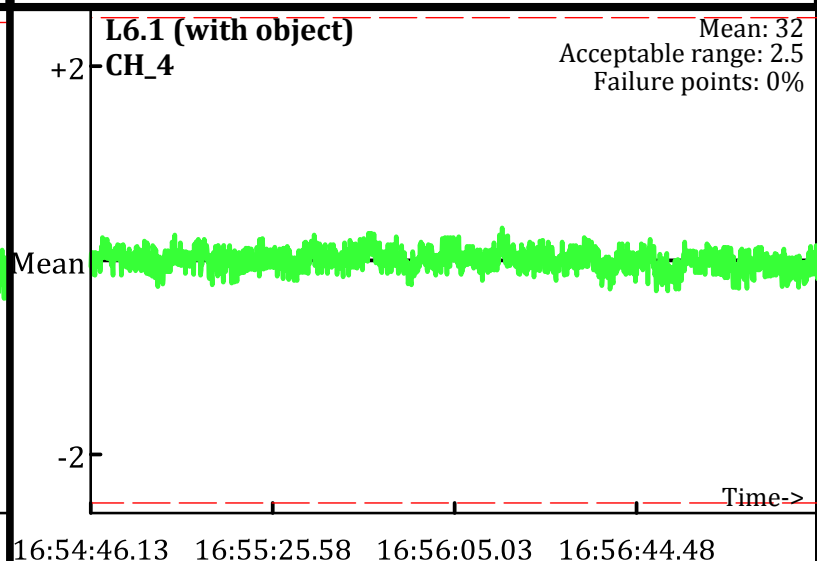Line Name: L5.1 L6.1 L5.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/14/2010
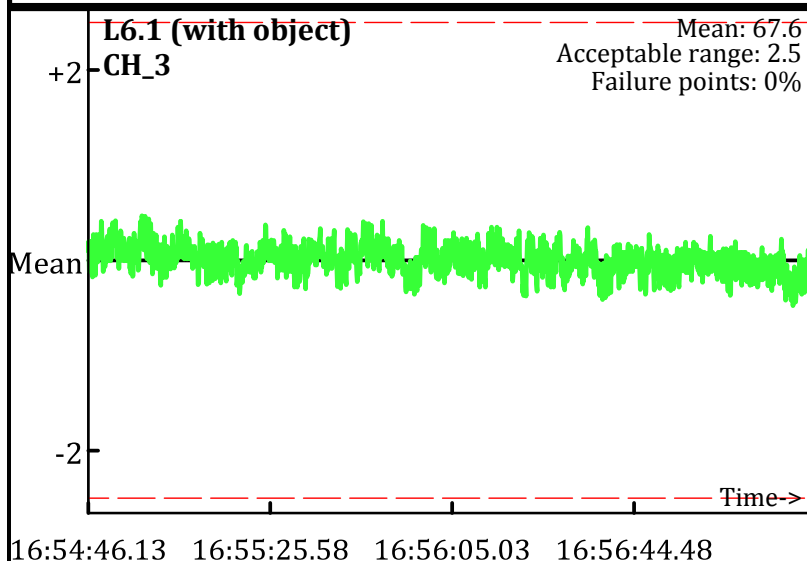
PM Cable Shake Test not performed – battery died

L6.2 (with object)
CH_1
Mean: 33.87
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:46.16   16:55:25.58   16:56:05.00   16:56:44.42

L6.2 (with object)
CH_2
Mean: 58.35
Acceptable range: 2.5
Failure points: 0%

Time->

16:54:46.16   16:55:25.58   16:56:05.00   16:56:44.42

L5.2 (without object)
CH_1
Mean: -51
Acceptable range: 2.5
Failure points: 0%

Time->

16:50:41.36   16:51:26.78   16:52:12.20   16:52:57.62

L5.2 (without object)
CH_2
Mean: 5.71
Acceptable range: 2.5
Failure points: 0%

Time->

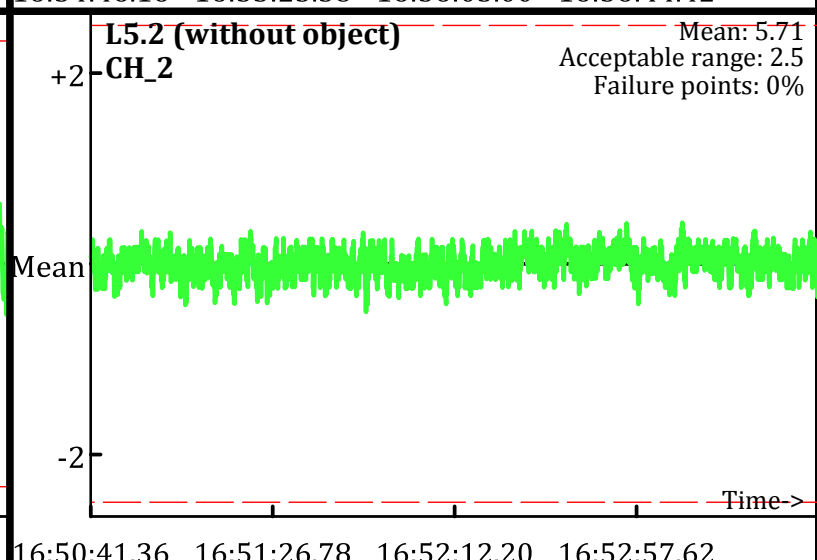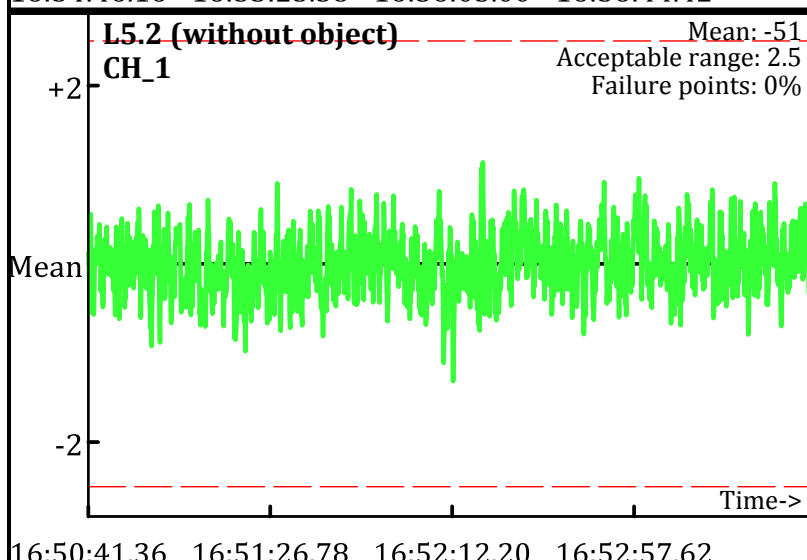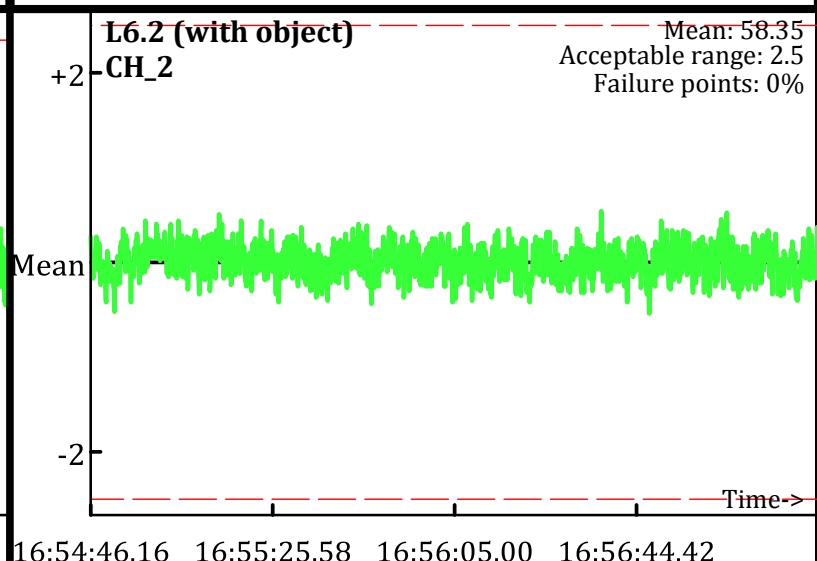16:50:41.36   16:51:26.78   16:52:12.20   16:52:57.62

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/14/2010
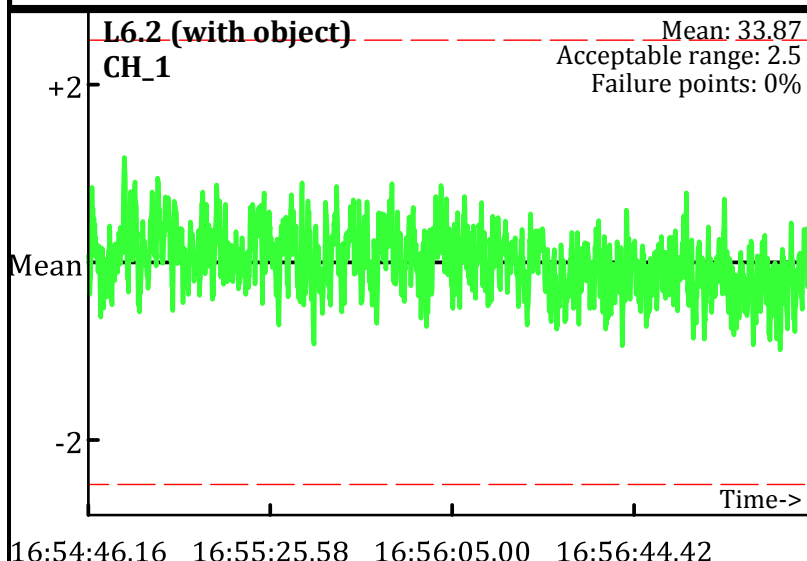
PM Cable Shake Test not performed – battery died

L6.2 (with object)
CH_3
Mean: 34.25
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:46.16   16:55:25.58   16:56:05.00   16:56:44.42

L6.2 (with object)
CH_4
Mean: 11.35
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:54:46.16   16:55:25.58   16:56:05.00   16:56:44.42

L5.2 (without object)
CH_3
Mean: 6.67
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:50:41.36   16:51:26.78   16:52:12.20   16:52:57.62

L5.2 (without object)
CH_4
Mean: -0.64
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

16:50:41.36   16:51:26.78   16:52:12.20   16:52:57.62

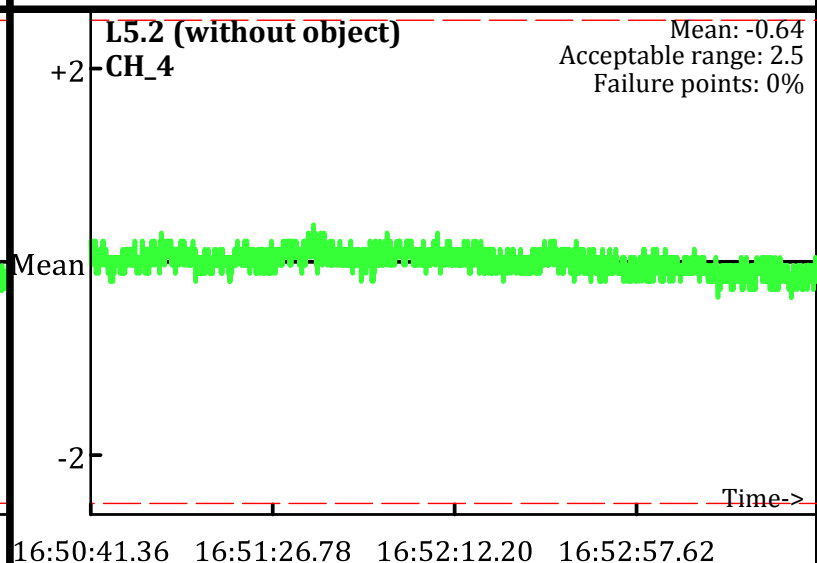Database: D:\Projects_QCReports_Ord_Data\011410\QC\011410_TA_QC.gdb
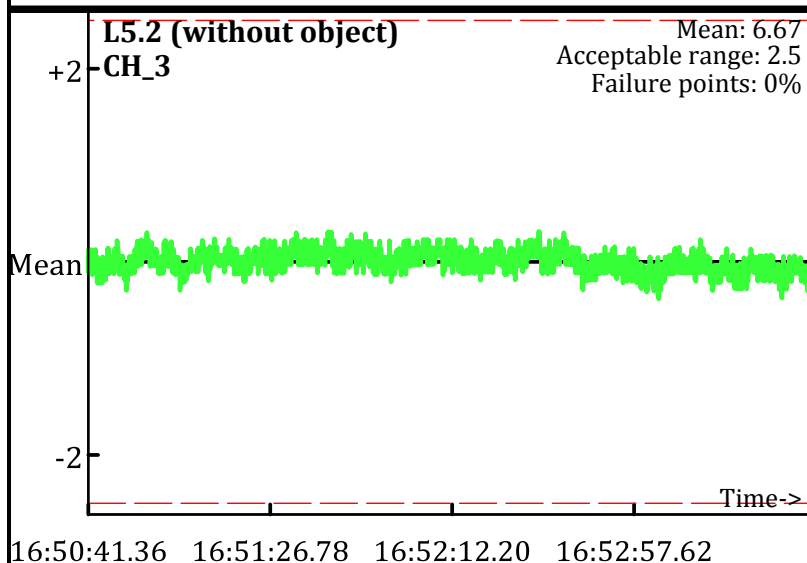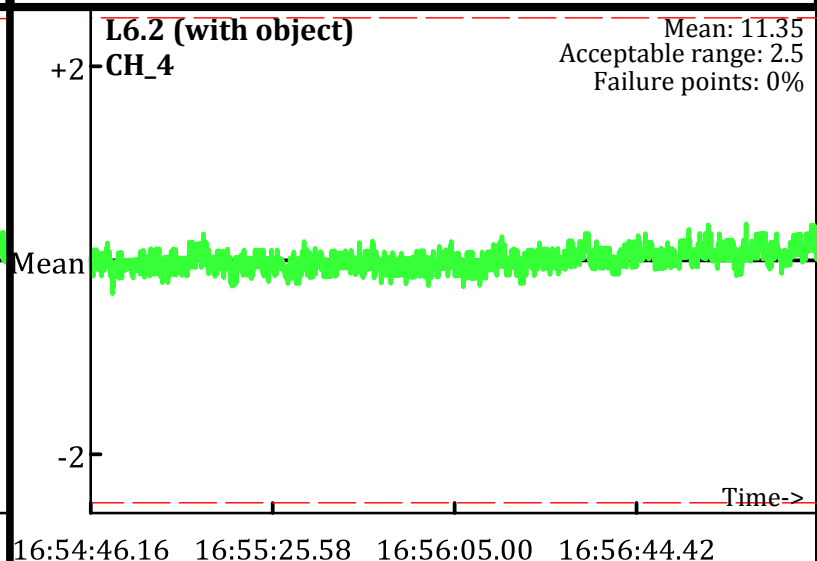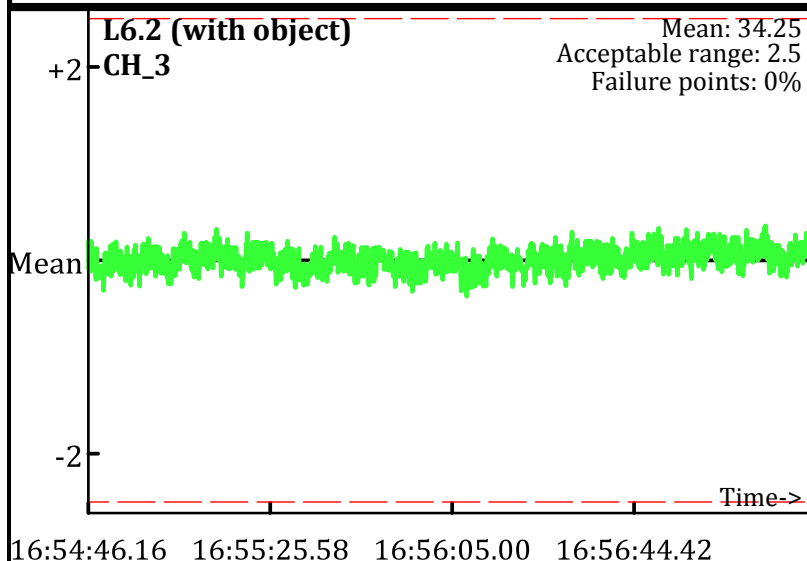Line Name: L5.2 L6.2 L5.2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
-- Acceptable limits

AM test
Operator: PN & SH
Date: 1/18/2010

L0 (without object)
CH_1
Mean: -187
Acceptable range:
Failure points: 1.61%

L0 (without object)
CH_2
Mean: -24.72
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_1
Mean: -86.35
Acceptable range: 2.5
Failure points: 32.6%

L1 (with object)
CH_2
Mean: 36.17
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_1
Mean: -179.09
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_2
Mean: -22.1
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
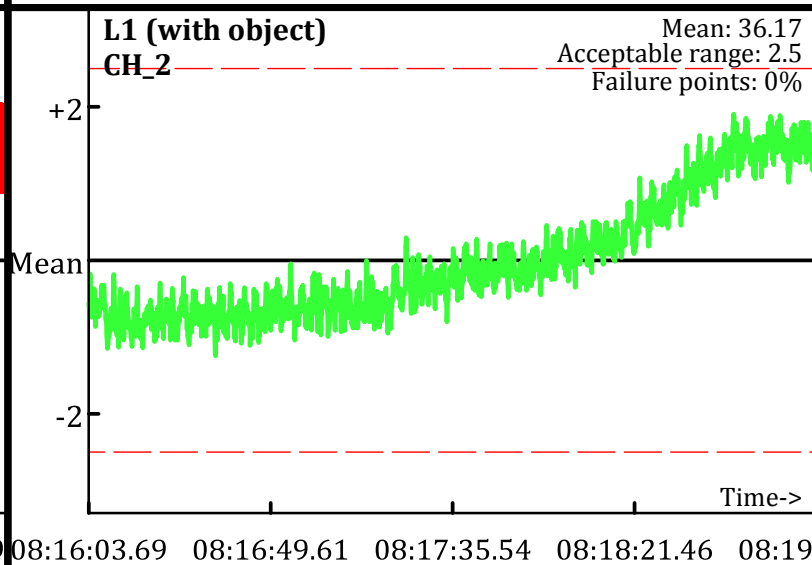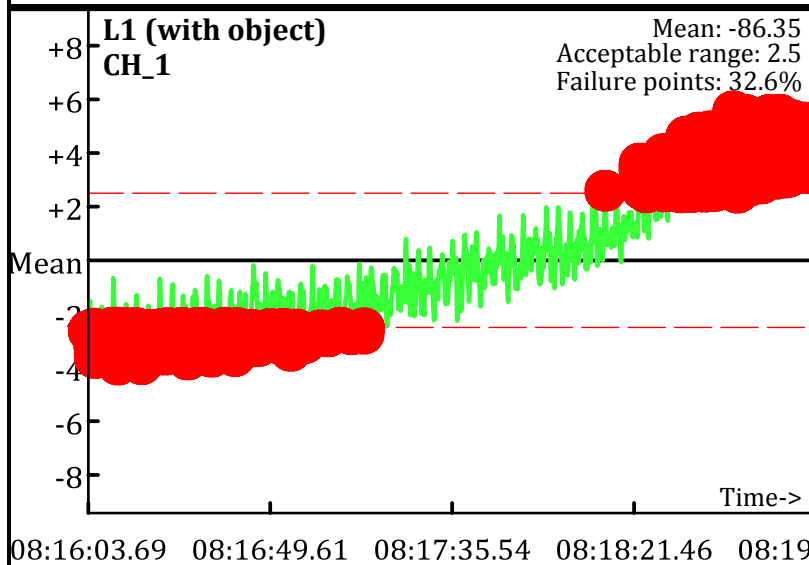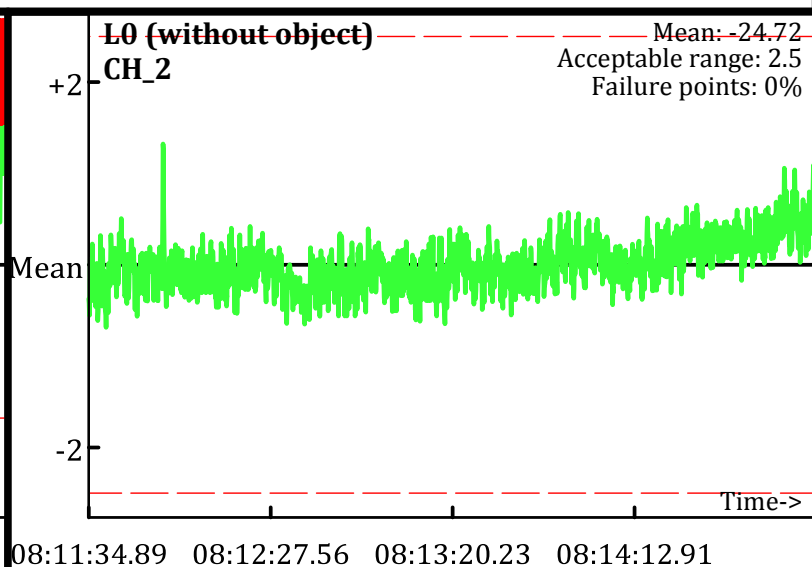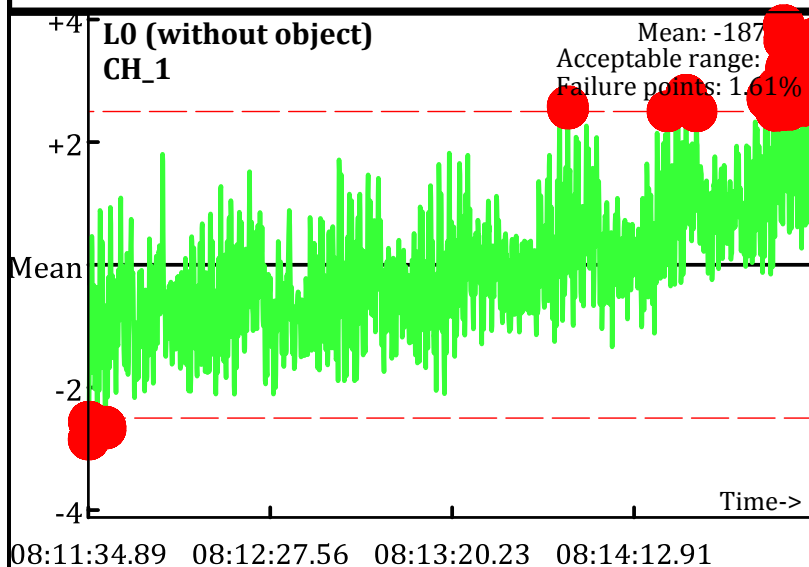Operator: PN & SH
Date: 1/18/2010

L0 (without object)
CH_3
Mean: 1.02
Acceptable range: 2.5
Failure points: 0%

L0 (without object)
CH_4
Mean: -2.41
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_3
Mean: 31.8
Acceptable range: 2.5
Failure points: 0%

L1 (with object)
CH_4
Mean: 10.74
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_3
Mean: 1.7
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_4
Mean: -2.32
Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
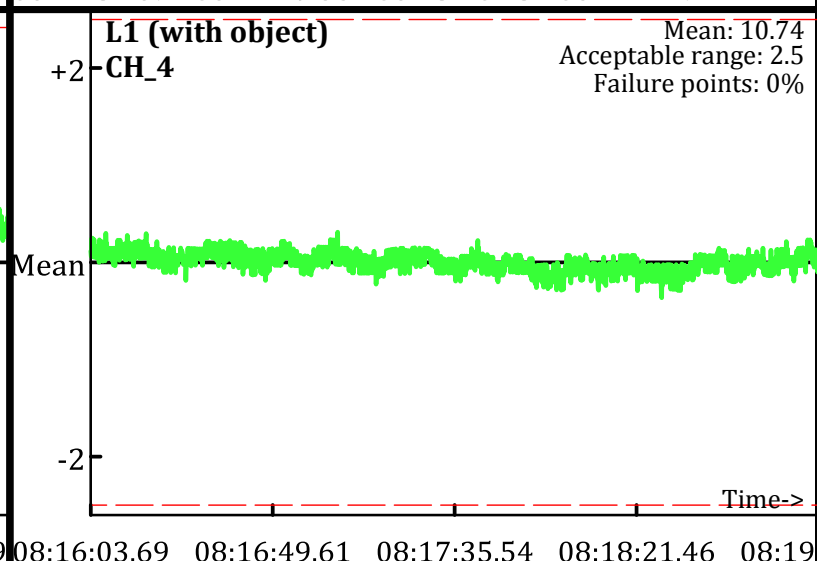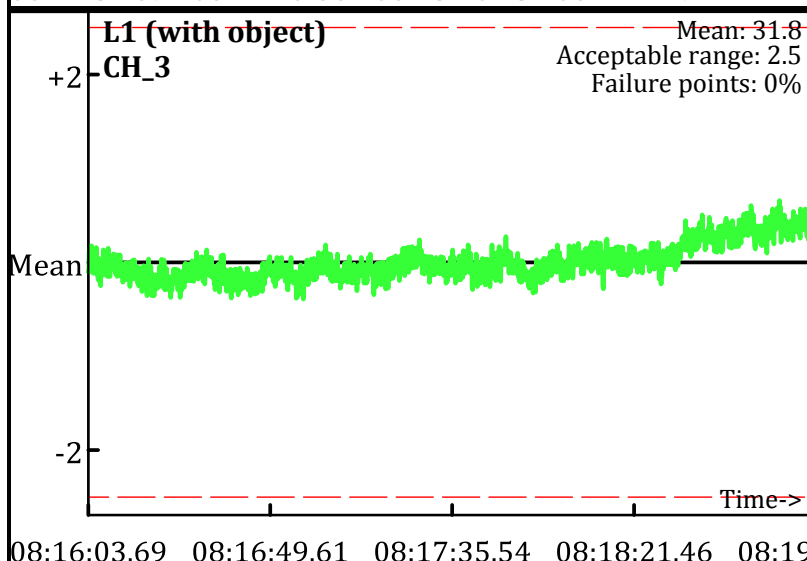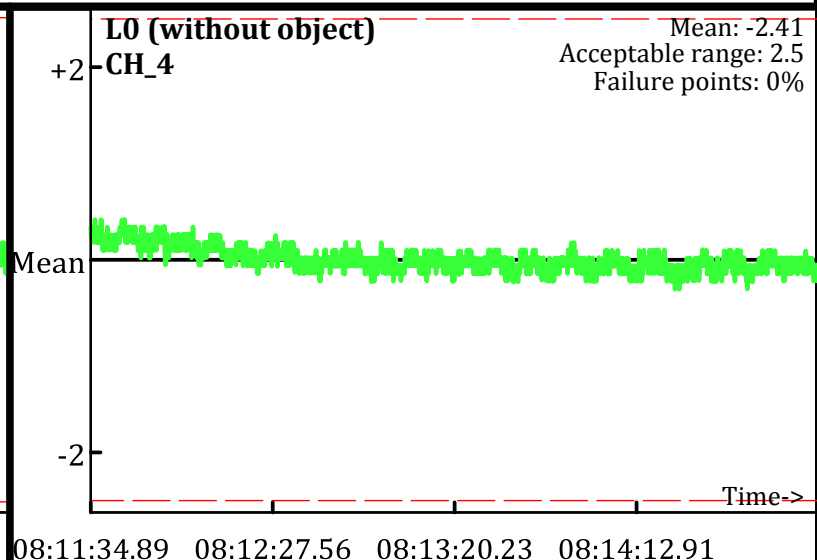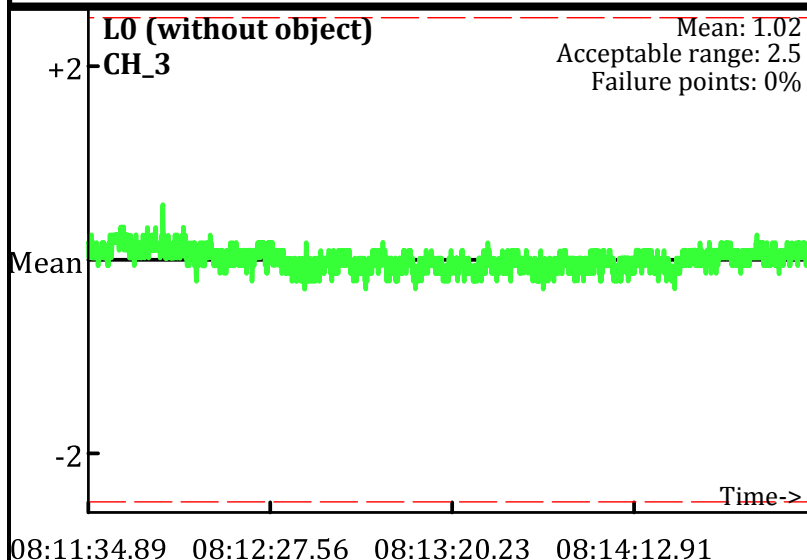Grid/Location: QC Area

⬤ Outside range
--- Acceptable limits

AM test
Operator: PN & SH
Date: 1/18/2010

L0.1 (without object)
CH_1

Mean: -144.59
Acceptable range: 2.5
Failure points: 0.237%

L0.1 (without object)
CH_2

Mean: -15.37
Acceptable range: 2.5
Failure points: 0%

08:11:34.91   08:12:27.58   08:13:20.26   08:14:12.93

08:11:34.91   08:12:27.58   08:13:20.26   08:14:12.93

L1.1 (with object)
CH_1

Mean: -21.75
Acceptable range: 2.5
Failure points: 6.85%

L1.1 (with object)
CH_2

Mean: 76.92
Acceptable range: 2.5
Failure points: 0%

08:16:03.61   08:16:49.56   08:17:35.51   08:18:21.47

08:16:03.61   08:16:49.56   08:17:35.51   08:18:21.47

L2.1 (without object)
CH_1

Mean: -135.51
Acceptable range: 2.5
Failure points: 0.119%

L2.1 (without object)
CH_2

Mean: -10.26
Acceptable range: 2.5
Failure points: 0%

08:20:16.42   08:20:37.37   08:20:58.31   08:21:19.26   08:21

08:20:16.42   08:20:37.37   08:20:58.31   08:21:19.26   08:21

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits

AM test
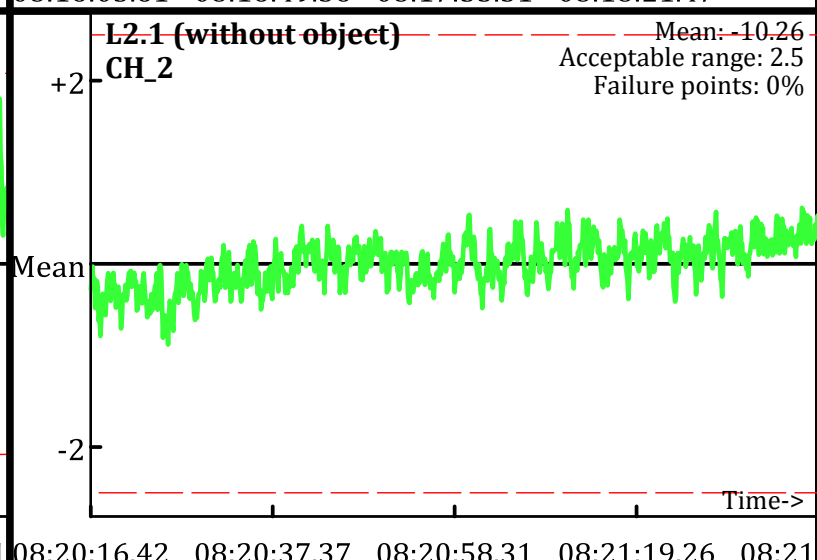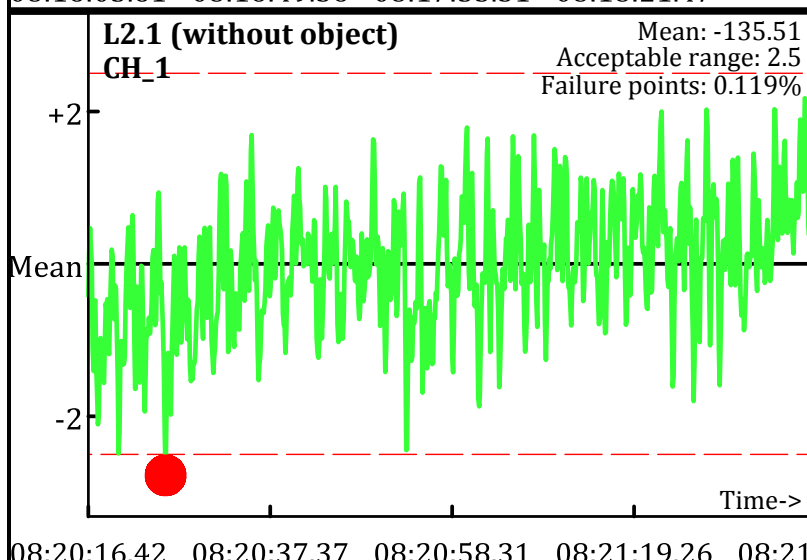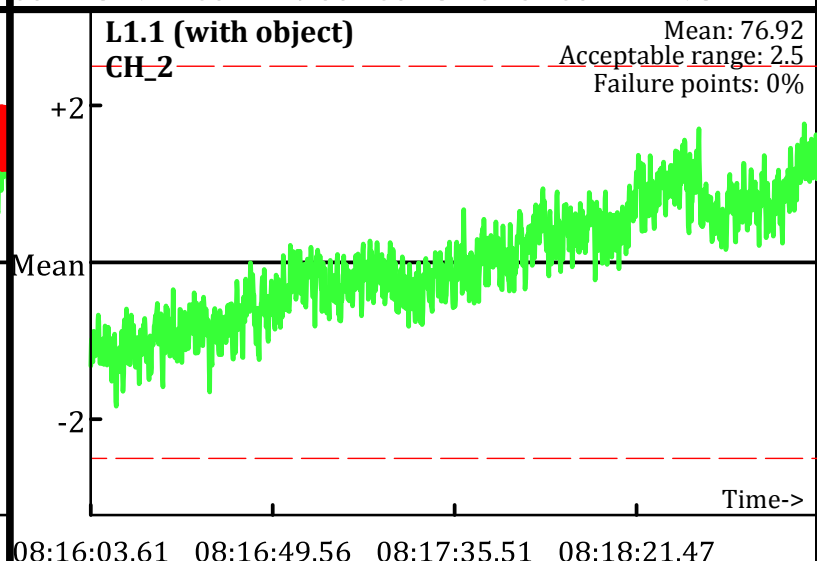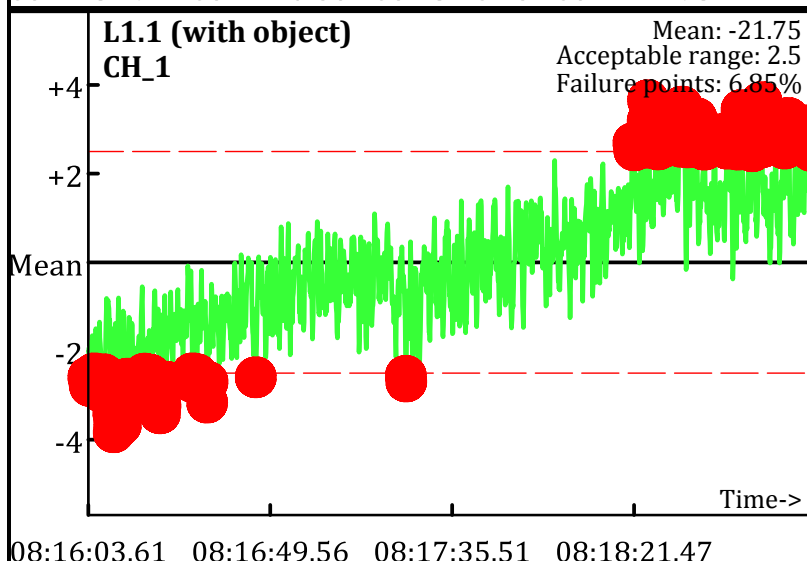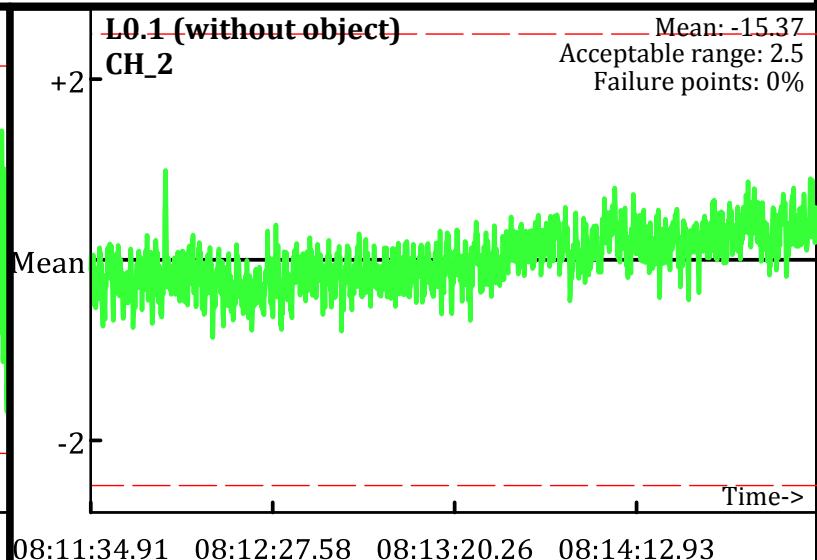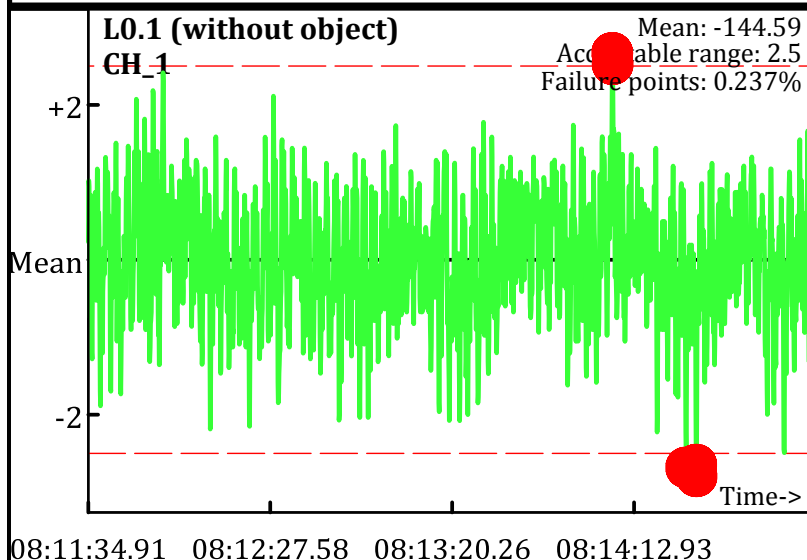Operator: PN & SH
Date: 1/18/2010

L0.1 (without object)
CH_3
Mean: 6.65
Acceptable range: 2.5
Failure points: 0%
Time->
08:11:34.91 08:12:27.58 08:13:20.26 08:14:12.93

L0.1 (without object)
CH_4
Mean: 1.57
Acceptable range: 2.5
Failure points: 0%
Time->
08:11:34.91 08:12:27.58 08:13:20.26 08:14:12.93

L1.1 (with object)
CH_3
Mean: 65.08
Acceptable range: 2.5
Failure points: 0%
Time->
08:16:03.61 08:16:49.56 08:17:35.51 08:18:21.47

L1.1 (with object)
CH_4
Mean: 32.53
Acceptable range: 2.5
Failure points: 0%
Time->
08:16:03.61 08:16:49.56 08:17:35.51 08:18:21.47

L2.1 (without object)
CH_3
Mean: 8.15
Acceptable range: 2.5
Failure points: 0%
Time->
08:20:16.42 08:20:37.37 08:20:58.31 08:21:19.26 08:21

L2.1 (without object)
CH_4
Mean: 1.62
Acceptable range: 2.5
Failure points: 0%
Time->
08:20:16.42 08:20:37.37 08:20:58.31 08:21:19.26 08:21

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
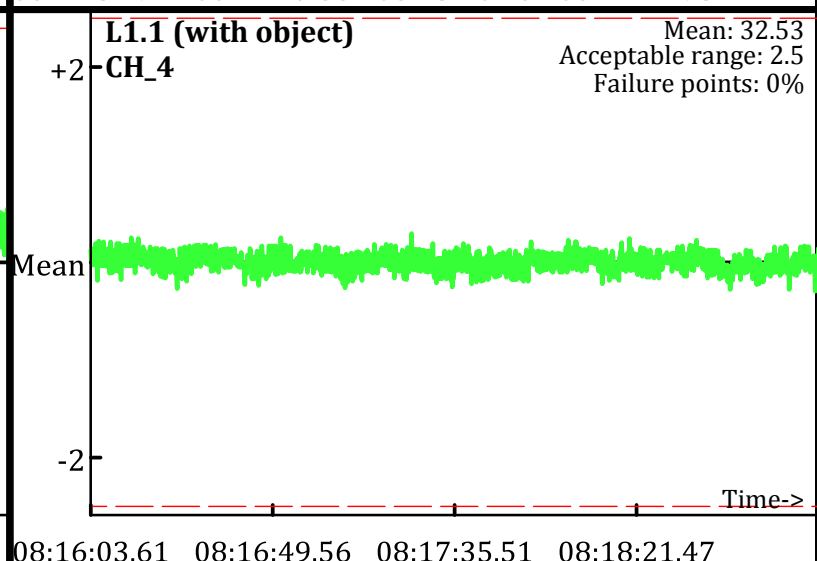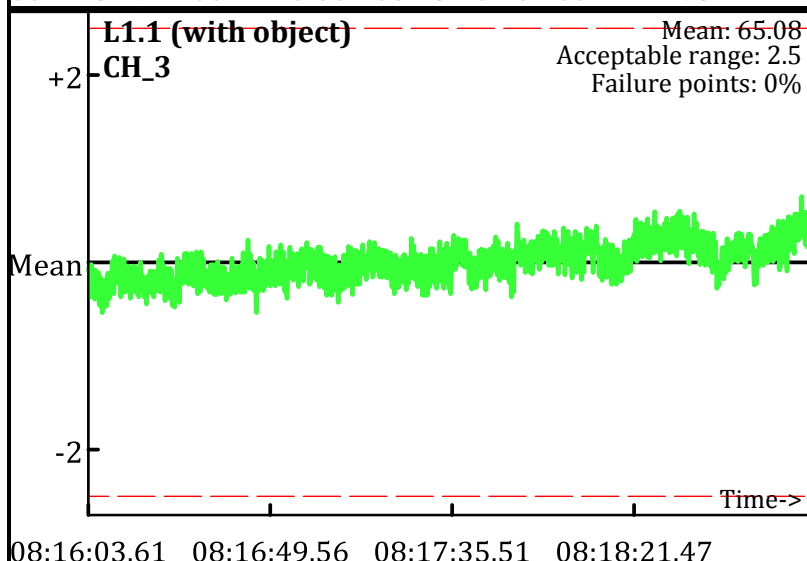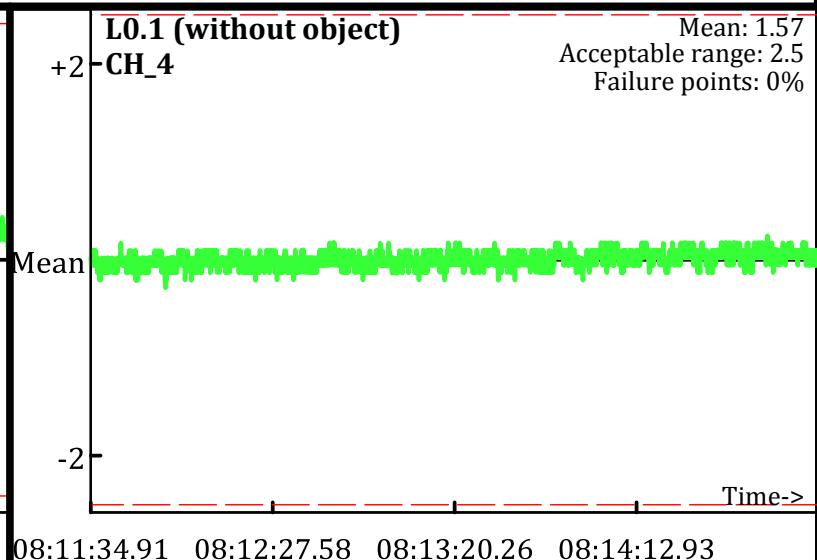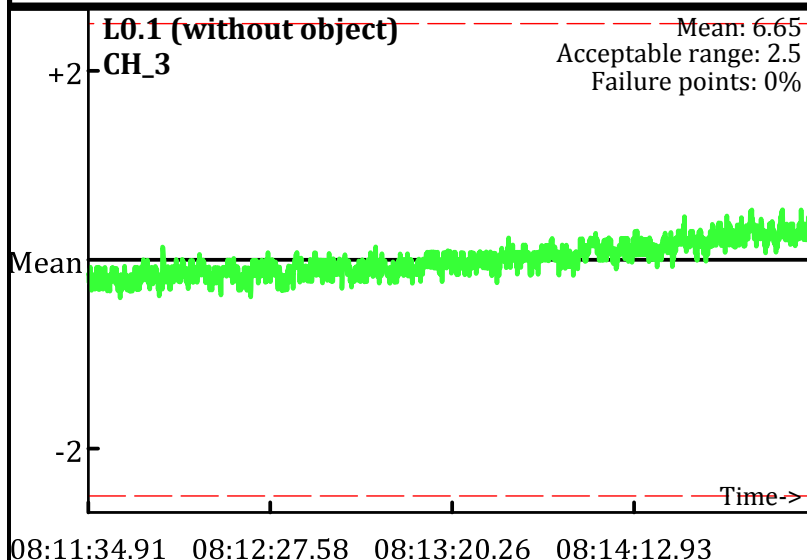Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & SH
Date: 1/18/2010

L0.2 (without object)
CH_1

Mean: -68.48
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

08:11:34.94   08:12:27.61   08:13:20.29   08:14:12.96

L0.2 (without object)
CH_2

Mean: 2.27
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

08:11:34.94   08:12:27.61   08:13:20.29   08:14:12.96

L1.2 (with object)
CH_1

Mean: 19.69
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

08:16:03.64   08:16:49.56   08:17:35.48   08:18:21.41   08:19

L1.2 (with object)
CH_2

Mean: 56.76
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

08:16:03.64   08:16:49.56   08:17:35.48   08:18:21.41   08:19

L2.2 (without object)
CH_1

Mean: -73.01
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

08:20:16.44   08:20:37.39   08:20:58.34   08:21:19.30

L2.2 (without object)
CH_2

Mean: -0.0066
Acceptable range: 2.5
Failure points: 0%

+2

Mean

-2

Time->

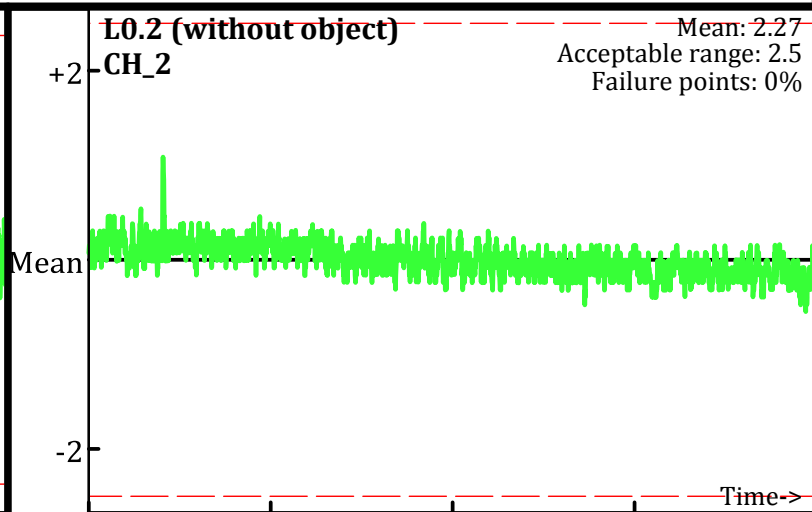08:20:16.44   08:20:37.39   08:20:58.34   08:21:19.30

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
— — Acceptable limits

AM test
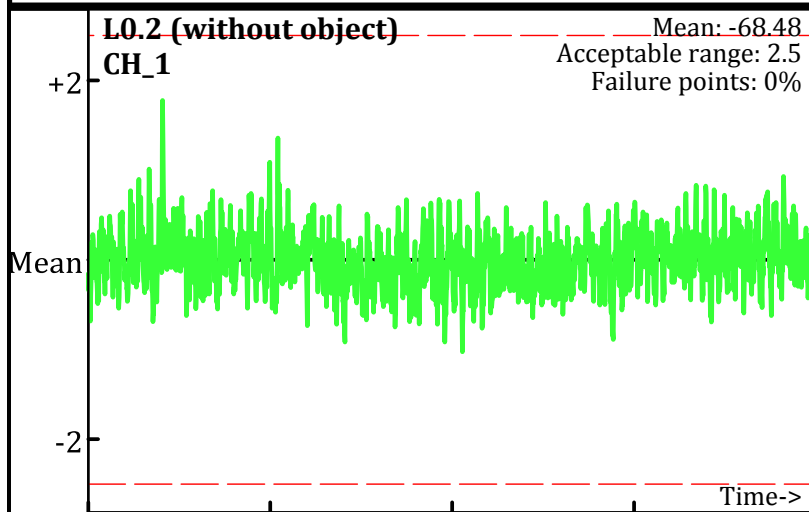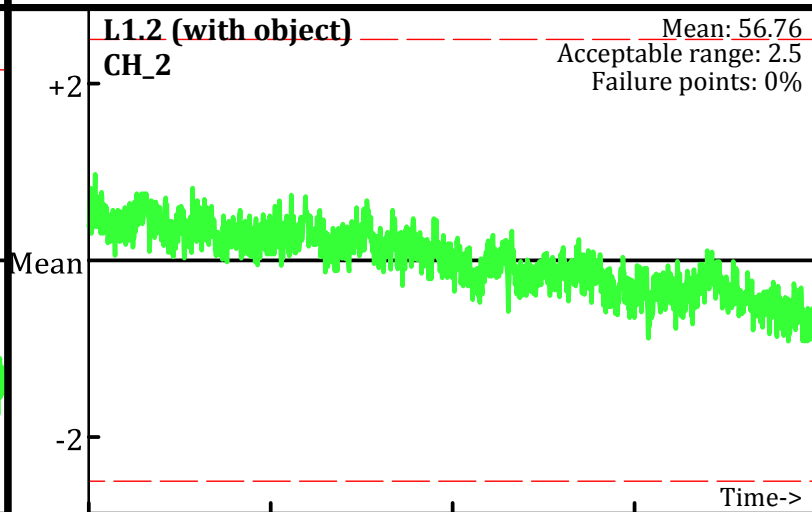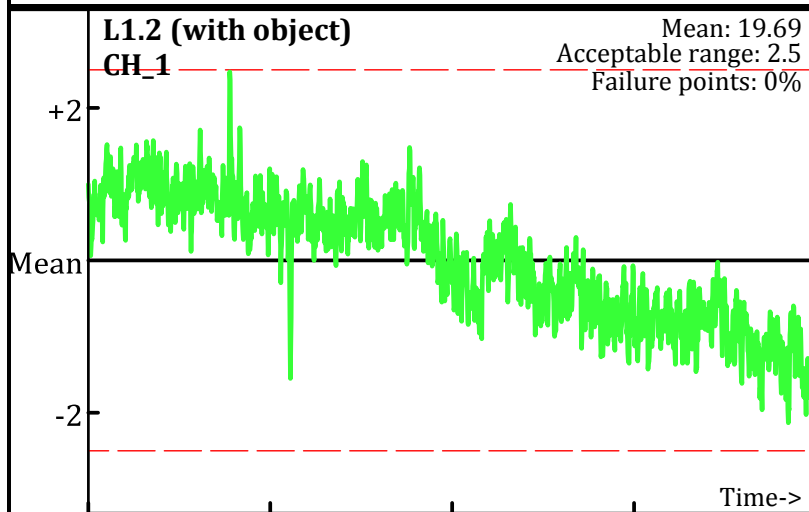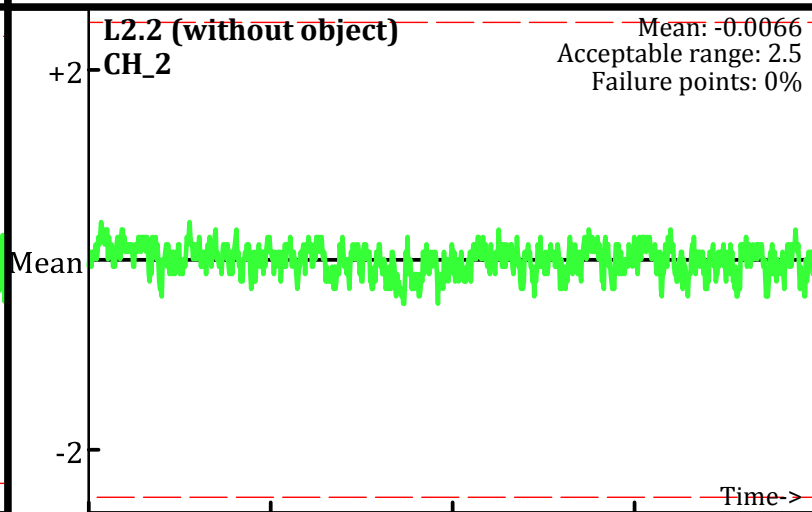Operator: PN & SH
Date: 1/18/2010

L0.2 (without object)
CH_3

Mean: 6.08
Acceptable range: 2.5
Failure points: 0%

08:11:34.94   08:12:27.61   08:13:20.29   08:14:12.96

L0.2 (without object)
CH_4

Mean: -0.5
Acceptable range: 2.5
Failure points: 0%

08:11:34.94   08:12:27.61   08:13:20.29   08:14:12.96

L1.2 (with object)
CH_3

Mean: 34.9
Acceptable range: 2.5
Failure points: 0%

08:16:03.64   08:16:49.56   08:17:35.48   08:18:21.41   08:19

L1.2 (with object)
CH_4

Mean: 12.25
Acceptable range: 2.5
Failure points: 0%

08:16:03.64   08:16:49.56   08:17:35.48   08:18:21.41   08:19

L2.2 (without object)
CH_3
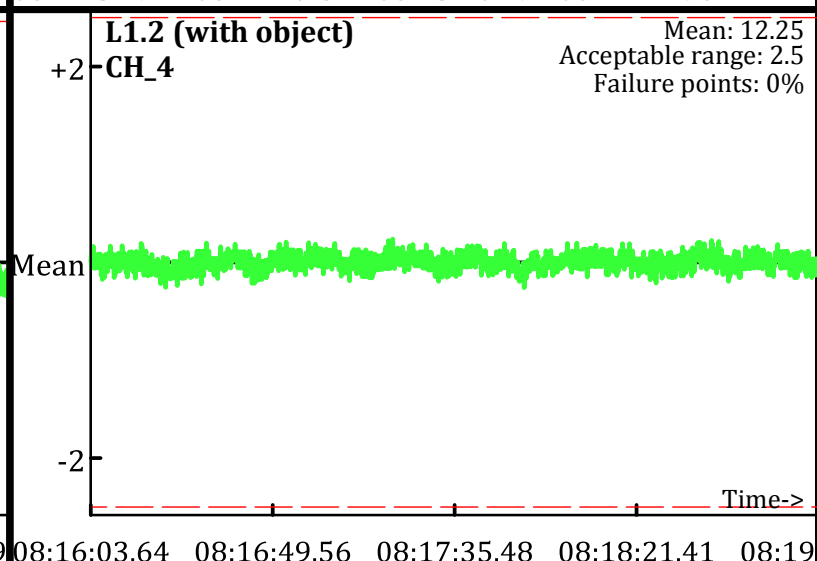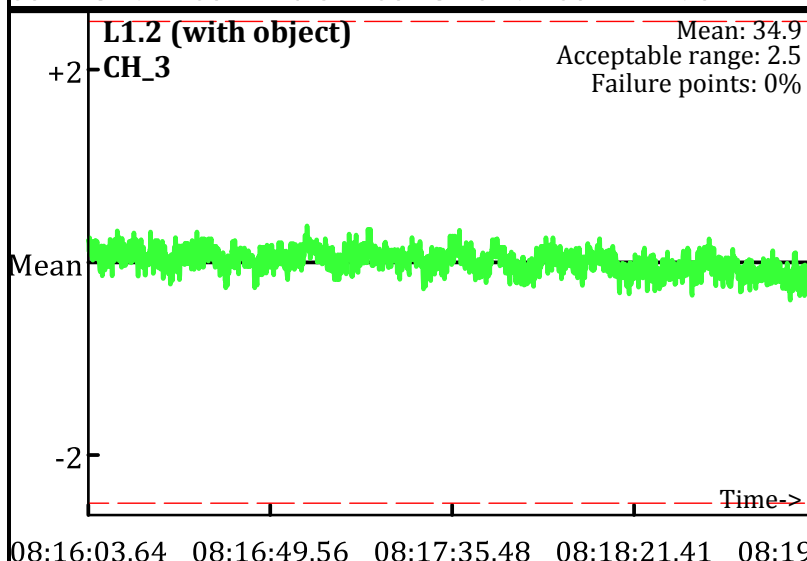
Mean: 5.46
Acceptable range: 2.5
Failure points: 0%

08:20:16.44   08:20:37.39   08:20:58.34   08:21:19.30

L2.2 (without object)
CH_4

Mean: -0.57
Acceptable range: 2.5
Failure points: 0%

08:20:16.44   08:20:37.39   08:20:58.34   08:21:19.30

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

PM test
Operator: PN & SH
Date: 1/18/2010

L5 (without object) CH_1
Mean: -133.9
Acceptable range: 2.5
Failure points: 0.0541%

L5 (without object) CH_2
Mean: -9.33
Acceptable range: 2.5
Failure points: 0%

14:52:48.33 14:53:34.53 14:54:20.73 14:55:06.93

L6 (with object) CH_1
Mean: -38.53
Acceptable range: 2.5
Failure points: 0%

L6 (with object) CH_2
Mean: 50.14
Acceptable range: 2.5
Failure points: 0%

14:57:05.12 14:57:48.30 14:58:31.48 14:59:14.65

L7 (without object) CH_1
Mean: -134.31
Acceptable range: 2.5
Failure points: 0.358%

L7 (without object) CH_2
Mean: -9.36
Acceptable range: 2.5
Failure points: 0%

15:00:57.94 15:01:11.88 15:01:25.83 15:01:39.77

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L5 L6 L7

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

⬤ Outside range
‑ ‑ ‑ Acceptable limits
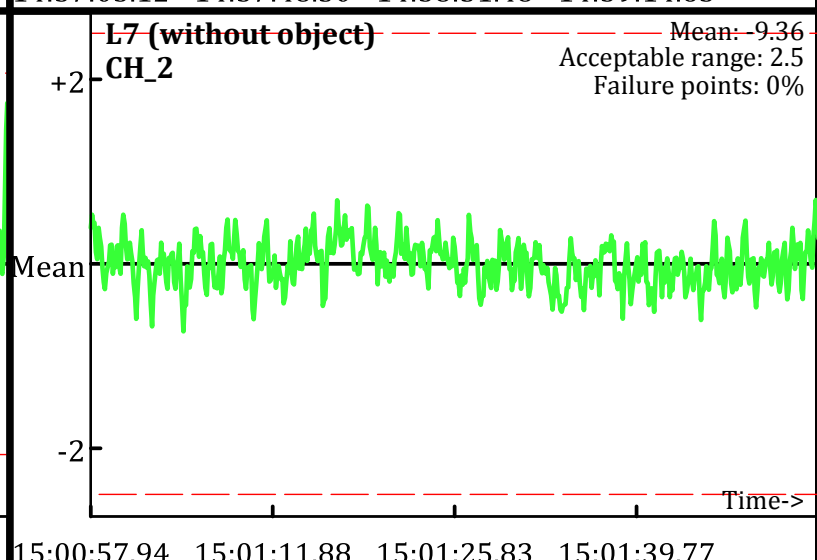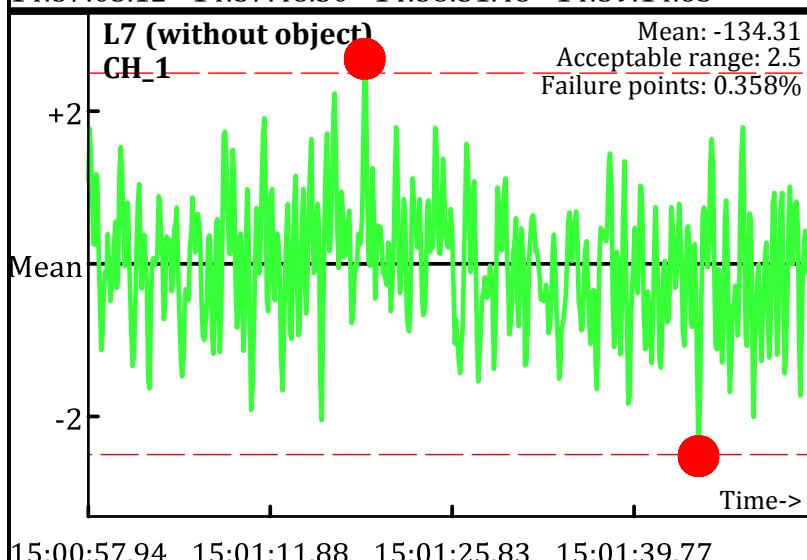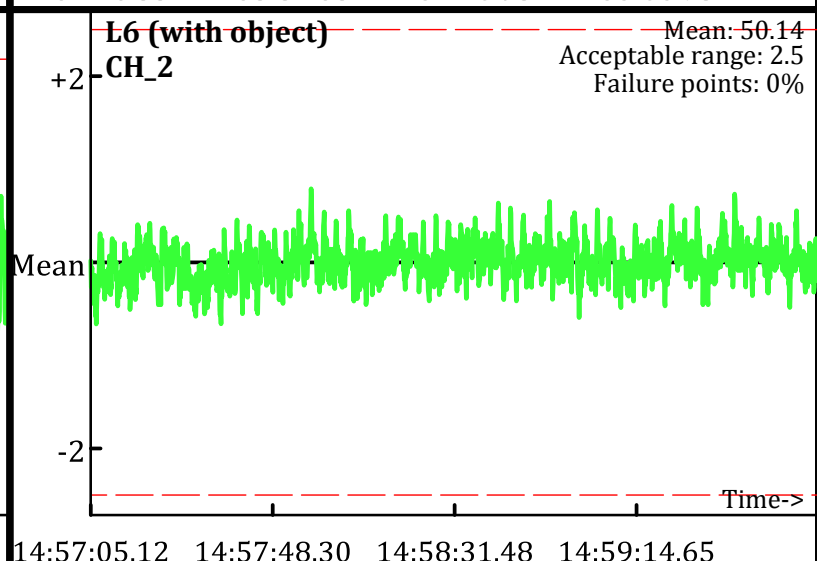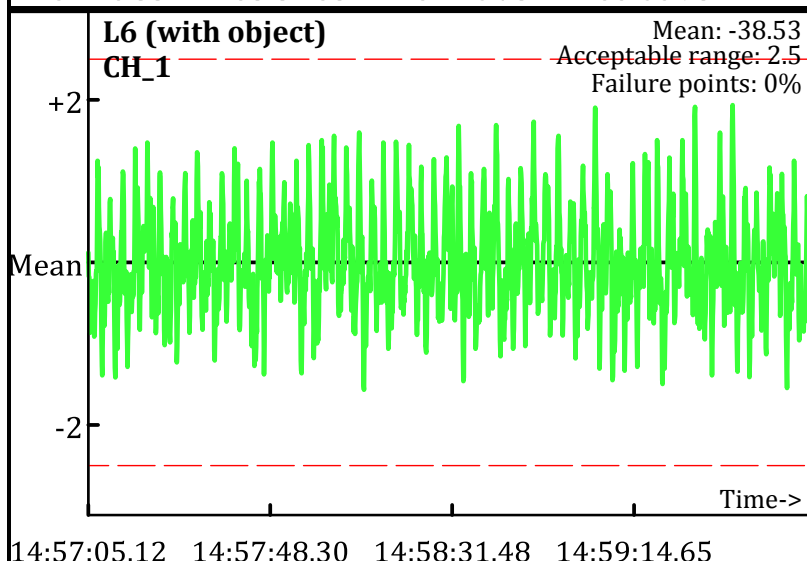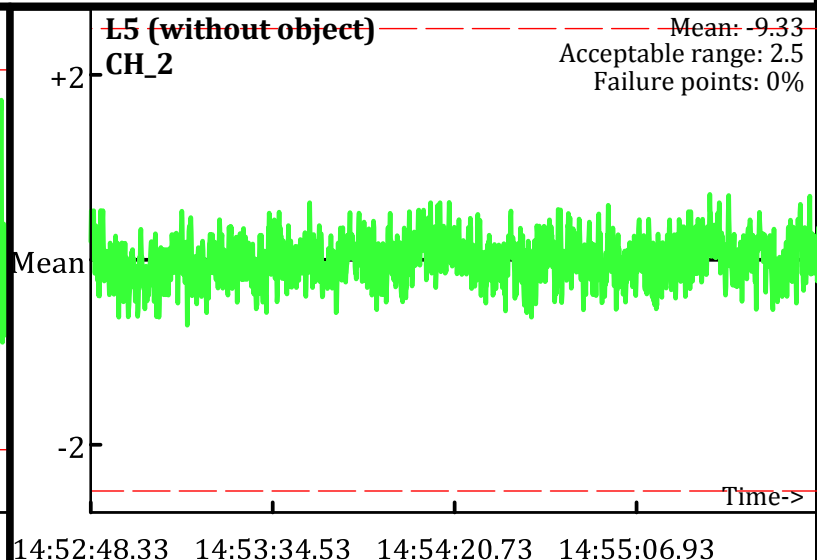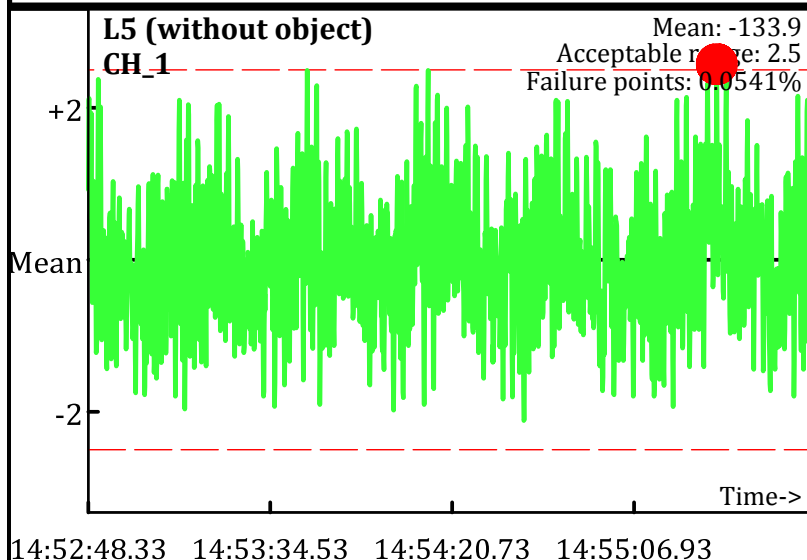
PM test
Operator: PN & SH
Date: 1/18/2010

L5 (without object)
CH_3
Mean: 4.1
Acceptable range: 2.5
Failure points: 0%

L5 (without object)
CH_4
Mean: -2.27
Acceptable range: 2.5
Failure points: 0%

14:52:48.33   14:53:34.53   14:54:20.73   14:55:06.93

14:52:48.33   14:53:34.53   14:54:20.73   14:55:06.93

L6 (with object)
CH_3
Mean: 35.05
Acceptable range: 2.5
Failure points: 0%

L6 (with object)
CH_4
Mean: 11.26
Acceptable range: 2.5
Failure points: 0%

14:57:05.12   14:57:48.30   14:58:31.48   14:59:14.65

14:57:05.12   14:57:48.30   14:58:31.48   14:59:14.65

L7 (without object)
CH_3
Mean: 4.2
Acceptable range: 2.5
Failure points: 0%

L7 (without object)
CH_4
Mean: -2.26
Acceptable range: 2.5
Failure points: 0%

15:00:57.94   15:01:11.88   15:01:25.83   15:01:39.77

15:00:57.94   15:01:11.88   15:01:25.83   15:01:39.77

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L5 L6 L7

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
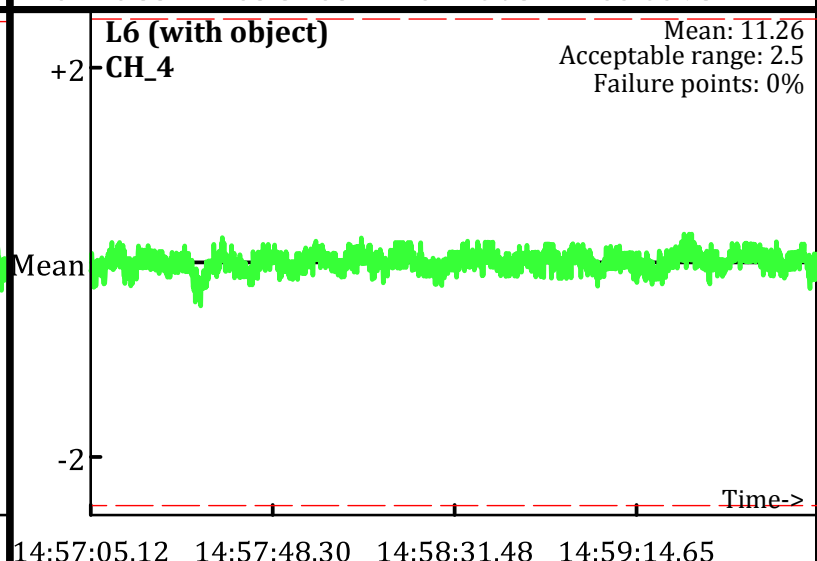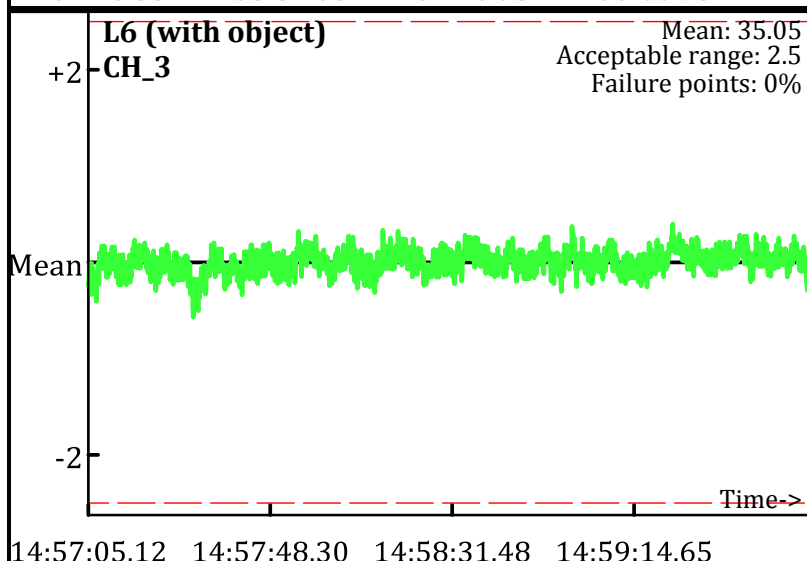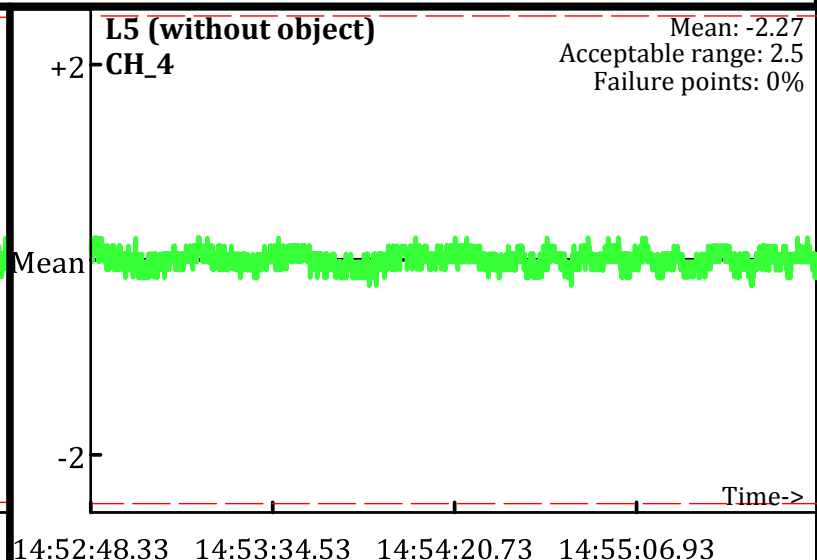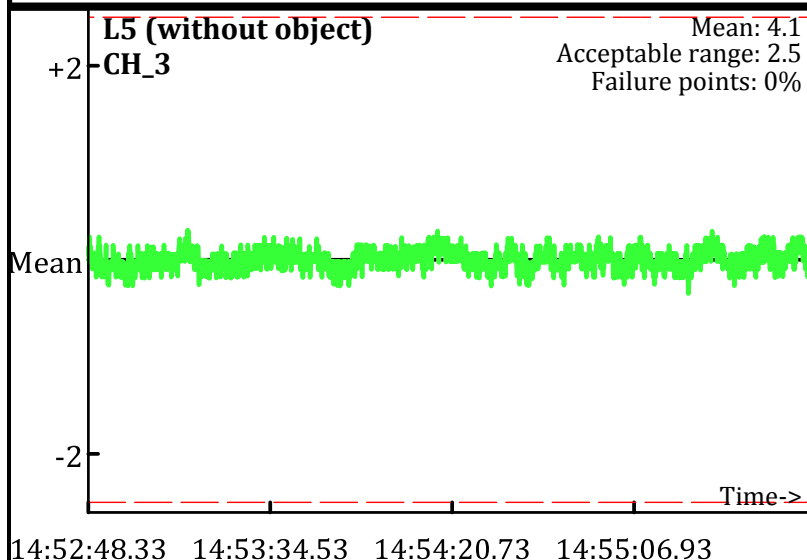Grid/Location: QC Area

● Outside range
– – Acceptable limits

PM test
Operator: PN & SH
Date: 1/18/2010

L5.1 (without object)
CH_1
Mean: -77.3
Acceptable range: 2.5
Failure points: 0.27%

14:52:48.34 14:53:34.55 14:54:20.75 14:55:06.95

L5.1 (without object)
CH_2
Mean: 6.22
Acceptable range: 2.5
Failure points: 0%

14:52:48.34 14:53:34.55 14:54:20.75 14:55:06.95

L6.1 (with object)
CH_1
Mean: 42.92
Acceptable range: 2.5
Failure points: 0%

14:57:05.14 14:57:48.32 14:58:31.50 14:59:14.68

L6.1 (with object)
CH_2
Mean: 96.99
Acceptable range: 2.5
Failure points: 0%

14:57:05.14 14:57:48.32 14:58:31.50 14:59:14.68

L7.1 (without object)
CH_1
Mean: -78.25
Acceptable range: 2.5
Failure points: 0%

15:00:57.84 15:01:11.82 15:01:25.80 15:01:39.77

L7.1 (without object)
CH_2
Mean: 6.03
Acceptable range: 2.5
Failure points: 0%

15:00:57.84 15:01:11.82 15:01:25.80 15:01:39.77

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L5.1 L6.1 L7.1

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
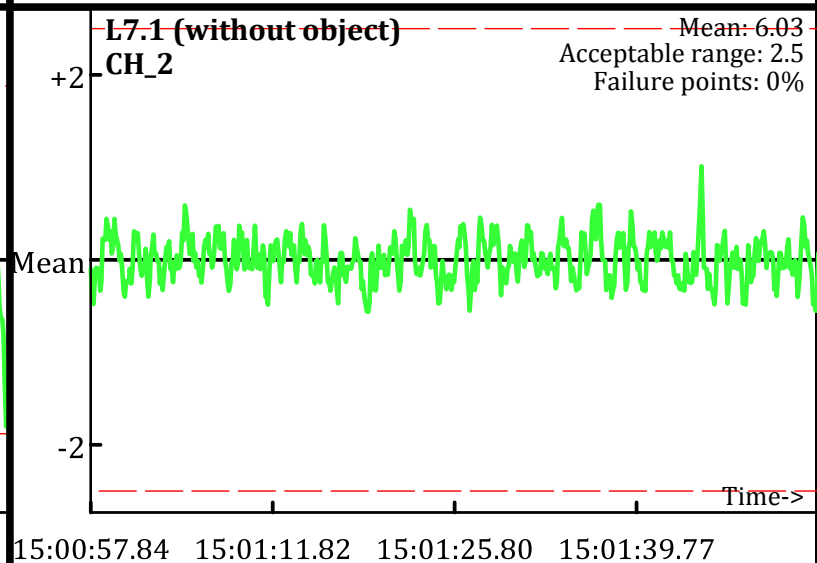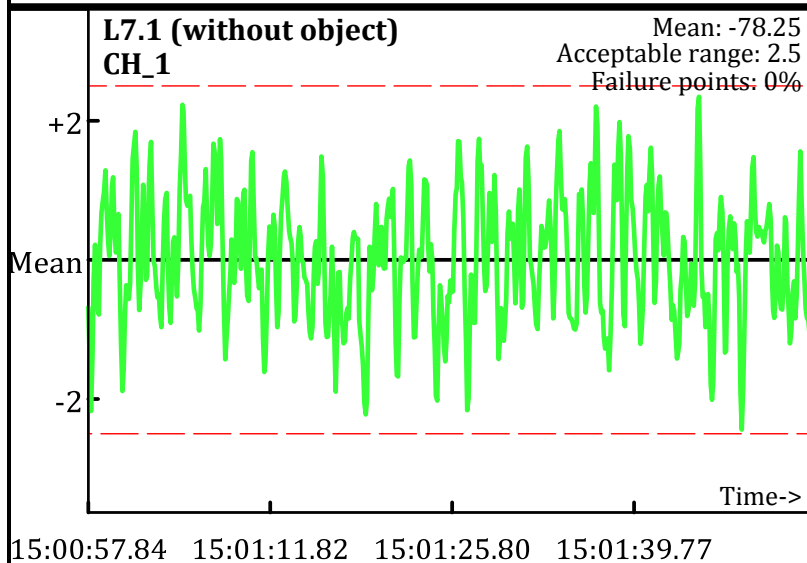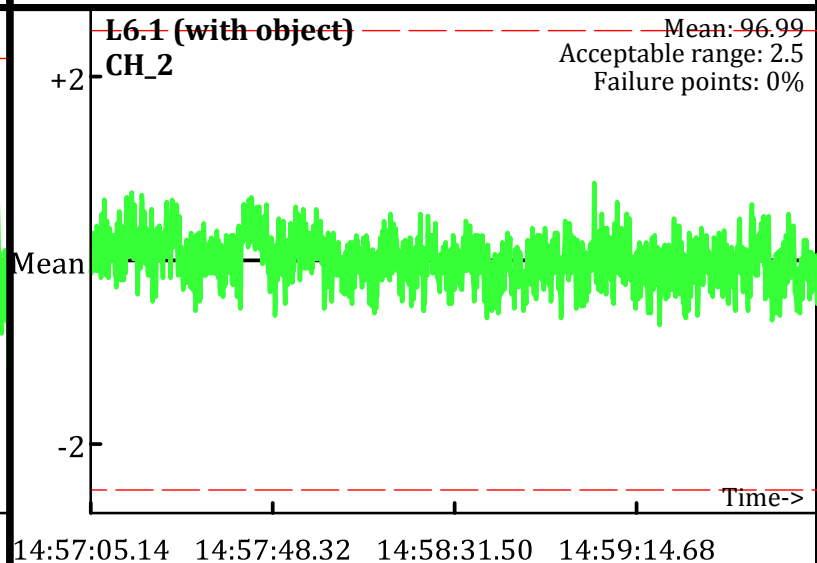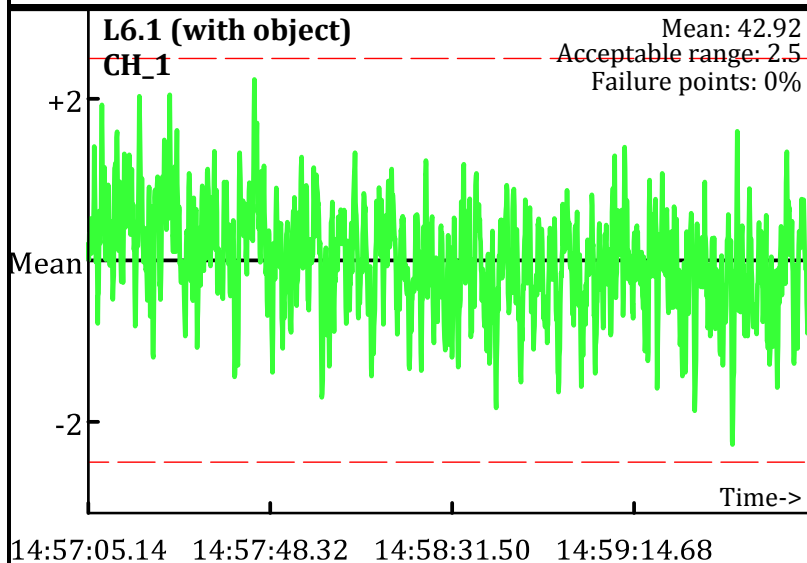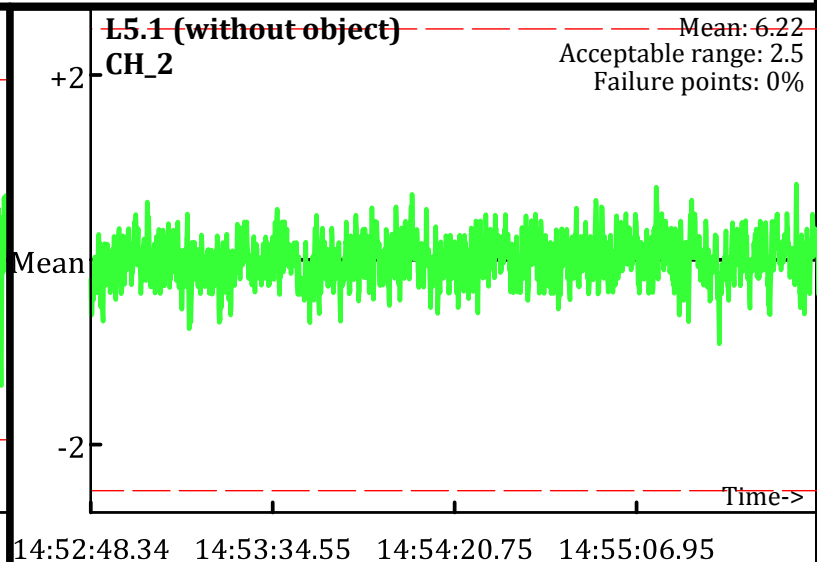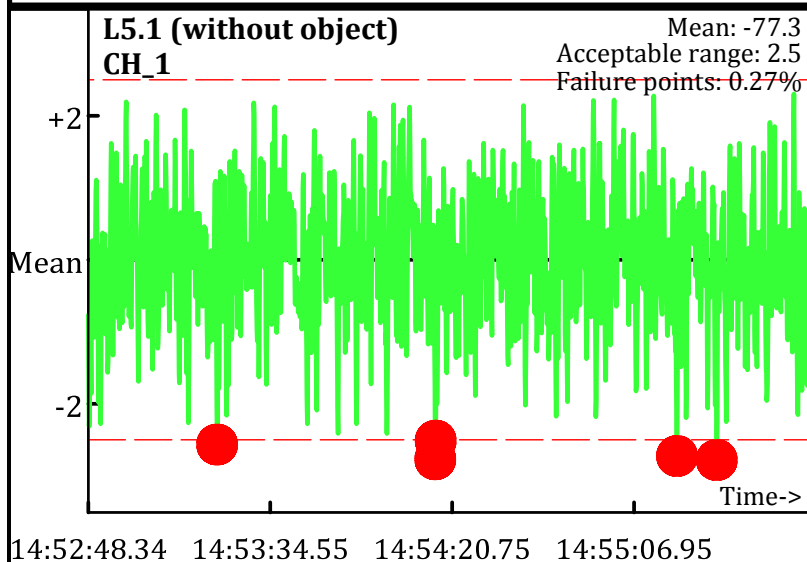– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/18/2010

L5.1 (without object)
CH_3
Mean: 11.34
Acceptable range: 2.5
Failure points: 0%

14:52:48.34   14:53:34.55   14:54:20.75   14:55:06.95

L5.1 (without object)
CH_4
Mean: 2.13
Acceptable range: 2.5
Failure points: 0%

14:52:48.34   14:53:34.55   14:54:20.75   14:55:06.95

L6.1 (with object)
CH_3
Mean: 69.58
Acceptable range: 2.5
Failure points: 0%

14:57:05.14   14:57:48.32   14:58:31.50   14:59:14.68

L6.1 (with object)
CH_4
Mean: 33.4
Acceptable range: 2.5
Failure points: 0%

14:57:05.14   14:57:48.32   14:58:31.50   14:59:14.68

L7.1 (without object)
CH_3
Mean: 11.39
Acceptable range: 2.5
Failure points: 0%

15:00:57.84   15:01:11.82   15:01:25.80   15:01:39.77

L7.1 (without object)
CH_4
Mean: 2.15
Acceptable range: 2.5
Failure points: 0%

15:00:57.84   15:01:11.82   15:01:25.80   15:01:39.77

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L5.1 L6.1 L7.1

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
--- Acceptable limits

PM test
Operator: PN & SH
Date: 1/18/2010
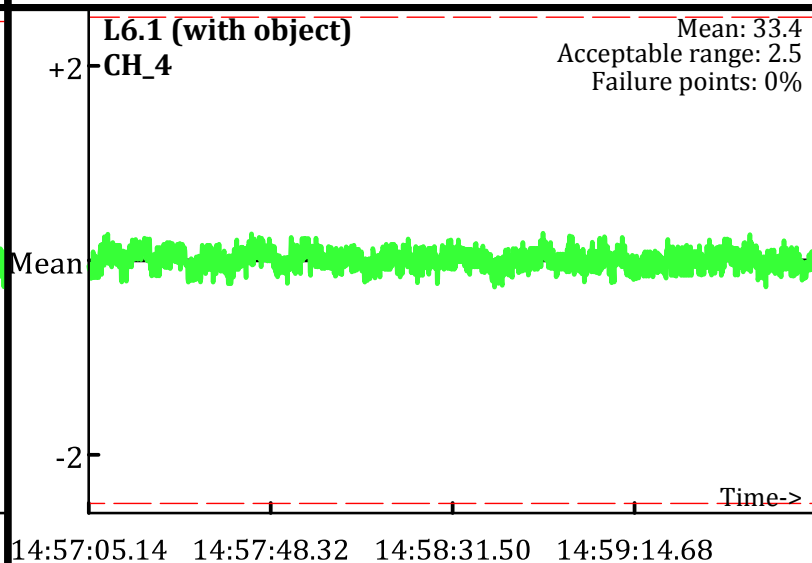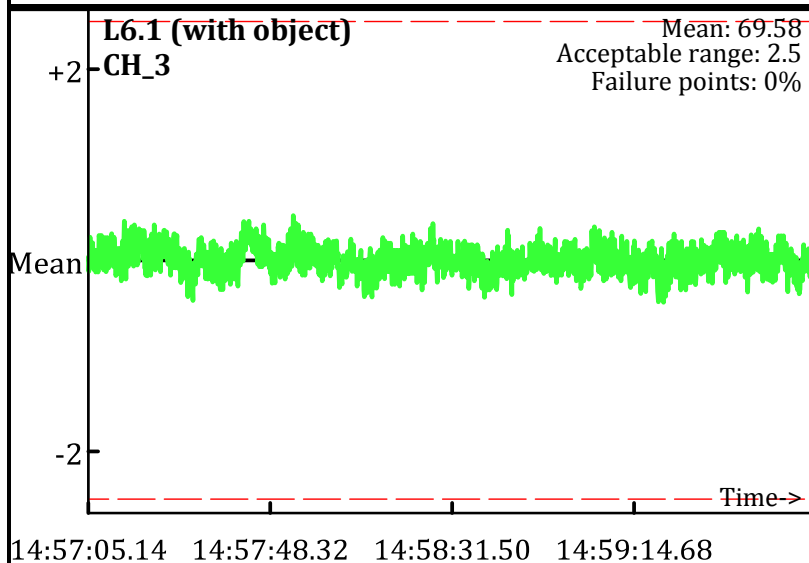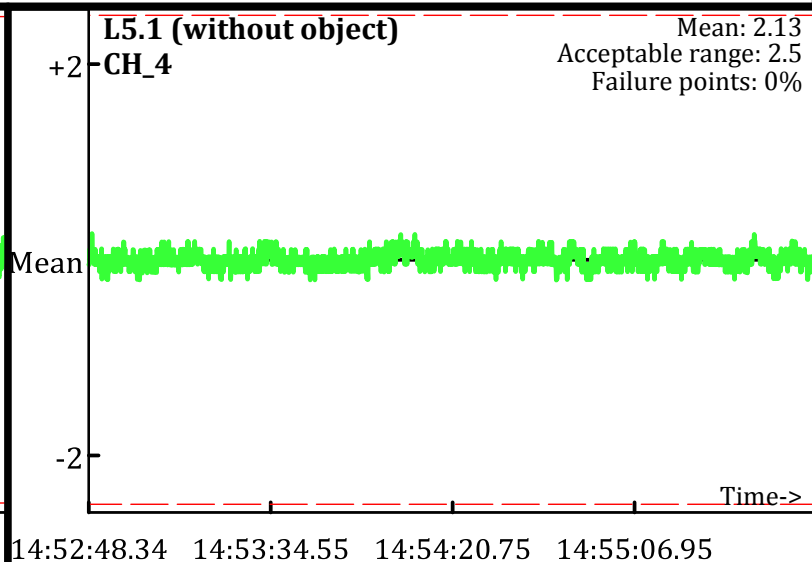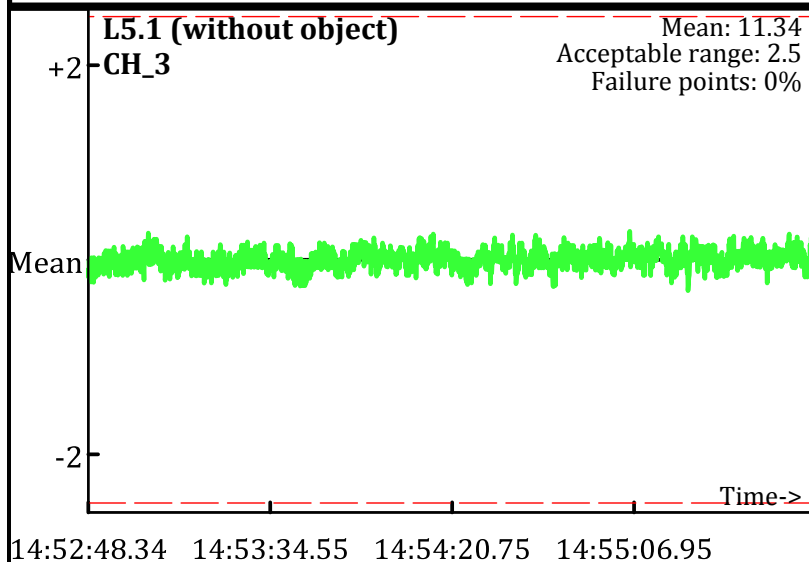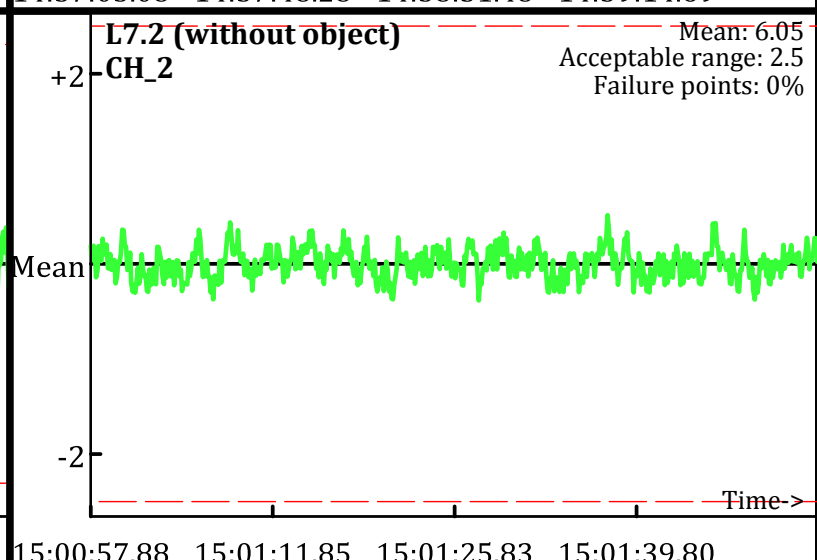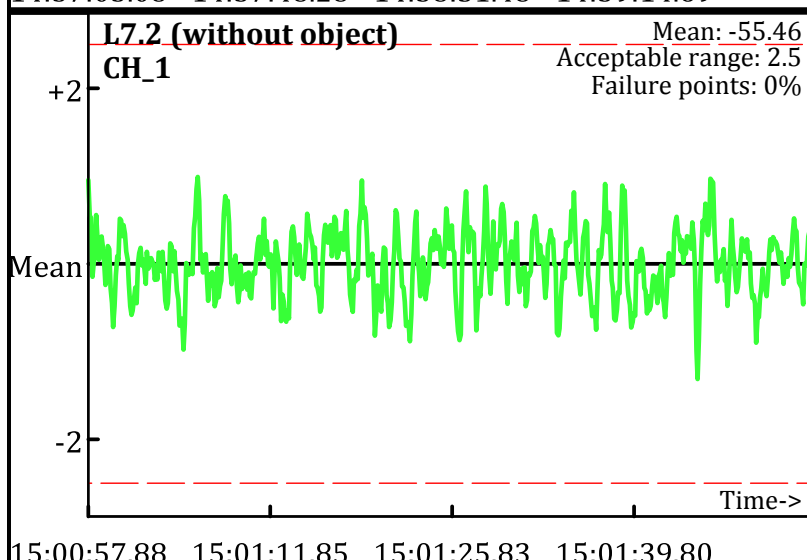
L5.2 (without object)
CH_1
Mean: -55.72
Acceptable range: 2.5
Failure points: 0%

Time->

14:52:48.39   14:53:34.56   14:54:20.73   14:55:06.91   14:55

L5.2 (without object)
CH_2
Mean: 5.91
Acceptable range: 2.5
Failure points: 0%

Time->

14:52:48.39   14:53:34.56   14:54:20.73   14:55:06.91   14:55

L6.2 (with object)
CH_1
Mean: 31.25
Acceptable range: 2.5
Failure points: 0%

Time->

14:57:05.08   14:57:48.28   14:58:31.48   14:59:14.69

L6.2 (with object)
CH_2
Mean: 59.71
Acceptable range: 2.5
Failure points: 0%

Time->

14:57:05.08   14:57:48.28   14:58:31.48   14:59:14.69

L7.2 (without object)
CH_1
Mean: -55.46
Acceptable range: 2.5
Failure points: 0%

Time->

15:00:57.88   15:01:11.85   15:01:25.83   15:01:39.80

L7.2 (without object)
CH_2
Mean: 6.05
Acceptable range: 2.5
Failure points: 0%

Time->

15:00:57.88   15:01:11.85   15:01:25.83   15:01:39.80

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
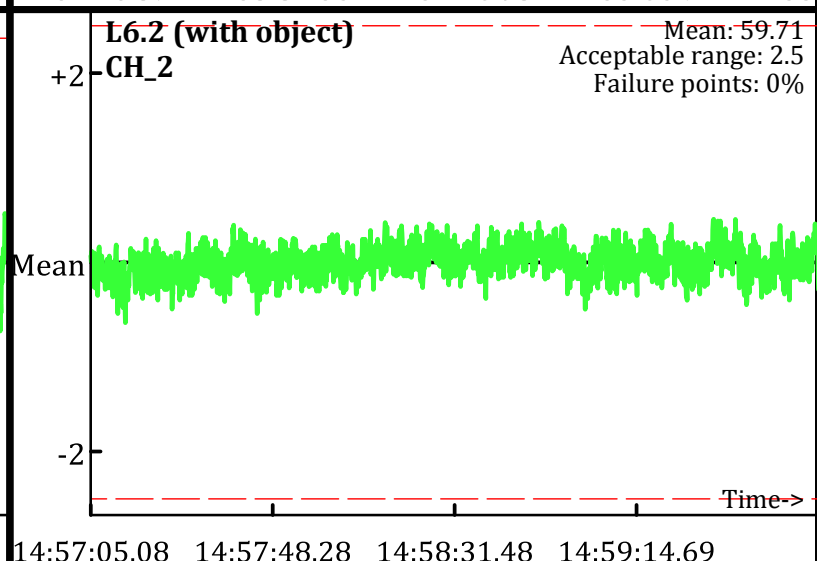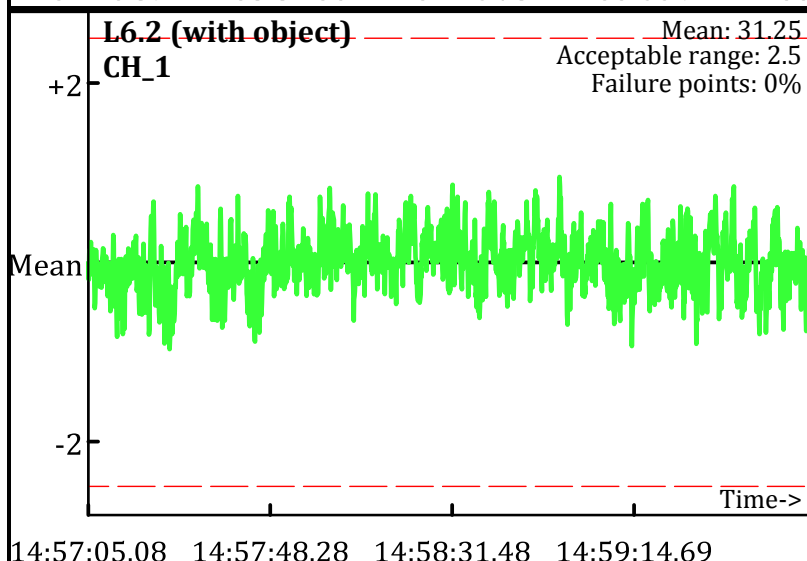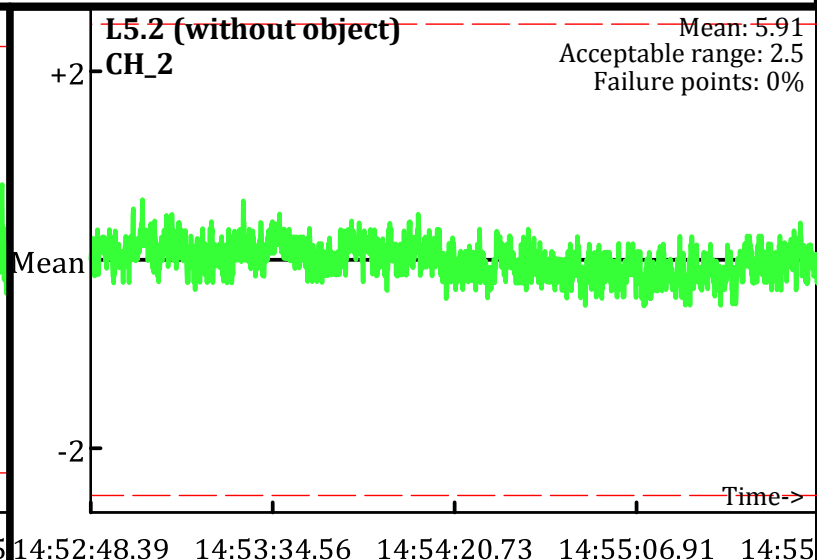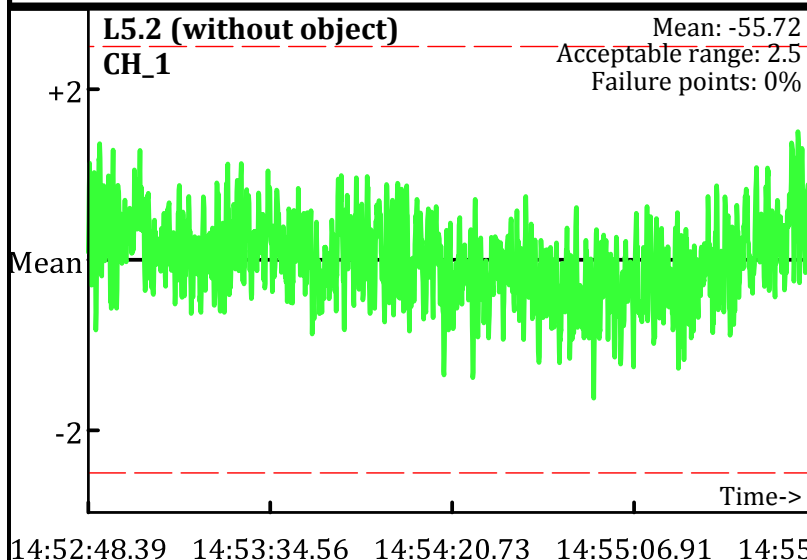Line Name: L5.2 L6.2 L7.2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
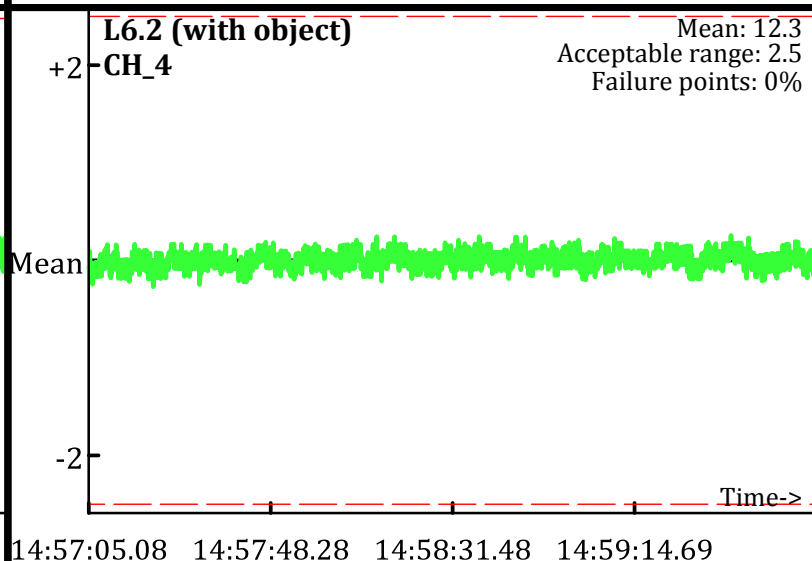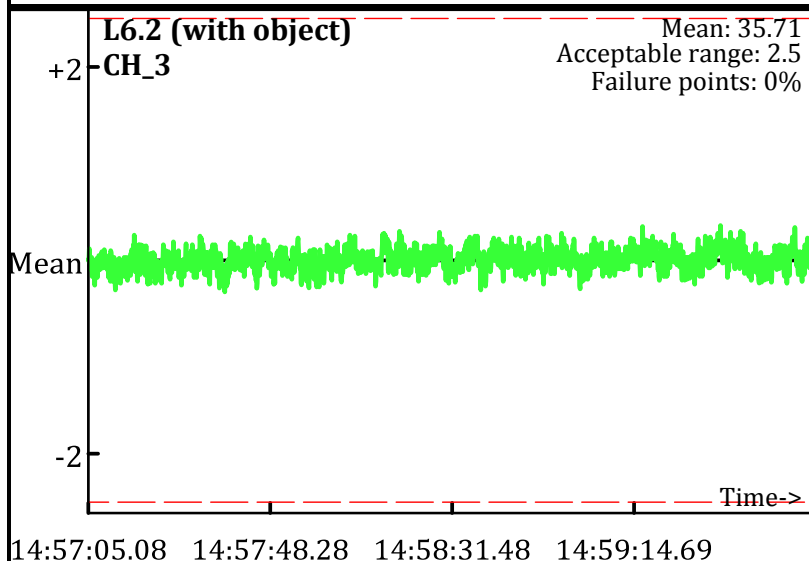Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
Operator: PN & SH
Date: 1/18/2010

L5.2 (without object)
CH_3
Mean: 7.49
Acceptable range: 2.5
Failure points: 0%

L5.2 (without object)
CH_4
Mean: 0.078
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_3
Mean: 35.71
Acceptable range: 2.5
Failure points: 0%

L6.2 (with object)
CH_4
Mean: 12.3
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_3
Mean: 7.51
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_4
Mean: 0.068
Acceptable range: 2.5
Failure points: 0%

Database: D:\Projects_QCReports_Ord_Data\011810\QC\011810_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

L0 (without object)
CH_1
Mean: -140.16
Acceptable range: 2.5
Failure points: 0.477%

L0 (without object)
CH_2
Mean: -9.45
Acceptable range: 2.5
Failure points: 0%

Time->

11:24:25.41   11:24:56.86   11:25:28.30   11:25:59.75

L1 (with object)
CH_1
Mean: -42.38
Acceptable range: 2.5
Failure points: 0.115%

L1 (with object)
CH_2
Mean: 49.45
Acceptable range: 2.5
Failure points: 0%

Time->

11:29:09.20   11:29:30.90   11:29:52.60   11:30:14.30

L2 (without object)
CH_1
Mean: -134.32
Acceptable range: 2.5
Failure points: 0%

L2 (without object)
CH_2
Mean: -8.36
Acceptable range: 2.5
Failure points: 0%

Time->

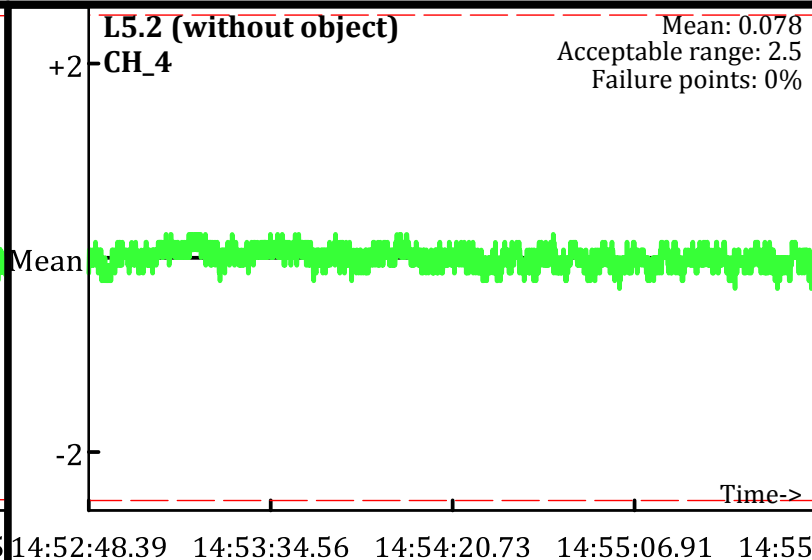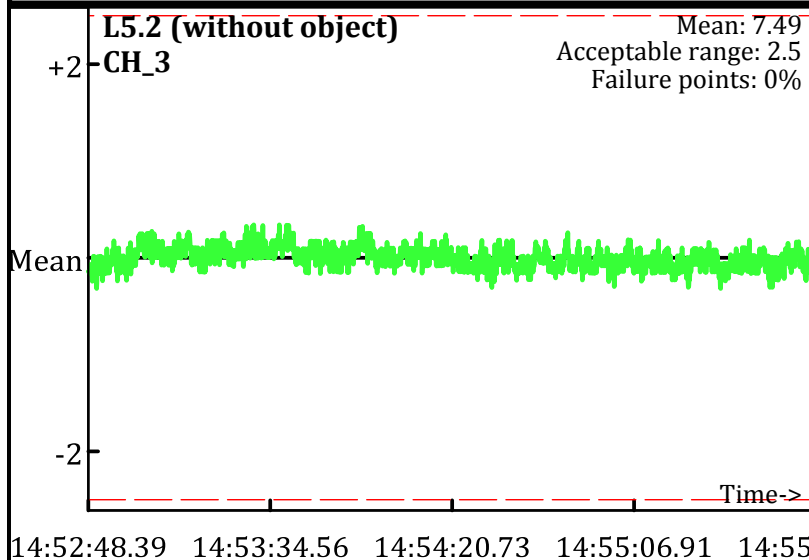11:32:14.00   11:32:17.72   11:32:21.44   11:32:25.17   11:32

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
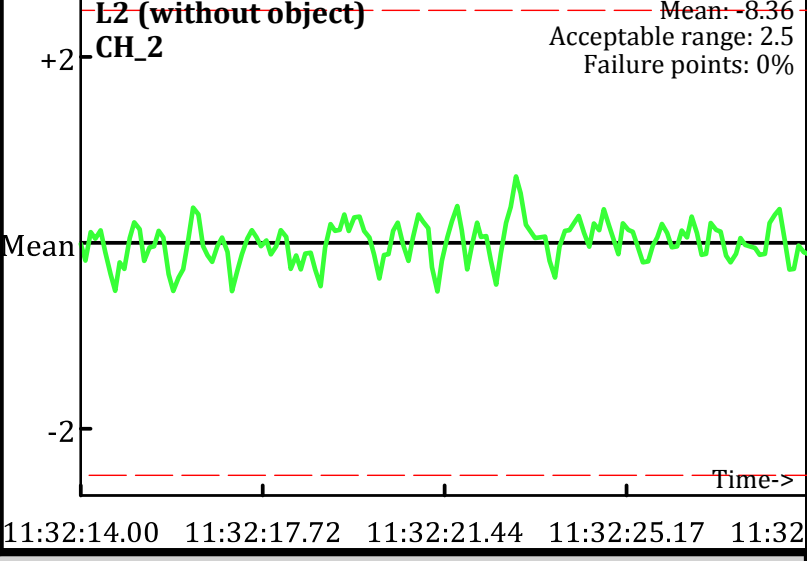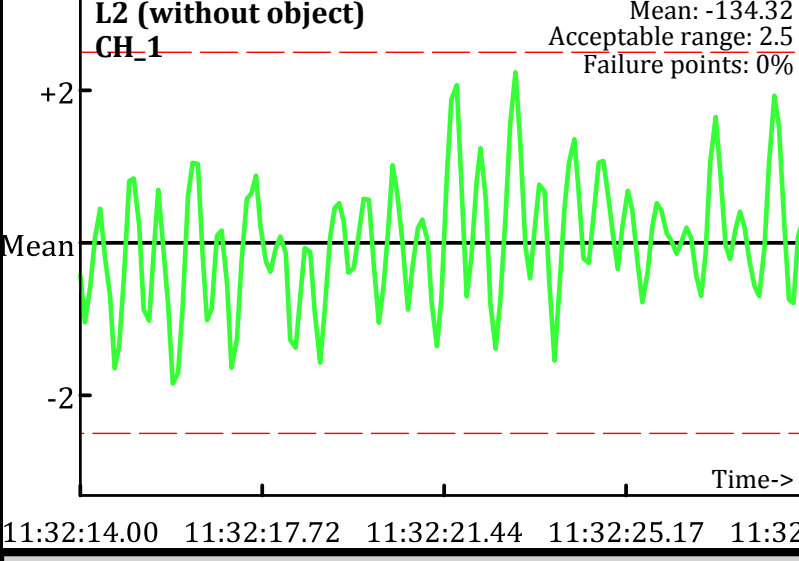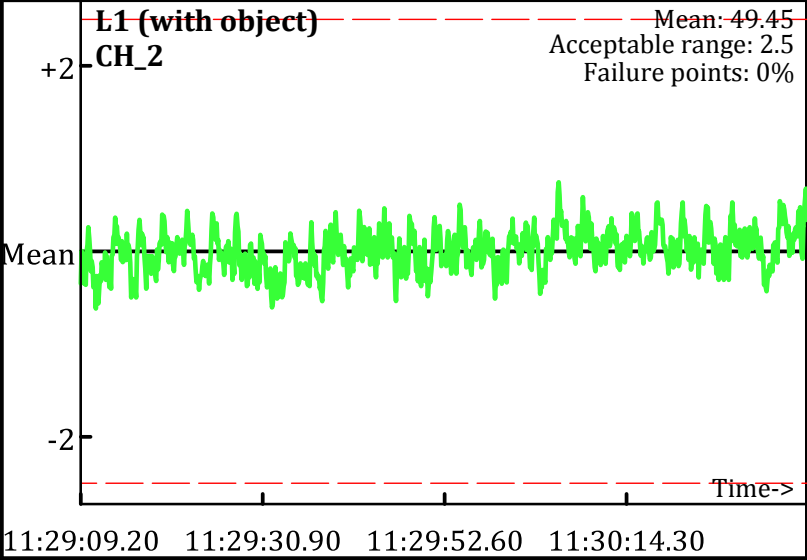– – – Acceptable limits

AM test
Operator: PN & BS
Date: 1/20/2010

L0 (without object)
CH_3
Mean: 4.55
Acceptable range: 2.5
Failure points: 0%

11:24:25.41　11:24:56.86　11:25:28.30　11:25:59.75

L0 (without object)
CH_4
Mean: -1.85
Acceptable range: 2.5
Failure points: 0%

11:24:25.41　11:24:56.86　11:25:28.30　11:25:59.75

L1 (with object)
CH_3
Mean: 34.64
Acceptable range: 2.5
Failure points: 0%

11:29:09.20　11:29:30.90　11:29:52.60　11:30:14.30

L1 (with object)
CH_4
Mean: 11.29
Acceptable range: 2.5
Failure points: 0%

11:29:09.20　11:29:30.90　11:29:52.60　11:30:14.30

L2 (without object)
CH_3
Mean: 4.69
Acceptable range: 2.5
Failure points: 0%

11:32:14.00　11:32:17.72　11:32:21.44　11:32:25.17　11:32

L2 (without object)
CH_4
Mean: -1.75
Acceptable range: 2.5
Failure points: 0%

11:32:14.00　11:32:17.72　11:32:21.44　11:32:25.17　11:32

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
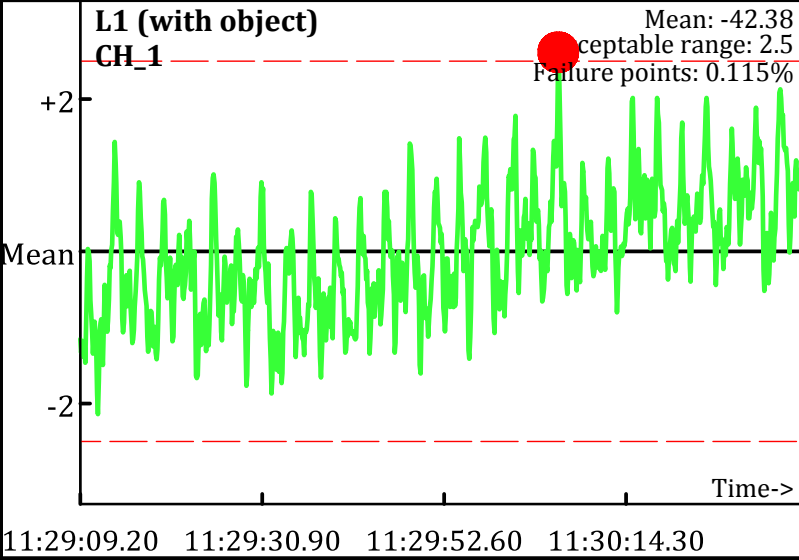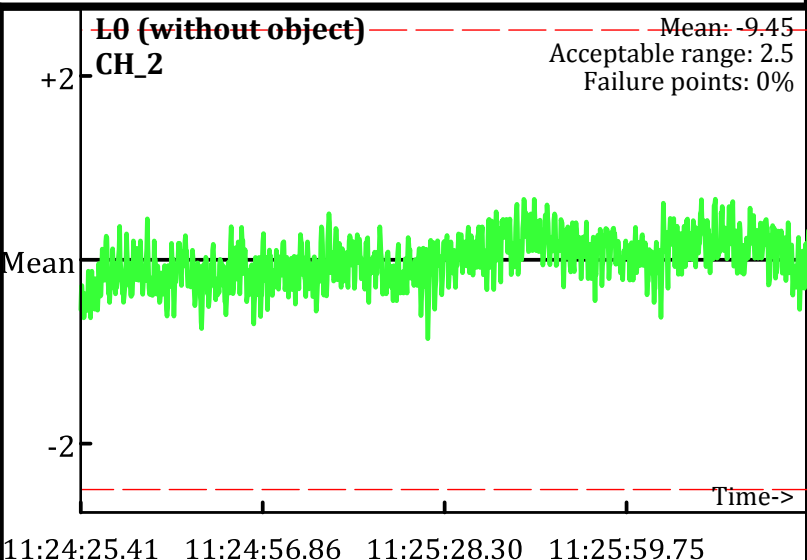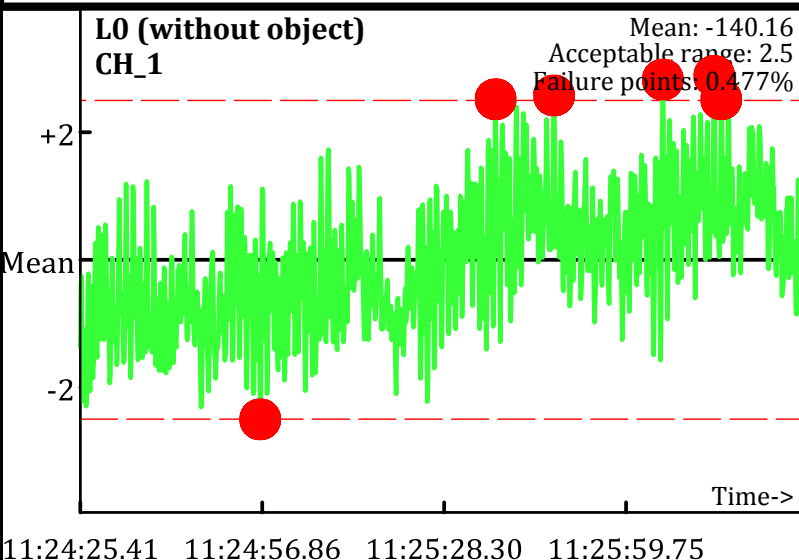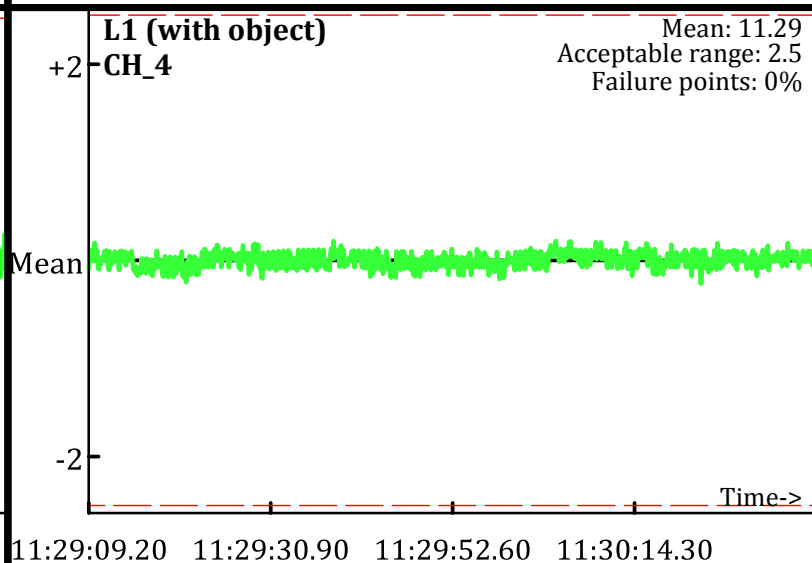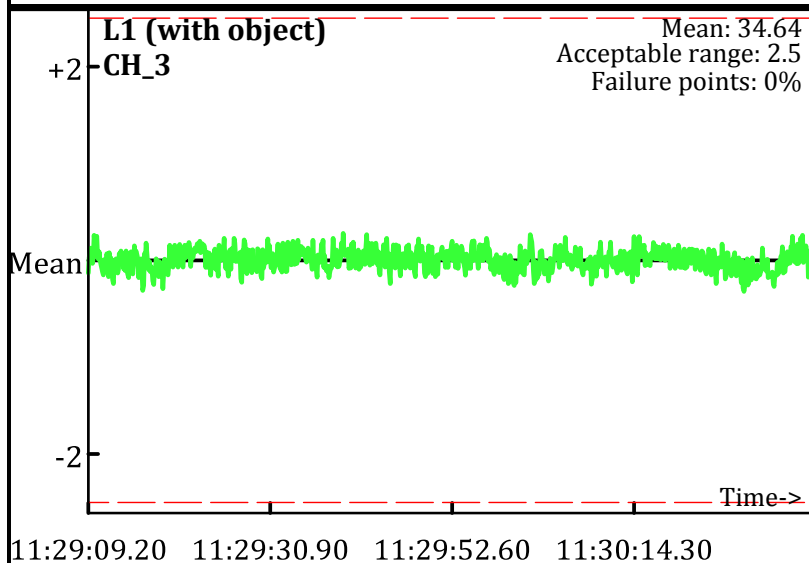-- Acceptable limits

AM test
Operator: PN & BS
Date: 1/20/2010

L0.1 (without object)
CH_1
Mean: -84.95
Acceptable range: 2.5
Failure points: 0.556%

L0.1 (without object)
CH_2
Mean: 5.01
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_1
Mean: 32.65
Acceptable range: 2.5
Failure points: 0%

L1.1 (with object)
CH_2
Mean: 92.63
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_1
Mean: -83.06
Acceptable range: 2.5
Failure points: 0%

L2.1 (without object)
CH_2
Mean: 5.14
Acceptable range: 2.5
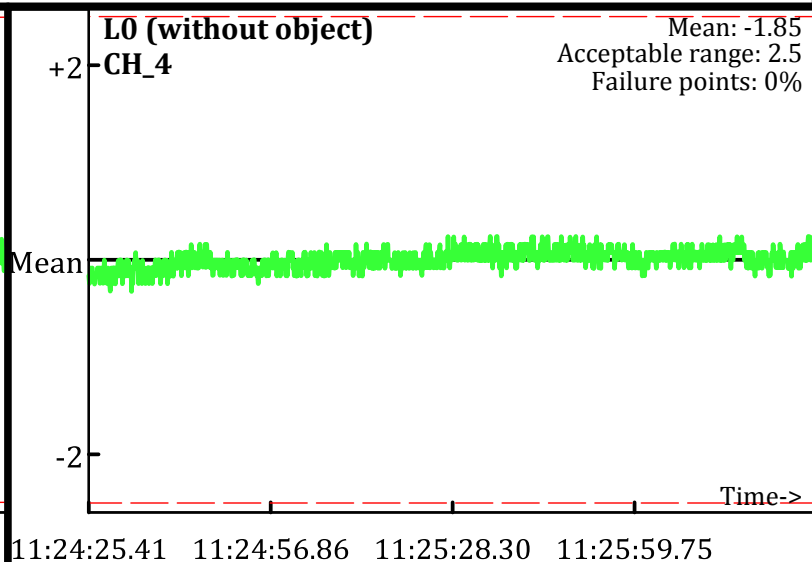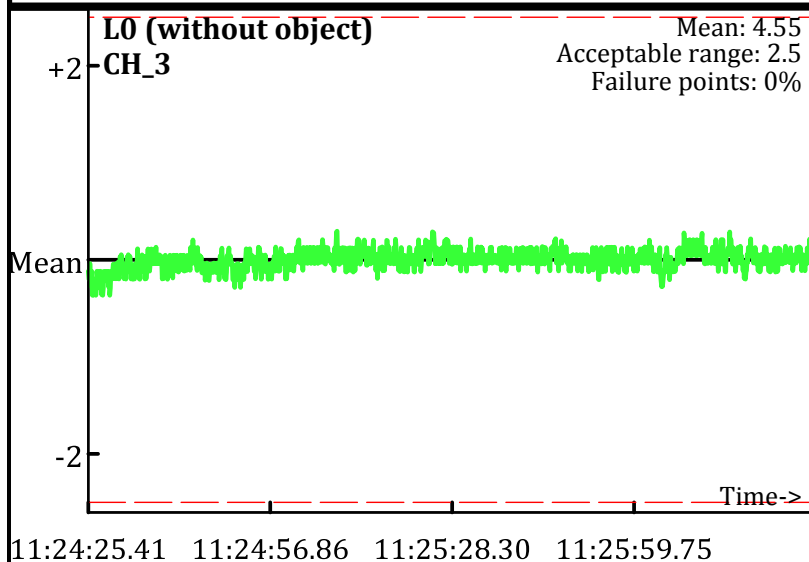Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
— — — Acceptable limits

AM test
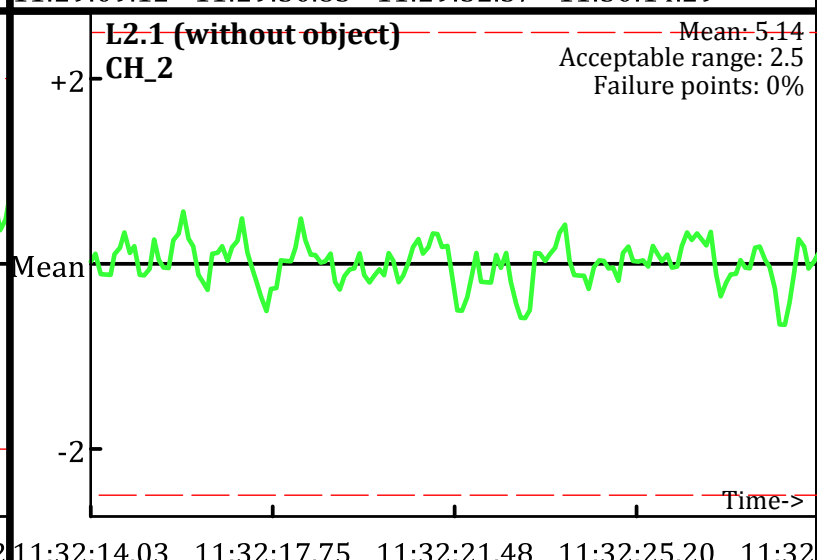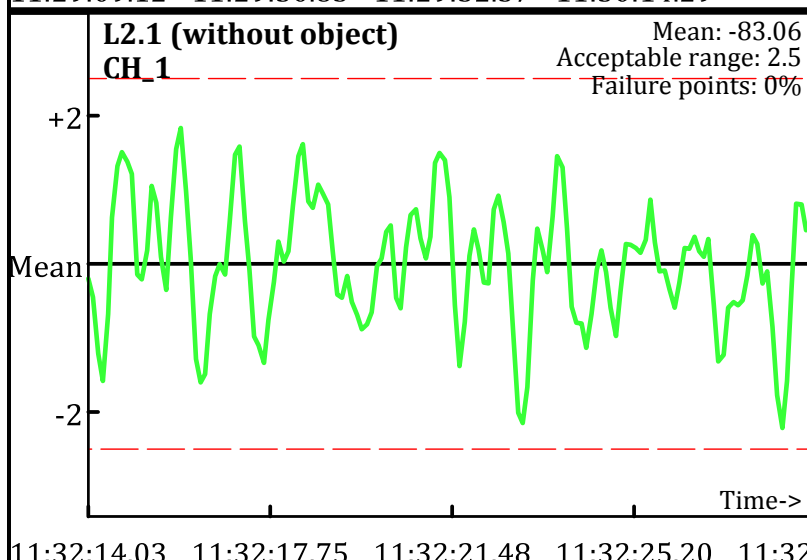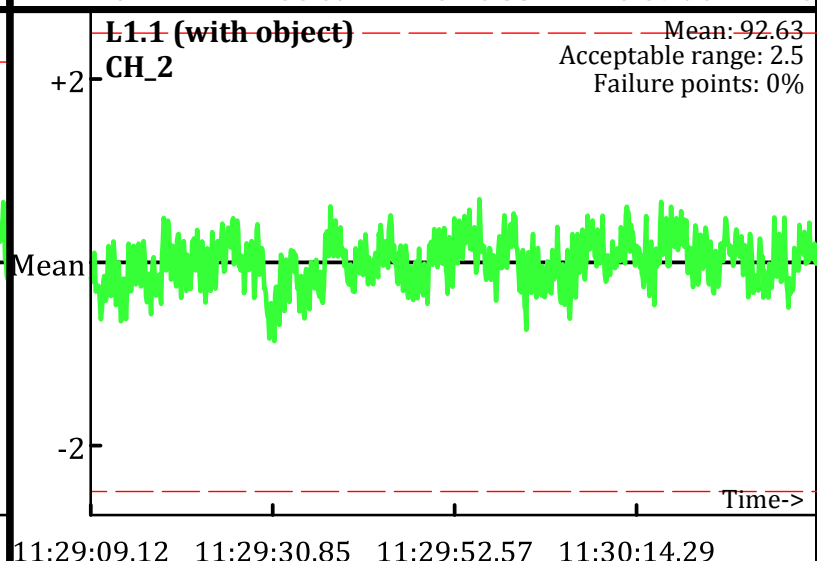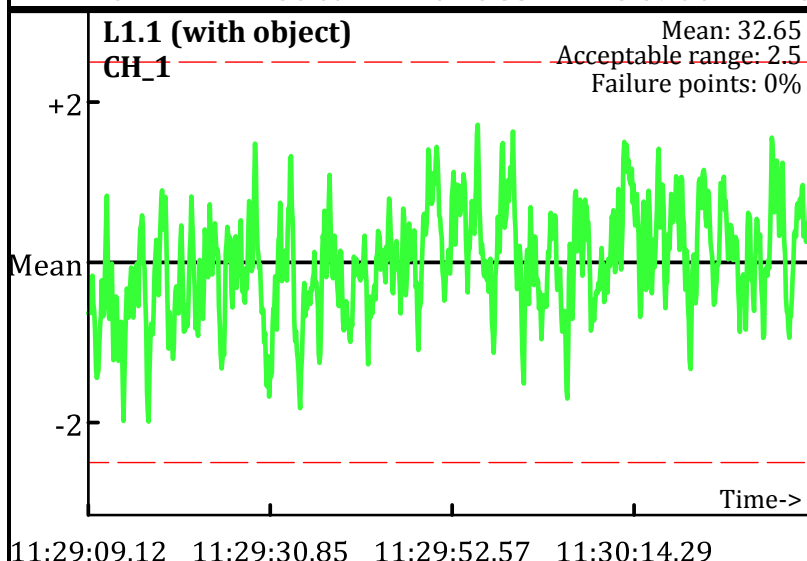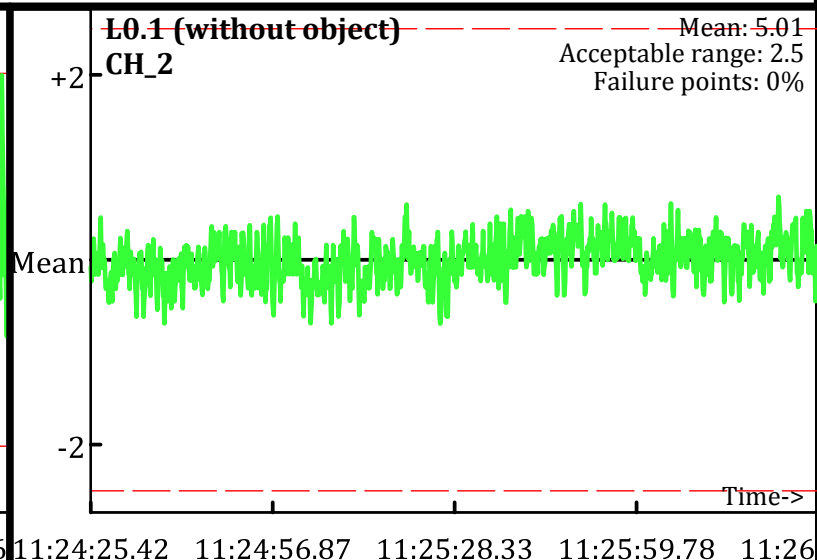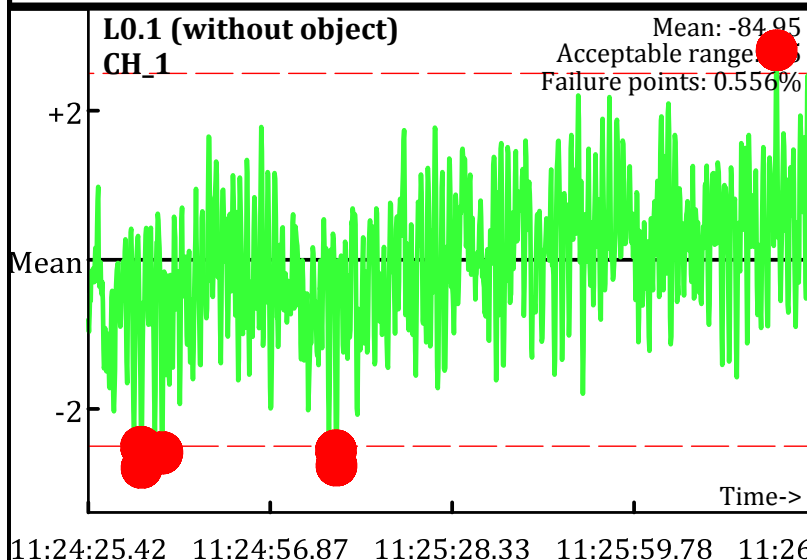Operator: PN & BS
Date: 1/20/2010

L0.1 (without object)
CH_3
Mean: 11.13
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:24:25.42   11:24:56.87   11:25:28.33   11:25:59.78   11:26

L0.1 (without object)
CH_4
Mean: 2.13
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:24:25.42   11:24:56.87   11:25:28.33   11:25:59.78   11:26

L1.1 (with object)
CH_3
Mean: 67.18
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:29:09.12   11:29:30.85   11:29:52.57   11:30:14.29

L1.1 (with object)
CH_4
Mean: 32.2
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:29:09.12   11:29:30.85   11:29:52.57   11:30:14.29

L2.1 (without object)
CH_3
Mean: 11.1
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:32:14.03   11:32:17.75   11:32:21.48   11:32:25.20   11:32

L2.1 (without object)
CH_4
Mean: 2.12
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->
11:32:14.03   11:32:17.75   11:32:21.48   11:32:25.20   11:32

Database: D:\Projects_QCReports_Ord_Data\012010\QC\012010_TA_QC.gdb
Line Name: L0.1 L1.1 L2.1

Page: 2

Static Calibration Test

L0.2 (without object)
CH_1
Mean: -65.46
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:24:25.45   11:24:56.90   11:25:28.35   11:25:59.80

L0.2 (without object)
CH_2
Mean: 2.85
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:24:25.45   11:24:56.90   11:25:28.35   11:25:59.80

L1.2 (with object)
CH_1
Mean: 24.52
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:29:09.16   11:29:30.86   11:29:52.55   11:30:14.25

L1.2 (with object)
CH_2
Mean: 57.83
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:29:09.16   11:29:30.86   11:29:52.55   11:30:14.25

L2.2 (without object)
CH_1
Mean: -63.86
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:32:13.95   11:32:17.68   11:32:21.41   11:32:25.13   11:32

L2.2 (without object)
CH_2
Mean: 2.87
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:32:13.95   11:32:17.68   11:32:21.41   11:32:25.13   11:32

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
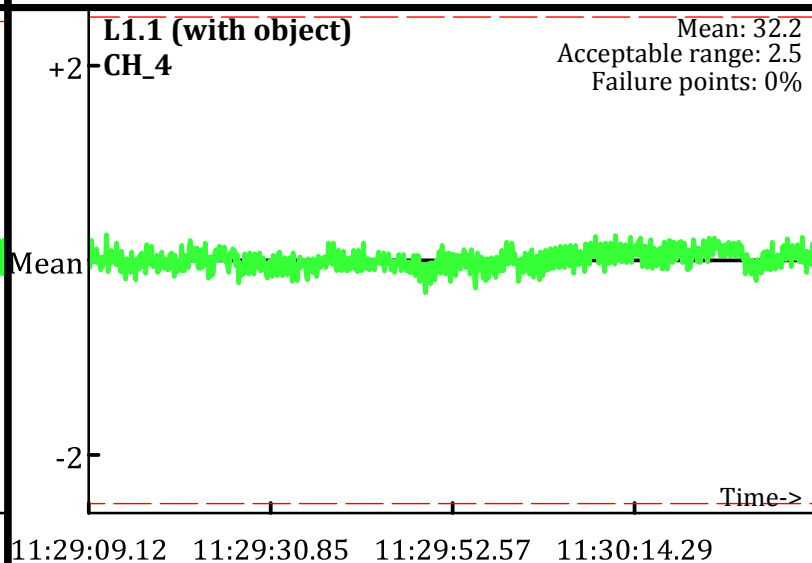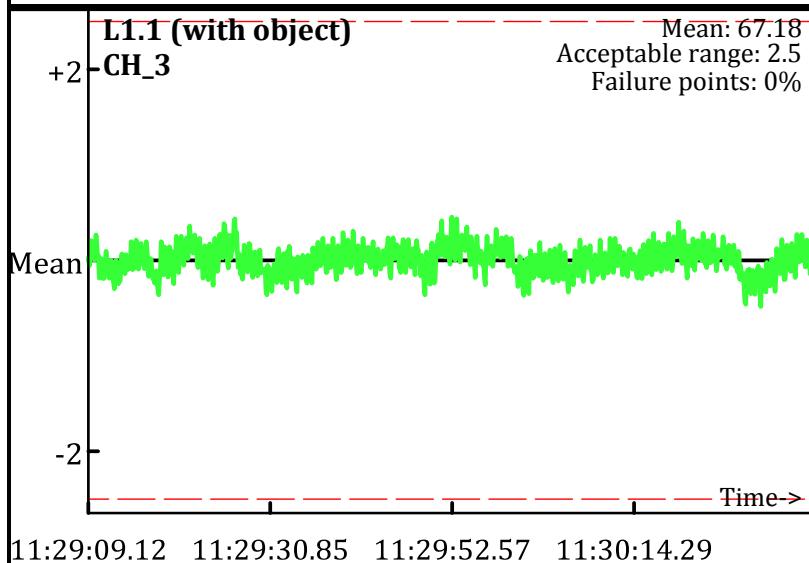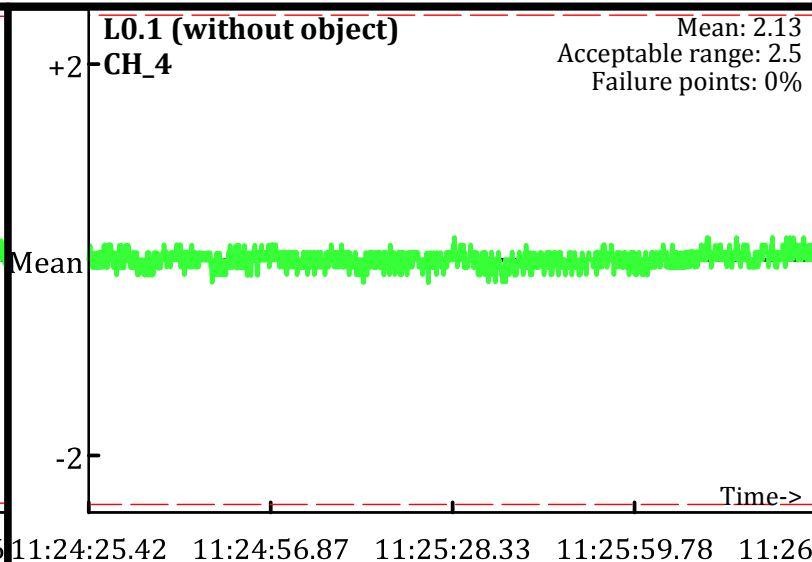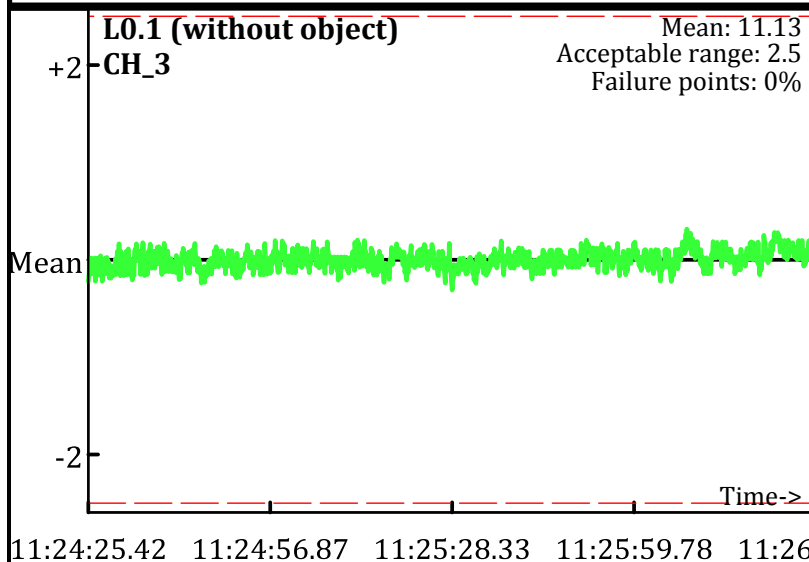Grid/Location: QC Area

● Outside range
- - - Acceptable limits
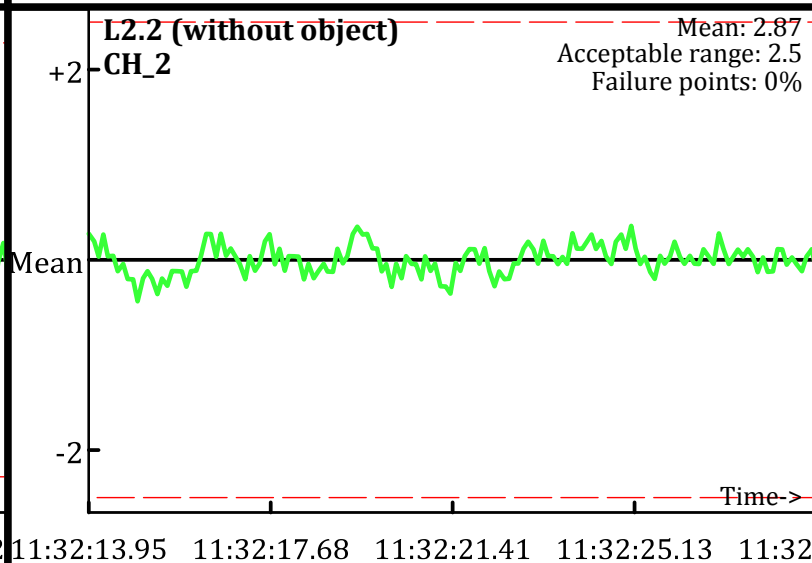
AM test
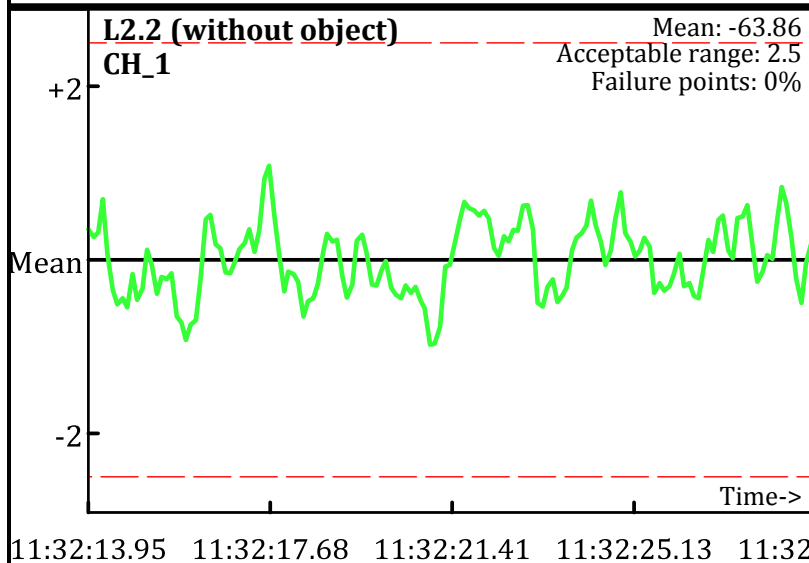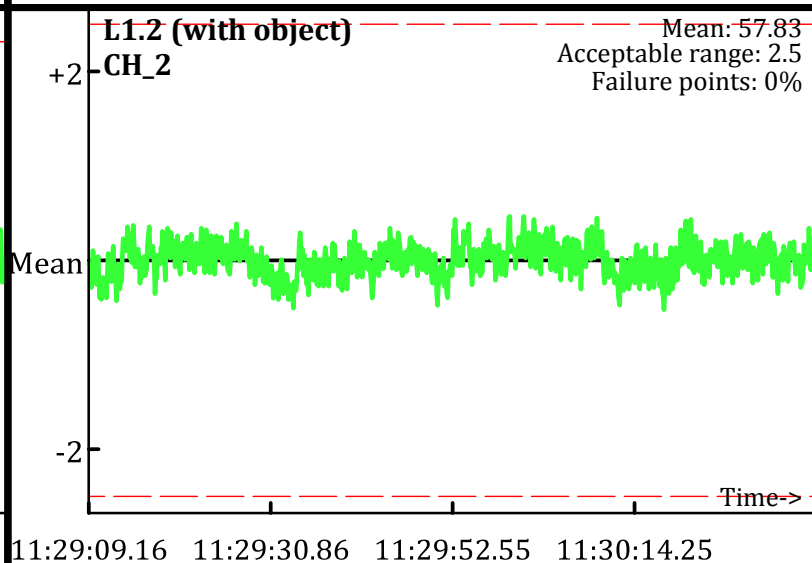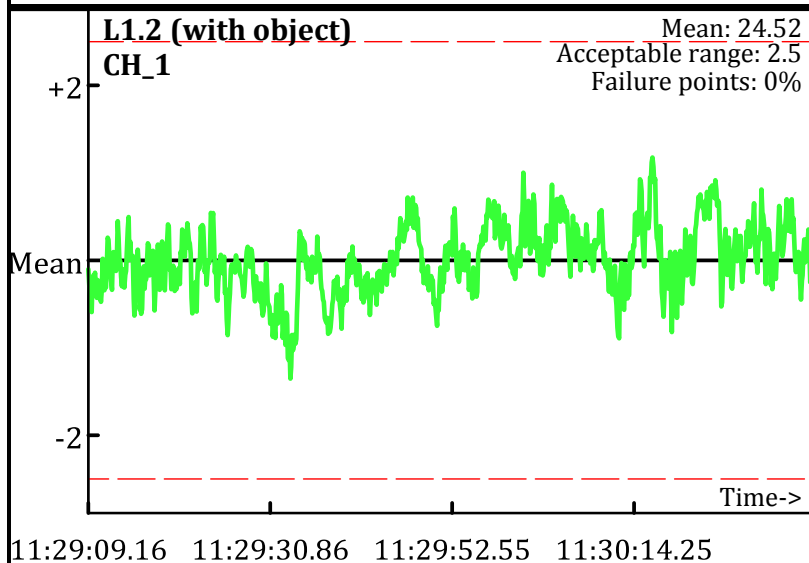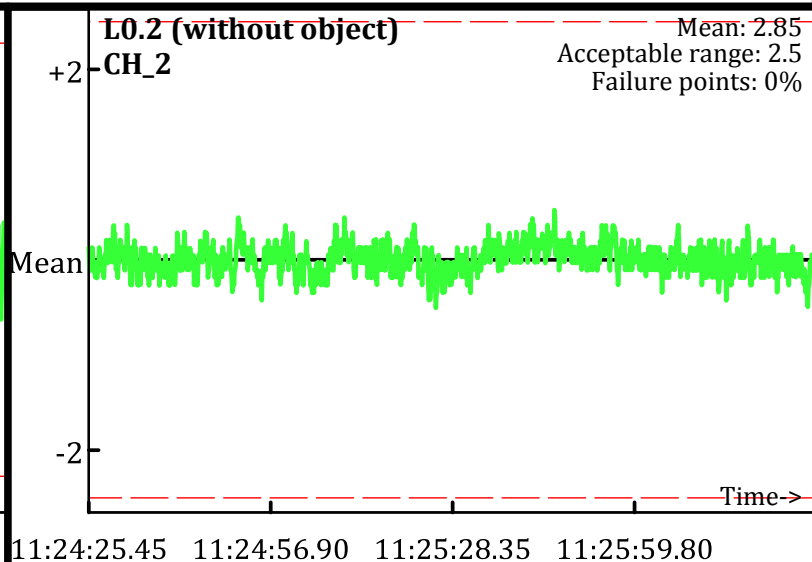Operator: PN & BS
Date: 1/20/2010

L0.2 (without object)
CH_3
Mean: 6.37
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:24:25.45   11:24:56.90   11:25:28.35   11:25:59.80

L0.2 (without object)
CH_4
Mean: -0.33
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:24:25.45   11:24:56.90   11:25:28.35   11:25:59.80

L1.2 (with object)
CH_3
Mean: 35.17
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:29:09.16   11:29:30.86   11:29:52.55   11:30:14.25

L1.2 (with object)
CH_4
Mean: 12.26
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:29:09.16   11:29:30.86   11:29:52.55   11:30:14.25

L2.2 (without object)
CH_3
Mean: 6.3
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:32:13.95   11:32:17.68   11:32:21.41   11:32:25.13   11:32

L2.2 (without object)
CH_4
Mean: -0.4
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

11:32:13.95   11:32:17.68   11:32:21.41   11:32:25.13   11:32

Database: D:\Projects_QCReports_Ord_Data\012010\QC\012010_TA_QC.gdb
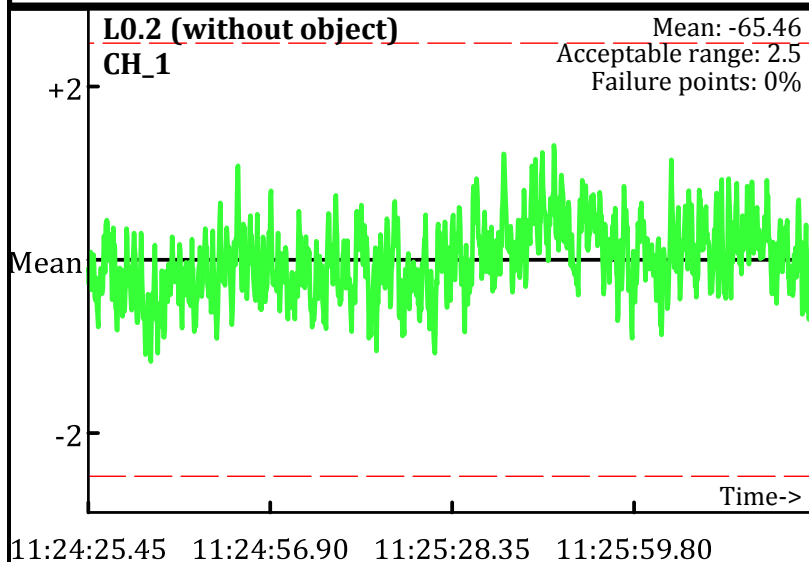Line Name: L0.2 L1.2 L2.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits

PM test
Operator: PN & BS
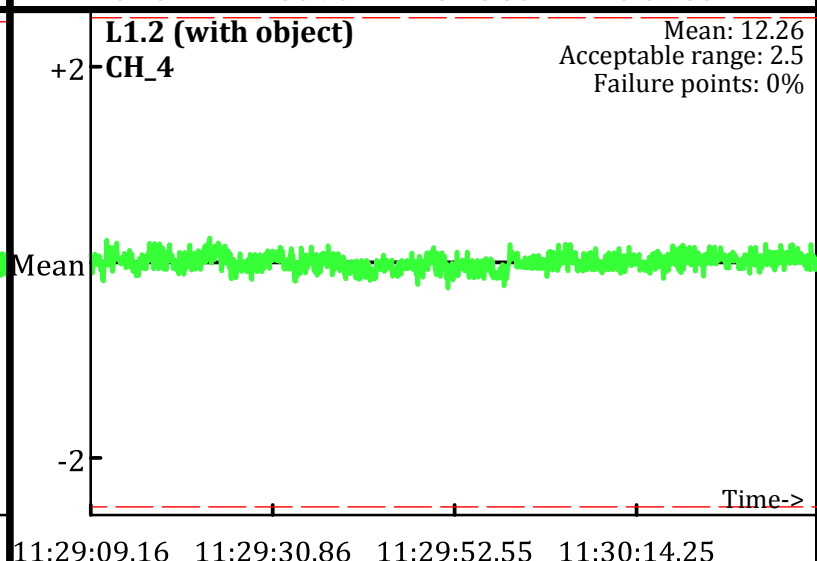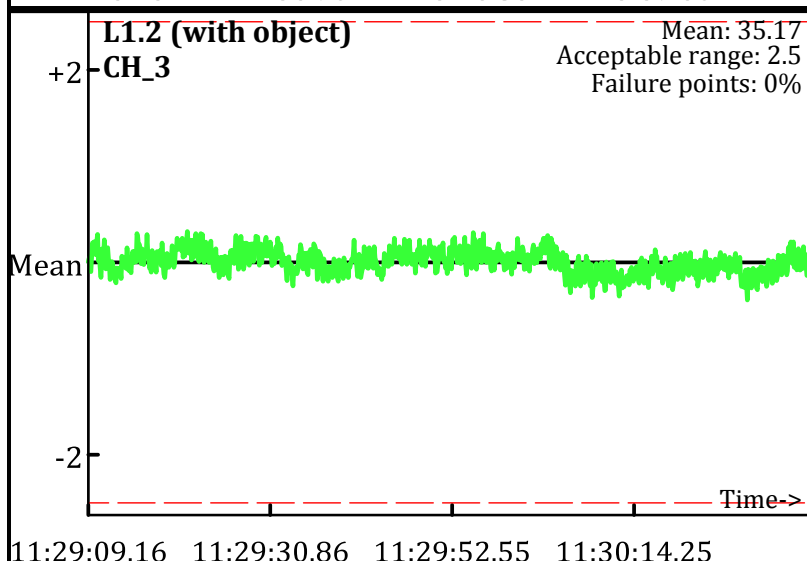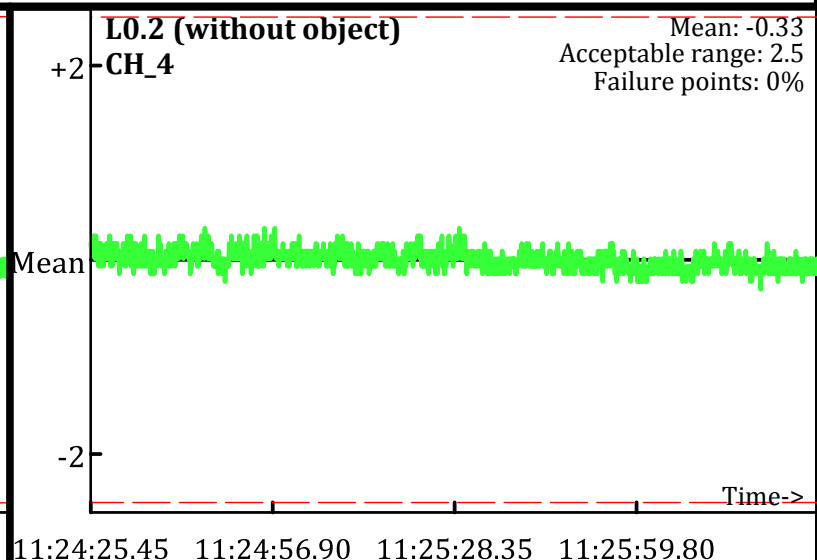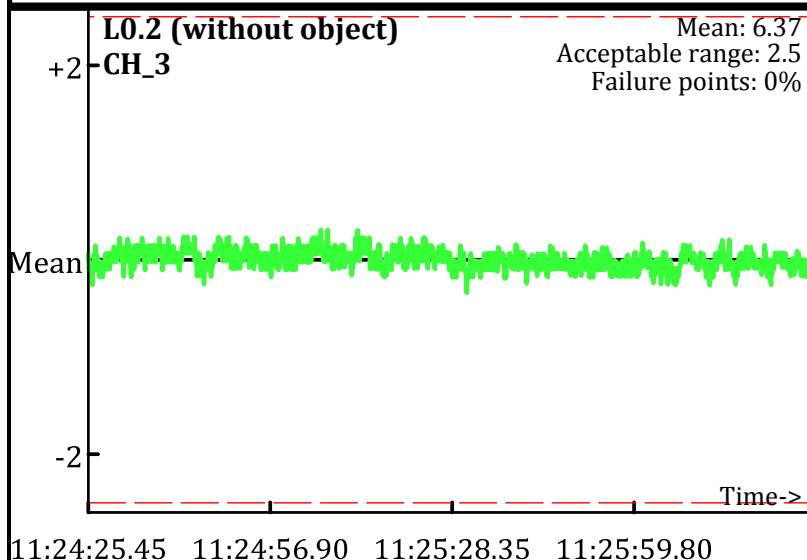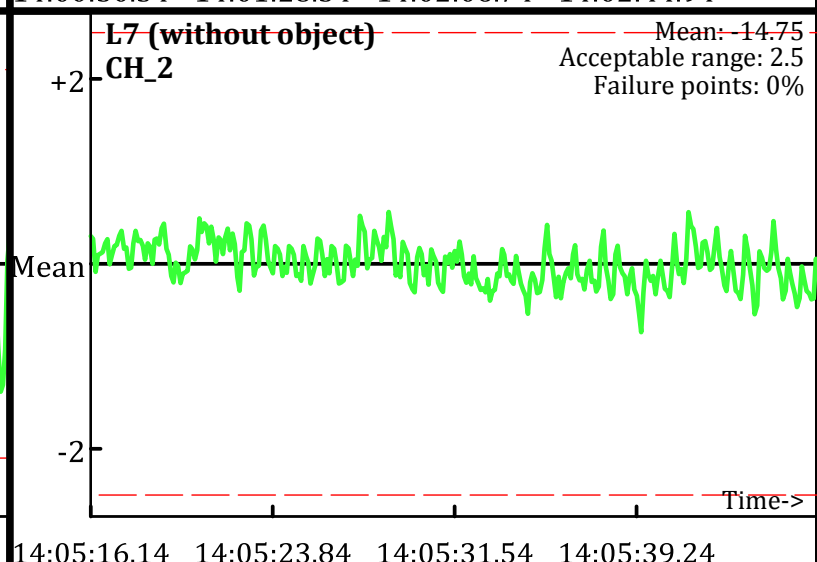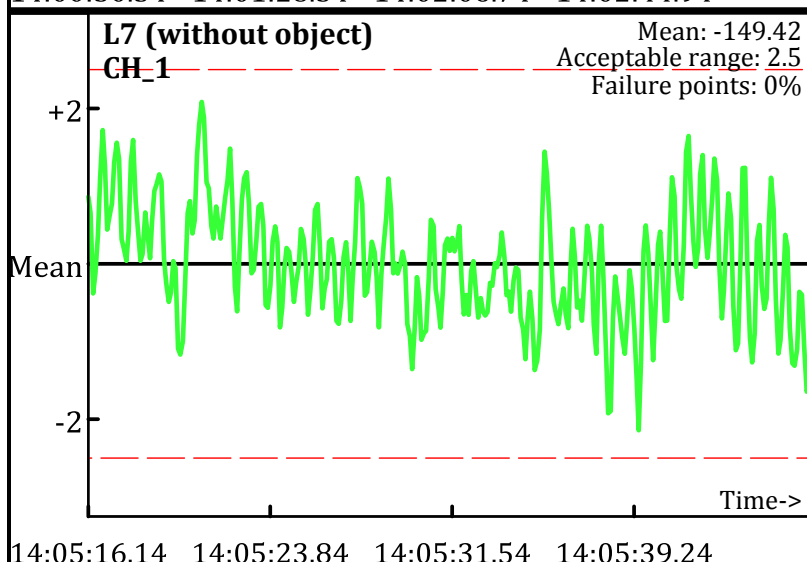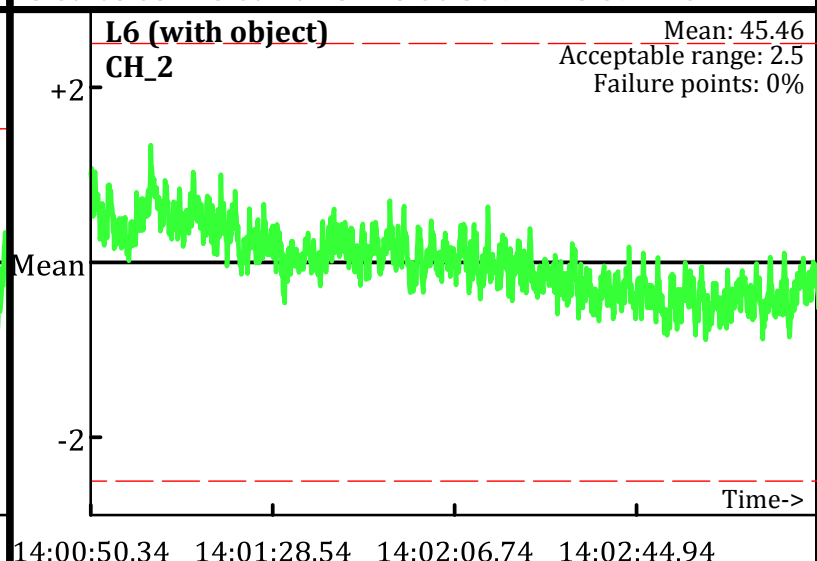**Date:** 1/20/2010

L5 (without object) CH_1
Mean: -148.59
Acceptable range: 2.5
Failure points: 39.5%
13:57:03.53   13:57:47.23   13:58:30.94   13:59:14.64

L5 (without object) CH_2
Mean: -15.28
Acceptable range: 2.5
Failure points: 5.03%
13:57:03.53   13:57:47.23   13:58:30.94   13:59:14.64

L6 (with object) CH_1
Mean: -52.26
Acceptable range: 2.5
Failure points: 4.05%
14:00:50.34   14:01:28.54   14:02:06.74   14:02:44.94

L6 (with object) CH_2
Mean: 45.46
Acceptable range: 2.5
Failure points: 0%
14:00:50.34   14:01:28.54   14:02:06.74   14:02:44.94

L7 (without object) CH_1
Mean: -149.42
Acceptable range: 2.5
Failure points: 0%
14:05:16.14   14:05:23.84   14:05:31.54   14:05:39.24

L7 (without object) CH_2
Mean: -14.75
Acceptable range: 2.5
Failure points: 0%
14:05:16.14   14:05:23.84   14:05:31.54   14:05:39.24

Database: D:\Projects_QCReports_Ord_Data\012010\QC\012010_TA_QC.gdb
Line Name: L5 L6 L7

Page: 1

Static Calibration Test

L5 (without object)
CH_3
Mean: 2.49
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:57:03.53   13:57:47.23   13:58:30.94   13:59:14.64

L5 (without object)
CH_4
Mean: -2.58
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

13:57:03.53   13:57:47.23   13:58:30.94   13:59:14.64

L6 (with object)
CH_3
Mean: 33.88
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:00:50.34   14:01:28.54   14:02:06.74   14:02:44.94

L6 (with object)
CH_4
Mean: 11
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:00:50.34   14:01:28.54   14:02:06.74   14:02:44.94

L7 (without object)
CH_3
Mean: 2.83
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:05:16.14   14:05:23.84   14:05:31.54   14:05:39.24

L7 (without object)
CH_4
Mean: -2.46
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

14:05:16.14   14:05:23.84   14:05:31.54   14:05:39.24

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
- - - Acceptable limits
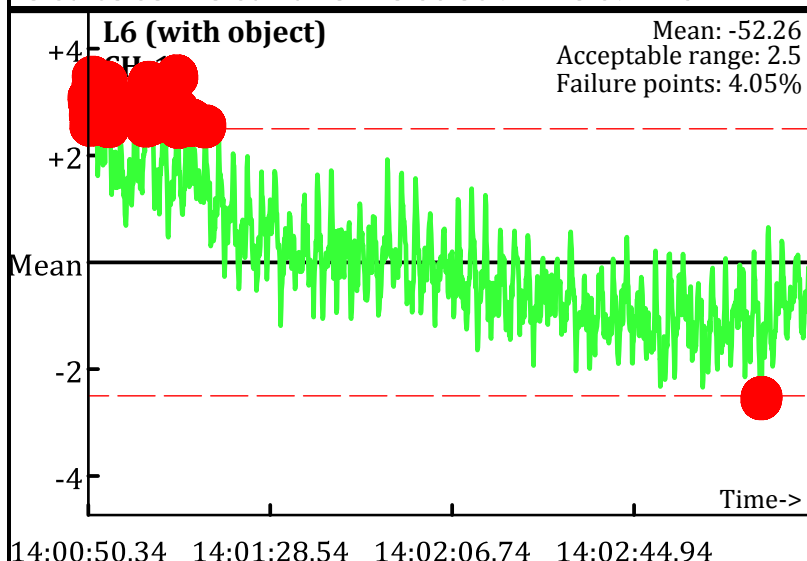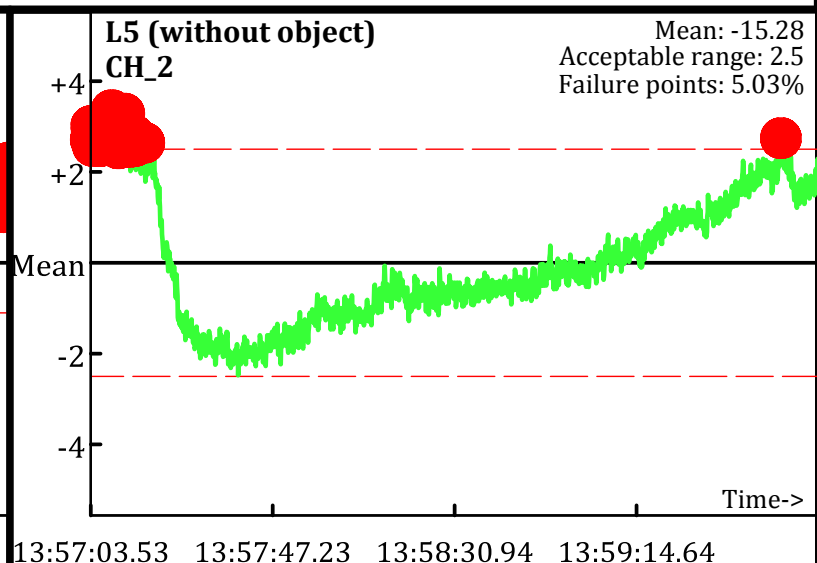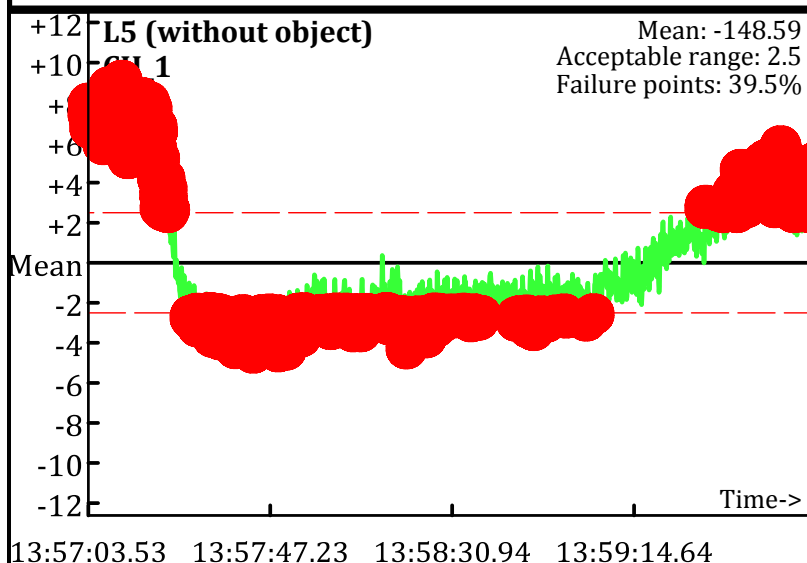
PM test
Operator: PN & BS
Date: 1/20/2010
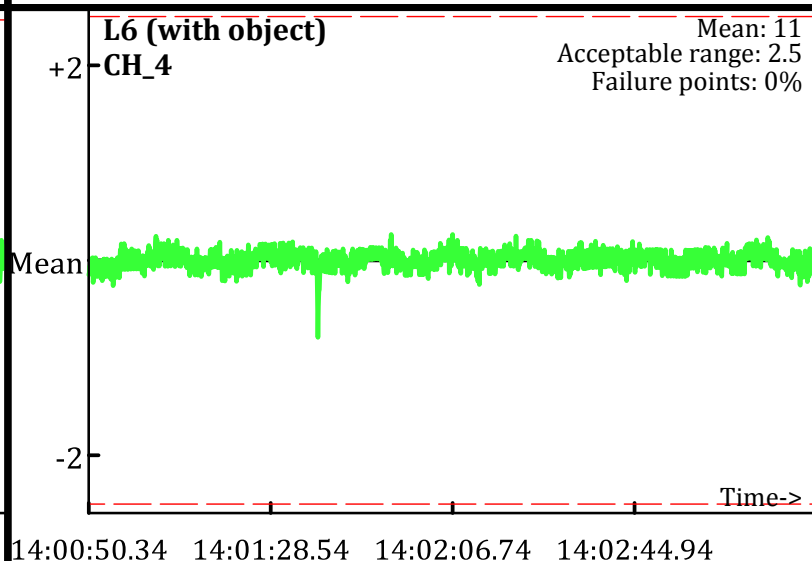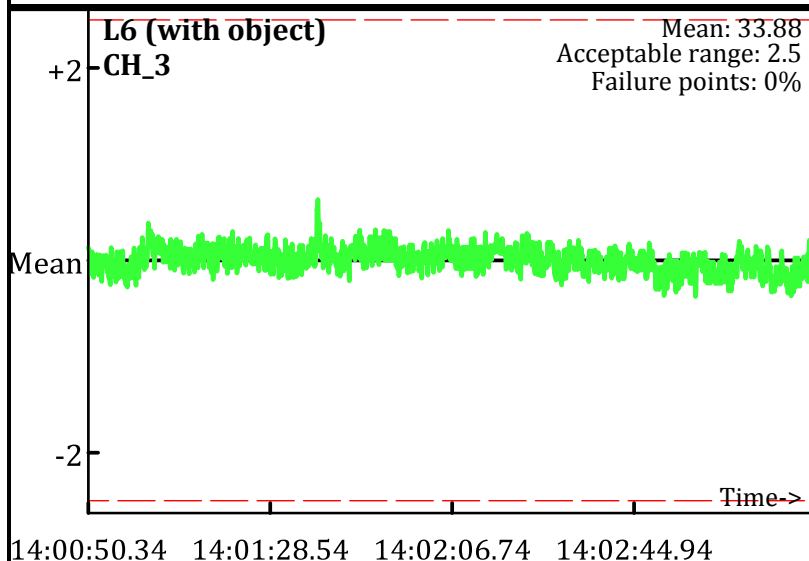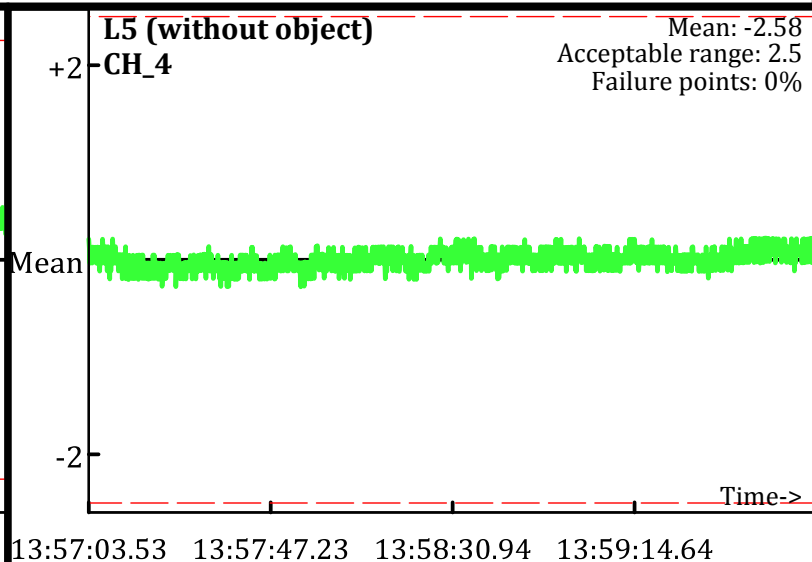
L5.1 (without object)
CH_1
Mean: -88.04
Acceptable range: 2.5
Failure points: 42.5%

L5.1 (without object)
CH_2
Mean: 1.65
Acceptable range: 2.5
Failure points: 7.49%

L6.1 (with object)
CH_1
Mean: 24.21
Acceptable range: 2.5
Failure points: 1.18%

L6.1 (with object)
CH_2
Mean: 88.67
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_1
Mean: -93.12
Acceptable range: 2.5
Failure points: 0%

L7.1 (without object)
CH_2
Mean: -0.046
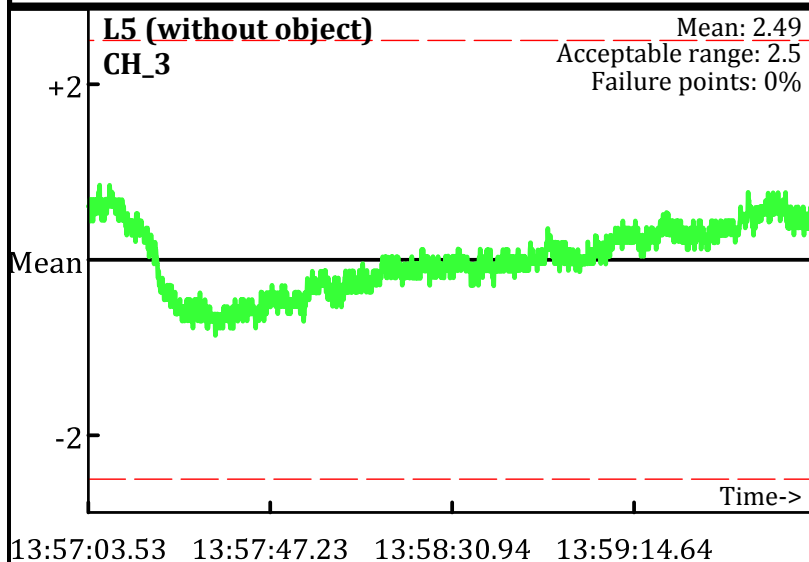Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
– – – Acceptable limits

PM test
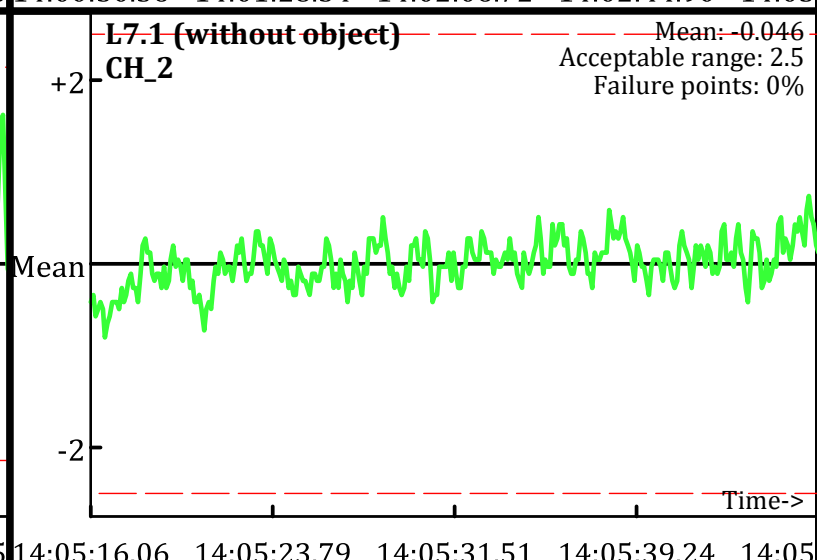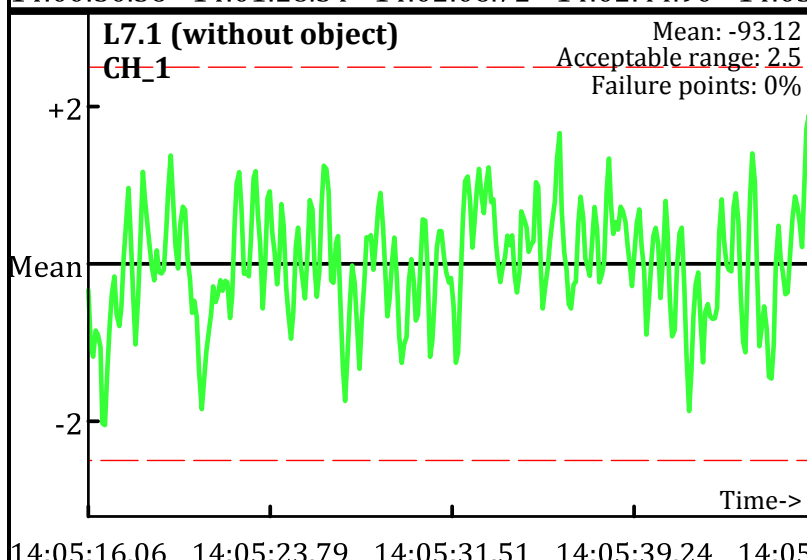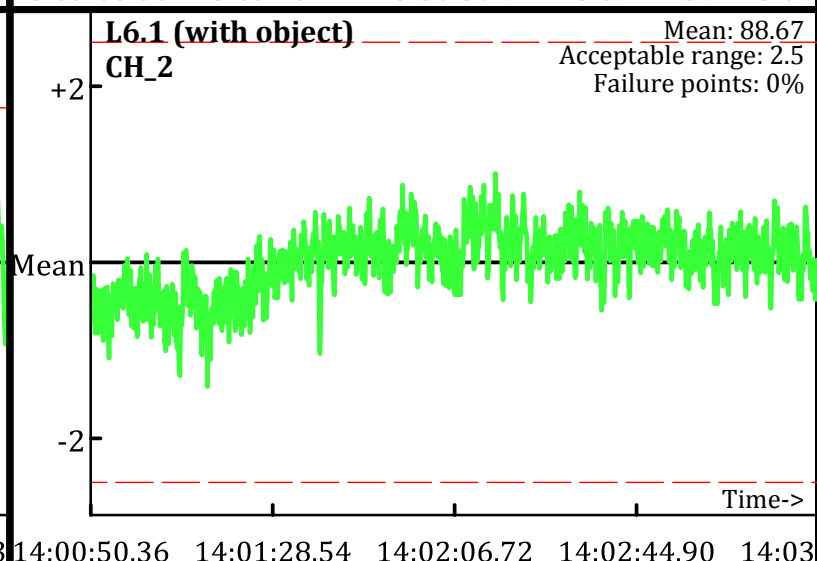Operator: PN & BS
Date: 1/20/2010

L5.1 (without object)
CH_3
Mean: 9.64
Acceptable range: 2.5
Failure points: 0%

Time->

13:57:03.56   13:57:47.24   13:58:30.91   13:59:14.59   13:59

L5.1 (without object)
CH_4
Mean: 1.6
Acceptable range: 2.5
Failure points: 0%

Time->

13:57:03.56   13:57:47.24   13:58:30.91   13:59:14.59   13:59

L6.1 (with object)
CH_3
Mean: 66.31
Acceptable range: 2.5
Failure points: 0%

Time->

14:00:50.36   14:01:28.54   14:02:06.72   14:02:44.90   14:03

L6.1 (with object)
CH_4
Mean: 32.18
Acceptable range: 2.5
Failure points: 0%

Time->

14:00:50.36   14:01:28.54   14:02:06.72   14:02:44.90   14:03

L7.1 (without object)
CH_3
Mean: 9.24
Acceptable range: 2.5
Failure points: 0%

Time->

14:05:16.06   14:05:23.79   14:05:31.51   14:05:39.24   14:05

L7.1 (without object)
CH_4
Mean: 1.49
Acceptable range: 2.5
Failure points: 0%

Time->

14:05:16.06   14:05:23.79   14:05:31.51   14:05:39.24   14:05

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits
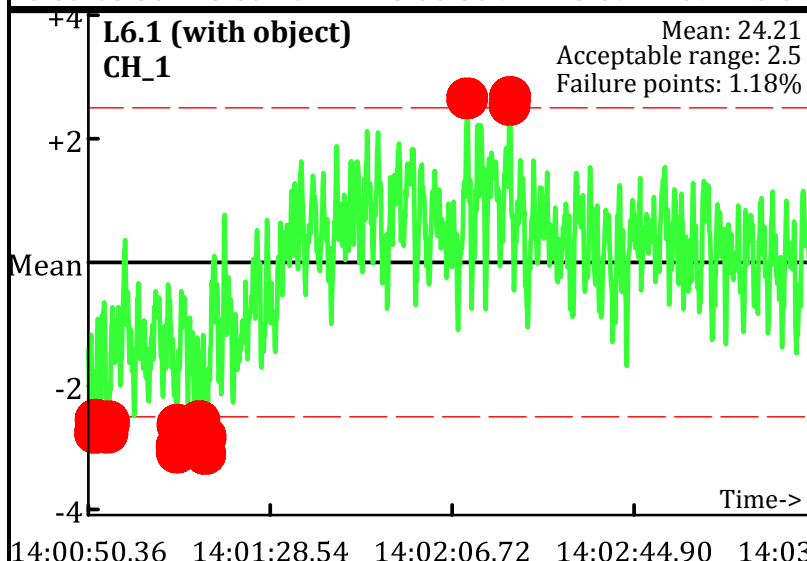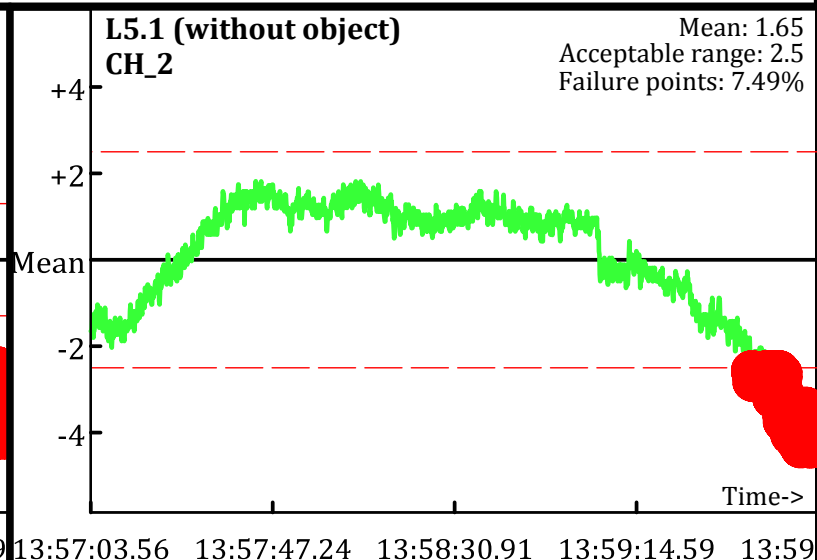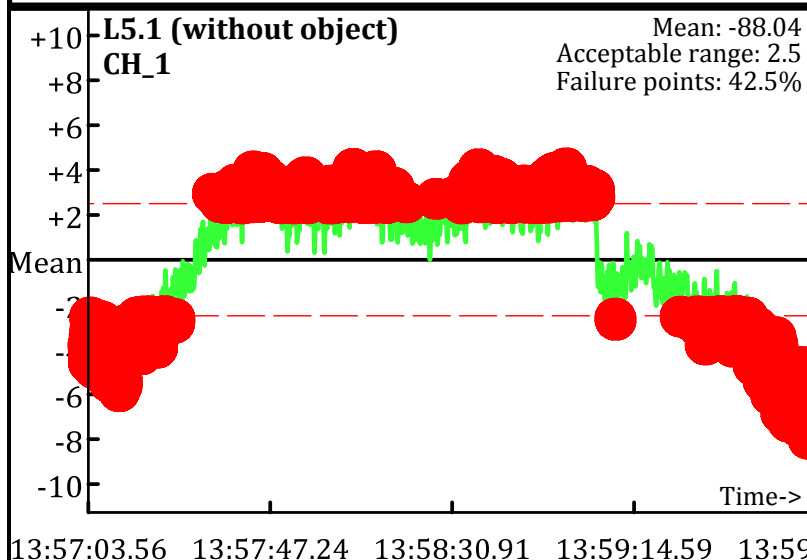
PM test
Operator: PN & BS
Date: 1/20/2010
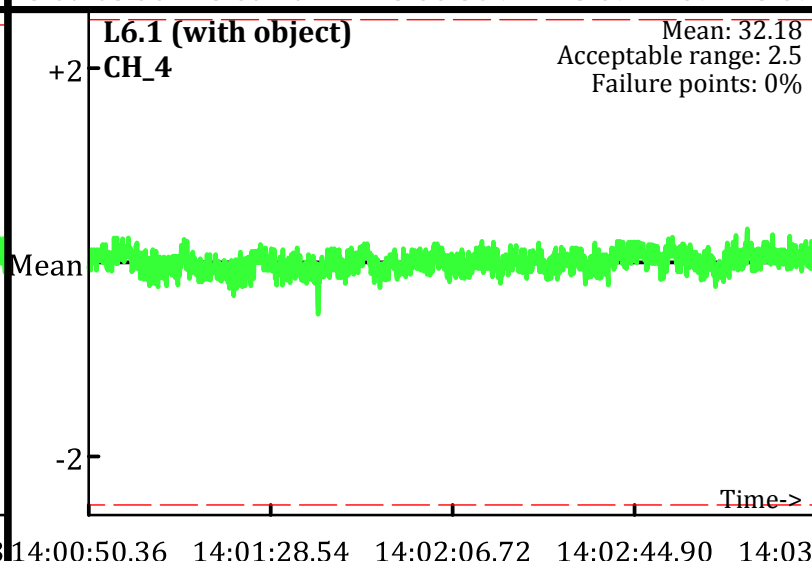

L5.2 (without object)
CH_1
Mean: -69.09
Acceptable range: 2.5
Failure points: 56.8%

L5.2 (without object)
CH_2
Mean: 1.17
Acceptable range: 2.5
Failure points: 6.41%

L6.2 (with object)
CH_1
Mean: 8.91
Acceptable range: 2.5
Failure points: 0.719%

L6.2 (with object)
CH_2
Mean: 52.36
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_1
Mean: -81.24
Acceptable range: 2.5
Failure points: 0%

L7.2 (without object)
CH_2
Mean: -2.96
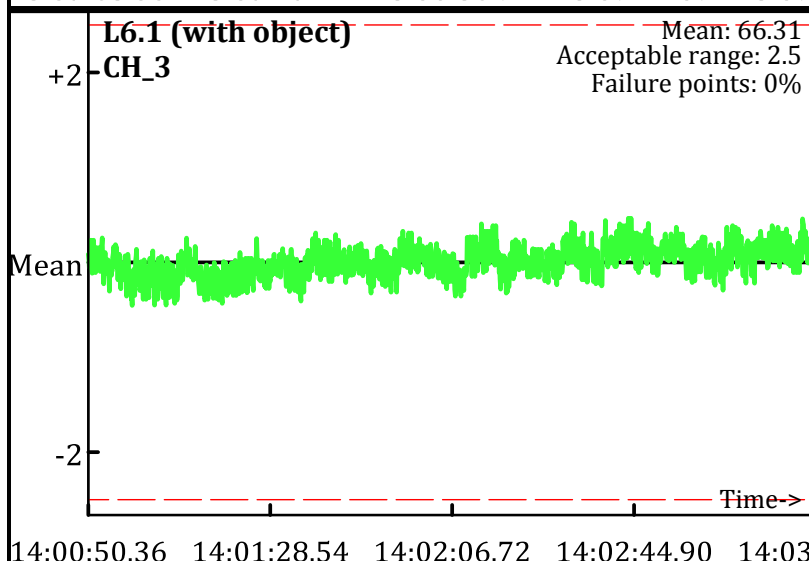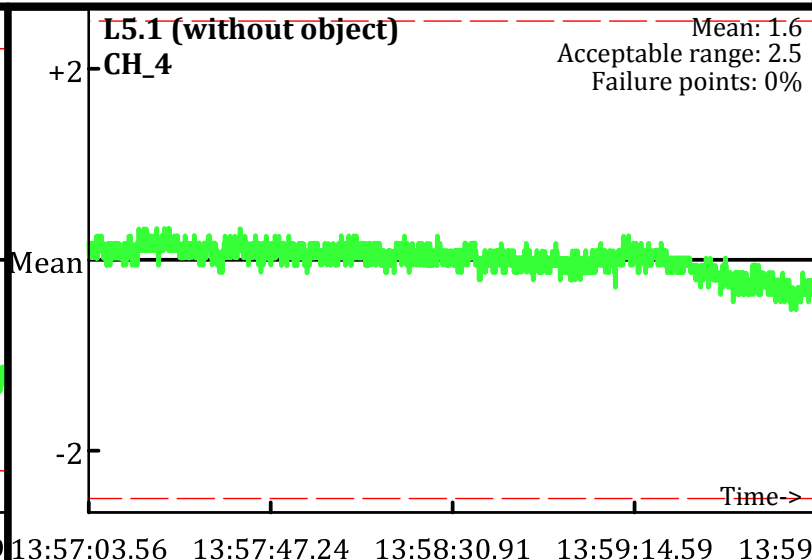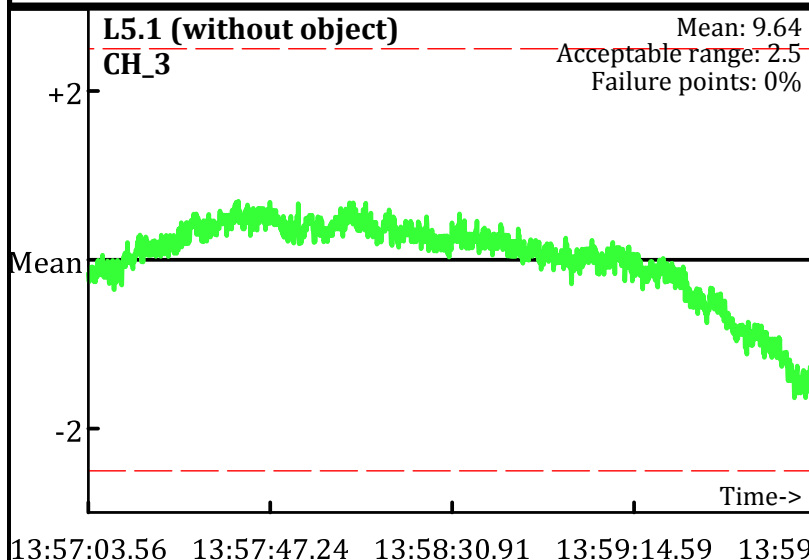Acceptable range: 2.5
Failure points: 0%

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

● Outside range
--- Acceptable limits

PM test
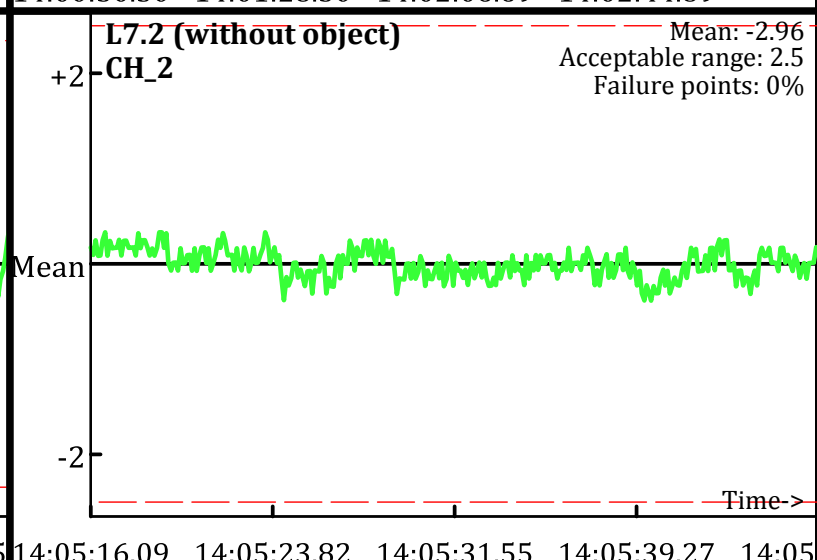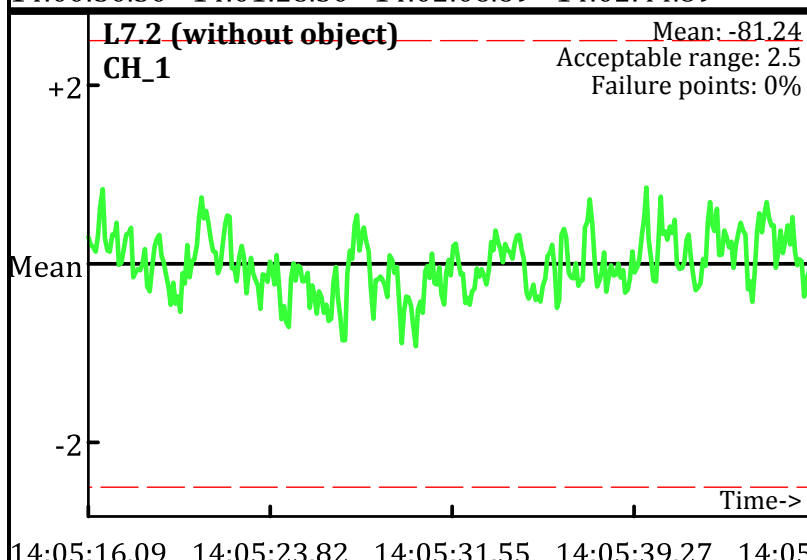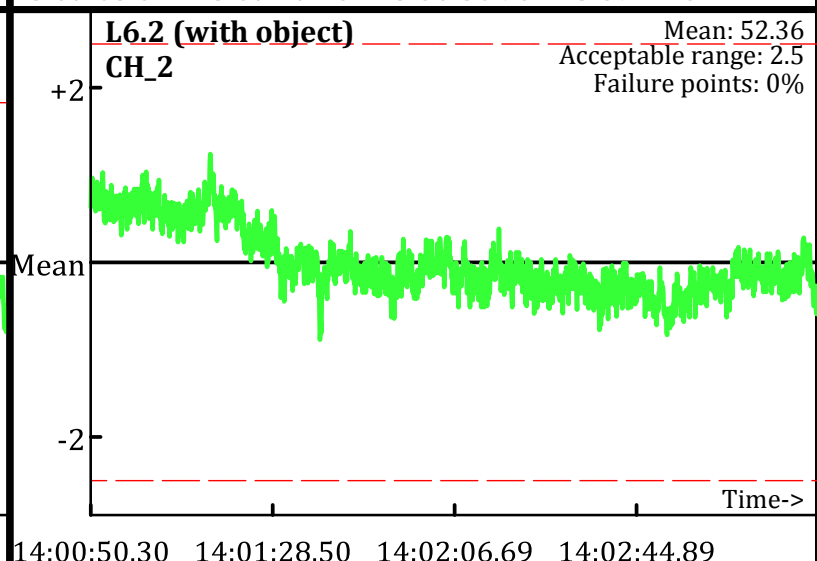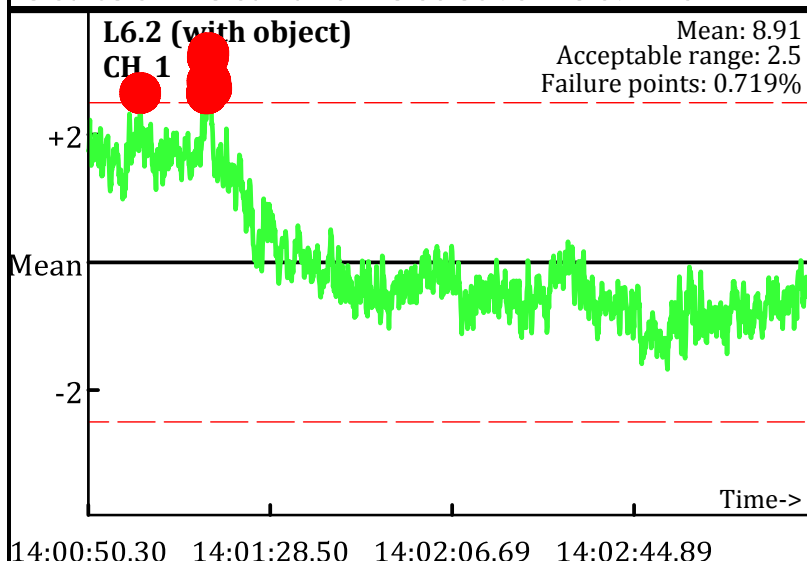Operator: PN & BS
Date: 1/20/2010

L5.2 (without object)
CH_3

Mean: 6.51
Acceptable range: 2.5
Failure points: 0%

13:57:03.61   13:57:47.28   13:58:30.95   13:59:14.62

L5.2 (without object)
CH_4

Mean: 0.087
Acceptable range: 2.5
Failure points: 0%

13:57:03.61   13:57:47.28   13:58:30.95   13:59:14.62

L6.2 (with object)
CH_3

Mean: 34.29
Acceptable range: 2.5
Failure points: 0%

14:00:50.30   14:01:28.50   14:02:06.69   14:02:44.89

L6.2 (with object)
CH_4

Mean: 12.34
Acceptable range: 2.5
Failure points: 0%

14:00:50.30   14:01:28.50   14:02:06.69   14:02:44.89

L7.2 (without object)
CH_3

Mean: 5.61
Acceptable range: 2.5
Failure points: 0%

14:05:16.09   14:05:23.82   14:05:31.55   14:05:39.27   14:05

L7.2 (without object)
CH_4

Mean: -0.05
Acceptable range: 2.5
Failure points: 0%

14:05:16.09   14:05:23.82   14:05:31.55   14:05:39.27   14:05

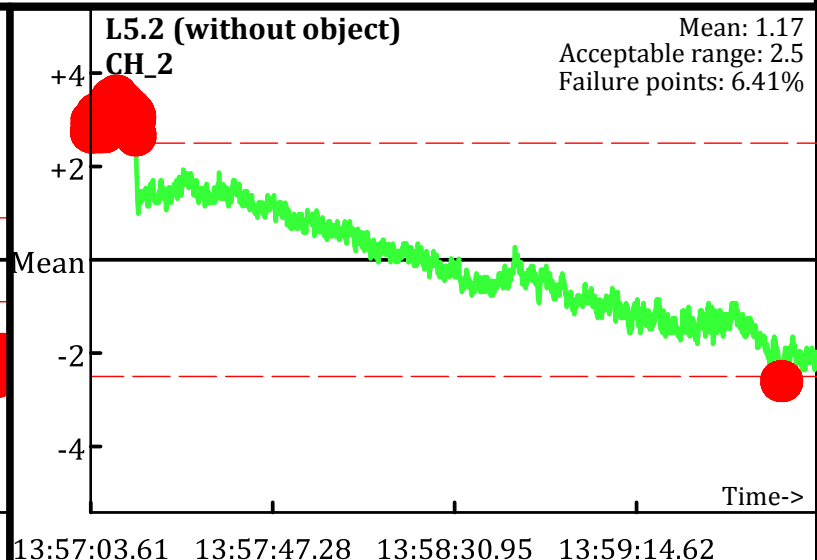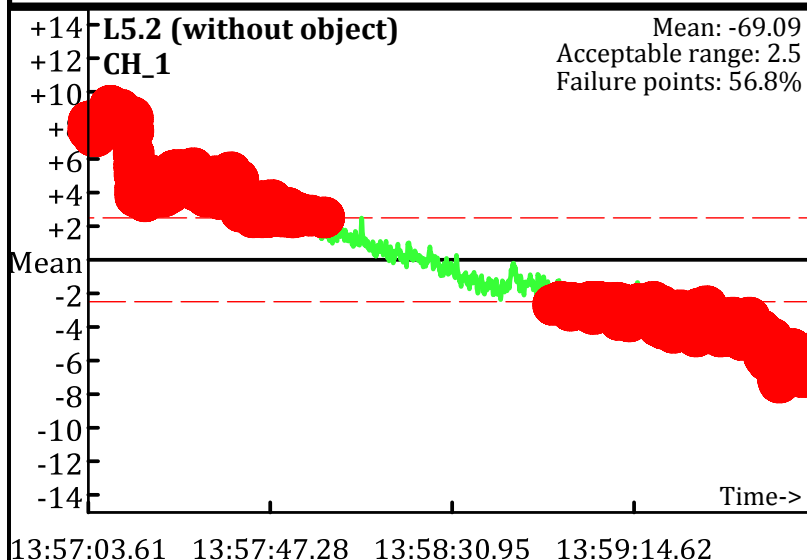Database: D:\Projects_QCReports_Ord_Data\012010\QC\012010_TA_QC.gdb
Line Name: L5.2 L6.2 L7.2

Page: 2

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
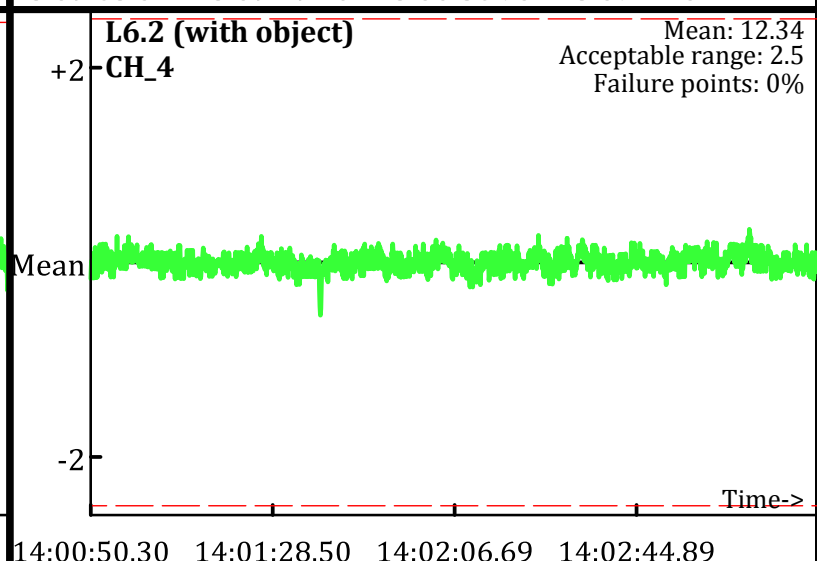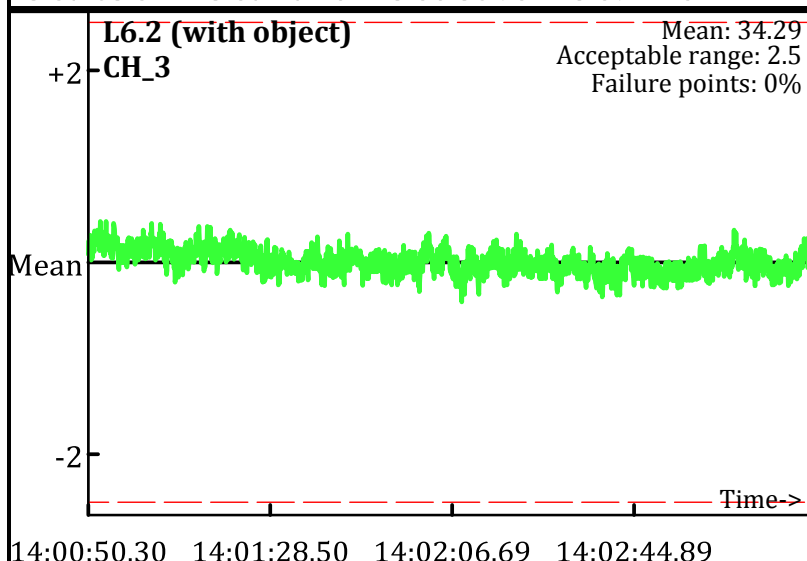Grid/Location: QC Area

● Outside range
– – – Acceptable limits

AM test
Operator: PN & MG
Date: 1/22/2010

L0 (without object)
CH_1
Mean: -150.35
Acceptable range: 2.5
Failure points: 4.87%

+4
+2
Mean
-2
-4
Time->

12:18:29.81   12:19:16.01   12:20:02.21   12:20:48.41

L0 (without object)
CH_2
Mean: -10.76
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:18:29.81   12:19:16.01   12:20:02.21   12:20:48.41

L1 (with object)
CH_1
Mean: -50.39
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:22:18.61   12:23:05.31   12:23:52.01   12:24:38.71   12:25

L1 (with object)
CH_2
Mean: 50.41
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:22:18.61   12:23:05.31   12:23:52.01   12:24:38.71   12:25

L2 (without object)
CH_1
Mean: -146.97
Acceptable range: 2.5
Failure points: 0.313%

+2
Mean
-2
Time->

12:26:14.41   12:26:30.38   12:26:46.36   12:27:02.34

L2 (without object)
CH_2
Mean: -10
Acceptable range: 2.5
Failure points: 0%

+2
Mean
-2
Time->

12:26:14.41   12:26:30.38   12:26:46.36   12:27:02.34

Database: D:\Projects_QCReports_Ord_Data\012210\QC\012210_TA_QC.gdb
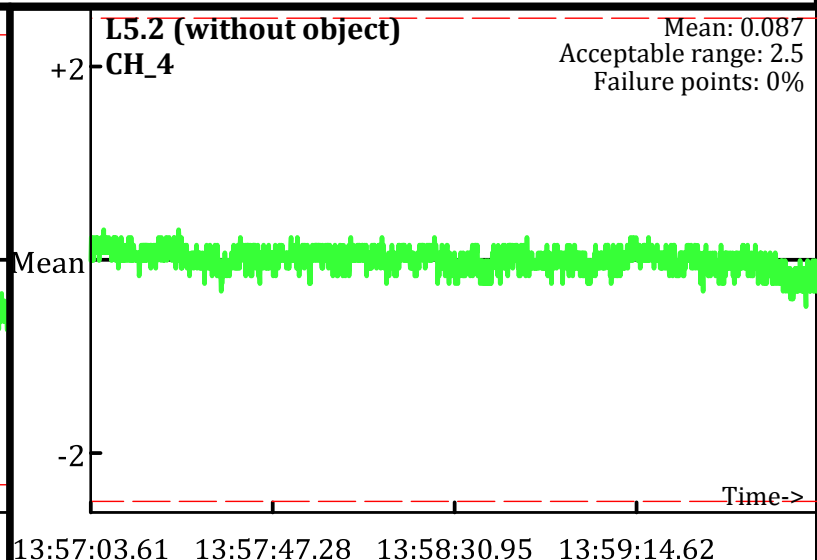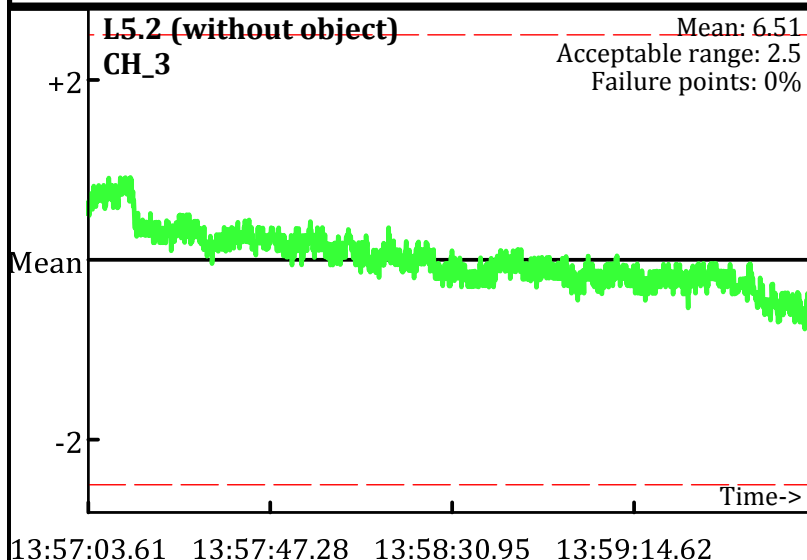Line Name: L0 L1 L2

Page: 1

Static Calibration Test

Project: Fort Ord Parker Flats - E.18.1.1-E18.1.2
Equipment: EM-61 Mark II
Grid/Location: QC Area

🔴 Outside range
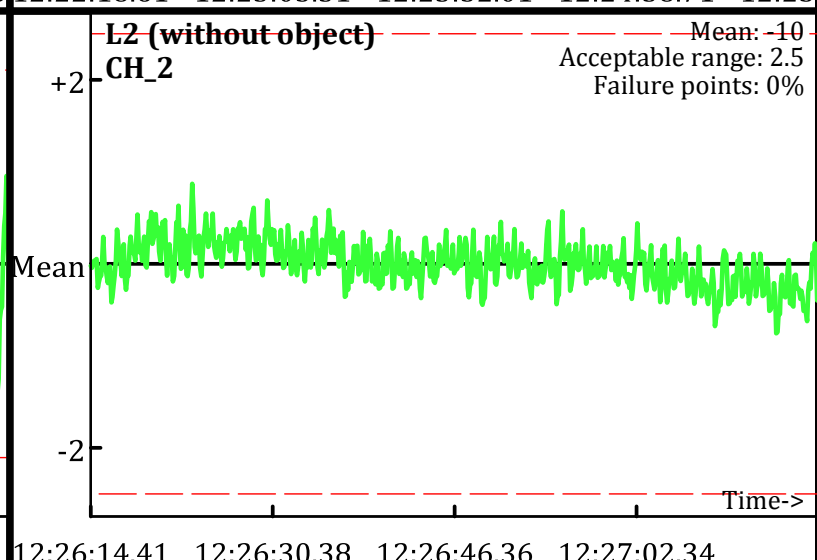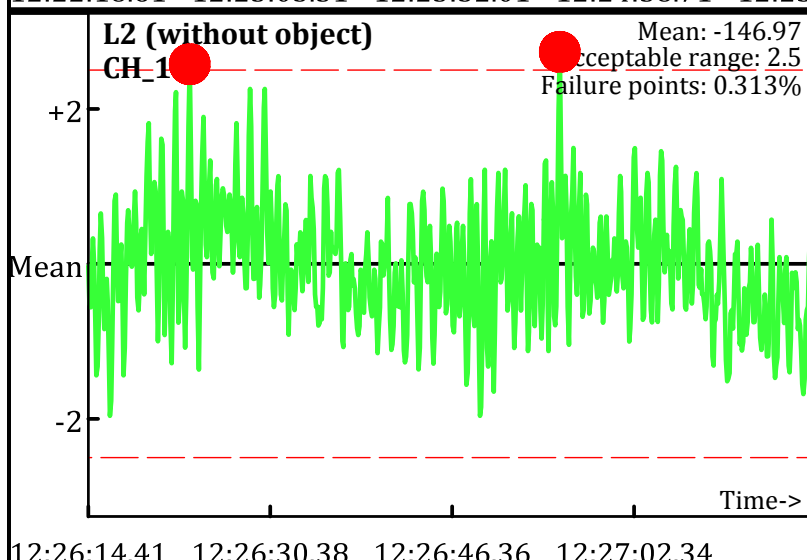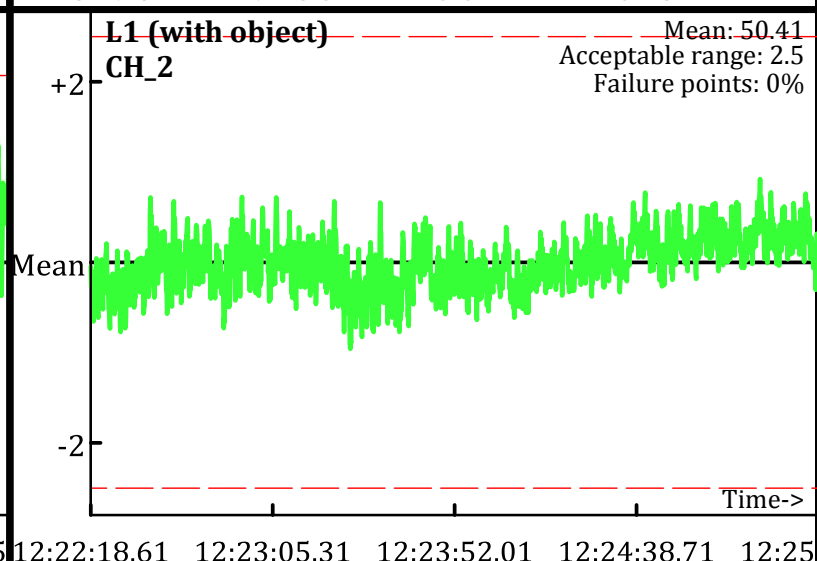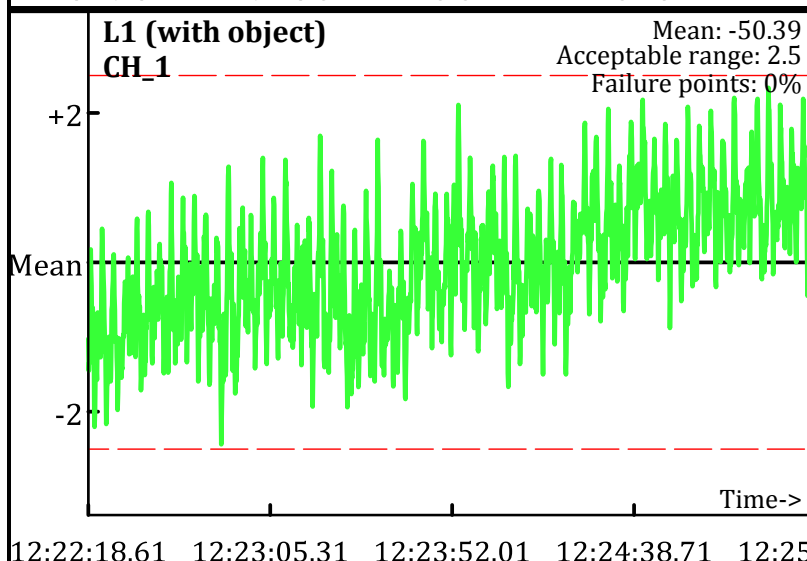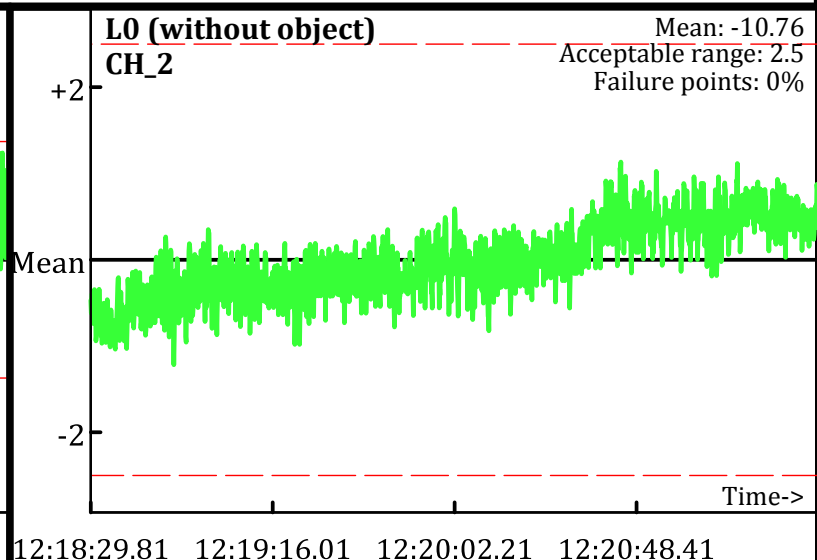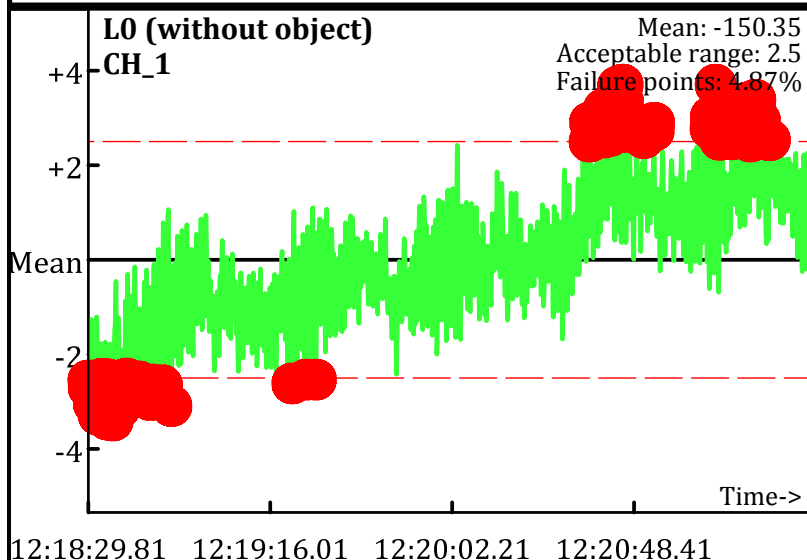--- Acceptable limits

AM test
Operator: PN & MG
Date: 1/22/2010

L0 (without object)
CH_3
Mean: 4.96
Acceptable range: 2.5
Failure points: 0%

Time->

12:18:29.81   12:19:16.01   12:20:02.21   12:20:48.41

L0 (without object)
CH_4
Mean: -1.57
Acceptable range: 2.5
Failure points: 0%

Time->

12:18:29.81   12:19:16.01   12:20:02.21   12:20:48.41

L1 (with object)
CH_3
Mean: 36.49
Acceptable range: 2.5
Failure points: 0%

Time->

12:22:18.61   12:23:05.31   12:23:52.01   12:24:38.71   12:25

L1 (with object)
CH_4
Mean: 12.27
Acceptable range: 2.5
Failure points: 0%

Time->

12:22:18.61   12:23:05.31   12:23:52.01   12:24:38.71   12:25

L2 (without object)
CH_3
Mean: 5.15
Acceptable range: 2.5
Failure points: 0%

Time->

12:26:14.41   12:26:30.38   12:26:46.36   12:27:02.34

L2 (without object)
CH_4
Mean: -1.46
Acceptable range: 2.5
Failure points: 0%

Time->

12:26:14.41   12:26:30.38   12:26:46.36   12:27:02.34